

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
 Data File : PP039654.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2021 6:05
 Operator : AJ\MA
 Sample : M3986-01
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P287-DITCH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 07:06:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.904	3.994	448062	272008	14.153	16.694
2)	SA Decachlor...	10.926	9.329	295132	298267	13.604	13.649

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
Data File : PP039654.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2021 6:05
Operator : AJ\MA
Sample : M3986-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
P287-DITCH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 07:06:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

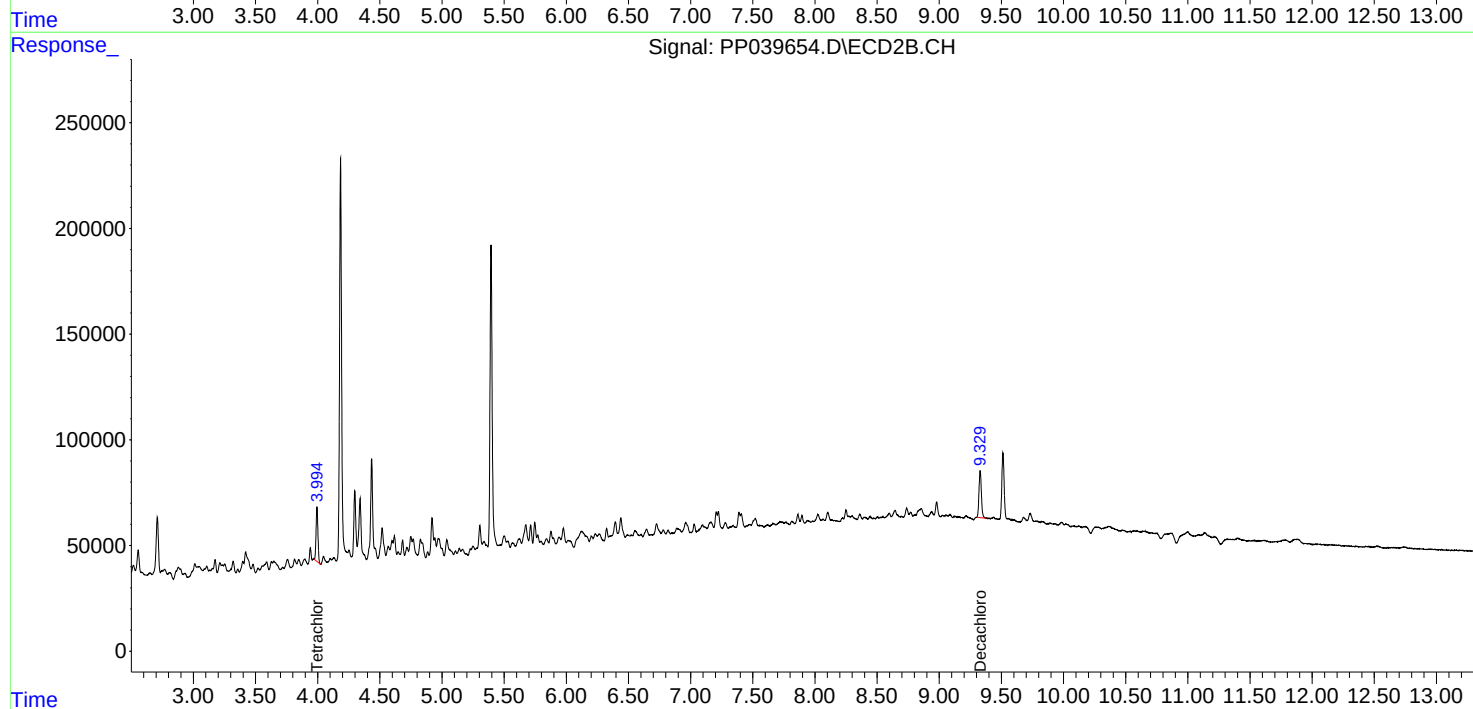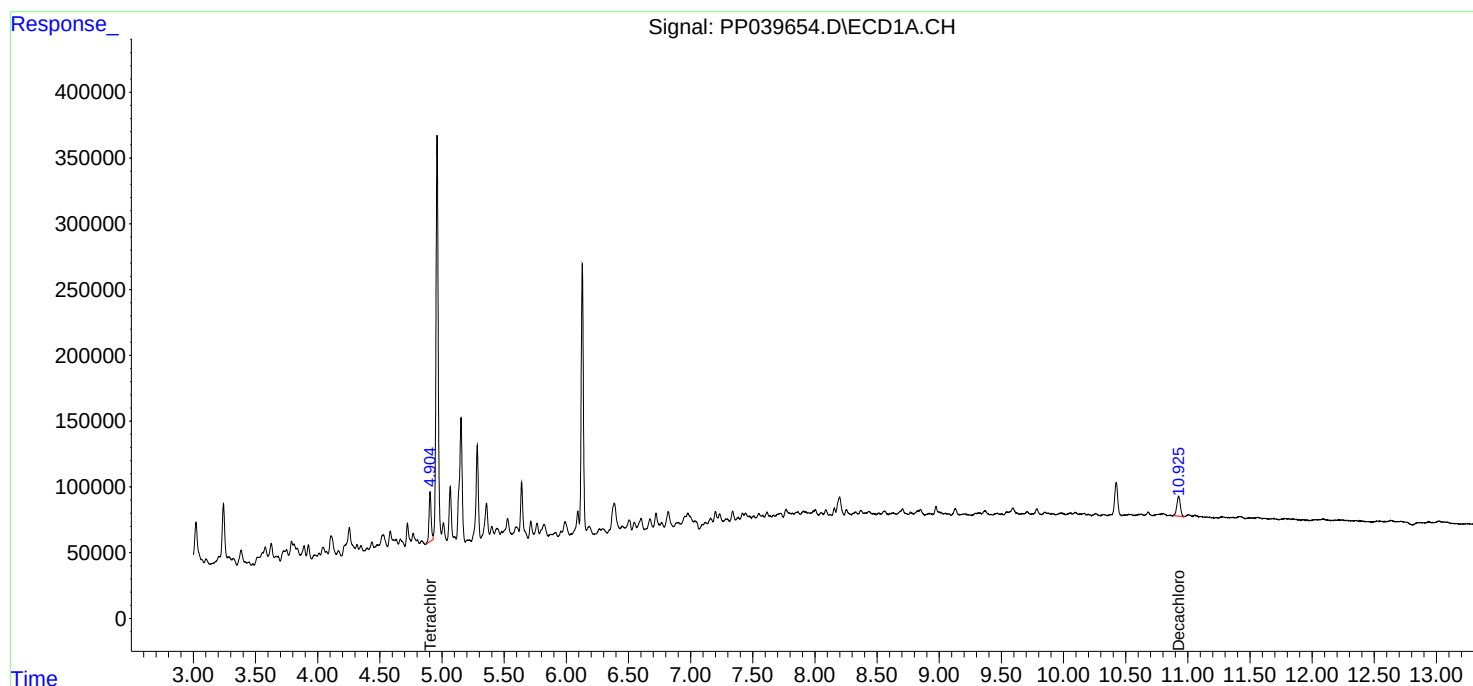


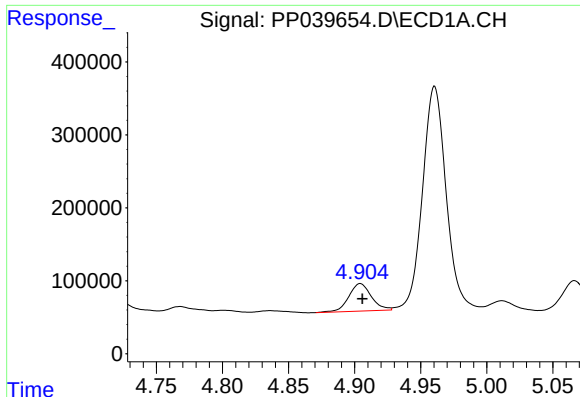

#1 Tetrachloro-m-xylene


R.T.: 4.904 min
Delta R.T.: -0.002 min
Response: 448062
Conc: 14.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
P287-DITCH

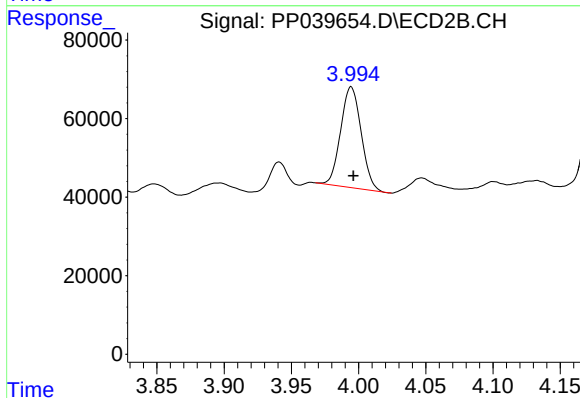


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 272008
Conc: 16.69 ng/ml

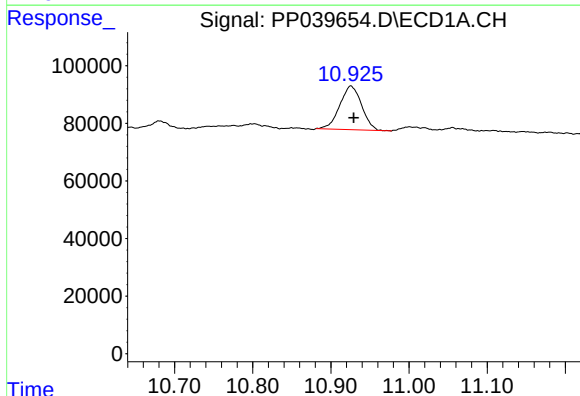

#2 Decachlorobiphenyl

R.T.: 10.926 min
Delta R.T.: -0.004 min
Response: 295132
Conc: 13.60 ng/ml

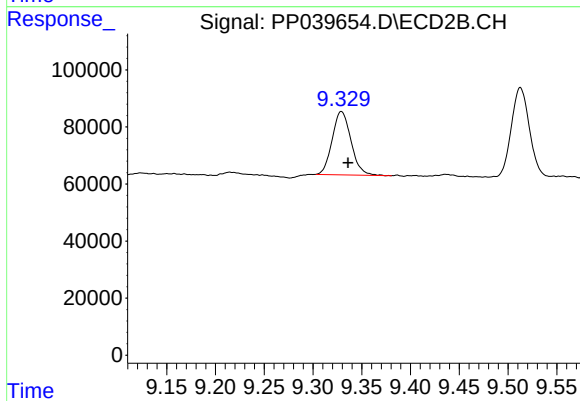

#2 Decachlorobiphenyl

R.T.: 9.329 min
Delta R.T.: -0.007 min
Response: 298267
Conc: 13.65 ng/ml