

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092923\
Data File : PP060423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 20:24
Operator : YP\AJ
Sample : 04627-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
280-300FB-BACKFILL-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 00:22:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.532	3.684	49527246	35671382	22.115	23.965
2) SA Decachlor...	10.453	8.748	47368732	34083038	26.830	20.895

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092923\
Data File : PP060423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 20:24
Operator : YP\AJ
Sample : 04627-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
280-300FB-BACKFILL-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 00:22:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

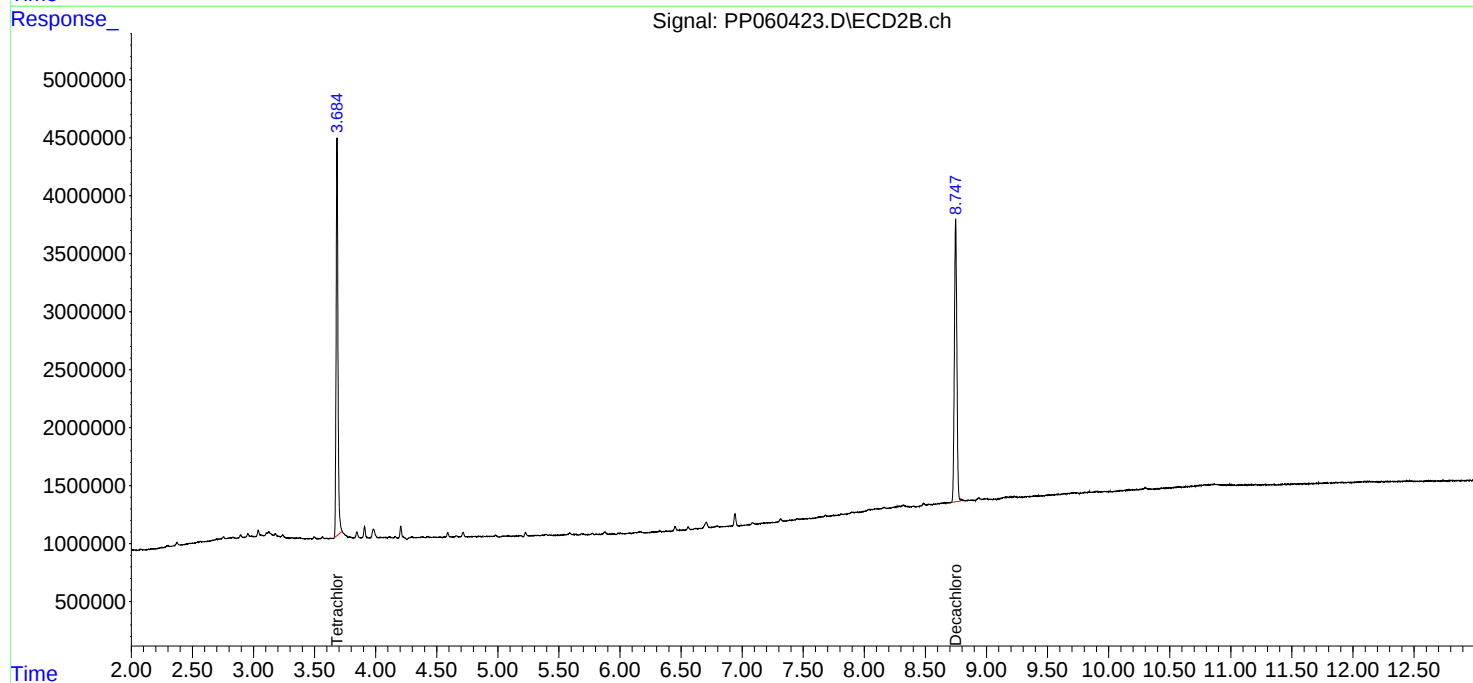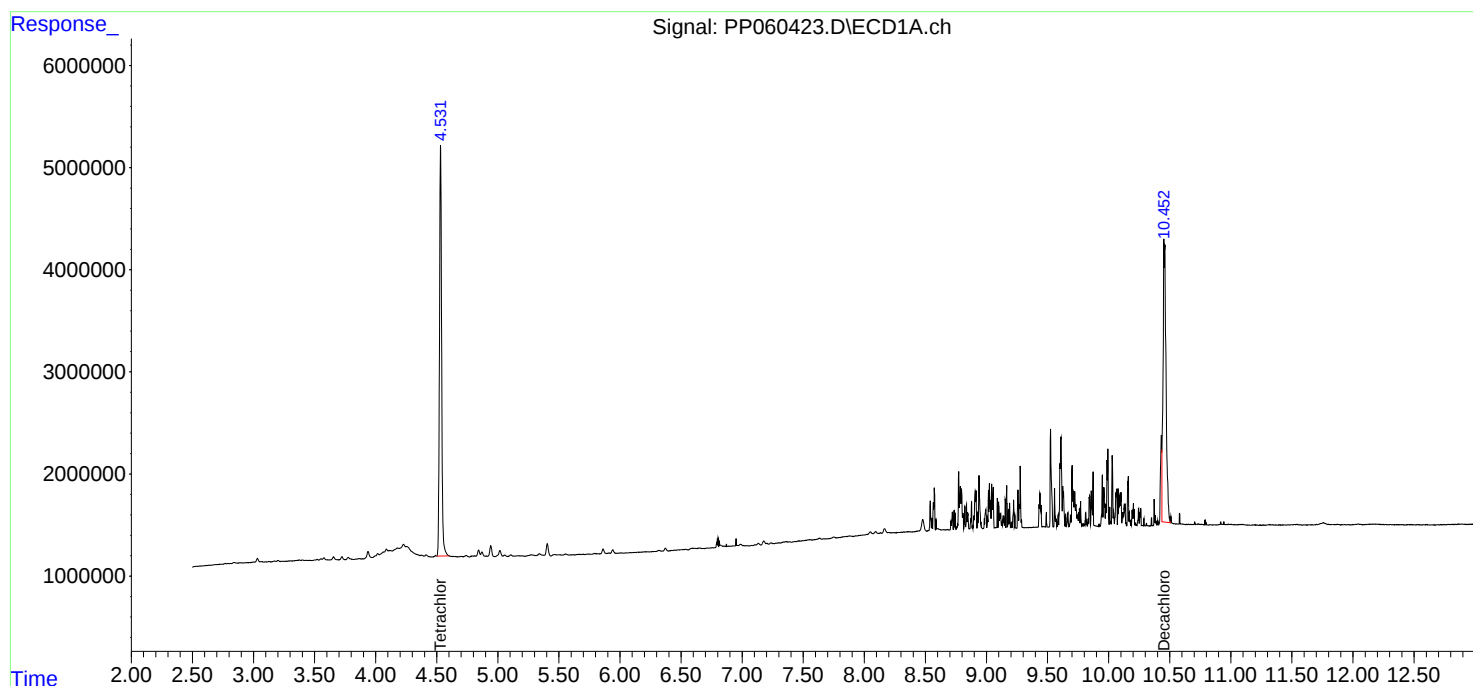


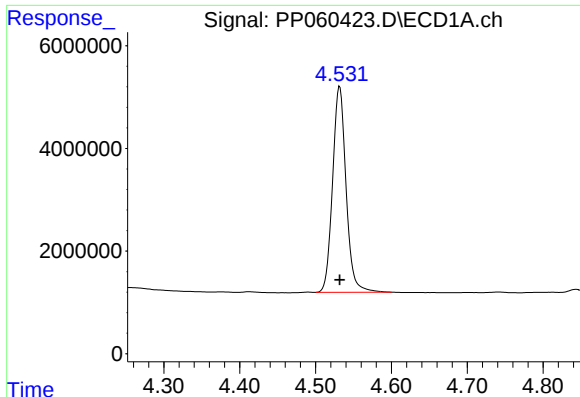

#1 Tetrachloro-m-xylene


R.T.: 4.532 min
Delta R.T.: 0.000 min
Response: 49527246
Conc: 22.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
280-300FB-BACKFILL-11

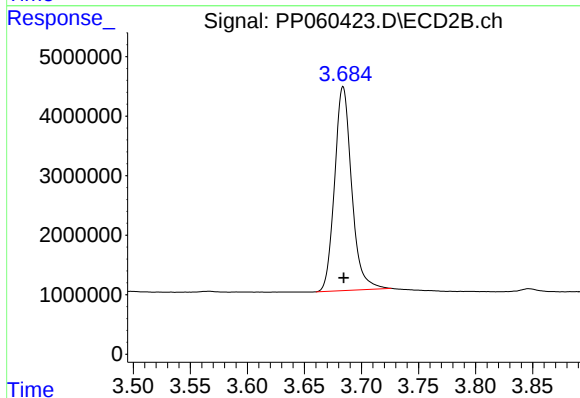


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.000 min
Response: 35671382
Conc: 23.96 ng/ml

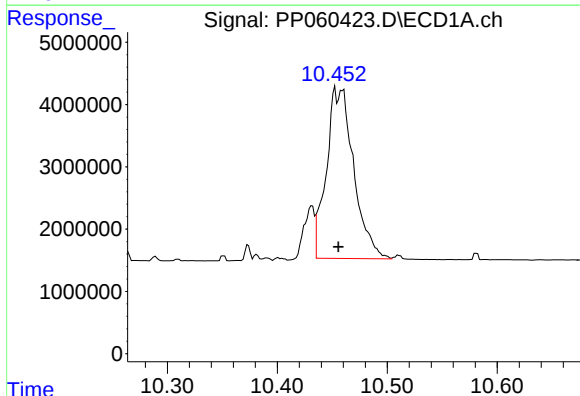

#2 Decachlorobiphenyl

R.T.: 10.453 min
Delta R.T.: -0.003 min
Response: 47368732
Conc: 26.83 ng/ml

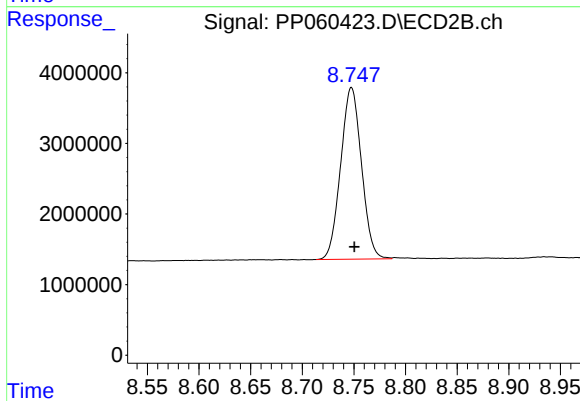

#2 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: -0.003 min
Response: 34083038
Conc: 20.89 ng/ml