

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092923\
 Data File : PP060425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 20:56
 Operator : YP\AJ
 Sample : 04627-25
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 280-300FB-BACKFILL-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 00:23:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.531	3.684	53144203	38608589	23.730	25.938
2) SA Decachlor...	10.455	8.747	41309791	36241098	23.398	22.218

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092923\
Data File : PP060425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 20:56
Operator : YP\AJ
Sample : 04627-25
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
280-300FB-BACKFILL-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 00:23:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

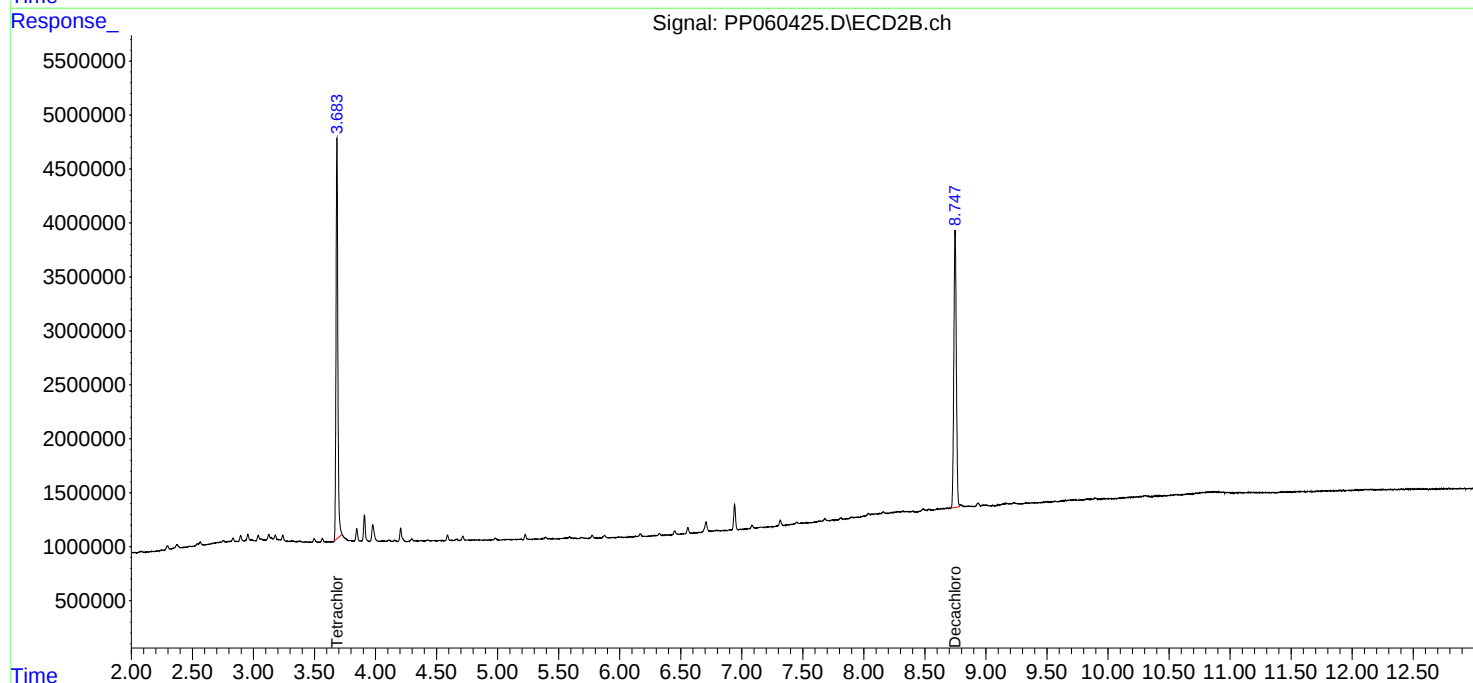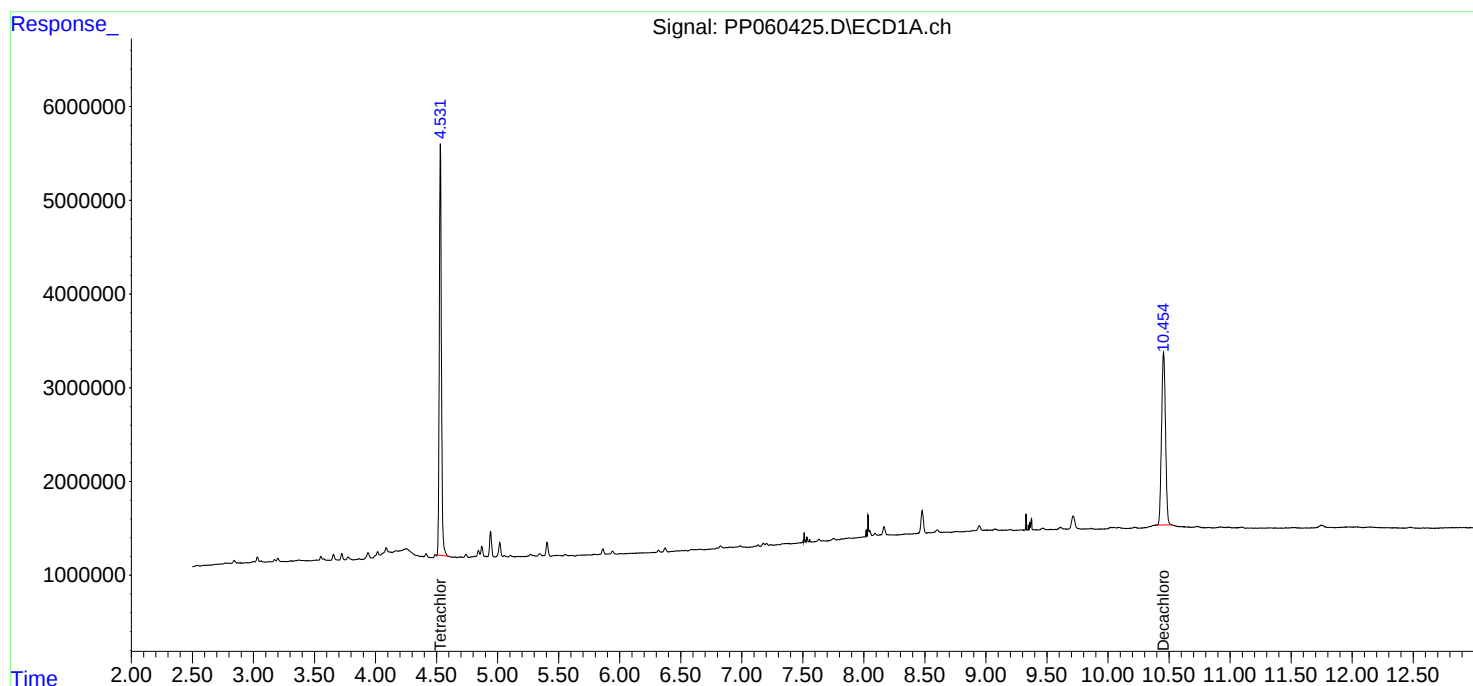


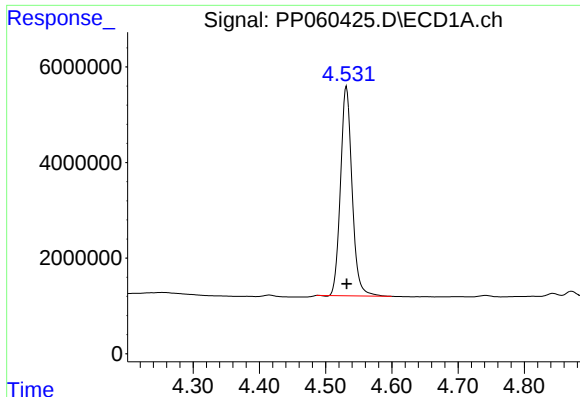

#1 Tetrachloro-m-xylene


R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 53144203
Conc: 23.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
280-300FB-BACKFILL-13

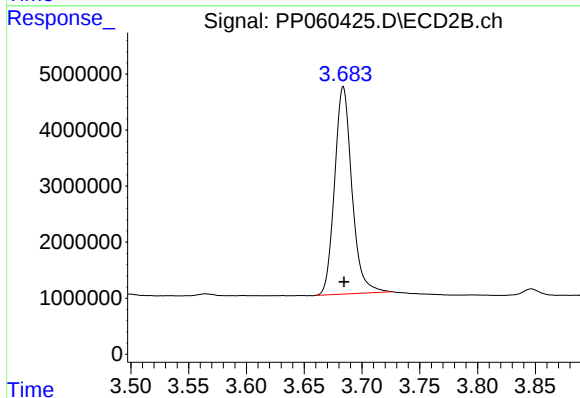


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.000 min
Response: 38608589
Conc: 25.94 ng/ml

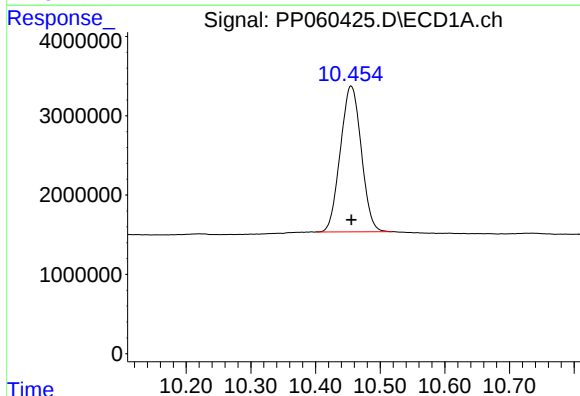

#2 Decachlorobiphenyl

R.T.: 10.455 min
Delta R.T.: 0.000 min
Response: 41309791
Conc: 23.40 ng/ml

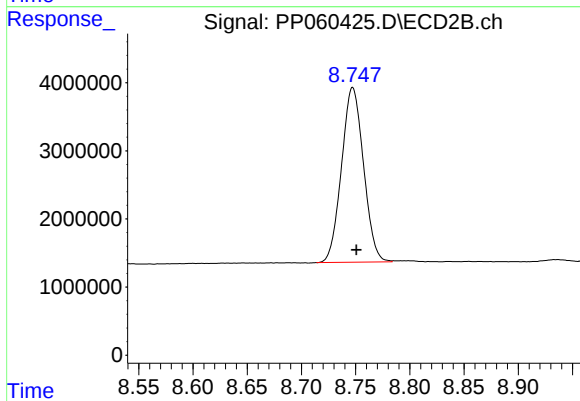

#2 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: -0.003 min
Response: 36241098
Conc: 22.22 ng/ml