

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092923\
 Data File : PP060430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2023 22:18
 Operator : YP\AJ
 Sample : 04668-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RBR251697

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/02/2023
 Supervised By :Ankita Jodhani 10/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 00:24:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.536	3.692	32444318	23007425	14.487	15.457m
2) SA Decachlor...	10.456	8.748	39576793	32600690	22.416	19.986

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092923\
Data File : PP060430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2023 22:18
Operator : YP\AJ
Sample : 04668-05
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RBR251697


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/02/2023
Supervised By :Ankita Jodhani 10/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 00:24:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

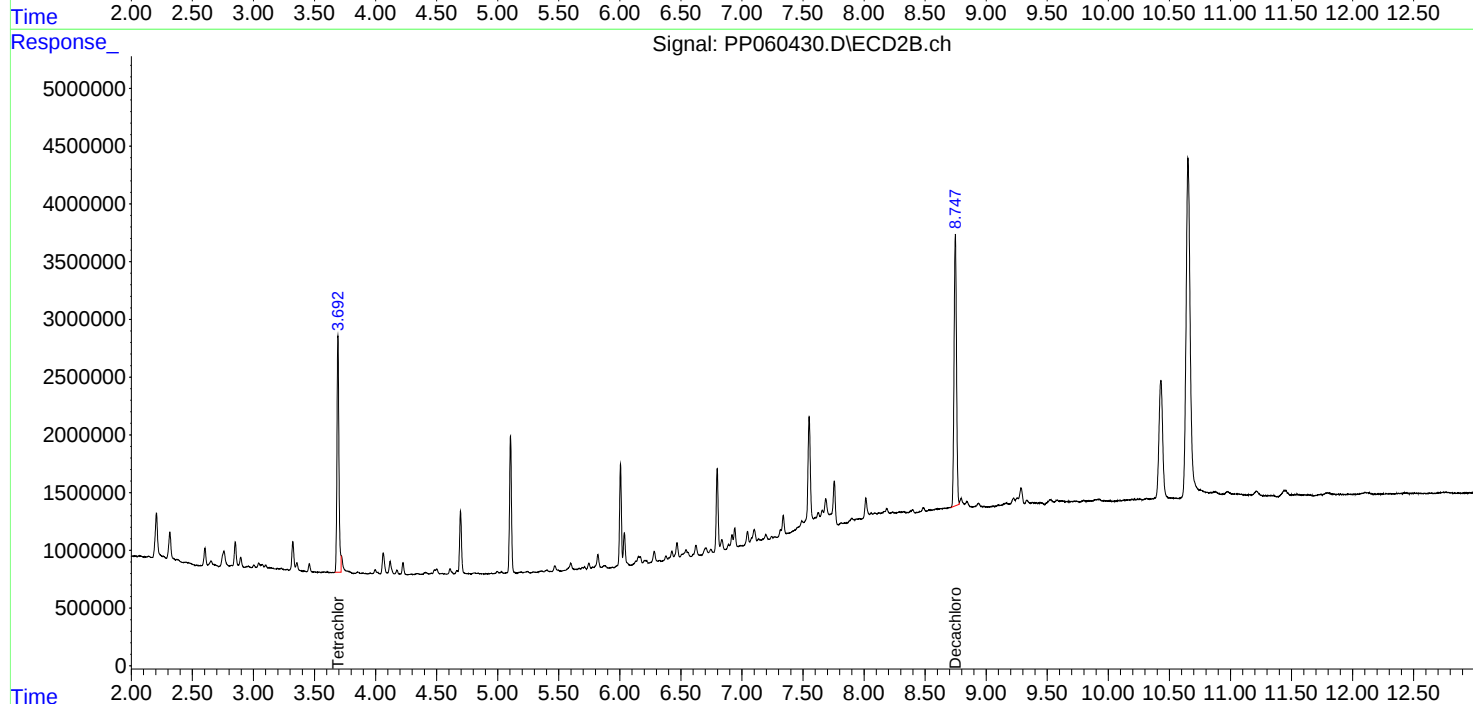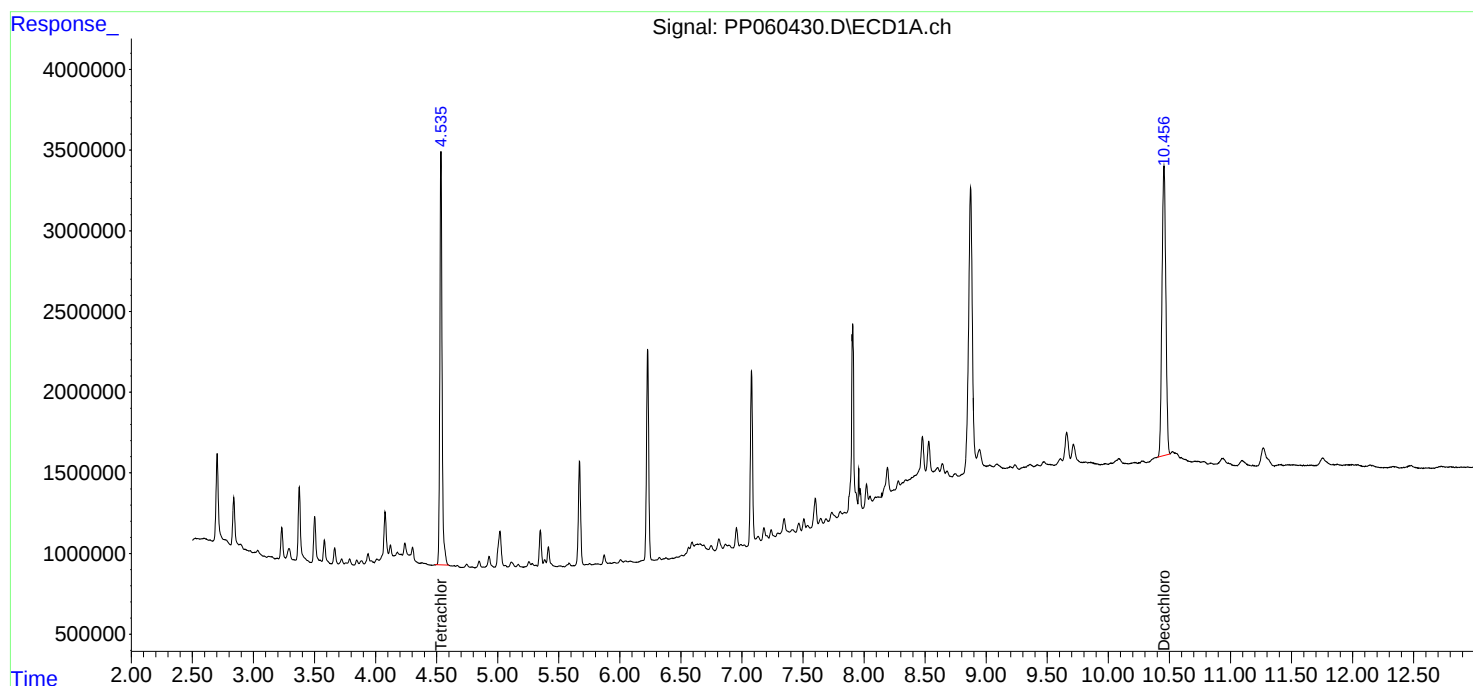

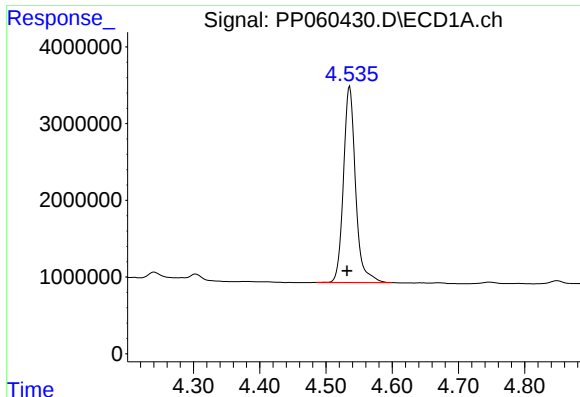


#1 Tetrachloro-m-xylene

R.T.: 4.536 min
Delta R.T.: 0.004 min
Response: 32444318
Conc: 14.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
RBR251697


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/02/2023
Supervised By :Ankita Jodhani 10/02/2023

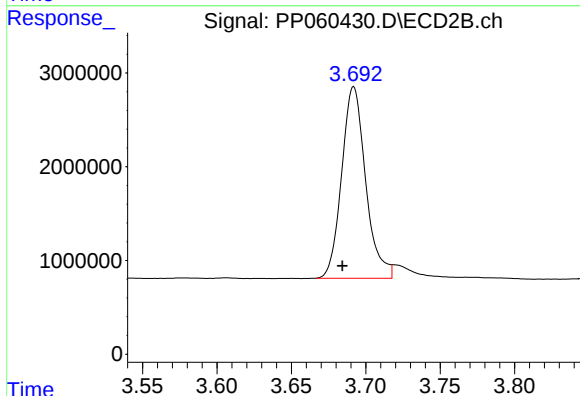


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: 0.007 min
Response: 23007425
Conc: 15.46 ng/ml m

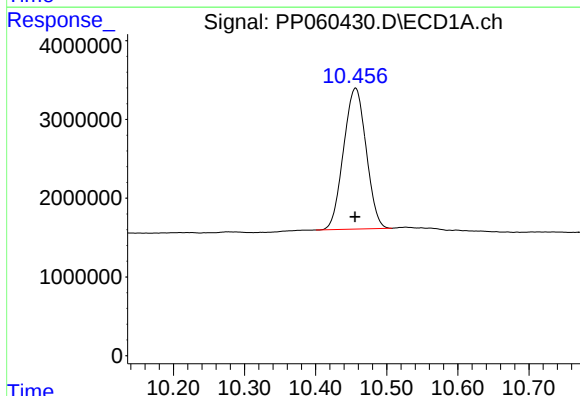

#2 Decachlorobiphenyl

R.T.: 10.456 min
Delta R.T.: 0.000 min
Response: 39576793
Conc: 22.42 ng/ml

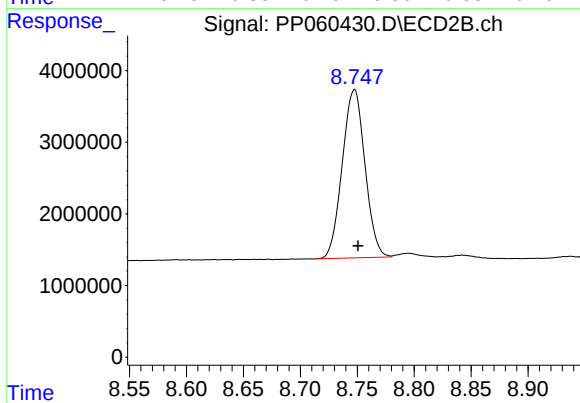

#2 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: -0.003 min
Response: 32600690
Conc: 19.99 ng/ml