

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP093021\
 Data File : PP039675.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2021 15:57
 Operator : AJ\MA
 Sample : M3984-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:48:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.904	3.993	700474	406811	22.127	24.967
2)	SA Decachlor...	10.926	9.329	504610	546683	23.260	25.017
Target Compounds							
14)	L3 AR-1232-4	0.000	5.573	0	11549	N.D.	49.209 #
19)	L4 AR-1242-4	0.000	5.573	0	11549	N.D.	27.340 #
23)	L5 AR-1248-3	0.000	5.573	0	11549	N.D.	19.061 #
30)	L6 AR-1254-5	0.000	7.386	0	12000	N.D.	8.525 #
32)	L7 AR-1260-2	0.000	7.030f	0	7541	N.D.	5.887 #
36)	L8 AR-1262-1	0.000	7.386	0	12000	N.D.	17.021 #
38)	L8 AR-1262-3	0.000	8.227	0	69479	N.D.	68.359 #
41)	L9 AR-1268-1	0.000	8.227	0	69479	N.D.	23.828 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP093021\
Data File : PP039675.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2021 15:57
Operator : AJ\MA
Sample : M3984-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:48:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

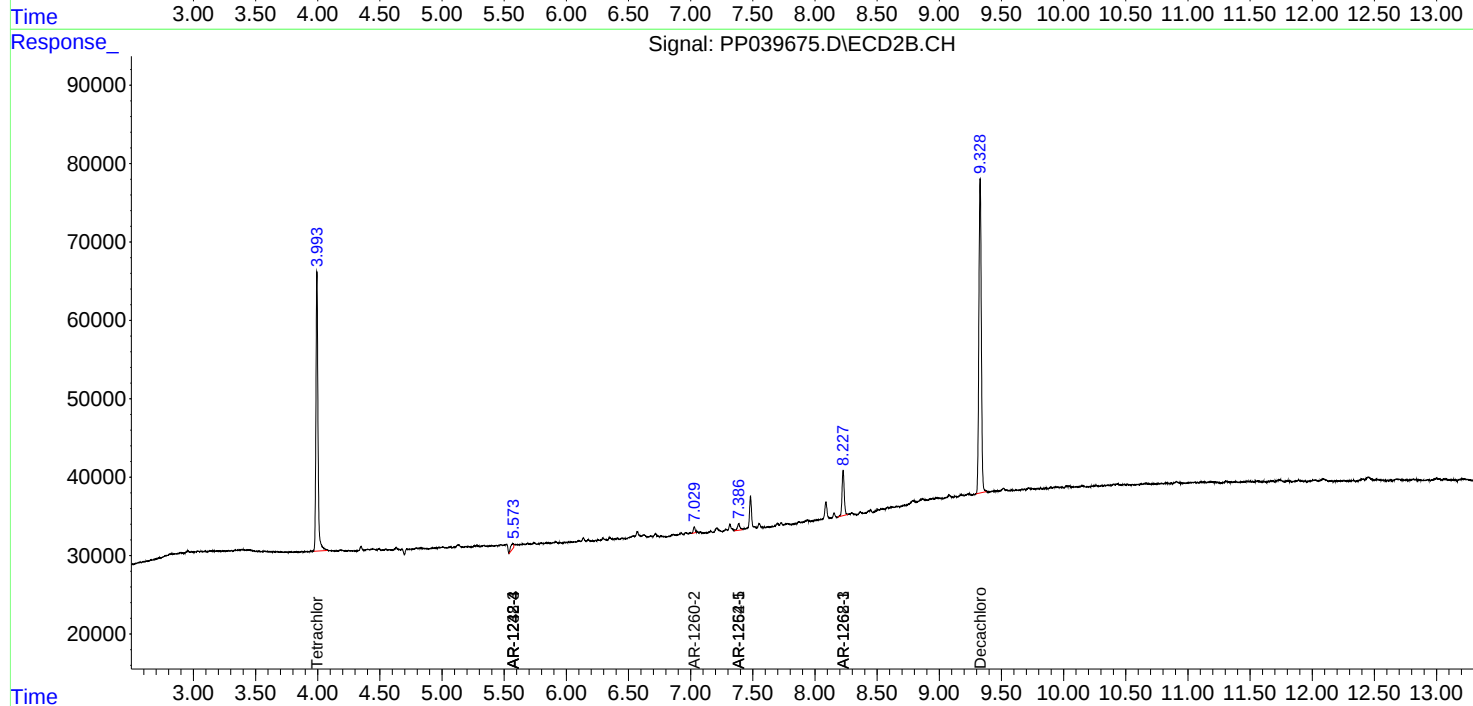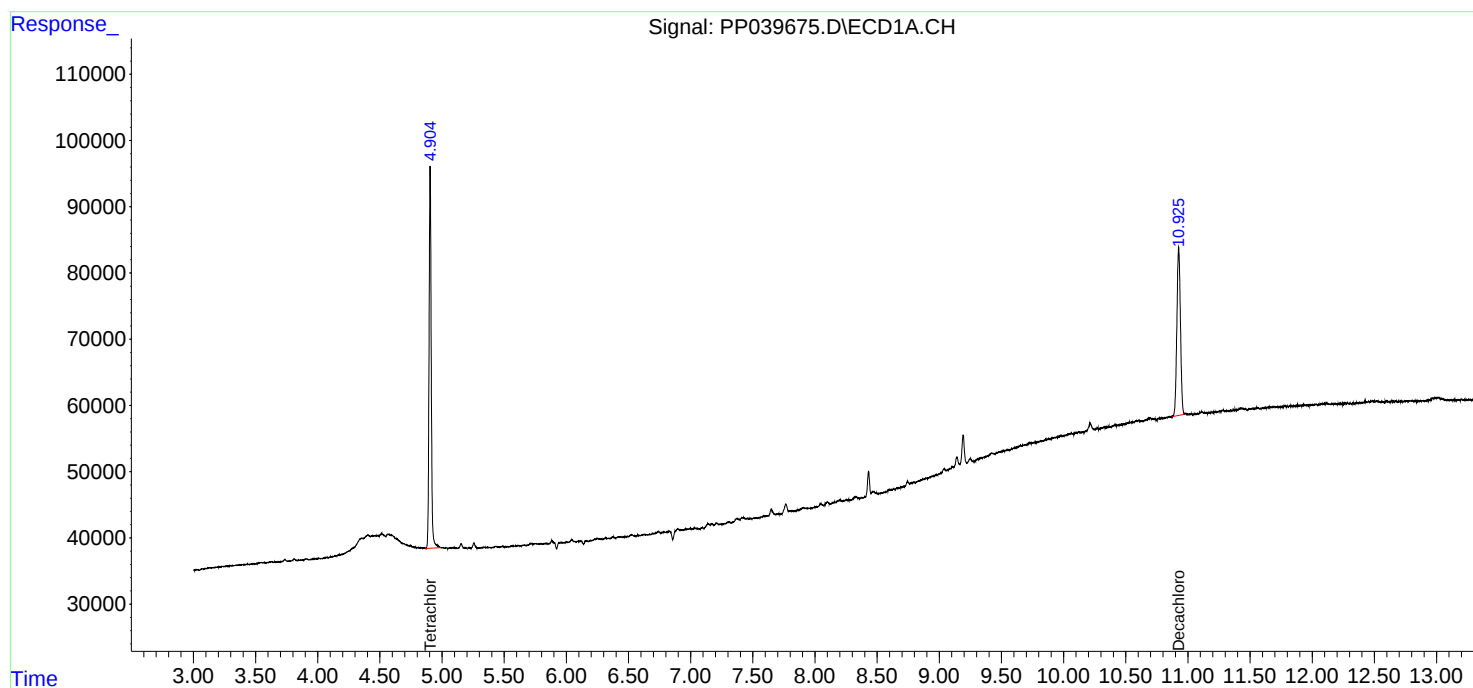


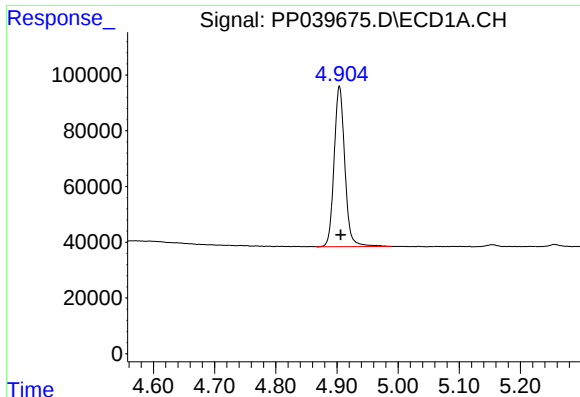

#1 Tetrachloro-m-xylene


R.T.: 4.904 min
Delta R.T.: -0.002 min
Response: 700474
Conc: 22.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

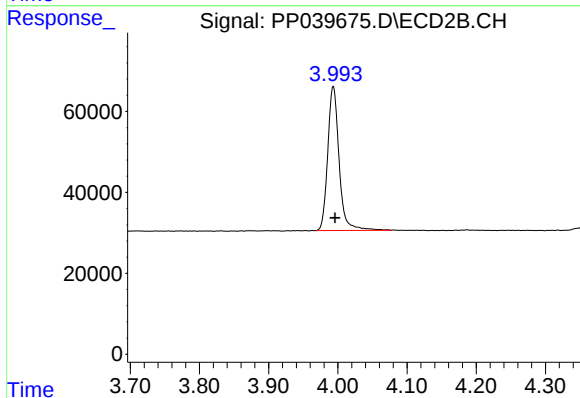


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: -0.003 min
Response: 406811
Conc: 24.97 ng/ml

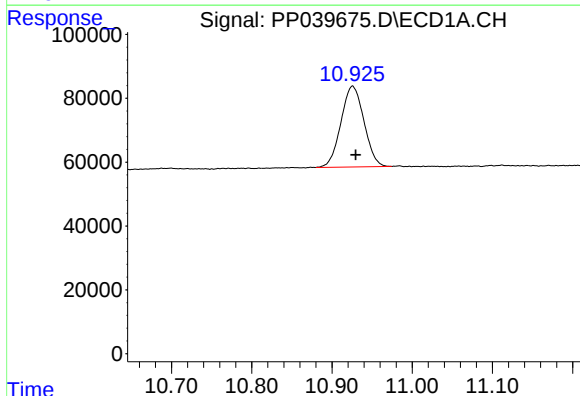


#2 Decachlorobiphenyl

R.T.: 10.926 min
Delta R.T.: -0.004 min
Response: 504610
Conc: 23.26 ng/ml

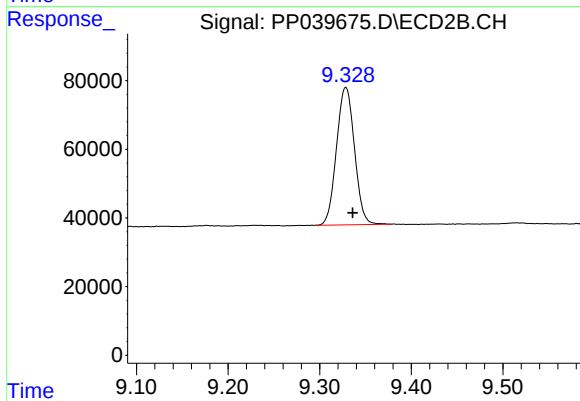

#2 Decachlorobiphenyl


R.T.: 9.329 min
Delta R.T.: -0.008 min
Response: 546683
Conc: 25.02 ng/ml

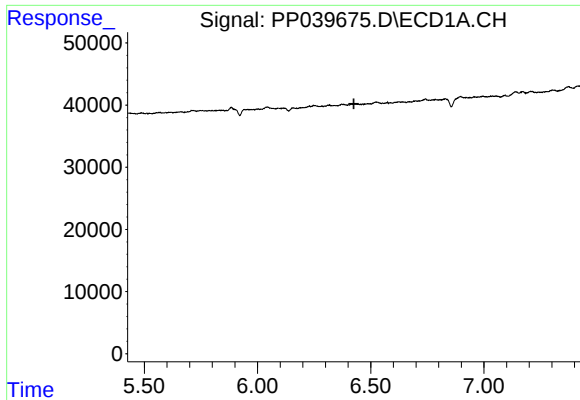

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 6.426 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

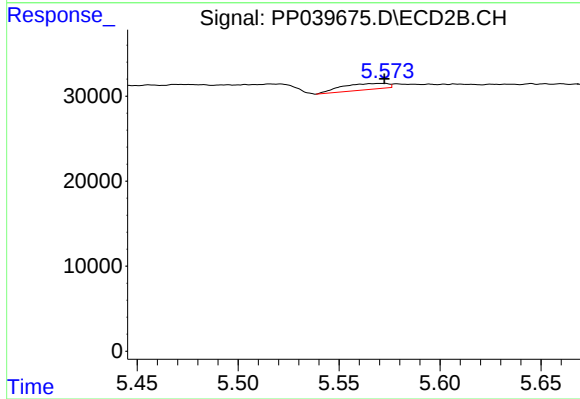


#14 AR-1232-4

R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 11549
Conc: 49.21 ng/ml

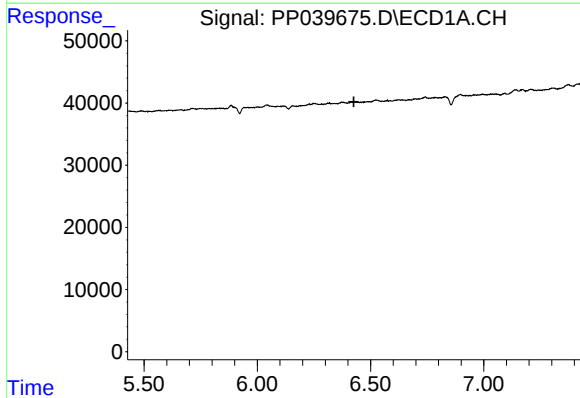


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 6.426 min
Response: 0
Conc: N.D.

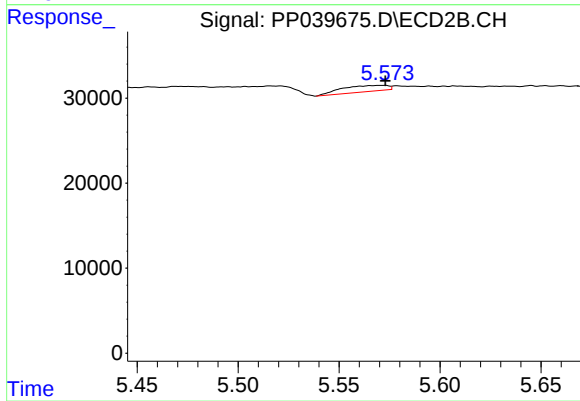

#19 AR-1242-4


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 11549
Conc: 27.34 ng/ml

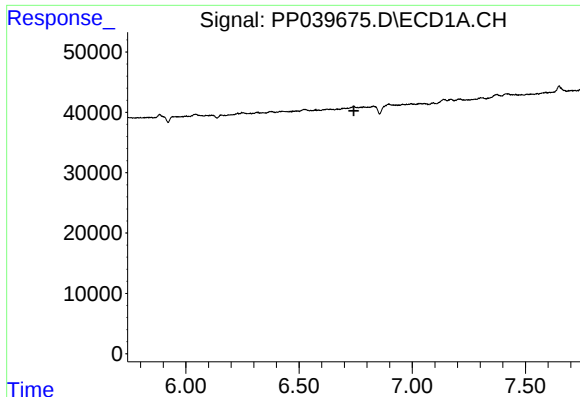

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T. : 6.742 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

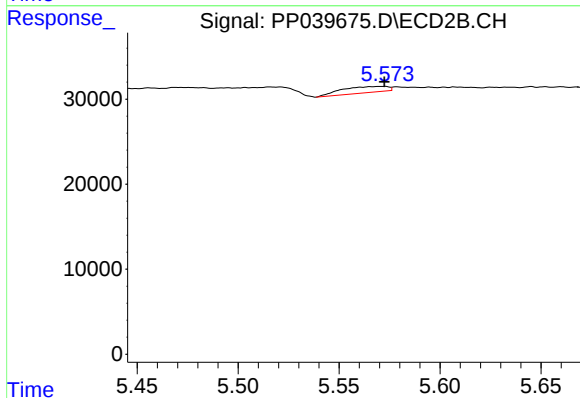


#23 AR-1248-3

R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 11549
Conc: 19.06 ng/ml

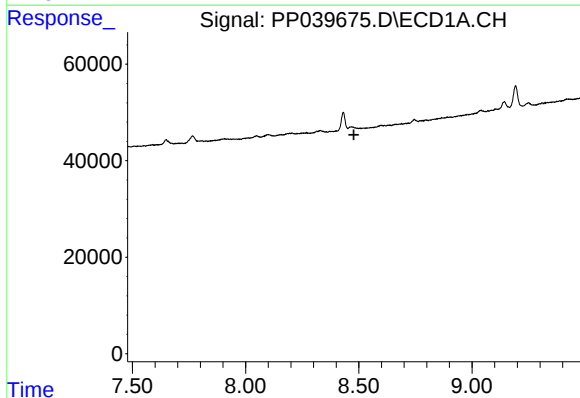


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.478 min
Response: 0
Conc: N.D.

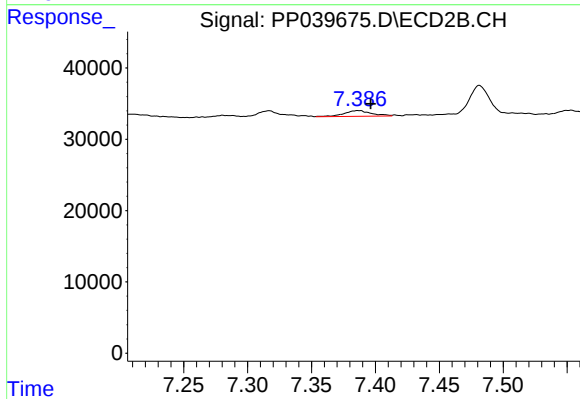

#30 AR-1254-5


R.T.: 7.386 min
Delta R.T.: -0.010 min
Response: 12000
Conc: 8.53 ng/ml

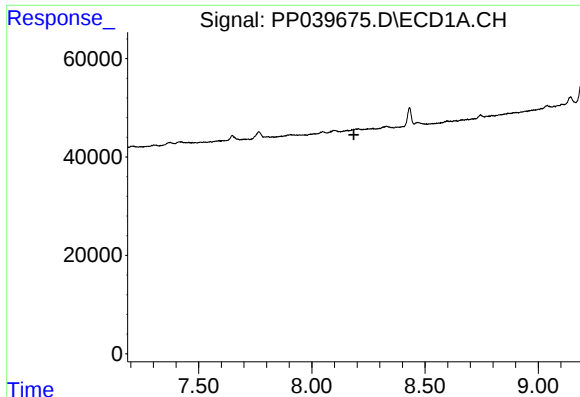

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

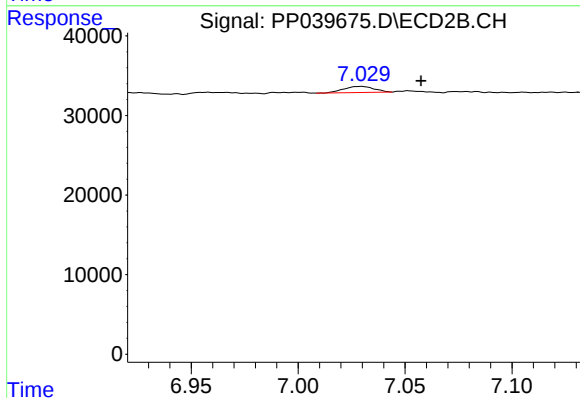


#32 AR-1260-2

R.T.: 7.030 min
Delta R.T.: -0.028 min
Response: 7541
Conc: 5.89 ng/ml

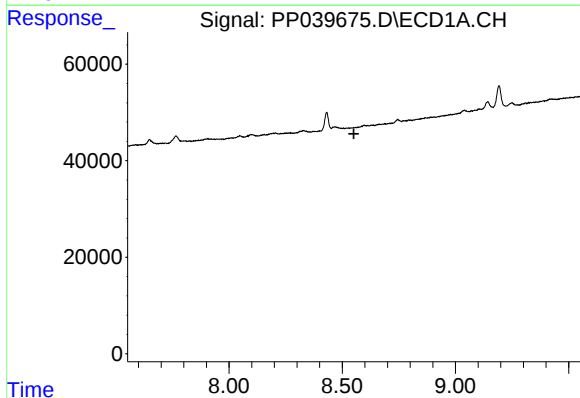


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.552 min
Response: 0
Conc: N.D.

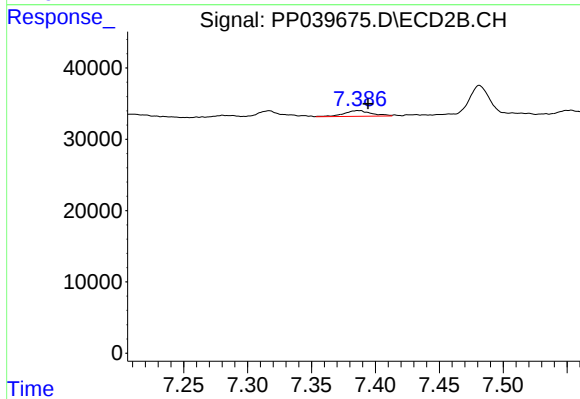

#36 AR-1262-1


R.T.: 7.386 min
Delta R.T.: -0.008 min
Response: 12000
Conc: 17.02 ng/ml

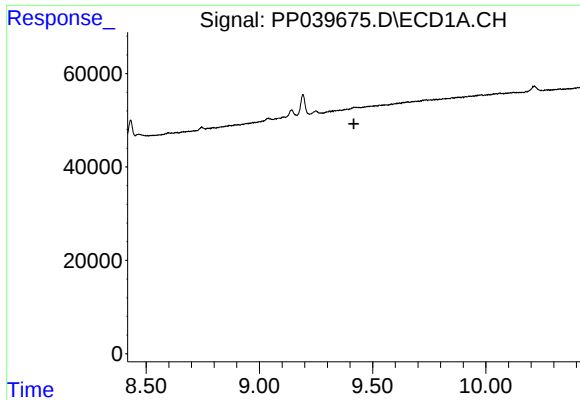

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

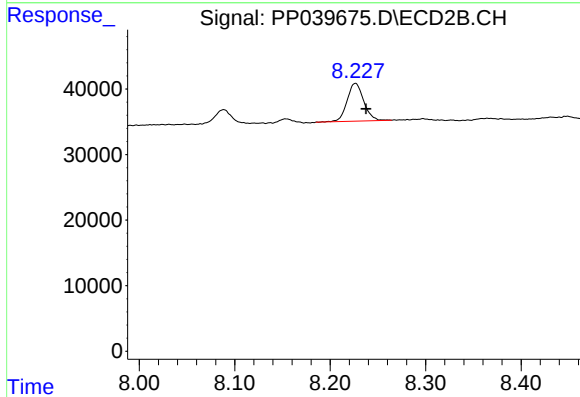


#38 AR-1262-3

R.T.: 8.227 min
Delta R.T.: -0.011 min
Response: 69479
Conc: 68.36 ng/ml

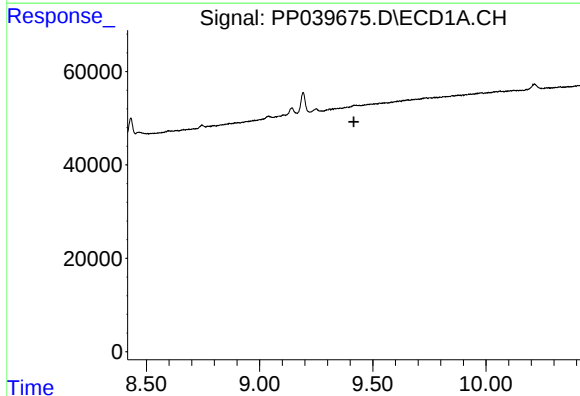

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

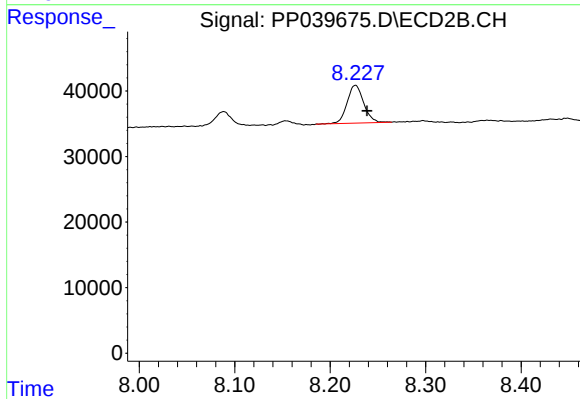

#41 AR-1268-1

R.T.: 8.227 min
Delta R.T.: -0.012 min
Response: 69479
Conc: 23.83 ng/ml