

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP093021\  
 Data File : PP039689.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 30 Sep 2021 19:53  
 Operator : AJ\MA  
 Sample : M3990-03  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 S-840-R-SO-6-6.5-092921

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 01 01:53:22 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP092421.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Sat Sep 25 01:28:12 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|--------|--------|--------|--------|
| -----                       |        |       |        |        |        |        |
| System Monitoring Compounds |        |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.904  | 3.993 | 647640 | 378865 | 20.458 | 23.251 |
| 2) SA Decachlor...          | 10.923 | 9.327 | 441349 | 475361 | 20.344 | 21.753 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP093021\  
Data File : PP039689.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 30 Sep 2021 19:53  
Operator : AJ\MA  
Sample : M3990-03  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
S-840-R-SO-6-6.5-092921

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 01 01:53:22 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP092421.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Sep 25 01:28:12 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

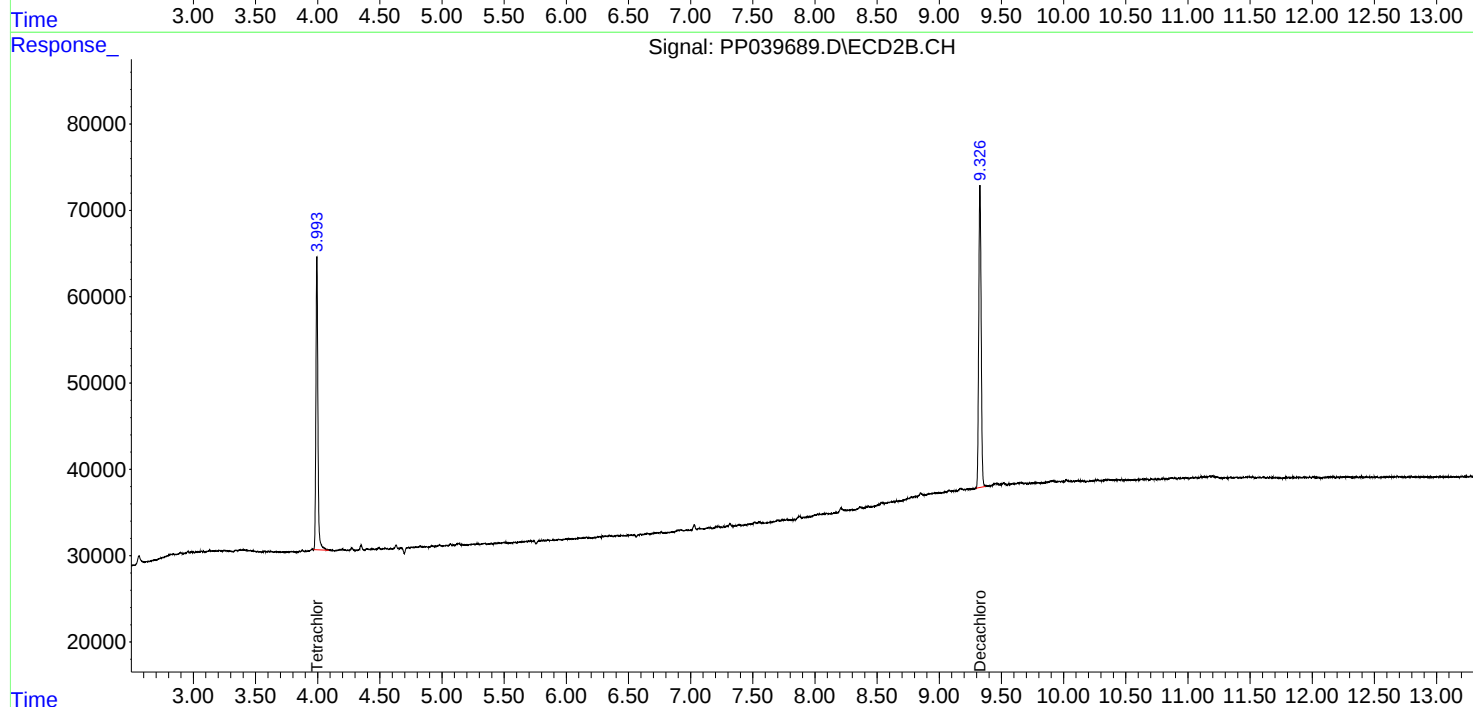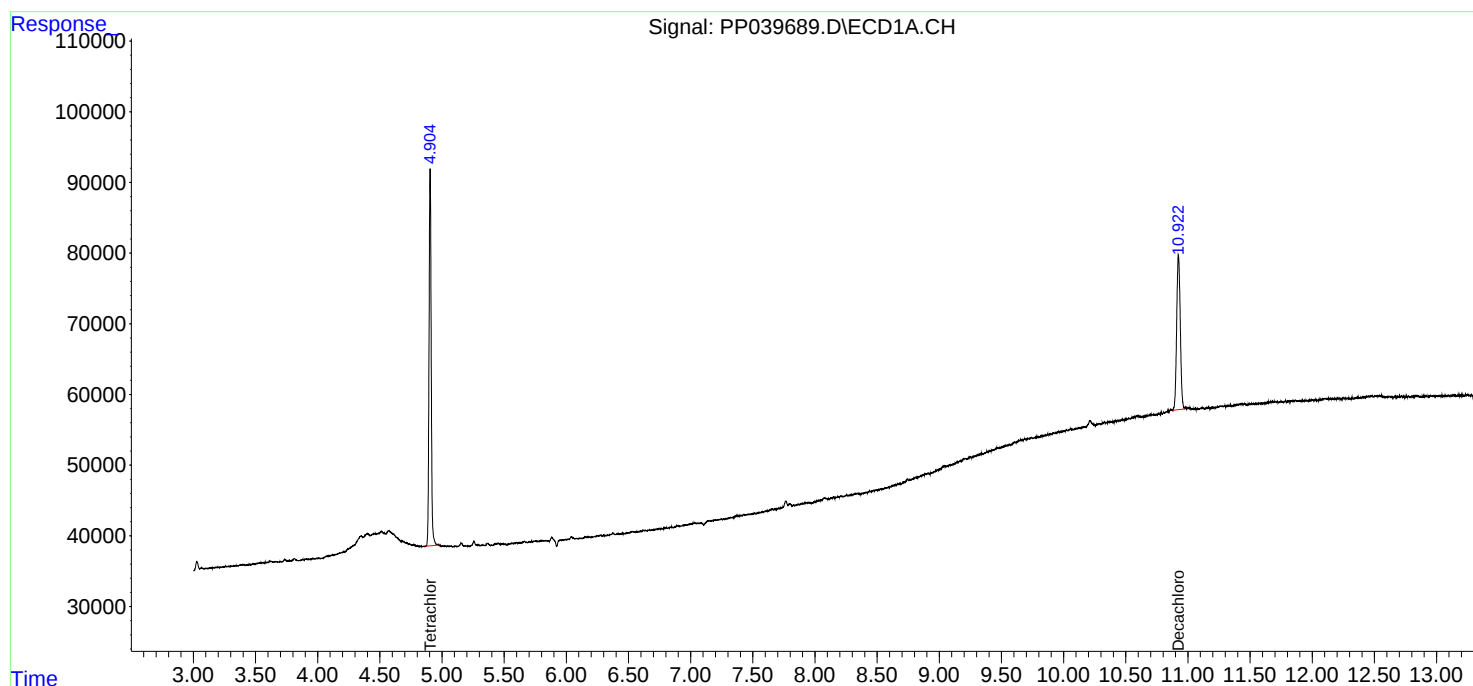


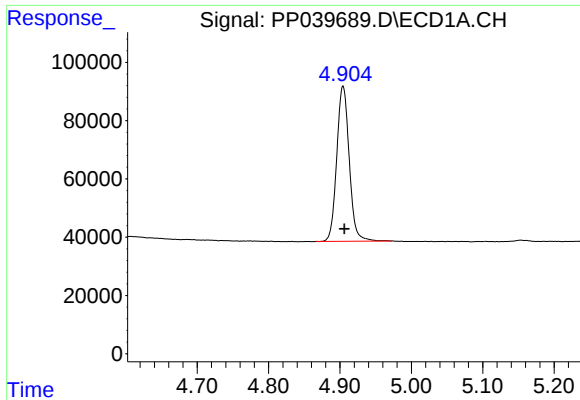

#1 Tetrachloro-m-xylene


R.T.: 4.904 min  
Delta R.T.: -0.002 min  
Response: 647640  
Conc: 20.46 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
S-840-R-SO-6-6.5-092921

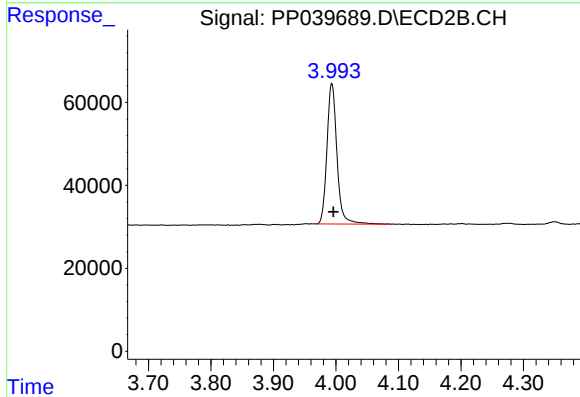


#1 Tetrachloro-m-xylene

R.T.: 3.993 min  
Delta R.T.: -0.003 min  
Response: 378865  
Conc: 23.25 ng/ml

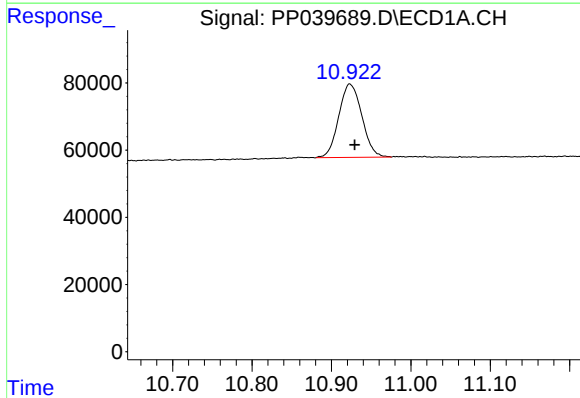

#2 Decachlorobiphenyl

R.T.: 10.923 min  
Delta R.T.: -0.007 min  
Response: 441349  
Conc: 20.34 ng/ml

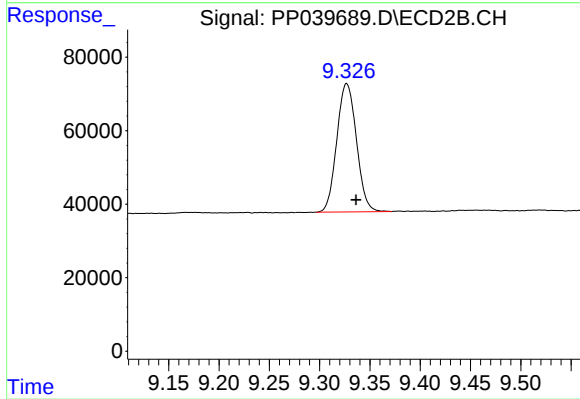

#2 Decachlorobiphenyl

R.T.: 9.327 min  
Delta R.T.: -0.009 min  
Response: 475361  
Conc: 21.75 ng/ml