

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100125\
 Data File : PP075481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 10:24
 Operator : YP\AJ
 Sample : Q3243-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 91825ABRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/01/2025
 Supervised By :mohammad ahmed 10/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 13:49:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.657	3.792	1099553	6193659	0.840m	1.015m
2) SA Decachlor...	10.432	8.797	3063527	16481350	3.071	2.732

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100125\
Data File : PP075481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 10:24
Operator : YP\AJ
Sample : Q3243-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
91825ABRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/01/2025
Supervised By :mohammad ahmed 10/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 13:49:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

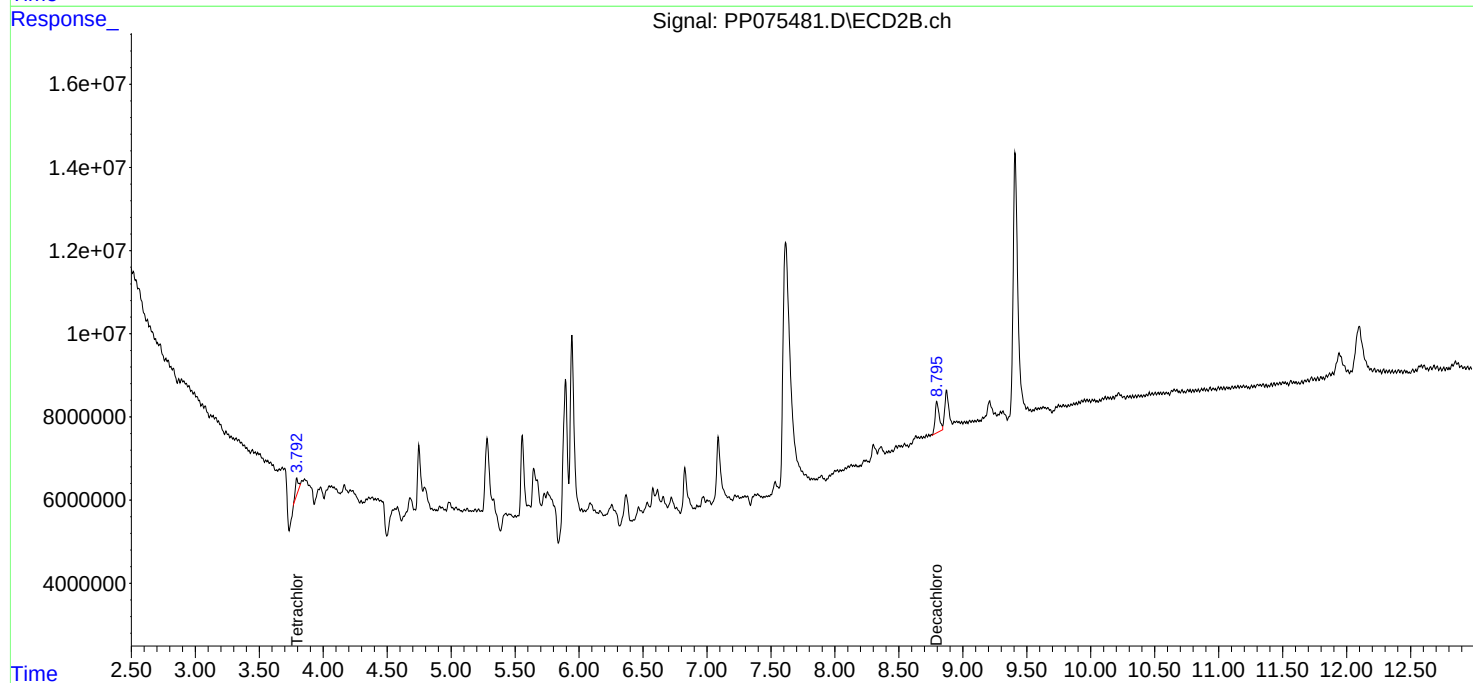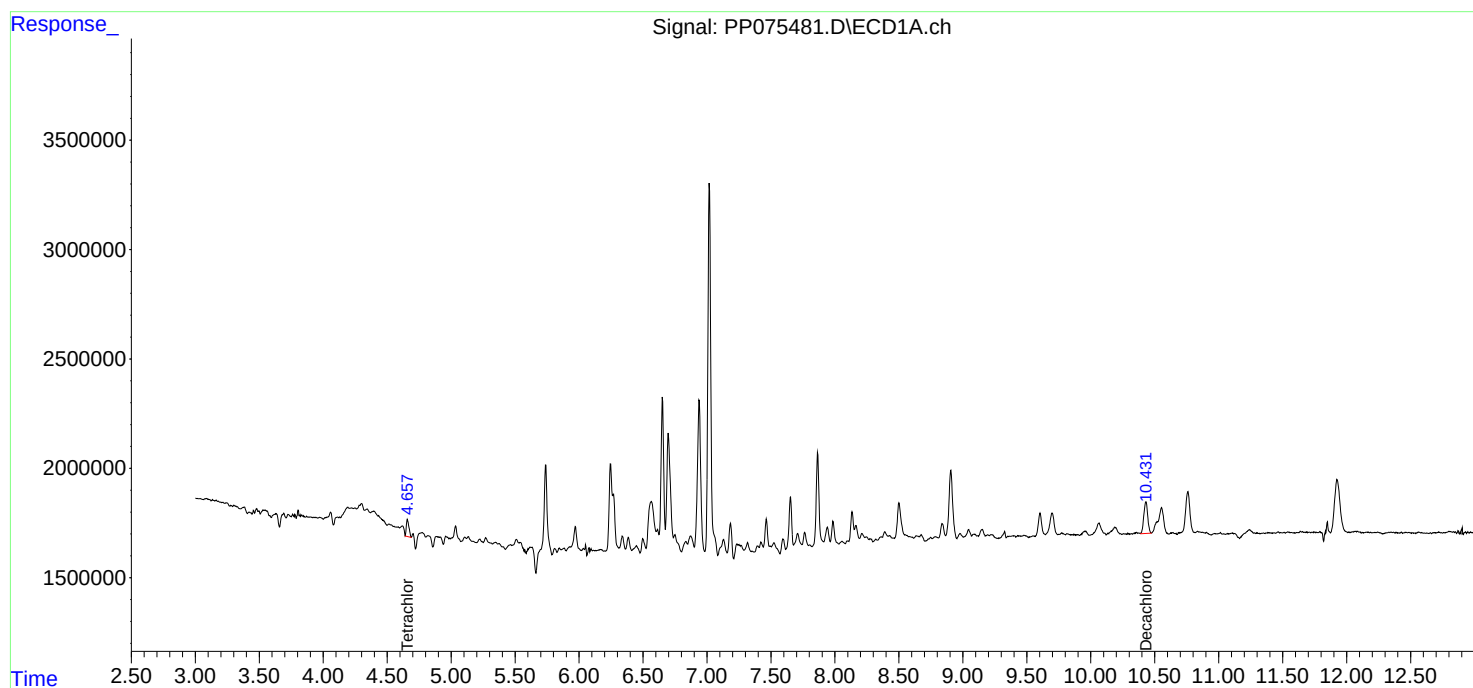

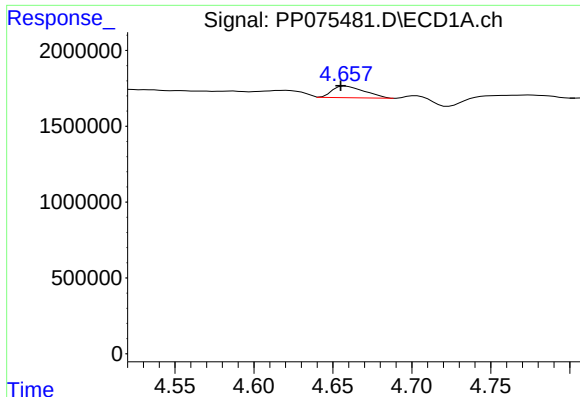


#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.002 min
Response: 1099553
Conc: 0.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
91825ABRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/01/2025
Supervised By :mohammad ahmed 10/04/2025

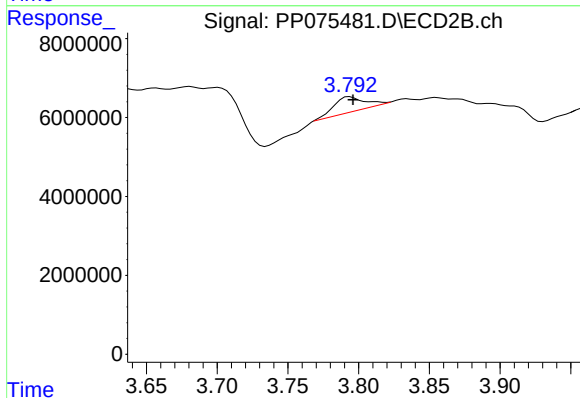


#1 Tetrachloro-m-xylene

R.T.: 3.792 min
Delta R.T.: -0.004 min
Response: 6193659
Conc: 1.02 ng/ml m

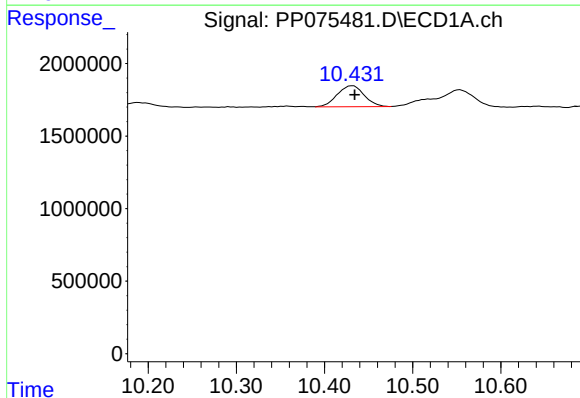

#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: -0.003 min
Response: 3063527
Conc: 3.07 ng/ml

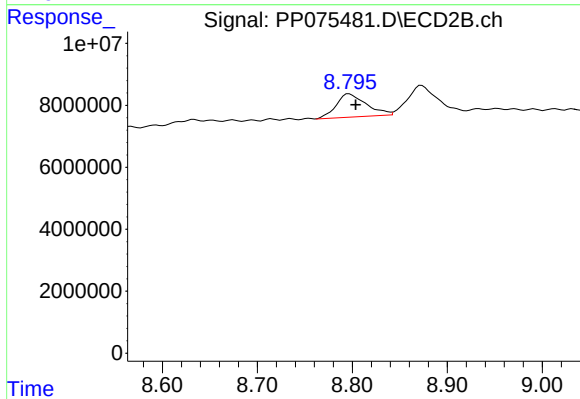

#2 Decachlorobiphenyl

R.T.: 8.797 min
Delta R.T.: -0.007 min
Response: 16481350
Conc: 2.73 ng/ml