

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100125\
 Data File : PP075495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 15:35
 Operator : YP\AJ
 Sample : Q3242-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 92325

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/03/2025
 Supervised By :mohammad ahmed 10/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 06:46:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.656	3.810	34871517	263.7E6	26.650m	43.217 #
2) SA Decachlor...	10.435	8.801	18814699	122.5E6	18.861m	20.314

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100125\
Data File : PP075495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 15:35
Operator : YP\AJ
Sample : Q3242-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
92325


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/03/2025
Supervised By :mohammad ahmed 10/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 06:46:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

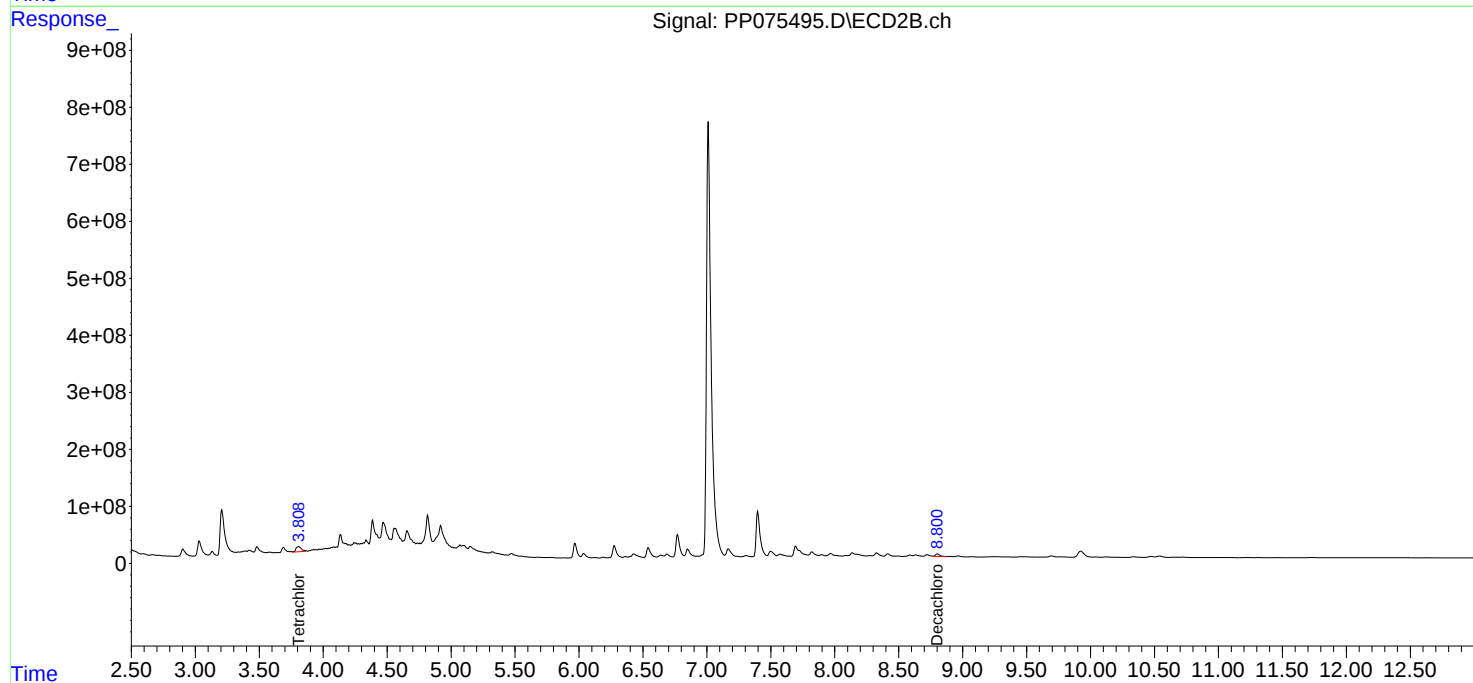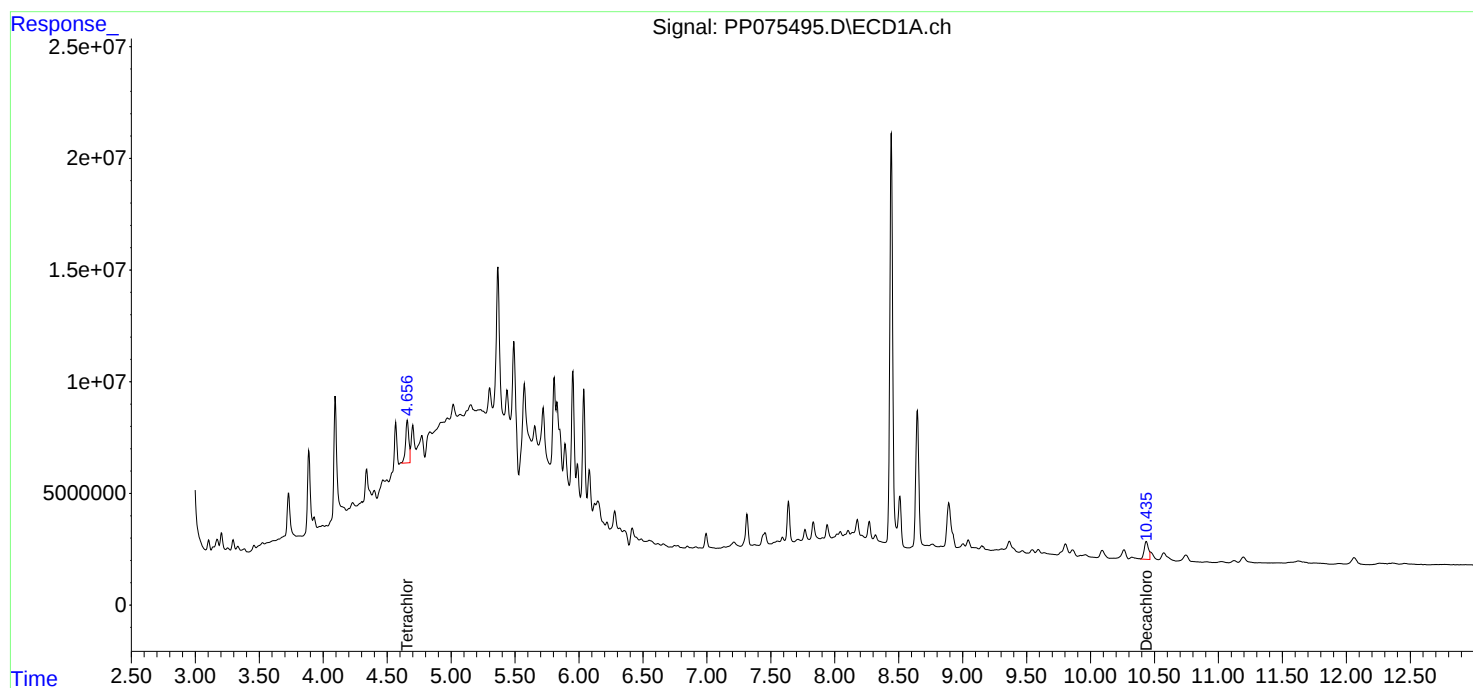

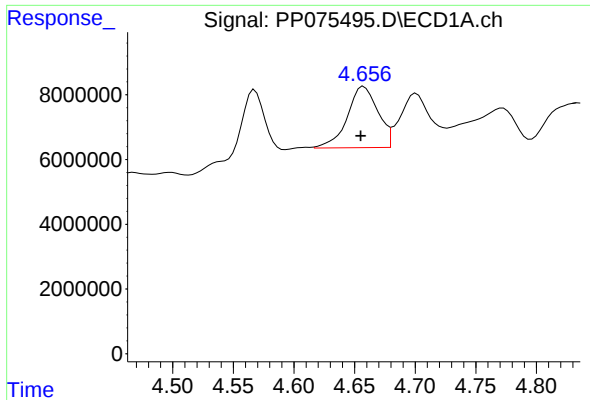


#1 Tetrachloro-m-xylene

R.T.: 4.656 min
Delta R.T.: 0.001 min
Response: 34871517
Conc: 26.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
92325


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/03/2025
Supervised By :mohammad ahmed 10/04/2025

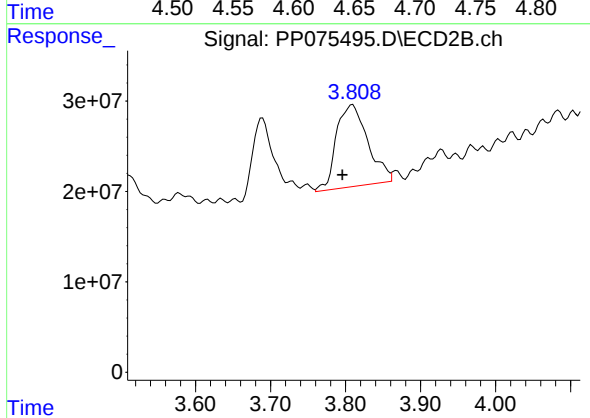


#1 Tetrachloro-m-xylene

R.T.: 3.810 min
Delta R.T.: 0.014 min
Response: 263663286
Conc: 43.22 ng/ml

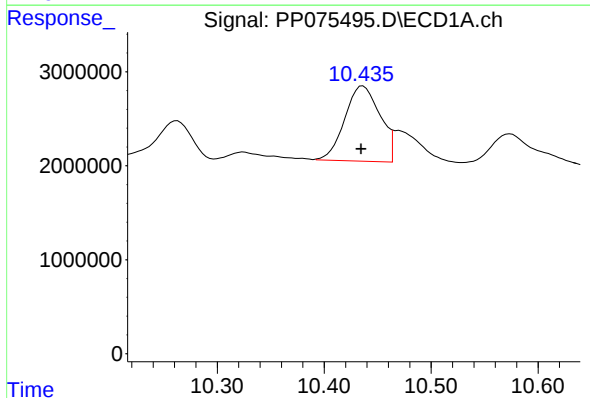

#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.000 min
Response: 18814699
Conc: 18.86 ng/ml m

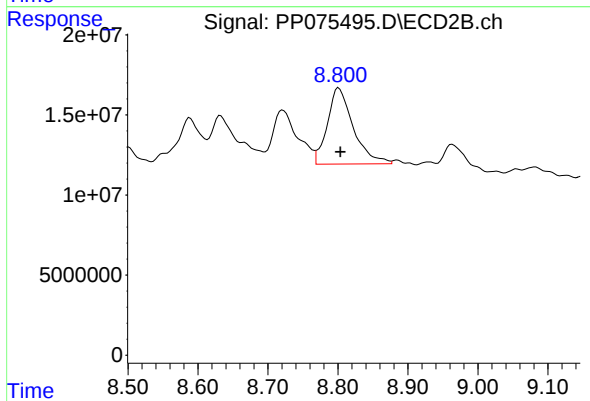

#2 Decachlorobiphenyl

R.T.: 8.801 min
Delta R.T.: -0.002 min
Response: 122543982
Conc: 20.31 ng/ml