

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100224\
 Data File : PP067446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2024 23:15
 Operator : YP\AJ
 Sample : P4258-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Chamberlain Ave

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/03/2024
 Supervised By :Ankita Jodhani 10/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 00:20:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 27 06:59:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.752	4.050	19247595	21181524	14.320	14.176
2) SA Decachlor...	10.660	9.217	19020608	18624385	13.102	13.515m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100224\
Data File : PP067446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2024 23:15
Operator : YP\AJ
Sample : P4258-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Chamberlain Ave


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/03/2024
Supervised By :Ankita Jodhani 10/03/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 00:20:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 27 06:59:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

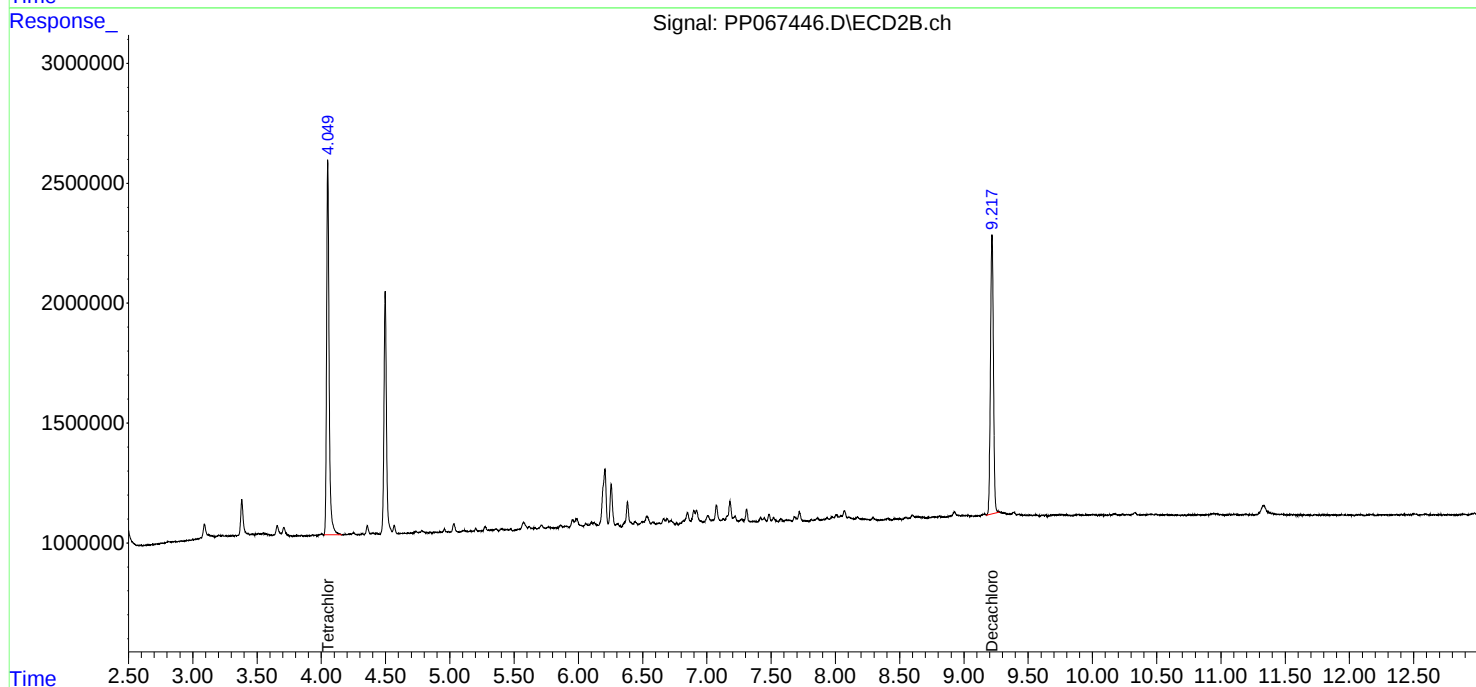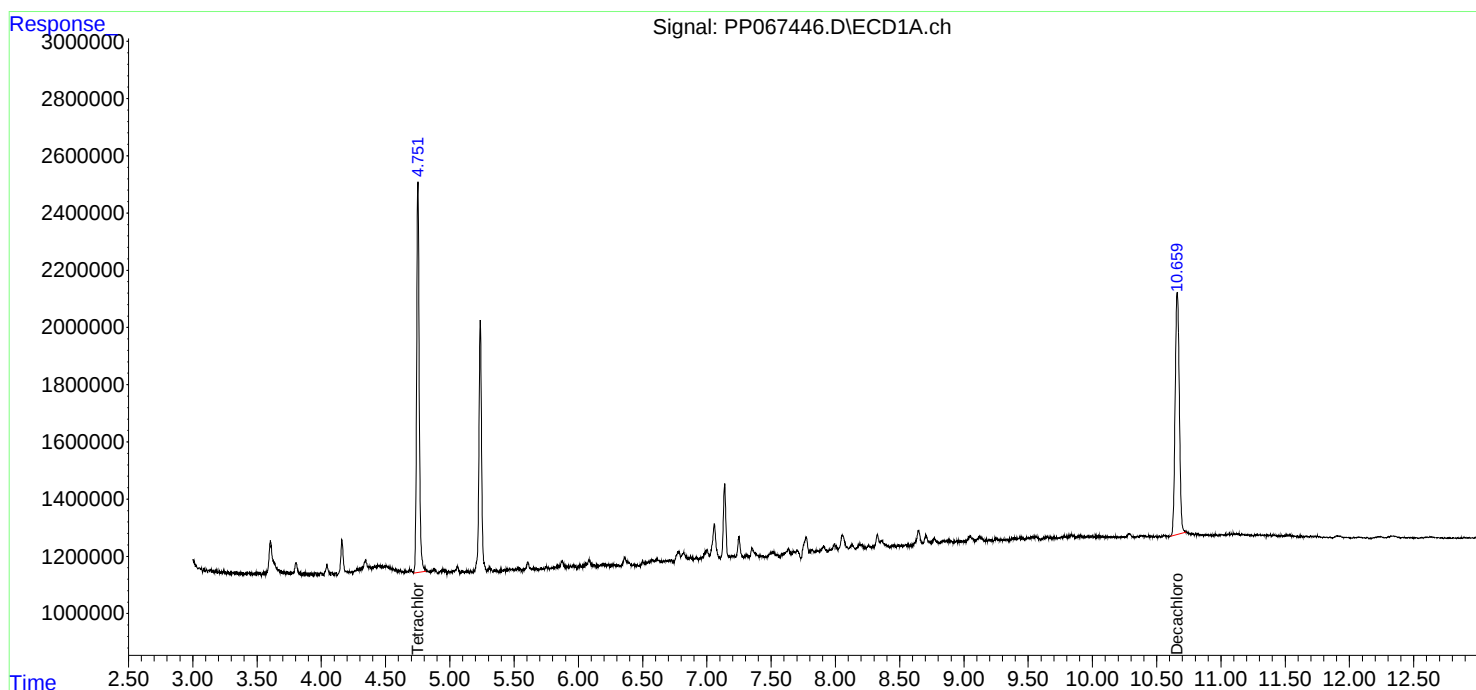

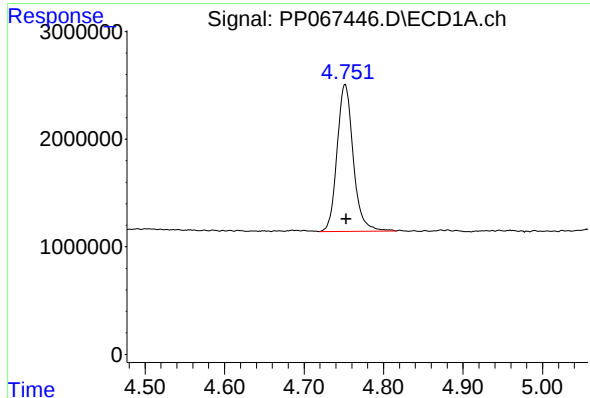


#1 Tetrachloro-m-xylene

R.T.: 4.752 min
Delta R.T.: -0.001 min
Response: 19247595
Conc: 14.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
Chamberlain Ave


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/03/2024
Supervised By :Ankita Jodhani 10/03/2024

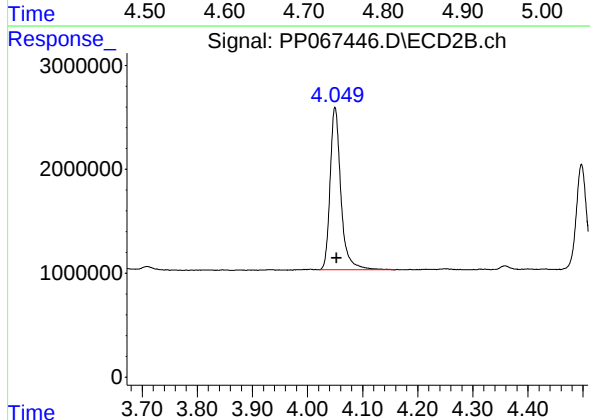


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.003 min
Response: 21181524
Conc: 14.18 ng/ml

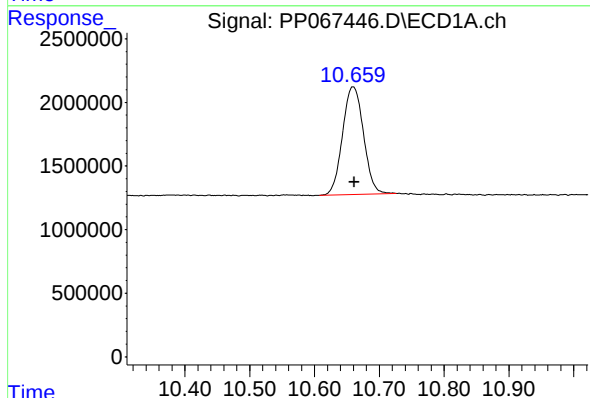

#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.002 min
Response: 19020608
Conc: 13.10 ng/ml

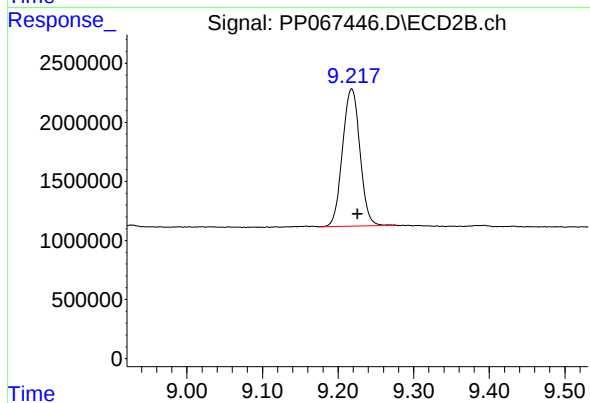

#2 Decachlorobiphenyl

R.T.: 9.217 min
Delta R.T.: -0.009 min
Response: 18624385
Conc: 13.52 ng/ml m