

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100318\
 Data File : PP027618.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2018 23:39
 Operator : EI\MA
 Sample : J5198-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 06:51:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092418.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 25 01:51:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.044	12.158	128.1E6	177.9E6	505.056	410.987
Target Compounds							
1) T	Dalapon	3.272	2.945	79780097	104.8E6	133.568	192.669 #
6) T	MCCP	12.726	0.000	27511994	0	62.330	N.D. #
7) T	MCPA	0.000	12.981	0	42287254	N.D.	31.498 #
8) T	DICHLORPROP	13.496	13.594	13354528	17852971	36.859	43.033
12) T	2,4,5-T	0.000	15.891	0	11083589	N.D.	5.601 #
13) T	2,4-DB	0.000	16.553	0	2036998	N.D.	8.375 #
14) T	DINOSEB	17.833	0.000	9482322	0	4.926	N.D. #
15) T	Picloram	17.612	18.276	2133445	7008744	0.694	2.800 #
16) T	DCPA	0.000	18.147	0	19406504	N.D.	6.079 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100318\
Data File : PP027618.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2018 23:39
Operator : EI\MA
Sample : J5198-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 06:51:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092418.M
Quant Title : 8080.M
QLast Update : Tue Sep 25 01:51:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

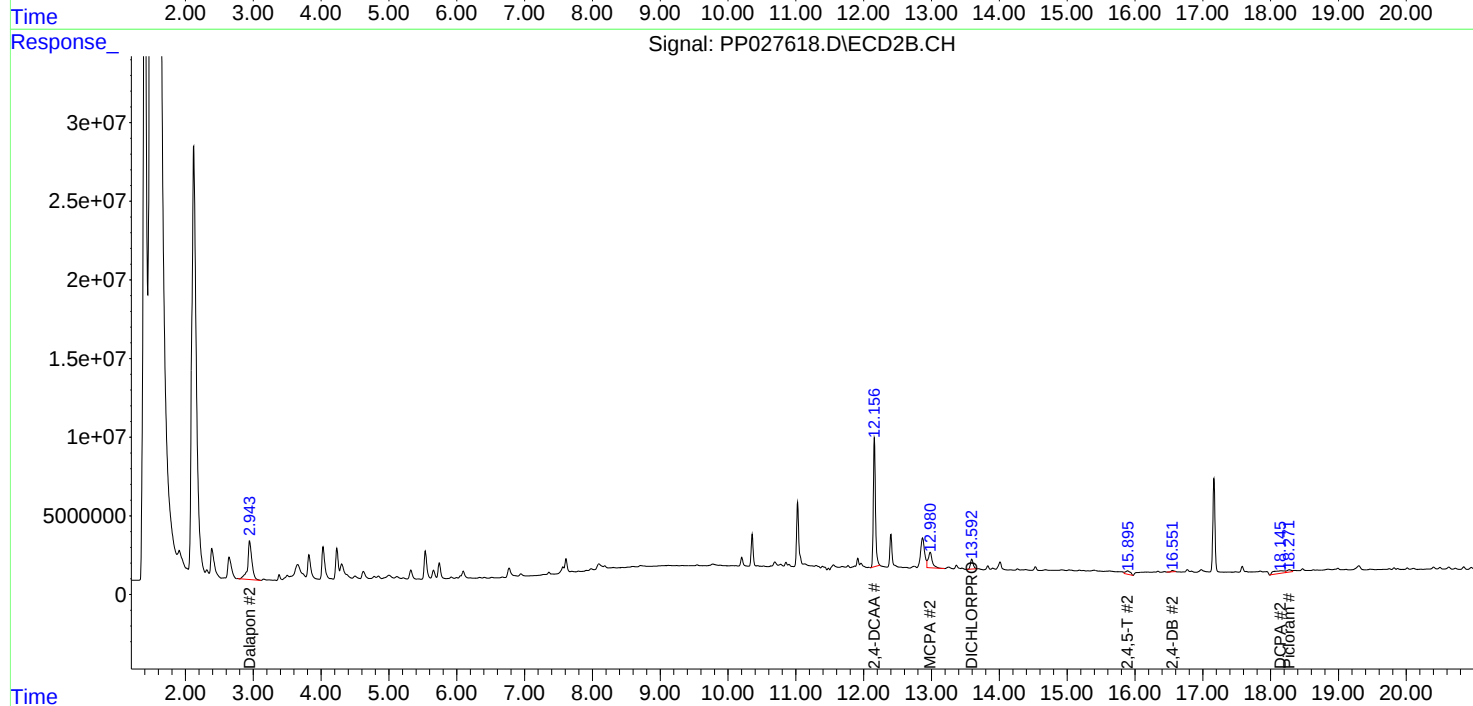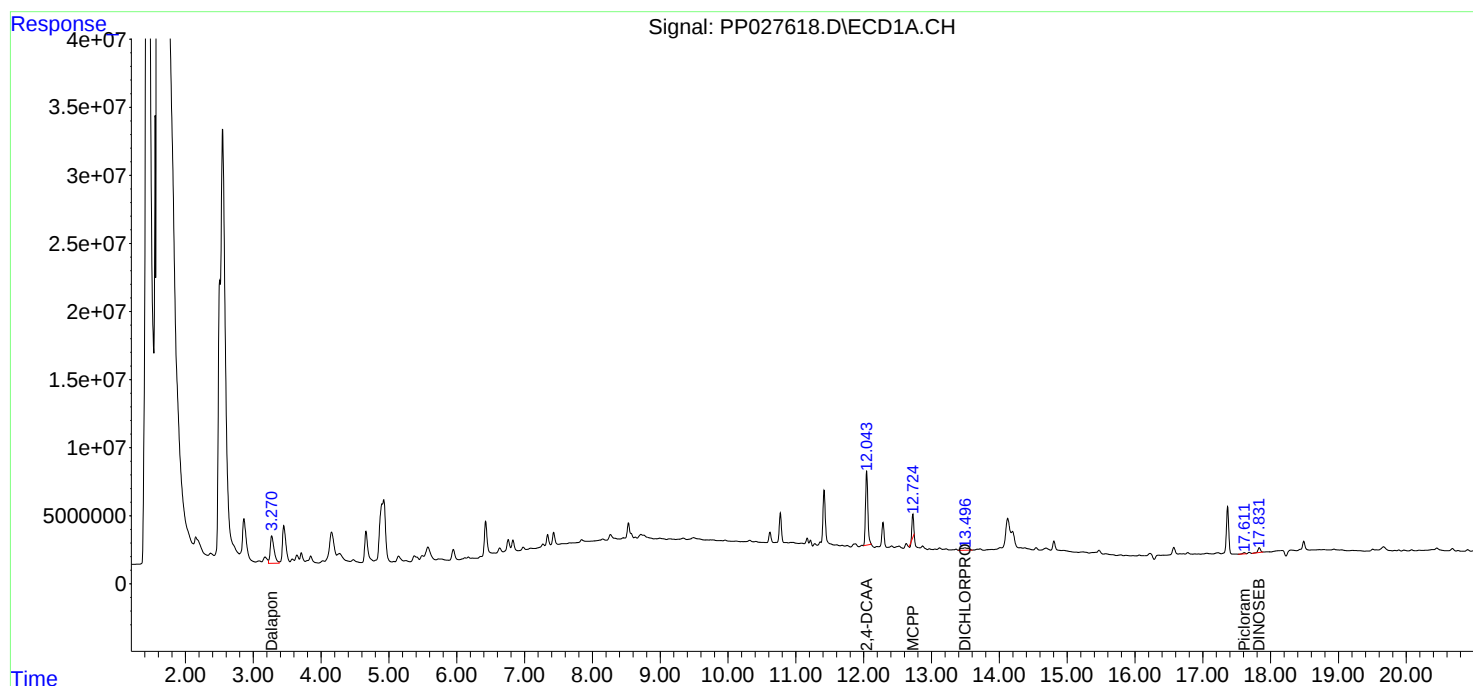


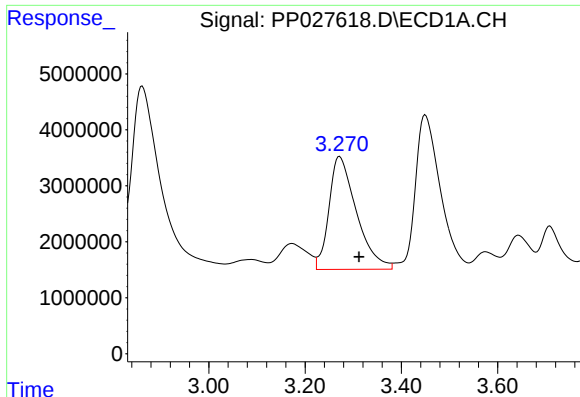

#1 Dalapon


R.T.: 3.272 min
Delta R.T.: -0.040 min
Response: 79780097
Conc: 133.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

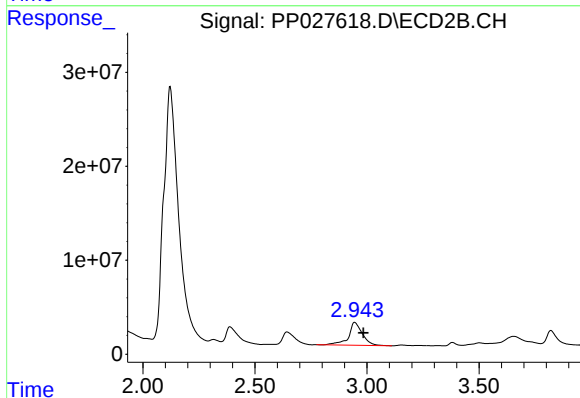


#1 Dalapon

R.T.: 2.945 min
Delta R.T.: -0.038 min
Response: 104791883
Conc: 192.67 ng/ml

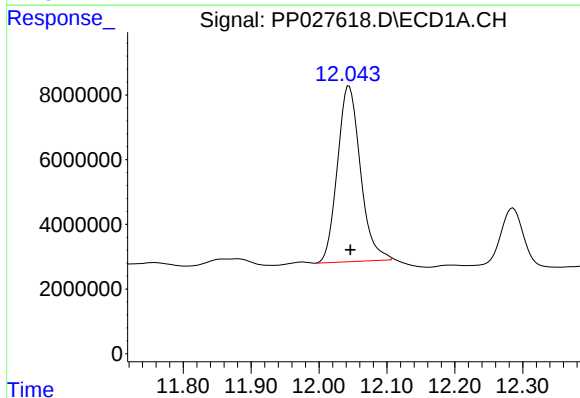


#4 2,4-DCAA

R.T.: 12.044 min
Delta R.T.: -0.002 min
Response: 128089459
Conc: 505.06 ng/ml

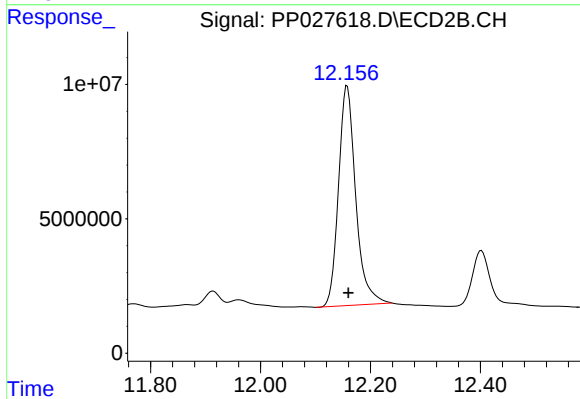

#4 2,4-DCAA


R.T.: 12.158 min
Delta R.T.: -0.002 min
Response: 177886402
Conc: 410.99 ng/ml

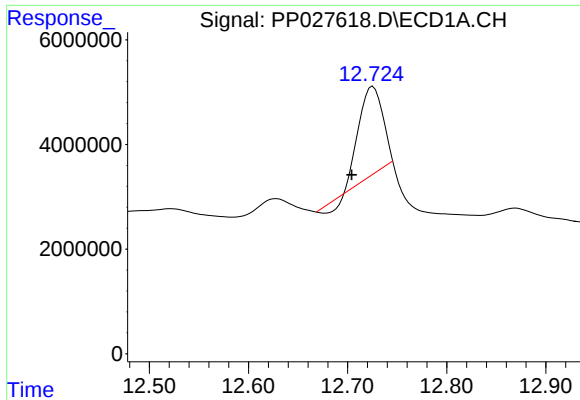

#6 MCP


R.T.: 12.726 min
Delta R.T.: 0.021 min
Response: 27511994
Conc: 62.33 ug/ml

Instrument :
ECD_P
ClientSampleId :

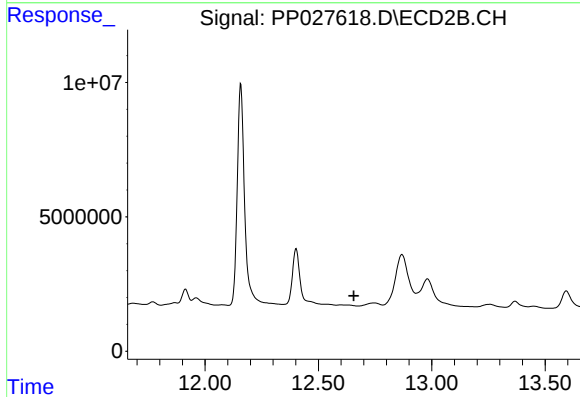


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.656 min
Response: 0
Conc: N.D.

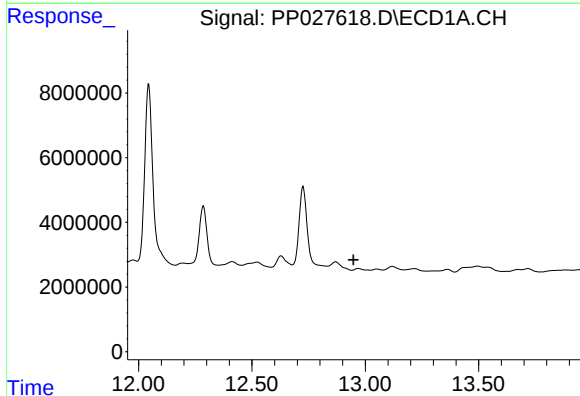


#7 MCP

R.T.: 0.000 min
Exp R.T. : 12.948 min
Response: 0
Conc: N.D.

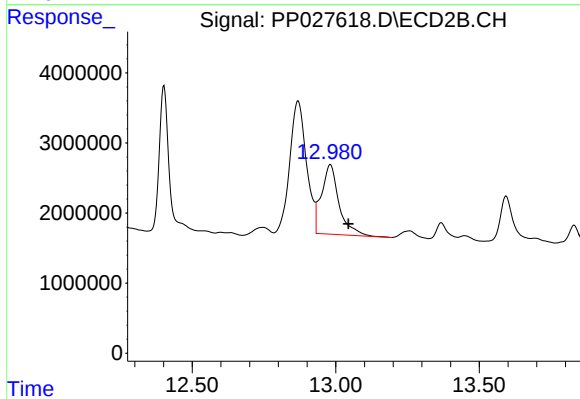

#7 MCP


R.T.: 12.981 min
Delta R.T.: -0.063 min
Response: 42287254
Conc: 31.50 ug/ml

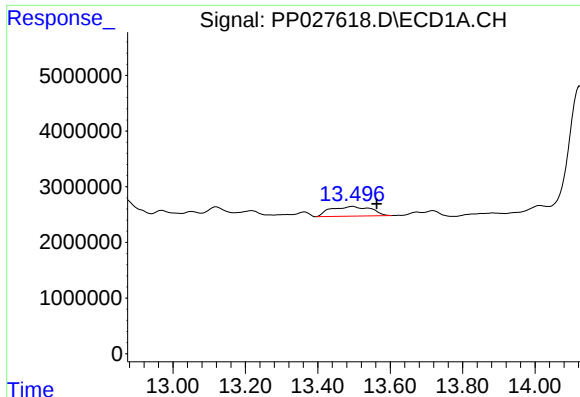

#8 DICHLORPROP


R.T.: 13.496 min
Delta R.T.: -0.067 min
Response: 13354528
Conc: 36.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

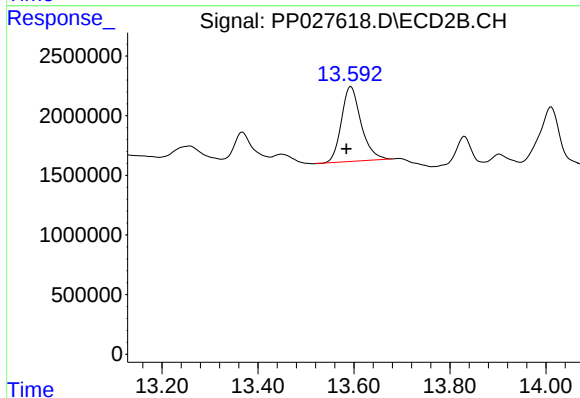


#8 DICHLORPROP

R.T.: 13.594 min
Delta R.T.: 0.009 min
Response: 17852971
Conc: 43.03 ng/ml

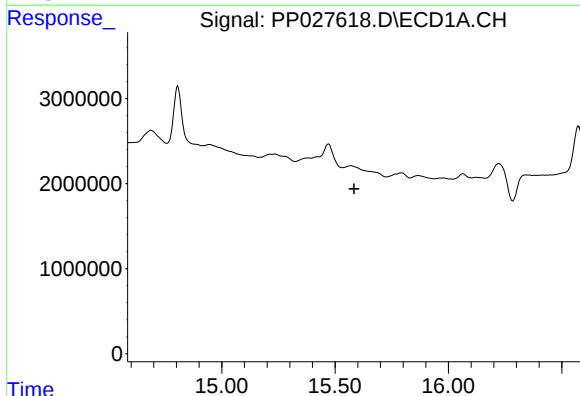


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.584 min
Response: 0
Conc: N.D.

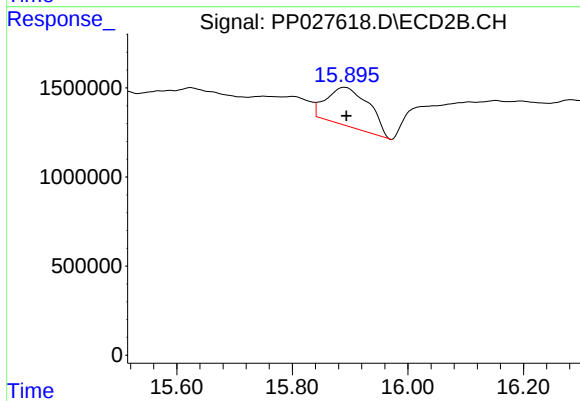

#12 2,4,5-T


R.T.: 15.891 min
Delta R.T.: -0.003 min
Response: 11083589
Conc: 5.60 ng/ml

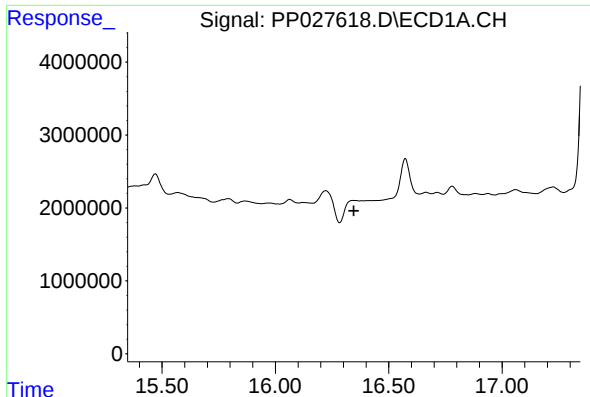

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

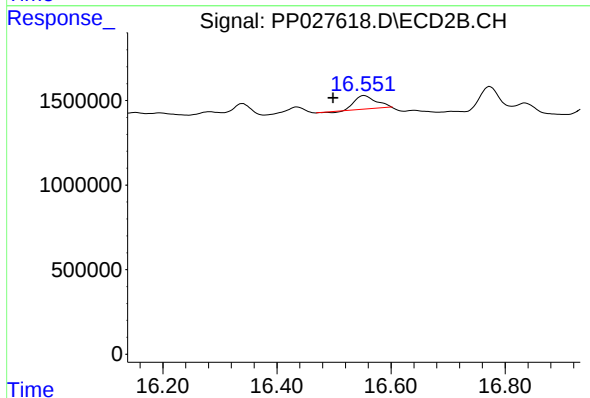


#13 2,4-DB

R.T.: 16.553 min
Delta R.T.: 0.055 min
Response: 2036998
Conc: 8.38 ng/ml

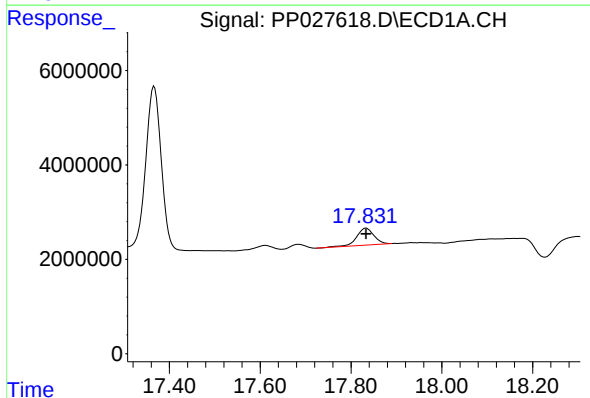


#14 DINOSEB

R.T.: 17.833 min
Delta R.T.: 0.000 min
Response: 9482322
Conc: 4.93 ng/ml

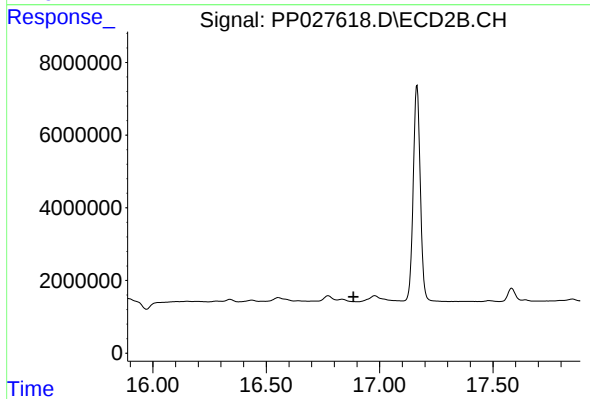

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.885 min
Response: 0
Conc: N.D.

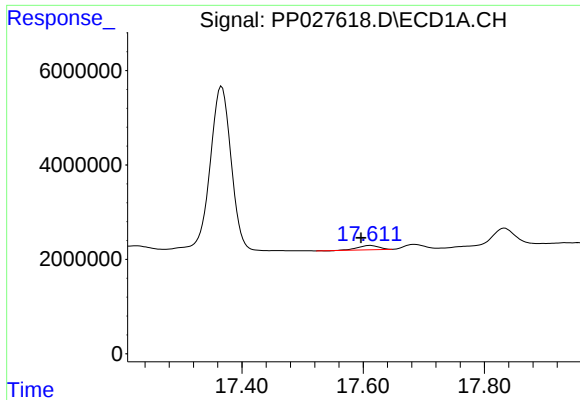

#15 Picloram


R.T.: 17.612 min
Delta R.T.: 0.015 min
Response: 2133445
Conc: 0.69 ng/ml

Instrument :
ECD_P
ClientSampleId :

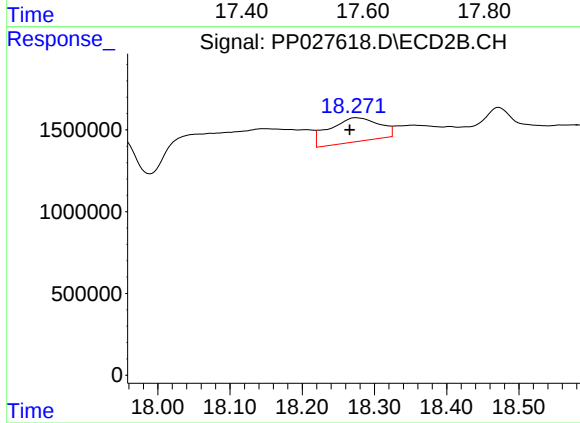


#15 Picloram

R.T.: 18.276 min
Delta R.T.: 0.010 min
Response: 7008744
Conc: 2.80 ng/ml

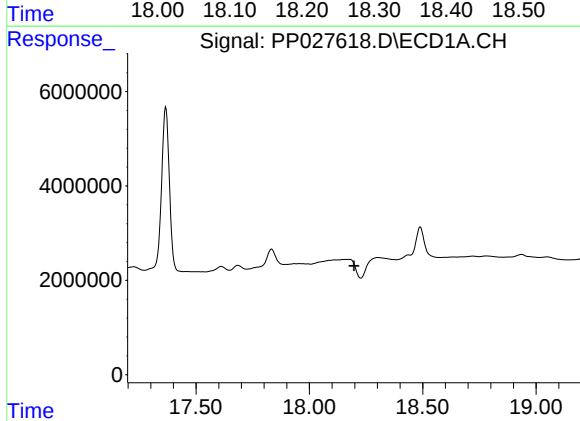

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.197 min
Response: 0
Conc: N.D.

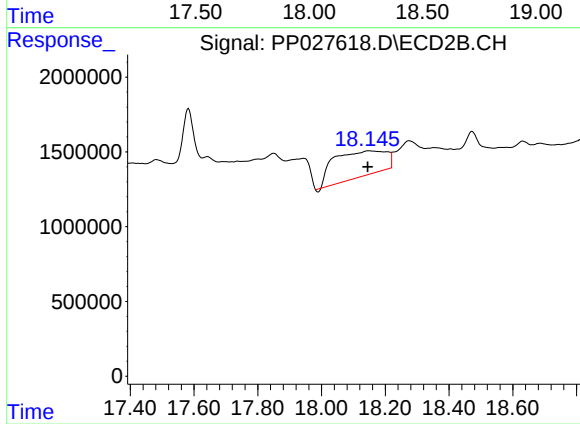

#16 DCPA

R.T.: 18.147 min
Delta R.T.: 0.002 min
Response: 19406504
Conc: 6.08 ng/ml