

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
 Data File : PP051825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 15:23
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 17:53:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 03 17:53:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.674	93337530	64983741	50.000	50.000
2) SA Decachlor...	10.241	8.771	62066885	62181058	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.632	3.892	10778297	7830988	500.000	500.000
9) L2 AR-1221-2	4.719	3.979	7970236	5973635	500.000	500.000
10) L2 AR-1221-3	4.795	4.056	24211292	18758279	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
Data File : PP051825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 15:23
Operator : YP\AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 17:53:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 03 17:53:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

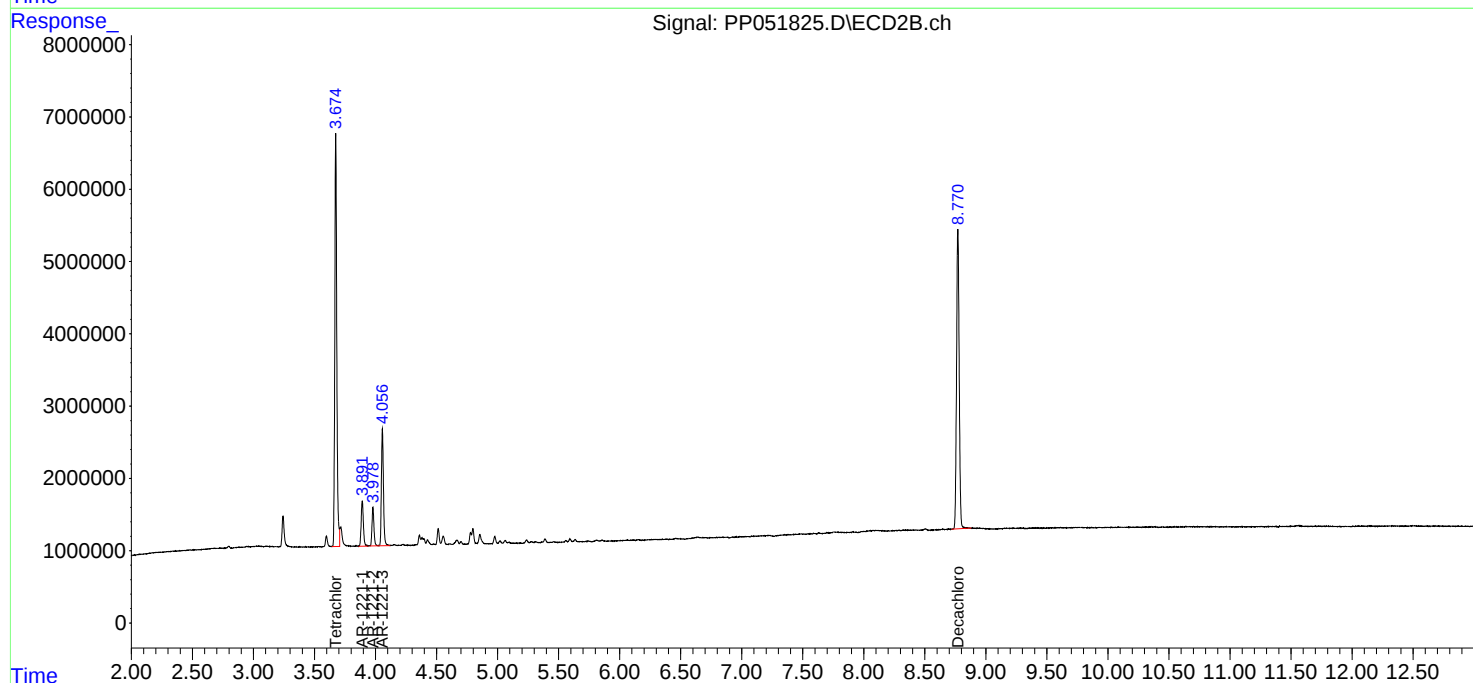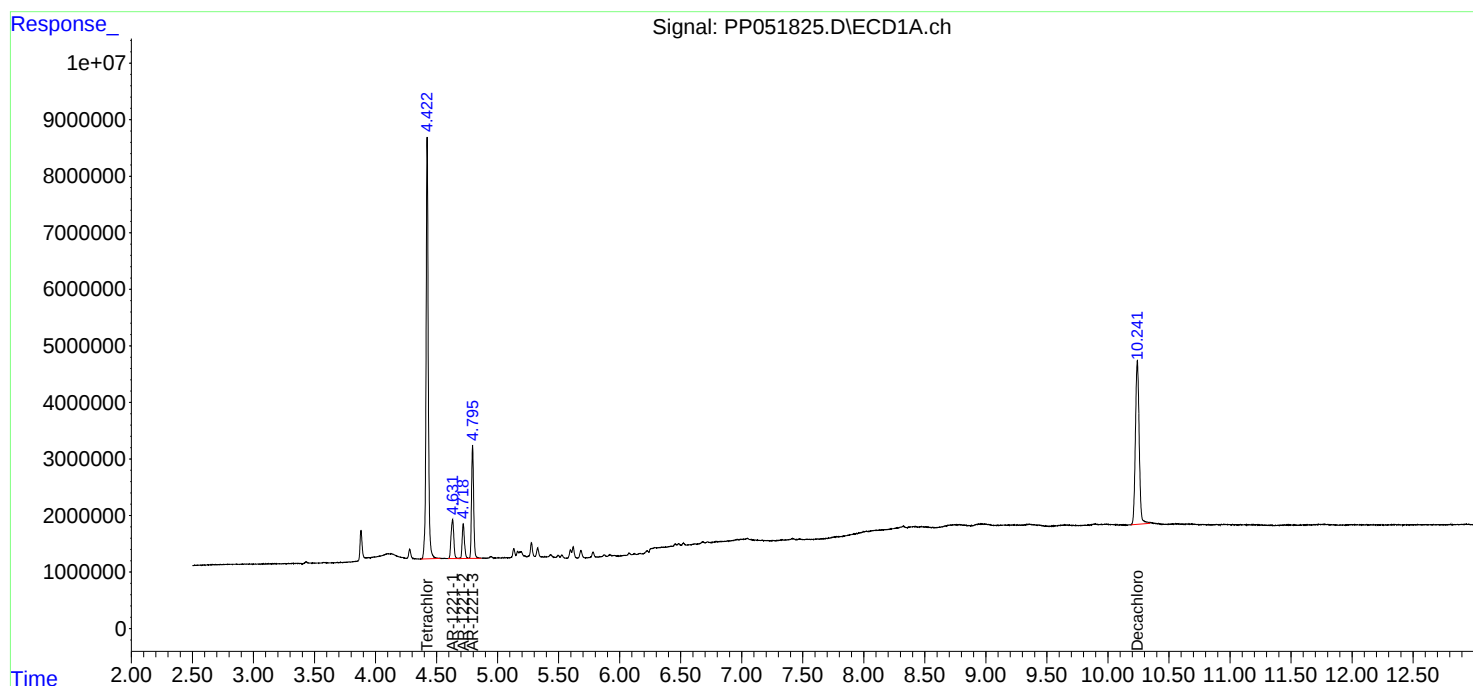


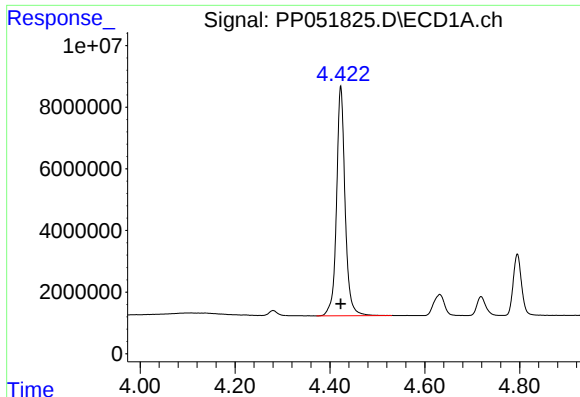

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: 0.000 min
Response: 93337530
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

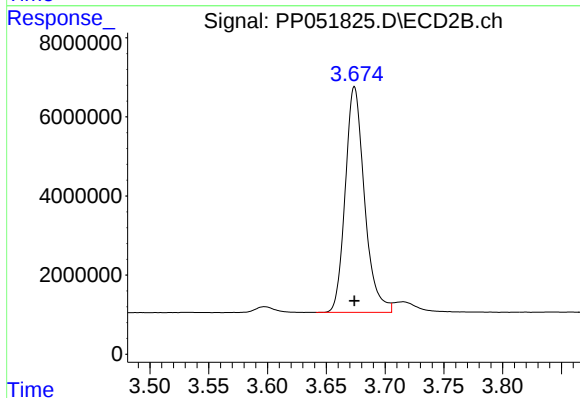


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: 0.000 min
Response: 64983741
Conc: 50.00 ng/ml

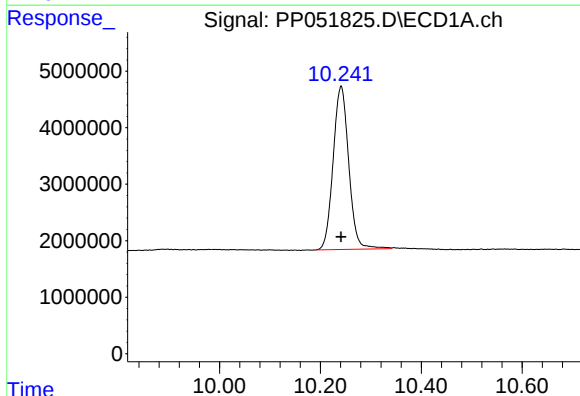


#2 Decachlorobiphenyl

R.T.: 10.241 min
Delta R.T.: 0.000 min
Response: 62066885
Conc: 50.00 ng/ml

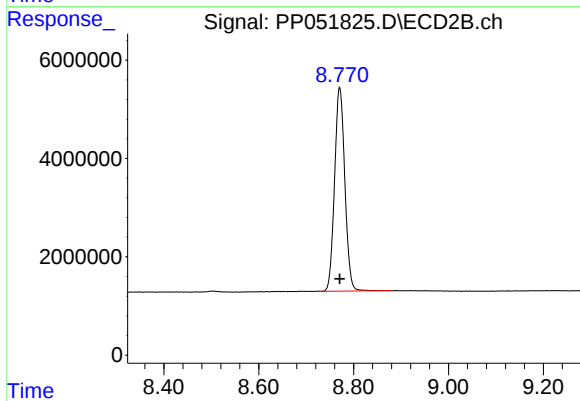

#2 Decachlorobiphenyl


R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 62181058
Conc: 50.00 ng/ml

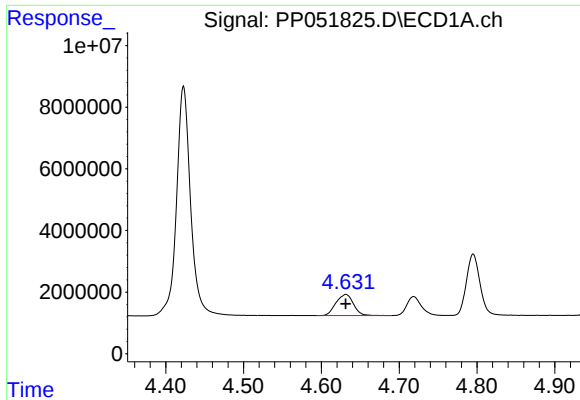

#8 AR-1221-1


R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 10778297
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

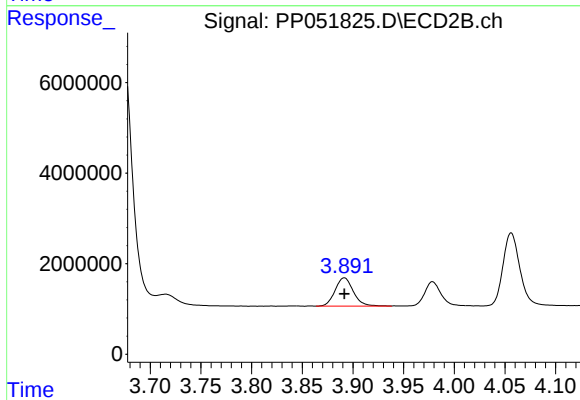


#8 AR-1221-1

R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 7830988
Conc: 500.00 ng/ml

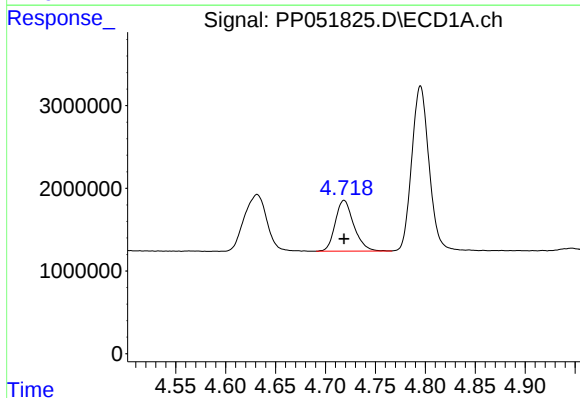


#9 AR-1221-2

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 7970236
Conc: 500.00 ng/ml

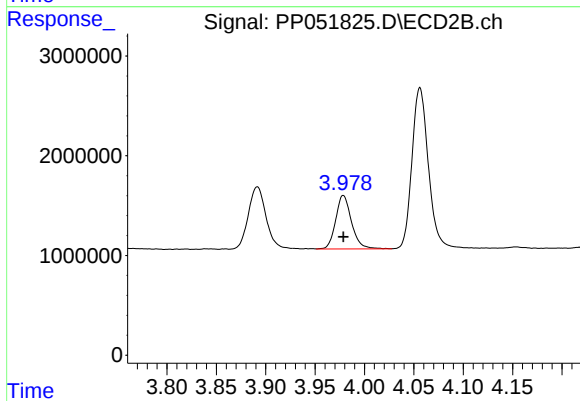

#9 AR-1221-2


R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 5973635
Conc: 500.00 ng/ml

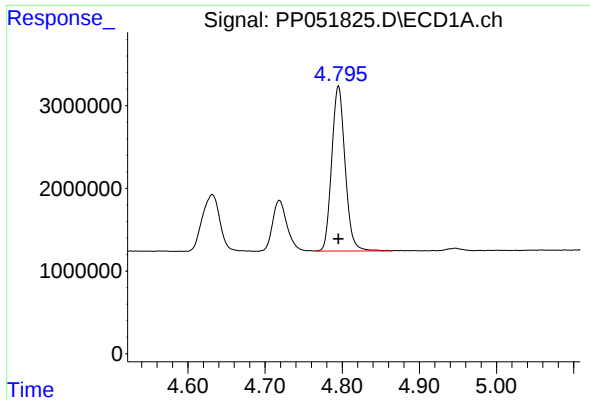

#10 AR-1221-3

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 24211292
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

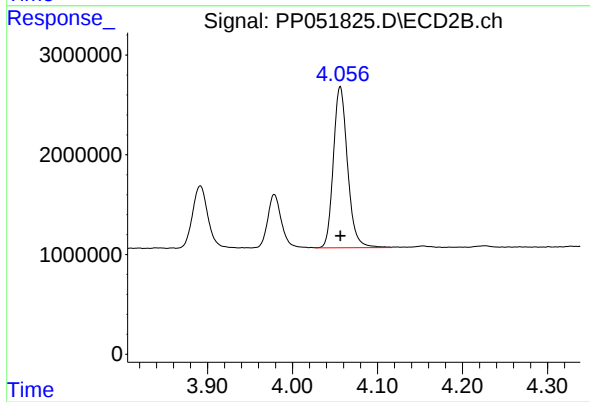

#10 AR-1221-3

R.T.: 4.056 min
Delta R.T.: 0.000 min
Response: 18758279
Conc: 500.00 ng/ml