

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
 Data File : PP051865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 02:51
 Operator : YP\AJ
 Sample : N4888-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BUS-WORK-FOUNDATION-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:03:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 03:12:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.422	3.673	43141566	31183544	24.138	24.528
2)	SA Decachlor...	10.238	8.769	32055809	31997881	26.442	27.091
Target Compounds							
3)	L1 AR-1016-1	5.617f	0.000	82349	0	1.817	N.D. #
4)	L1 AR-1016-2	5.617	0.000	82349	0	1.283	N.D. #
5)	L1 AR-1016-3	5.682	0.000	32168	0	0.805	N.D. #
6)	L1 AR-1016-4	5.788	0.000	15038	0	0.429	N.D. #
7)	L1 AR-1016-5	6.080	5.225	50256	208804	1.217	6.063 #
8)	L2 AR-1221-1	4.630	0.000	992947	0	46.062	N.D. #
9)	L2 AR-1221-2	4.729	3.978	573395	1453377	35.971	121.649 #
10)	L2 AR-1221-3	4.810f	4.053	384880	1793359	7.948	47.802 #
11)	L3 AR-1232-1	4.810	4.053	384880	1793359	9.592	57.610 #
12)	L3 AR-1232-2	5.349f	0.000	1115879	0	59.462	N.D. #
13)	L3 AR-1232-3	5.617	0.000	82349	0	2.773	N.D. #
14)	L3 AR-1232-4	5.788	0.000	15038	0	1.051	N.D. #
15)	L3 AR-1232-5	5.883	5.225	239465	208804	20.015	14.139 #
16)	L4 AR-1242-1	5.617f	0.000	82349	0	2.009	N.D. #
17)	L4 AR-1242-2	5.617	0.000	82349	0	1.432	N.D. #
18)	L4 AR-1242-3	5.682	0.000	32168	0	0.898	N.D. #
19)	L4 AR-1242-4	5.788	0.000	15038	0	0.522	N.D. #
20)	L4 AR-1242-5	6.516	5.617f	242706	270064	6.444	7.398
21)	L5 AR-1248-1	5.617f	0.000	82349	0	2.719	N.D. #
22)	L5 AR-1248-2	5.883	0.000	239465	0	5.285	N.D. #
23)	L5 AR-1248-3	6.080	0.000	50256	0	0.990	N.D. #
24)	L5 AR-1248-4	6.487	5.225	173621	208804	2.599	4.160 #
25)	L5 AR-1248-5	6.516	5.617f	242706	270064	3.693	5.509 #
26)	L6 AR-1254-1	6.455	5.617f	374316	270064	5.486	3.630 #
27)	L6 AR-1254-2	6.678	0.000	274394	0	2.681	N.D. #
28)	L6 AR-1254-3	7.043	6.152	282954	341304	2.764	3.242
29)	L6 AR-1254-4	7.329	0.000	101089	0	1.409	N.D. #
30)	L6 AR-1254-5	7.748	6.805	176410	262339	2.345	2.836
31)	L7 AR-1260-1	7.202	0.000	125561	0	1.766	N.D. #
32)	L7 AR-1260-2	7.468	6.460	264279	262377	3.236	3.118
33)	L7 AR-1260-3	7.834	0.000	254253	0	4.445	N.D. #
34)	L7 AR-1260-4	8.060	0.000	35530	0	0.542	N.D. #
35)	L7 AR-1260-5	8.376	0.000	84925	0	0.668	N.D. #
36)	L8 AR-1262-1	7.834	0.000	254253	0	2.924	N.D. #
37)	L8 AR-1262-2	8.376	0.000	84925	0	0.576	N.D. #
38)	L8 AR-1262-3	8.692	7.636	17068	299475	0.166	4.270 #
39)	L8 AR-1262-4	8.788	7.708	203101	121581	4.412	0.973 #
40)	L8 AR-1262-5	9.456	8.203	199661	197088	3.504	3.479
41)	L9 AR-1268-1	8.692	7.636	17068	299475	0.096	1.509 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
 Data File : PP051865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 02:51
 Operator : YP\AJ
 Sample : N4888-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 BUS-WORK-FOUNDATION-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:03:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 03:12:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.788	7.708	203101	121581	1.225	0.680 #
43) L9	AR-1268-3	9.035	0.000	219934	0	1.534	N.D. #
44) L9	AR-1268-4	9.456	8.203	199661	197088	3.117	3.140
45) L9	AR-1268-5	9.889	0.000	69898	0	0.152	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

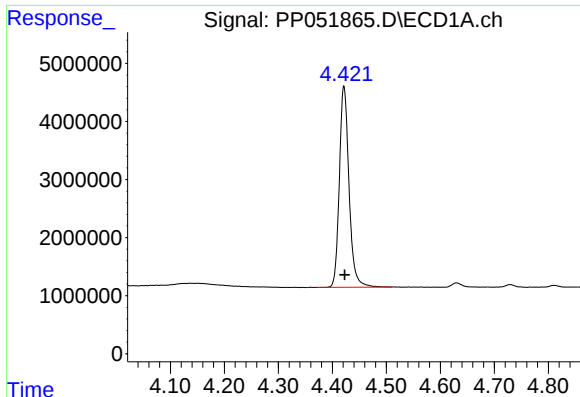

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: -0.001 min
Response: 43141566
Conc: 24.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

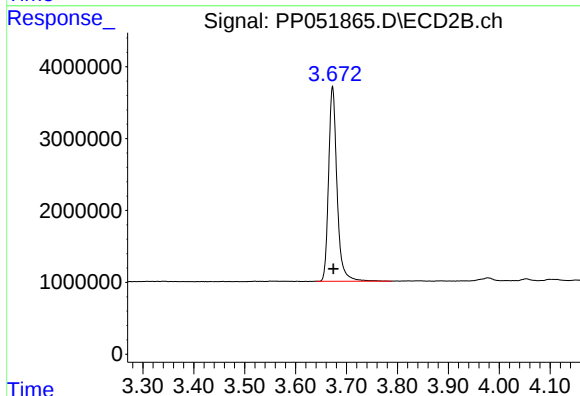


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.001 min
Response: 31183544
Conc: 24.53 ng/ml

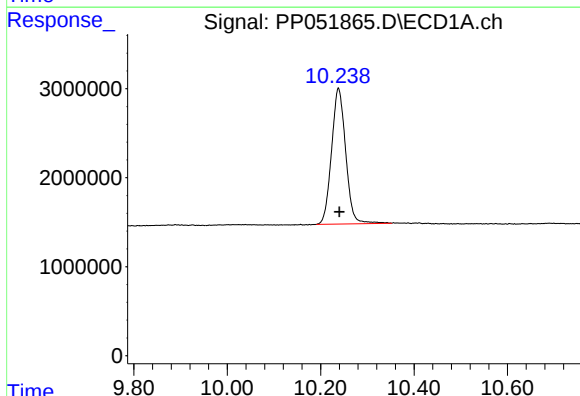


#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: -0.002 min
Response: 32055809
Conc: 26.44 ng/ml

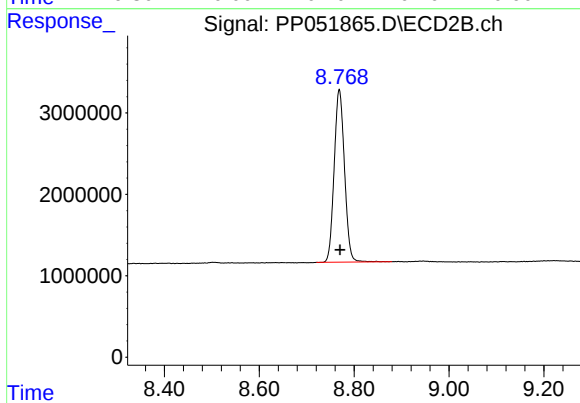

#2 Decachlorobiphenyl


R.T.: 8.769 min
Delta R.T.: -0.002 min
Response: 31997881
Conc: 27.09 ng/ml

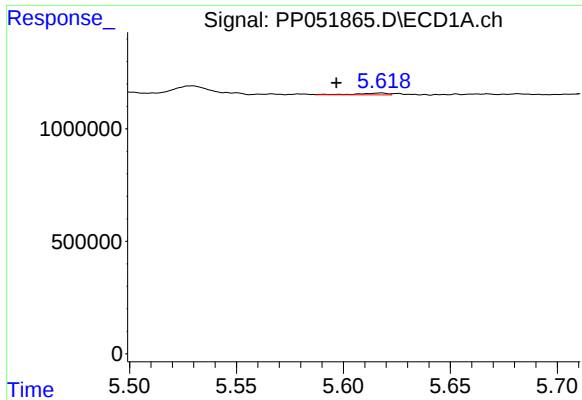

#3 AR-1016-1


R.T.: 5.617 min
Delta R.T.: 0.021 min
Response: 82349
Conc: 1.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

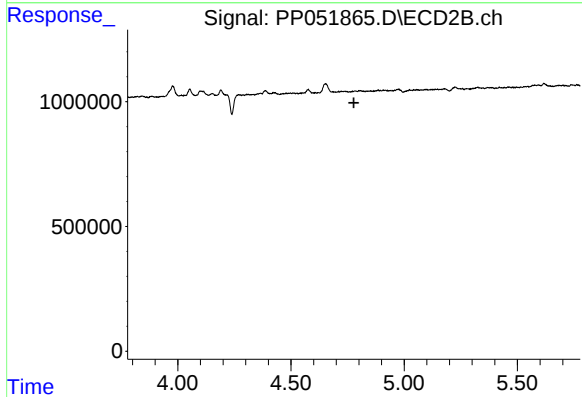


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.778 min
Response: 0
Conc: N.D.

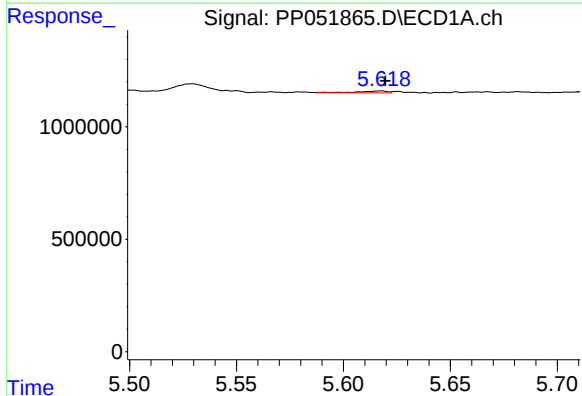


#4 AR-1016-2

R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 82349
Conc: 1.28 ng/ml

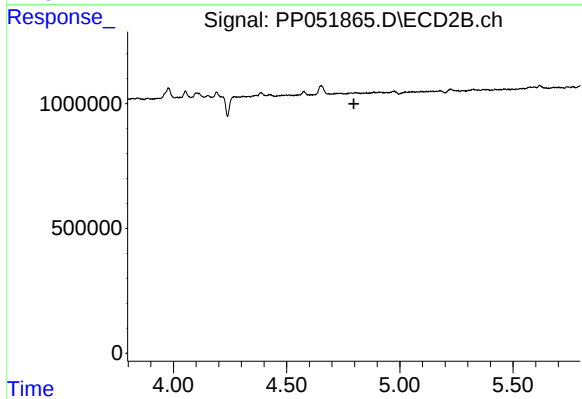

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.797 min
Response: 0
Conc: N.D.

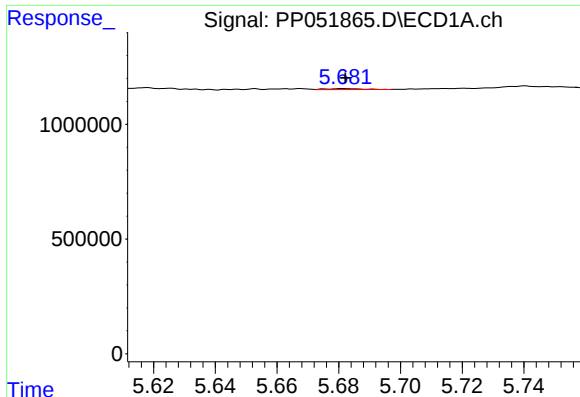

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 32168
Conc: 0.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

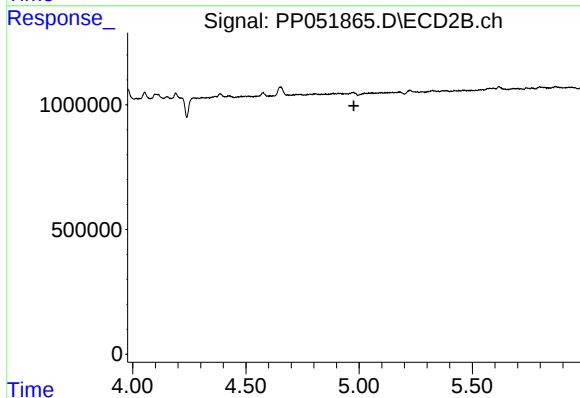


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.977 min
Response: 0
Conc: N.D.

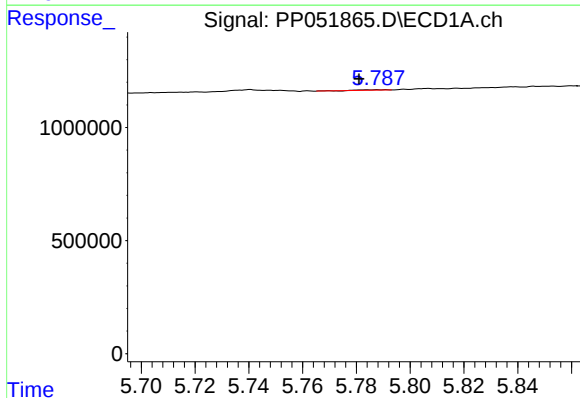


#6 AR-1016-4

R.T.: 5.788 min
Delta R.T.: 0.007 min
Response: 15038
Conc: 0.43 ng/ml

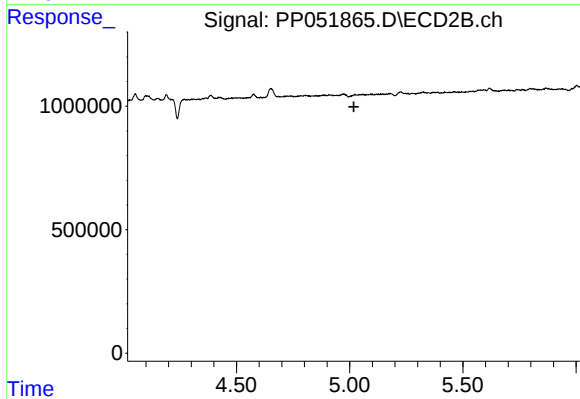

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

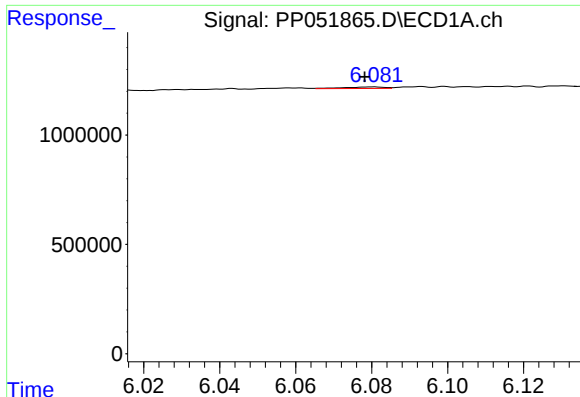

#7 AR-1016-5


R.T.: 6.080 min
Delta R.T.: 0.002 min
Response: 50256
Conc: 1.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

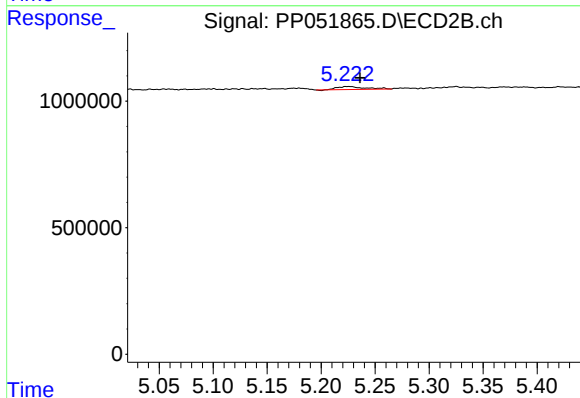


#7 AR-1016-5

R.T.: 5.225 min
Delta R.T.: -0.011 min
Response: 208804
Conc: 6.06 ng/ml

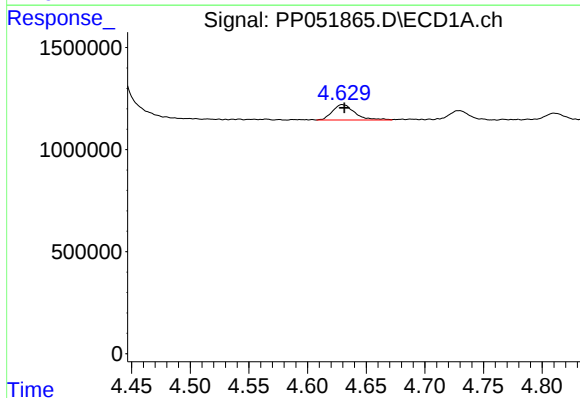


#8 AR-1221-1

R.T.: 4.630 min
Delta R.T.: -0.002 min
Response: 992947
Conc: 46.06 ng/ml

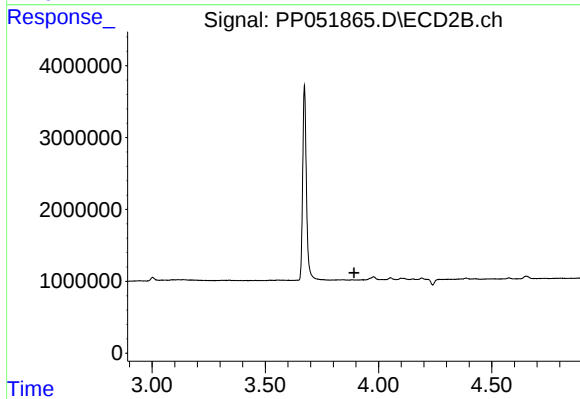

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.892 min
Response: 0
Conc: N.D.

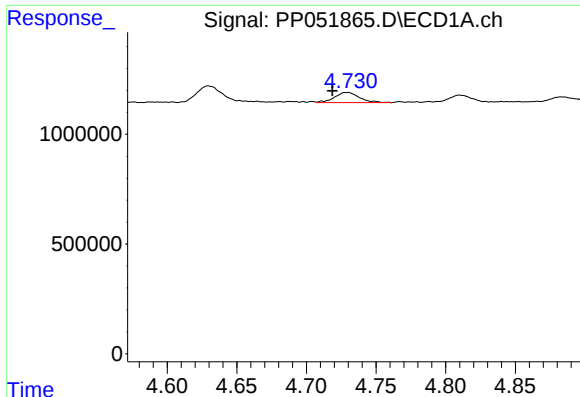

#9 AR-1221-2


R.T.: 4.729 min
Delta R.T.: 0.010 min
Response: 573395
Conc: 35.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

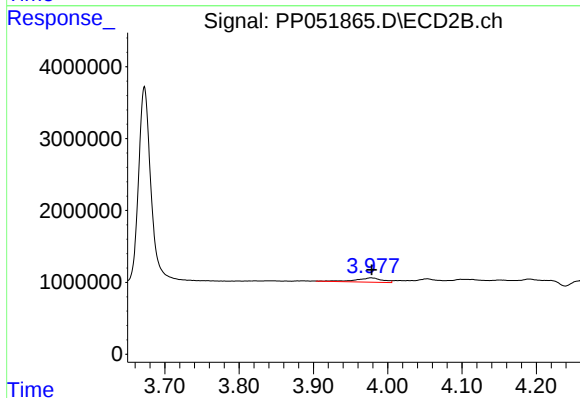


#9 AR-1221-2

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 1453377
Conc: 121.65 ng/ml

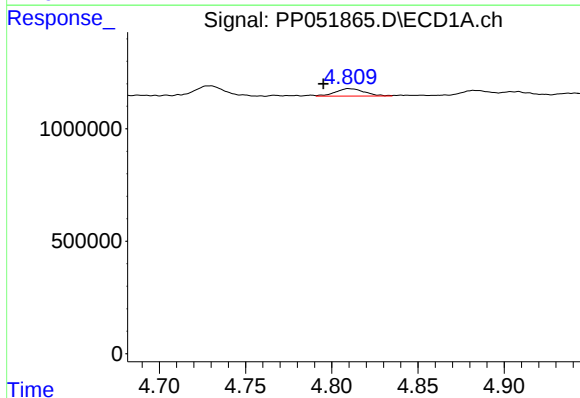


#10 AR-1221-3

R.T.: 4.810 min
Delta R.T.: 0.015 min
Response: 384880
Conc: 7.95 ng/ml

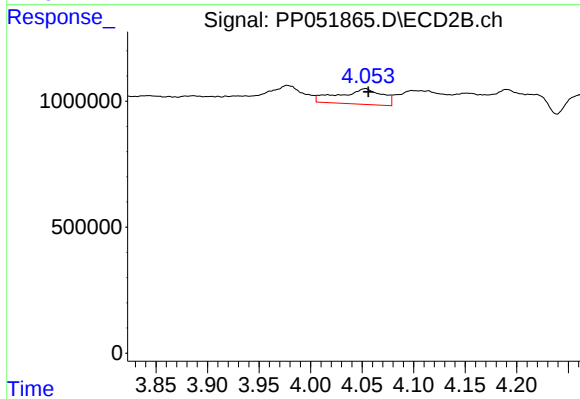

#10 AR-1221-3


R.T.: 4.053 min
Delta R.T.: -0.003 min
Response: 1793359
Conc: 47.80 ng/ml

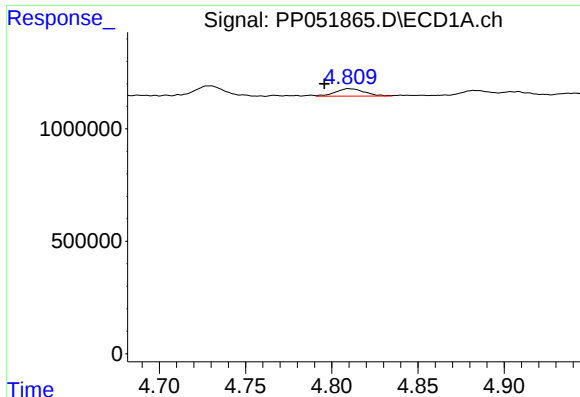

#11 AR-1232-1


R.T.: 4.810 min
Delta R.T.: 0.015 min
Response: 384880
Conc: 9.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

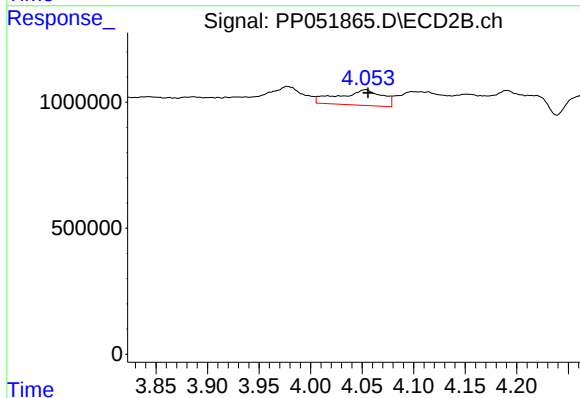


#11 AR-1232-1

R.T.: 4.053 min
Delta R.T.: -0.003 min
Response: 1793359
Conc: 57.61 ng/ml

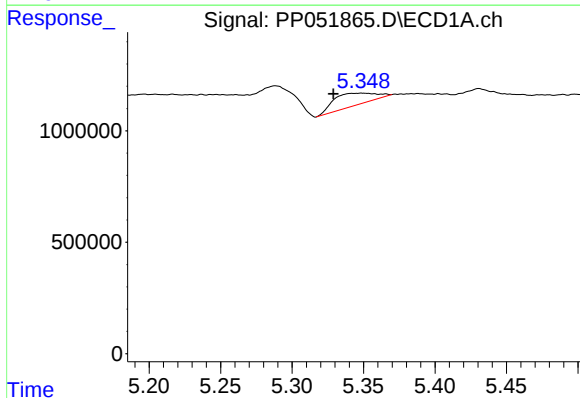


#12 AR-1232-2

R.T.: 5.349 min
Delta R.T.: 0.020 min
Response: 1115879
Conc: 59.46 ng/ml

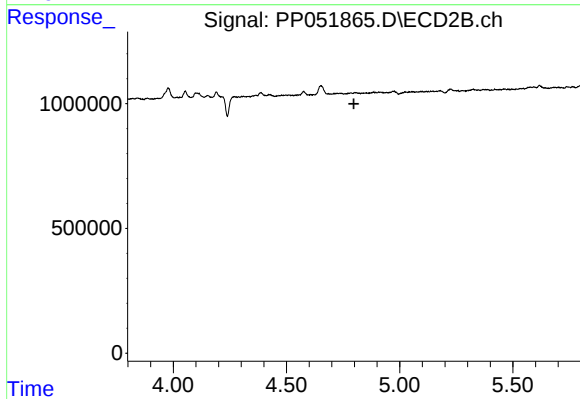

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.797 min
Response: 0
Conc: N.D.

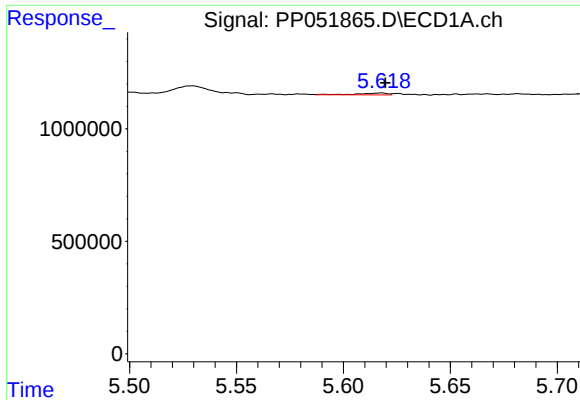

#13 AR-1232-3


R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 82349
Conc: 2.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

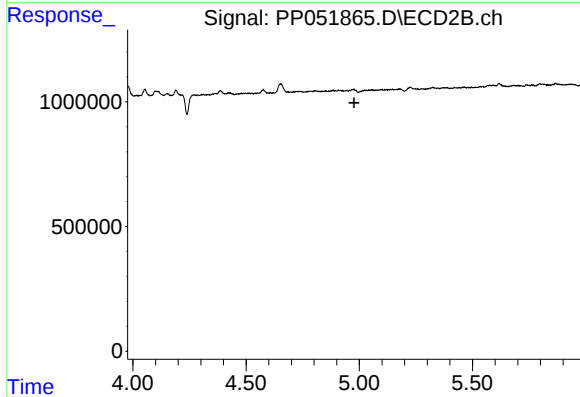


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.977 min
Response: 0
Conc: N.D.

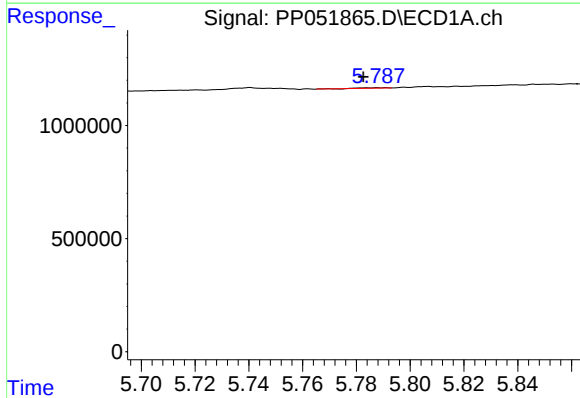


#14 AR-1232-4

R.T.: 5.788 min
Delta R.T.: 0.005 min
Response: 15038
Conc: 1.05 ng/ml

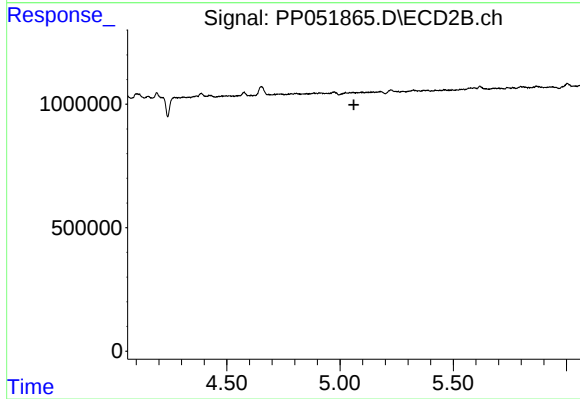

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.061 min
Response: 0
Conc: N.D.

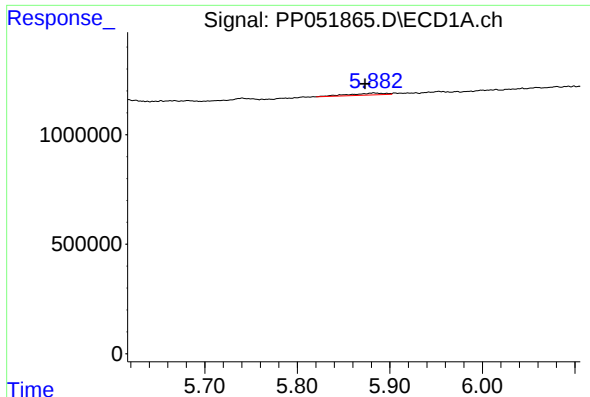

#15 AR-1232-5


R.T.: 5.883 min
Delta R.T.: 0.009 min
Response: 239465
Conc: 20.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

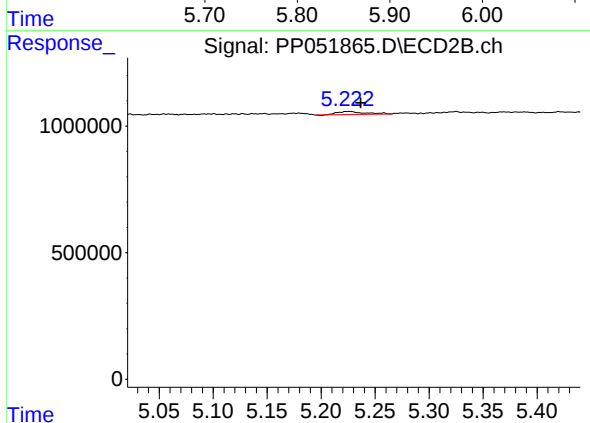


#15 AR-1232-5

R.T.: 5.225 min
Delta R.T.: -0.011 min
Response: 208804
Conc: 14.14 ng/ml

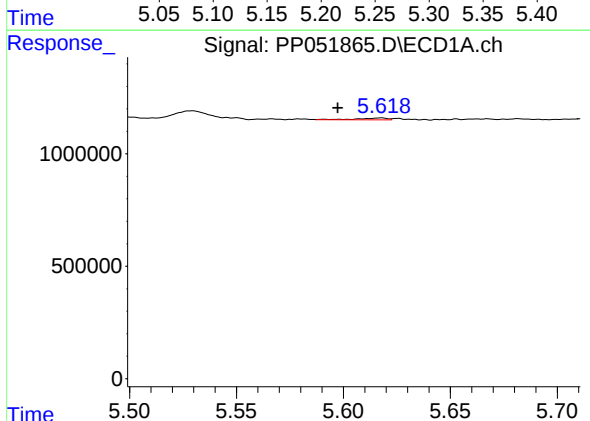


#16 AR-1242-1

R.T.: 5.617 min
Delta R.T.: 0.020 min
Response: 82349
Conc: 2.01 ng/ml

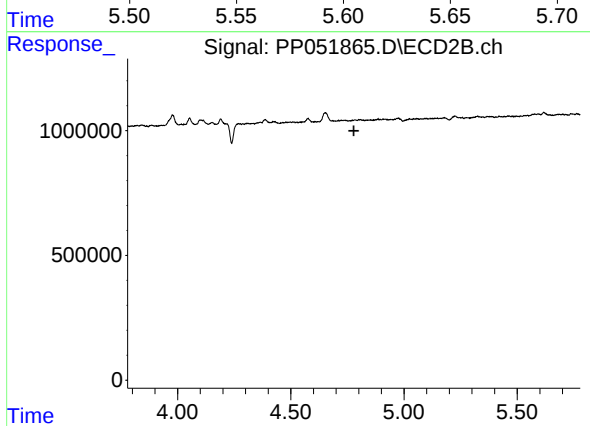

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 4.778 min
Response: 0
Conc: N.D.

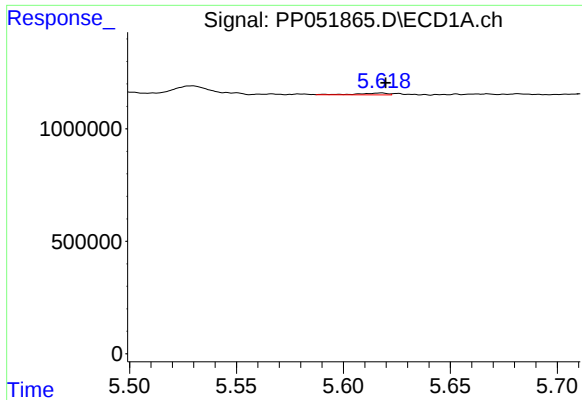

#17 AR-1242-2


R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 82349
Conc: 1.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

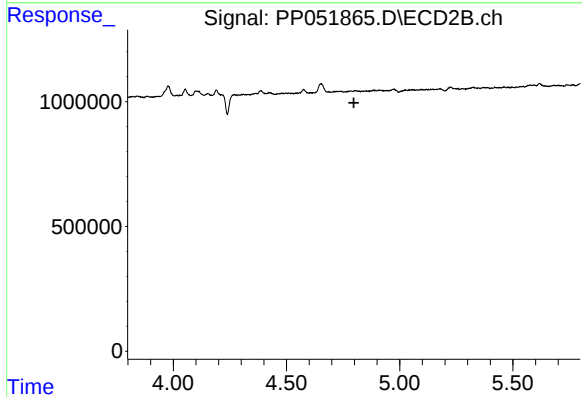


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

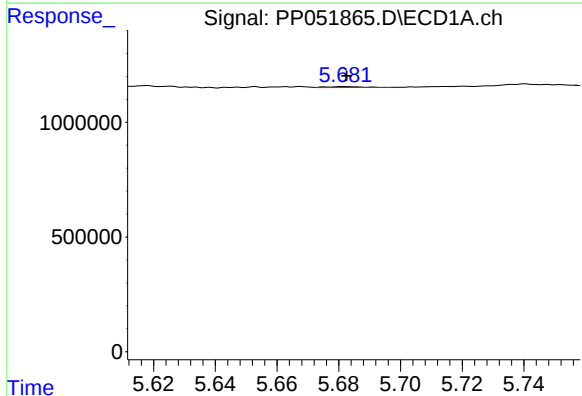


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 32168
Conc: 0.90 ng/ml

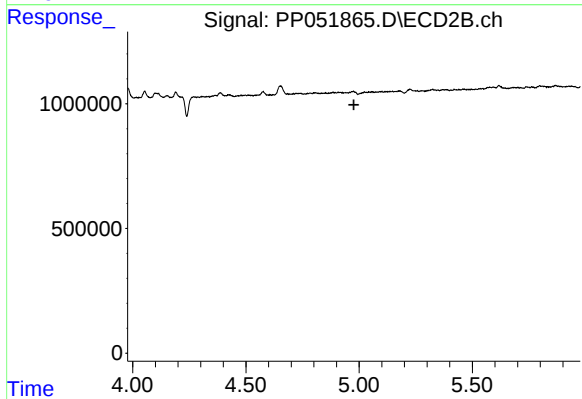

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.977 min
Response: 0
Conc: N.D.

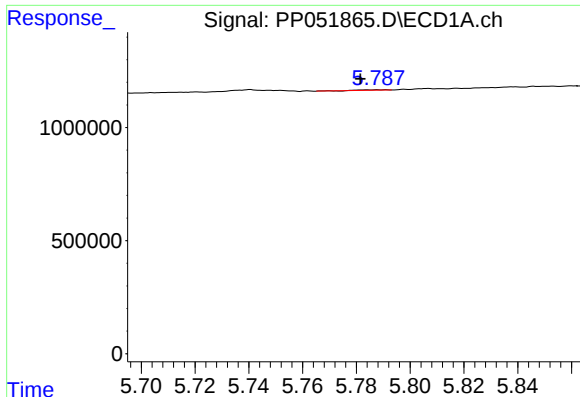

#19 AR-1242-4


R.T.: 5.788 min
Delta R.T.: 0.006 min
Response: 15038
Conc: 0.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

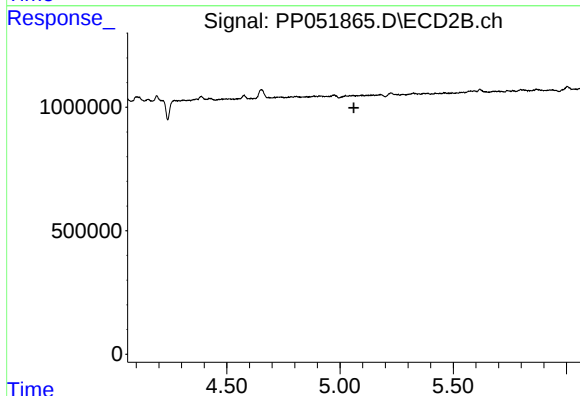


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.061 min
Response: 0
Conc: N.D.

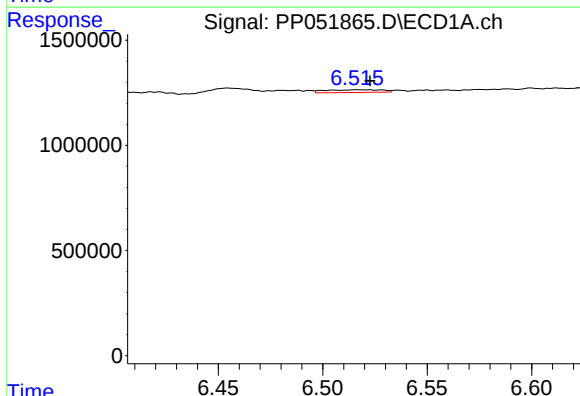


#20 AR-1242-5

R.T.: 6.516 min
Delta R.T.: -0.007 min
Response: 242706
Conc: 6.44 ng/ml

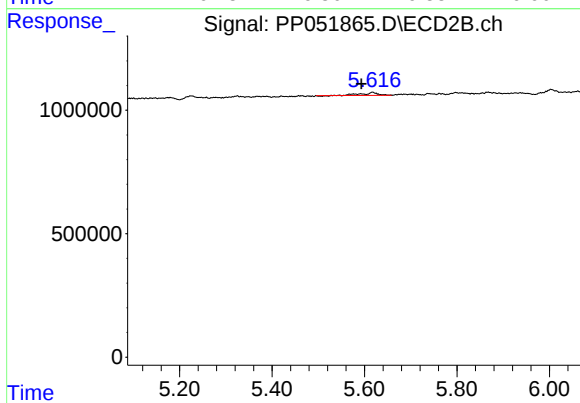

#20 AR-1242-5


R.T.: 5.617 min
Delta R.T.: 0.024 min
Response: 270064
Conc: 7.40 ng/ml

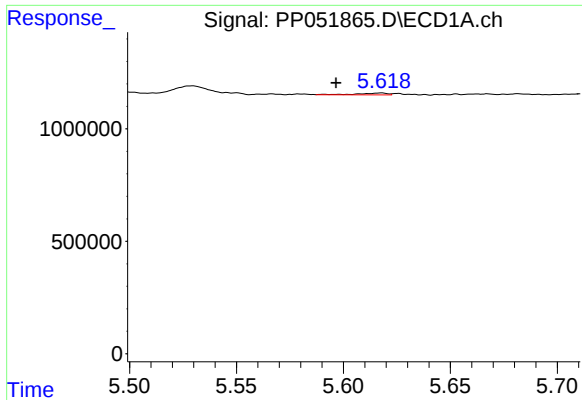

#21 AR-1248-1


R.T.: 5.617 min
Delta R.T.: 0.021 min
Response: 82349
Conc: 2.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

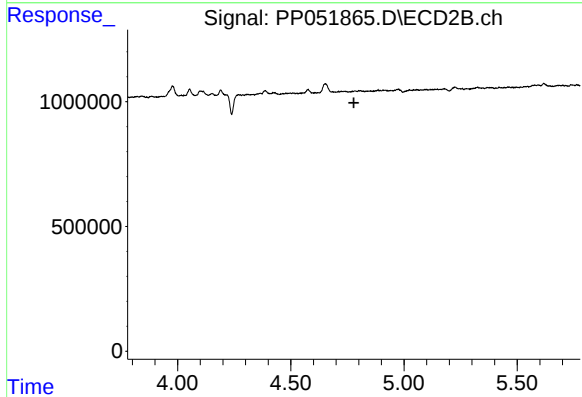


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.778 min
Response: 0
Conc: N.D.

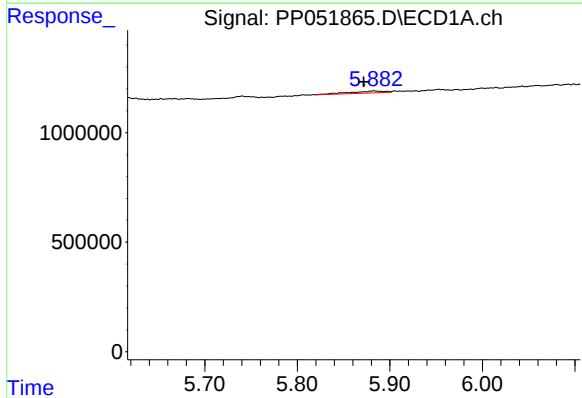


#22 AR-1248-2

R.T.: 5.883 min
Delta R.T.: 0.011 min
Response: 239465
Conc: 5.28 ng/ml

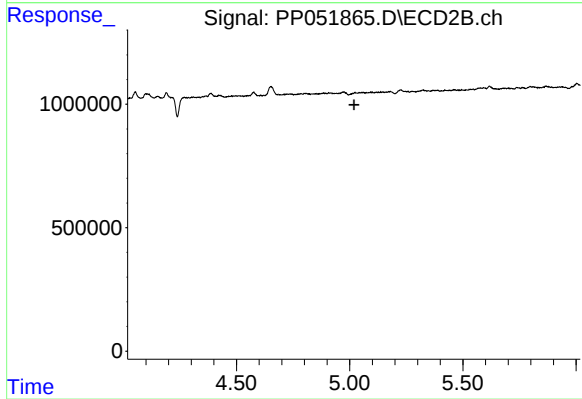

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

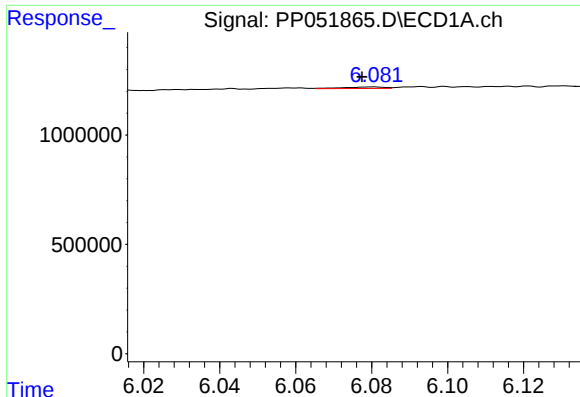

#23 AR-1248-3


R.T.: 6.080 min
Delta R.T.: 0.003 min
Response: 50256
Conc: 0.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

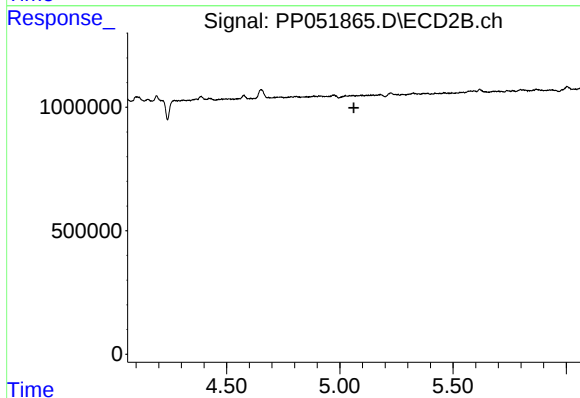


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.062 min
Response: 0
Conc: N.D.

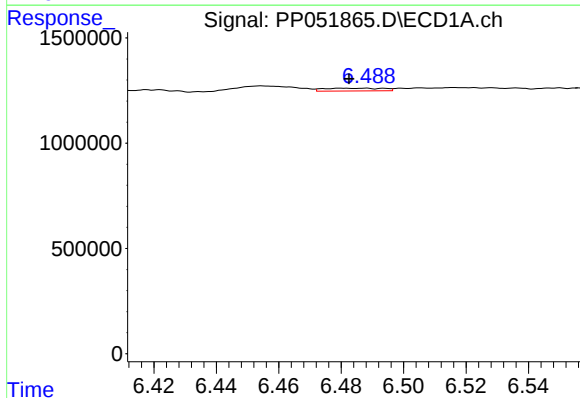


#24 AR-1248-4

R.T.: 6.487 min
Delta R.T.: 0.005 min
Response: 173621
Conc: 2.60 ng/ml

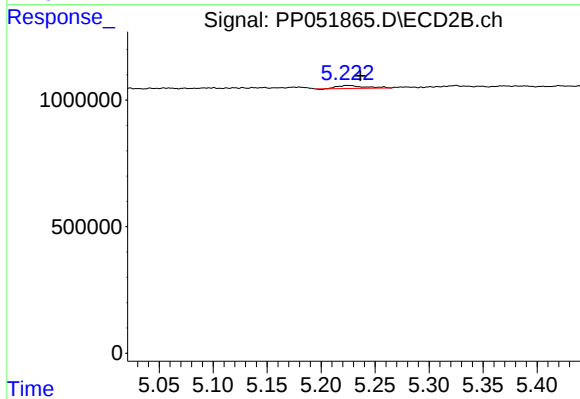

#24 AR-1248-4


R.T.: 5.225 min
Delta R.T.: -0.011 min
Response: 208804
Conc: 4.16 ng/ml

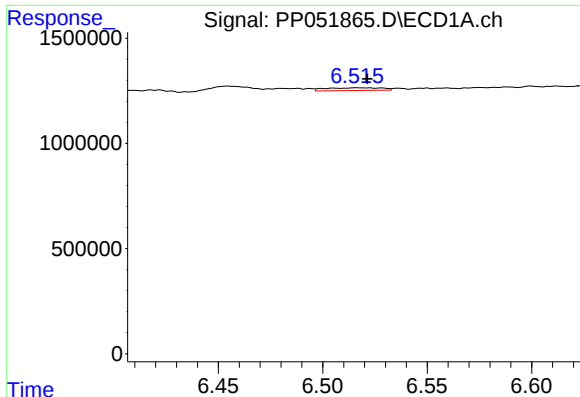

#25 AR-1248-5


R.T.: 6.516 min
Delta R.T.: -0.005 min
Response: 242706
Conc: 3.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

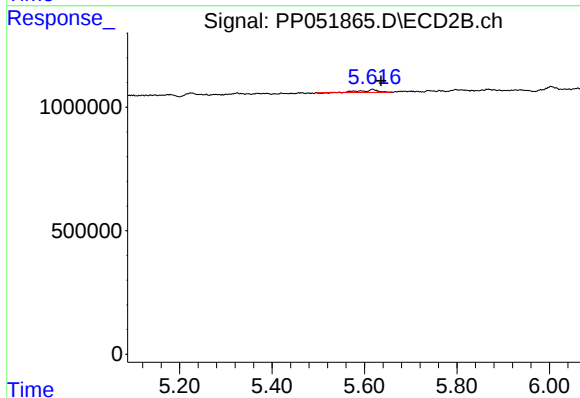


#25 AR-1248-5

R.T.: 5.617 min
Delta R.T.: -0.019 min
Response: 270064
Conc: 5.51 ng/ml

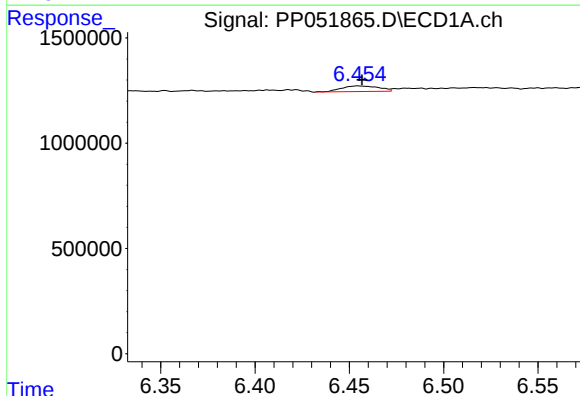


#26 AR-1254-1

R.T.: 6.455 min
Delta R.T.: -0.002 min
Response: 374316
Conc: 5.49 ng/ml

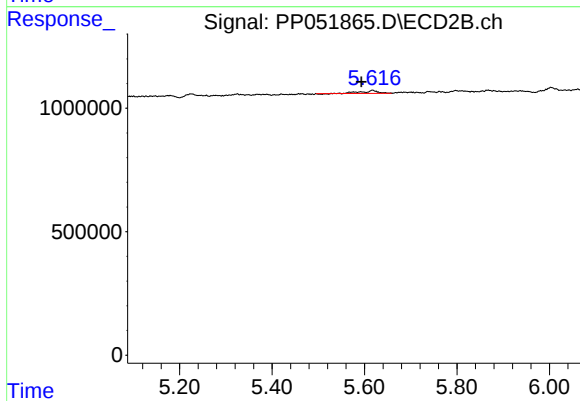

#26 AR-1254-1


R.T.: 5.617 min
Delta R.T.: 0.024 min
Response: 270064
Conc: 3.63 ng/ml

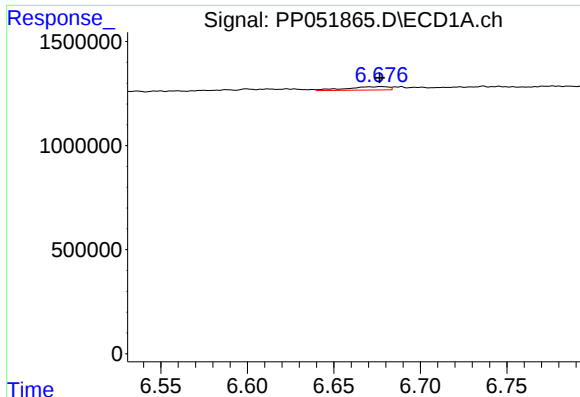

#27 AR-1254-2


R.T.: 6.678 min
Delta R.T.: 0.001 min
Response: 274394
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

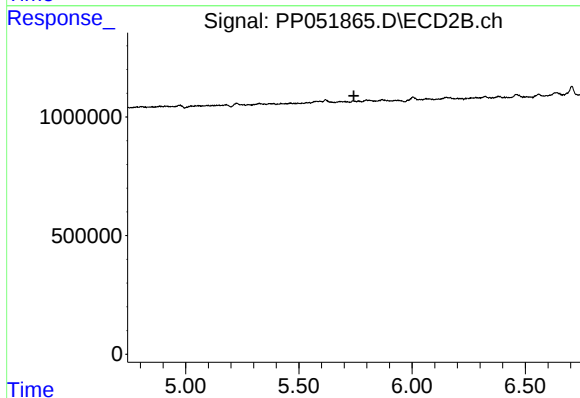


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.743 min
Response: 0
Conc: N.D.

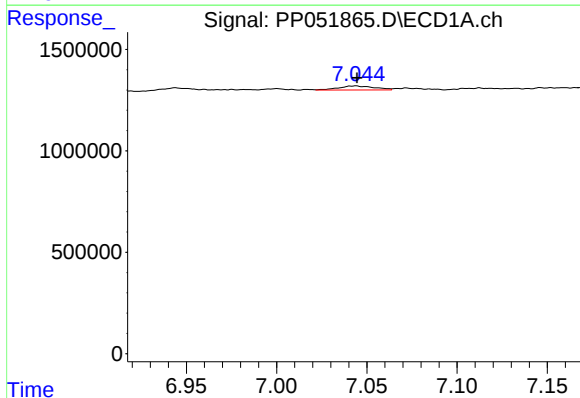


#28 AR-1254-3

R.T.: 7.043 min
Delta R.T.: -0.001 min
Response: 282954
Conc: 2.76 ng/ml

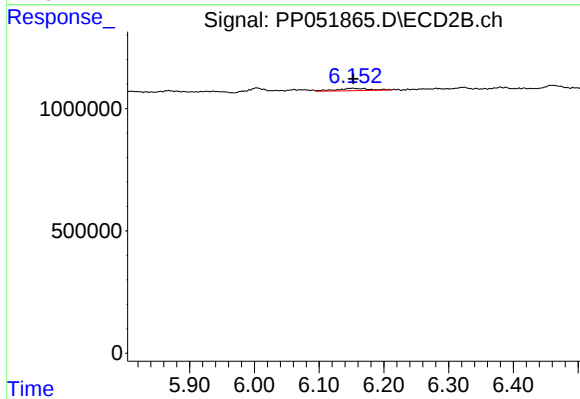

#28 AR-1254-3


R.T.: 6.152 min
Delta R.T.: -0.001 min
Response: 341304
Conc: 3.24 ng/ml

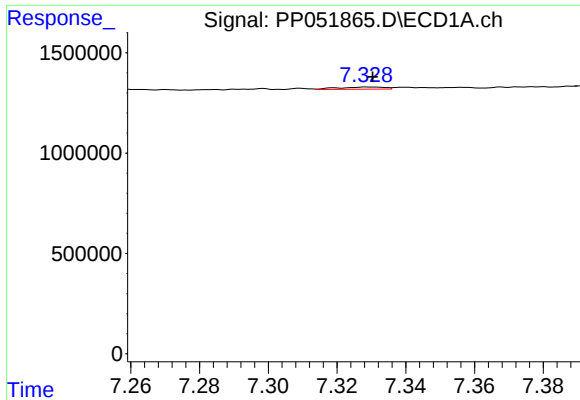

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 101089
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

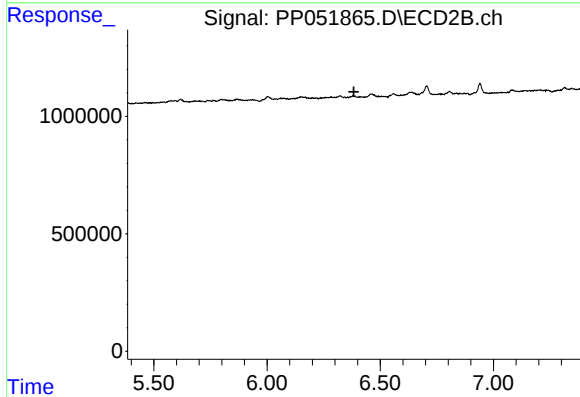


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.384 min
Response: 0
Conc: N.D.

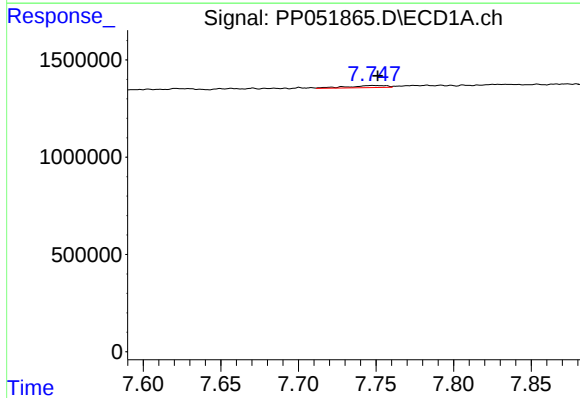


#30 AR-1254-5

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 176410
Conc: 2.34 ng/ml

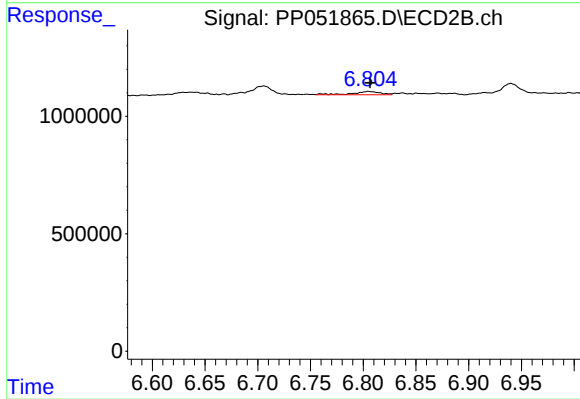

#30 AR-1254-5


R.T.: 6.805 min
Delta R.T.: -0.001 min
Response: 262339
Conc: 2.84 ng/ml

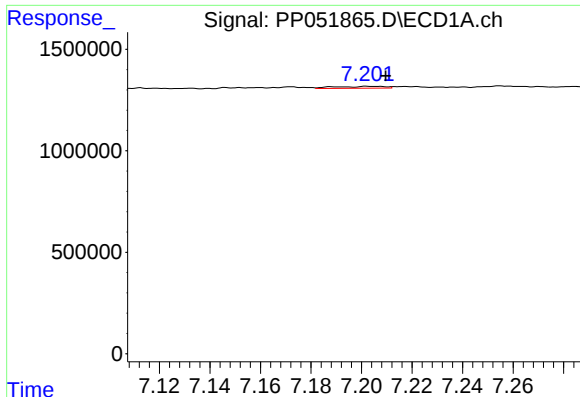

#31 AR-1260-1


R.T.: 7.202 min
Delta R.T.: -0.007 min
Response: 125561
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

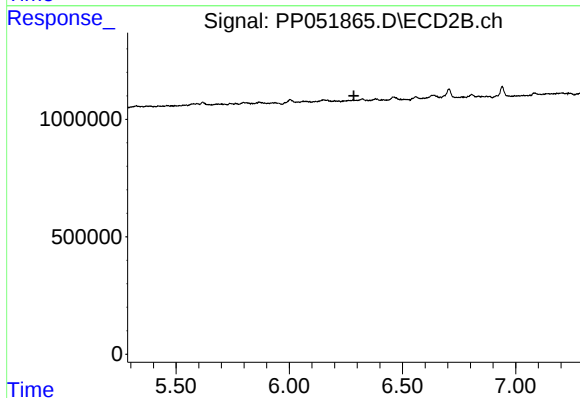


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.285 min
Response: 0
Conc: N.D.

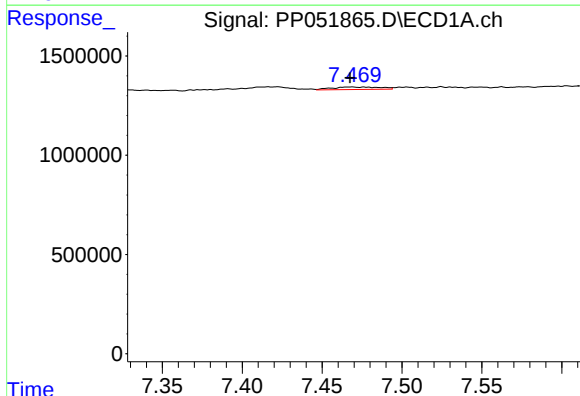


#32 AR-1260-2

R.T.: 7.468 min
Delta R.T.: 0.000 min
Response: 264279
Conc: 3.24 ng/ml

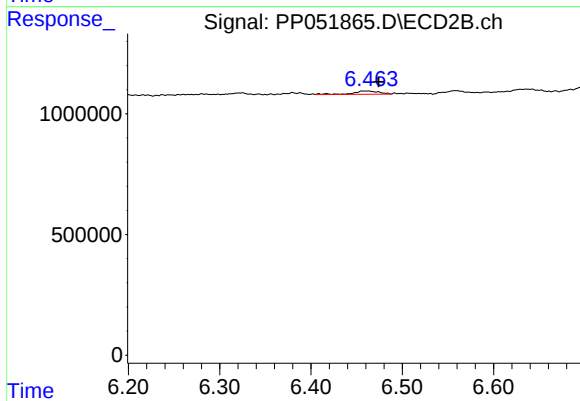

#32 AR-1260-2


R.T.: 6.460 min
Delta R.T.: -0.014 min
Response: 262377
Conc: 3.12 ng/ml

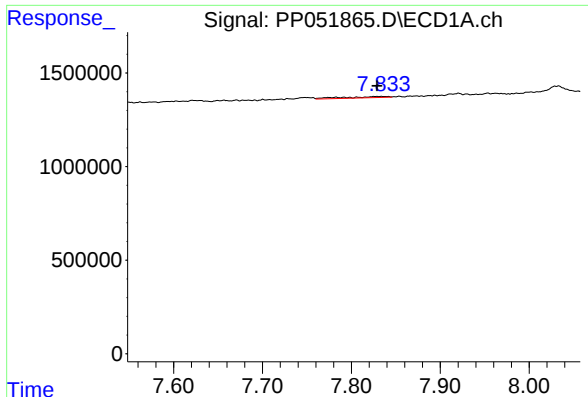

#33 AR-1260-3


R.T.: 7.834 min
Delta R.T.: 0.005 min
Response: 254253
Conc: 4.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

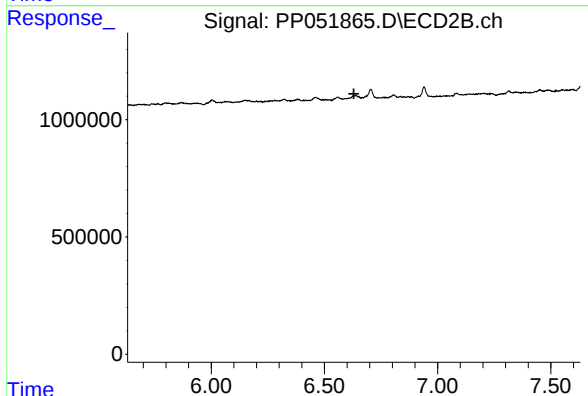


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.631 min
Response: 0
Conc: N.D.

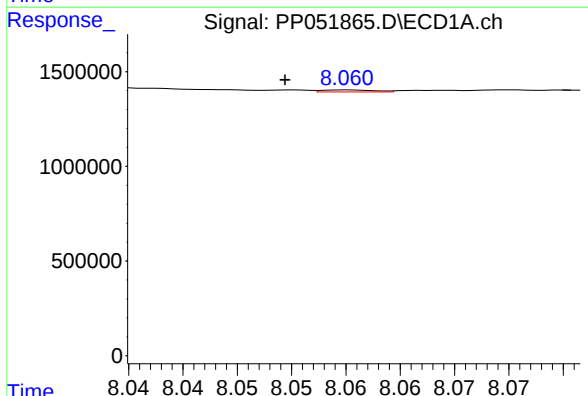


#34 AR-1260-4

R.T.: 8.060 min
Delta R.T.: 0.005 min
Response: 35530
Conc: 0.54 ng/ml

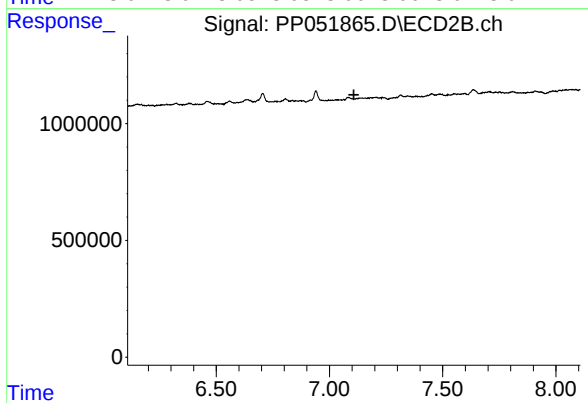

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.108 min
Response: 0
Conc: N.D.

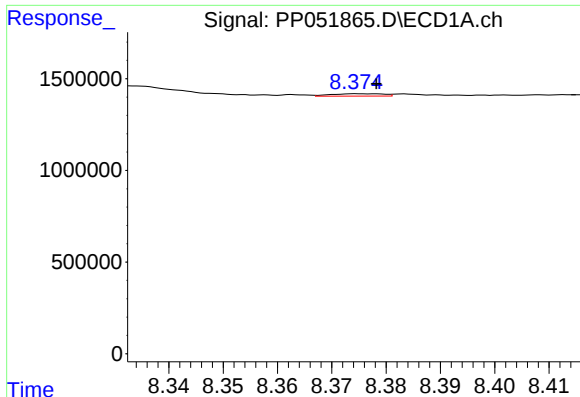

#35 AR-1260-5


R.T.: 8.376 min
Delta R.T.: -0.002 min
Response: 84925
Conc: 0.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

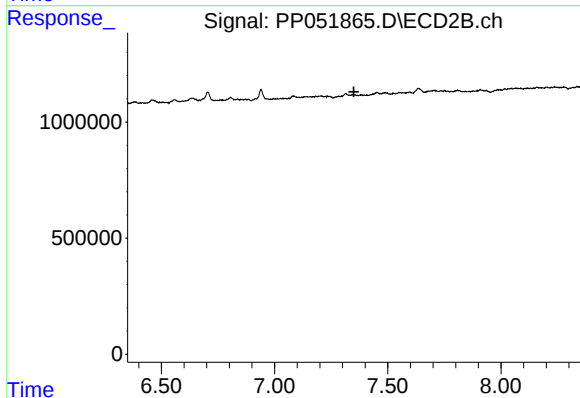


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

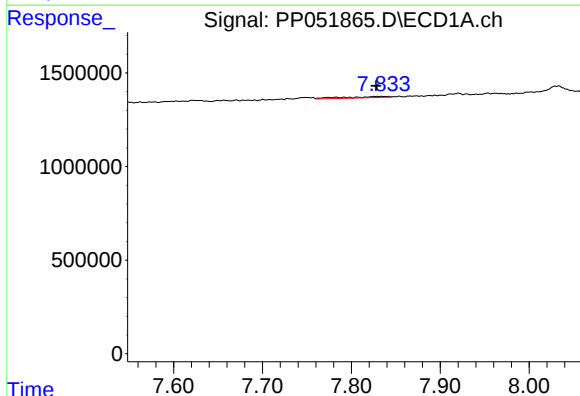


#36 AR-1262-1

R.T.: 7.834 min
Delta R.T.: 0.006 min
Response: 254253
Conc: 2.92 ng/ml

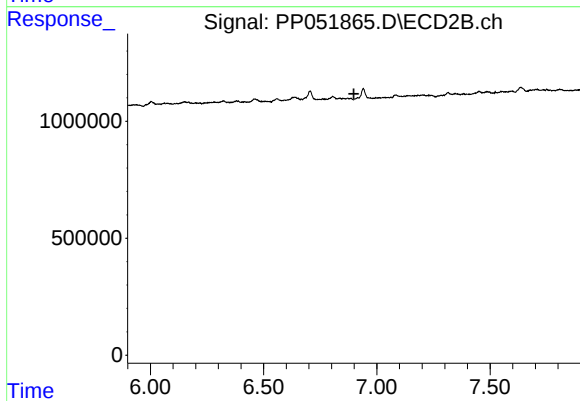

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.899 min
Response: 0
Conc: N.D.

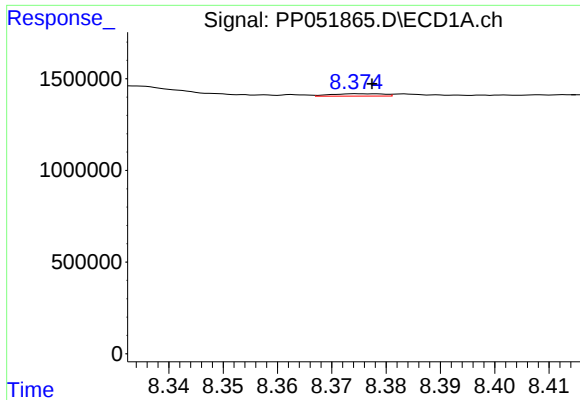

#37 AR-1262-2


R.T.: 8.376 min
Delta R.T.: -0.002 min
Response: 84925
Conc: 0.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

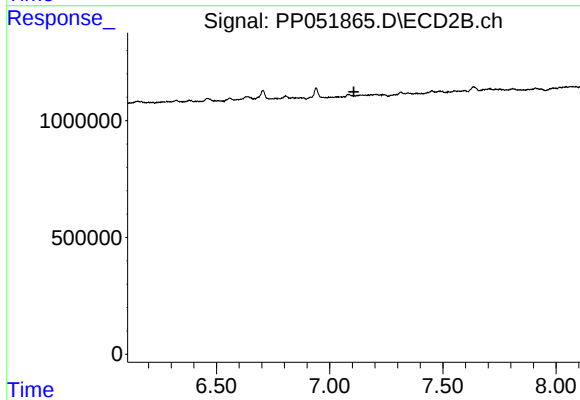


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.107 min
Response: 0
Conc: N.D.

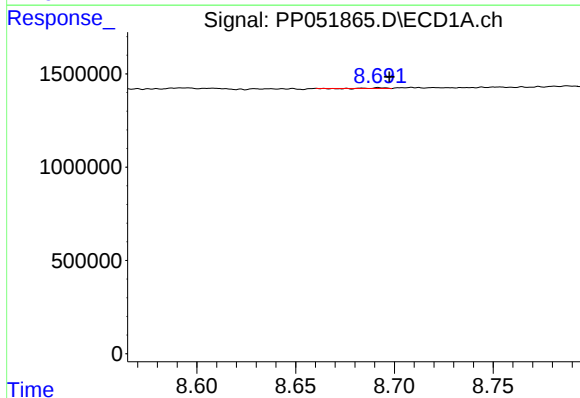


#38 AR-1262-3

R.T.: 8.692 min
Delta R.T.: -0.005 min
Response: 17068
Conc: 0.17 ng/ml

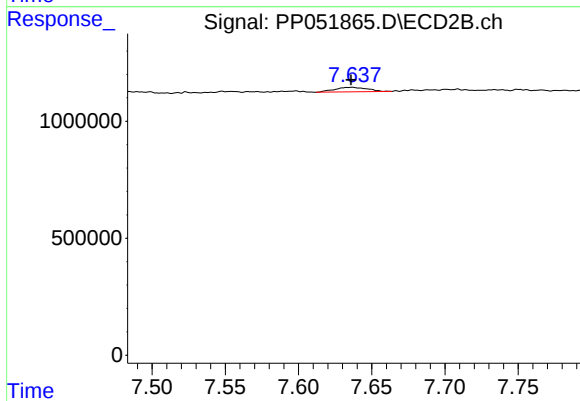

#38 AR-1262-3


R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 299475
Conc: 4.27 ng/ml

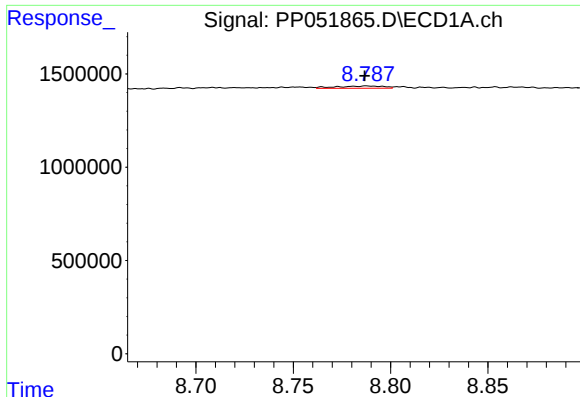

#39 AR-1262-4


R.T.: 8.788 min
Delta R.T.: 0.001 min
Response: 203101
Conc: 4.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

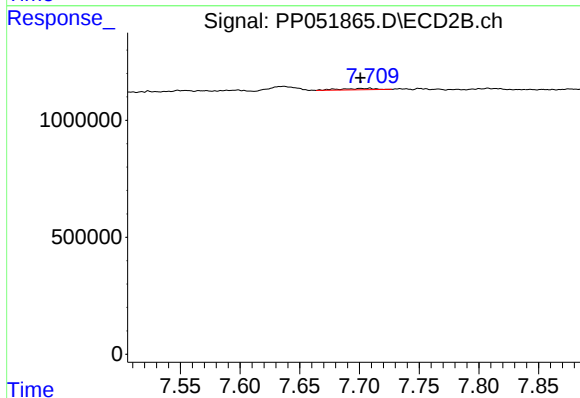


#39 AR-1262-4

R.T.: 7.708 min
Delta R.T.: 0.007 min
Response: 121581
Conc: 0.97 ng/ml

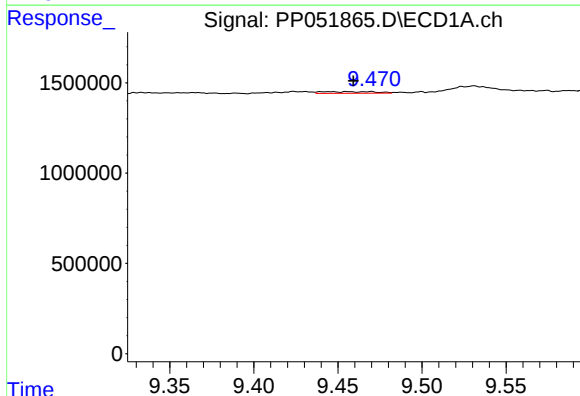


#40 AR-1262-5

R.T.: 9.456 min
Delta R.T.: -0.004 min
Response: 199661
Conc: 3.50 ng/ml

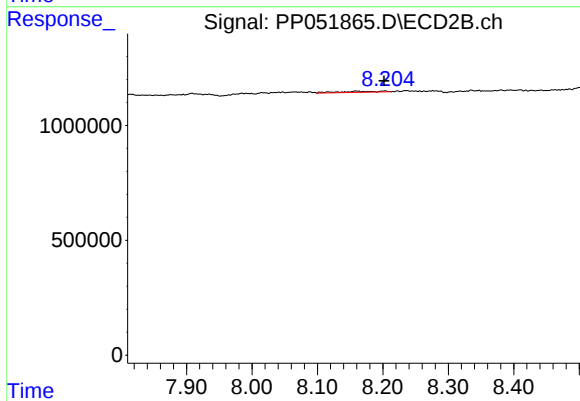

#40 AR-1262-5


R.T.: 8.203 min
Delta R.T.: 0.001 min
Response: 197088
Conc: 3.48 ng/ml

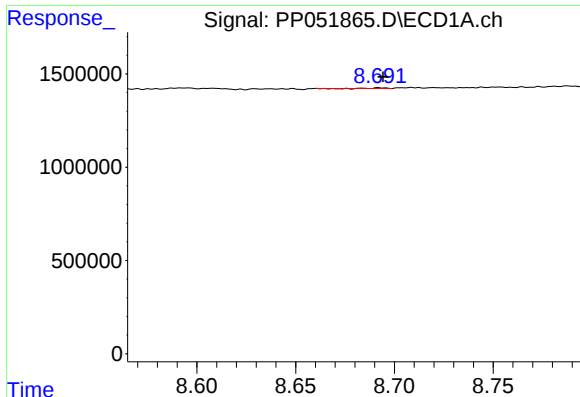

#41 AR-1268-1


R.T.: 8.692 min
Delta R.T.: -0.002 min
Response: 17068
Conc: 0.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

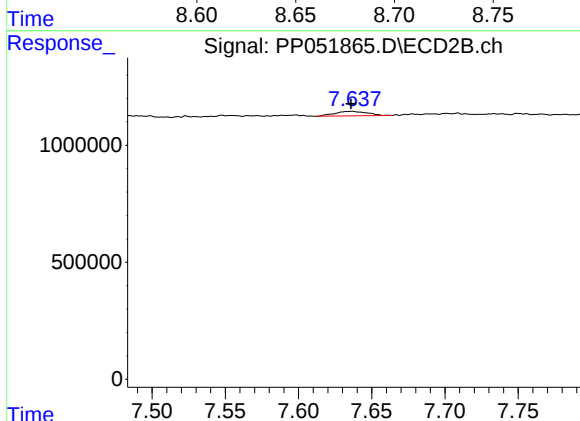


#41 AR-1268-1

R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 299475
Conc: 1.51 ng/ml

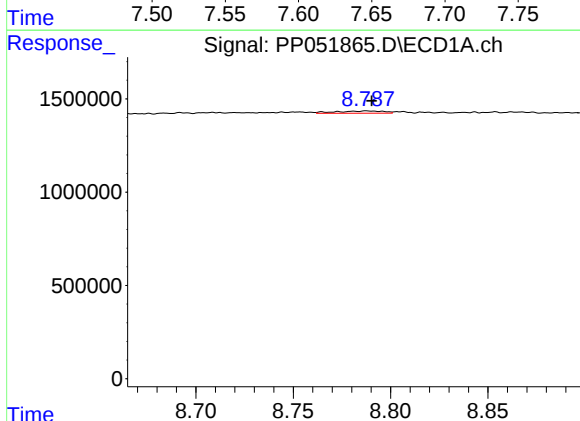


#42 AR-1268-2

R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 203101
Conc: 1.23 ng/ml

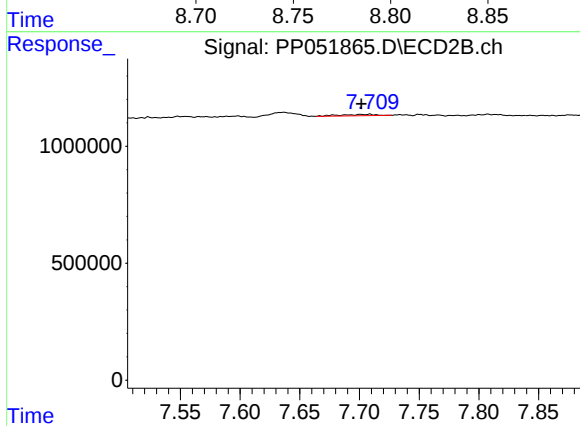

#42 AR-1268-2


R.T.: 7.708 min
Delta R.T.: 0.006 min
Response: 121581
Conc: 0.68 ng/ml

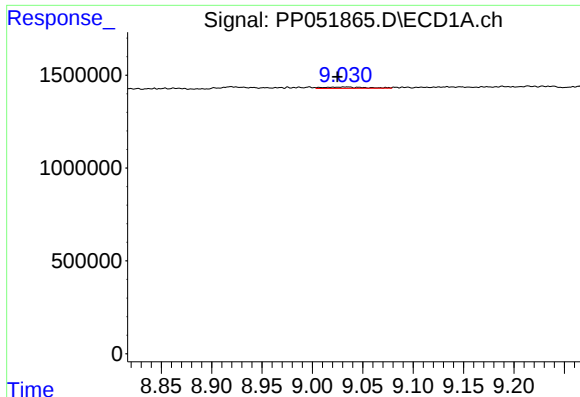

#43 AR-1268-3


R.T.: 9.035 min
Delta R.T.: 0.011 min
Response: 219934
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

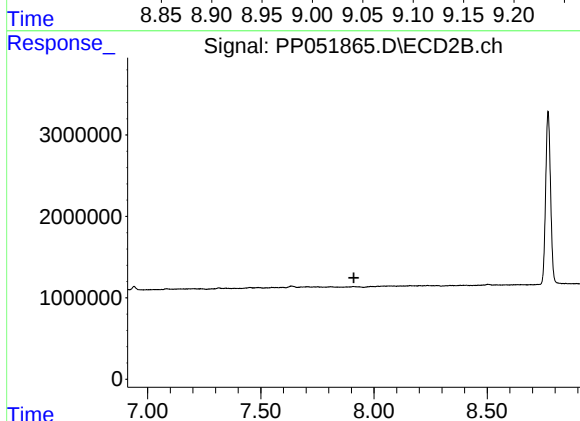


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.911 min
Response: 0
Conc: N.D.

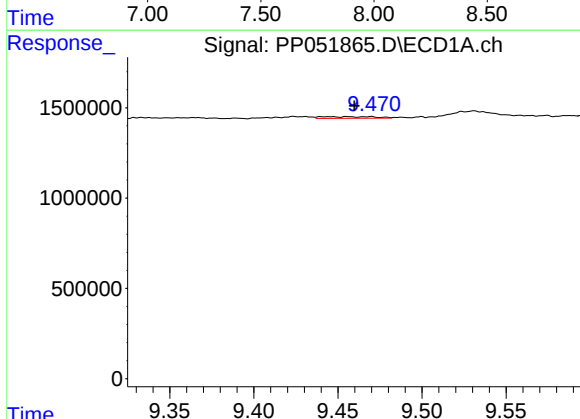


#44 AR-1268-4

R.T.: 9.456 min
Delta R.T.: -0.004 min
Response: 199661
Conc: 3.12 ng/ml

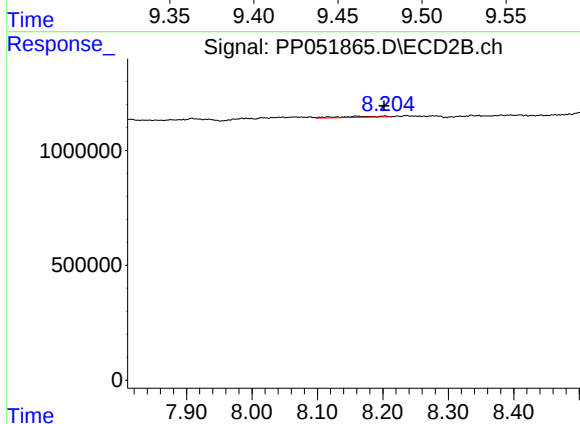

#44 AR-1268-4


R.T.: 8.203 min
Delta R.T.: 0.000 min
Response: 197088
Conc: 3.14 ng/ml

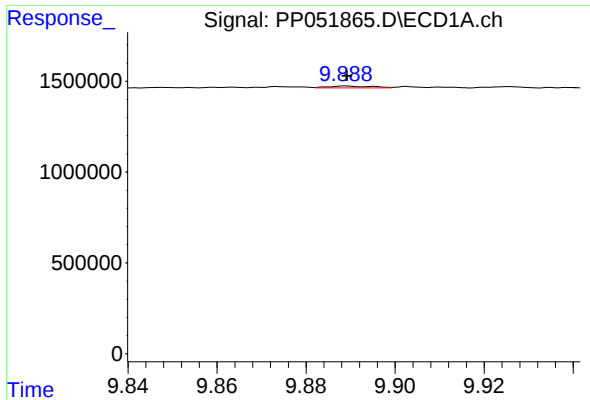

#45 AR-1268-5

R.T.: 9.889 min
Delta R.T.: 0.000 min
Response: 69898
Conc: 0.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
BUS-WORK-FOUNDATION-2

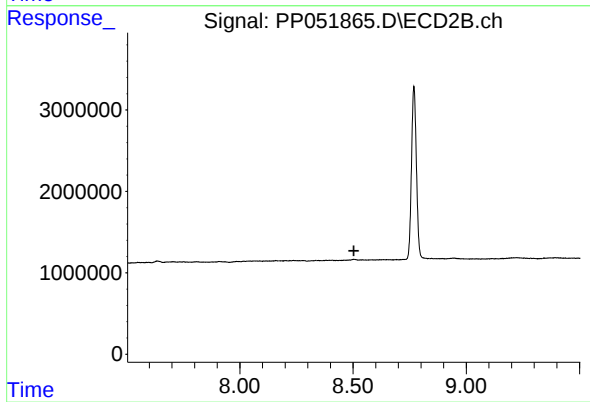

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.503 min
Response: 0
Conc: N.D.