

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
 Data File : PP051866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 03:07
 Operator : YP\AJ
 Sample : N4888-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 REGULATORY-FOUNDATION-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:04:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 03:12:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.422	3.673	31707893	22923496	17.741	18.031
2)	SA Decachlor...	10.239	8.769	32688828	30964120	26.964	26.216
Target Compounds							
3)	L1 AR-1016-1	5.596	4.777	26367829	24381513	581.803	555.998
4)	L1 AR-1016-2	5.619	4.797	37355505	35973804	582.020	583.094
5)	L1 AR-1016-3	5.681	4.976	23631201	18340365	591.159	558.175
6)	L1 AR-1016-4	5.780	5.018	19165078	11616544	546.675	449.166
7)	L1 AR-1016-5	6.077	5.236	20376956	16837710	493.411	488.927
8)	L2 AR-1221-1	4.626	3.888	1240731	533940	57.557	34.091 #
9)	L2 AR-1221-2	4.717	3.978	1681026	1397587	105.456	116.980
10)	L2 AR-1221-3	4.794	4.055	8281129	6286474	171.018	167.565
11)	L3 AR-1232-1	4.794	4.055	8281129	6286474	206.375	201.947
12)	L3 AR-1232-2	5.327	4.797	20241209	35973804	1078.589	1272.964
13)	L3 AR-1232-3	5.619	4.976	37355505	18340365	1257.919	1255.885
14)	L3 AR-1232-4	5.780	5.061	19165078	15634692	1338.905	1171.570
15)	L3 AR-1232-5	5.872	5.236	15107465	16837710	1262.721	1140.118
16)	L4 AR-1242-1	5.596	4.777	26367829	24381513	643.176	625.692
17)	L4 AR-1242-2	5.619	4.797	37355505	35973804	649.560	656.450
18)	L4 AR-1242-3	5.681	4.976	23631201	18340365	659.967	622.742
19)	L4 AR-1242-4	5.780	5.061	19165078	15634692	665.590	530.047
20)	L4 AR-1242-5	6.521	5.593	23462831	20133819	622.951	551.516
21)	L5 AR-1248-1	5.596	4.777	26367829	24381513	870.571	834.849
22)	L5 AR-1248-2	5.872	5.018	15107465	11616544	333.403	288.337
23)	L5 AR-1248-3	6.077	5.061	20376956	15634692	401.271	368.363
24)	L5 AR-1248-4	6.482	5.236	22454222	16837710	336.061	335.418
25)	L5 AR-1248-5	6.521	5.635	23462831	18207259	357.022	371.425
26)	L6 AR-1254-1	6.454	5.593	15026148	20133819	220.213	270.638
27)	L6 AR-1254-2	6.679	5.742	18580003	4778103	181.560	74.096 #
28)	L6 AR-1254-3	7.044	6.153	4861610	6599594	47.484	62.684 #
29)	L6 AR-1254-4	7.329	6.383	3980171	3298619	55.483	48.391
30)	L6 AR-1254-5	7.749	6.805	7759674	6896604	103.143	74.546 #
31)	L7 AR-1260-1	7.208	6.284	5401322	7730346	75.988	112.230 #
32)	L7 AR-1260-2	7.465	6.473	7243167	6368690	88.681	75.680
33)	L7 AR-1260-3	7.827	6.630	3970030	5054049	69.413	64.925
34)	L7 AR-1260-4	8.052	7.106	5724905	3770394	87.411	59.893 #
35)	L7 AR-1260-5	8.377	7.349	10450565	10524393	82.188	71.759
36)	L8 AR-1262-1	7.827	6.897	3970030	2026661	45.655	53.927
37)	L8 AR-1262-2	8.377	7.106	10450565	3770394	70.832	44.516 #
38)	L8 AR-1262-3	8.709	7.636	6901143	2576092	67.033	36.735 #
39)	L8 AR-1262-4	8.787	7.699	1915687	7513385	41.611	60.133 #
40)	L8 AR-1262-5	9.459	8.201	3163586	2665981	55.519	47.054
41)	L9 AR-1268-1	8.709	7.636	6901143	2576092	38.689	12.978 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
 Data File : PP051866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 03:07
 Operator : YP\AJ
 Sample : N4888-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 REGULATORY-FOUNDATION-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:04:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 03:12:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.787	7.699	1915687	7513385	11.556	42.044 #
43) L9	AR-1268-3	9.022	7.911	391149	369063	2.728	2.413
44) L9	AR-1268-4	9.459	8.201	3163586	2665981	49.388	42.473
45) L9	AR-1268-5	9.887	8.503	1016383	944808	2.213	2.026



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
Data File : PP051866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 03:07
Operator : YP\AJ
Sample : N4888-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:04:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 04 03:12:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

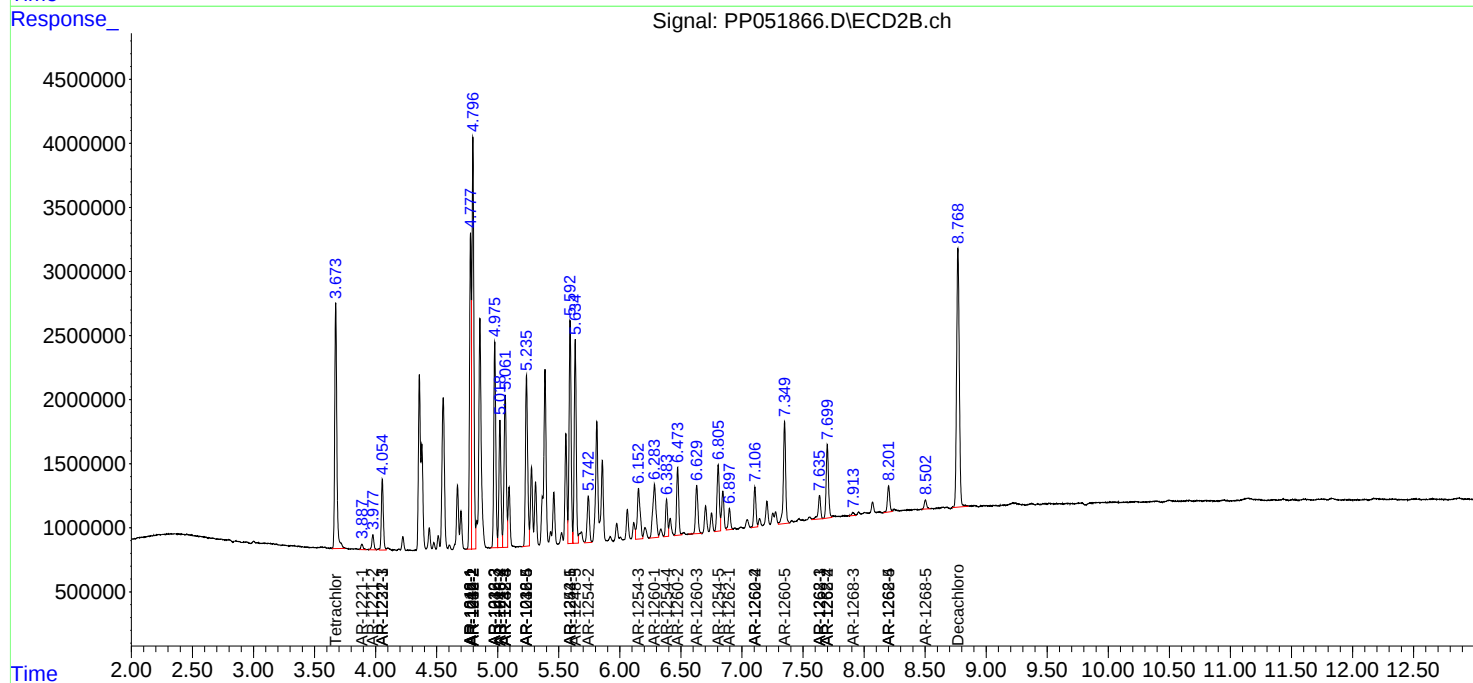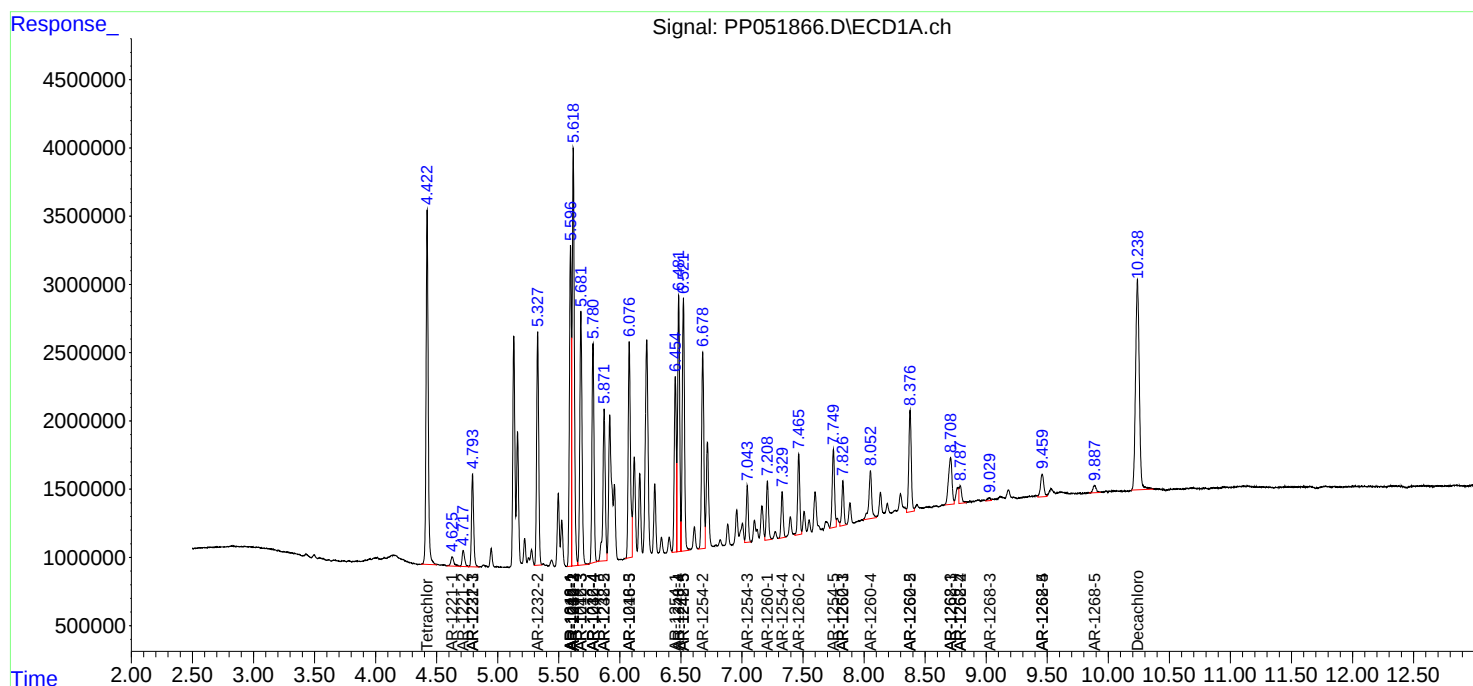


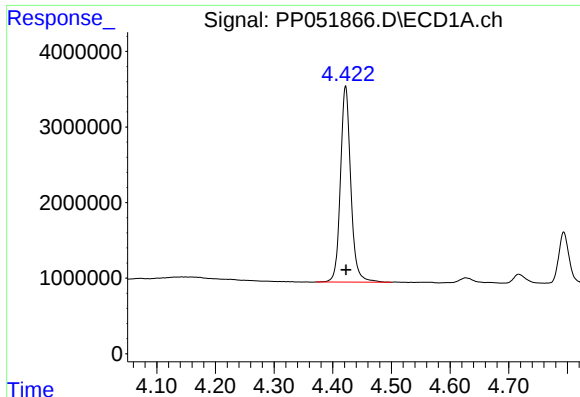

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: -0.001 min
Response: 31707893
Conc: 17.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

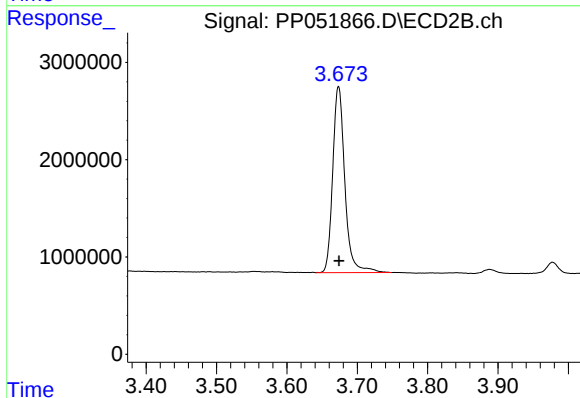


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 22923496
Conc: 18.03 ng/ml

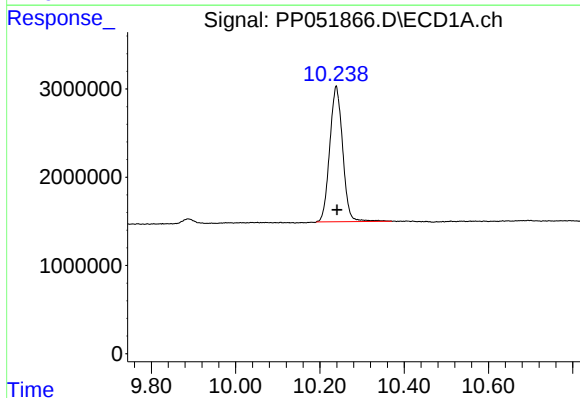


#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: -0.002 min
Response: 32688828
Conc: 26.96 ng/ml

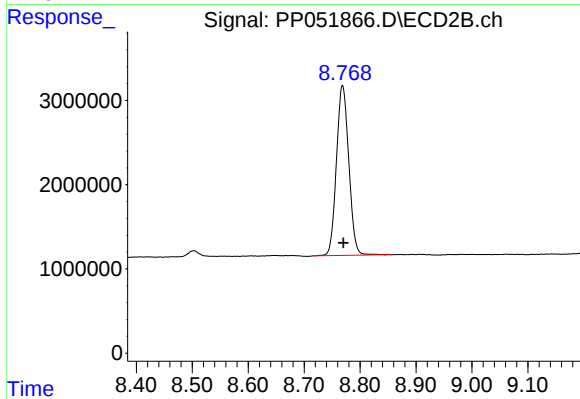

#2 Decachlorobiphenyl


R.T.: 8.769 min
Delta R.T.: -0.002 min
Response: 30964120
Conc: 26.22 ng/ml

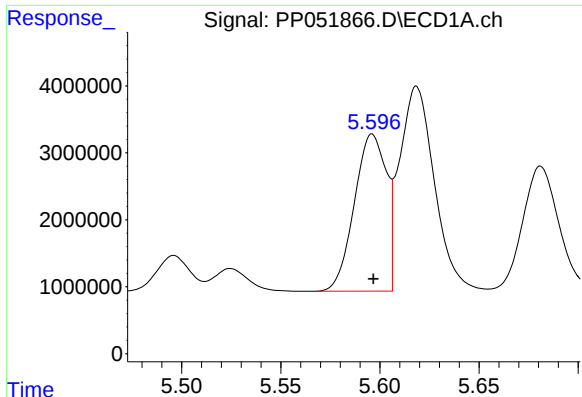

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 26367829
Conc: 581.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

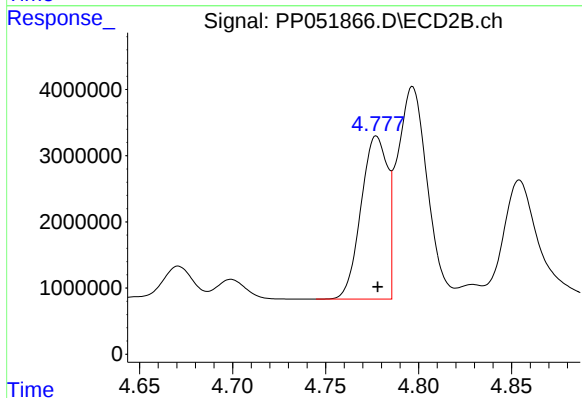


#3 AR-1016-1

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 24381513
Conc: 556.00 ng/ml

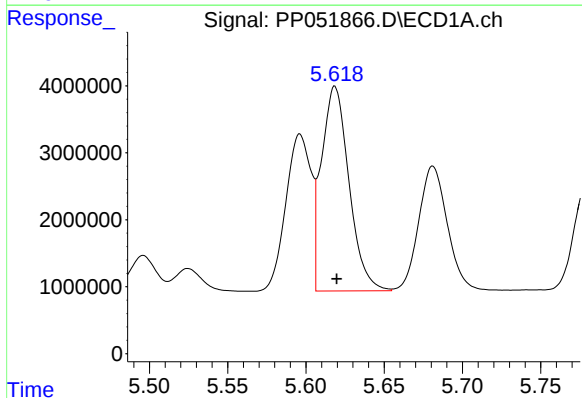


#4 AR-1016-2

R.T.: 5.619 min
Delta R.T.: -0.001 min
Response: 37355505
Conc: 582.02 ng/ml

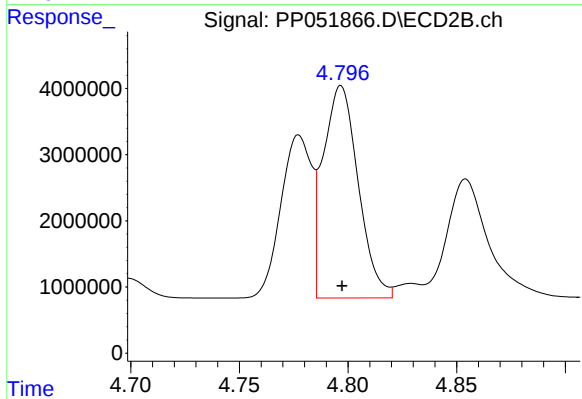

#4 AR-1016-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 35973804
Conc: 583.09 ng/ml

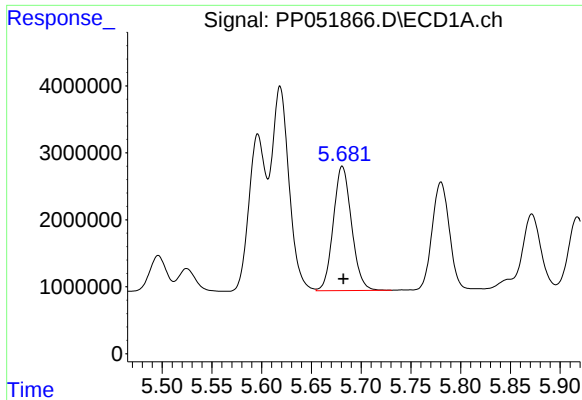

#5 AR-1016-3


R.T.: 5.681 min
Delta R.T.: -0.001 min
Response: 23631201
Conc: 591.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

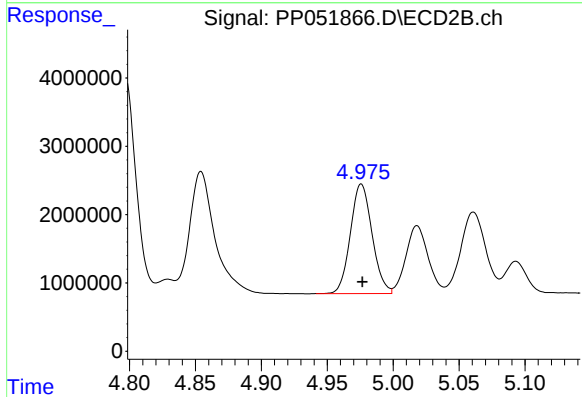


#5 AR-1016-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 18340365
Conc: 558.18 ng/ml

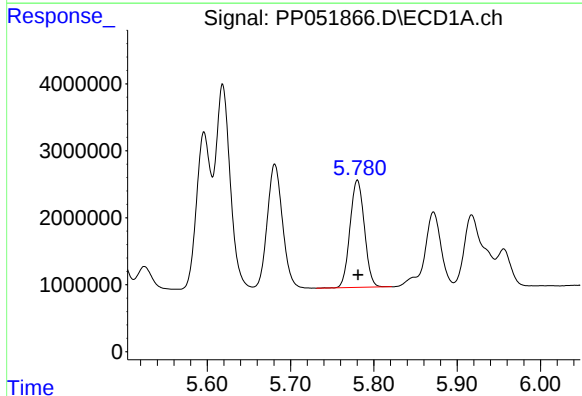


#6 AR-1016-4

R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 19165078
Conc: 546.67 ng/ml

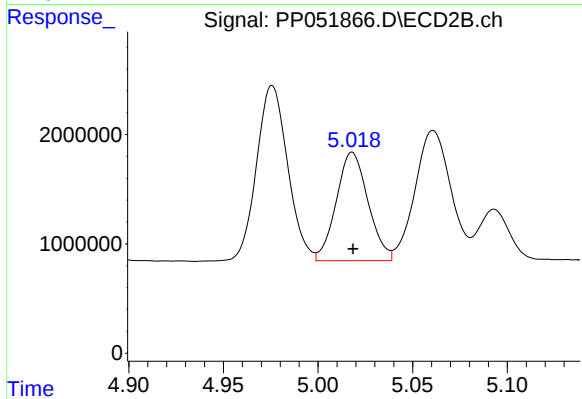

#6 AR-1016-4


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 11616544
Conc: 449.17 ng/ml

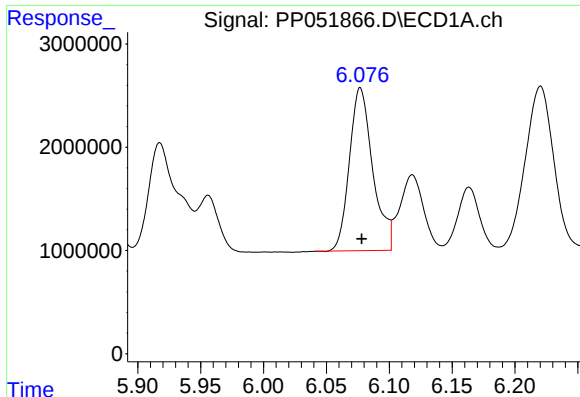

#7 AR-1016-5


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 20376956
Conc: 493.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

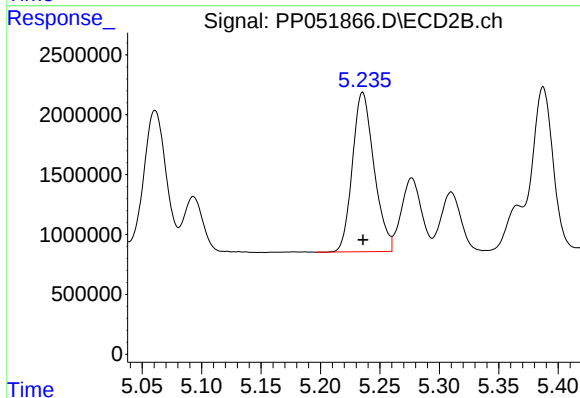


#7 AR-1016-5

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 16837710
Conc: 488.93 ng/ml

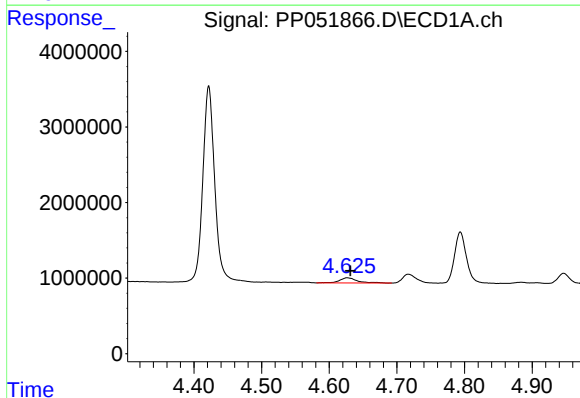


#8 AR-1221-1

R.T.: 4.626 min
Delta R.T.: -0.005 min
Response: 1240731
Conc: 57.56 ng/ml

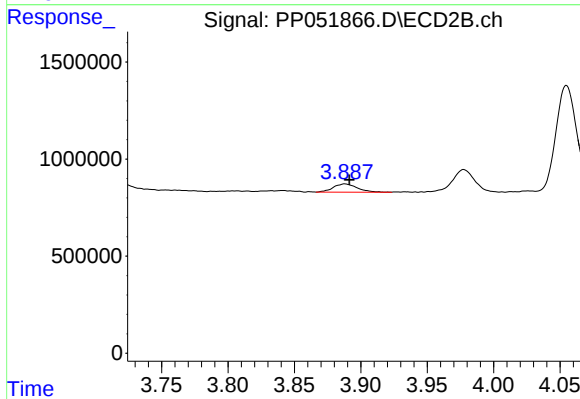

#8 AR-1221-1


R.T.: 3.888 min
Delta R.T.: -0.003 min
Response: 533940
Conc: 34.09 ng/ml

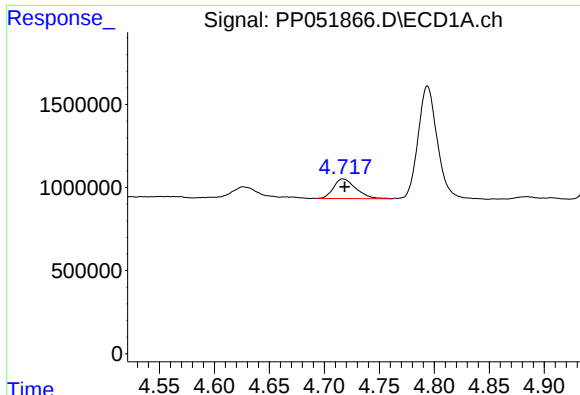

#9 AR-1221-2


R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 1681026
Conc: 105.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

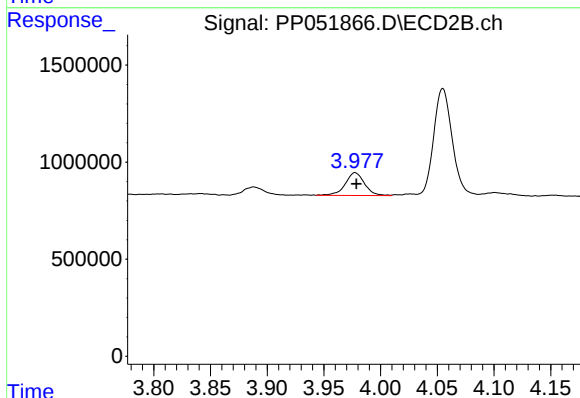


#9 AR-1221-2

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 1397587
Conc: 116.98 ng/ml

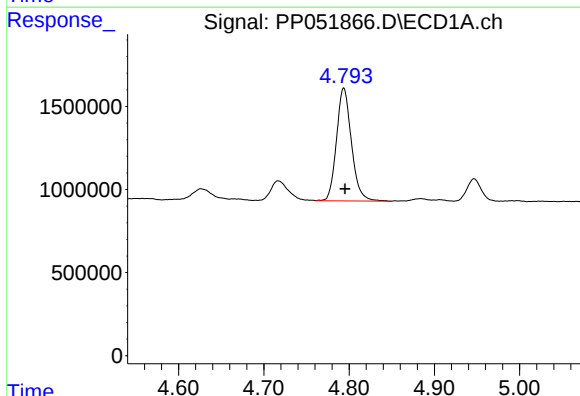


#10 AR-1221-3

R.T.: 4.794 min
Delta R.T.: -0.001 min
Response: 8281129
Conc: 171.02 ng/ml

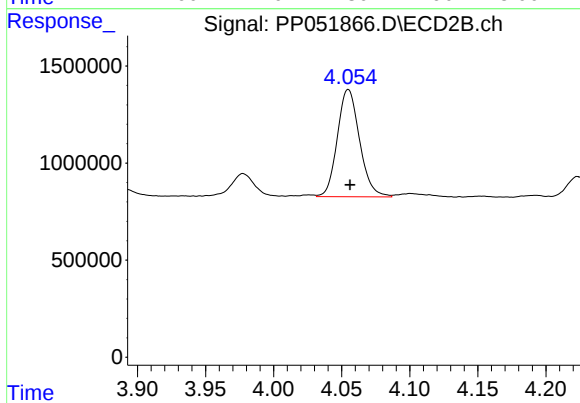

#10 AR-1221-3


R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 6286474
Conc: 167.57 ng/ml

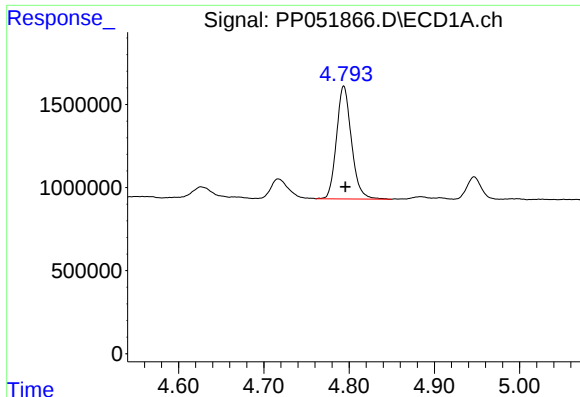

#11 AR-1232-1


R.T.: 4.794 min
Delta R.T.: -0.002 min
Response: 8281129
Conc: 206.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

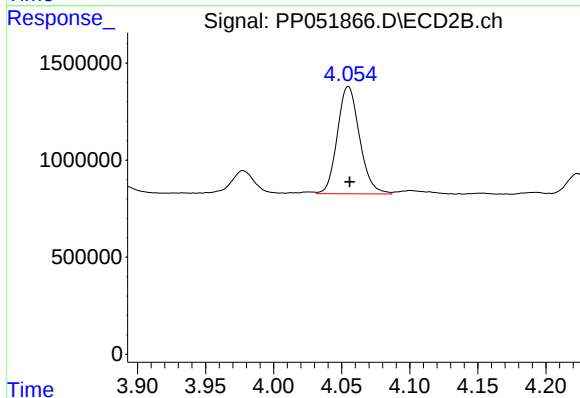


#11 AR-1232-1

R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 6286474
Conc: 201.95 ng/ml

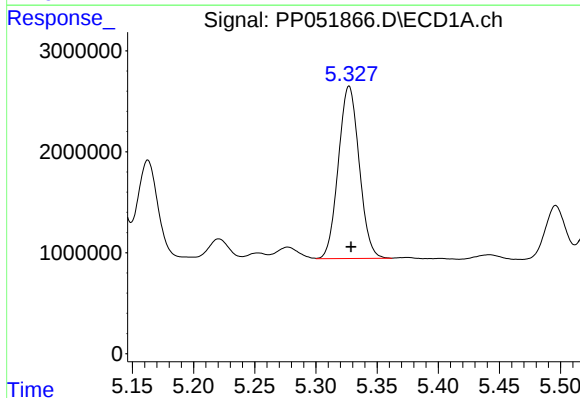


#12 AR-1232-2

R.T.: 5.327 min
Delta R.T.: -0.002 min
Response: 20241209
Conc: 1078.59 ng/ml

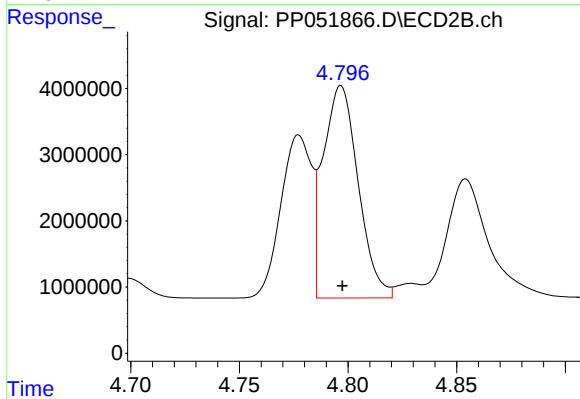

#12 AR-1232-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 35973804
Conc: 1272.96 ng/ml

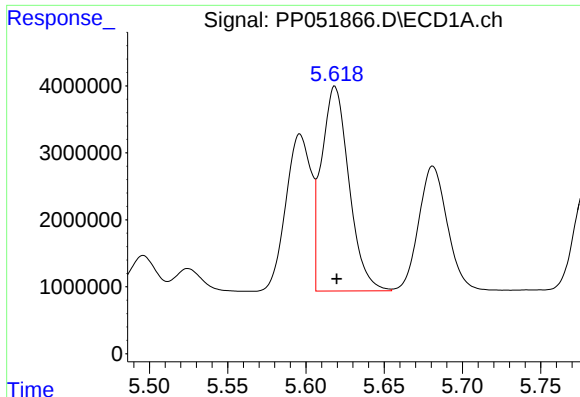

#13 AR-1232-3


R.T.: 5.619 min
Delta R.T.: -0.001 min
Response: 37355505
Conc: 1257.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

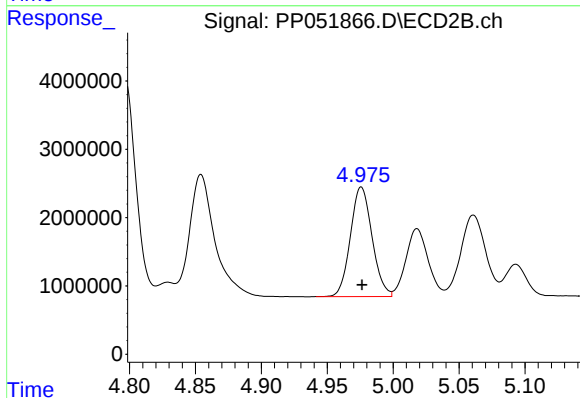


#13 AR-1232-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 18340365
Conc: 1255.89 ng/ml

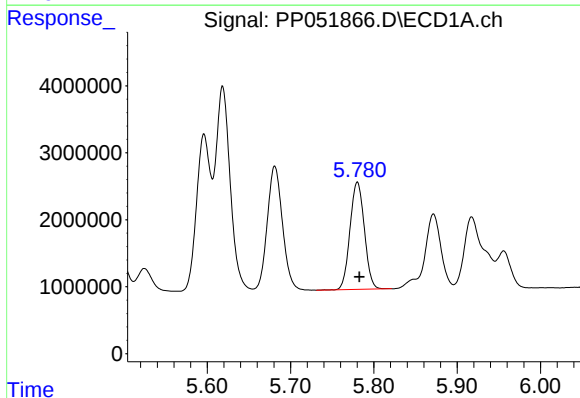


#14 AR-1232-4

R.T.: 5.780 min
Delta R.T.: -0.002 min
Response: 19165078
Conc: 1338.90 ng/ml

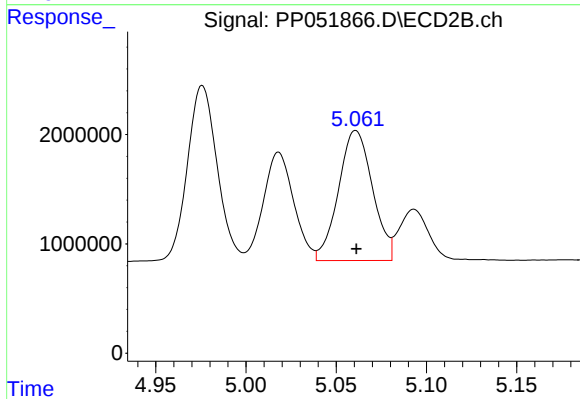

#14 AR-1232-4


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 15634692
Conc: 1171.57 ng/ml

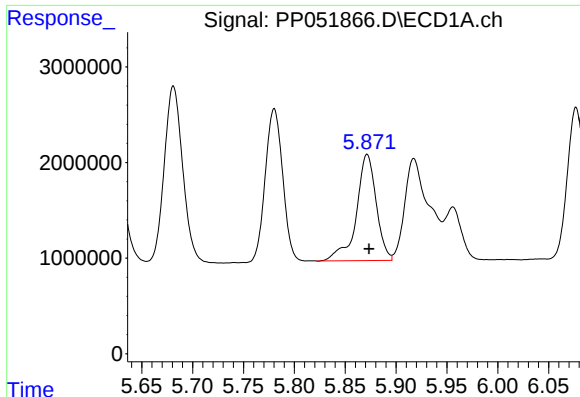

#15 AR-1232-5


R.T.: 5.872 min
Delta R.T.: -0.002 min
Response: 15107465
Conc: 1262.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

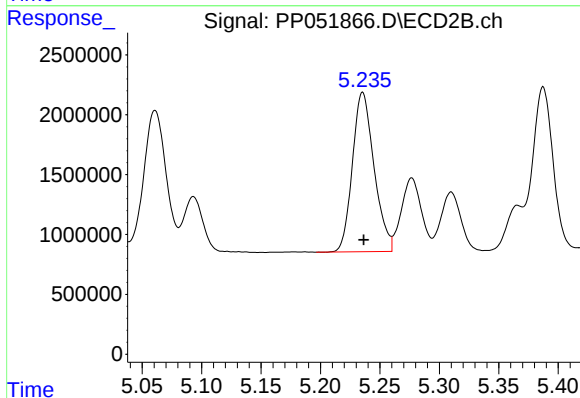


#15 AR-1232-5

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 16837710
Conc: 1140.12 ng/ml

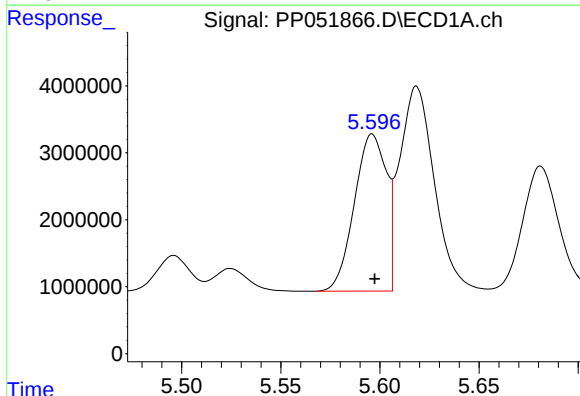


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: -0.001 min
Response: 26367829
Conc: 643.18 ng/ml

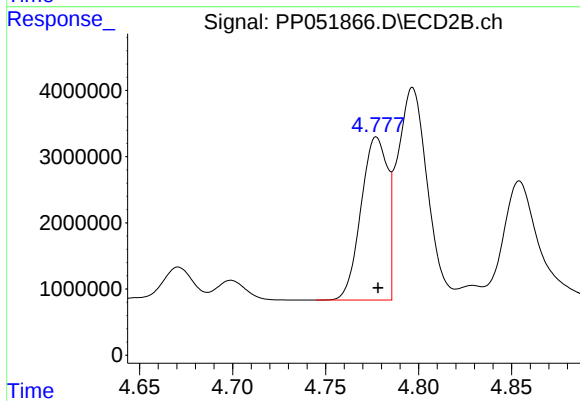

#16 AR-1242-1


R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 24381513
Conc: 625.69 ng/ml

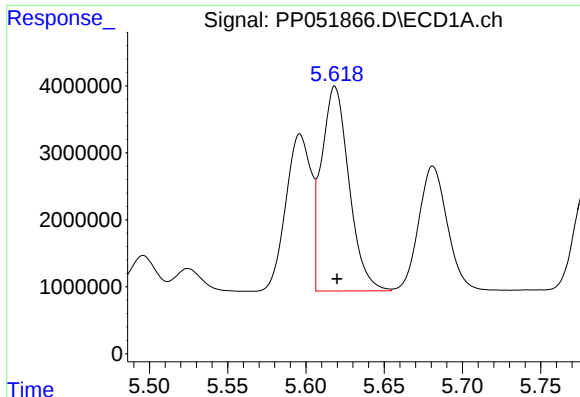

#17 AR-1242-2


R.T.: 5.619 min
Delta R.T.: -0.001 min
Response: 37355505
Conc: 649.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

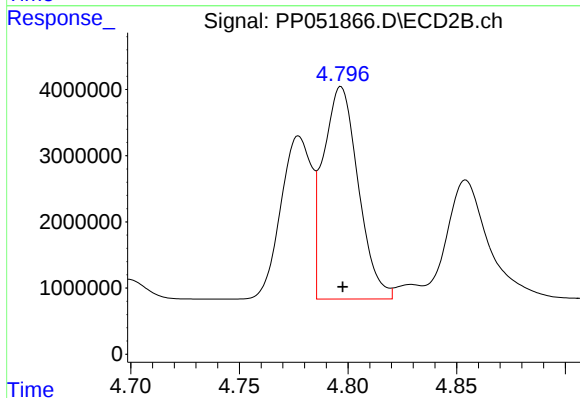


#17 AR-1242-2

R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 35973804
Conc: 656.45 ng/ml

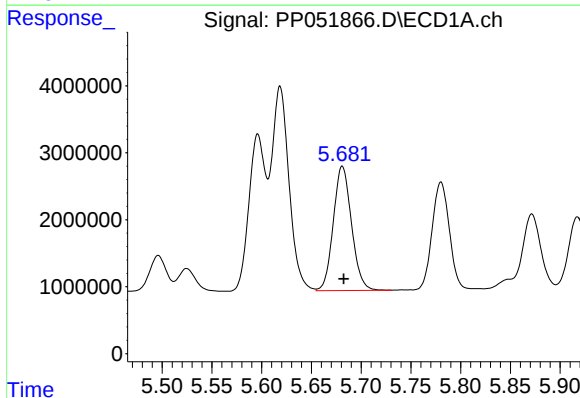


#18 AR-1242-3

R.T.: 5.681 min
Delta R.T.: -0.001 min
Response: 23631201
Conc: 659.97 ng/ml

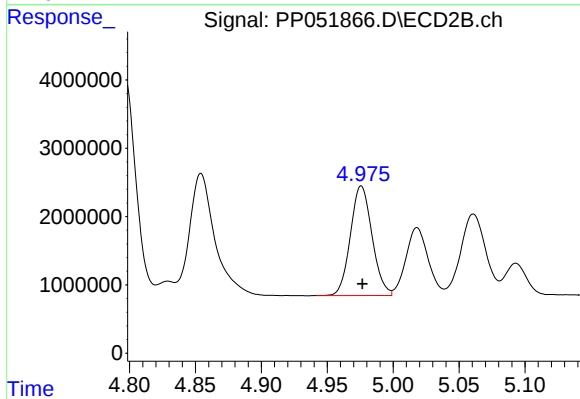

#18 AR-1242-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 18340365
Conc: 622.74 ng/ml

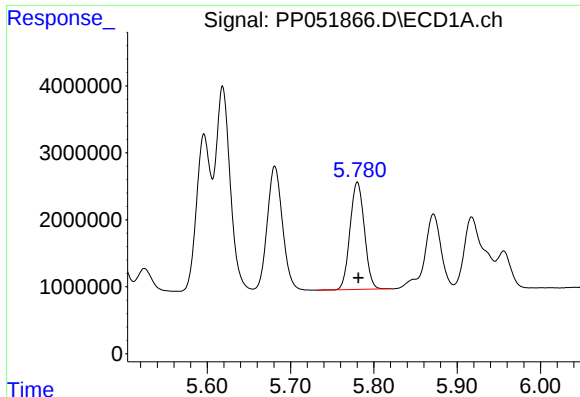

#19 AR-1242-4


R.T.: 5.780 min
Delta R.T.: -0.001 min
Response: 19165078
Conc: 665.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

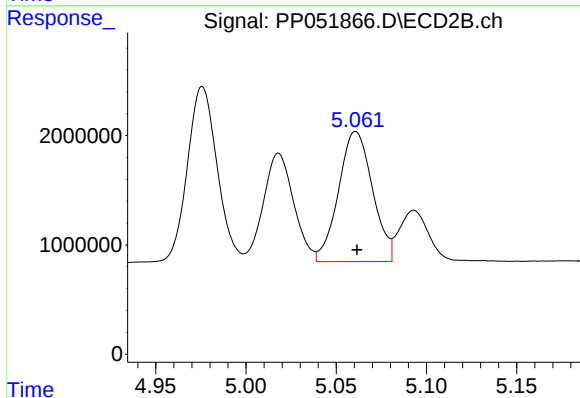


#19 AR-1242-4

R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 15634692
Conc: 530.05 ng/ml

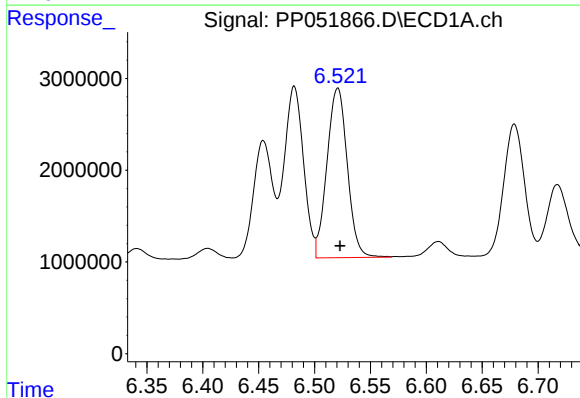


#20 AR-1242-5

R.T.: 6.521 min
Delta R.T.: -0.002 min
Response: 23462831
Conc: 622.95 ng/ml

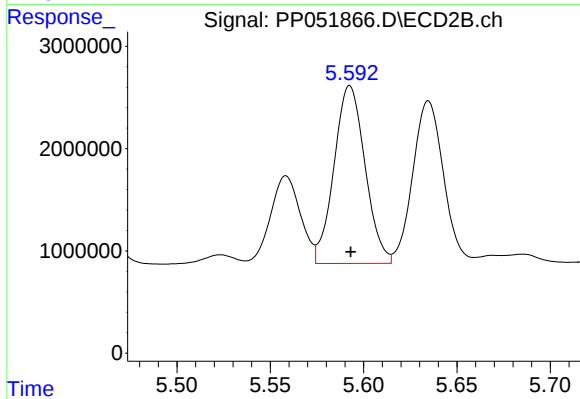

#20 AR-1242-5


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 20133819
Conc: 551.52 ng/ml

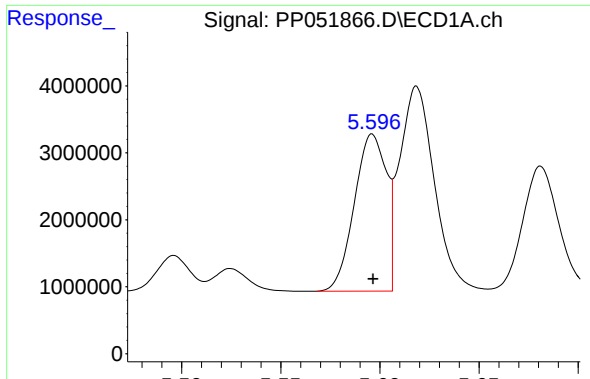

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 26367829
Conc: 870.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

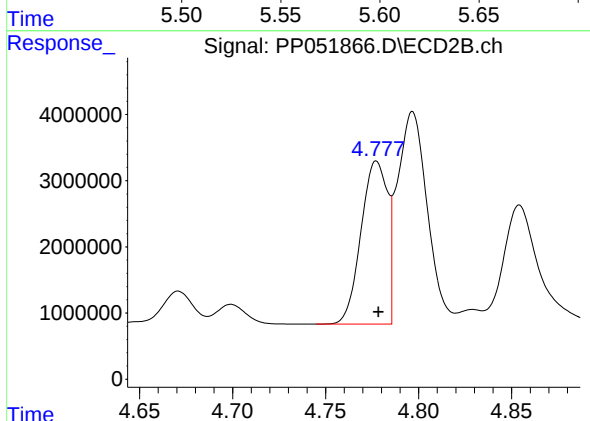


#21 AR-1248-1

R.T.: 4.777 min
Delta R.T.: -0.001 min
Response: 24381513
Conc: 834.85 ng/ml

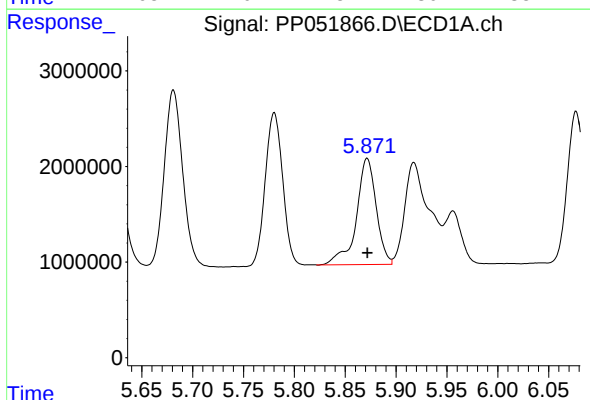


#22 AR-1248-2

R.T.: 5.872 min
Delta R.T.: 0.000 min
Response: 15107465
Conc: 333.40 ng/ml

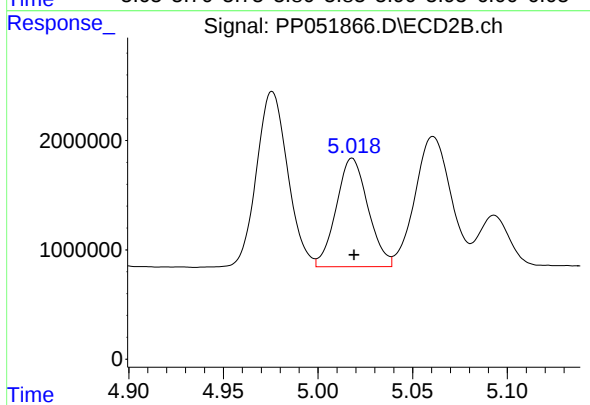

#22 AR-1248-2


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 11616544
Conc: 288.34 ng/ml

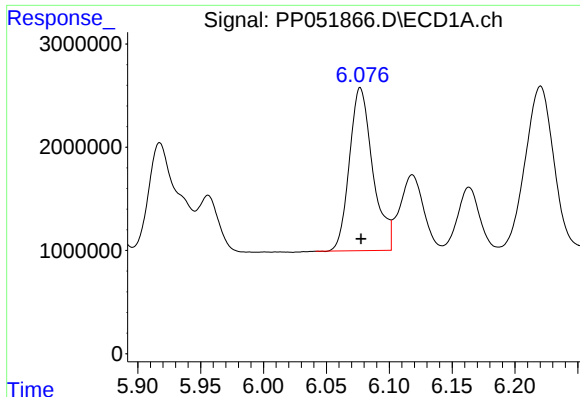

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 20376956
Conc: 401.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

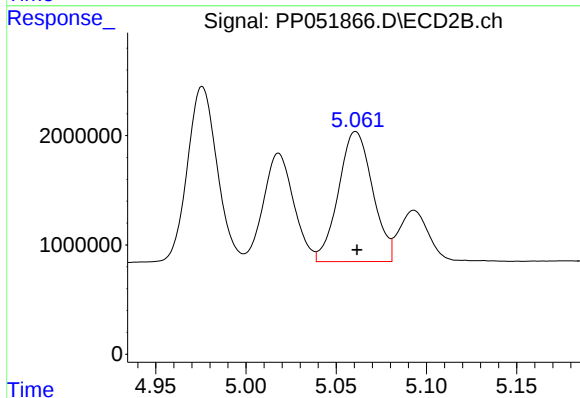


#23 AR-1248-3

R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 15634692
Conc: 368.36 ng/ml

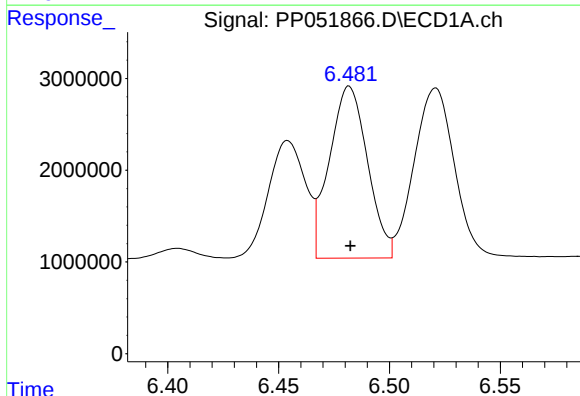


#24 AR-1248-4

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 22454222
Conc: 336.06 ng/ml

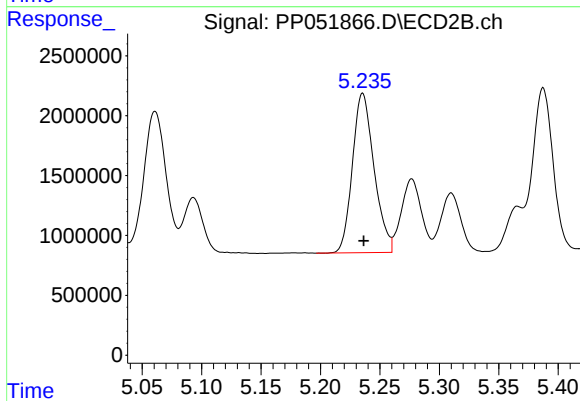

#24 AR-1248-4


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 16837710
Conc: 335.42 ng/ml

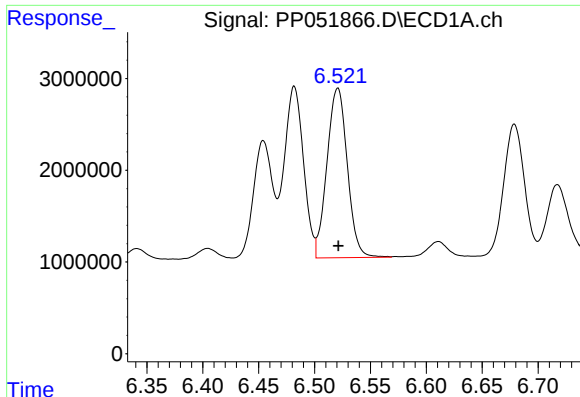

#25 AR-1248-5


R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 23462831
Conc: 357.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

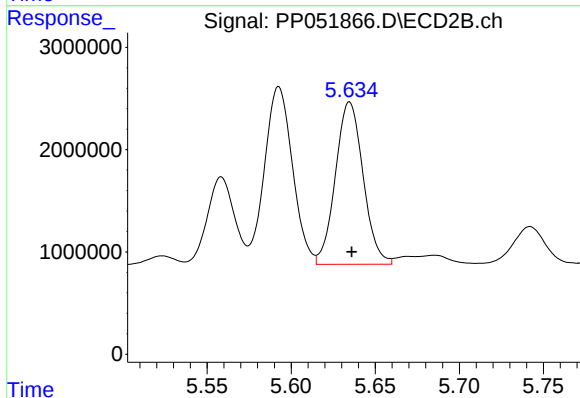


#25 AR-1248-5

R.T.: 5.635 min
Delta R.T.: -0.001 min
Response: 18207259
Conc: 371.42 ng/ml

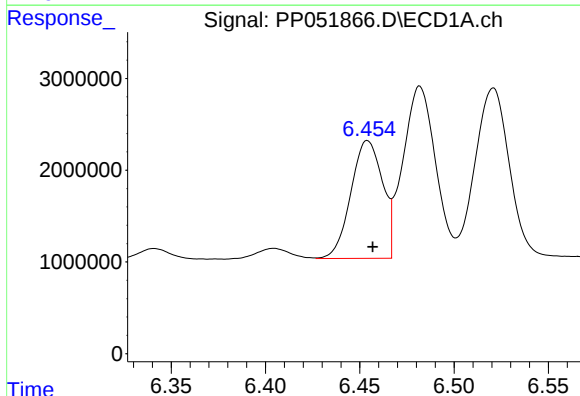


#26 AR-1254-1

R.T.: 6.454 min
Delta R.T.: -0.003 min
Response: 15026148
Conc: 220.21 ng/ml

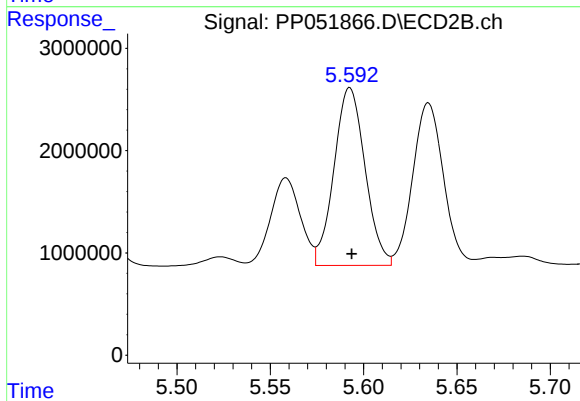

#26 AR-1254-1


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 20133819
Conc: 270.64 ng/ml

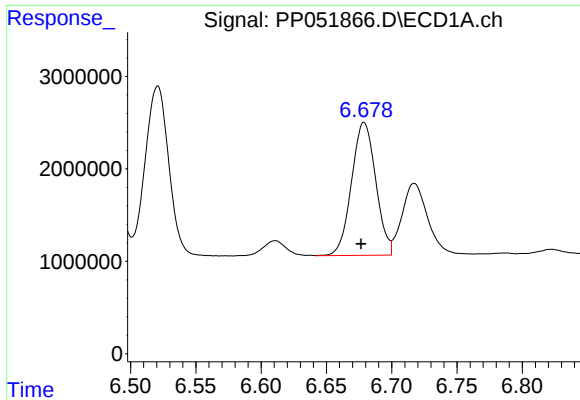

#27 AR-1254-2


R.T.: 6.679 min
Delta R.T.: 0.002 min
Response: 18580003
Conc: 181.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

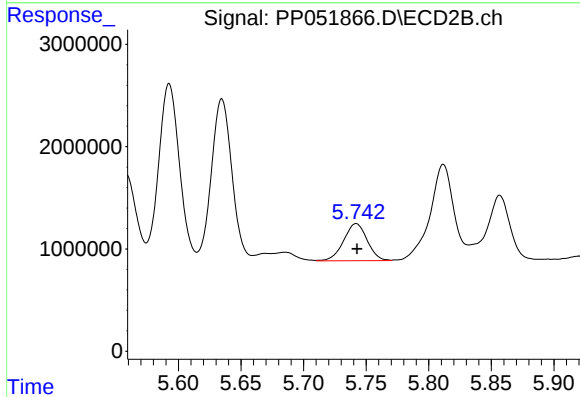


#27 AR-1254-2

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 4778103
Conc: 74.10 ng/ml

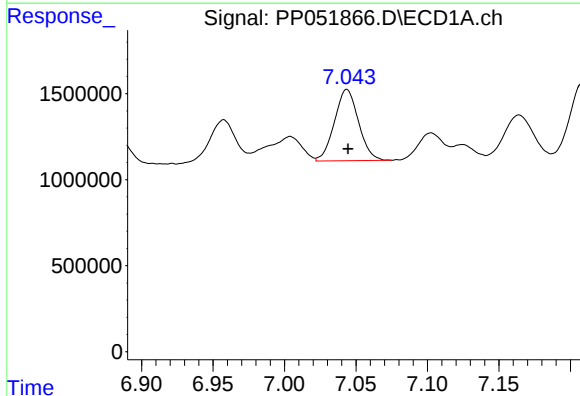


#28 AR-1254-3

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 4861610
Conc: 47.48 ng/ml

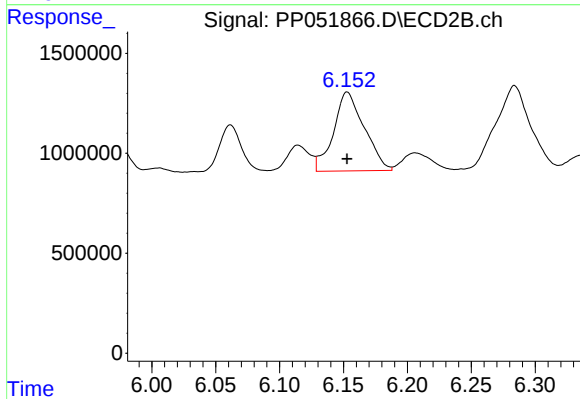

#28 AR-1254-3


R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 6599594
Conc: 62.68 ng/ml

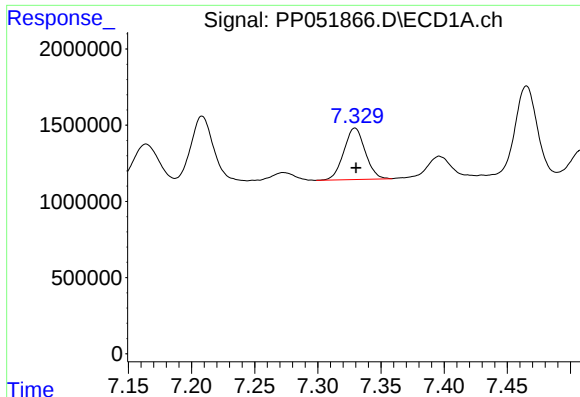

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 3980171
Conc: 55.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

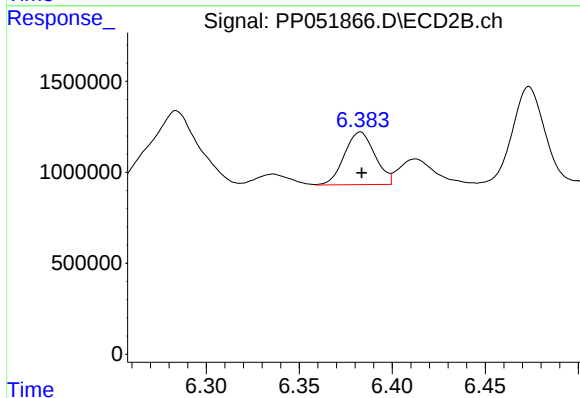


#29 AR-1254-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 3298619
Conc: 48.39 ng/ml

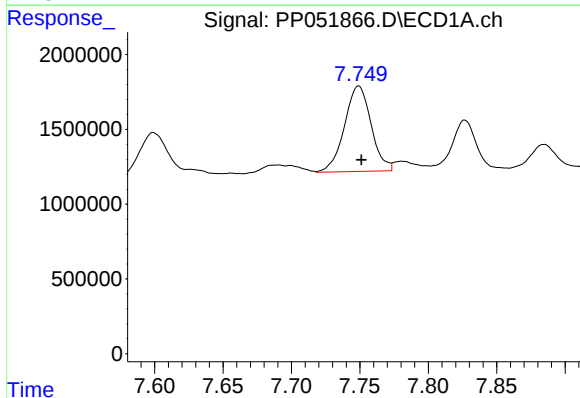


#30 AR-1254-5

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 7759674
Conc: 103.14 ng/ml

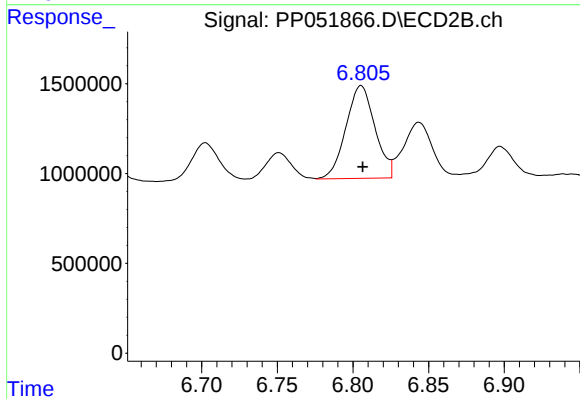

#30 AR-1254-5


R.T.: 6.805 min
Delta R.T.: -0.001 min
Response: 6896604
Conc: 74.55 ng/ml

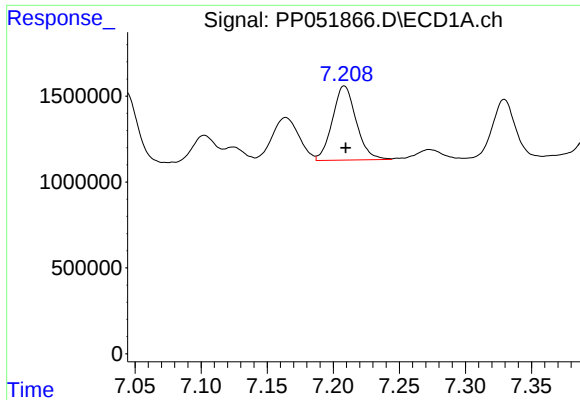

#31 AR-1260-1


R.T.: 7.208 min
Delta R.T.: -0.001 min
Response: 5401322
Conc: 75.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

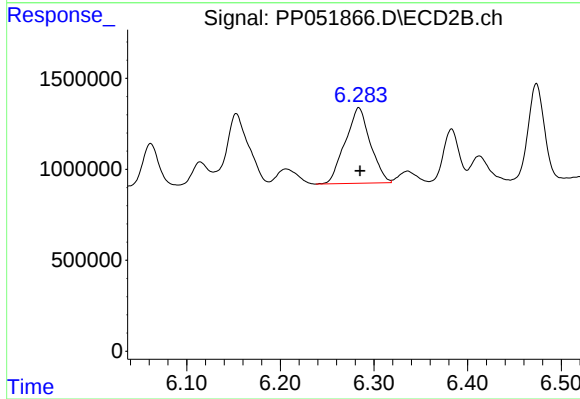


#31 AR-1260-1

R.T.: 6.284 min
Delta R.T.: -0.001 min
Response: 7730346
Conc: 112.23 ng/ml

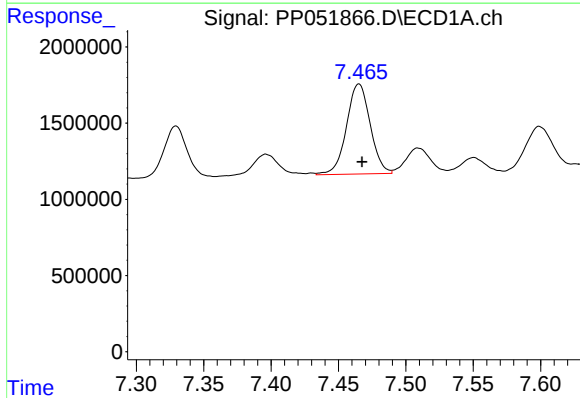


#32 AR-1260-2

R.T.: 7.465 min
Delta R.T.: -0.002 min
Response: 7243167
Conc: 88.68 ng/ml

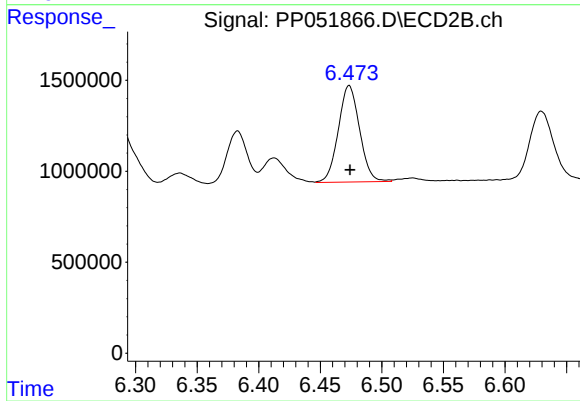

#32 AR-1260-2


R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 6368690
Conc: 75.68 ng/ml

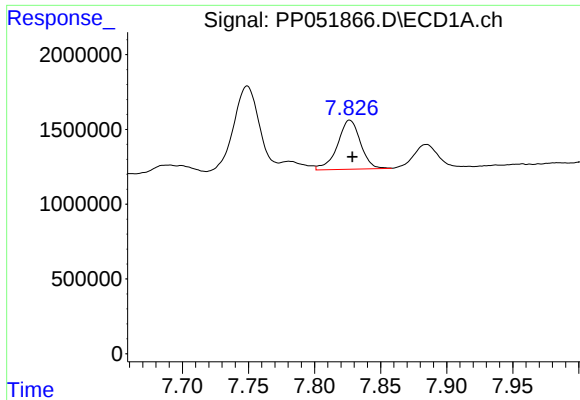

#33 AR-1260-3


R.T.: 7.827 min
Delta R.T.: -0.002 min
Response: 3970030
Conc: 69.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

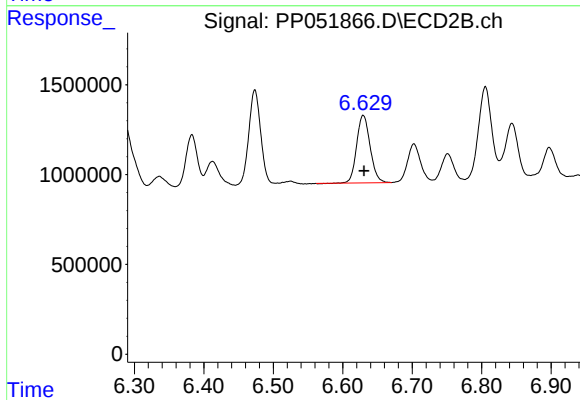


#33 AR-1260-3

R.T.: 6.630 min
Delta R.T.: -0.001 min
Response: 5054049
Conc: 64.93 ng/ml

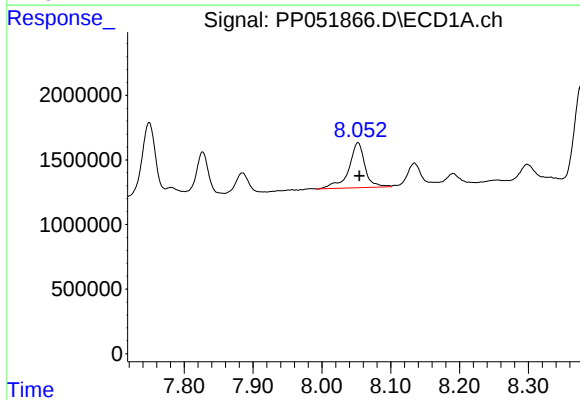


#34 AR-1260-4

R.T.: 8.052 min
Delta R.T.: -0.002 min
Response: 5724905
Conc: 87.41 ng/ml

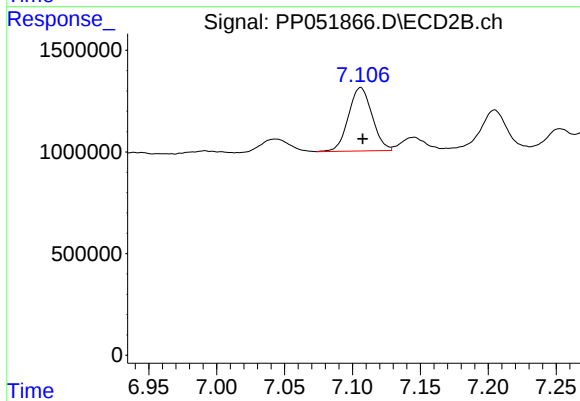

#34 AR-1260-4


R.T.: 7.106 min
Delta R.T.: -0.002 min
Response: 3770394
Conc: 59.89 ng/ml

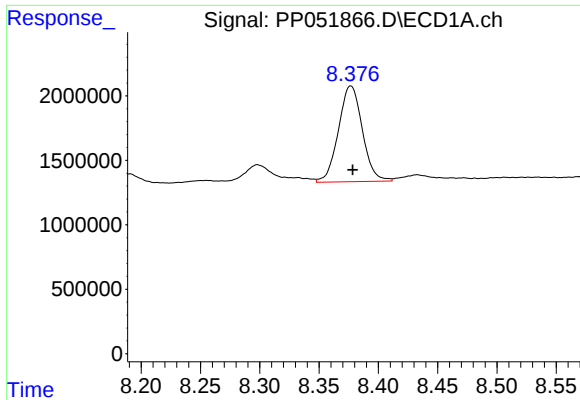

#35 AR-1260-5


R.T.: 8.377 min
Delta R.T.: -0.001 min
Response: 10450565
Conc: 82.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

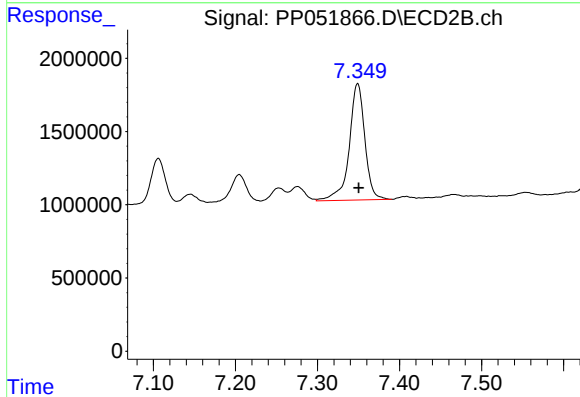


#35 AR-1260-5

R.T.: 7.349 min
Delta R.T.: -0.001 min
Response: 10524393
Conc: 71.76 ng/ml

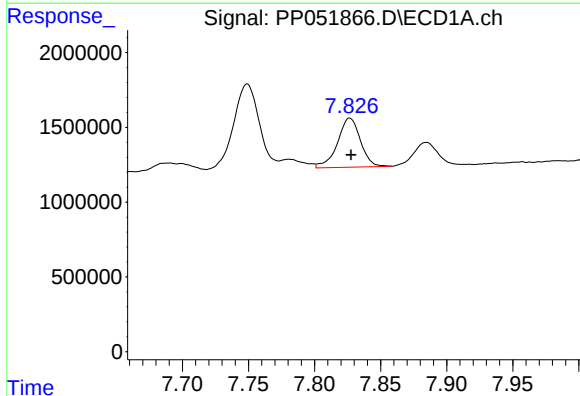


#36 AR-1262-1

R.T.: 7.827 min
Delta R.T.: 0.000 min
Response: 3970030
Conc: 45.66 ng/ml

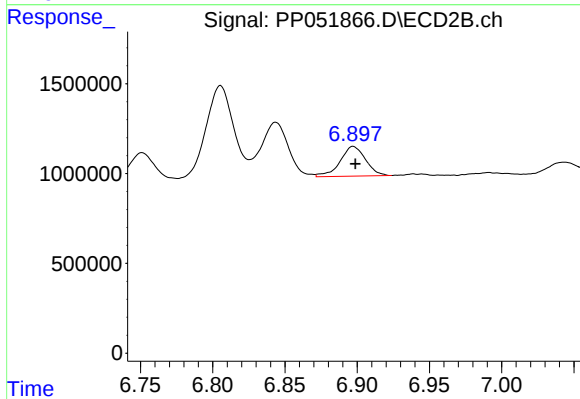

#36 AR-1262-1


R.T.: 6.897 min
Delta R.T.: -0.002 min
Response: 2026661
Conc: 53.93 ng/ml

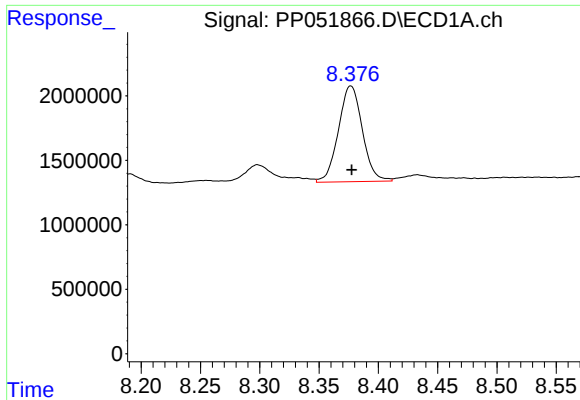

#37 AR-1262-2


R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 10450565
Conc: 70.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

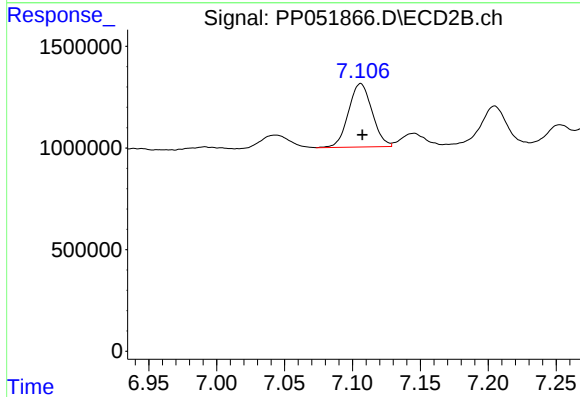


#37 AR-1262-2

R.T.: 7.106 min
Delta R.T.: -0.001 min
Response: 3770394
Conc: 44.52 ng/ml

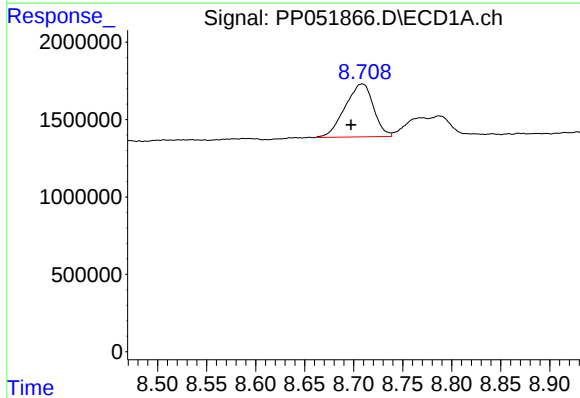


#38 AR-1262-3

R.T.: 8.709 min
Delta R.T.: 0.011 min
Response: 6901143
Conc: 67.03 ng/ml

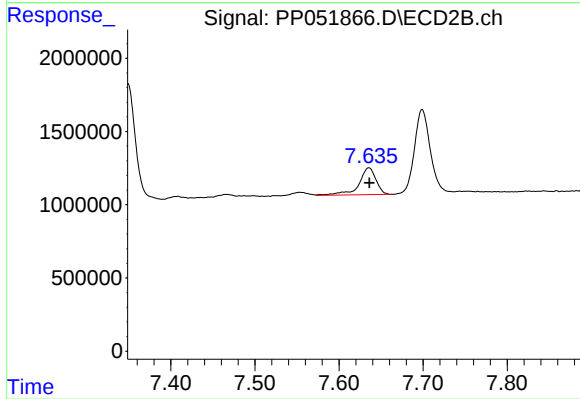

#38 AR-1262-3


R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 2576092
Conc: 36.73 ng/ml

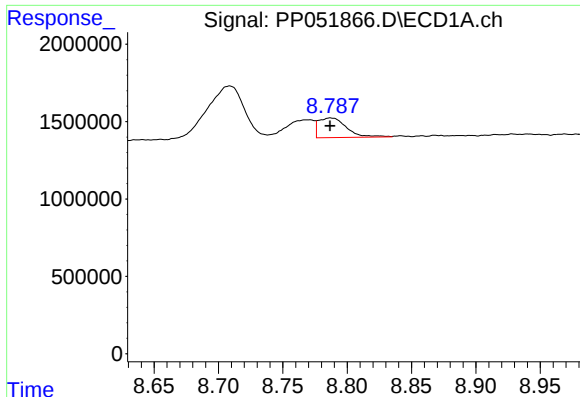

#39 AR-1262-4


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 1915687
Conc: 41.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

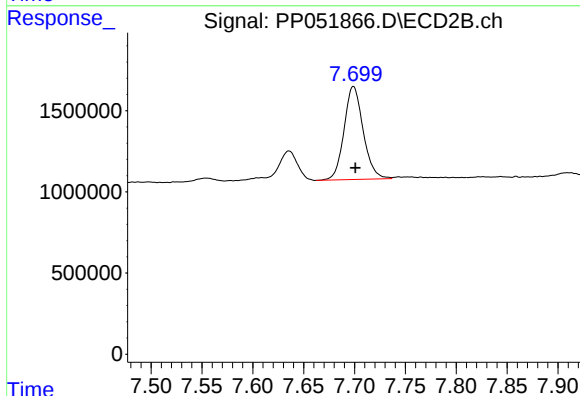


#39 AR-1262-4

R.T.: 7.699 min
Delta R.T.: -0.002 min
Response: 7513385
Conc: 60.13 ng/ml

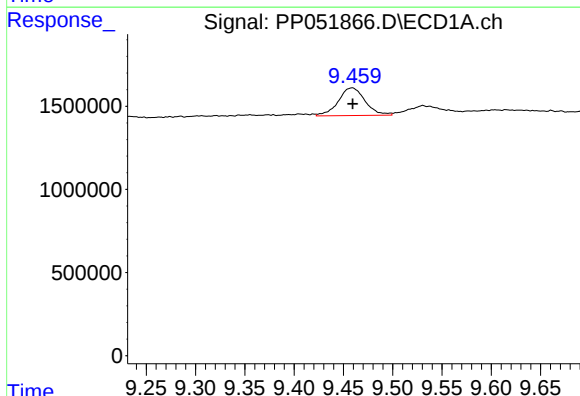


#40 AR-1262-5

R.T.: 9.459 min
Delta R.T.: 0.000 min
Response: 3163586
Conc: 55.52 ng/ml

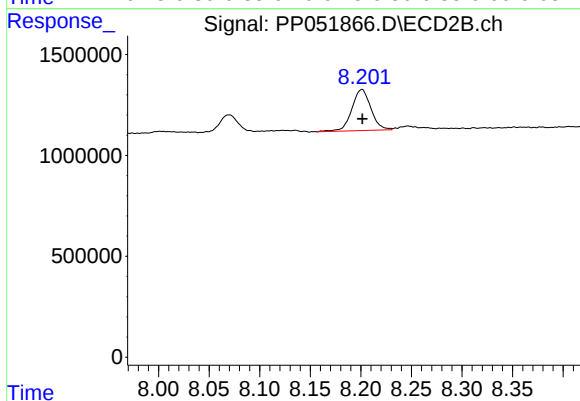

#40 AR-1262-5


R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 2665981
Conc: 47.05 ng/ml

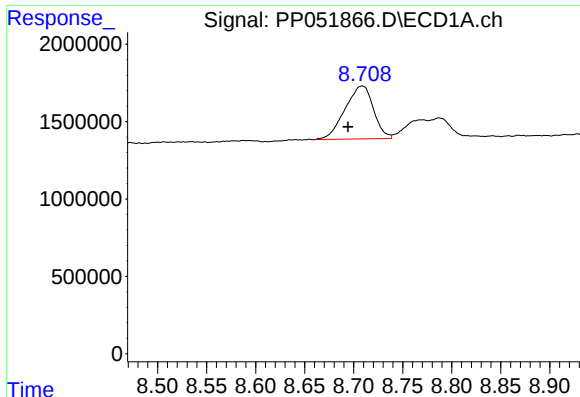

#41 AR-1268-1


R.T.: 8.709 min
Delta R.T.: 0.014 min
Response: 6901143
Conc: 38.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

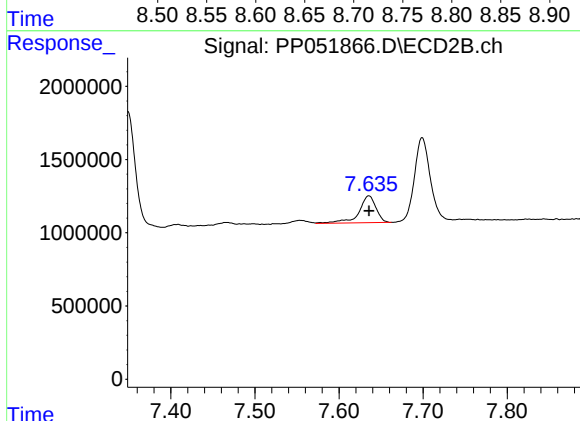


#41 AR-1268-1

R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 2576092
Conc: 12.98 ng/ml

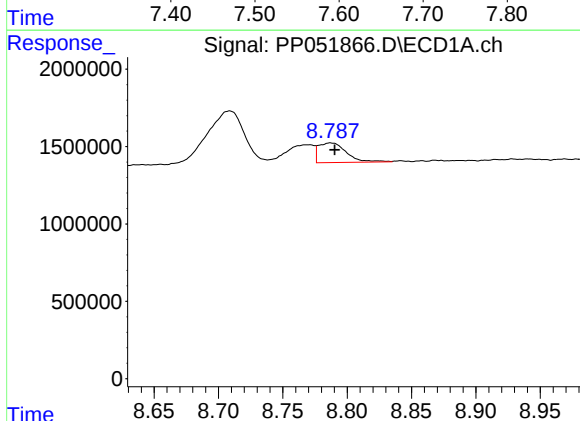


#42 AR-1268-2

R.T.: 8.787 min
Delta R.T.: -0.003 min
Response: 1915687
Conc: 11.56 ng/ml

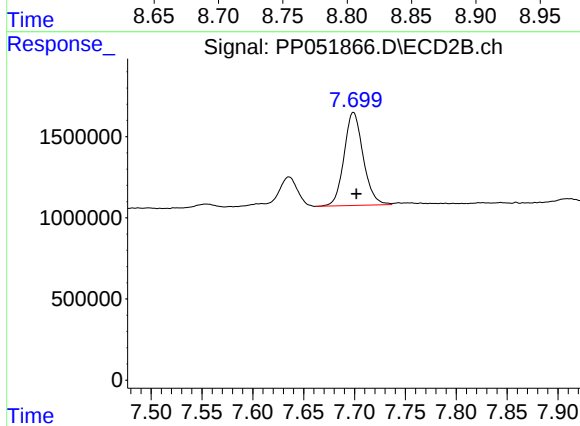

#42 AR-1268-2


R.T.: 7.699 min
Delta R.T.: -0.003 min
Response: 7513385
Conc: 42.04 ng/ml

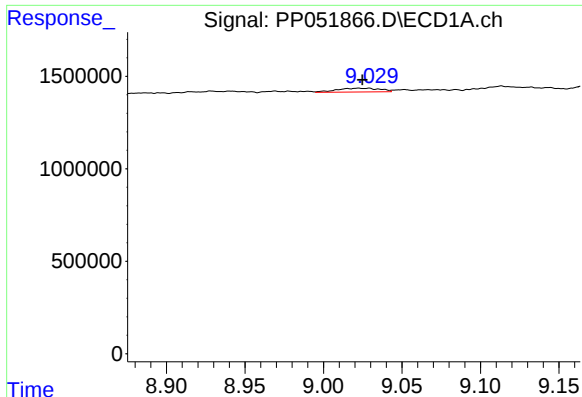

#43 AR-1268-3


R.T.: 9.022 min
Delta R.T.: -0.002 min
Response: 391149
Conc: 2.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

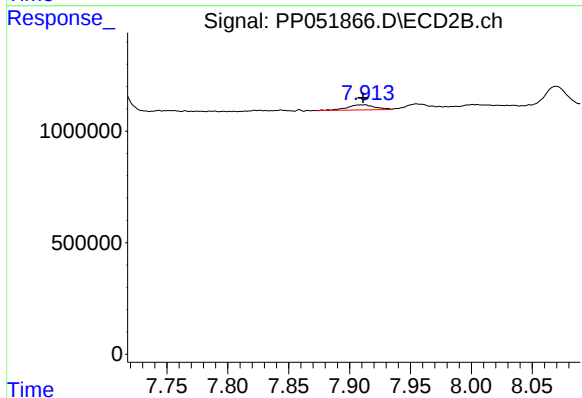


#43 AR-1268-3

R.T.: 7.911 min
Delta R.T.: 0.000 min
Response: 369063
Conc: 2.41 ng/ml

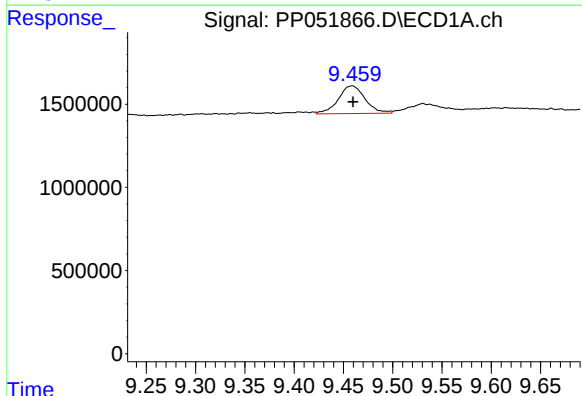


#44 AR-1268-4

R.T.: 9.459 min
Delta R.T.: -0.001 min
Response: 3163586
Conc: 49.39 ng/ml

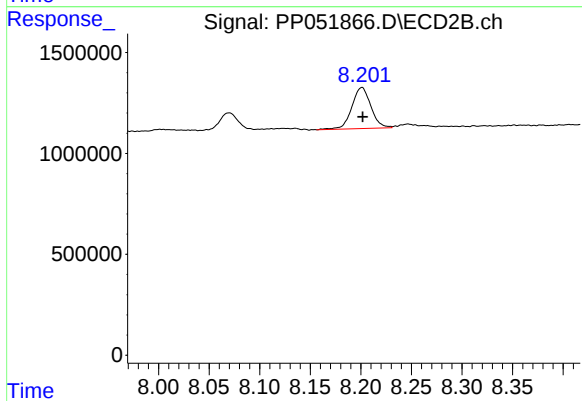

#44 AR-1268-4


R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 2665981
Conc: 42.47 ng/ml

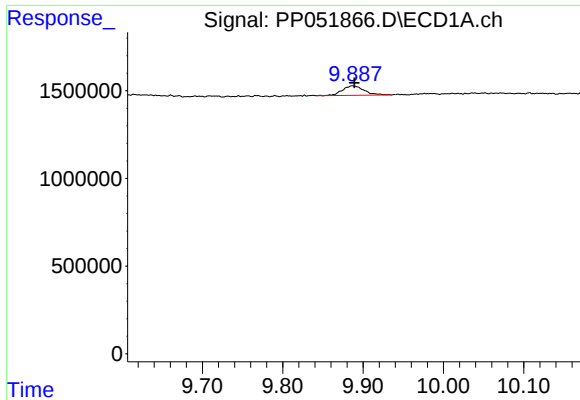

#45 AR-1268-5

R.T.: 9.887 min
Delta R.T.: -0.002 min
Response: 1016383
Conc: 2.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-1

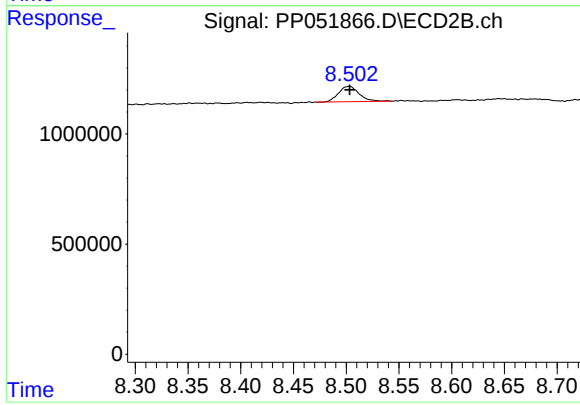

#45 AR-1268-5

R.T.: 8.503 min
Delta R.T.: 0.000 min
Response: 944808
Conc: 2.03 ng/ml