

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
 Data File : PP051867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 03:24
 Operator : YP\AJ
 Sample : N4888-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 REGULATORY-FOUNDATION-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:05:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 03:12:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.673	43456956	31367856	24.314	24.673
2) SA Decachlor...	10.240	8.769	33699344	32676732	27.798	27.666

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100322\
Data File : PP051867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 03:24
Operator : YP\AJ
Sample : N4888-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:05:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 04 03:12:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

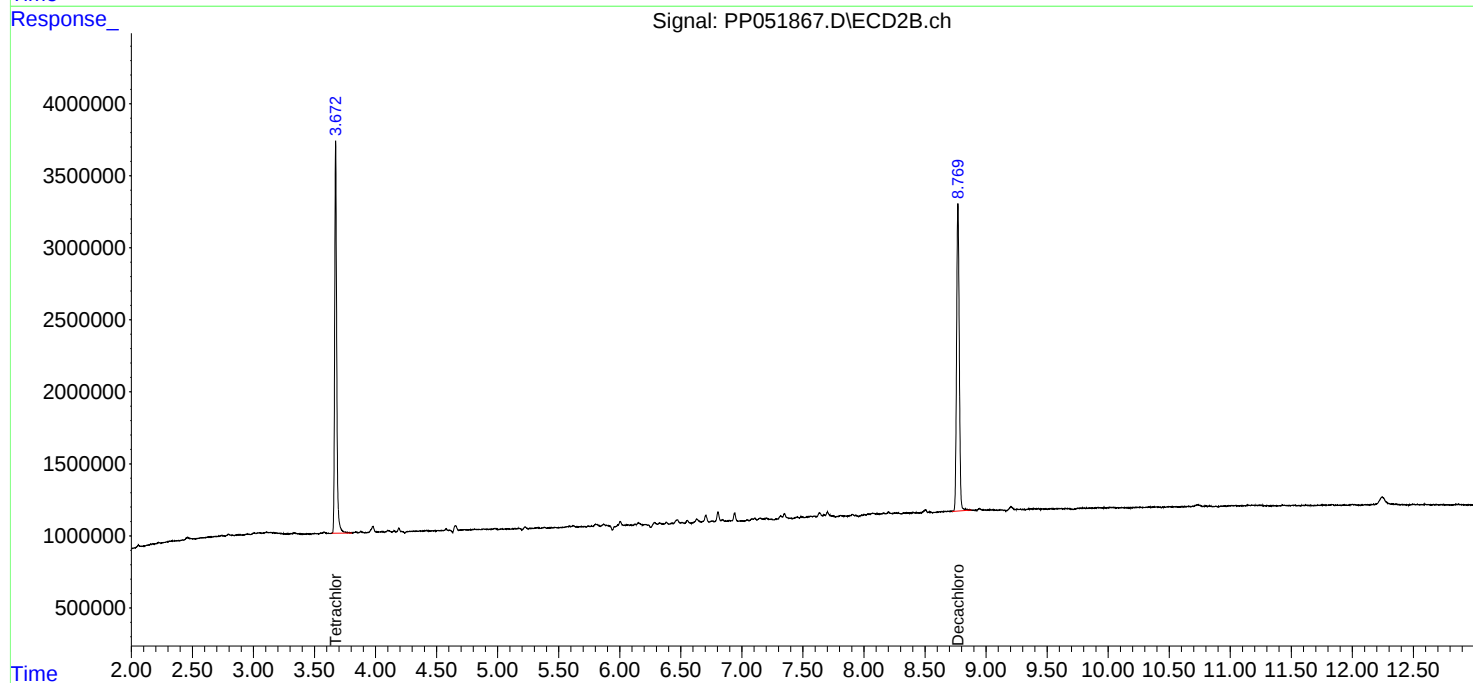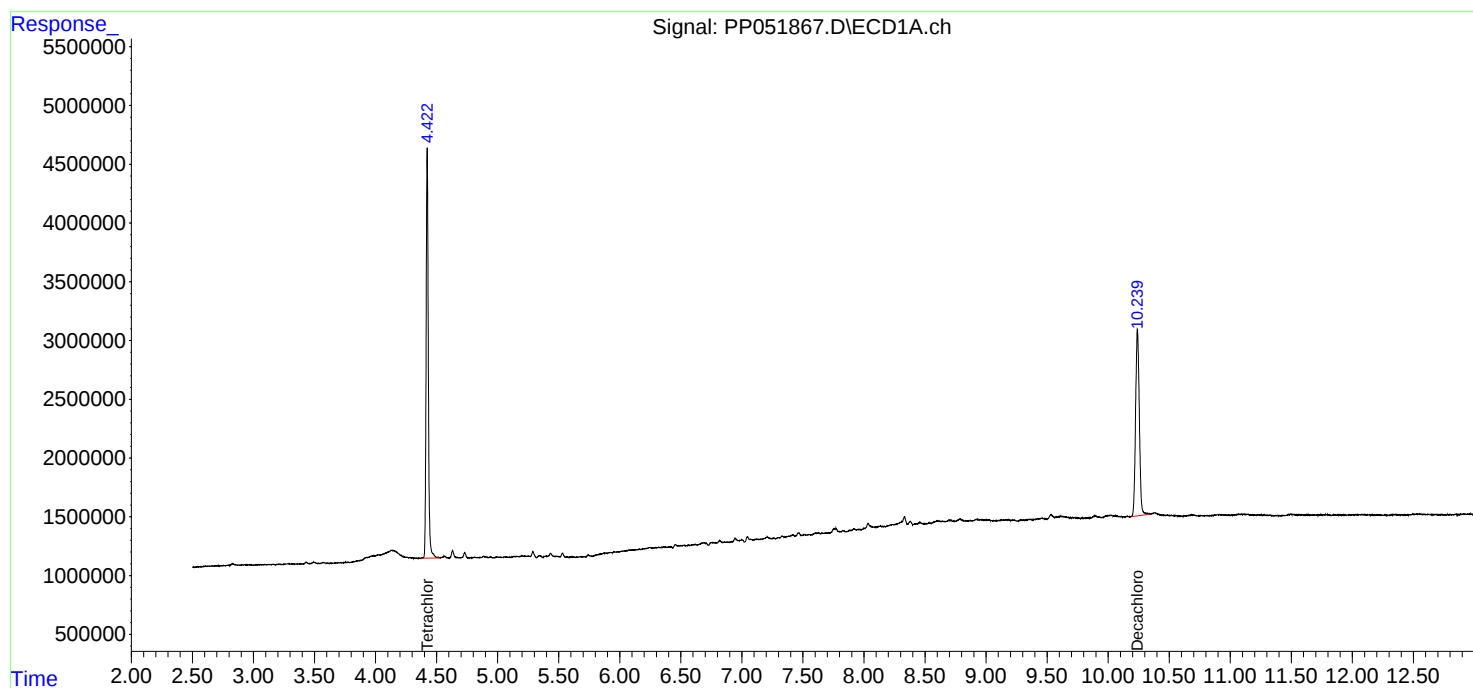


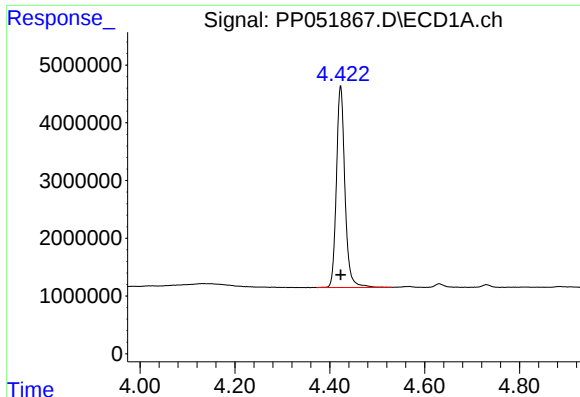

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: 0.000 min
Response: 43456956
Conc: 24.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
REGULATORY-FOUNDATION-2

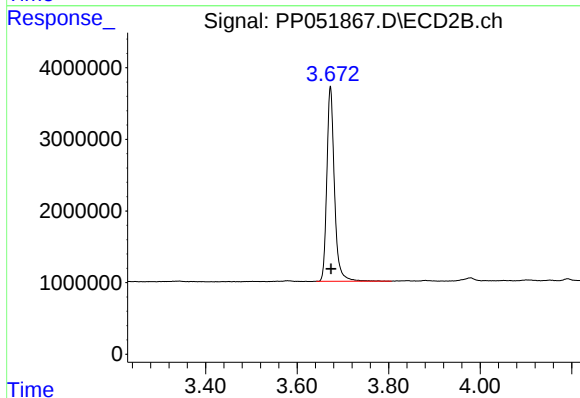


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.001 min
Response: 31367856
Conc: 24.67 ng/ml

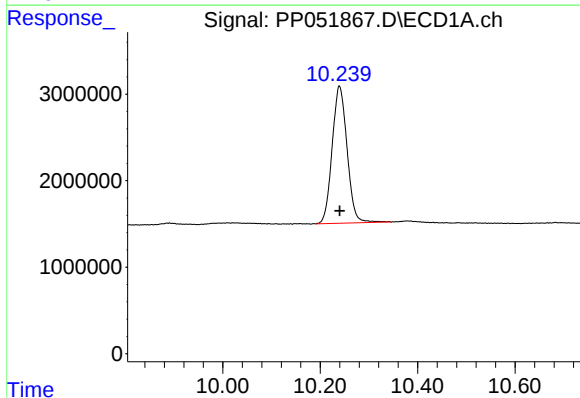

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.000 min
Response: 33699344
Conc: 27.80 ng/ml

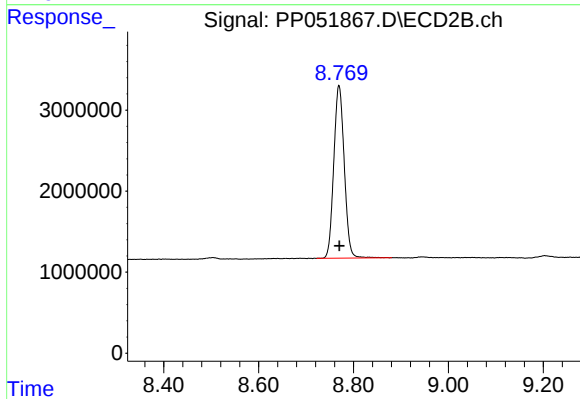

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: 0.000 min
Response: 32676732
Conc: 27.67 ng/ml