

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100323\
 Data File : PP060532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 14:34
 Operator : YP\AJ
 Sample : 04685-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PP-20230928-B4A-7.5-15

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/04/2023
 Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 17:17:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.533	3.686	35511252	24074533	15.857m	16.174m
2) SA Decachlor...	10.459	8.749	43333812	36615639	24.544	22.447

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100323\
Data File : PP060532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 14:34
Operator : YP\AJ
Sample : 04685-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PP-20230928-B4A-7.5-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 17:17:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

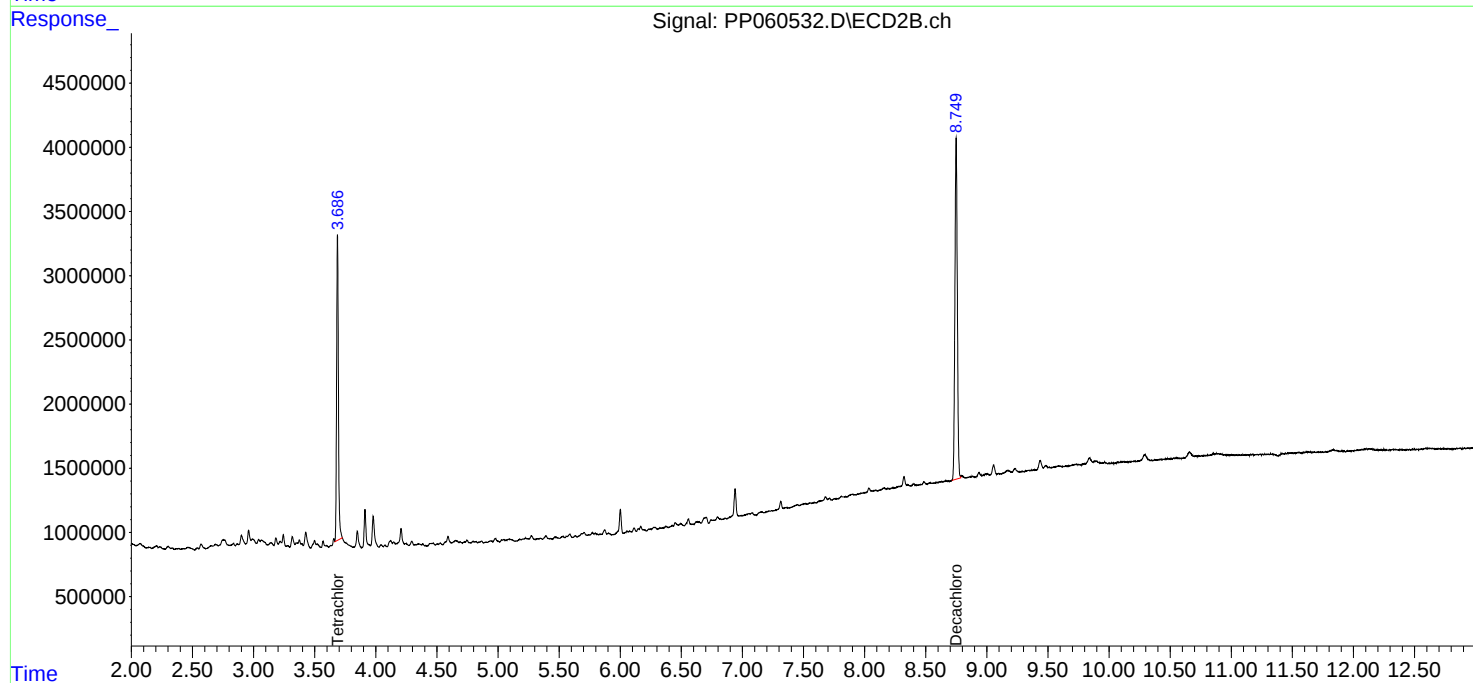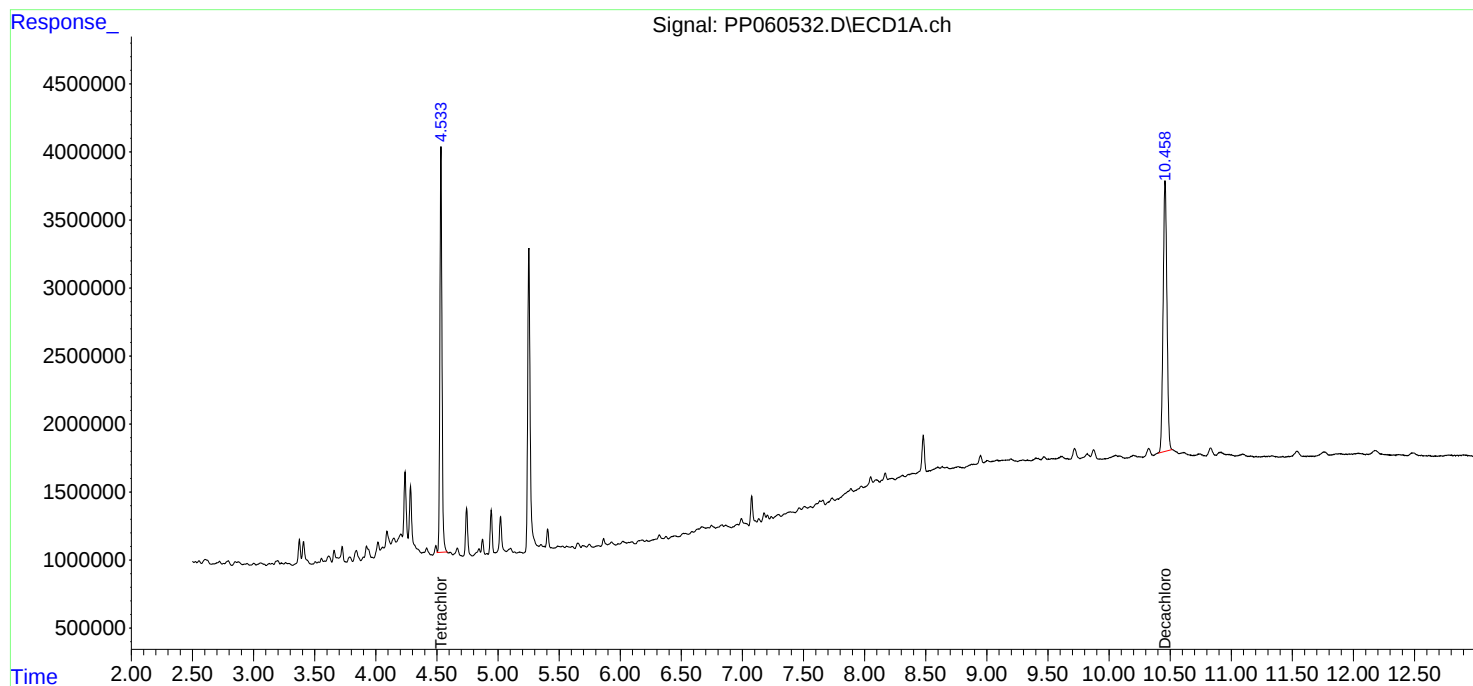

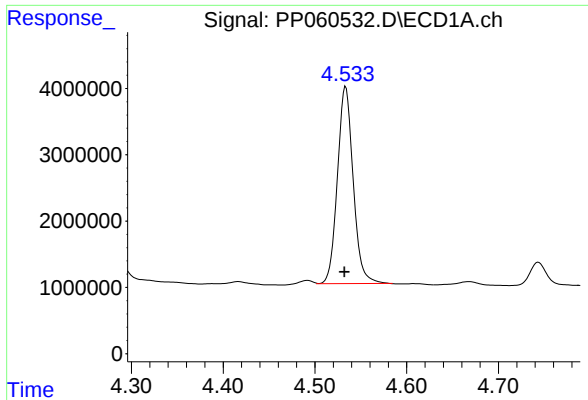


#1 Tetrachloro-m-xylene

R.T.: 4.533 min
Delta R.T.: 0.000 min
Response: 35511252
Conc: 15.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PP-20230928-B4A-7.5-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

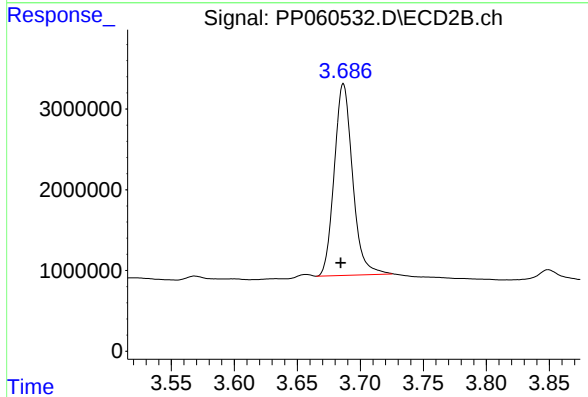


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: 0.002 min
Response: 24074533
Conc: 16.17 ng/ml m

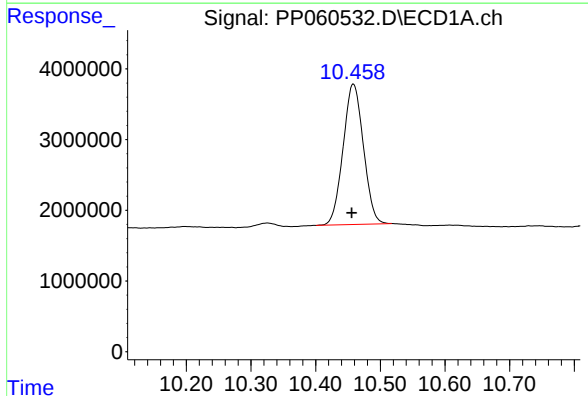

#2 Decachlorobiphenyl

R.T.: 10.459 min
Delta R.T.: 0.003 min
Response: 43333812
Conc: 24.54 ng/ml

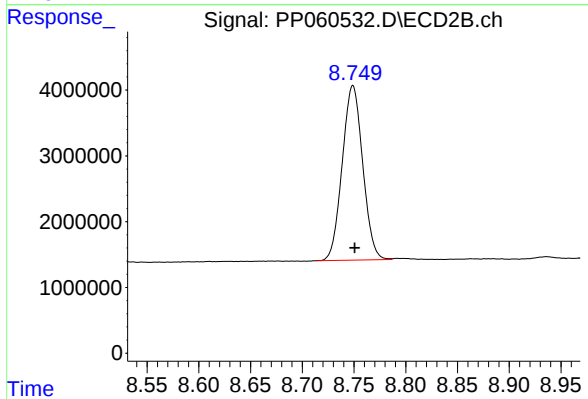

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.002 min
Response: 36615639
Conc: 22.45 ng/ml