

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100323\
 Data File : PP060558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 04:10
 Operator : YP\AJ
 Sample : 04704-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-104-1(5-10)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/04/2023
 Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 04:43:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.531	3.684	32264932	22091753	14.407	14.842
2) SA Decachlor...	10.456	8.747	20435874	15363917	11.575	9.419

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100323\
Data File : PP060558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 04:10
Operator : YP\AJ
Sample : 04704-05
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-104-1(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 04:43:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

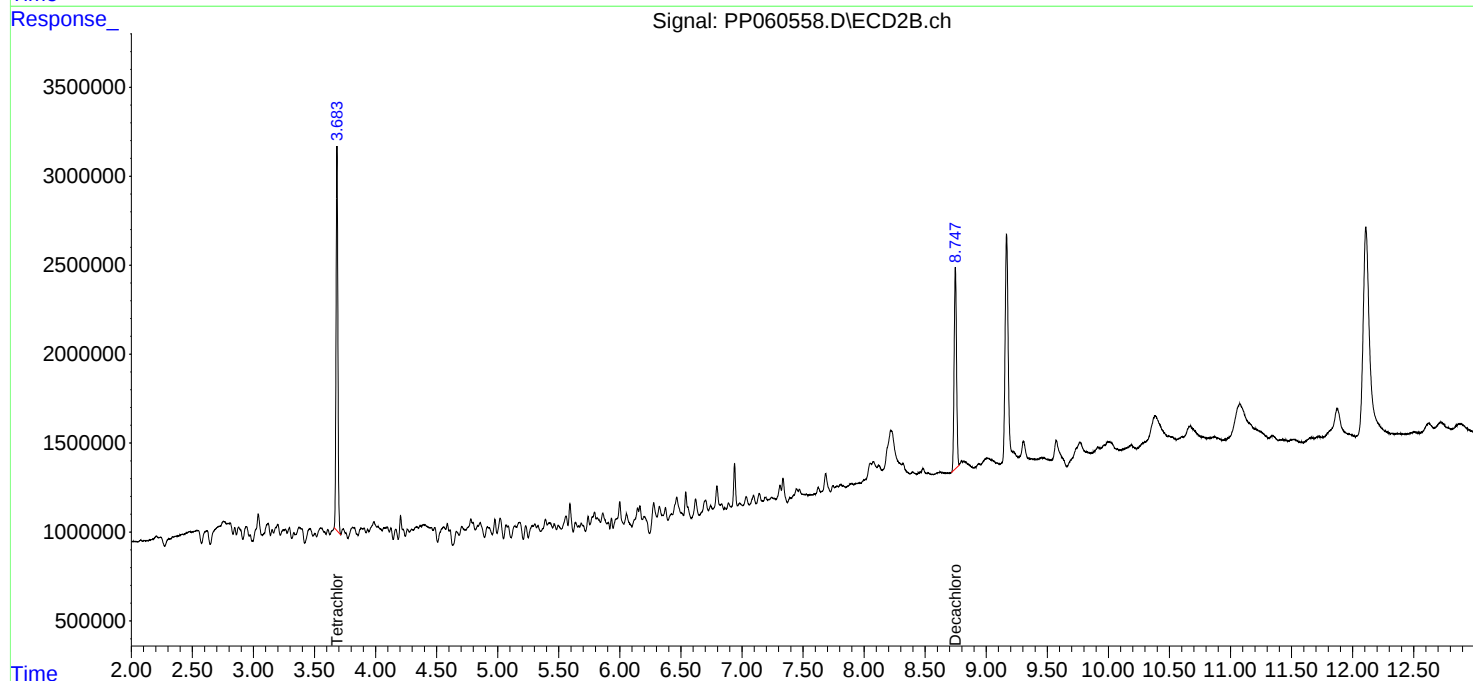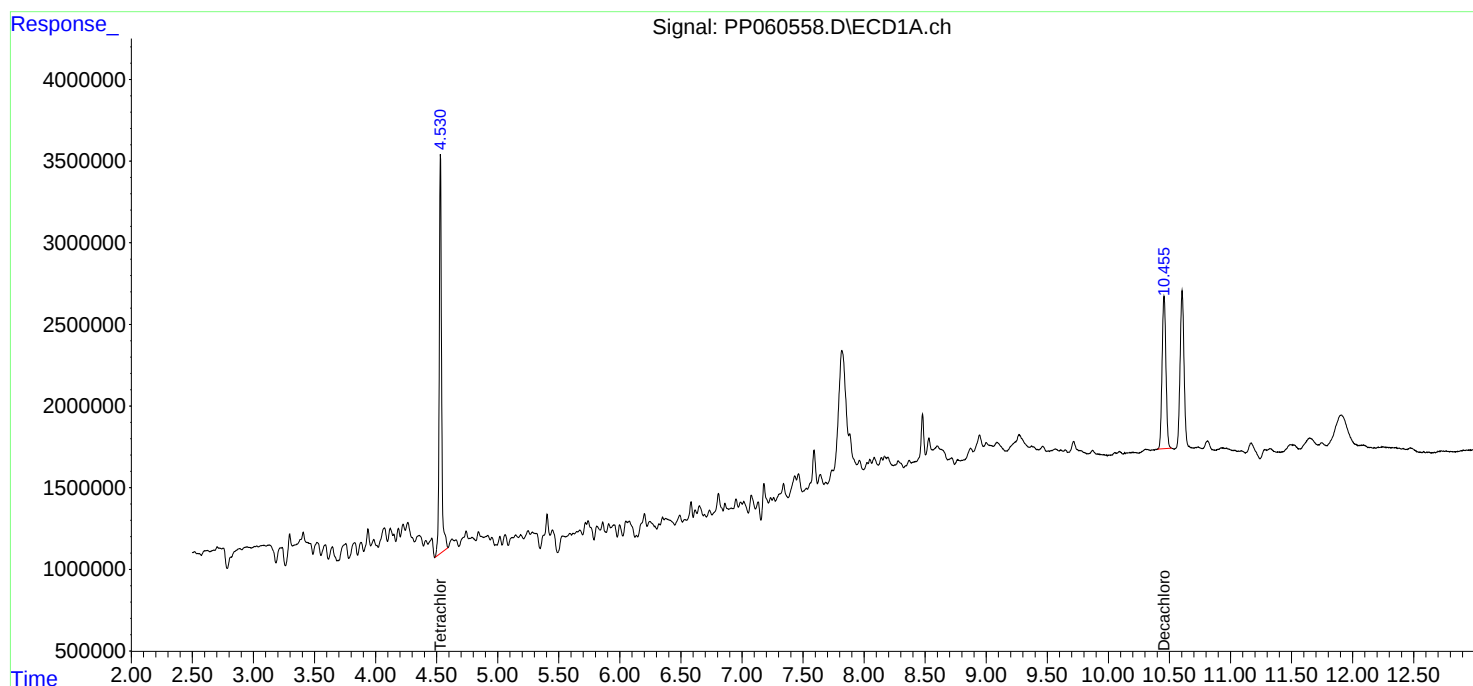

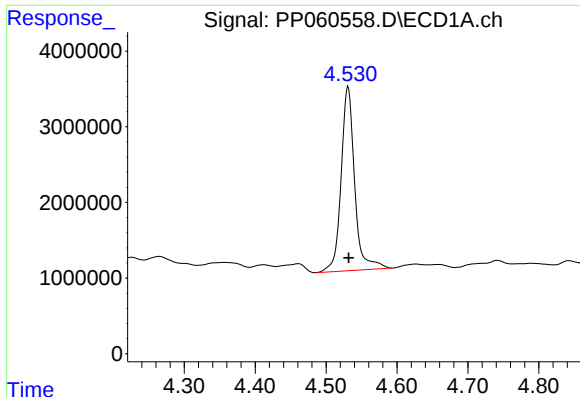

#1 Tetrachloro-m-xylene

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 32264932
Conc: 14.41 ng/ml

Instrument :

ECD_P


ClientSampleId :

SB-104-1(5-10)

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

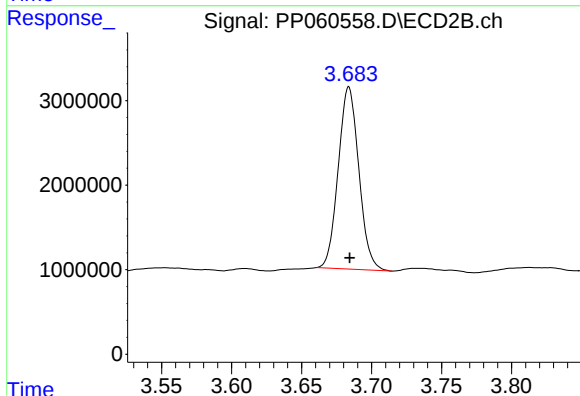


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.000 min
Response: 22091753
Conc: 14.84 ng/ml

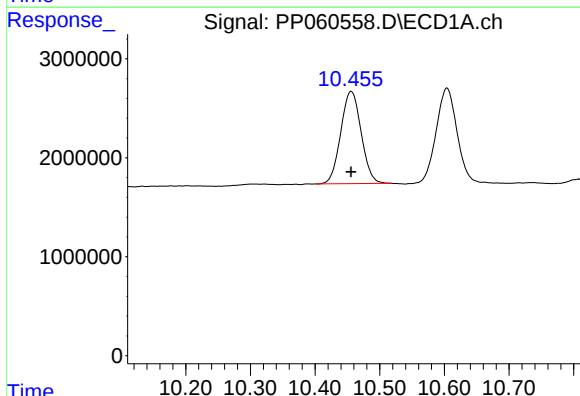

#2 Decachlorobiphenyl

R.T.: 10.456 min
Delta R.T.: 0.000 min
Response: 20435874
Conc: 11.57 ng/ml

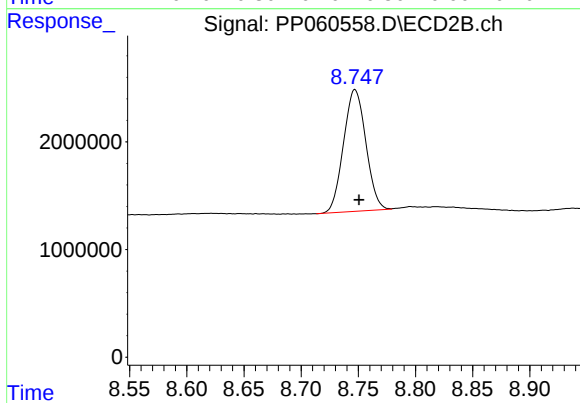

#2 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: -0.004 min
Response: 15363917
Conc: 9.42 ng/ml