

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
 Data File : PP039753.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 12:08
 Operator : AJ\MA
 Sample : M4021-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 16:36:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.905	3.995	647717	371715	20.460	22.813
2)	SA Decachlor...	10.930	9.327	503376	543625	23.204	24.877
Target Compounds							
28)	L6 AR-1254-3	7.769f	0.000	32614	0	19.601	N.D. #
30)	L6 AR-1254-5	0.000	7.389	0	20891	N.D.	14.842 #
32)	L7 AR-1260-2	0.000	7.028f	0	18654	N.D.	14.564 #
36)	L8 AR-1262-1	0.000	7.389	0	20891	N.D.	29.633 #
38)	L8 AR-1262-3	0.000	8.265f	0	19573	N.D.	19.258 #
40)	L8 AR-1262-5	0.000	8.784f	0	35652	N.D.	39.159 #
41)	L9 AR-1268-1	0.000	8.265f	0	19573	N.D.	6.713 #
44)	L9 AR-1268-4	0.000	8.784f	0	35652	N.D.	34.638 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
Data File : PP039753.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 12:08
Operator : AJ\MA
Sample : M4021-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 16:36:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

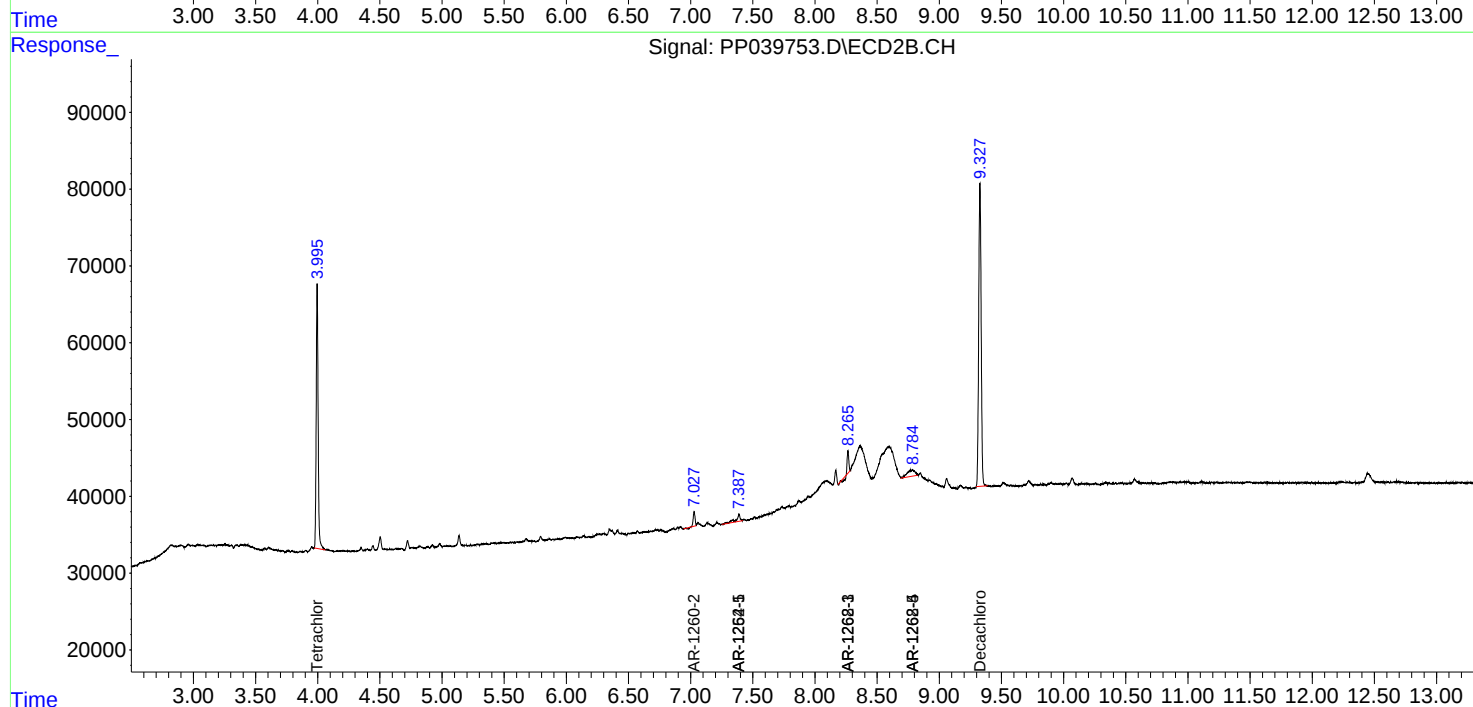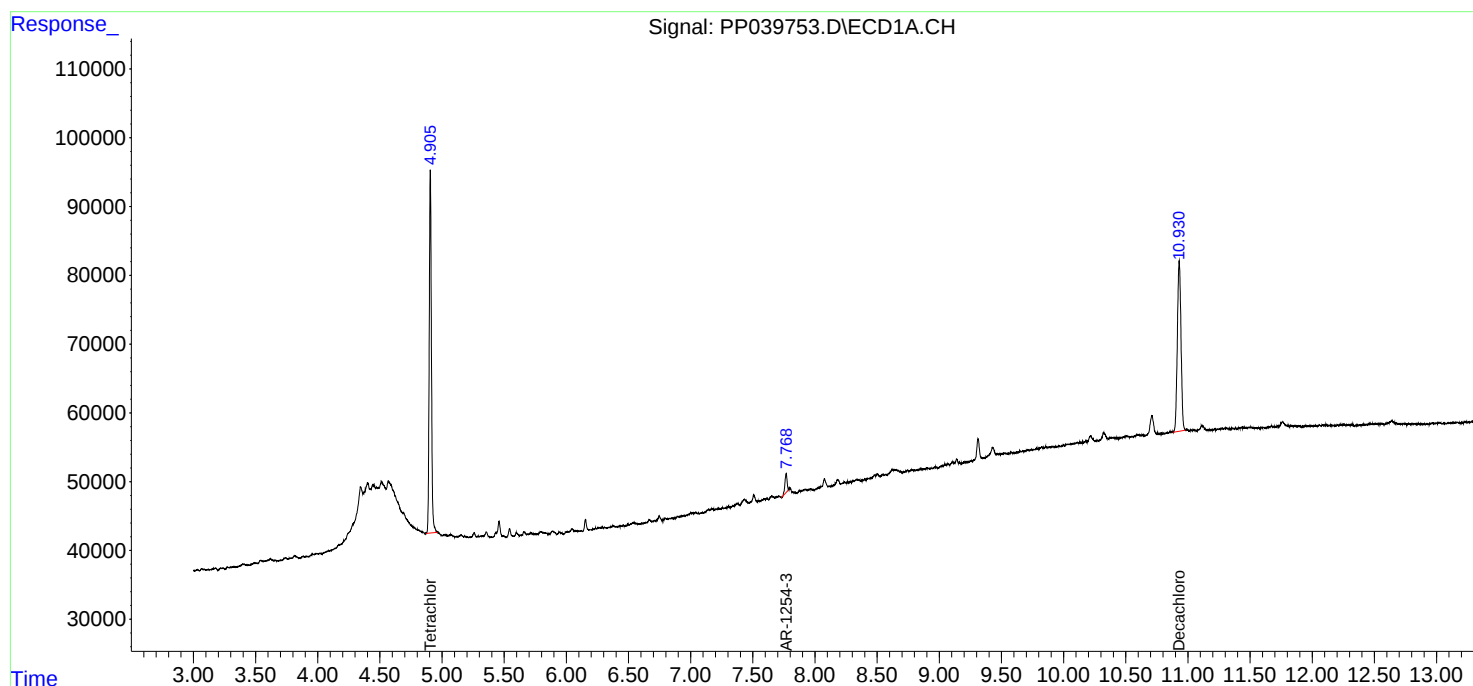


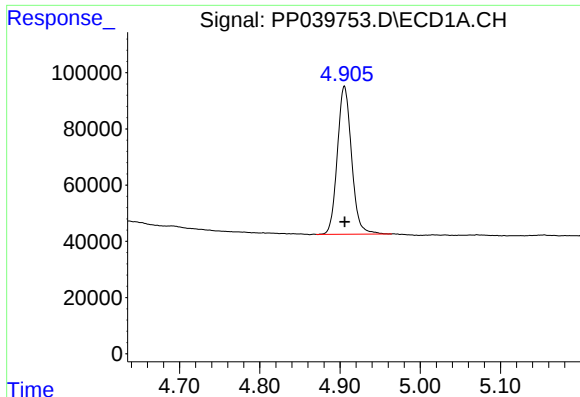

#1 Tetrachloro-m-xylene


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 647717
Conc: 20.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

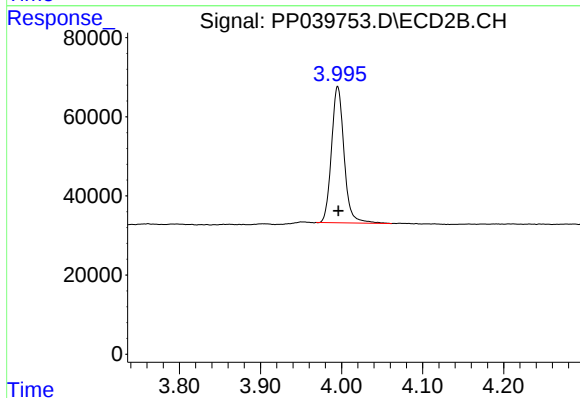


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 371715
Conc: 22.81 ng/ml

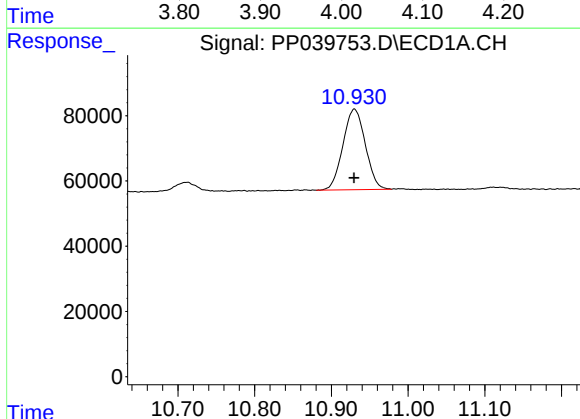


#2 Decachlorobiphenyl

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 503376
Conc: 23.20 ng/ml

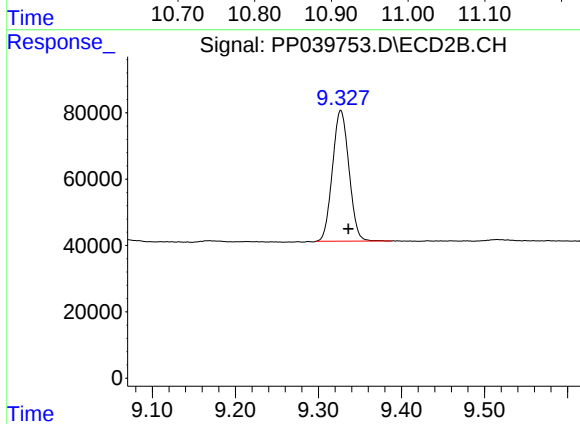

#2 Decachlorobiphenyl


R.T.: 9.327 min
Delta R.T.: -0.009 min
Response: 543625
Conc: 24.88 ng/ml

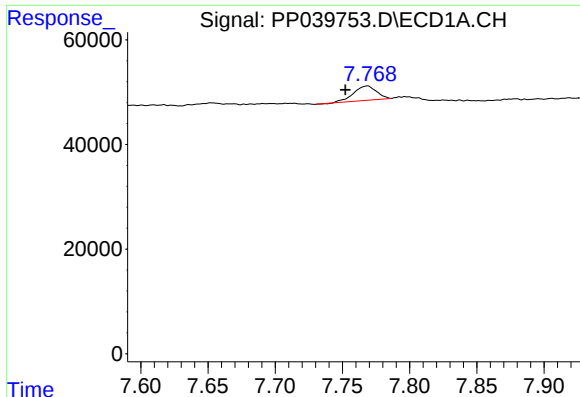

#28 AR-1254-3


R.T.: 7.769 min
Delta R.T.: 0.016 min
Response: 32614
Conc: 19.60 ng/ml

Instrument :
ECD_P
ClientSampleId :

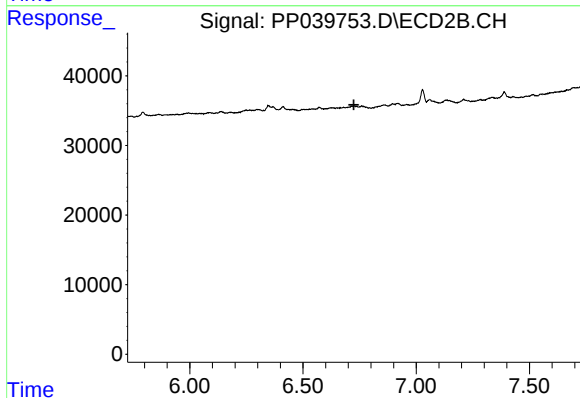


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

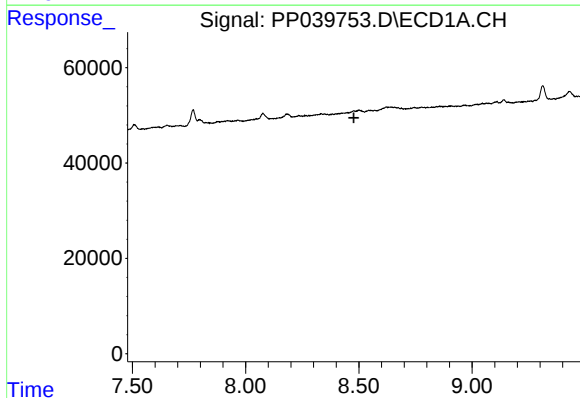


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.478 min
Response: 0
Conc: N.D.

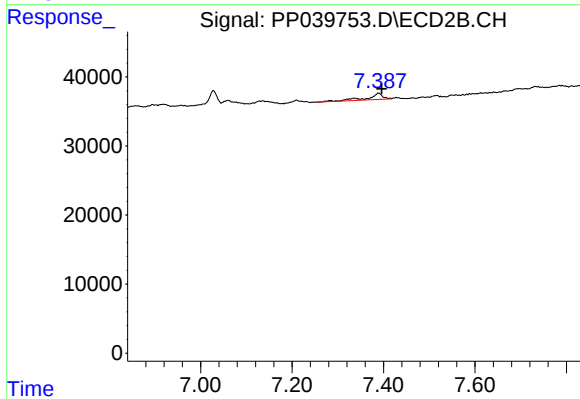

#30 AR-1254-5


R.T.: 7.389 min
Delta R.T.: -0.007 min
Response: 20891
Conc: 14.84 ng/ml

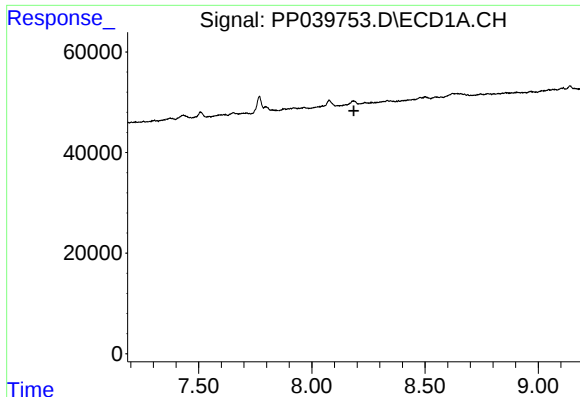

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

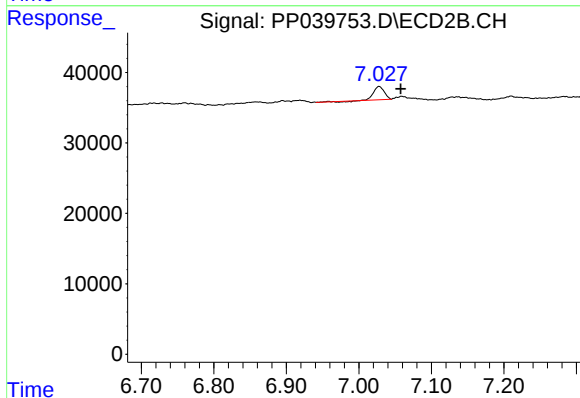


#32 AR-1260-2

R.T.: 7.028 min
Delta R.T.: -0.030 min
Response: 18654
Conc: 14.56 ng/ml

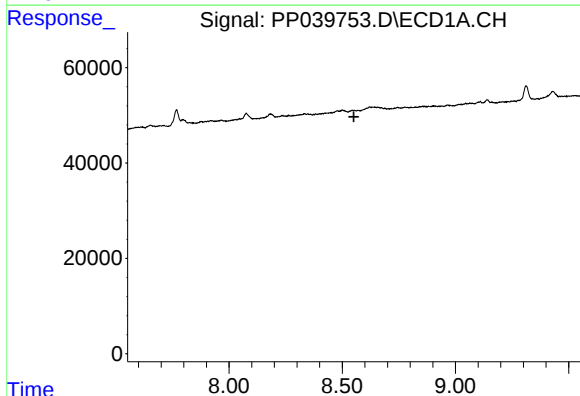


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.552 min
Response: 0
Conc: N.D.

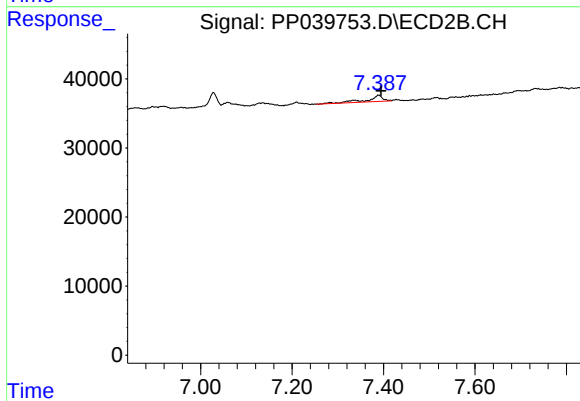

#36 AR-1262-1


R.T.: 7.389 min
Delta R.T.: -0.005 min
Response: 20891
Conc: 29.63 ng/ml

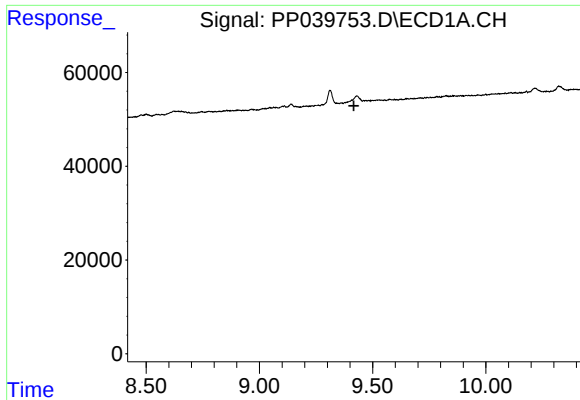

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

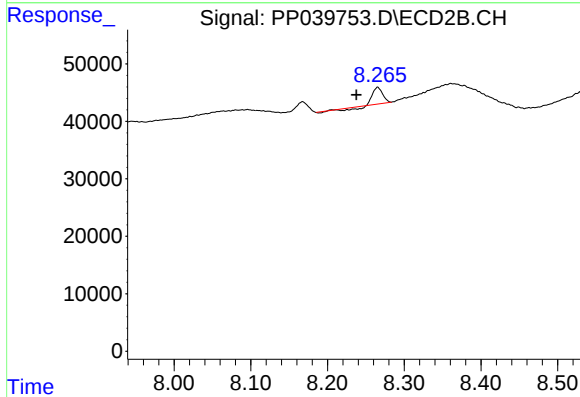


#38 AR-1262-3

R.T.: 8.265 min
Delta R.T.: 0.028 min
Response: 19573
Conc: 19.26 ng/ml

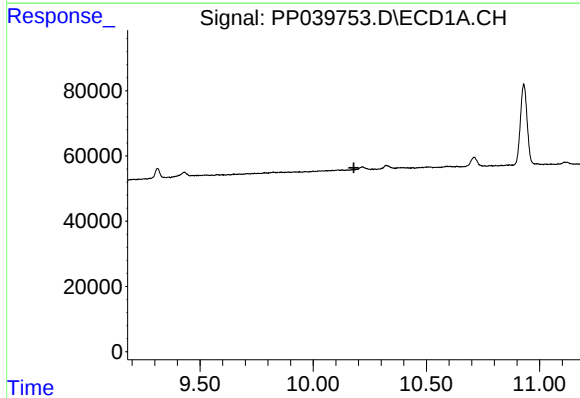


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 10.180 min
Response: 0
Conc: N.D.

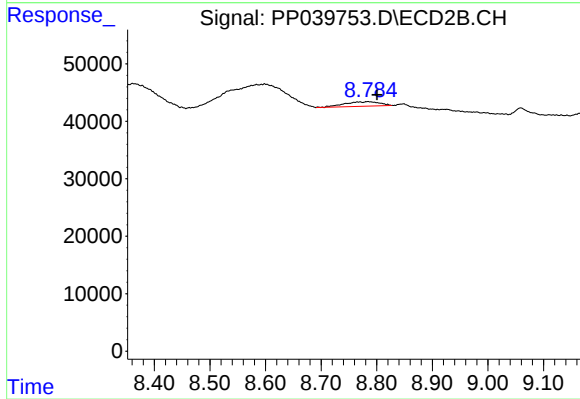

#40 AR-1262-5


R.T.: 8.784 min
Delta R.T.: -0.017 min
Response: 35652
Conc: 39.16 ng/ml

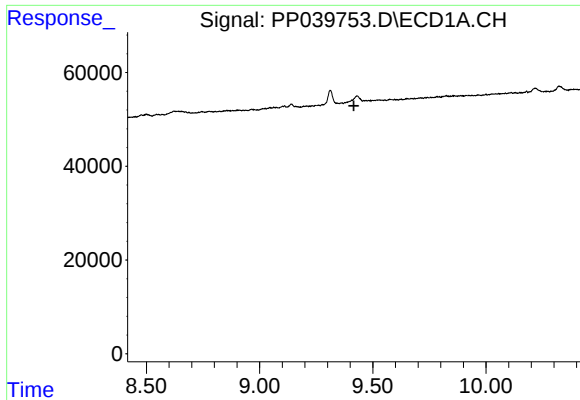

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

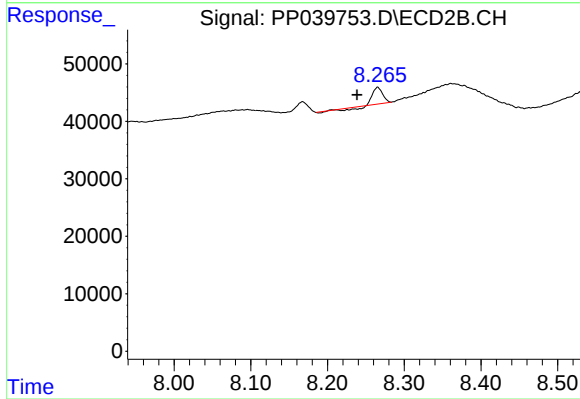


#41 AR-1268-1

R.T.: 8.265 min
Delta R.T.: 0.027 min
Response: 19573
Conc: 6.71 ng/ml

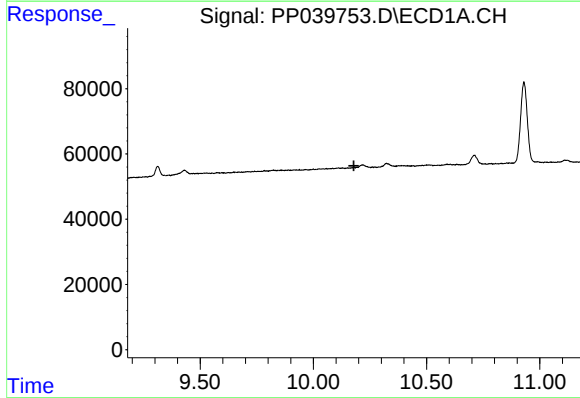

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.179 min
Response: 0
Conc: N.D.

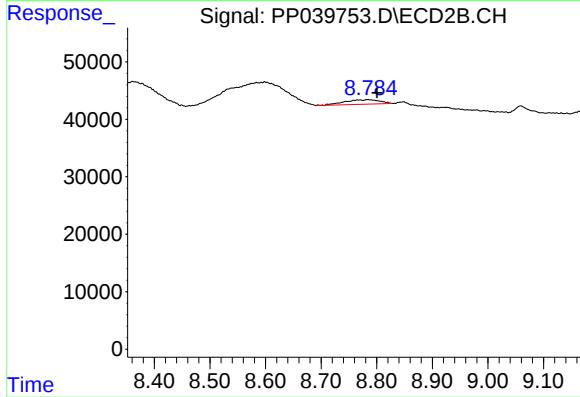

#44 AR-1268-4

R.T.: 8.784 min
Delta R.T.: -0.016 min
Response: 35652
Conc: 34.64 ng/ml