

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
 Data File : PP039764.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 15:12
 Operator : AJ\MA
 Sample : PB139547BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 17:27:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.906	3.996	581836	333003	18.379	20.437
2)	SA Decachlor...	10.930	9.328	462872	422246	21.337	19.323
Target Compounds							
9)	L2 AR-1221-2	5.285f	0.000	19276	0	70.808	N.D. #
10)	L2 AR-1221-3	0.000	4.433	0	12669	N.D.	23.432 #
11)	L3 AR-1232-1	0.000	4.433	0	12669	N.D.	31.329 #
28)	L6 AR-1254-3	7.768f	0.000	86128	0	51.764	N.D. #
32)	L7 AR-1260-2	0.000	7.028f	0	14608	N.D.	11.406 #
36)	L8 AR-1262-1	0.000	7.365f	0	239495	N.D.	339.716 #
40)	L8 AR-1262-5	0.000	8.807	0	60669	N.D.	66.636 #
44)	L9 AR-1268-4	0.000	8.807	0	60669	N.D.	58.942 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
Data File : PP039764.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 15:12
Operator : AJ\MA
Sample : PB139547BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 17:27:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

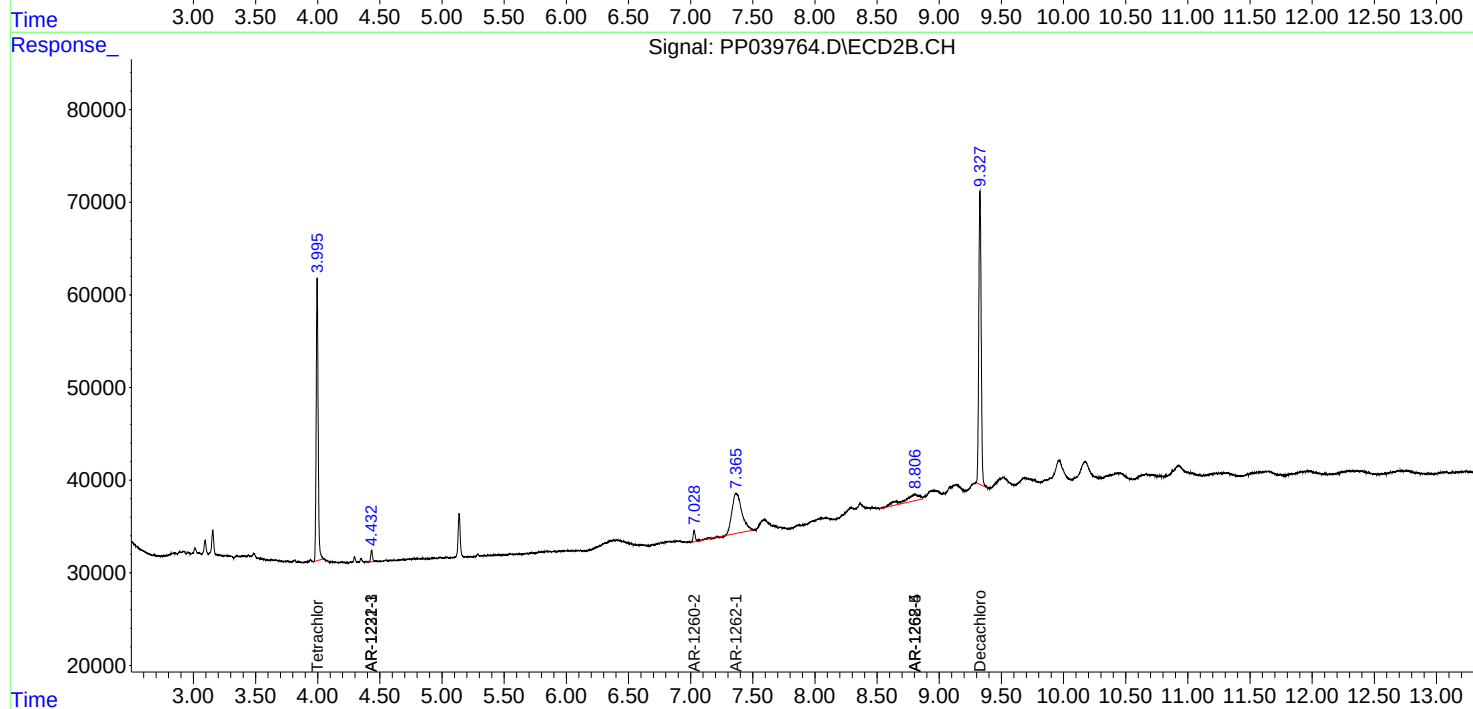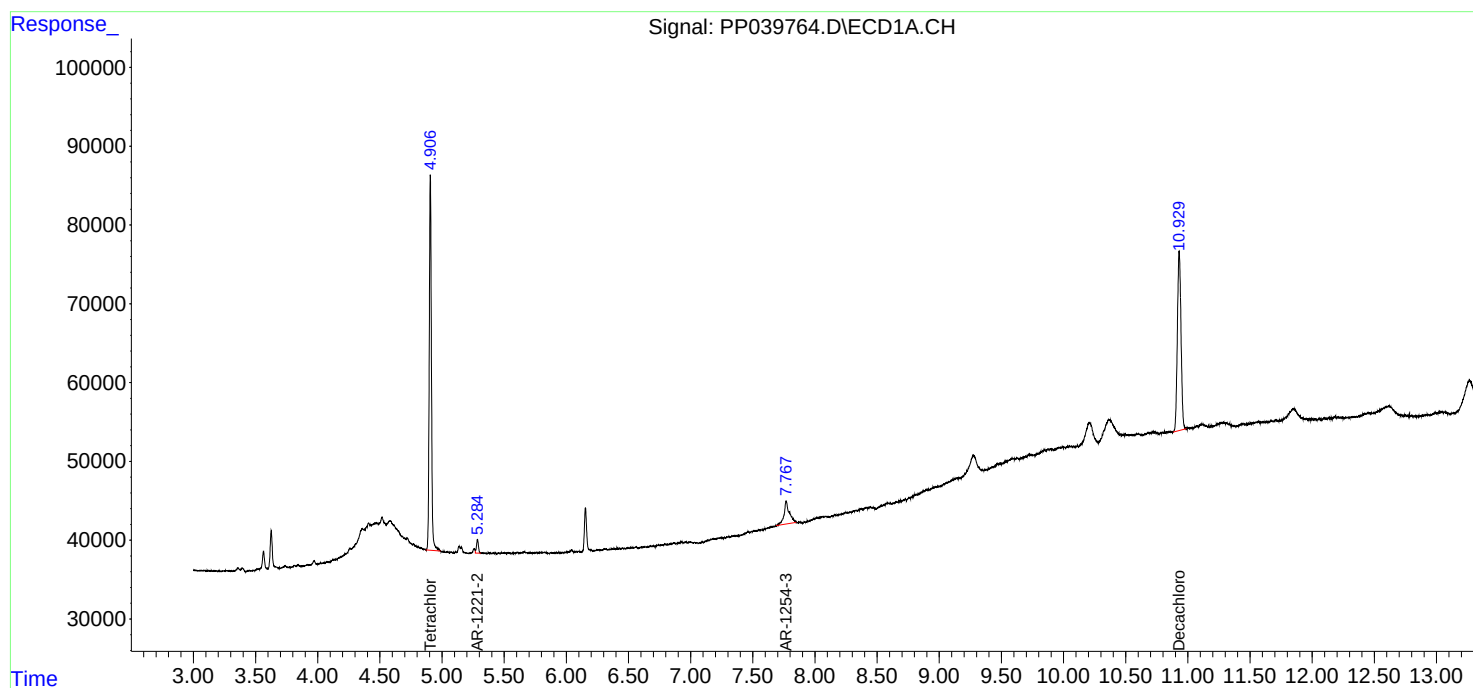


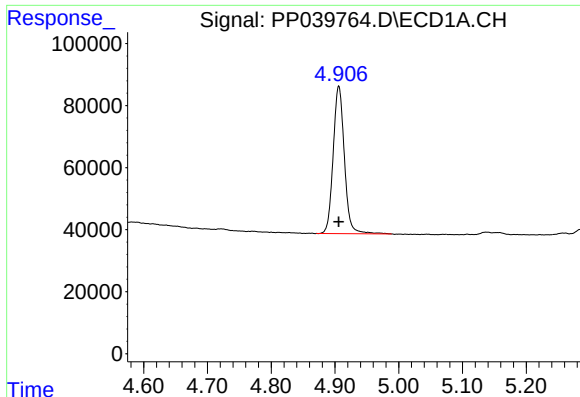

#1 Tetrachloro-m-xylene


R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 581836
Conc: 18.38 ng/ml

Instrument :
ECD_P
ClientSampleId :

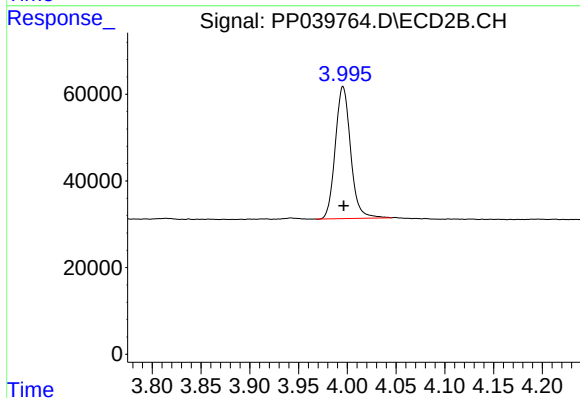


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 333003
Conc: 20.44 ng/ml

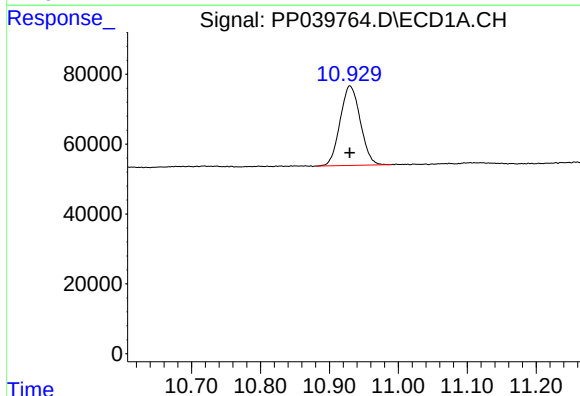


#2 Decachlorobiphenyl

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 462872
Conc: 21.34 ng/ml

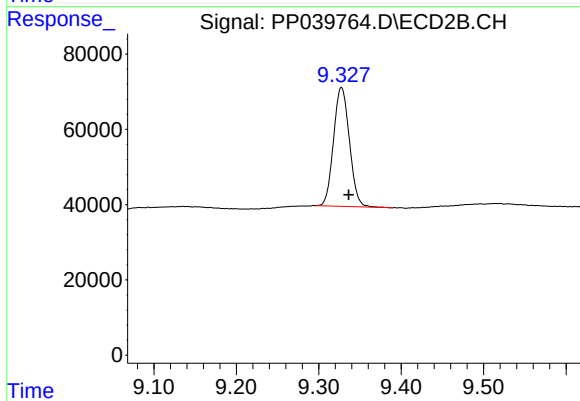

#2 Decachlorobiphenyl


R.T.: 9.328 min
Delta R.T.: -0.009 min
Response: 422246
Conc: 19.32 ng/ml

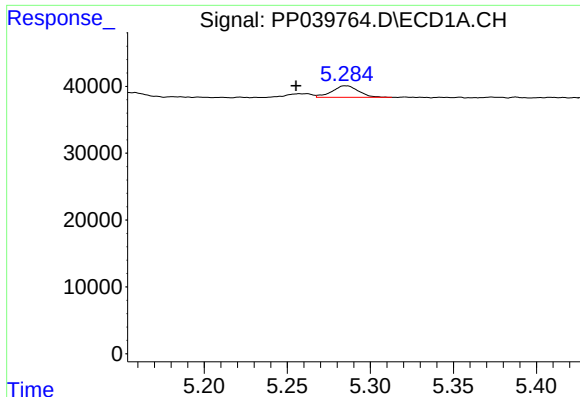

#9 AR-1221-2


R.T.: 5.285 min
Delta R.T.: 0.030 min
Response: 19276
Conc: 70.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

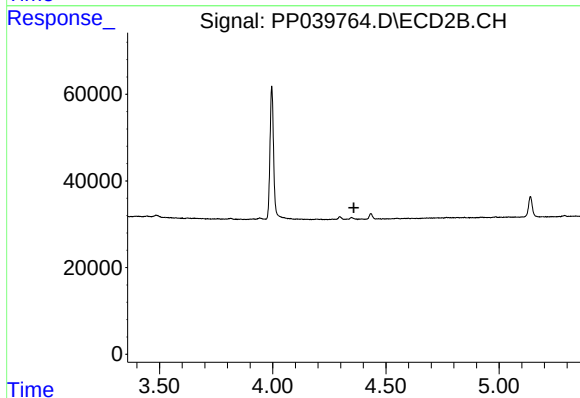


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.358 min
Response: 0
Conc: N.D.

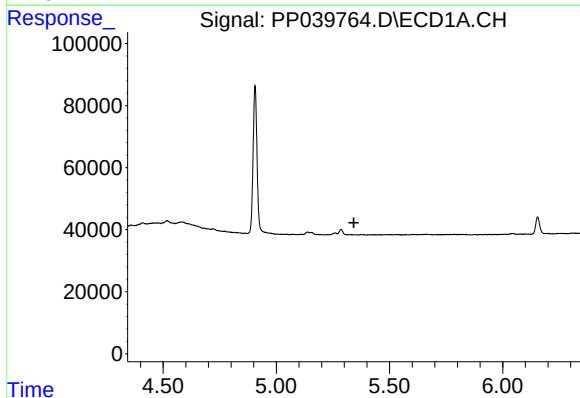


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.343 min
Response: 0
Conc: N.D.

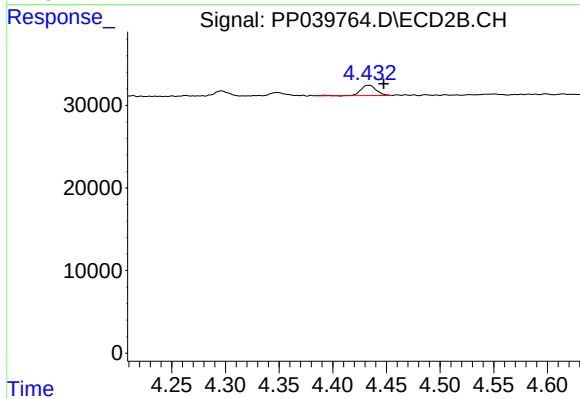

#10 AR-1221-3


R.T.: 4.433 min
Delta R.T.: -0.015 min
Response: 12669
Conc: 23.43 ng/ml

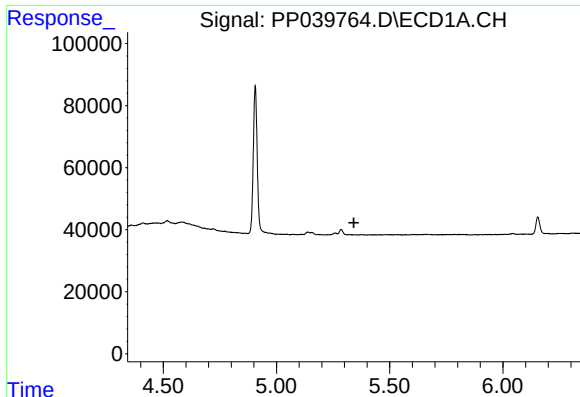

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

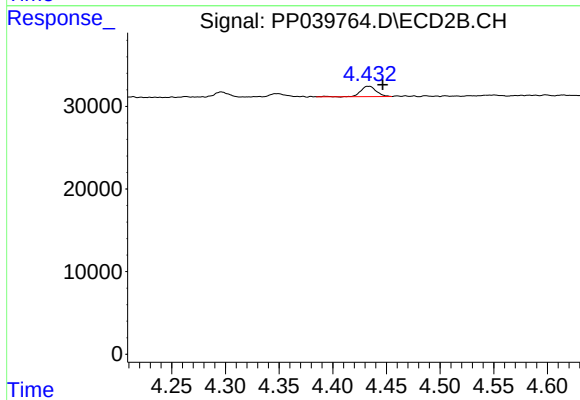


#11 AR-1232-1

R.T.: 4.433 min
Delta R.T.: -0.014 min
Response: 12669
Conc: 31.33 ng/ml

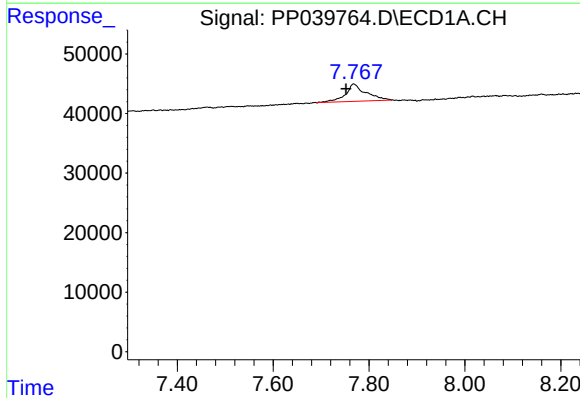


#28 AR-1254-3

R.T.: 7.768 min
Delta R.T.: 0.015 min
Response: 86128
Conc: 51.76 ng/ml

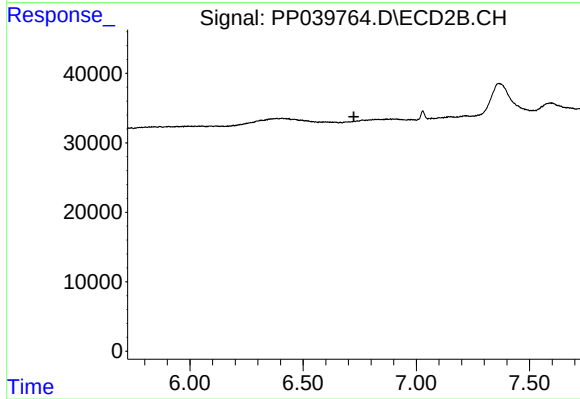

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.724 min
Response: 0
Conc: N.D.

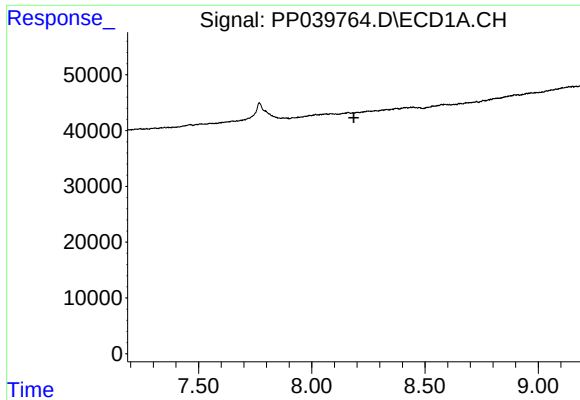

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

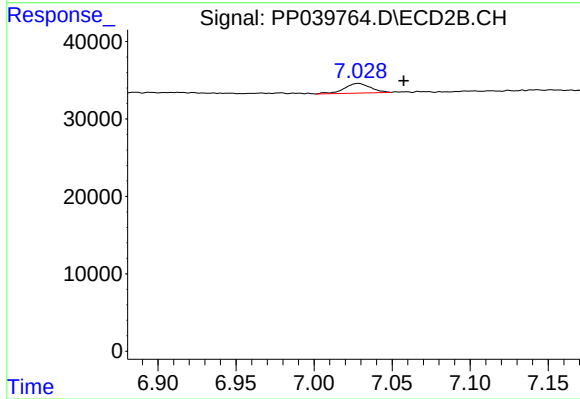


#32 AR-1260-2

R.T.: 7.028 min
Delta R.T.: -0.029 min
Response: 14608
Conc: 11.41 ng/ml

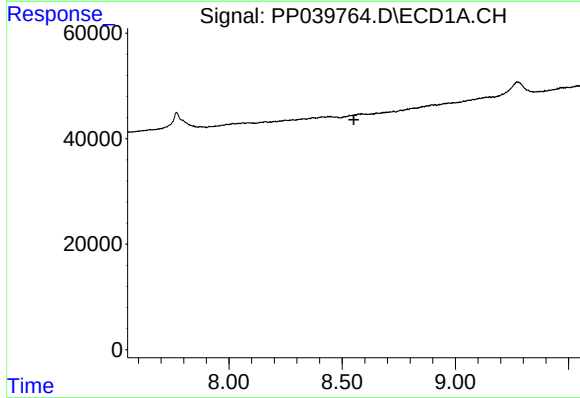


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.552 min
Response: 0
Conc: N.D.

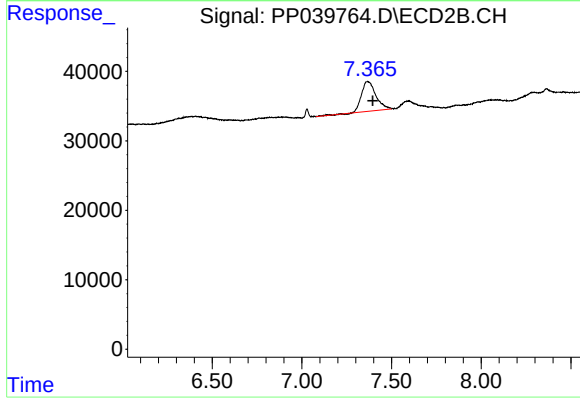

#36 AR-1262-1


R.T.: 7.365 min
Delta R.T.: -0.029 min
Response: 239495
Conc: 339.72 ng/ml

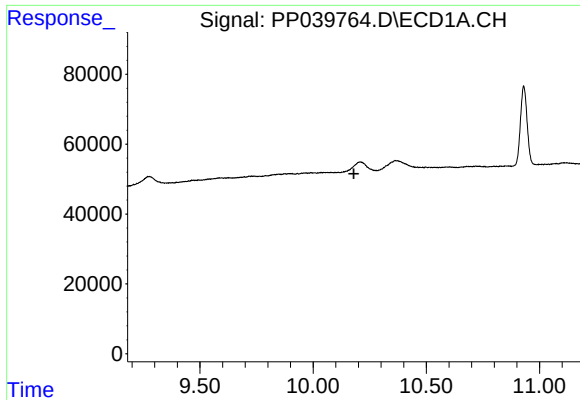

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.180 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

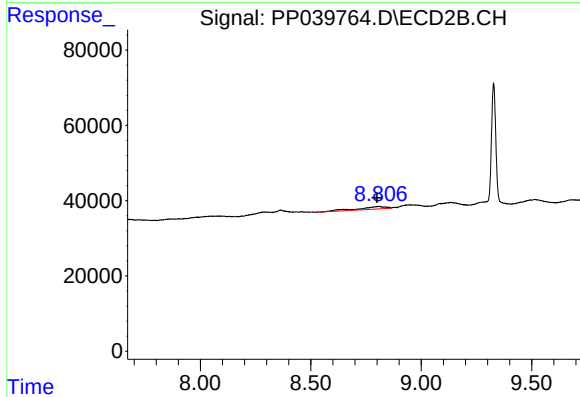


#40 AR-1262-5

R.T.: 8.807 min
Delta R.T.: 0.006 min
Response: 60669
Conc: 66.64 ng/ml

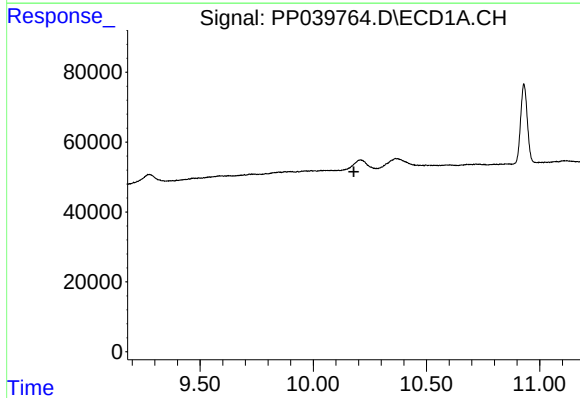

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.179 min
Response: 0
Conc: N.D.

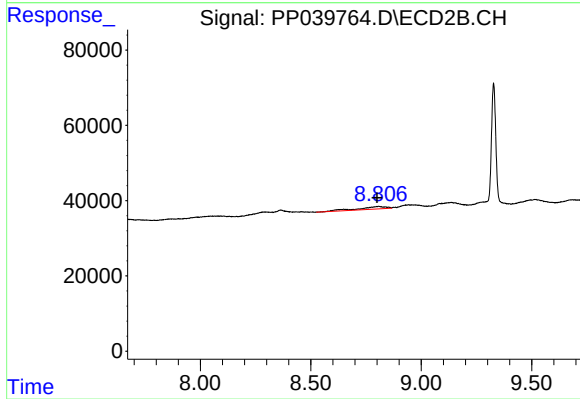

#44 AR-1268-4

R.T.: 8.807 min
Delta R.T.: 0.007 min
Response: 60669
Conc: 58.94 ng/ml