

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
 Data File : PP039766.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 15:46
 Operator : AJ\MA
 Sample : M4033-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 00:59:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.907	3.996	95385	53001	3.013	3.253
2)	SA Decachlor...	10.931	9.329	71330	76992	3.288	3.523
Target Compounds							
5)	L1 AR-1016-3	6.308	0.000	24748	0	25.274	N.D. #
10)	L2 AR-1221-3	0.000	4.434	0	14986	N.D.	27.717 #
11)	L3 AR-1232-1	0.000	4.434	0	14986	N.D.	37.058 #
14)	L3 AR-1232-4	0.000	5.600f	0	8860	N.D.	37.749 #
18)	L4 AR-1242-3	6.308	0.000	24748	0	33.765	N.D. #
19)	L4 AR-1242-4	0.000	5.600f	0	8860	N.D.	20.973 #
23)	L5 AR-1248-3	0.000	5.600f	0	8860	N.D.	14.622 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
Data File : PP039766.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 15:46
Operator : AJ\MA
Sample : M4033-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 00:59:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

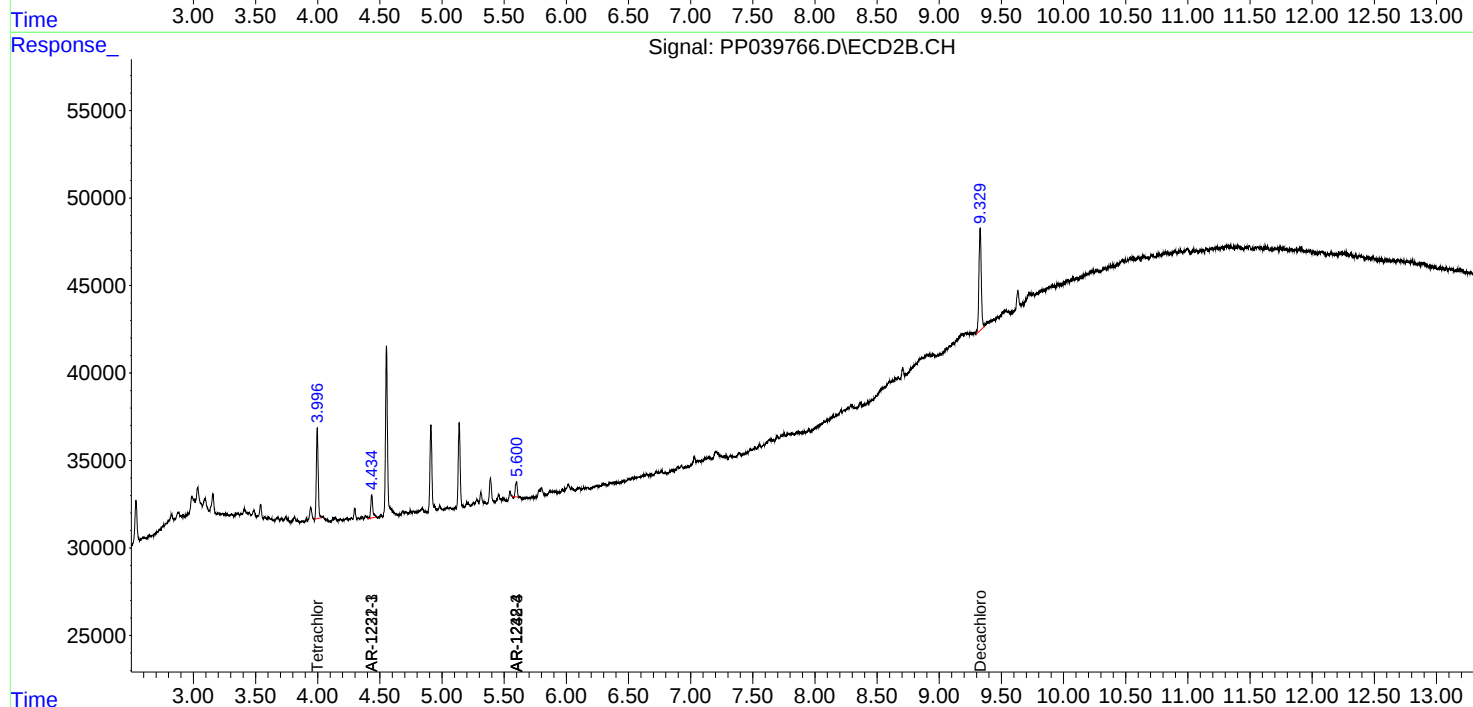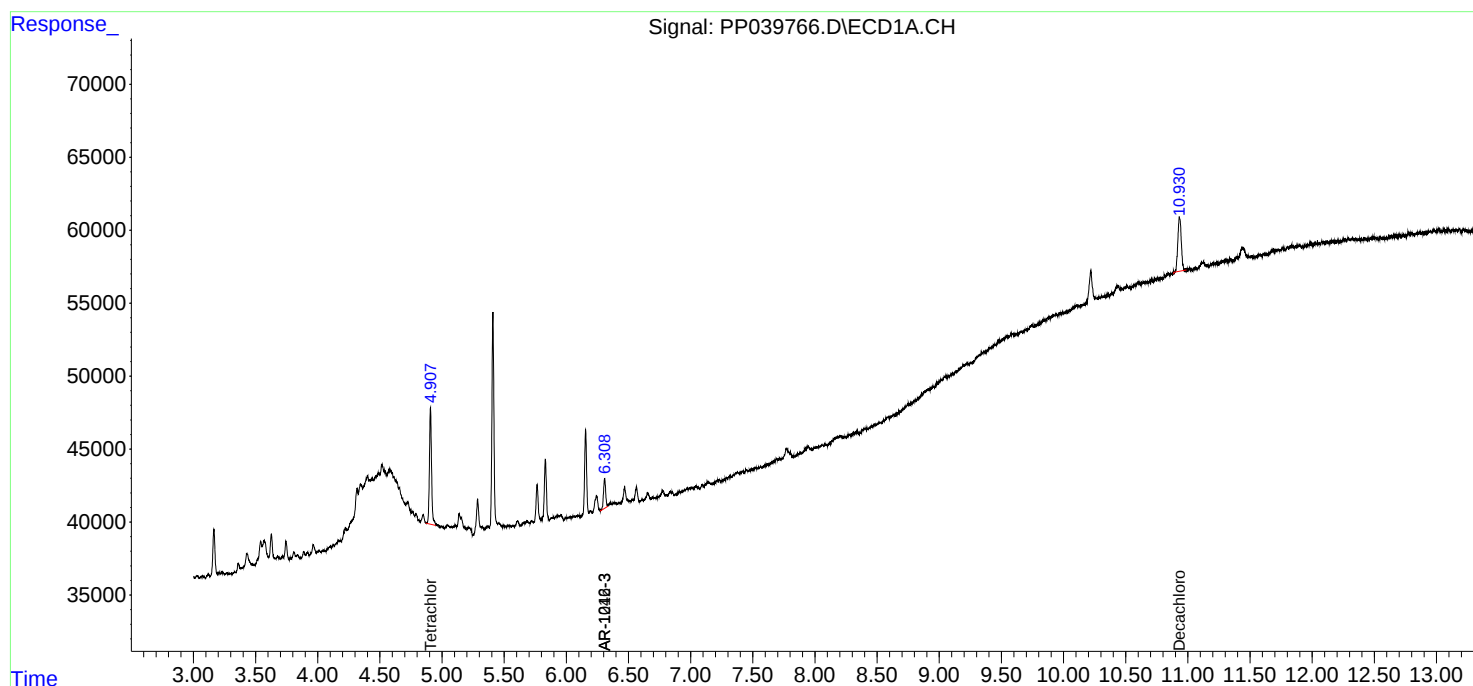


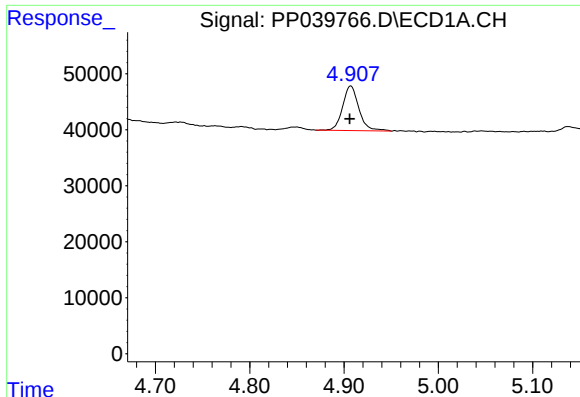

#1 Tetrachloro-m-xylene


R.T.: 4.907 min
Delta R.T.: 0.001 min
Response: 95385
Conc: 3.01 ng/ml

Instrument :
ECD_P
ClientSampleId :

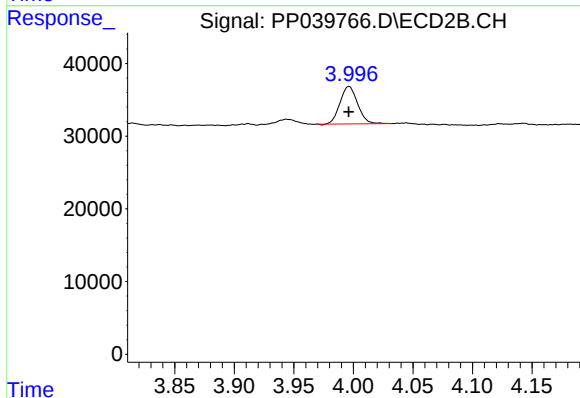


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 53001
Conc: 3.25 ng/ml

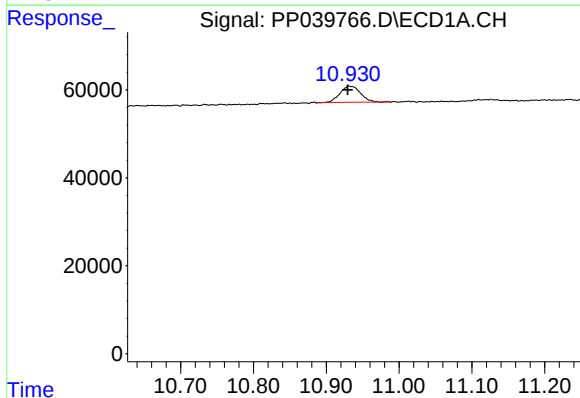


#2 Decachlorobiphenyl

R.T.: 10.931 min
Delta R.T.: 0.002 min
Response: 71330
Conc: 3.29 ng/ml

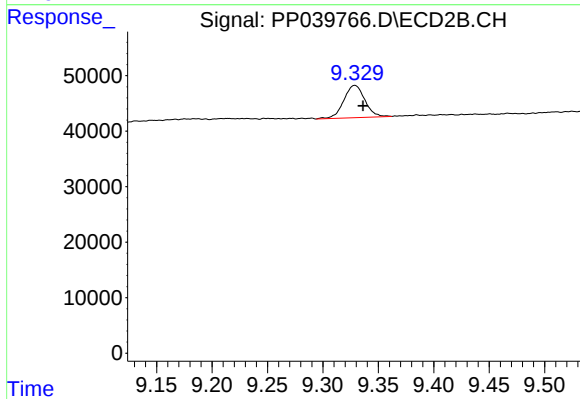

#2 Decachlorobiphenyl


R.T.: 9.329 min
Delta R.T.: -0.007 min
Response: 76992
Conc: 3.52 ng/ml

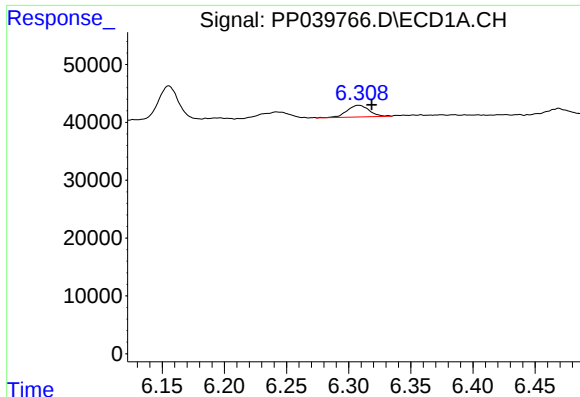

#5 AR-1016-3


R.T.: 6.308 min
Delta R.T.: -0.010 min
Response: 24748
Conc: 25.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

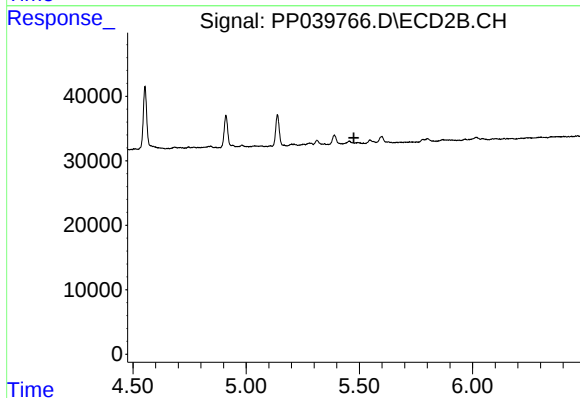


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

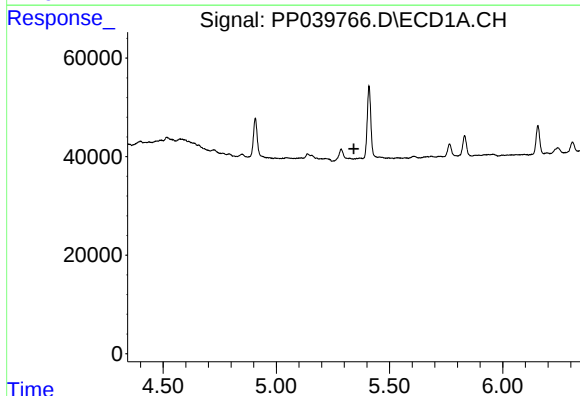


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.343 min
Response: 0
Conc: N.D.

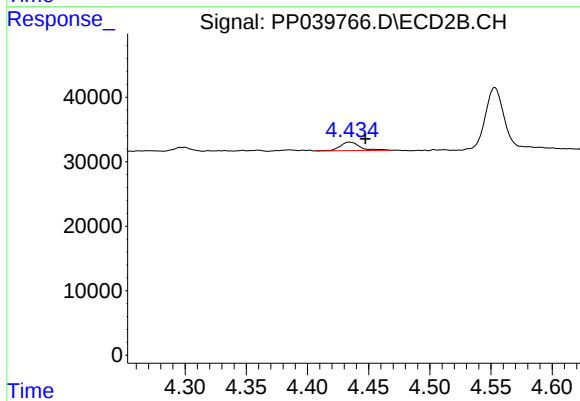

#10 AR-1221-3


R.T.: 4.434 min
Delta R.T.: -0.013 min
Response: 14986
Conc: 27.72 ng/ml

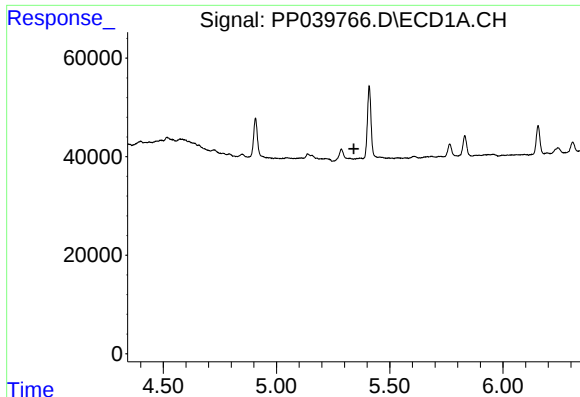

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

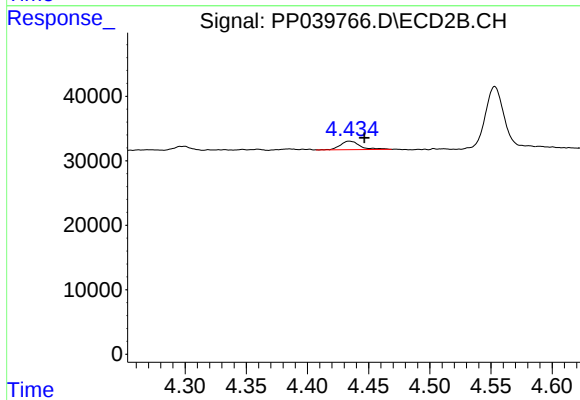


#11 AR-1232-1

R.T.: 4.434 min
Delta R.T.: -0.012 min
Response: 14986
Conc: 37.06 ng/ml

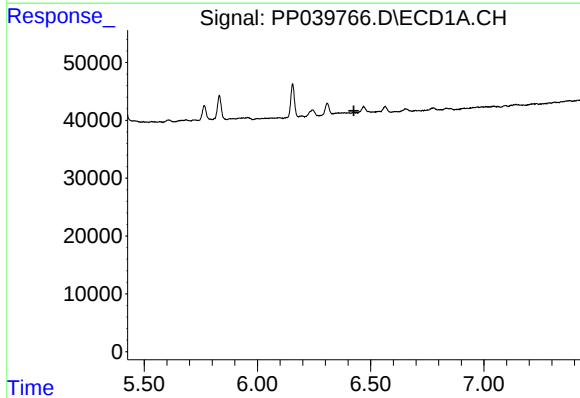


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 6.426 min
Response: 0
Conc: N.D.

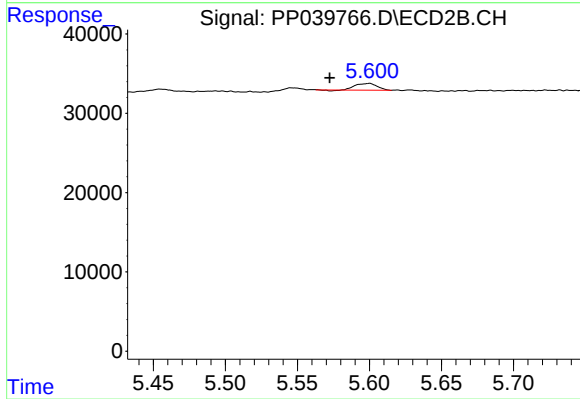

#14 AR-1232-4


R.T.: 5.600 min
Delta R.T.: 0.028 min
Response: 8860
Conc: 37.75 ng/ml

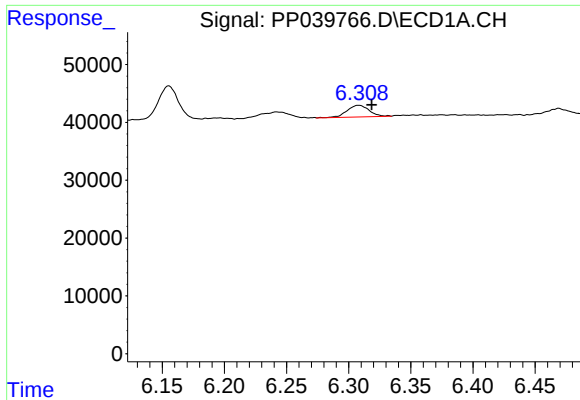

#18 AR-1242-3


R.T.: 6.308 min
Delta R.T.: -0.010 min
Response: 24748
Conc: 33.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

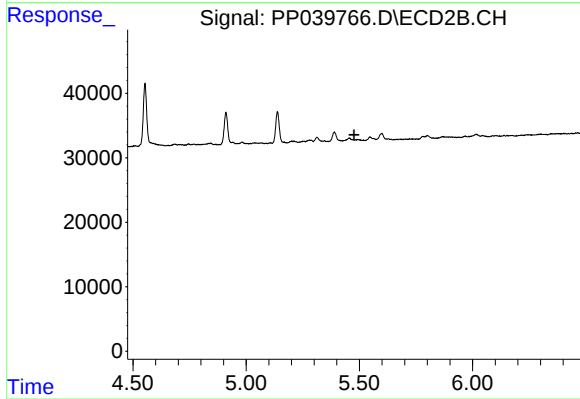


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

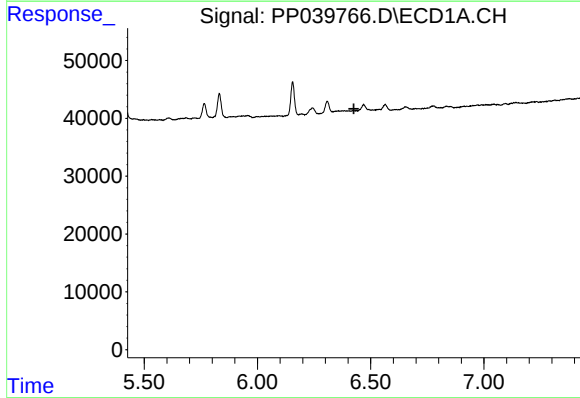


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 6.426 min
Response: 0
Conc: N.D.

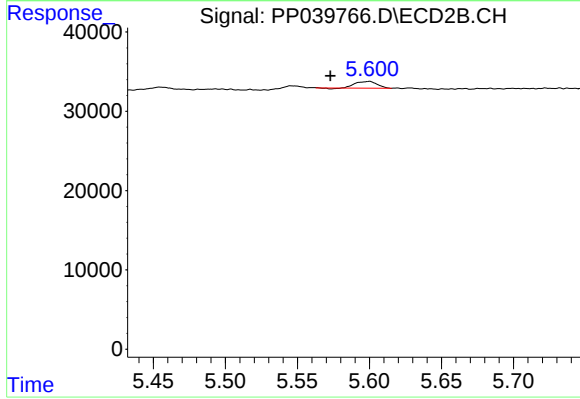

#19 AR-1242-4


R.T.: 5.600 min
Delta R.T.: 0.027 min
Response: 8860
Conc: 20.97 ng/ml

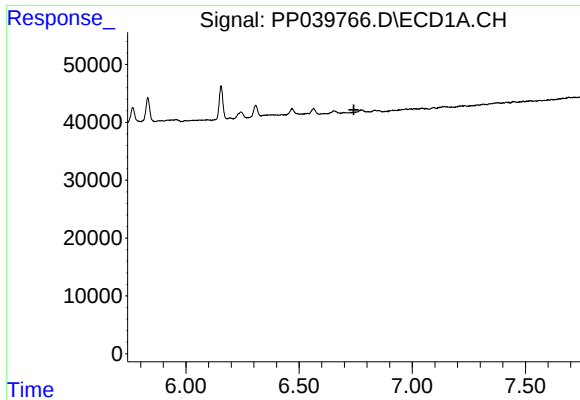

#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.742 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

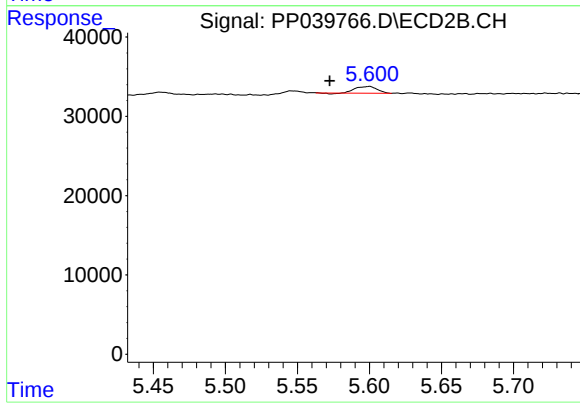

#23 AR-1248-3

R.T.: 5.600 min
Delta R.T.: 0.028 min
Response: 8860
Conc: 14.62 ng/ml