

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
 Data File : PP039802.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2021 2:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 05:29:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.904	3.993	644799	369984	20.368	22.706
2)	SA Decachlor...	10.926	9.324	515142	520542	23.746	23.821
Target Compounds							
28)	L6 AR-1254-3	7.765	0.000	12412	0	7.459	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100421\
Data File : PP039802.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2021 2:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 05:29:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

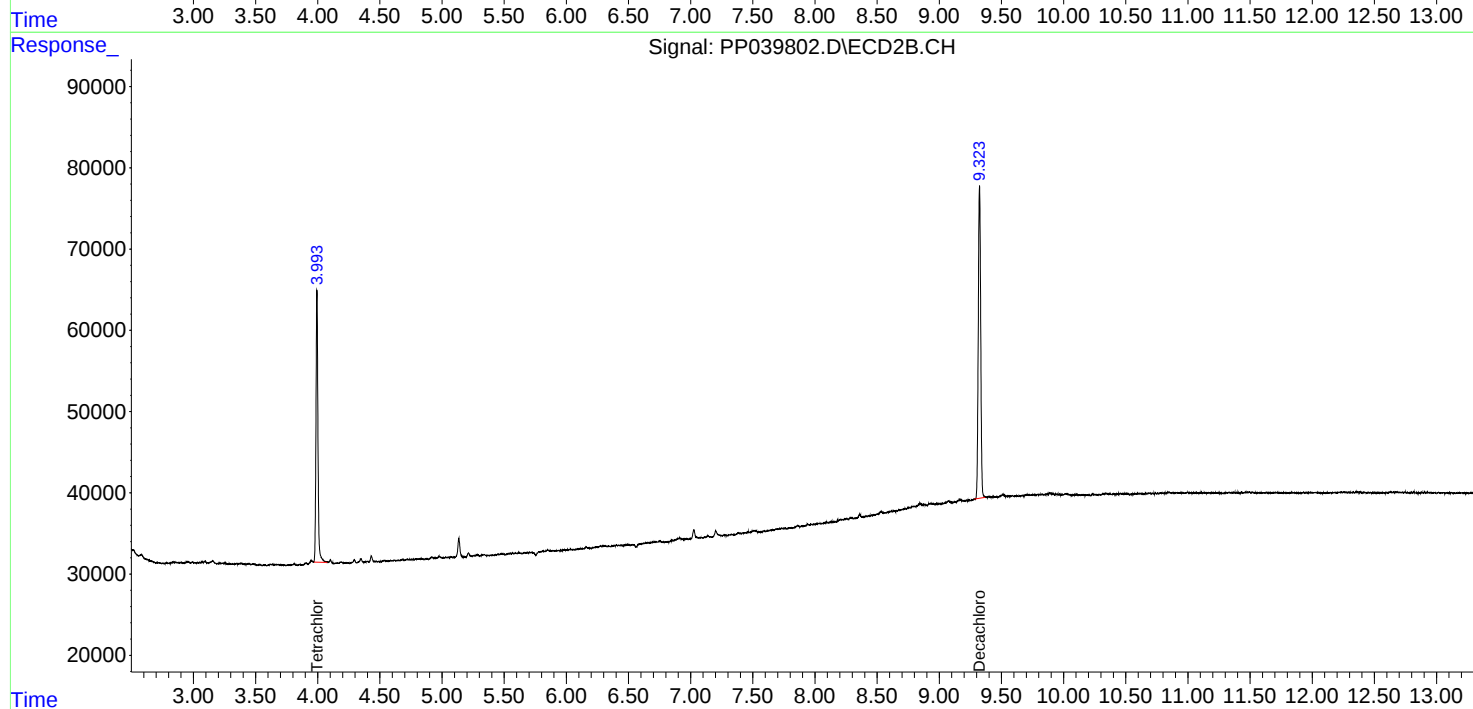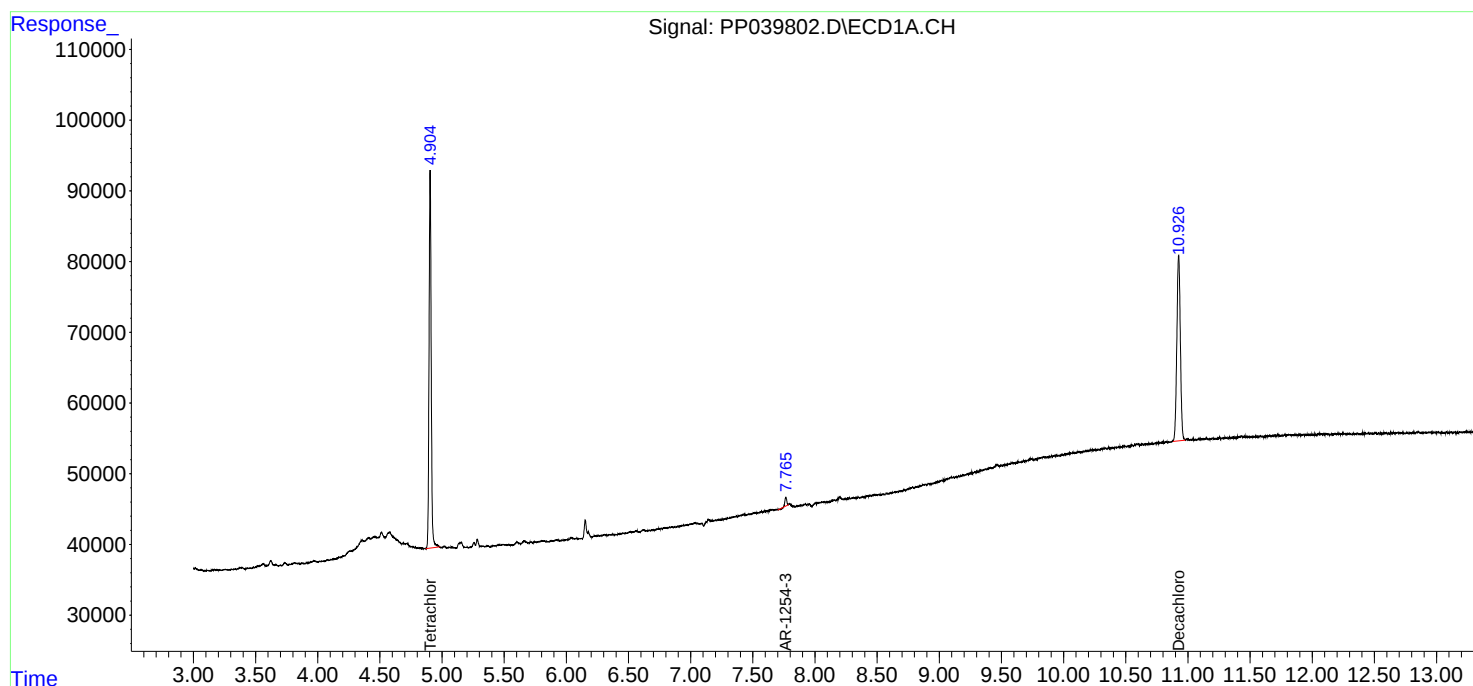


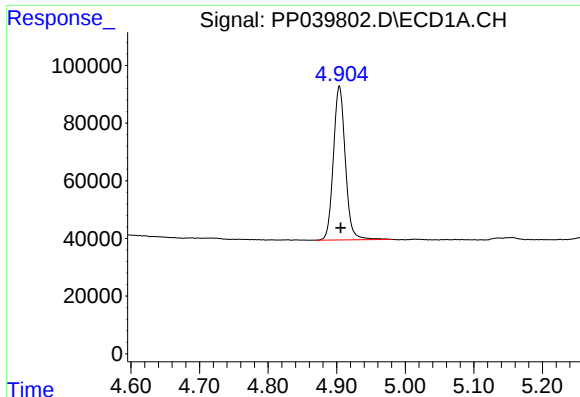

#1 Tetrachloro-m-xylene


R.T.: 4.904 min
Delta R.T.: -0.002 min
Response: 644799
Conc: 20.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

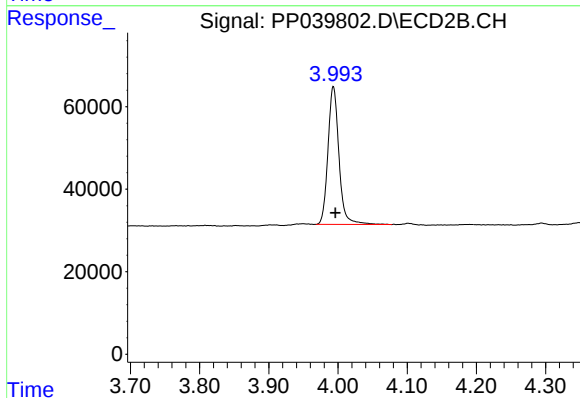


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: -0.003 min
Response: 369984
Conc: 22.71 ng/ml

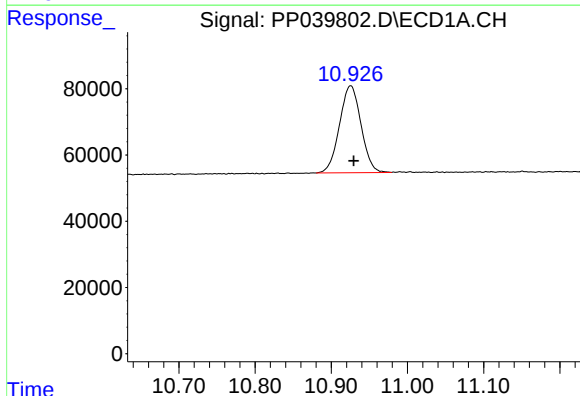


#2 Decachlorobiphenyl

R.T.: 10.926 min
Delta R.T.: -0.004 min
Response: 515142
Conc: 23.75 ng/ml

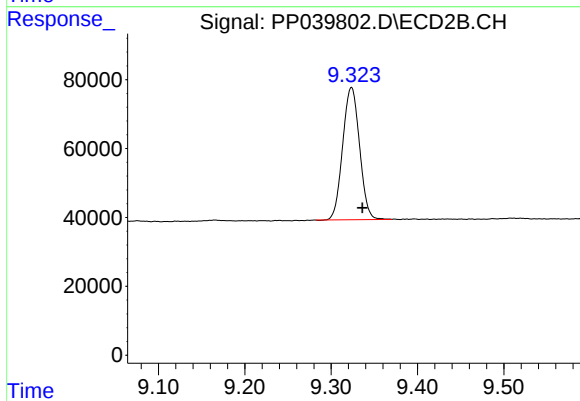

#2 Decachlorobiphenyl


R.T.: 9.324 min
Delta R.T.: -0.012 min
Response: 520542
Conc: 23.82 ng/ml

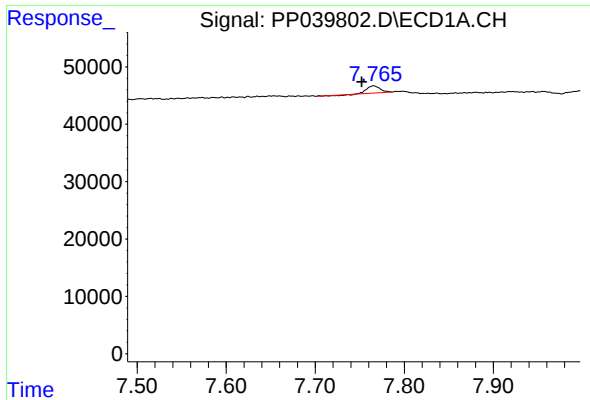

#28 AR-1254-3

R.T.: 7.765 min
Delta R.T.: 0.013 min
Response: 12412
Conc: 7.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

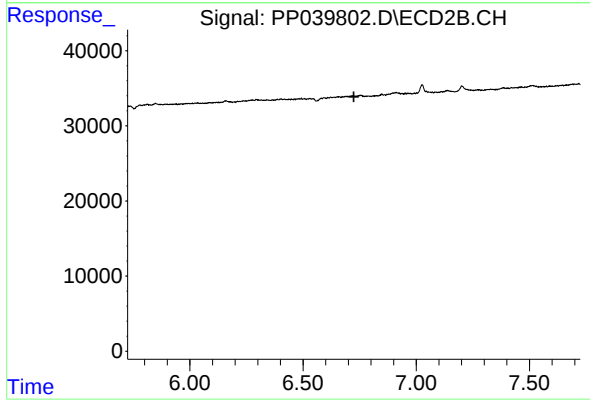

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.