

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100422\
 Data File : PP051901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 13:51
 Operator : YP\AJ
 Sample : N4936-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SASP2-T-2-(10-16)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/05/2022
 Supervised By :Ankita Jodhani 10/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 21:43:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 12:08:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.674	36034519	28807960	20.162	22.659
2) SA Decachlor...	10.243	8.772	26778472	21072807	22.089	17.841m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100422\
Data File : PP051901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 13:51
Operator : YP\AJ
Sample : N4936-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SASP2-T-2-(10-16)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2022
Supervised By :Ankita Jodhani 10/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 21:43:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 04 12:08:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

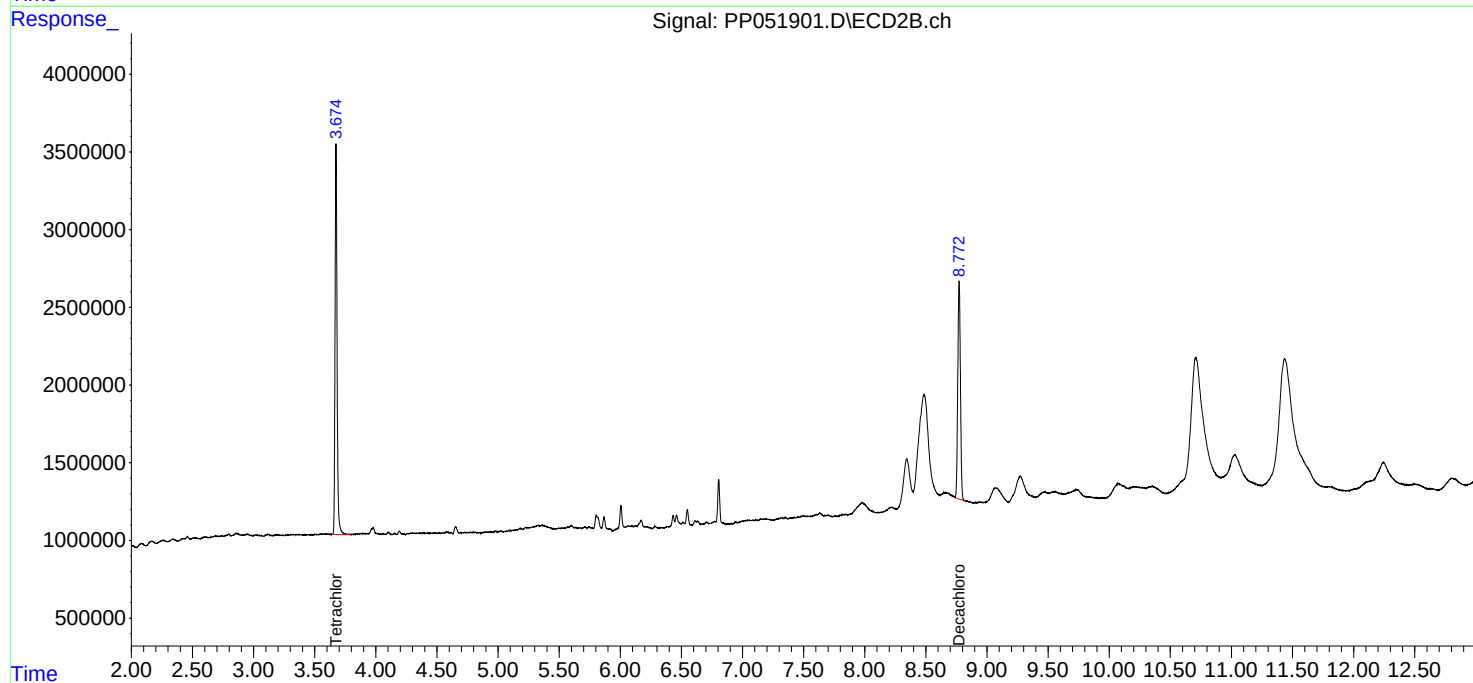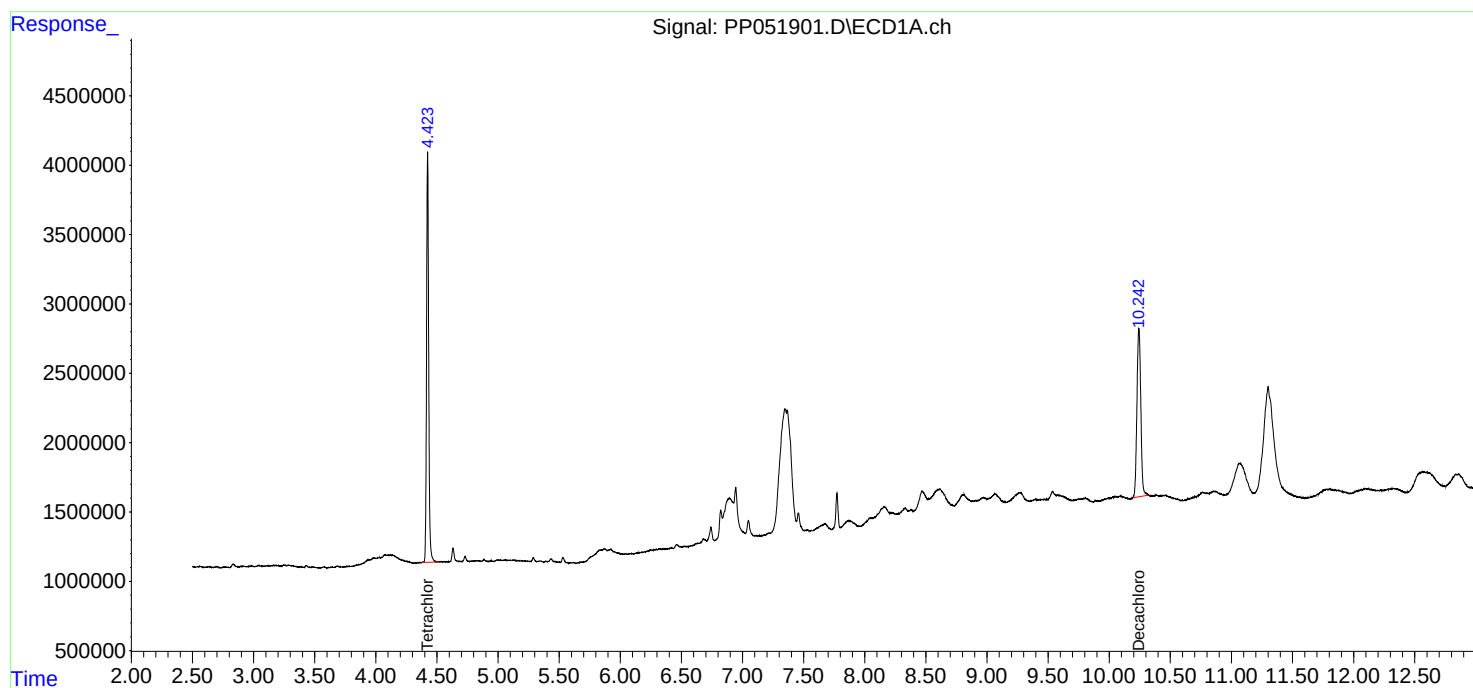

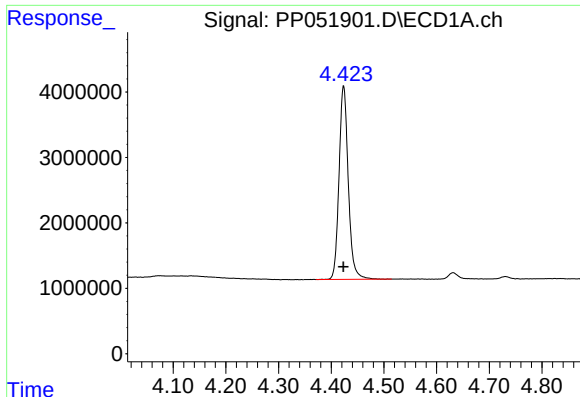


#1 Tetrachloro-m-xylene

R.T.: 4.423 min
Delta R.T.: 0.000 min
Response: 36034519
Conc: 20.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
SASP2-T-2-(10-16)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/05/2022
Supervised By :Ankita Jodhani 10/05/2022

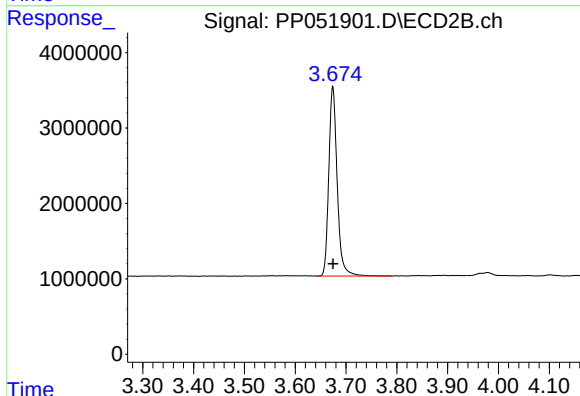


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: 0.000 min
Response: 28807960
Conc: 22.66 ng/ml

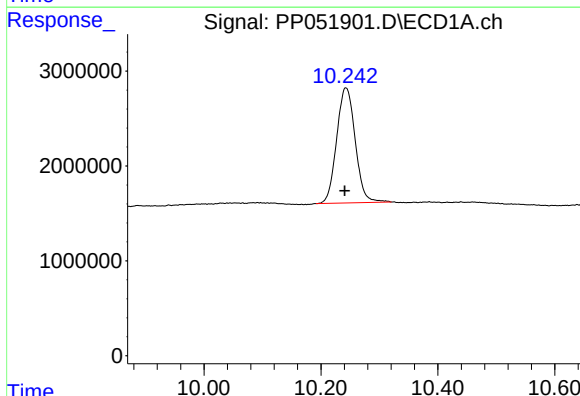

#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: 0.002 min
Response: 26778472
Conc: 22.09 ng/ml

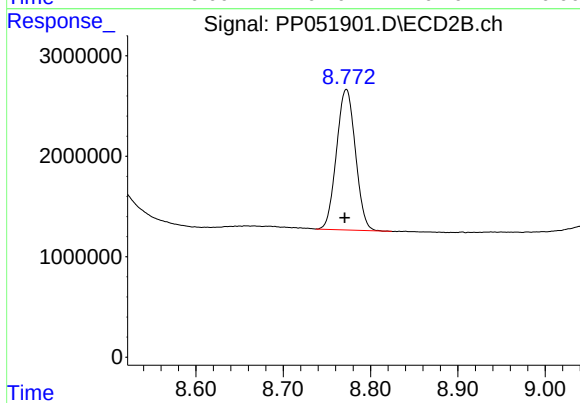

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: 0.002 min
Response: 21072807
Conc: 17.84 ng/ml m