

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100424\
 Data File : PP067516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2024 15:07
 Operator : YP\AJ
 Sample : P4288-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HR-03-100324

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/07/2024
 Supervised By :Ankita Jodhani 10/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 23:00:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 27 06:59:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.752	4.052	19021175	20496693	14.152	13.718
2) SA Decachlor...	10.660	9.216	20622975	18374381	14.206	13.334m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100424\
Data File : PP067516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2024 15:07
Operator : YP\AJ
Sample : P4288-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HR-03-100324


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/07/2024
Supervised By :Ankita Jodhani 10/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 23:00:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092624.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 27 06:59:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

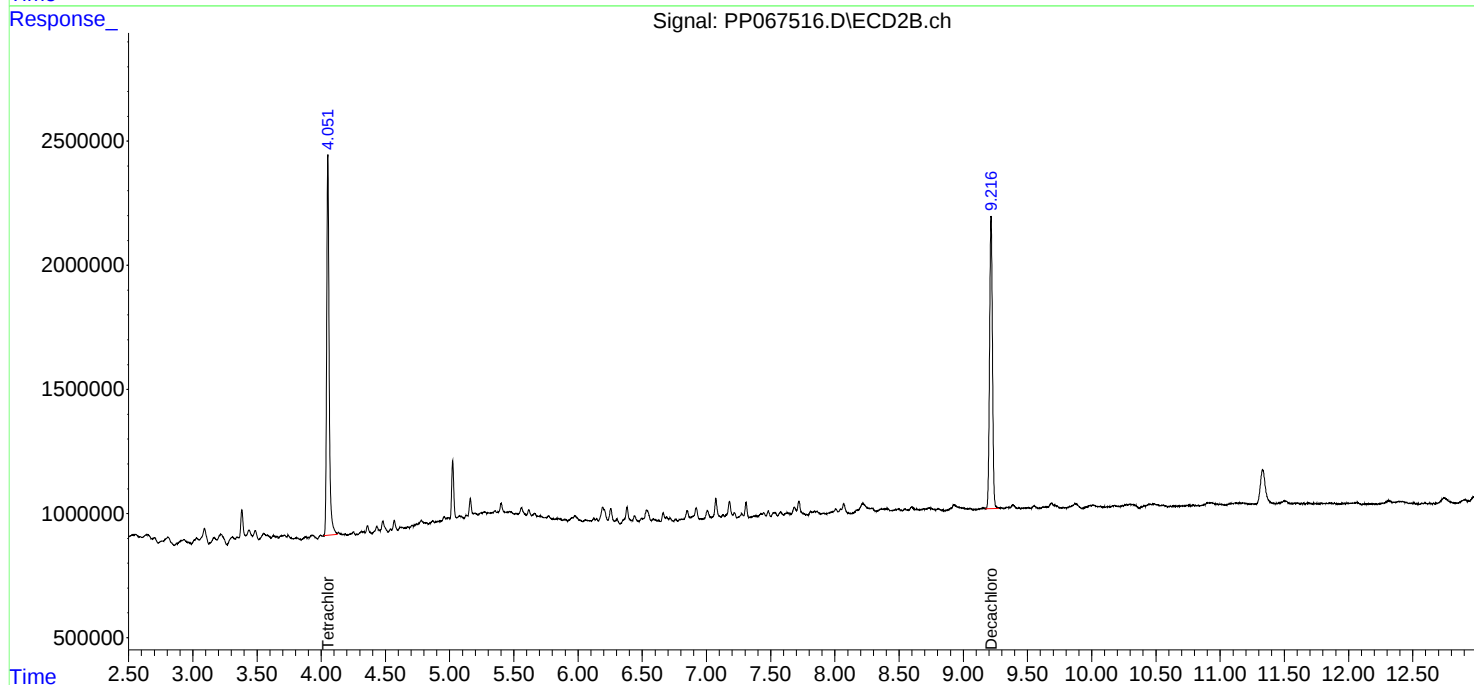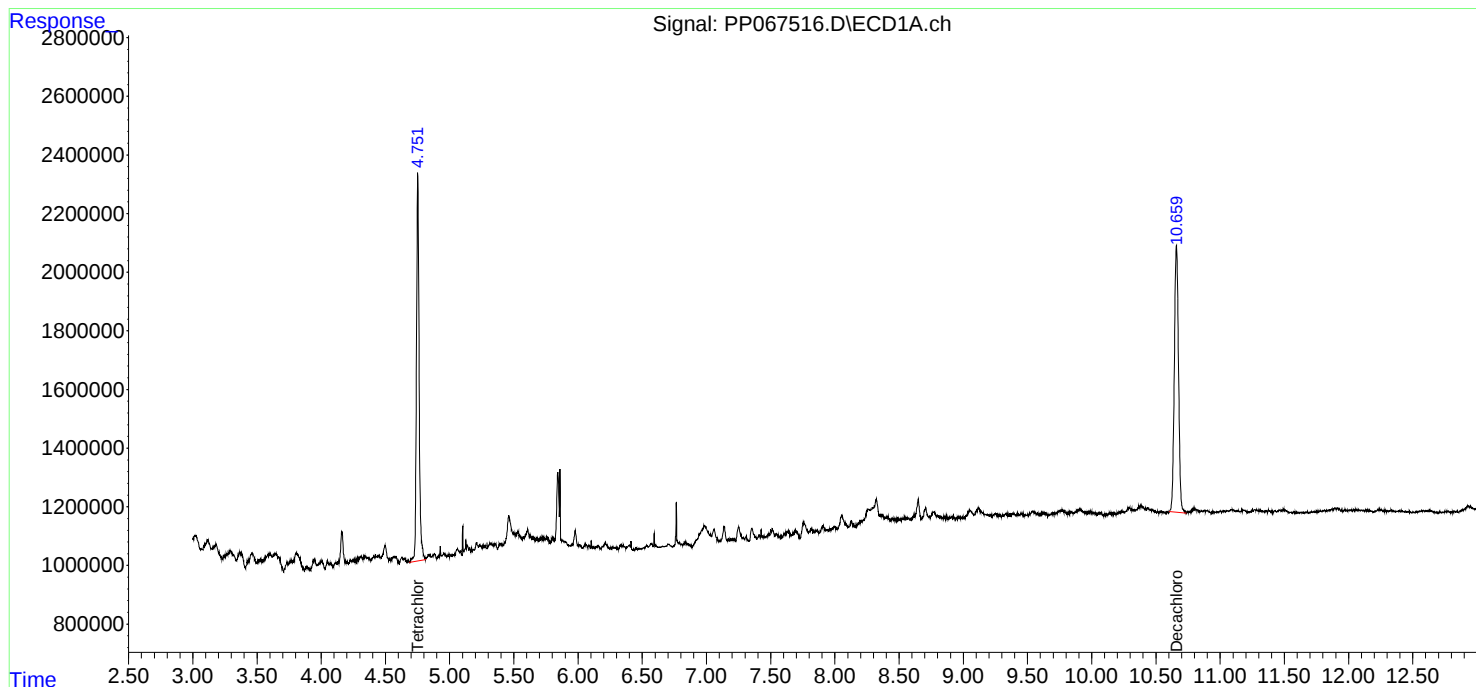

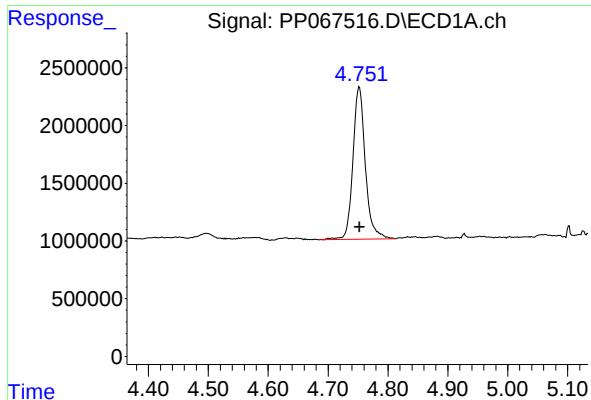


#1 Tetrachloro-m-xylene

R.T.: 4.752 min
Delta R.T.: 0.000 min
Response: 19021175
Conc: 14.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
HR-03-100324


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/07/2024
Supervised By :Ankita Jodhani 10/07/2024

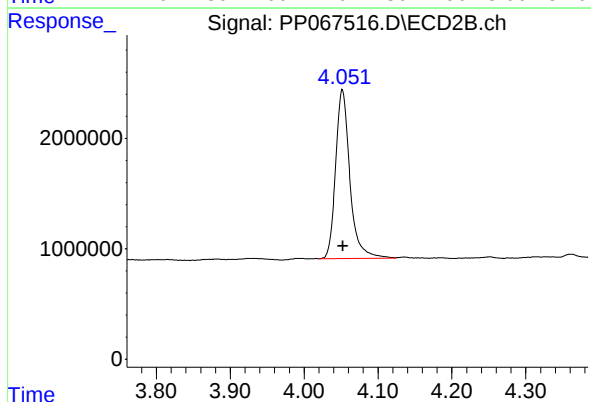


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: -0.001 min
Response: 20496693
Conc: 13.72 ng/ml

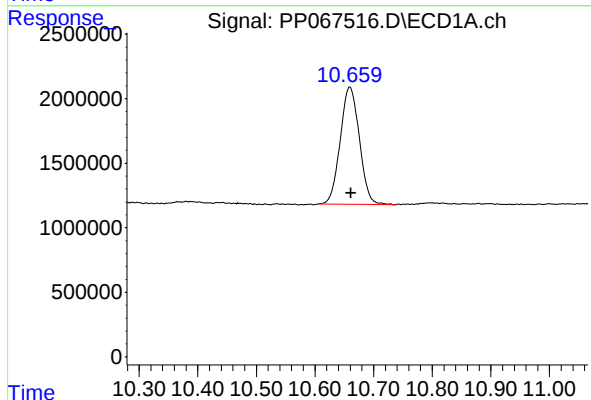

#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.002 min
Response: 20622975
Conc: 14.21 ng/ml

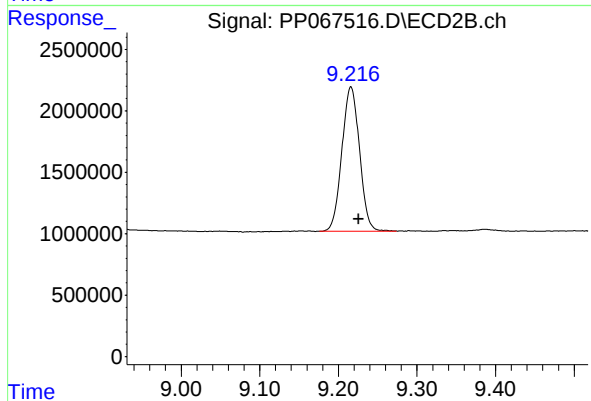

#2 Decachlorobiphenyl

R.T.: 9.216 min
Delta R.T.: -0.011 min
Response: 18374381
Conc: 13.33 ng/ml m