

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100523\
 Data File : PP060619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 14:29
 Operator : YP\AJ
 Sample : 04729-18
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K242-34A

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 18:41:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

10/06/2023
 Supervised By :Ankita
 Jodhani

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	10/06/2023
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	4.531	3.684	33517282	23874873	14.966	16.039
2) SA Decachlor...	10.456	8.747	19388580	15381418	10.982	9.430

Target Compounds

26) L6 AR-1254-1	6.579	5.594	10878444	6209405	127.471	62.773 #
27) L6 AR-1254-2	6.810	5.740	7921792	1985097	62.070	23.098 #
28) L6 AR-1254-3	7.178	6.146	9488070	9420920	71.384	65.730
29) L6 AR-1254-4	7.464	6.375	5888966	3532154	59.884	40.524 #
30) L6 AR-1254-5	7.894	6.795	10303863	24565155	95.104m	193.854 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100523\
Data File : PP060619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 14:29
Operator : YP\AJ
Sample : 04729-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
K242-34A



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 18:41:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

10/06/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

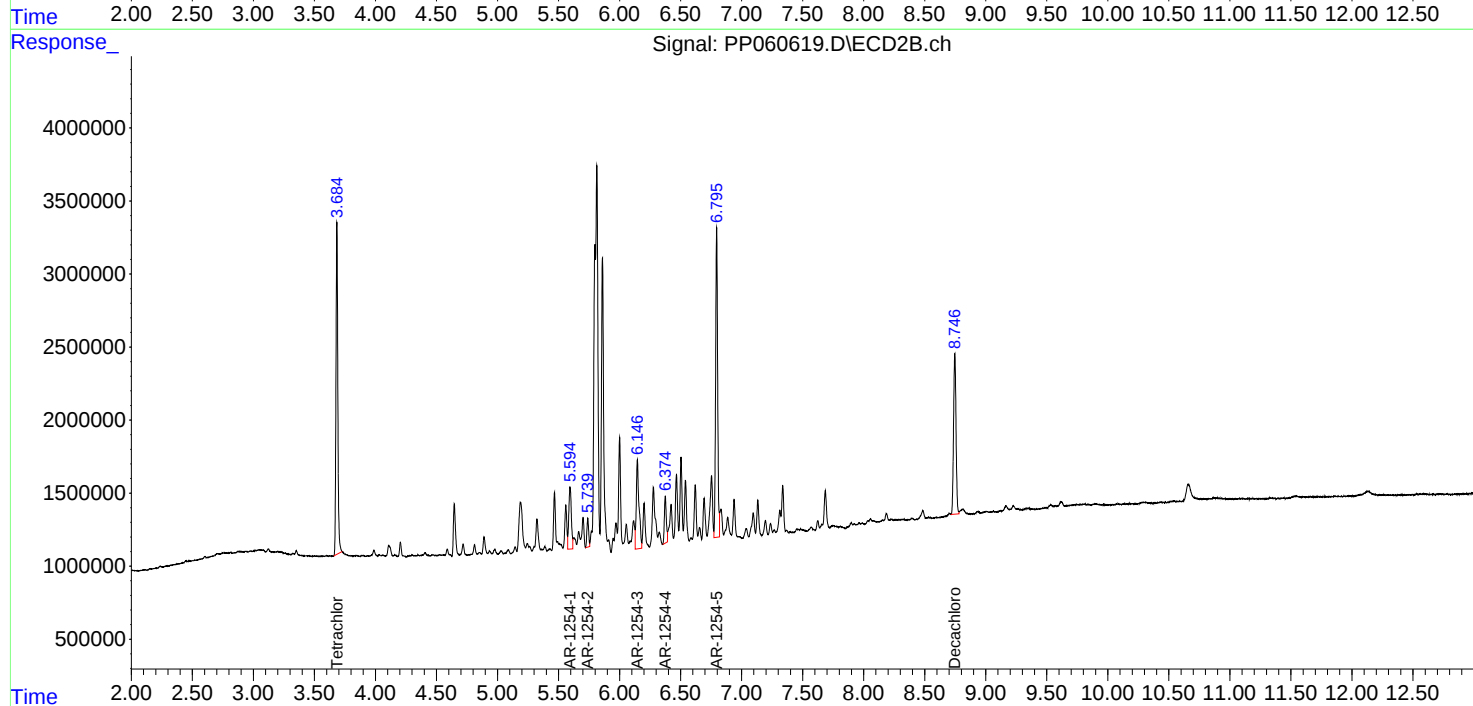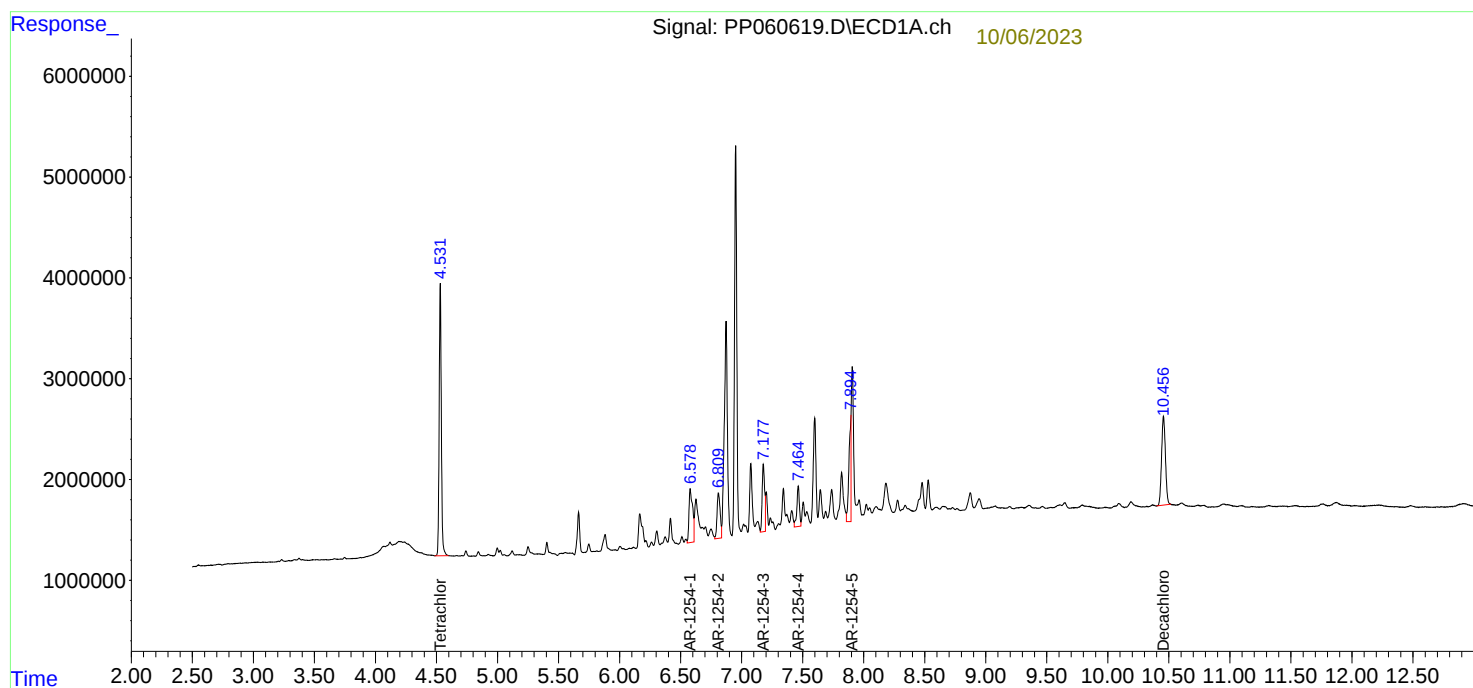

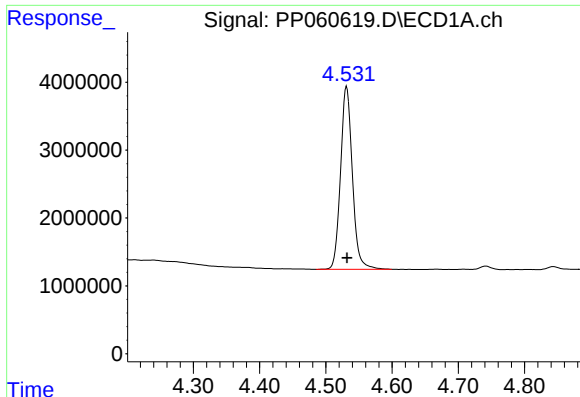


#1 Tetrachloro-m-xylene

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 33517282
Conc: 14.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-34A

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

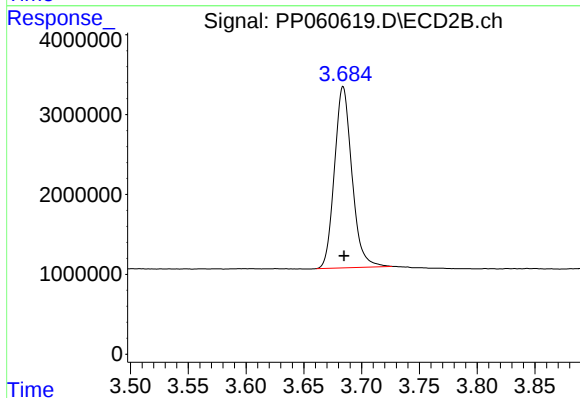


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.000 min
Response: 23874873
Conc: 16.04 ng/ml


10/06/2023
Supervised By :Ankita
Jodhani

10/06/2023

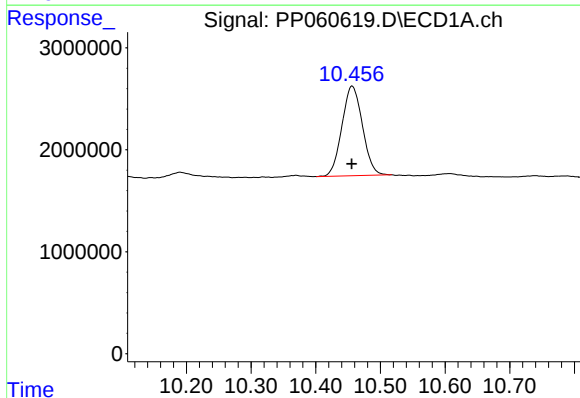


#2 Decachlorobiphenyl

R.T.: 10.456 min
Delta R.T.: 0.000 min
Response: 19388580
Conc: 10.98 ng/ml

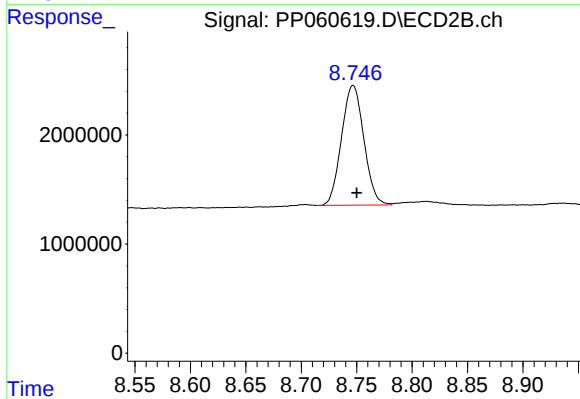

#2 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: -0.003 min
Response: 15381418
Conc: 9.43 ng/ml

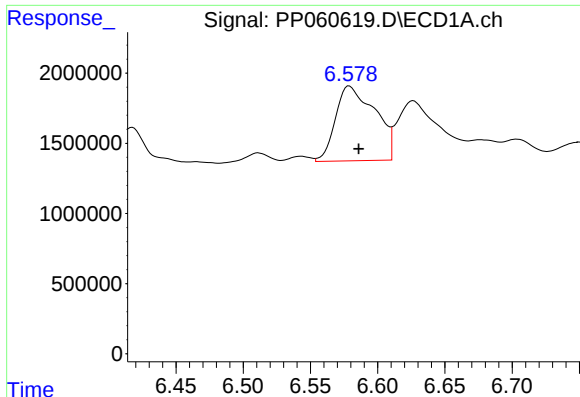


#26 AR-1254-1

R.T.: 6.579 min
Delta R.T.: -0.007 min
Response: 10878444
Conc: 127.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-34A

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

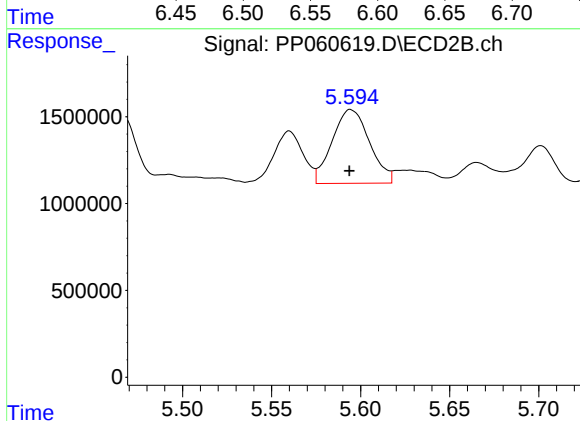


#26 AR-1254-1

R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 6209405
Conc: 62.77 ng/ml


10/06/2023
Supervised By :Ankita
Jodhani

10/06/2023

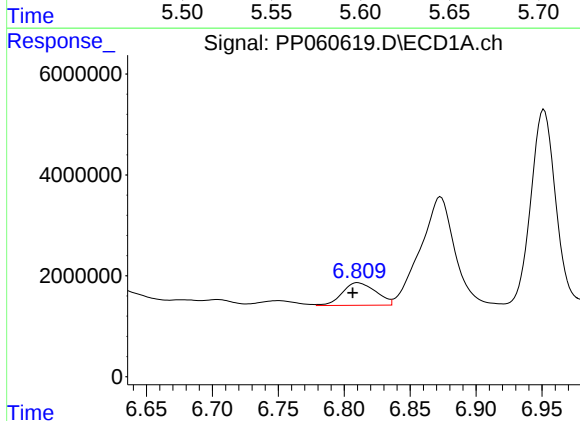


#27 AR-1254-2

R.T.: 6.810 min
Delta R.T.: 0.004 min
Response: 7921792
Conc: 62.07 ng/ml

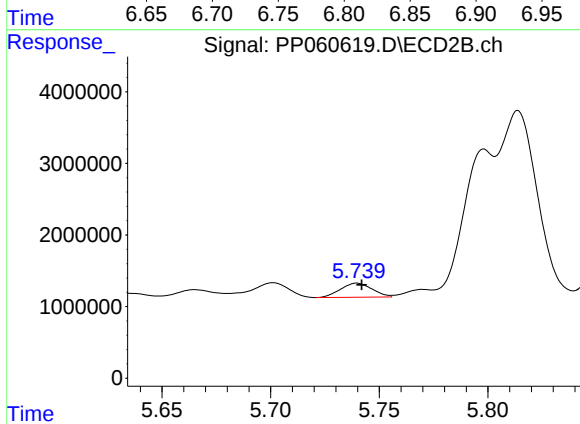

#27 AR-1254-2

R.T.: 5.740 min
Delta R.T.: -0.002 min
Response: 1985097
Conc: 23.10 ng/ml

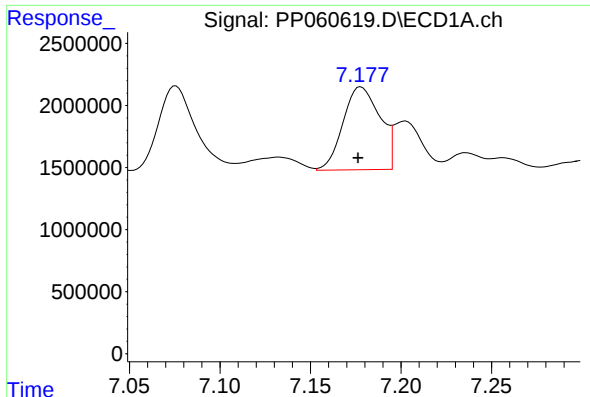


#28 AR-1254-3

R.T.: 7.178 min
Delta R.T.: 0.001 min
Response: 9488070
Conc: 71.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-34A

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

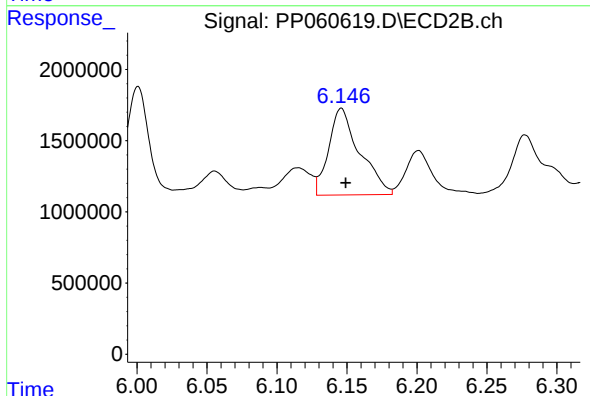


#28 AR-1254-3

R.T.: 6.146 min
Delta R.T.: -0.003 min
Response: 9420920
Conc: 65.73 ng/ml


10/06/2023
Supervised By :Ankita
Jodhani

10/06/2023

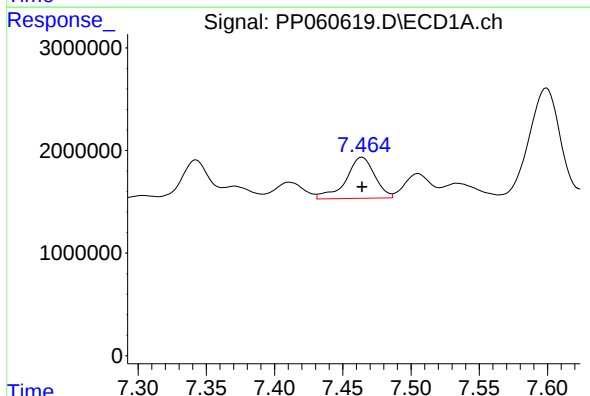


#29 AR-1254-4

R.T.: 7.464 min
Delta R.T.: 0.000 min
Response: 5888966
Conc: 59.88 ng/ml

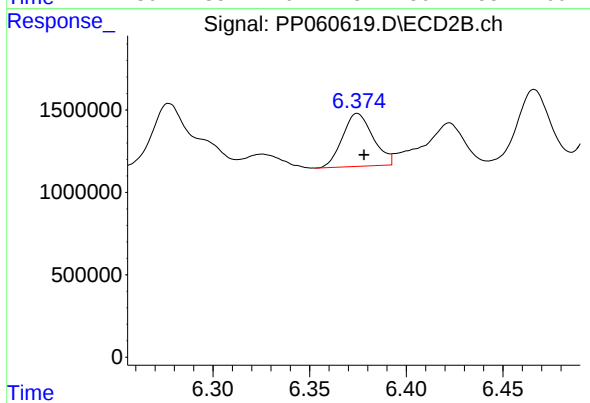

#29 AR-1254-4

R.T.: 6.375 min
Delta R.T.: -0.003 min
Response: 3532154
Conc: 40.52 ng/ml

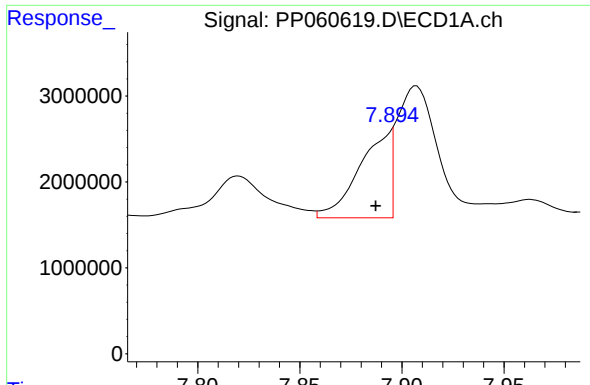


#30 AR-1254-5

R.T.: 7.894 min
Delta R.T.: 0.007 min
Response: 10303863
Conc: 95.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-34A

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

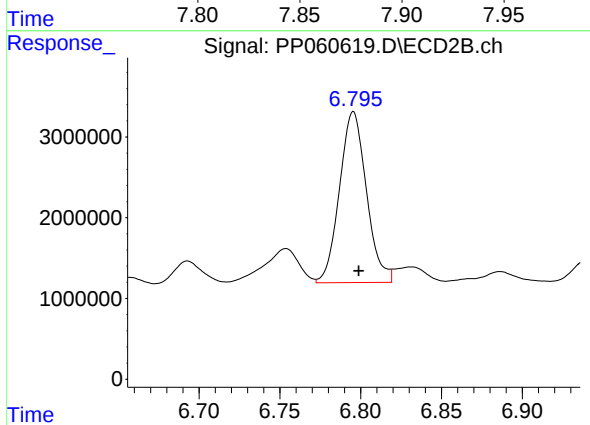

#30 AR-1254-5

R.T.: 6.795 min
Delta R.T.: -0.003 min
Response: 24565155
Conc: 193.85 ng/ml

10/06/2023
Supervised By :Ankita
Jodhani

10/06/2023