

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100523\
 Data File : PP060627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 16:44
 Operator : YP\AJ
 Sample : 04730-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K242-41A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 17:43:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.533	3.685	35755058	25383645	15.966	17.053
2) SA Decachlor...	10.462	8.749	21983222	18460678	12.451	11.317m
Target Compounds						
26) L6 AR-1254-1	6.587	5.593	16606402	12700367	194.590	128.392 #
27) L6 AR-1254-2	6.808	5.740	24411941	13267294	191.277	154.373
28) L6 AR-1254-3	7.178	6.147	44981413	43297114	338.419	302.087
29) L6 AR-1254-4	7.466	6.376	40116469	31745802	407.940	364.212
30) L6 AR-1254-5	7.889	6.797	68604523	71076200	633.215m	560.891m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100523\
Data File : PP060627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 16:44
Operator : YP\AJ
Sample : 04730-14
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
K242-41A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 17:43:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

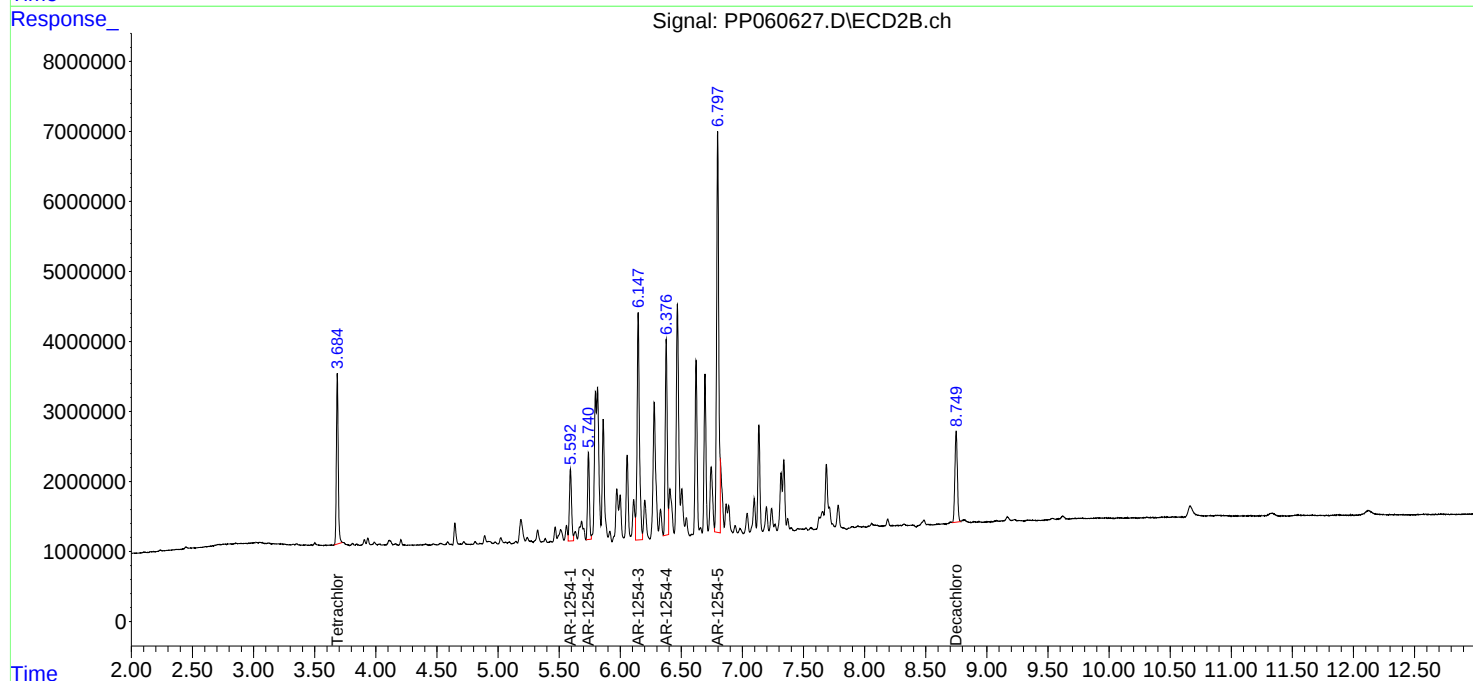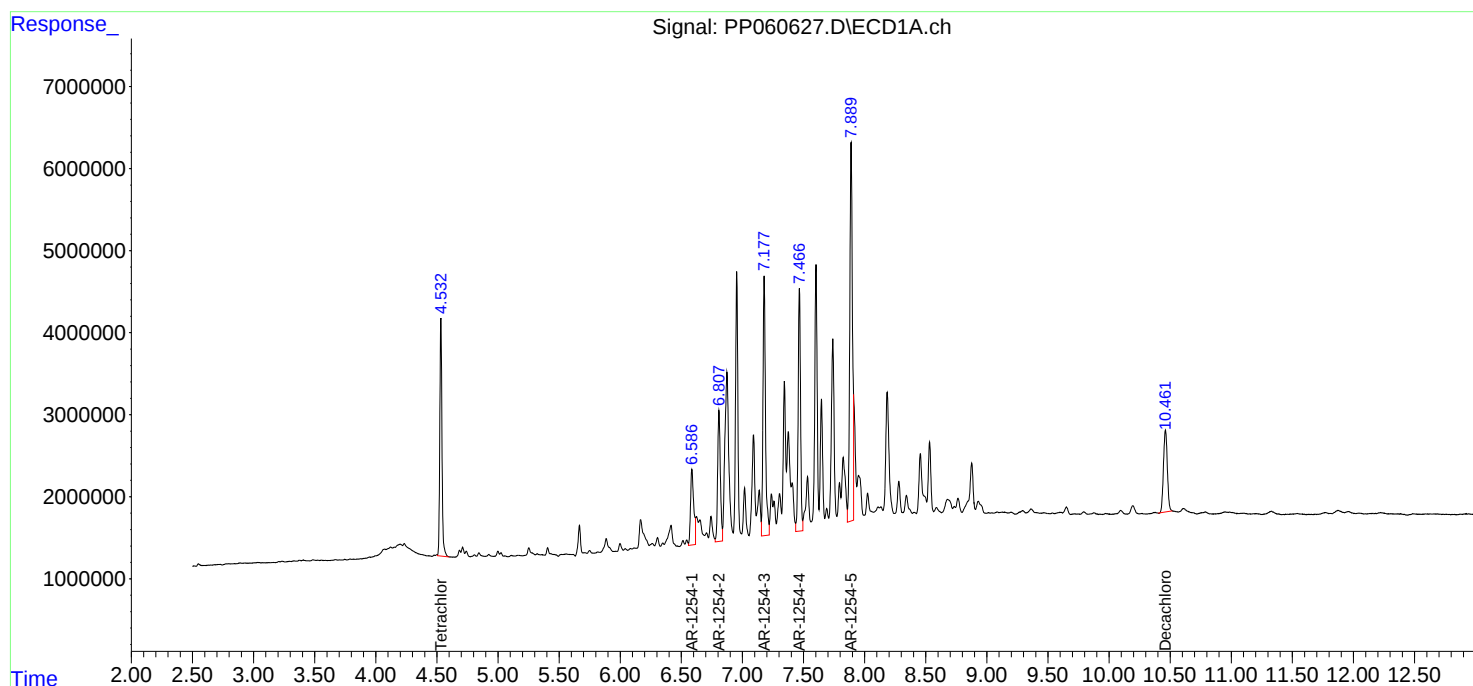

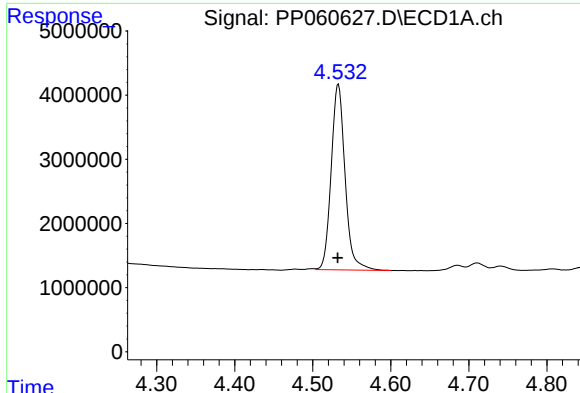


#1 Tetrachloro-m-xylene

R.T.: 4.533 min
Delta R.T.: 0.000 min
Response: 35755058
Conc: 15.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-41A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

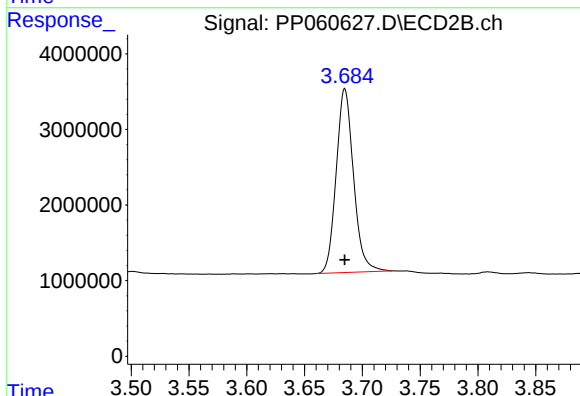


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 25383645
Conc: 17.05 ng/ml

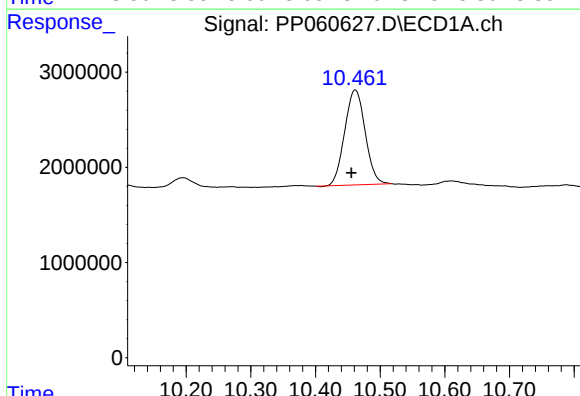


#2 Decachlorobiphenyl

R.T.: 10.462 min
Delta R.T.: 0.006 min
Response: 21983222
Conc: 12.45 ng/ml

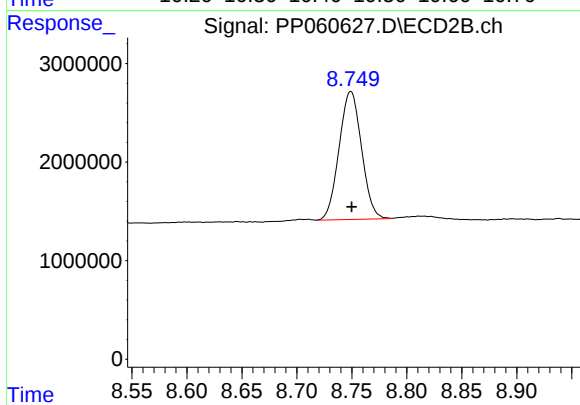

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.001 min
Response: 18460678
Conc: 11.32 ng/ml m

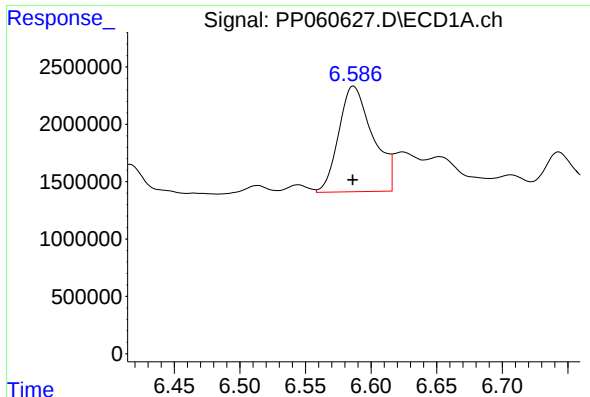


#26 AR-1254-1

R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 16606402
Conc: 194.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-41A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

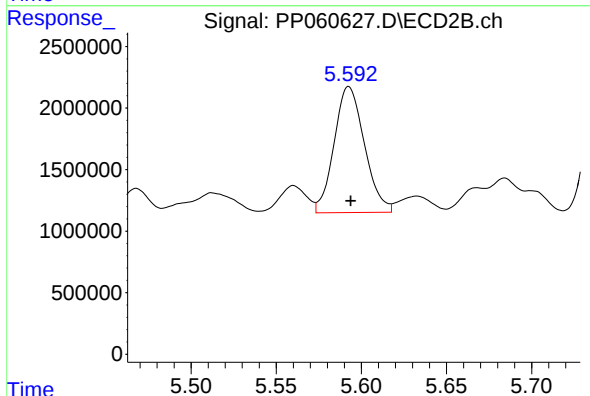


#26 AR-1254-1

R.T.: 5.593 min
Delta R.T.: -0.001 min
Response: 12700367
Conc: 128.39 ng/ml

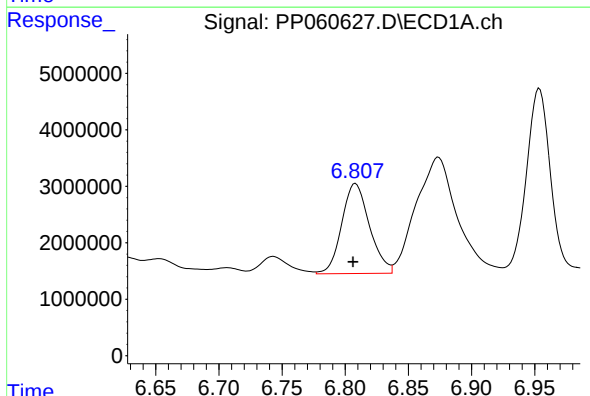


#27 AR-1254-2

R.T.: 6.808 min
Delta R.T.: 0.002 min
Response: 24411941
Conc: 191.28 ng/ml

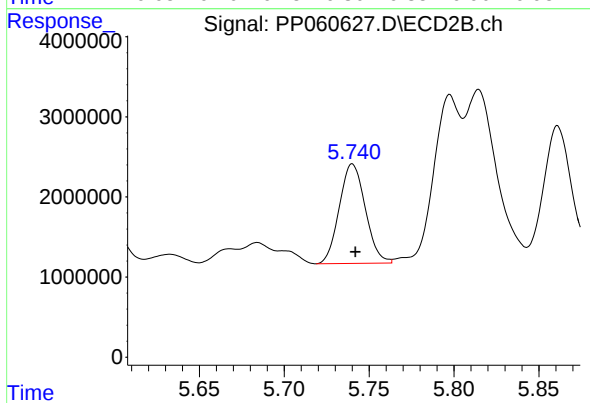

#27 AR-1254-2

R.T.: 5.740 min
Delta R.T.: -0.002 min
Response: 13267294
Conc: 154.37 ng/ml

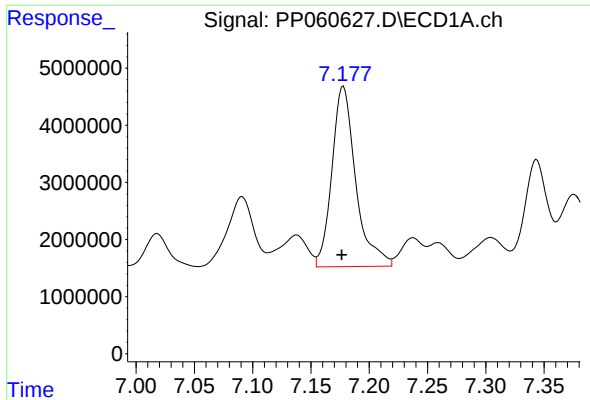


#28 AR-1254-3

R.T.: 7.178 min
Delta R.T.: 0.001 min
Response: 44981413
Conc: 338.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-41A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

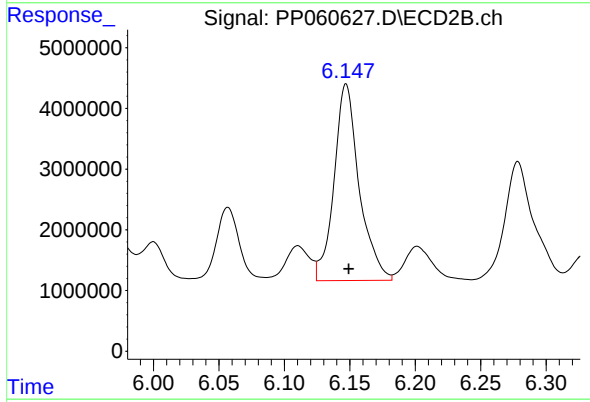


#28 AR-1254-3

R.T.: 6.147 min
Delta R.T.: -0.002 min
Response: 43297114
Conc: 302.09 ng/ml

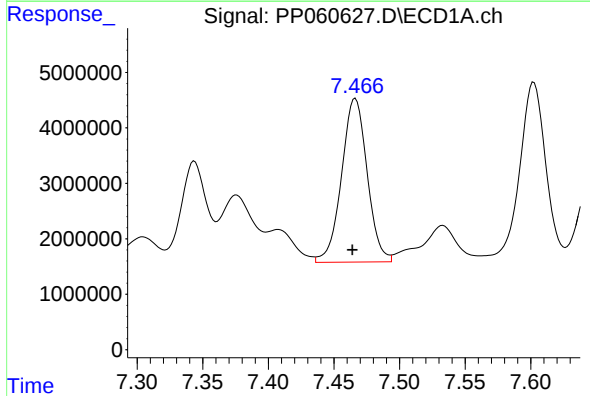


#29 AR-1254-4

R.T.: 7.466 min
Delta R.T.: 0.002 min
Response: 40116469
Conc: 407.94 ng/ml

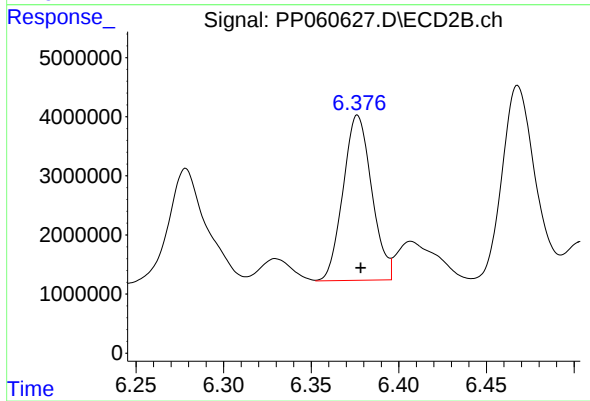

#29 AR-1254-4

R.T.: 6.376 min
Delta R.T.: -0.002 min
Response: 31745802
Conc: 364.21 ng/ml

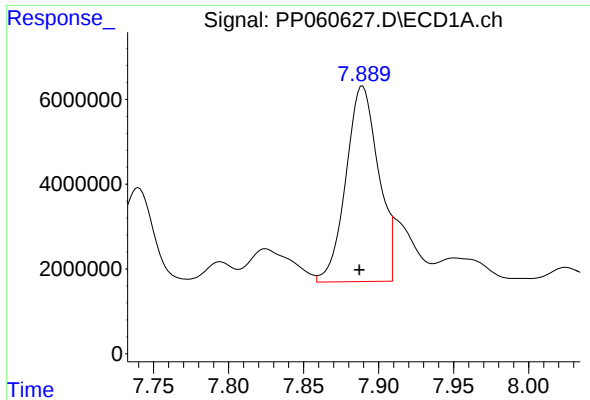


#30 AR-1254-5

R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 68604523
Conc: 633.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-41A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

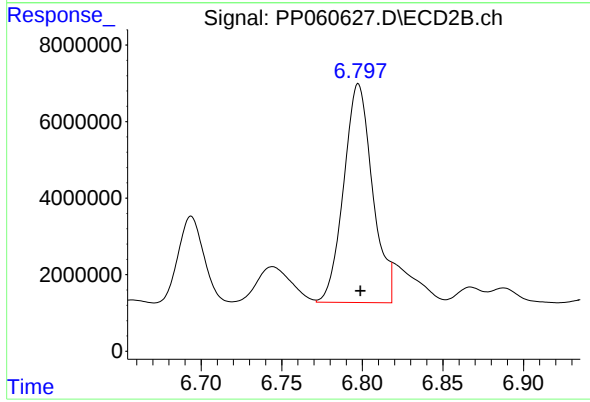

#30 AR-1254-5

R.T.: 6.797 min
Delta R.T.: -0.002 min
Response: 71076200
Conc: 560.89 ng/ml m