

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100523\
 Data File : PP060628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 17:00
 Operator : YP\AJ
 Sample : 04730-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K242-40A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/06/2023
 Supervised By :Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 17:44:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.533	3.685	40334083	28397604	18.010	19.078
2) SA Decachlor...	10.460	8.748	26500757	21344493	15.010m	13.085m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100523\
Data File : PP060628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 17:00
Operator : YP\AJ
Sample : 04730-18
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
K242-40A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 17:44:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

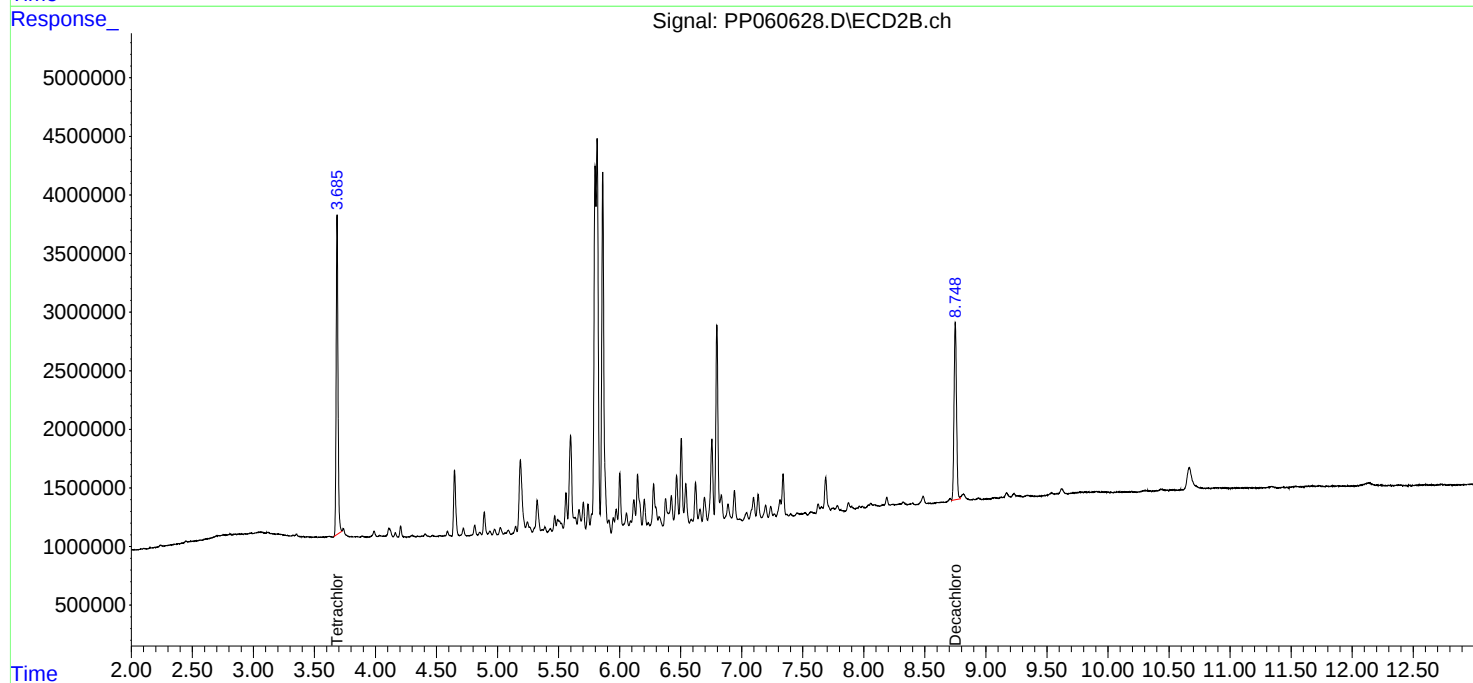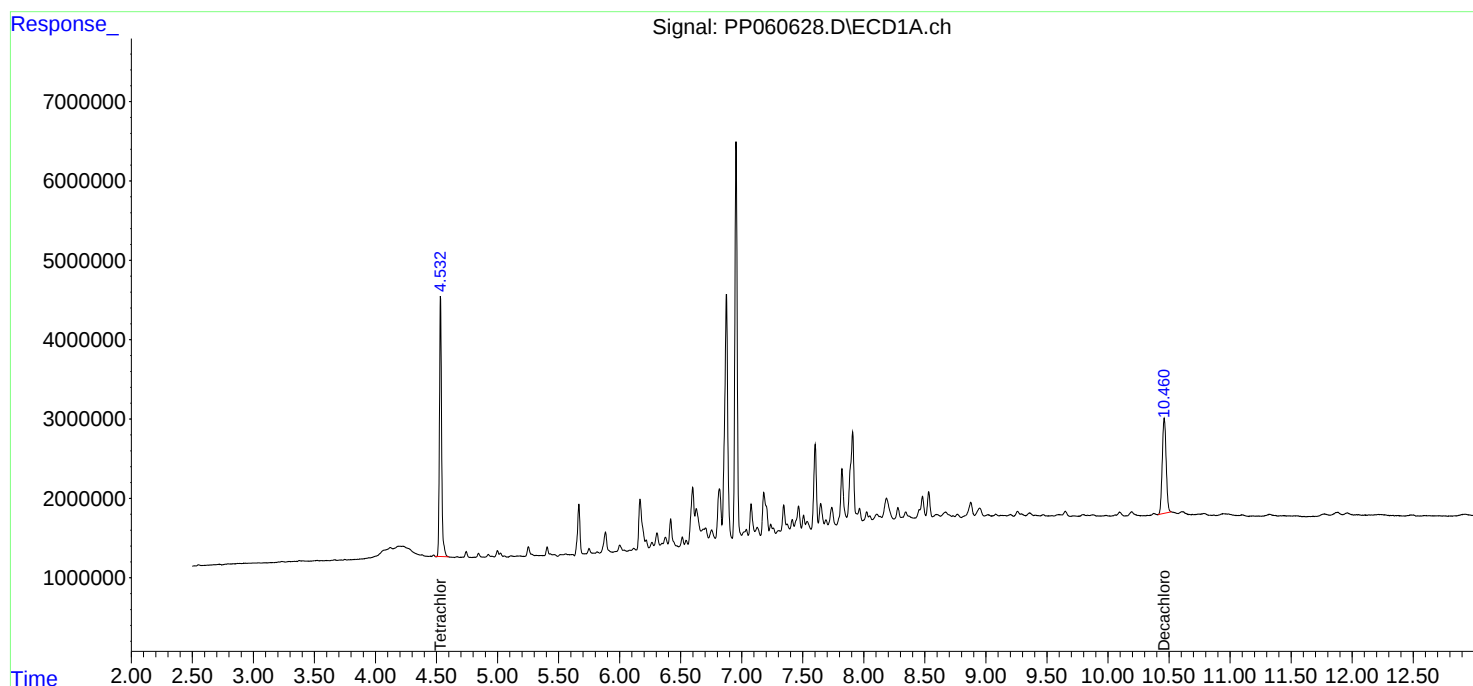

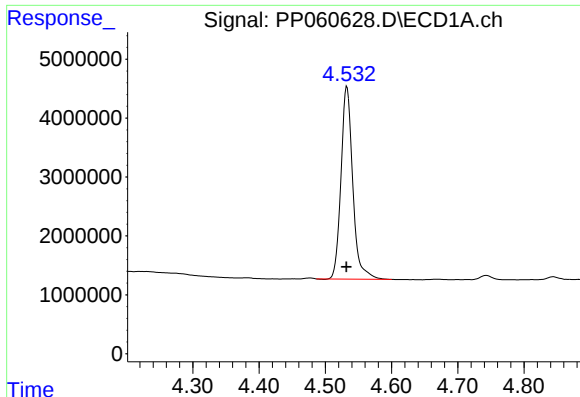


#1 Tetrachloro-m-xylene

R.T.: 4.533 min
Delta R.T.: 0.000 min
Response: 40334083
Conc: 18.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
K242-40A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

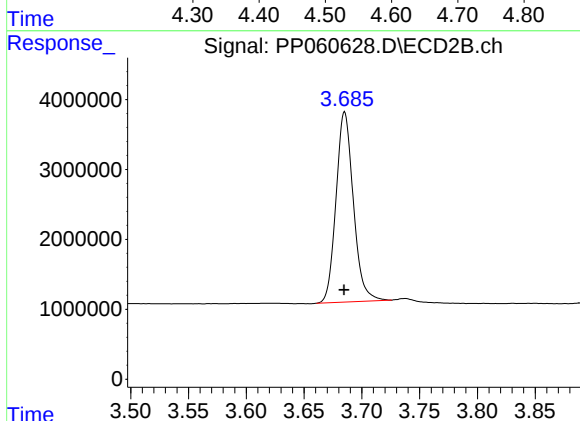


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 28397604
Conc: 19.08 ng/ml

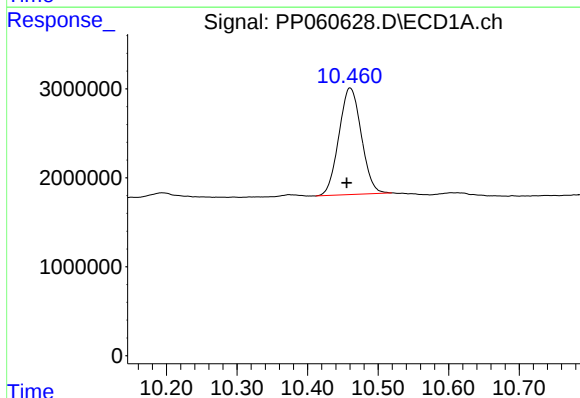

#2 Decachlorobiphenyl

R.T.: 10.460 min
Delta R.T.: 0.004 min
Response: 26500757
Conc: 15.01 ng/ml m

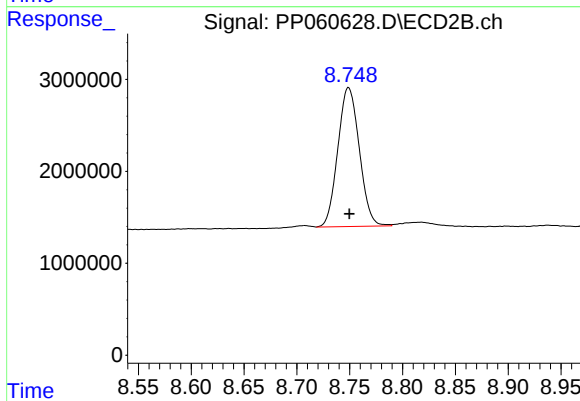

#2 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: -0.002 min
Response: 21344493
Conc: 13.09 ng/ml m