

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100622\
 Data File : PP052085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 00:18
 Operator : YP\AJ
 Sample : N5014-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-05-2.0-3.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/07/2022
 Supervised By :Ankita Jodhani 10/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 07:43:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 04 12:08:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.676	39899419	32128970	22.324	25.272
2) SA Decachlor...	10.243	8.769	29119815	20686515	24.020	17.514m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100622\
Data File : PP052085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 00:18
Operator : YP\AJ
Sample : N5014-03
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-05-2.0-3.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/07/2022
Supervised By :Ankita Jodhani 10/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 07:43:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100322.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 04 12:08:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

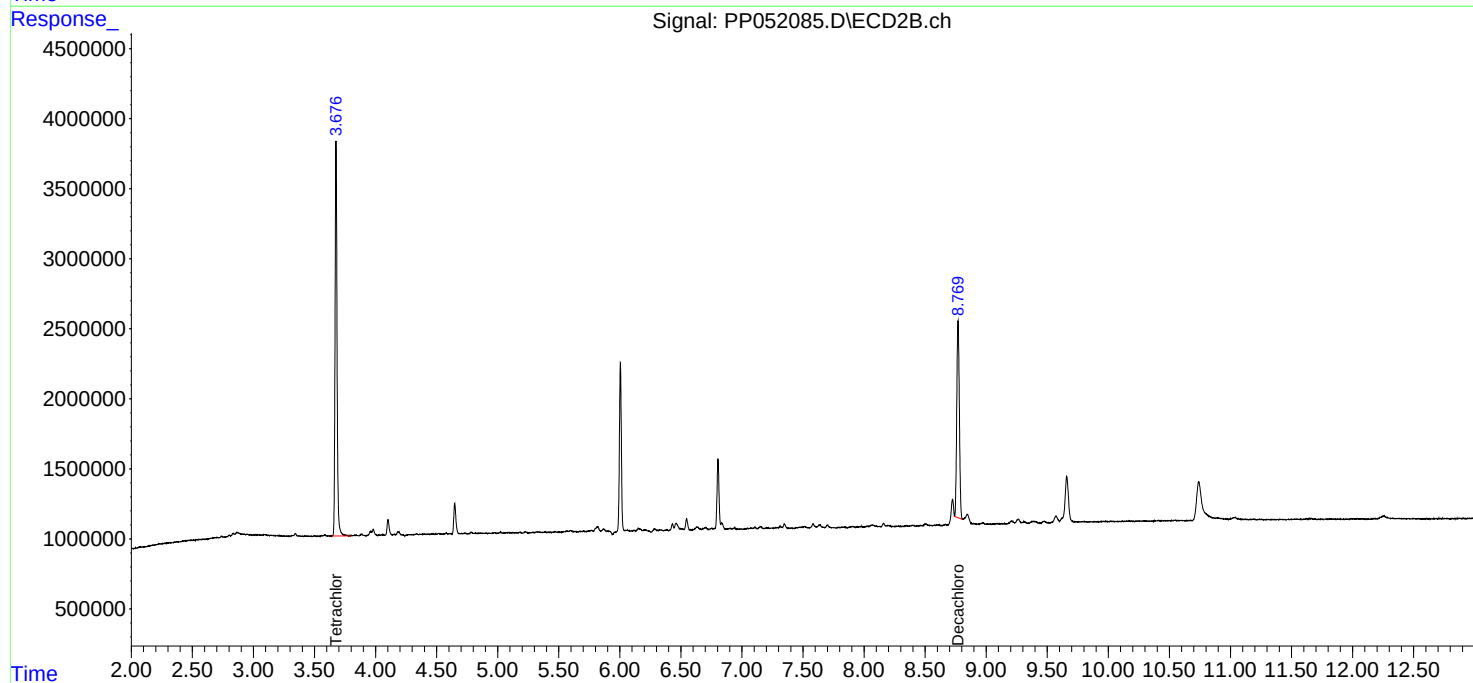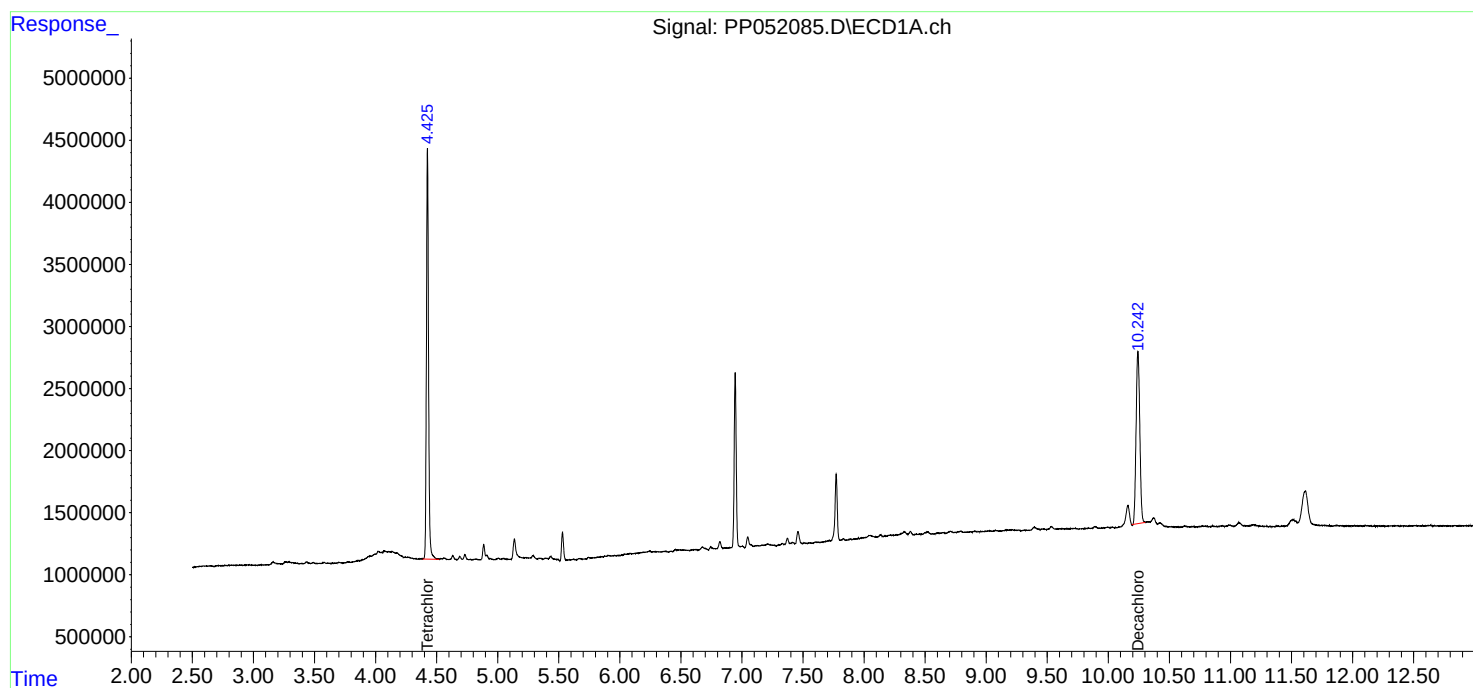

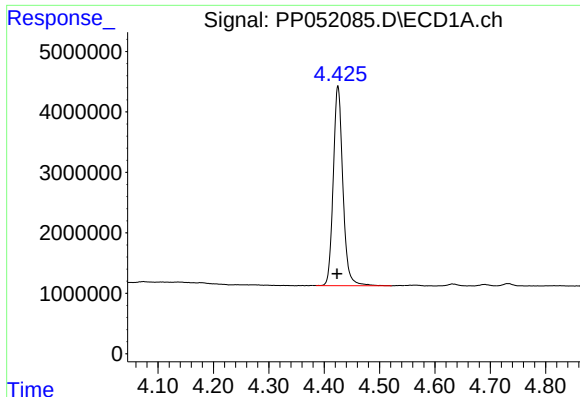

#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.002 min
Response: 39899419
Conc: 22.32 ng/ml

Instrument :

ECD_P


ClientSampleId :

SB-05-2.0-3.0

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/07/2022
Supervised By :Ankita Jodhani 10/07/2022

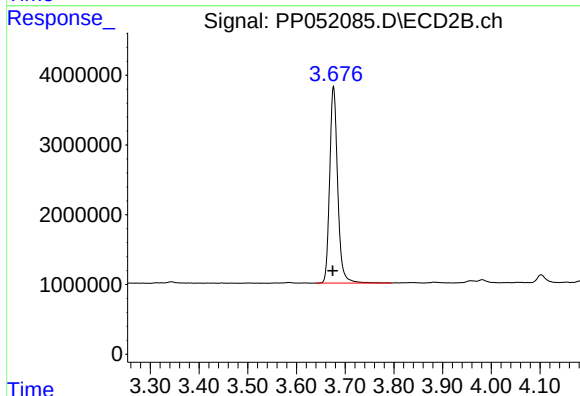


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: 0.002 min
Response: 32128970
Conc: 25.27 ng/ml

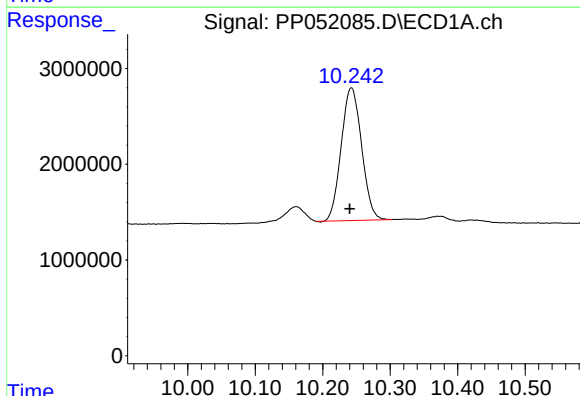

#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: 0.002 min
Response: 29119815
Conc: 24.02 ng/ml

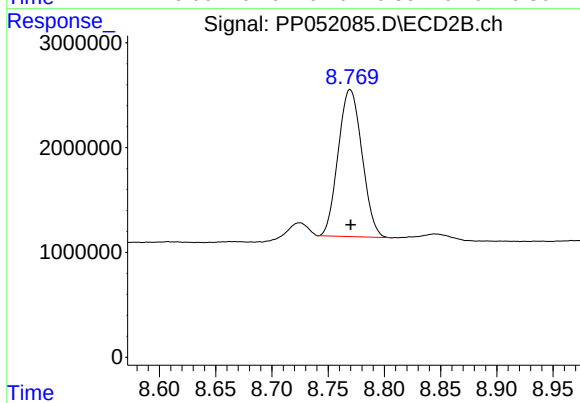

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.001 min
Response: 20686515
Conc: 17.51 ng/ml m