

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100623\
 Data File : PP060724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2023 23:38
 Operator : YP\AJ
 Sample : 04775-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-092723-33-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:02:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.533	3.685	54881314	35709780	24.506	23.990
2) SA Decachlor...	10.466	8.745	121.7E6	22454267	68.906m	13.766m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100623\
Data File : PP060724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2023 23:38
Operator : YP\AJ
Sample : 04775-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-092723-33-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:02:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

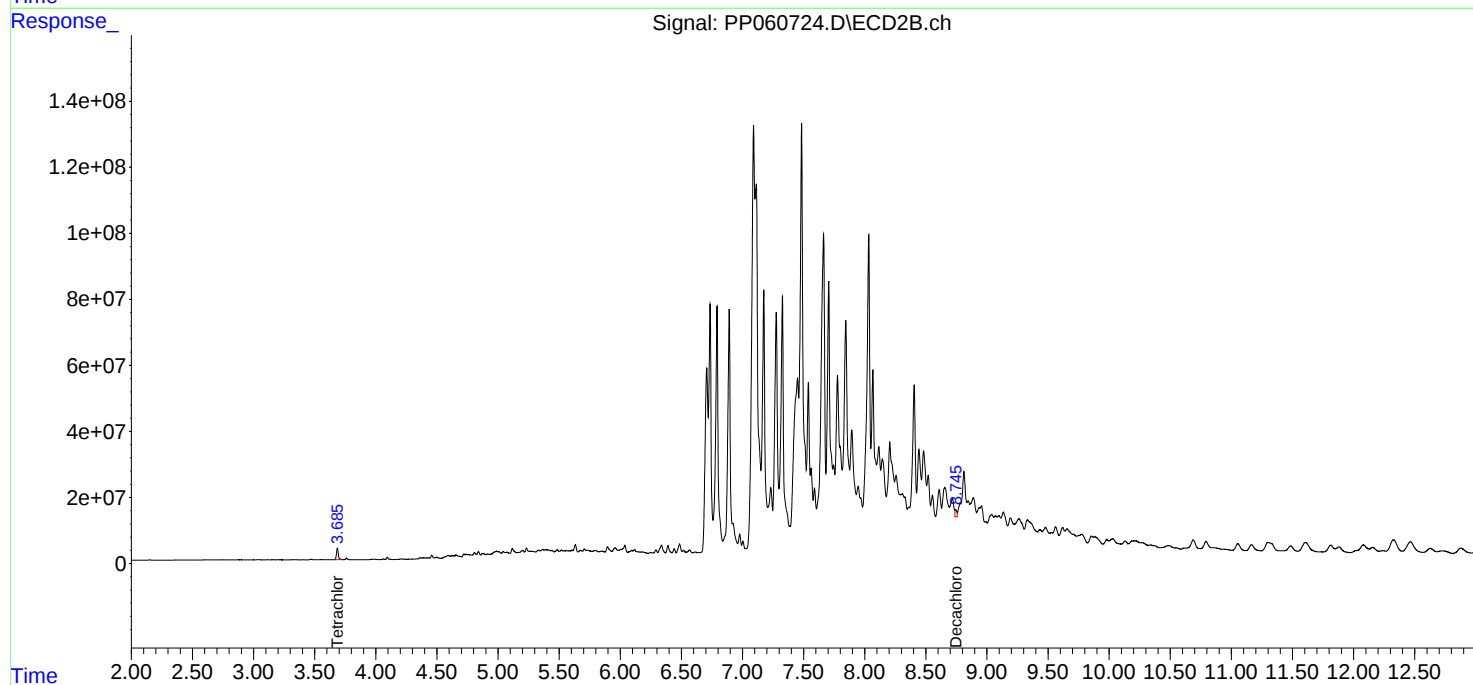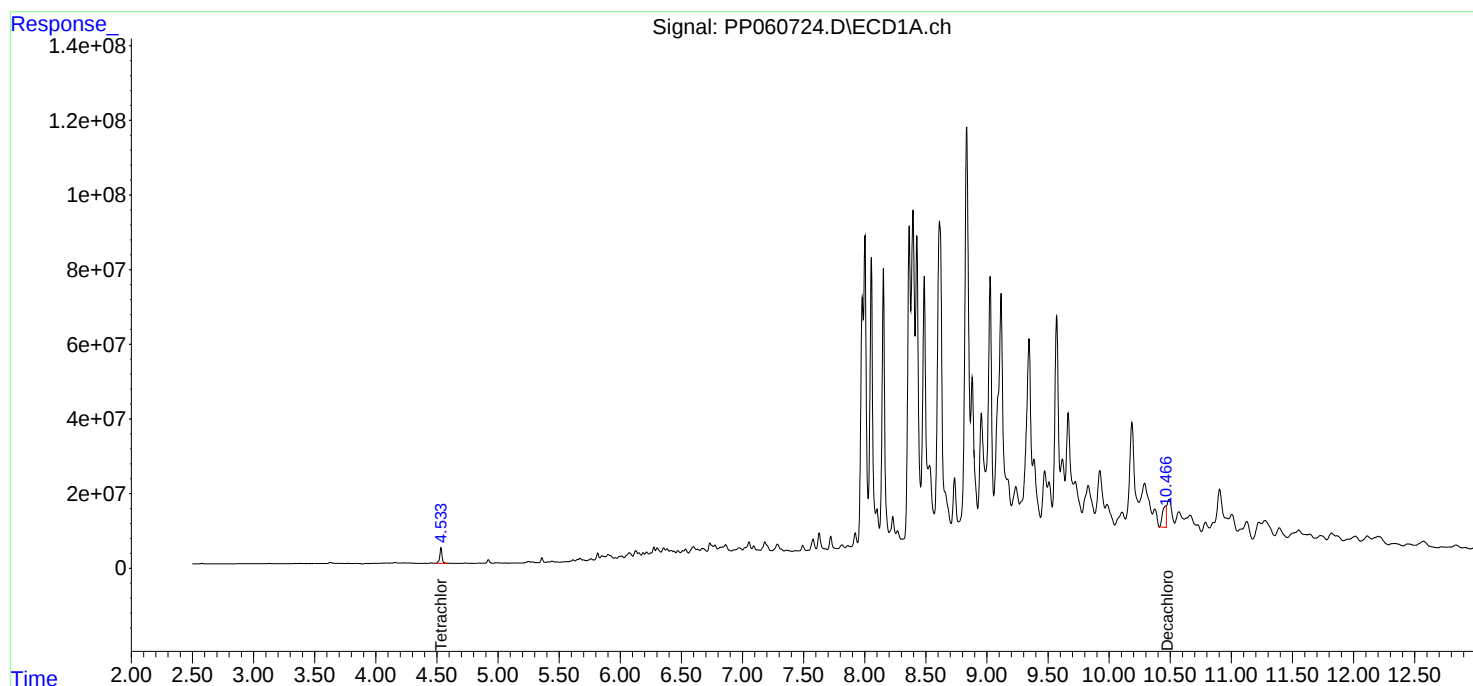


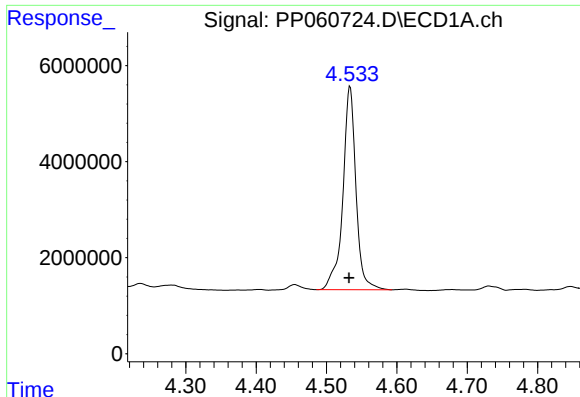

#1 Tetrachloro-m-xylene


R.T.: 4.533 min
Delta R.T.: 0.001 min
Response: 54881314
Conc: 24.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-092723-33-04

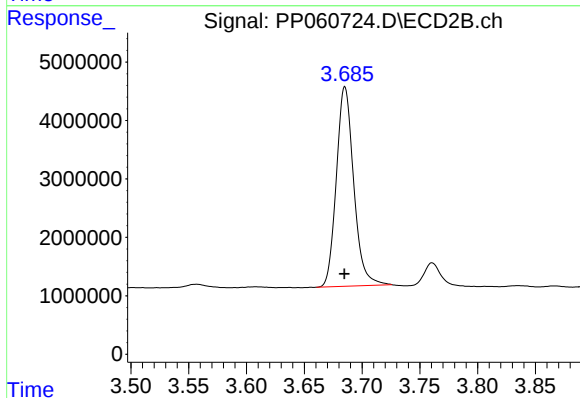


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 35709780
Conc: 23.99 ng/ml

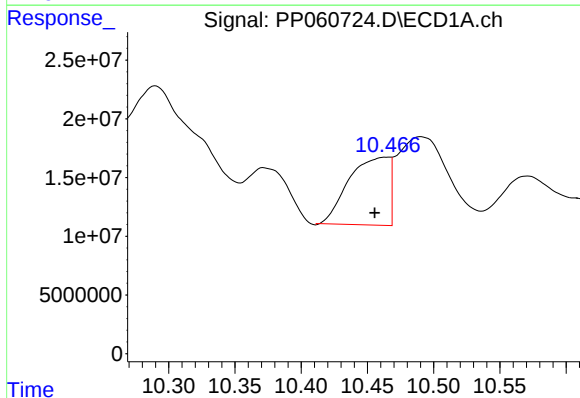

#2 Decachlorobiphenyl

R.T.: 10.466 min
Delta R.T.: 0.010 min
Response: 121655821
Conc: 68.91 ng/ml m

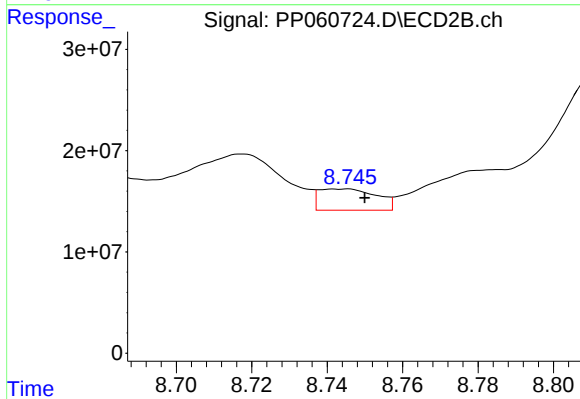

#2 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: -0.005 min
Response: 22454267
Conc: 13.77 ng/ml m