

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100625\
 Data File : PP075607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 13:25
 Operator : YP\AJ
 Sample : Q3286-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 245F102-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/07/2025
 Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 14:56:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.655	3.793	3092617	10094267	2.364	1.655 #
2) SA Decachlor...	10.427	8.797	1998059	9378771	2.003m	1.555

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100625\
Data File : PP075607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 13:25
Operator : YP\AJ
Sample : Q3286-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
245F102-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/07/2025
Supervised By :mohammad ahmed 10/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 14:56:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

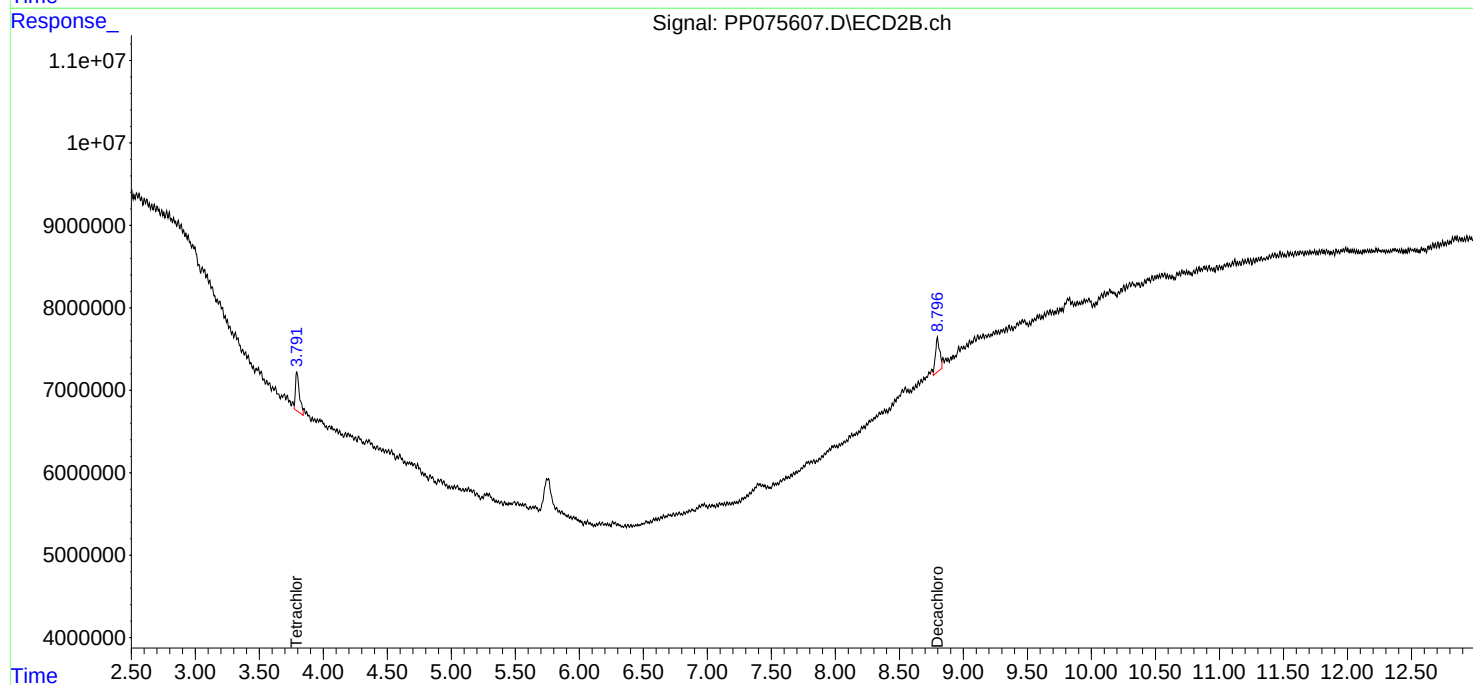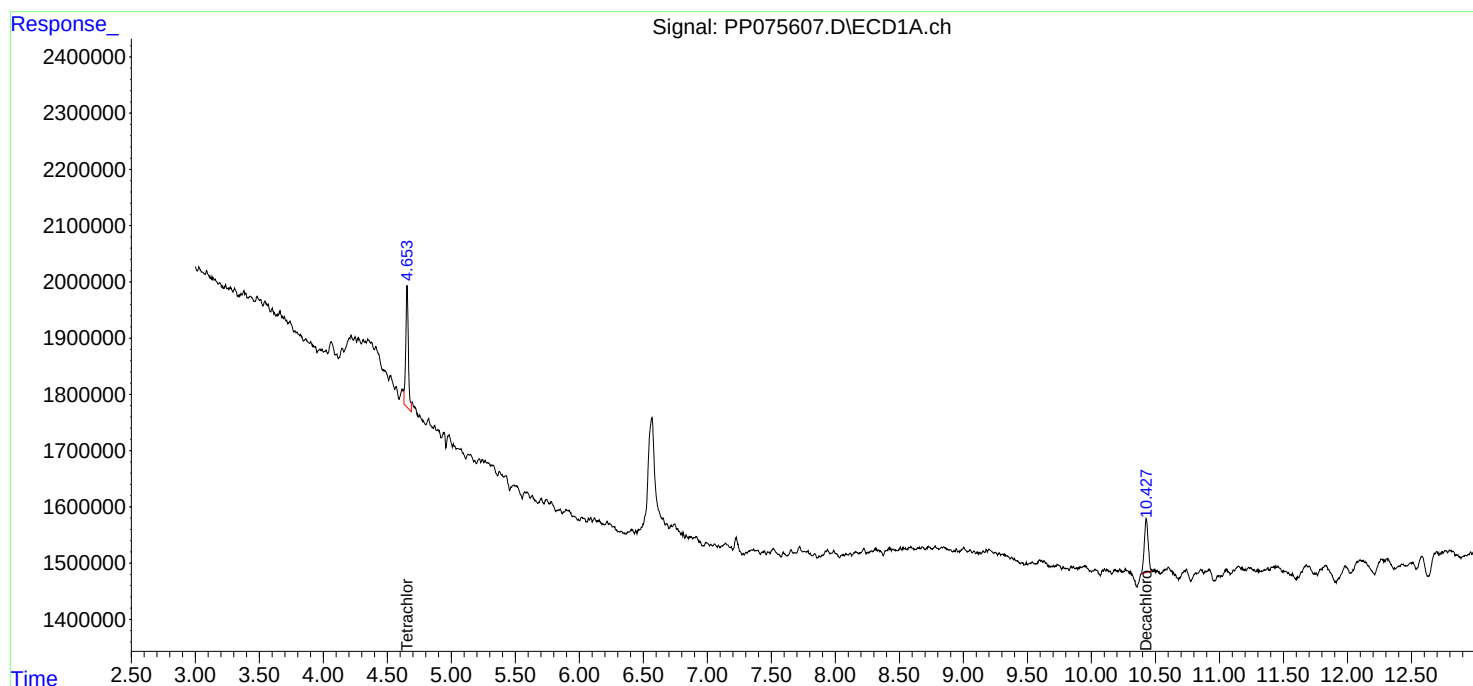

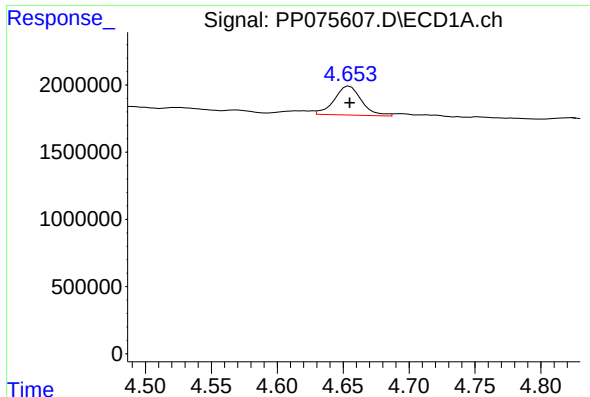


#1 Tetrachloro-m-xylene

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 3092617
Conc: 2.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
245F102-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/07/2025
Supervised By :mohammad ahmed 10/08/2025

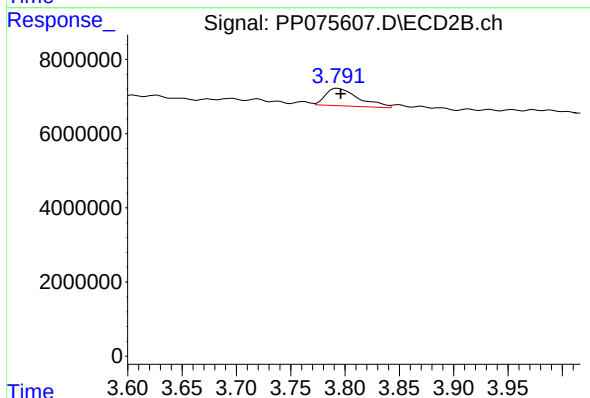


#1 Tetrachloro-m-xylene

R.T.: 3.793 min
Delta R.T.: -0.003 min
Response: 10094267
Conc: 1.65 ng/ml

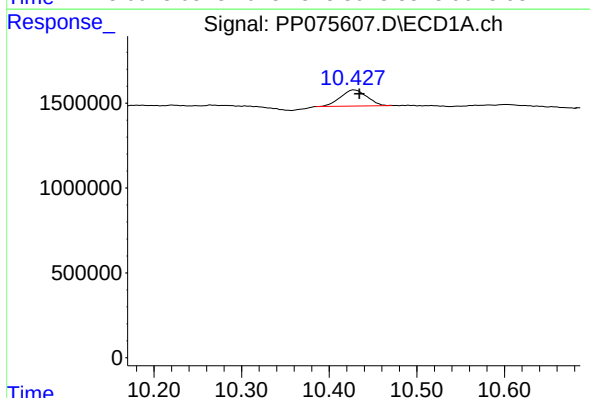

#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: -0.007 min
Response: 1998059
Conc: 2.00 ng/ml m

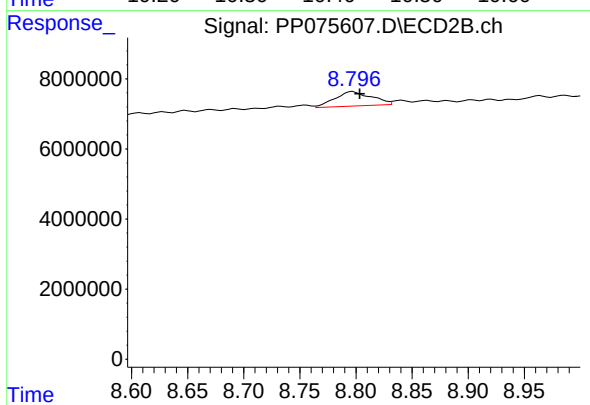

#2 Decachlorobiphenyl

R.T.: 8.797 min
Delta R.T.: -0.006 min
Response: 9378771
Conc: 1.55 ng/ml