

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100721\
 Data File : PP039876.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 00:04
 Operator : AJ\MA
 Sample : M4119-04
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20-TW-2-20211006-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 05:19:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.986	725546	386861	23.831	23.142
2) SA Decachlor...	10.920	9.318	356764	348336	15.869	15.528

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100721\
Data File : PP039876.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 00:04
Operator : AJ\MA
Sample : M4119-04
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20-TW-2-20211006-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 05:19:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

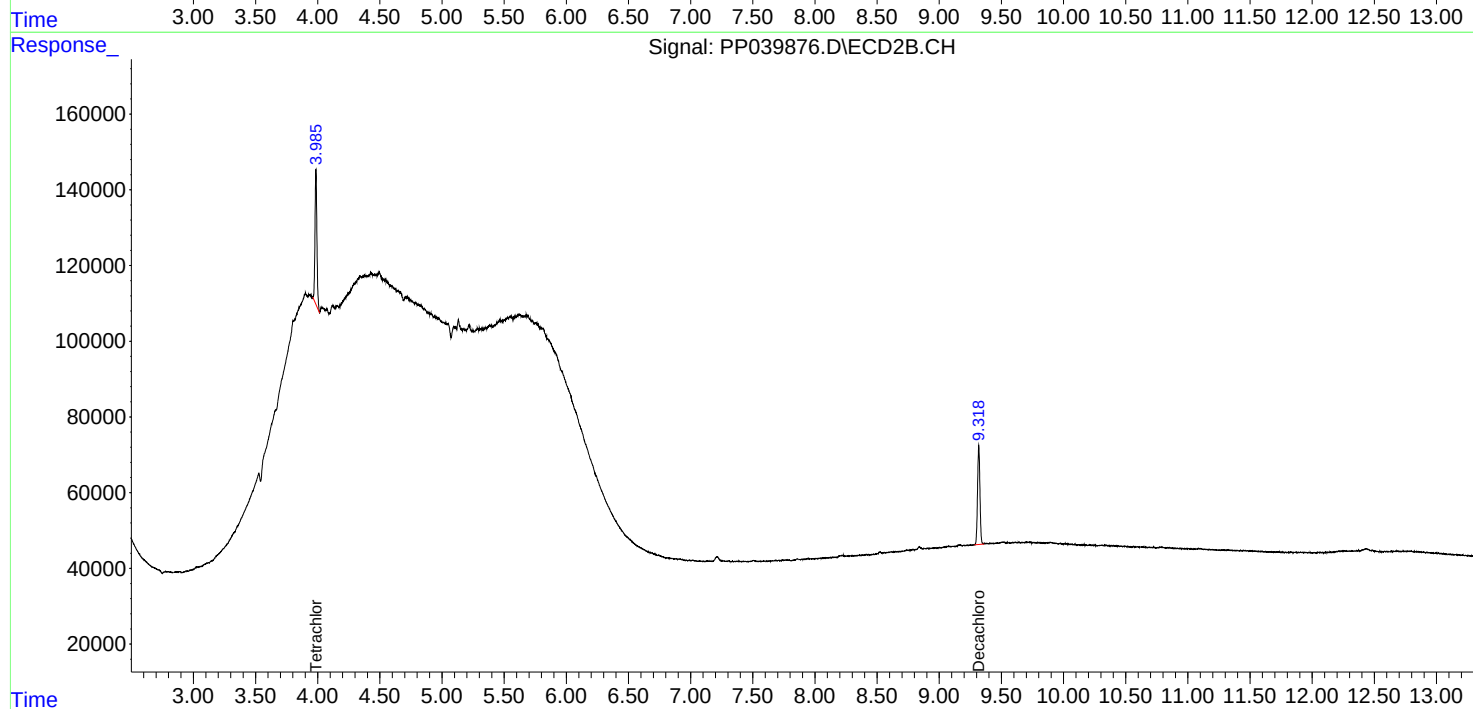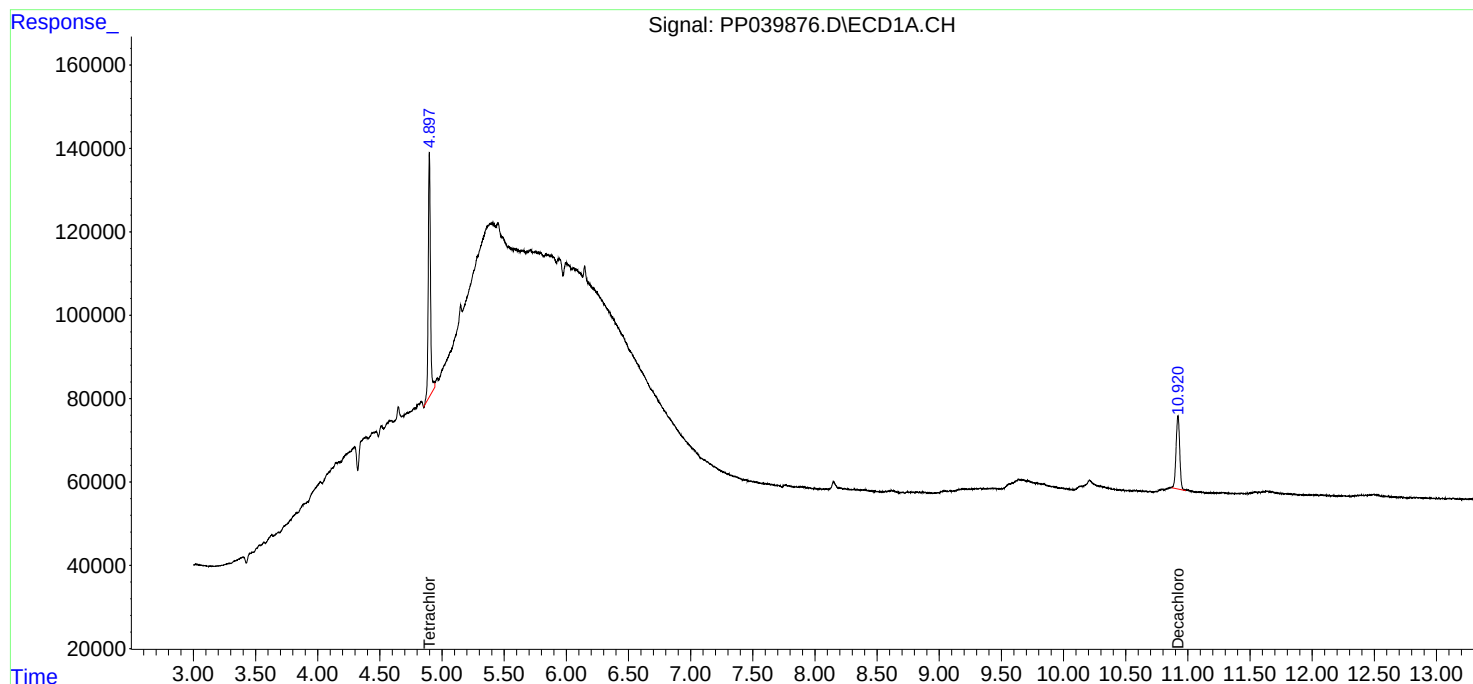


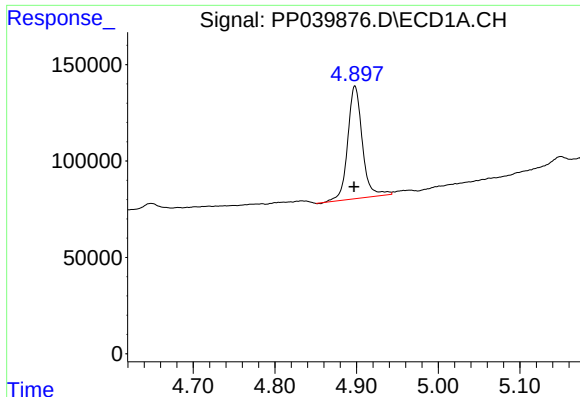

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: 0.001 min
Response: 725546
Conc: 23.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
20-TW-2-20211006-A

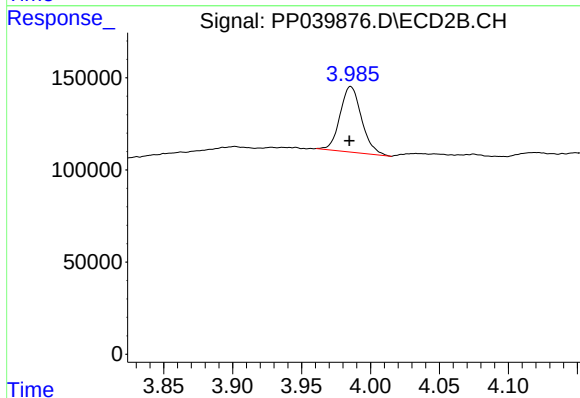


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 386861
Conc: 23.14 ng/ml

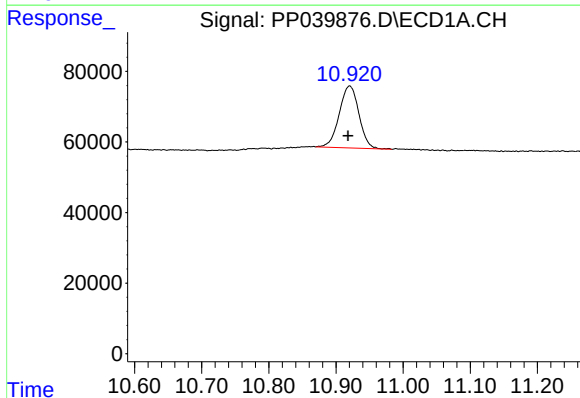

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: 0.003 min
Response: 356764
Conc: 15.87 ng/ml

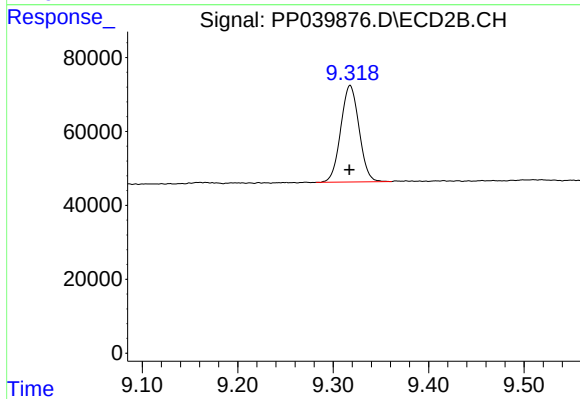

#2 Decachlorobiphenyl

R.T.: 9.318 min
Delta R.T.: 0.000 min
Response: 348336
Conc: 15.53 ng/ml