

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100721\
 Data File : PP039877.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 00:20
 Operator : AJ\MA
 Sample : M4119-05
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EB-20211006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 05:19:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.985	730248	414873	23.986	24.818
2) SA Decachlor...	10.919	9.316	525449	515858	23.373	22.996

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100721\
Data File : PP039877.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 00:20
Operator : AJ\MA
Sample : M4119-05
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
EB-20211006

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 05:19:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

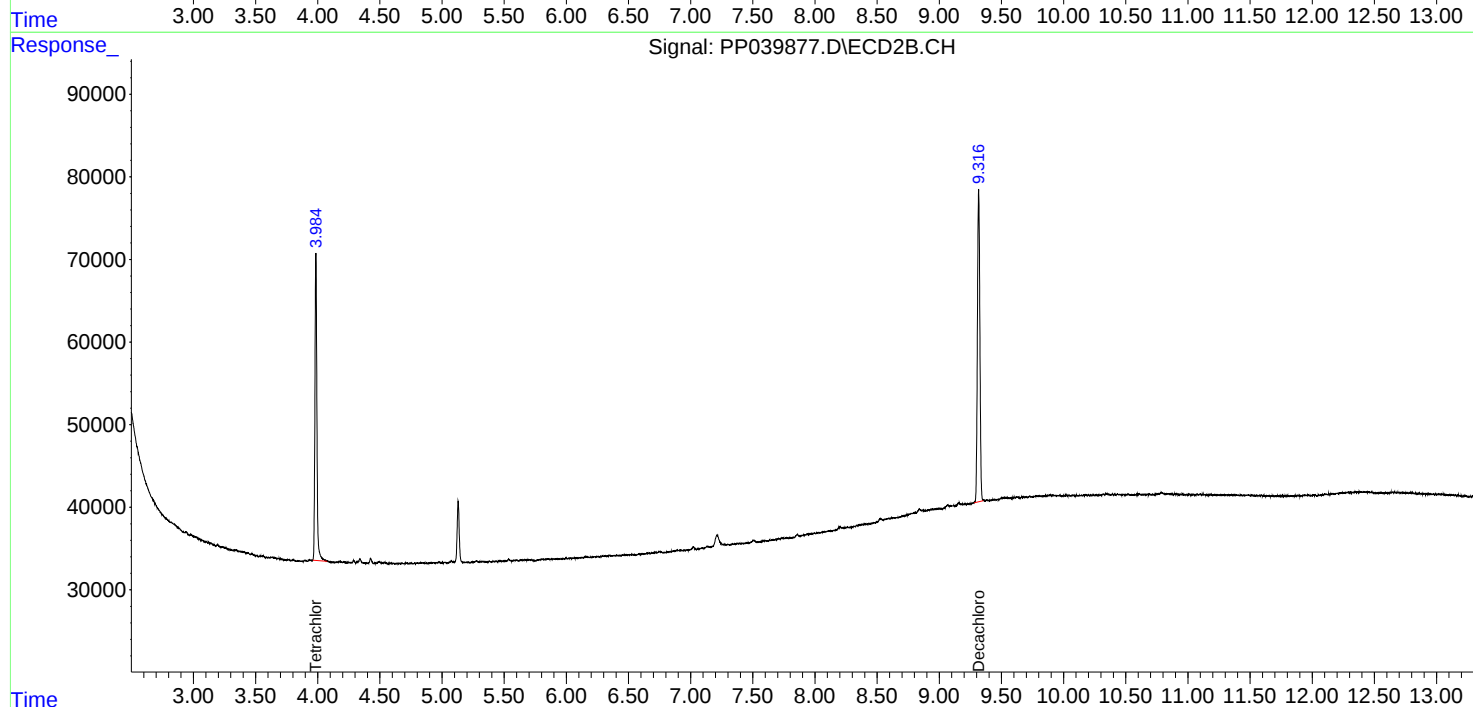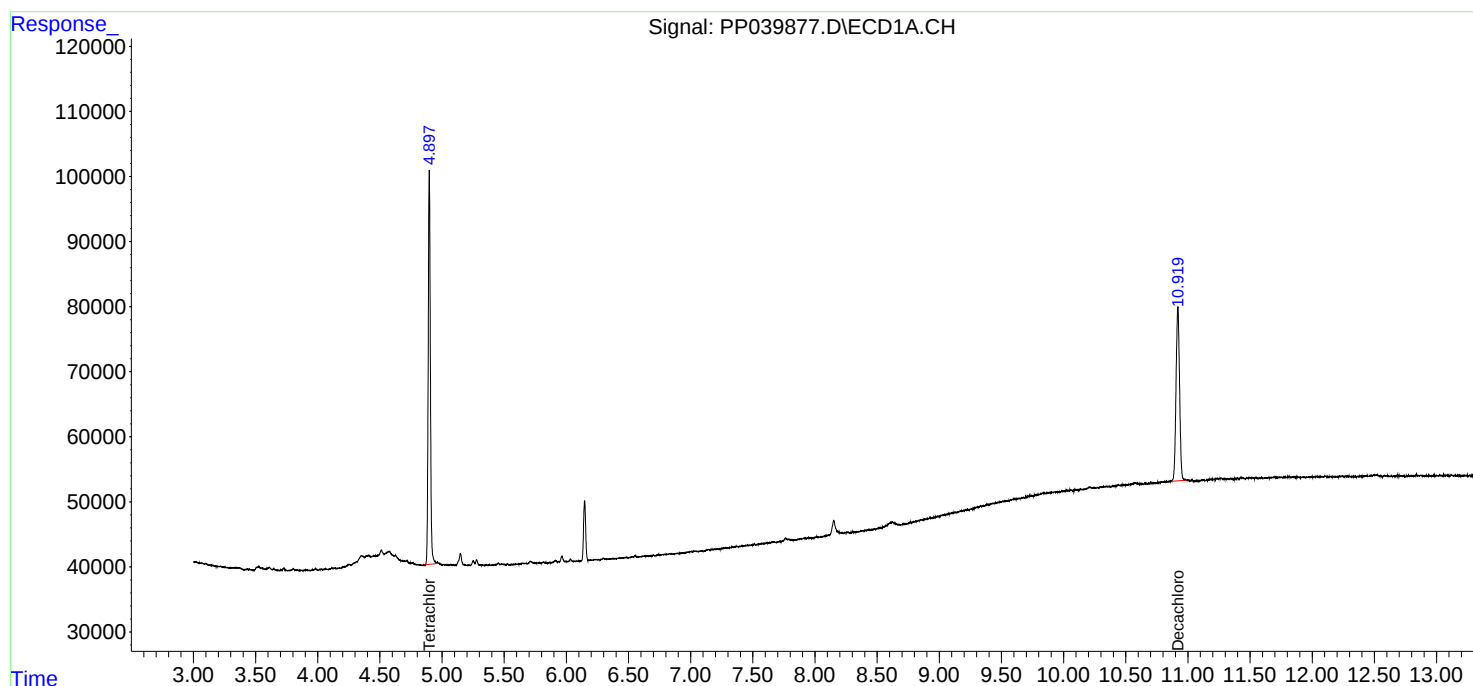


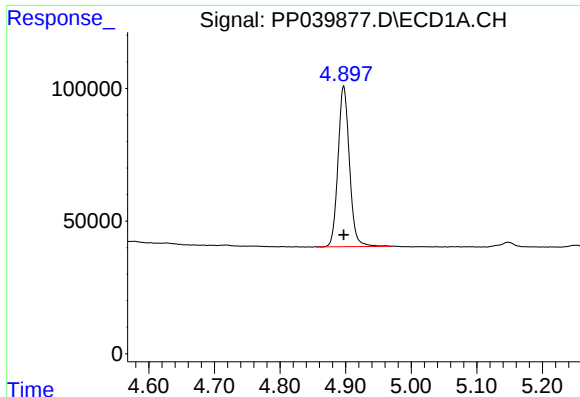

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 730248
Conc: 23.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
EB-20211006

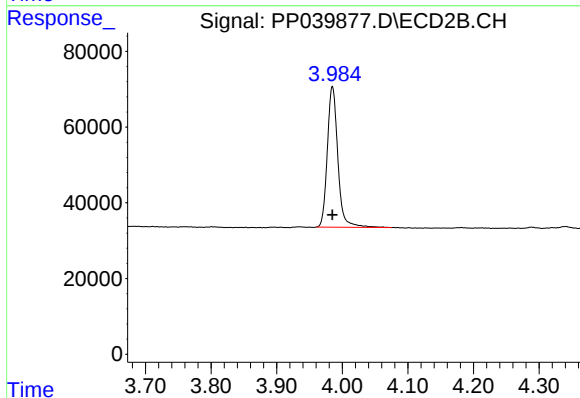


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 414873
Conc: 24.82 ng/ml

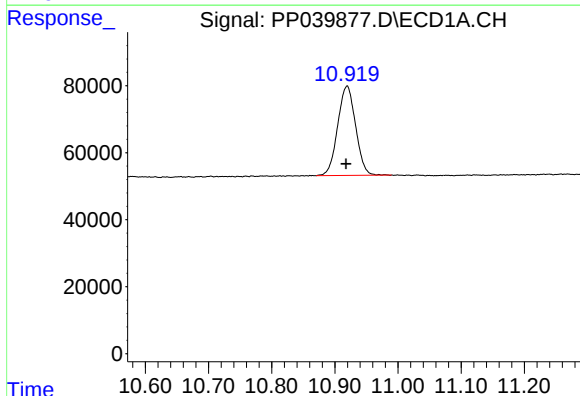

#2 Decachlorobiphenyl

R.T.: 10.919 min
Delta R.T.: 0.002 min
Response: 525449
Conc: 23.37 ng/ml

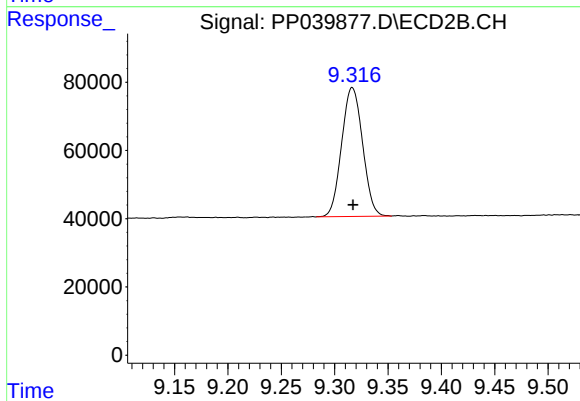

#2 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: 0.000 min
Response: 515858
Conc: 23.00 ng/ml