

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
 Data File : PP039894.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 9:54
 Operator : AJ\MA
 Sample : PB139717BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 12:58:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.896	3.983	578693	331067	19.008	19.805
2)	SA Decachlor...	10.917	9.315	445498	439850	19.816	19.608
Target Compounds							
9)	L2 AR-1221-2	5.278f	0.000	20832	0	75.710	N.D. #
10)	L2 AR-1221-3	0.000	4.424	0	13824	N.D.	25.818 #
11)	L3 AR-1232-1	0.000	4.424	0	13824	N.D.	34.522 #
33)	L7 AR-1260-3	0.000	7.210	0	25510	N.D.	19.239 #
38)	L8 AR-1262-3	0.000	8.194f	0	10121	N.D.	9.869 #
41)	L9 AR-1268-1	0.000	8.194f	0	10121	N.D.	3.466 #
43)	L9 AR-1268-3	0.000	8.523f	0	9600	N.D.	4.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
Data File : PP039894.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 9:54
Operator : AJ\MA
Sample : PB139717BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 12:58:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

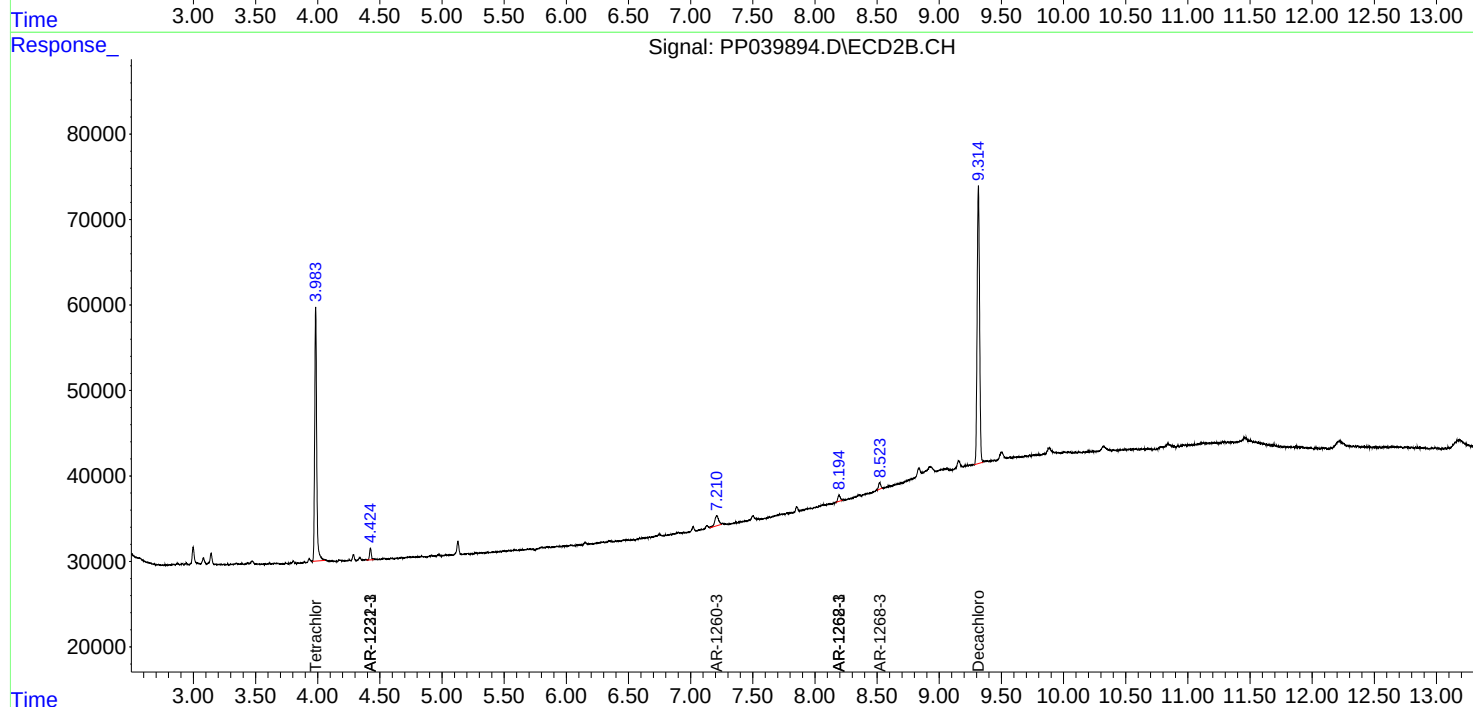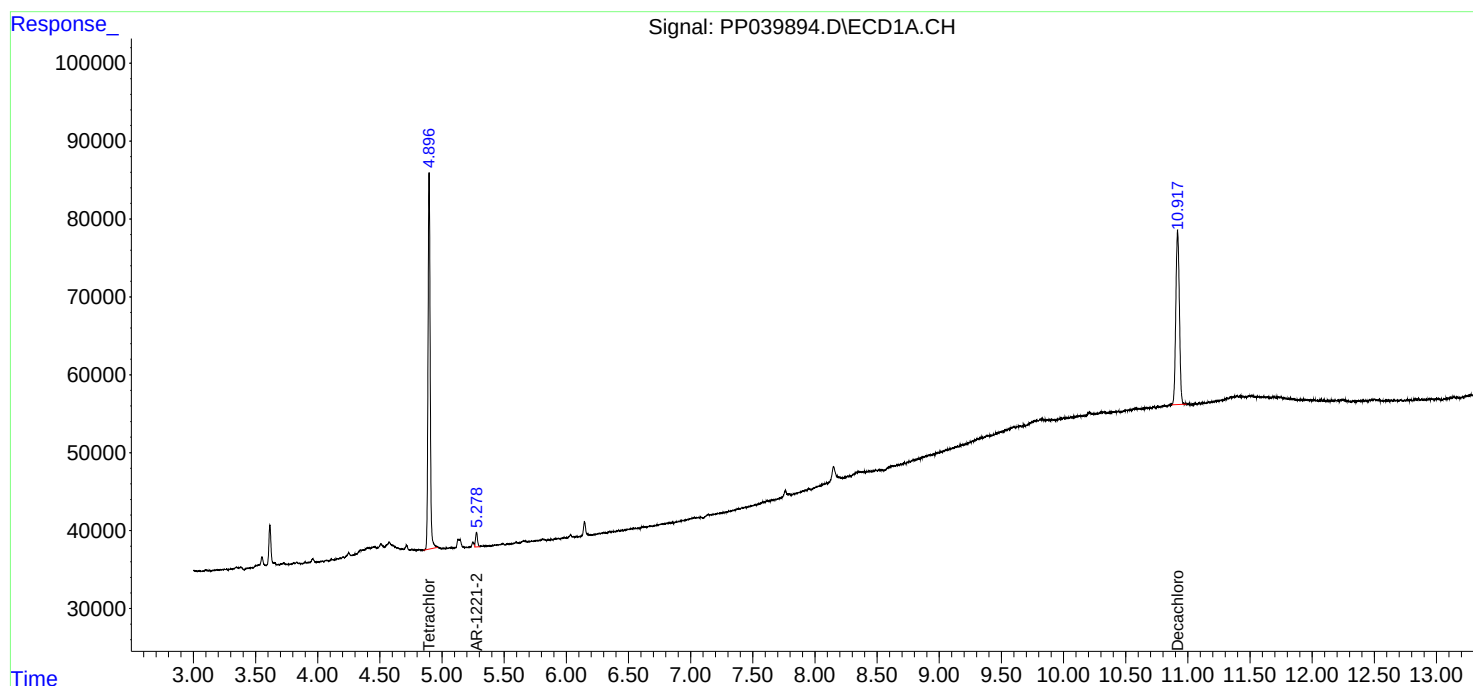


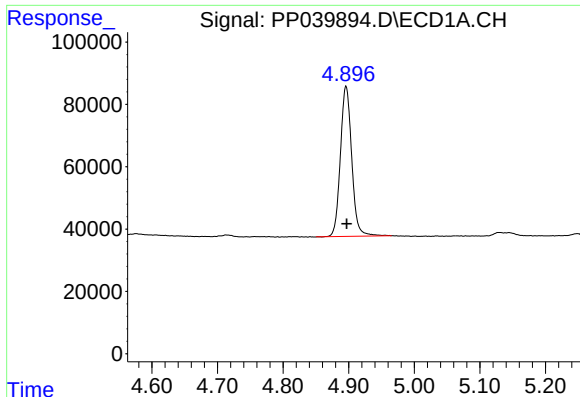

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 578693
Conc: 19.01 ng/ml

Instrument :
ECD_P
ClientSampleId :

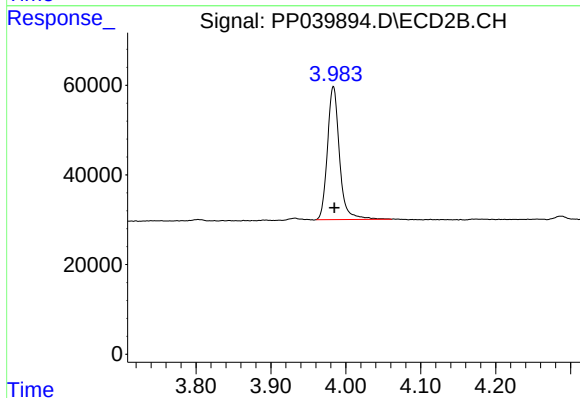


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.001 min
Response: 331067
Conc: 19.80 ng/ml

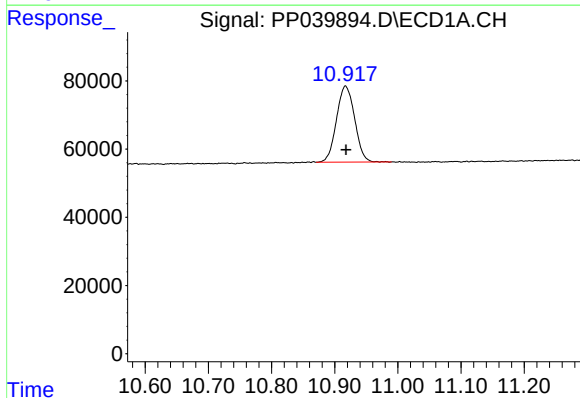


#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: 0.000 min
Response: 445498
Conc: 19.82 ng/ml

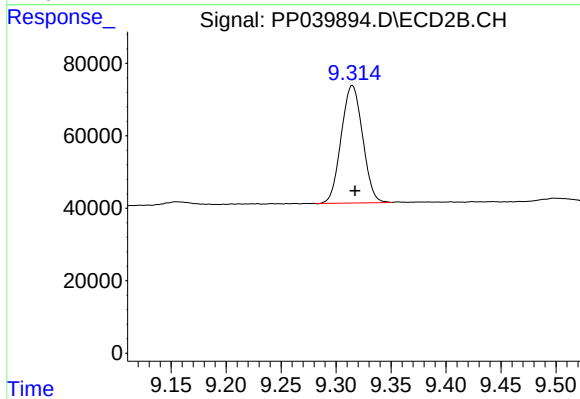

#2 Decachlorobiphenyl


R.T.: 9.315 min
Delta R.T.: -0.002 min
Response: 439850
Conc: 19.61 ng/ml

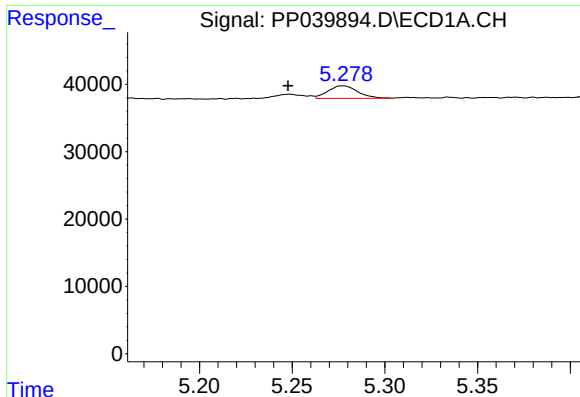

#9 AR-1221-2


R.T.: 5.278 min
Delta R.T.: 0.030 min
Response: 20832
Conc: 75.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

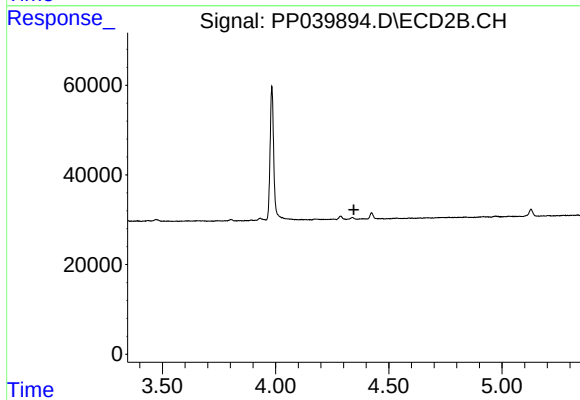


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.346 min
Response: 0
Conc: N.D.

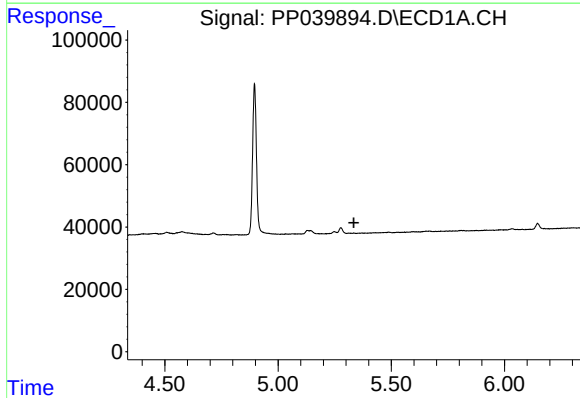


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

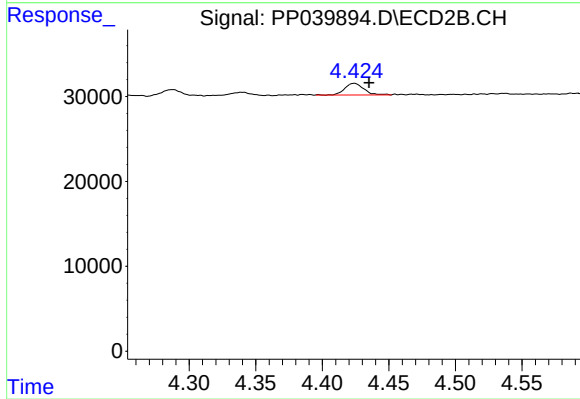

#10 AR-1221-3


R.T.: 4.424 min
Delta R.T.: -0.011 min
Response: 13824
Conc: 25.82 ng/ml

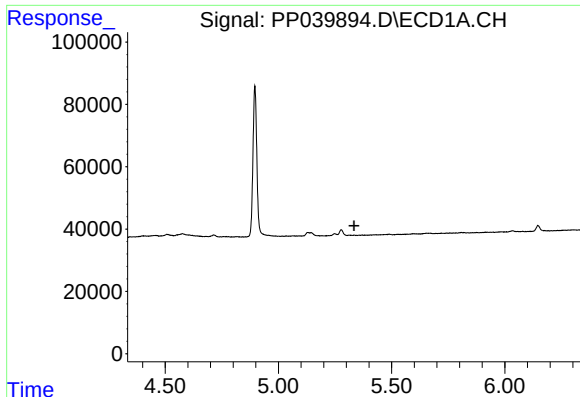

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 5.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

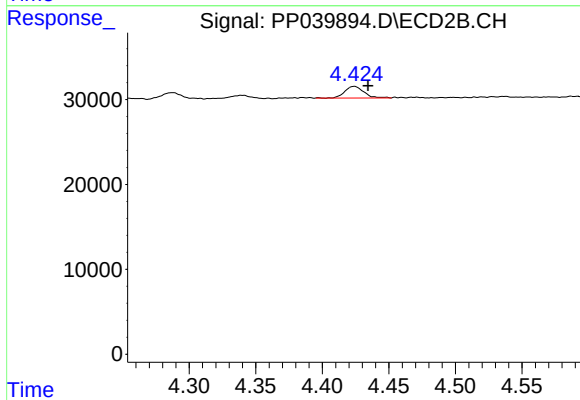


#11 AR-1232-1

R.T.: 4.424 min
Delta R.T.: -0.010 min
Response: 13824
Conc: 34.52 ng/ml

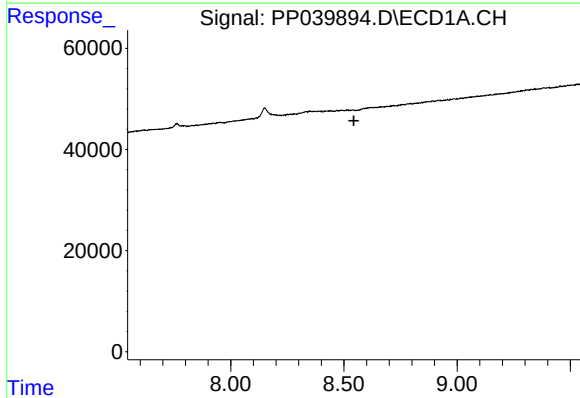


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.544 min
Response: 0
Conc: N.D.

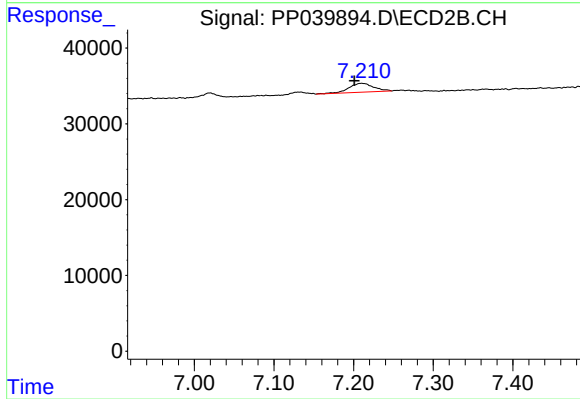

#33 AR-1260-3


R.T.: 7.210 min
Delta R.T.: 0.009 min
Response: 25510
Conc: 19.24 ng/ml

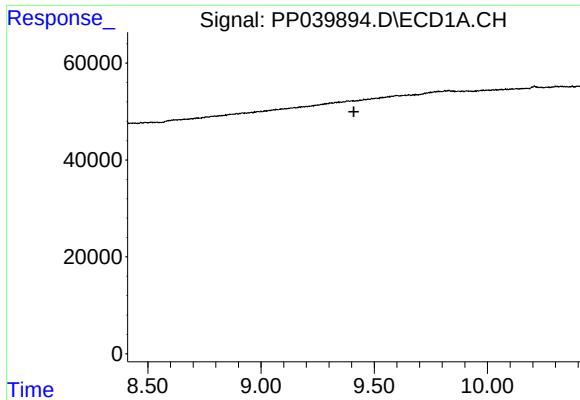

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

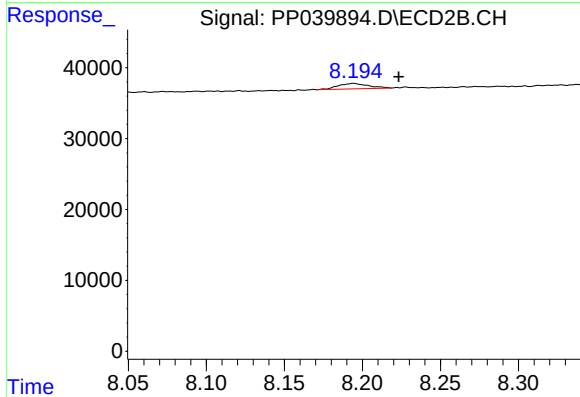


#38 AR-1262-3

R.T.: 8.194 min
Delta R.T.: -0.029 min
Response: 10121
Conc: 9.87 ng/ml

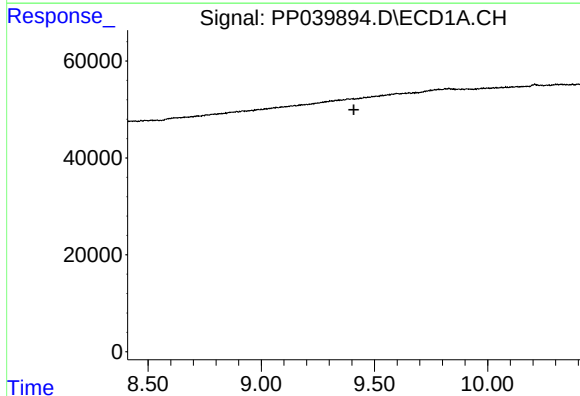


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.409 min
Response: 0
Conc: N.D.

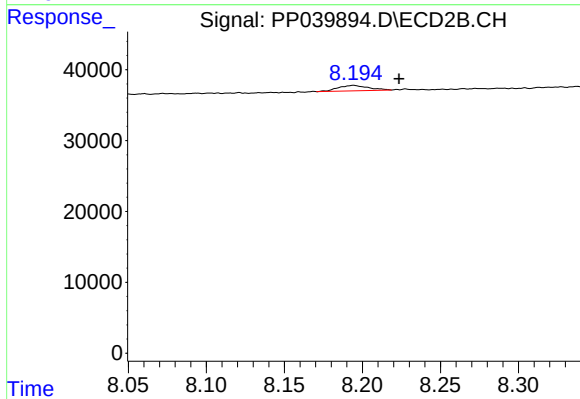

#41 AR-1268-1


R.T.: 8.194 min
Delta R.T.: -0.029 min
Response: 10121
Conc: 3.47 ng/ml

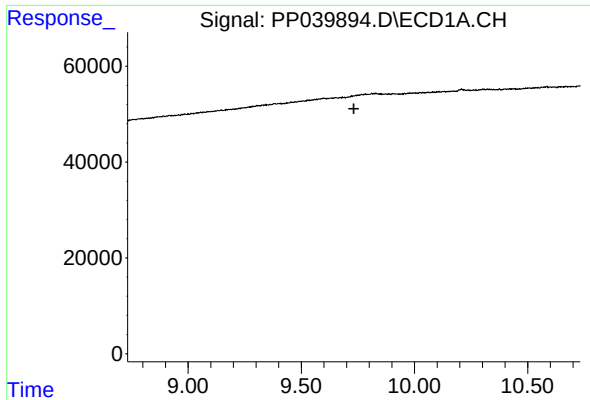

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

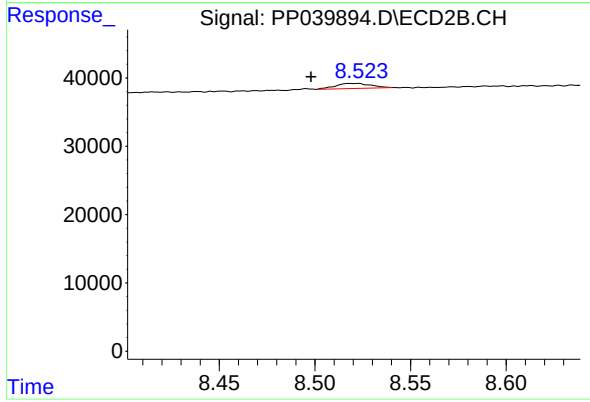

#43 AR-1268-3

R.T.: 8.523 min
Delta R.T.: 0.025 min
Response: 9600
Conc: 4.10 ng/ml