

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
 Data File : PP039896.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 10:27
 Operator : AJ\MA
 Sample : PB139721BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 12:59:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.896	3.984	587897	327123	19.310	19.569
2)	SA Decachlor...	10.918	9.316	447110	442228	19.888	19.714
Target Compounds							
10)	L2 AR-1221-3	0.000	4.424	0	14015	N.D.	26.175 #
11)	L3 AR-1232-1	0.000	4.424	0	14015	N.D.	35.000 #
32)	L7 AR-1260-2	8.150f	0.000	35038	0	21.842	N.D. #
33)	L7 AR-1260-3	0.000	7.209	0	27191	N.D.	20.507 #
38)	L8 AR-1262-3	0.000	8.195f	0	15974	N.D.	15.576 #
41)	L9 AR-1268-1	0.000	8.195f	0	15974	N.D.	5.470 #
43)	L9 AR-1268-3	0.000	8.521f	0	14523	N.D.	6.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
Data File : PP039896.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 10:27
Operator : AJ\MA
Sample : PB139721BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 12:59:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

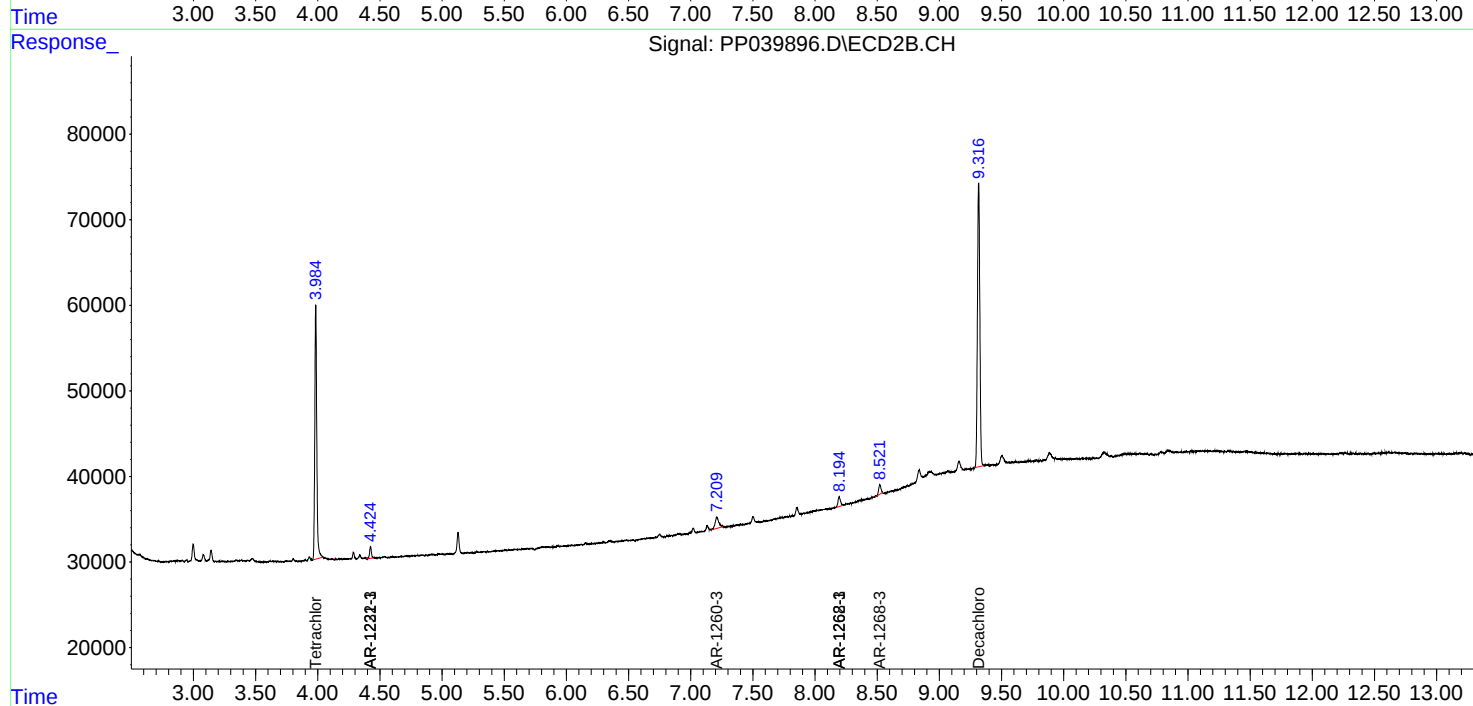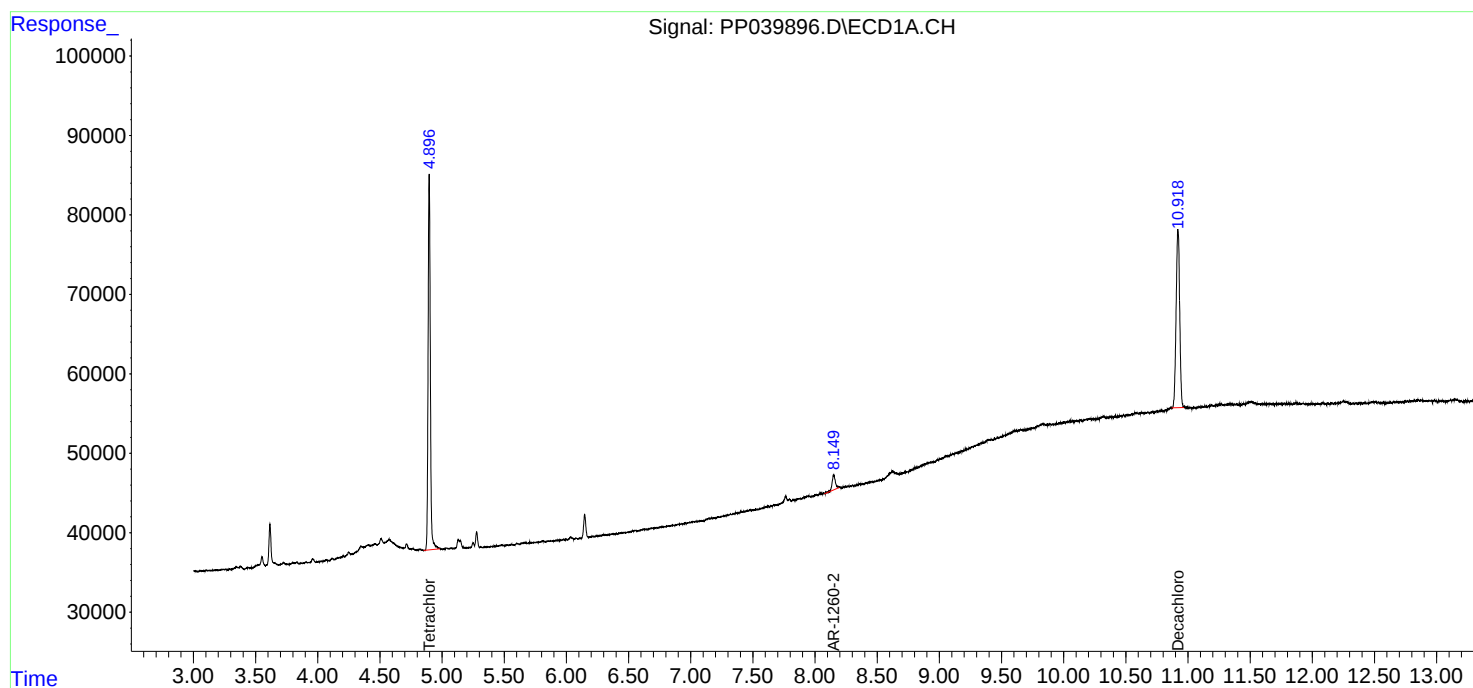


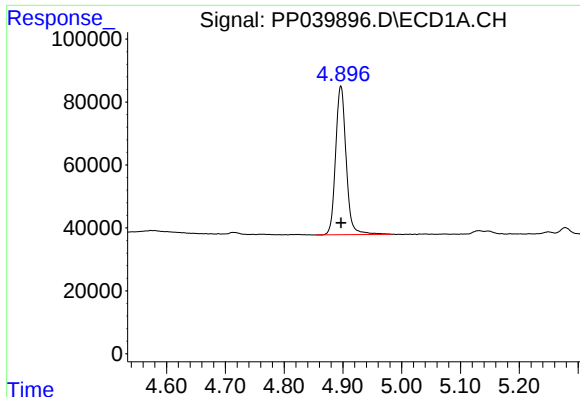

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 587897
Conc: 19.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

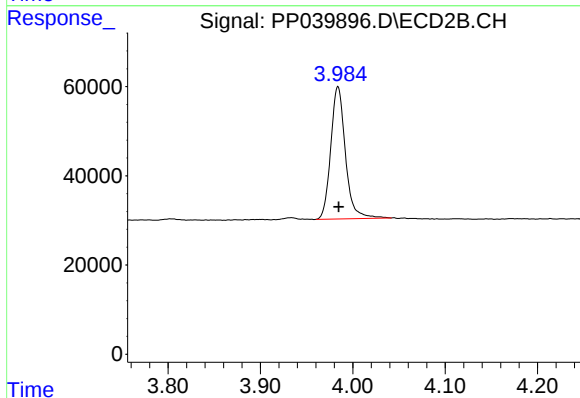


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 327123
Conc: 19.57 ng/ml

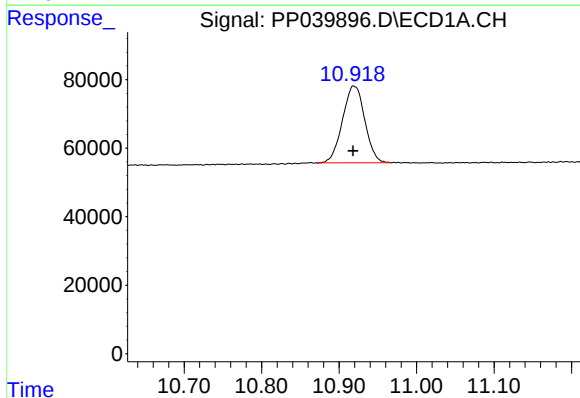


#2 Decachlorobiphenyl

R.T.: 10.918 min
Delta R.T.: 0.000 min
Response: 447110
Conc: 19.89 ng/ml

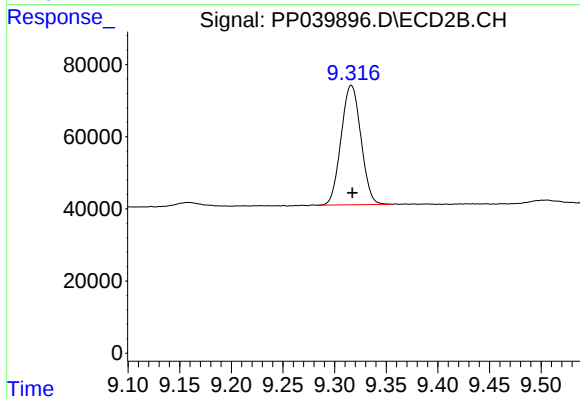

#2 Decachlorobiphenyl


R.T.: 9.316 min
Delta R.T.: 0.000 min
Response: 442228
Conc: 19.71 ng/ml

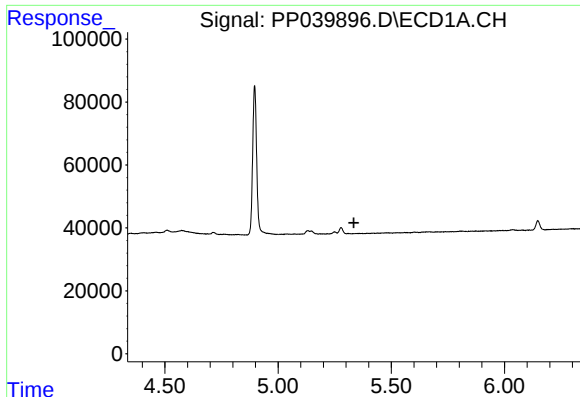

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

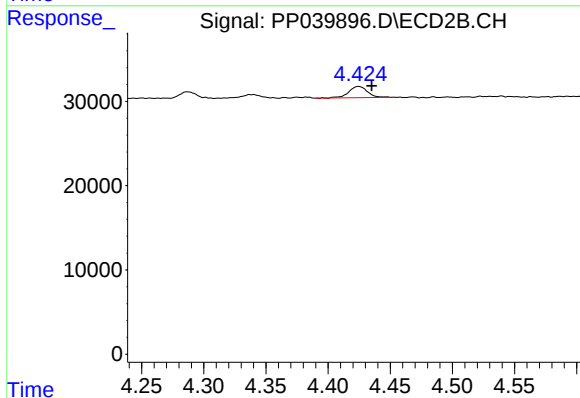


#10 AR-1221-3

R.T.: 4.424 min
Delta R.T.: -0.011 min
Response: 14015
Conc: 26.17 ng/ml

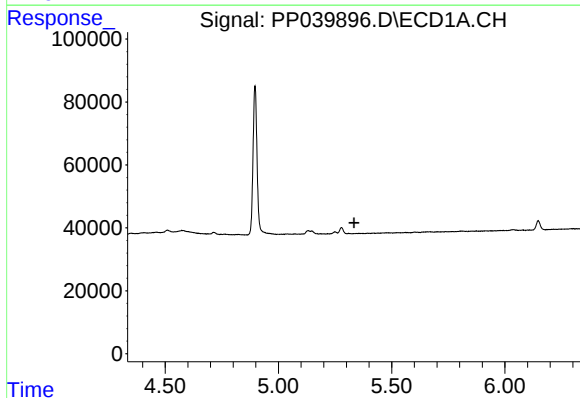


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.334 min
Response: 0
Conc: N.D.

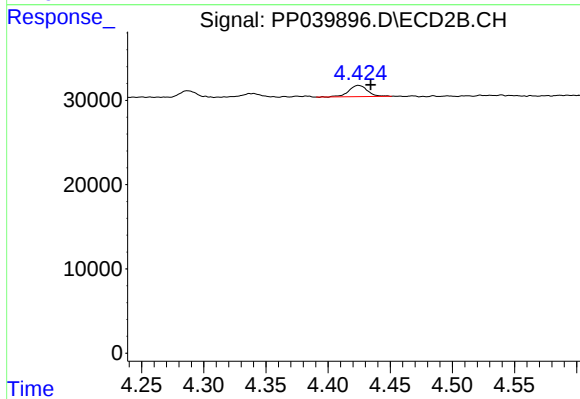

#11 AR-1232-1


R.T.: 4.424 min
Delta R.T.: -0.010 min
Response: 14015
Conc: 35.00 ng/ml

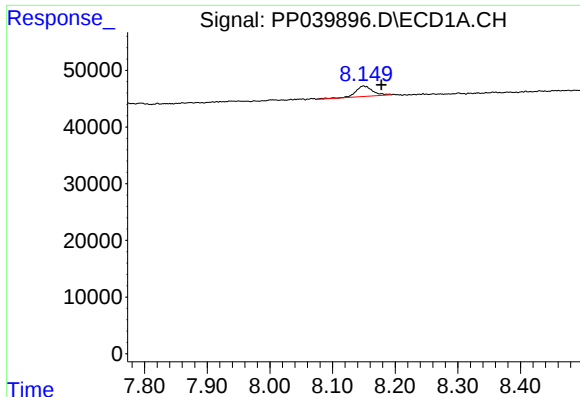

#32 AR-1260-2


R.T.: 8.150 min
Delta R.T.: -0.029 min
Response: 35038
Conc: 21.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

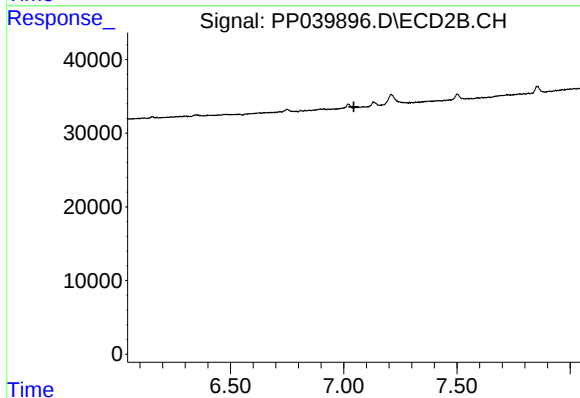


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

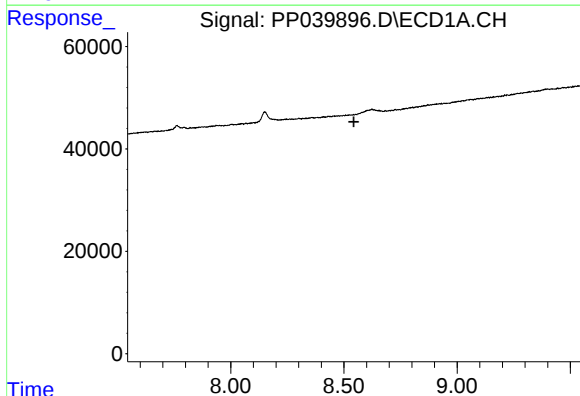


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.544 min
Response: 0
Conc: N.D.

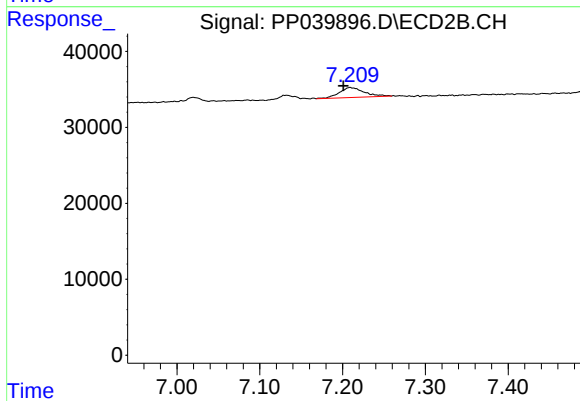

#33 AR-1260-3


R.T.: 7.209 min
Delta R.T.: 0.008 min
Response: 27191
Conc: 20.51 ng/ml

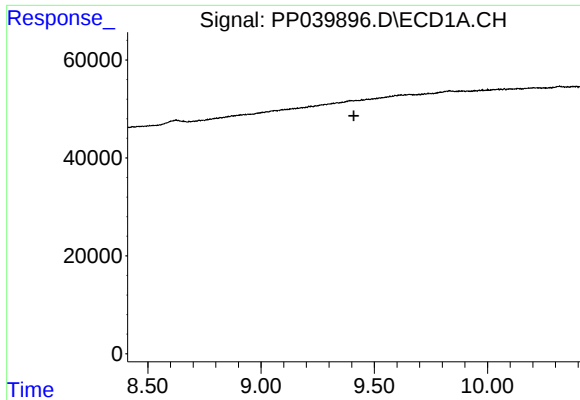

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

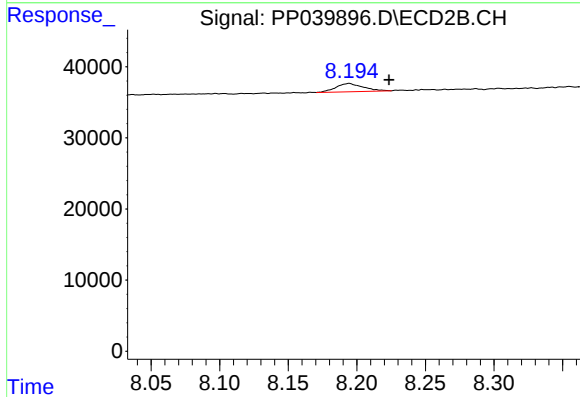


#38 AR-1262-3

R.T.: 8.195 min
Delta R.T.: -0.029 min
Response: 15974
Conc: 15.58 ng/ml

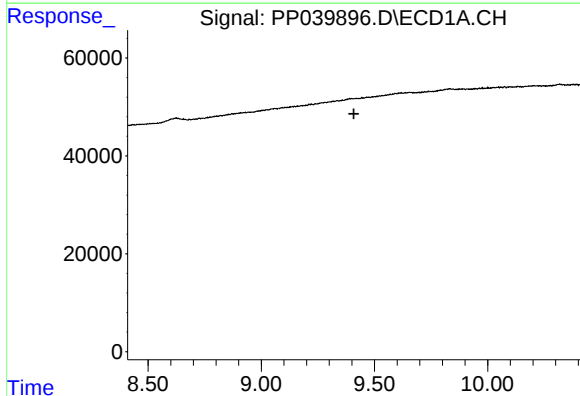


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.409 min
Response: 0
Conc: N.D.

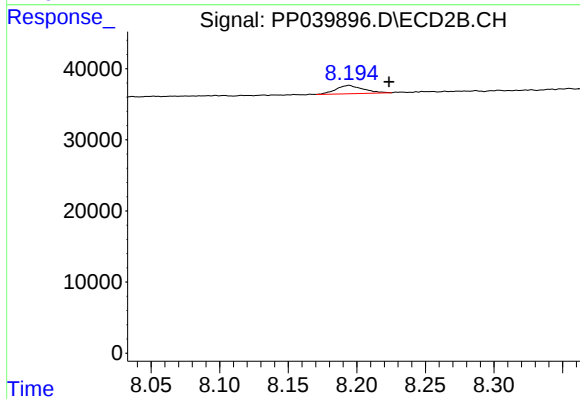

#41 AR-1268-1


R.T.: 8.195 min
Delta R.T.: -0.029 min
Response: 15974
Conc: 5.47 ng/ml

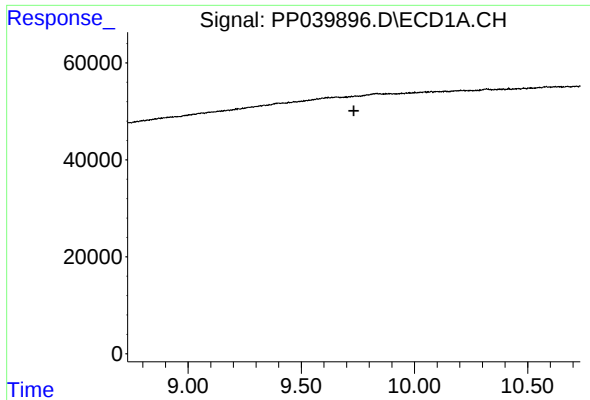

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

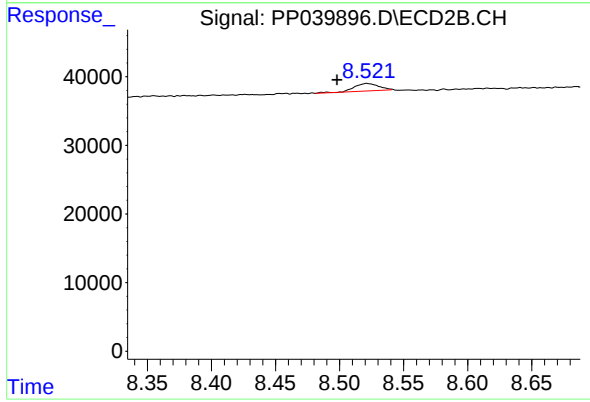

#43 AR-1268-3

R.T.: 8.521 min
Delta R.T.: 0.023 min
Response: 14523
Conc: 6.20 ng/ml