

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
 Data File : PP039932.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 21:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:02:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.897	3.984	620854	356044	20.393	21.299
2)	SA Decachlor...	10.917	9.315	525133	504354	23.359	22.483
Target Compounds							
10)	L2 AR-1221-3	0.000	4.425	0	9350	N.D.	17.462 #
11)	L3 AR-1232-1	0.000	4.425	0	9350	N.D.	23.350 #
20)	L4 AR-1242-5	0.000	6.153f	0	14073	N.D.	28.309 #
25)	L5 AR-1248-5	0.000	6.153f	0	14073	N.D.	21.939 #
26)	L6 AR-1254-1	0.000	6.153f	0	14073	N.D.	14.280 #
28)	L6 AR-1254-3	7.762f	0.000	76143	0	44.909	N.D. #
32)	L7 AR-1260-2	8.149f	7.020f	48713	50568	30.367	40.018 #
33)	L7 AR-1260-3	0.000	7.203	0	44194	N.D.	33.331 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
Data File : PP039932.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 21:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:02:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

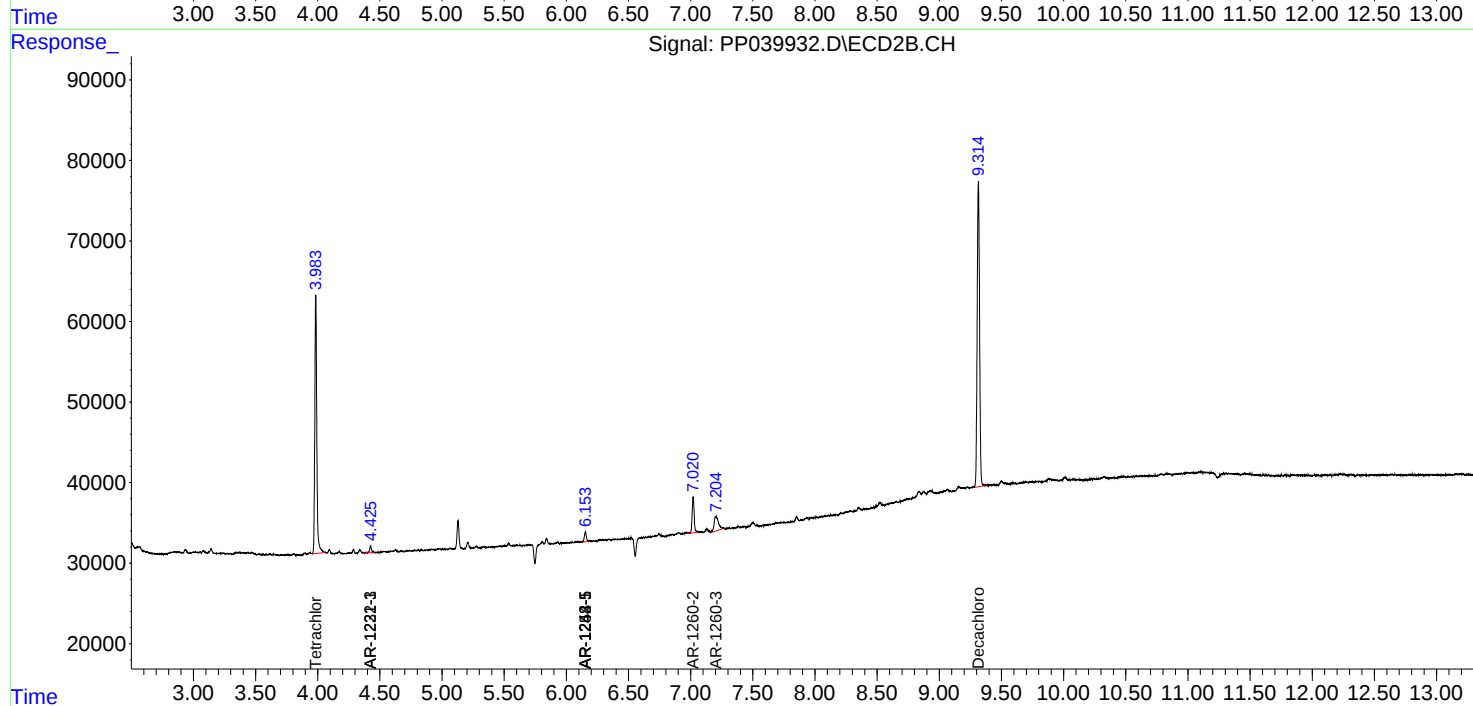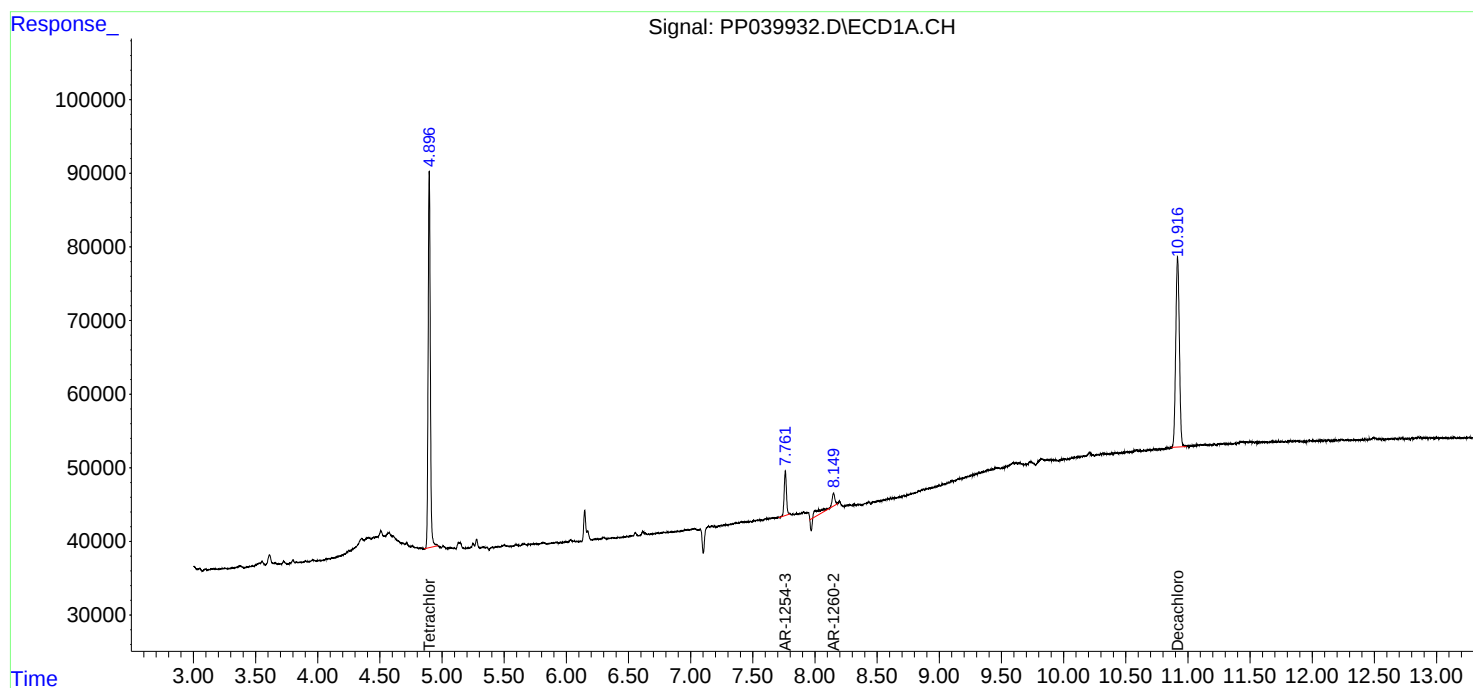


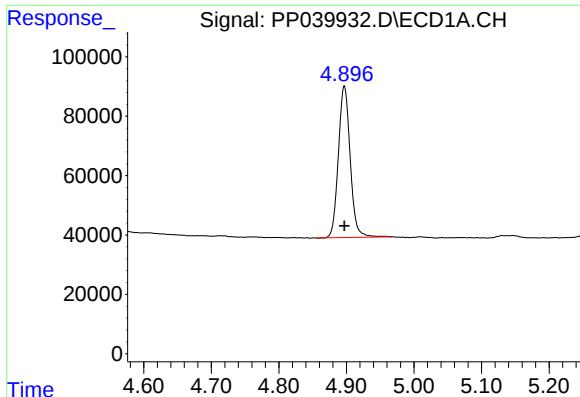

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 620854
Conc: 20.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

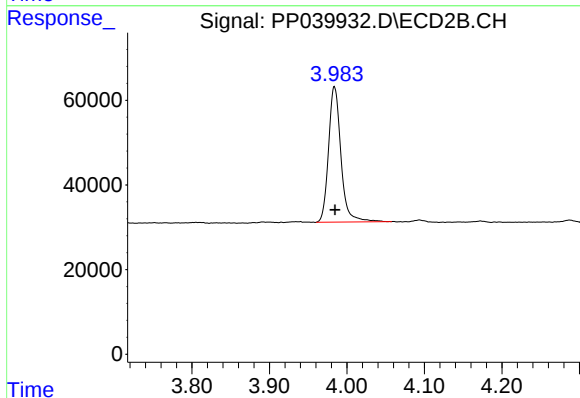


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 356044
Conc: 21.30 ng/ml

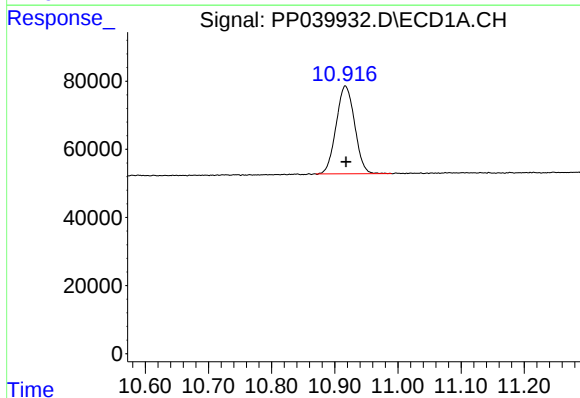


#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: -0.001 min
Response: 525133
Conc: 23.36 ng/ml

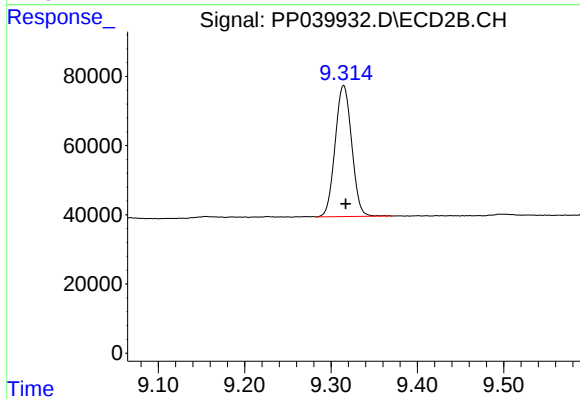

#2 Decachlorobiphenyl


R.T.: 9.315 min
Delta R.T.: -0.003 min
Response: 504354
Conc: 22.48 ng/ml

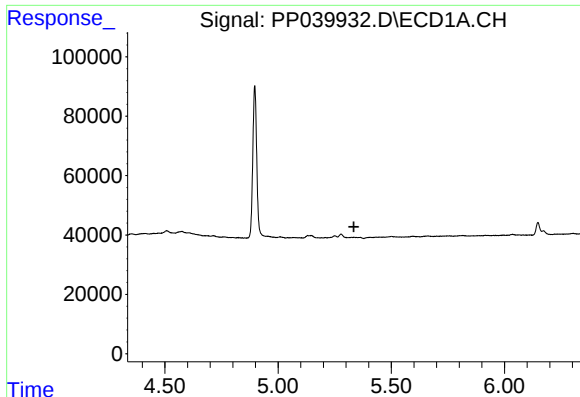

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

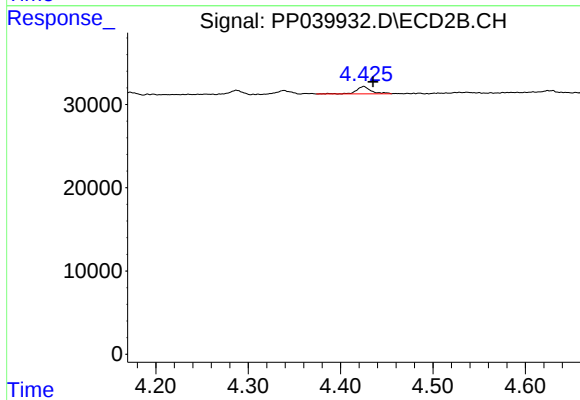


#10 AR-1221-3

R.T.: 4.425 min
Delta R.T.: -0.010 min
Response: 9350
Conc: 17.46 ng/ml

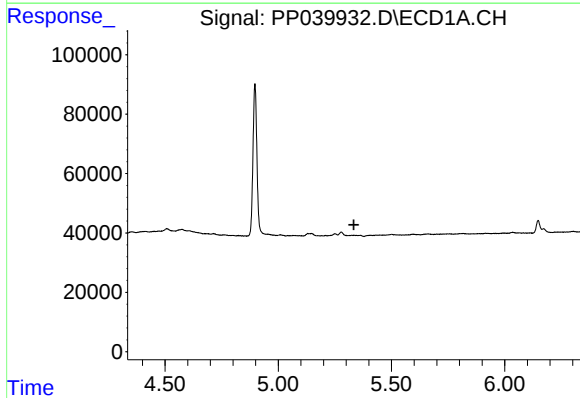


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.334 min
Response: 0
Conc: N.D.

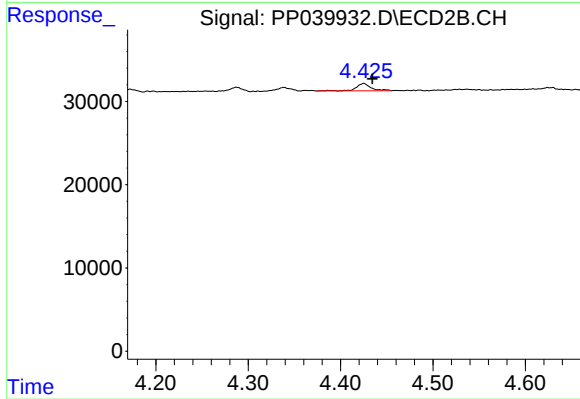

#11 AR-1232-1


R.T.: 4.425 min
Delta R.T.: -0.009 min
Response: 9350
Conc: 23.35 ng/ml

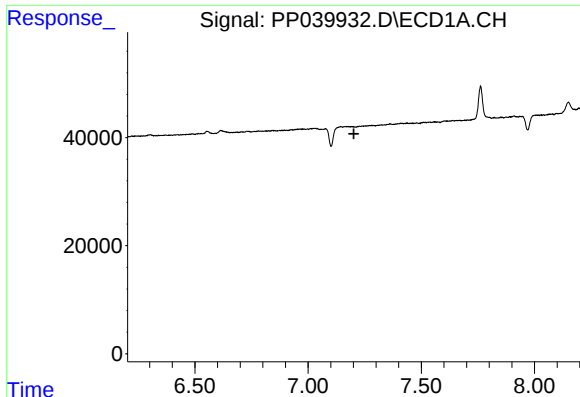

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

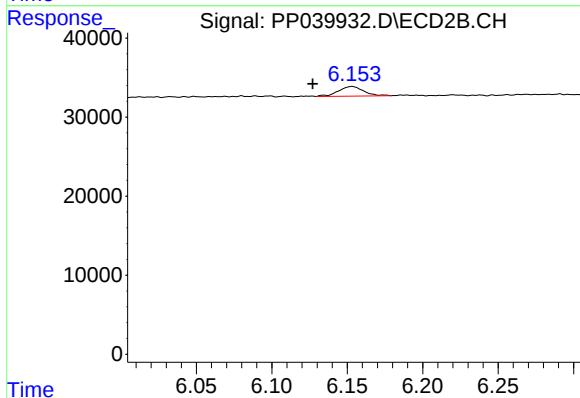


#20 AR-1242-5

R.T.: 6.153 min
Delta R.T.: 0.026 min
Response: 14073
Conc: 28.31 ng/ml

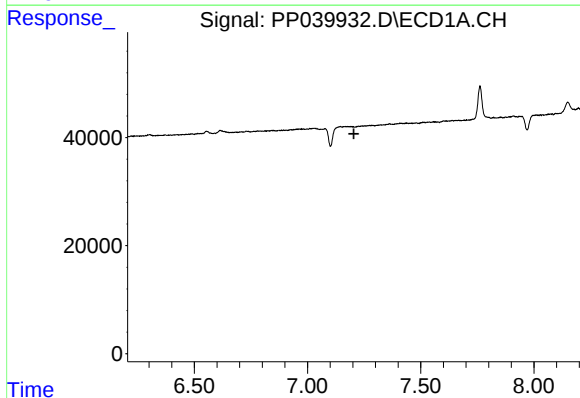


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.205 min
Response: 0
Conc: N.D.

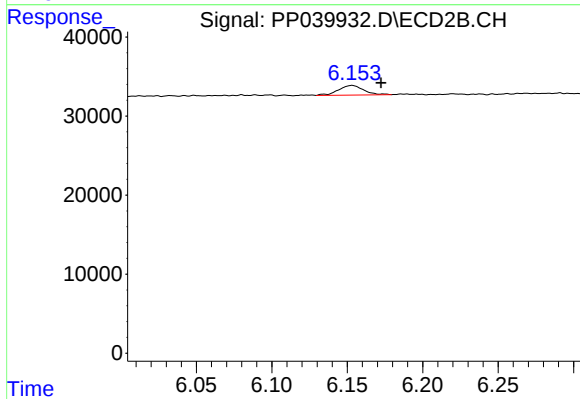

#25 AR-1248-5


R.T.: 6.153 min
Delta R.T.: -0.019 min
Response: 14073
Conc: 21.94 ng/ml

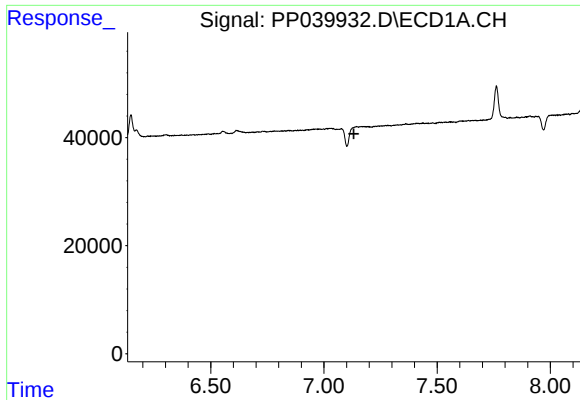

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

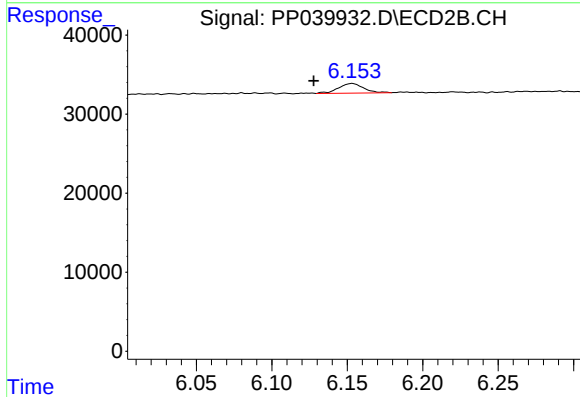


#26 AR-1254-1

R.T.: 6.153 min
Delta R.T.: 0.025 min
Response: 14073
Conc: 14.28 ng/ml

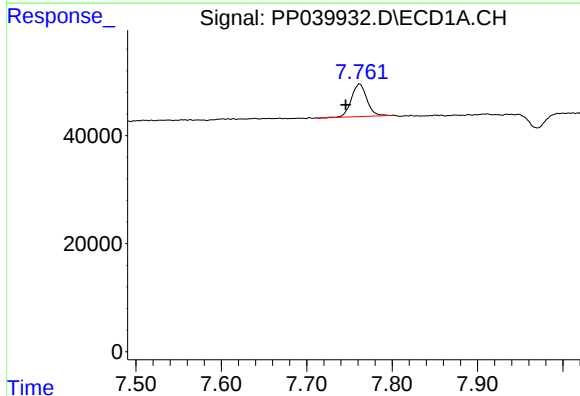


#28 AR-1254-3

R.T.: 7.762 min
Delta R.T.: 0.016 min
Response: 76143
Conc: 44.91 ng/ml

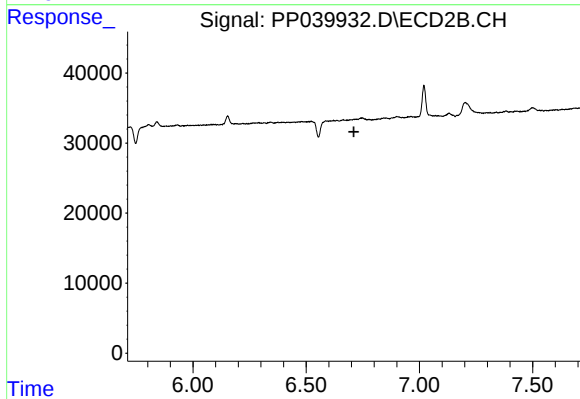

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.711 min
Response: 0
Conc: N.D.

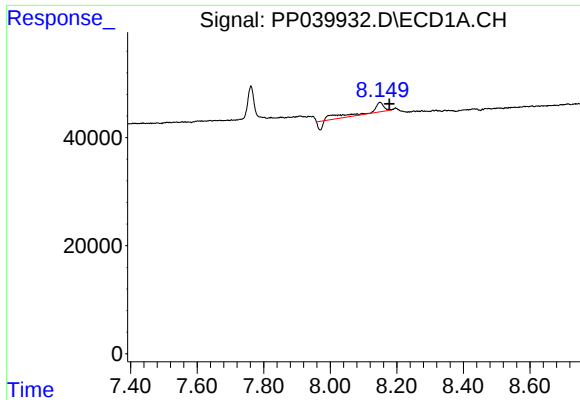

#32 AR-1260-2


R.T.: 8.149 min
Delta R.T.: -0.029 min
Response: 48713
Conc: 30.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

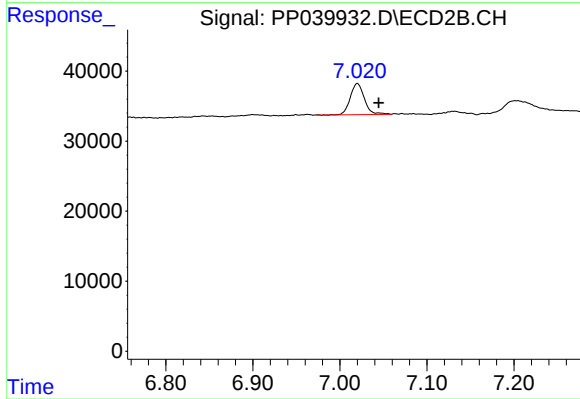


#32 AR-1260-2

R.T.: 7.020 min
Delta R.T.: -0.025 min
Response: 50568
Conc: 40.02 ng/ml

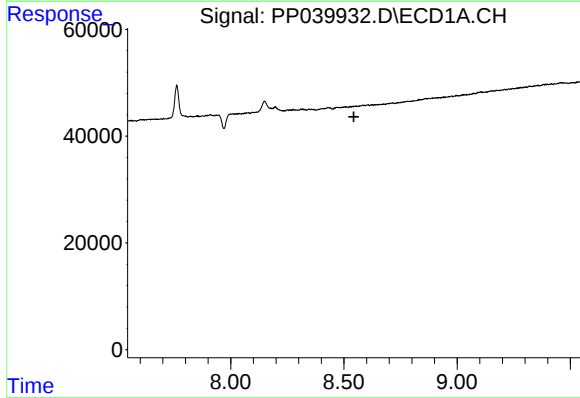

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.544 min
Response: 0
Conc: N.D.

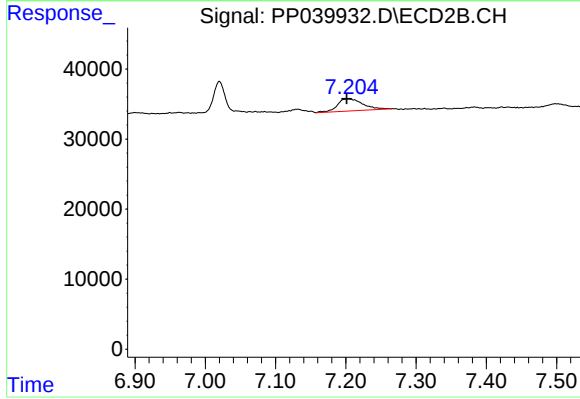

#33 AR-1260-3

R.T.: 7.203 min
Delta R.T.: 0.002 min
Response: 44194
Conc: 33.33 ng/ml