

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
 Data File : PP039939.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2021 00:02
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:07:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.899	3.985	657065	373346	21.582	22.334
2)	SA Decachlor...	10.921	9.317	536872	517809	23.881	23.083
Target Compounds							
10)	L2 AR-1221-3	0.000	4.426	0	8724	N.D.	16.294 #
11)	L3 AR-1232-1	0.000	4.426	0	8724	N.D.	21.788 #
20)	L4 AR-1242-5	0.000	6.155f	0	32093	N.D.	64.557 #
25)	L5 AR-1248-5	0.000	6.155f	0	32093	N.D.	50.031 #
26)	L6 AR-1254-1	7.144	6.155f	-8961	32093	N.D.	32.564 #
28)	L6 AR-1254-3	7.763f	0.000	77225	0	45.546	N.D. #
32)	L7 AR-1260-2	8.199f	7.022f	14376	47870	8.962	37.883 #
33)	L7 AR-1260-3	0.000	7.201	0	43454	N.D.	32.772 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
Data File : PP039939.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2021 00:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:07:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

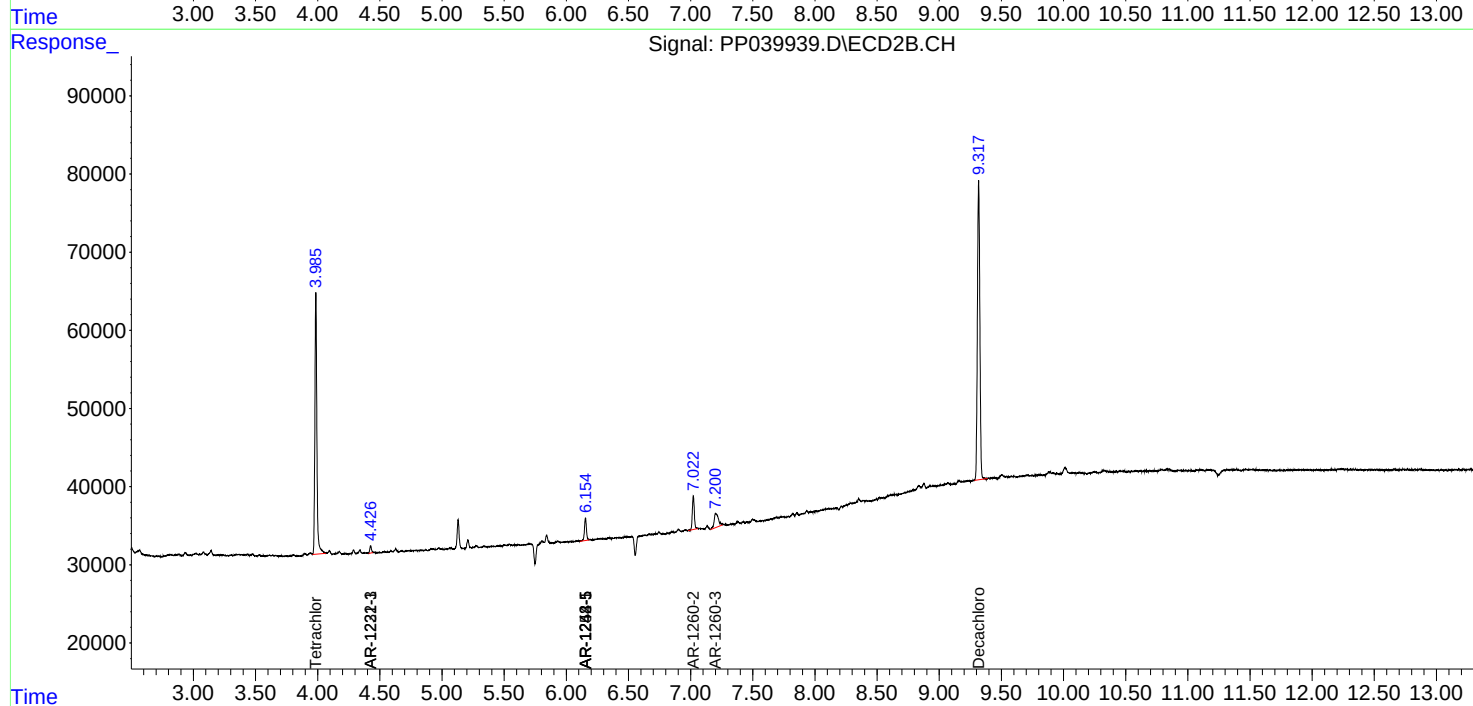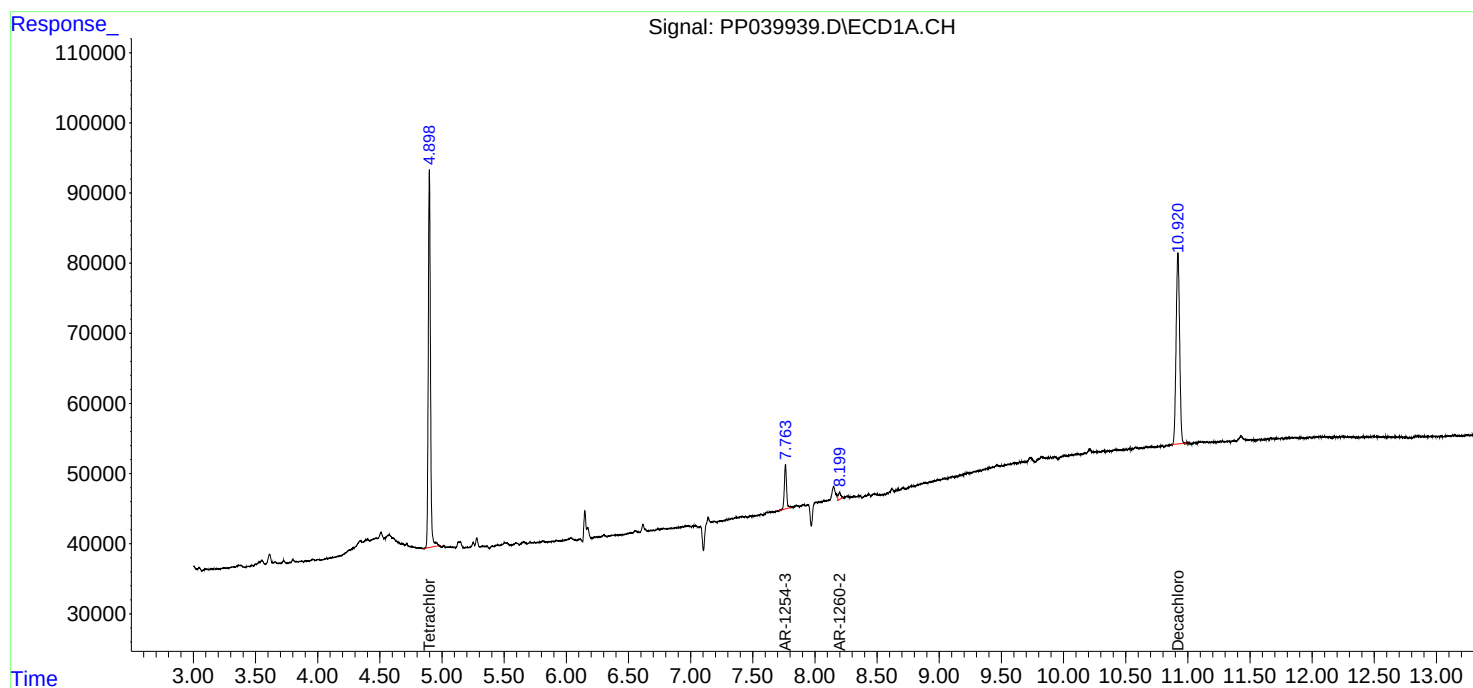


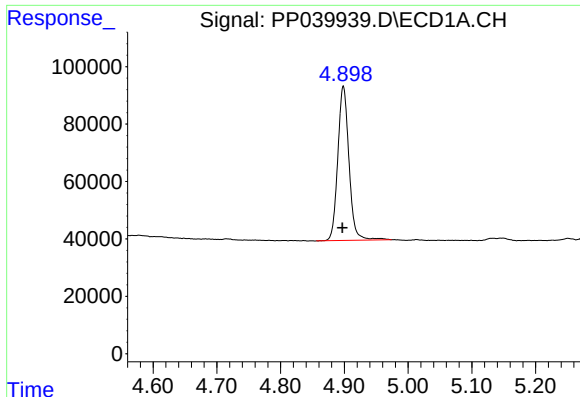

#1 Tetrachloro-m-xylene


R.T.: 4.899 min
Delta R.T.: 0.002 min
Response: 657065
Conc: 21.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

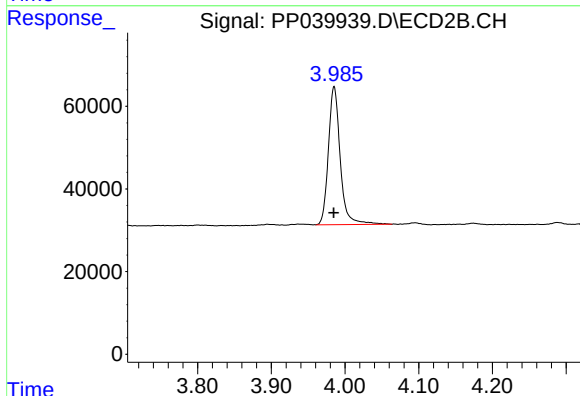


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 373346
Conc: 22.33 ng/ml

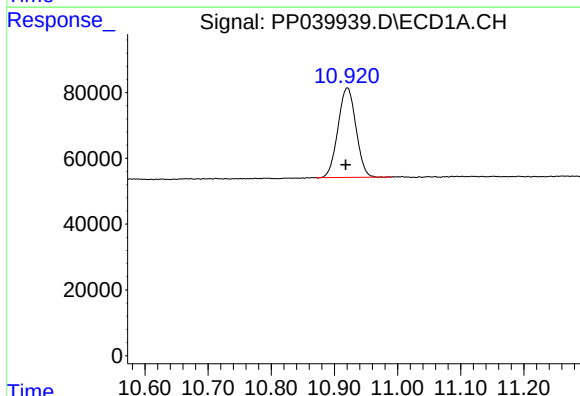


#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: 0.003 min
Response: 536872
Conc: 23.88 ng/ml

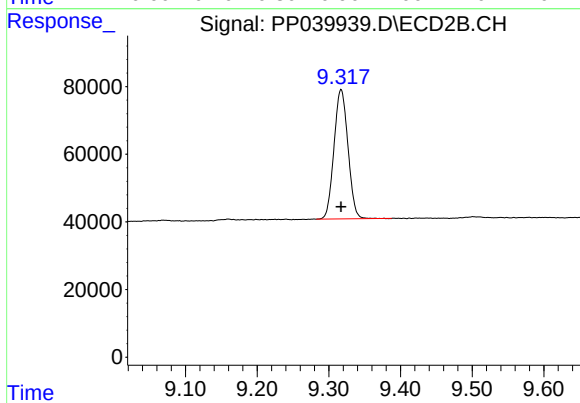

#2 Decachlorobiphenyl


R.T.: 9.317 min
Delta R.T.: 0.000 min
Response: 517809
Conc: 23.08 ng/ml

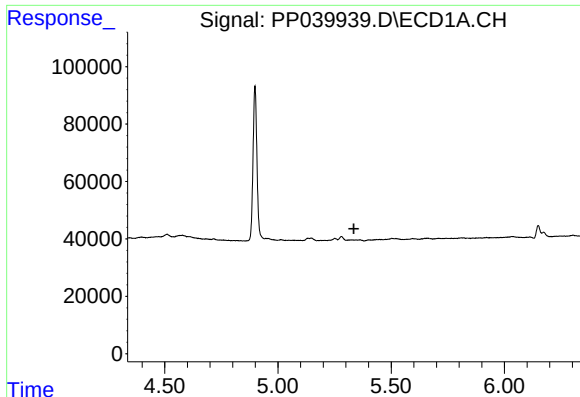

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

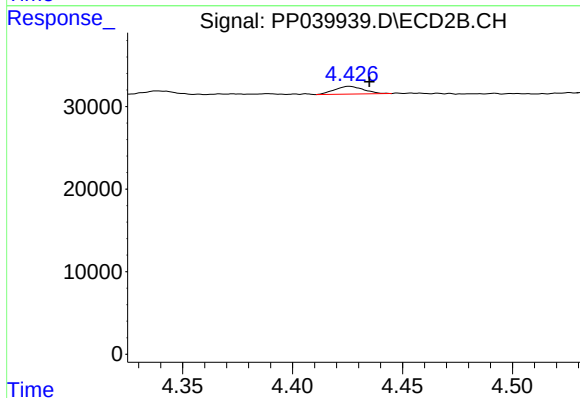


#10 AR-1221-3

R.T.: 4.426 min
Delta R.T.: -0.009 min
Response: 8724
Conc: 16.29 ng/ml

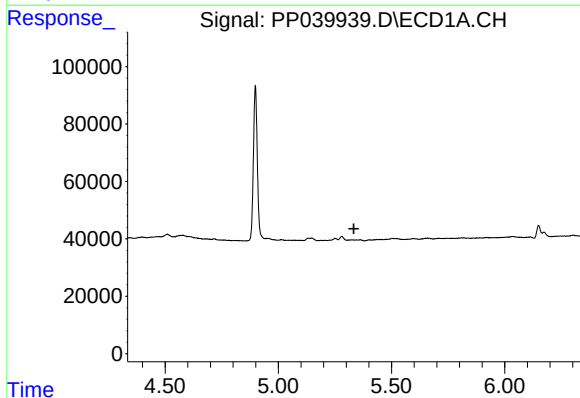


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.334 min
Response: 0
Conc: N.D.

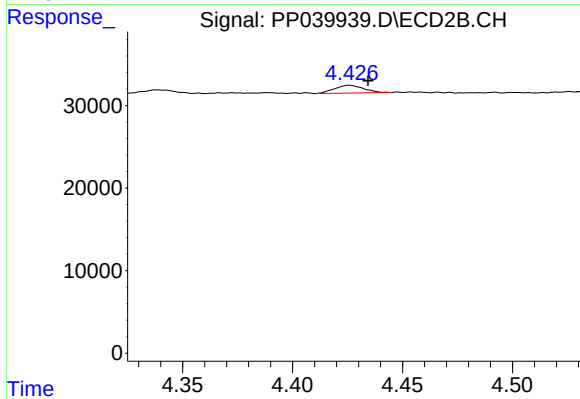

#11 AR-1232-1


R.T.: 4.426 min
Delta R.T.: -0.008 min
Response: 8724
Conc: 21.79 ng/ml

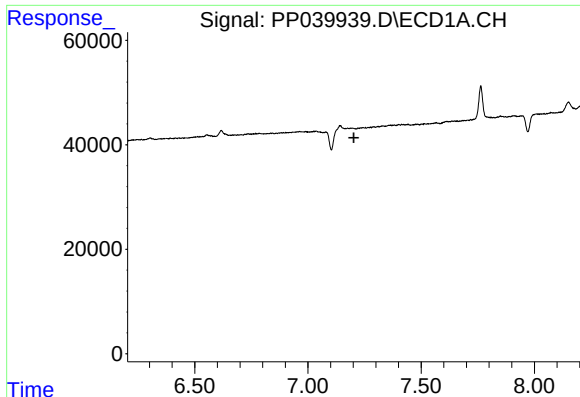

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

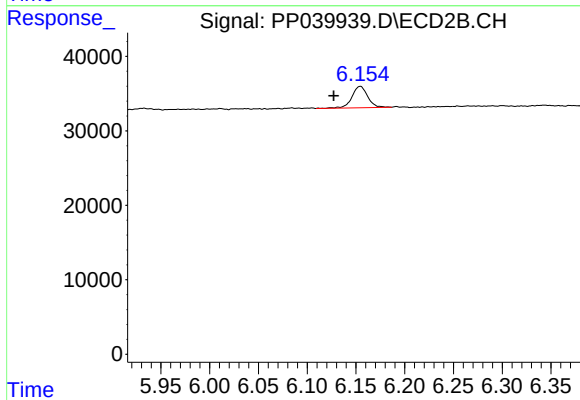


#20 AR-1242-5

R.T.: 6.155 min
Delta R.T.: 0.027 min
Response: 32093
Conc: 64.56 ng/ml

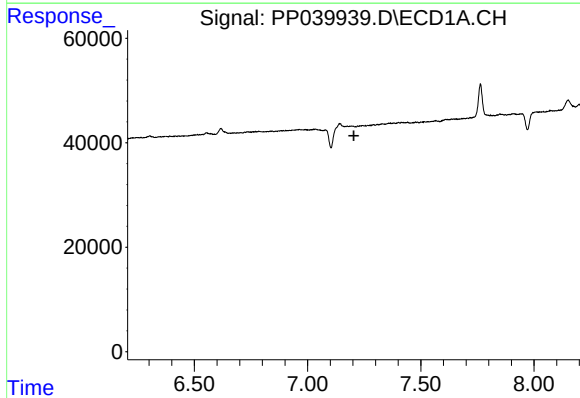


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.205 min
Response: 0
Conc: N.D.

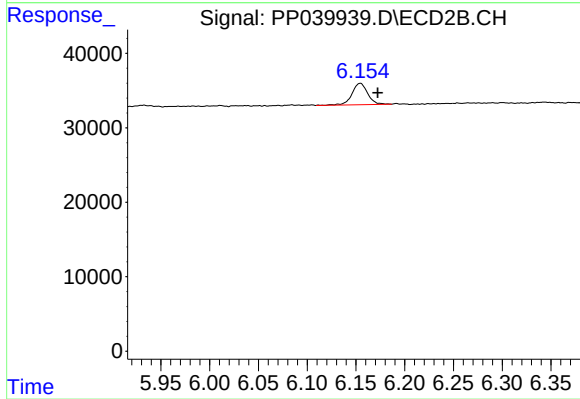

#25 AR-1248-5


R.T.: 6.155 min
Delta R.T.: -0.018 min
Response: 32093
Conc: 50.03 ng/ml

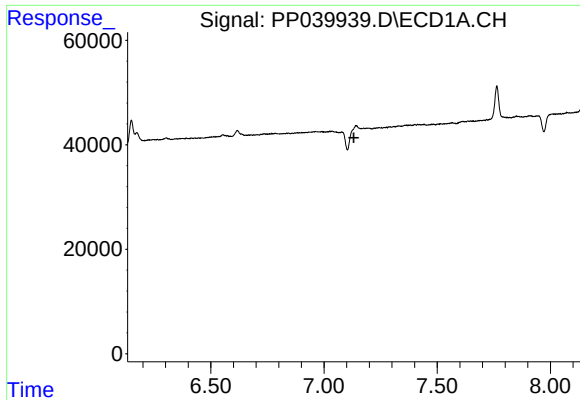

#26 AR-1254-1


R.T.: 7.144 min
Delta R.T.: 0.012 min
Response: -8961
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

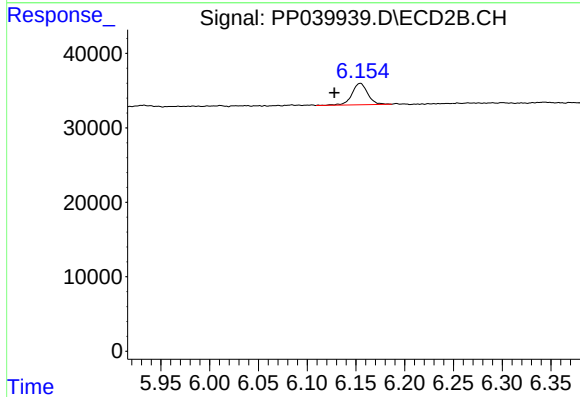


#26 AR-1254-1

R.T.: 6.155 min
Delta R.T.: 0.027 min
Response: 32093
Conc: 32.56 ng/ml

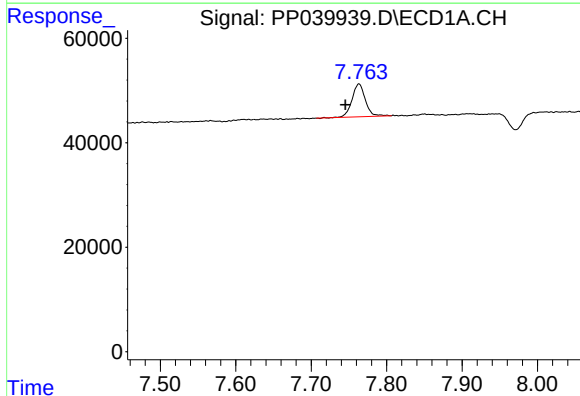


#28 AR-1254-3

R.T.: 7.763 min
Delta R.T.: 0.018 min
Response: 77225
Conc: 45.55 ng/ml

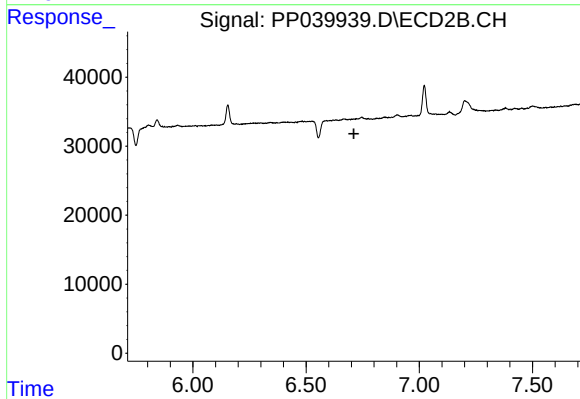

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.711 min
Response: 0
Conc: N.D.

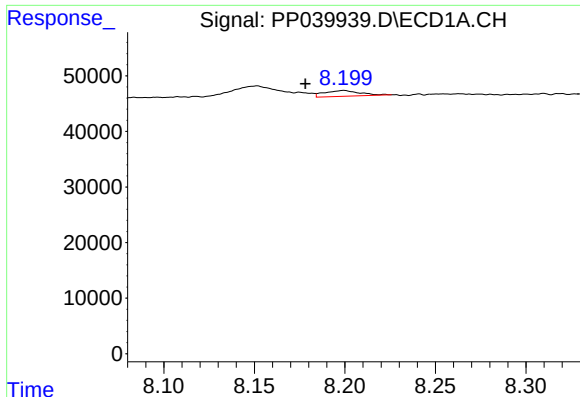

#32 AR-1260-2


R.T.: 8.199 min
Delta R.T.: 0.021 min
Response: 14376
Conc: 8.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

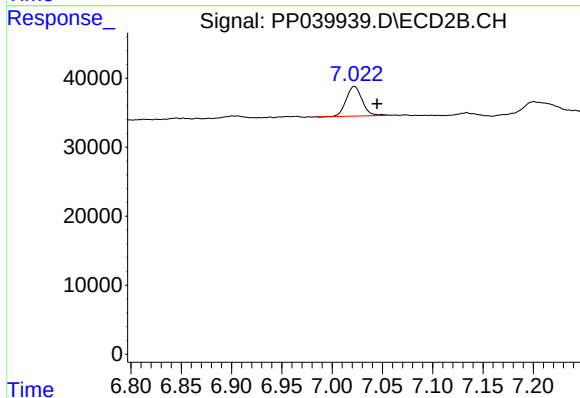


#32 AR-1260-2

R.T.: 7.022 min
Delta R.T.: -0.023 min
Response: 47870
Conc: 37.88 ng/ml

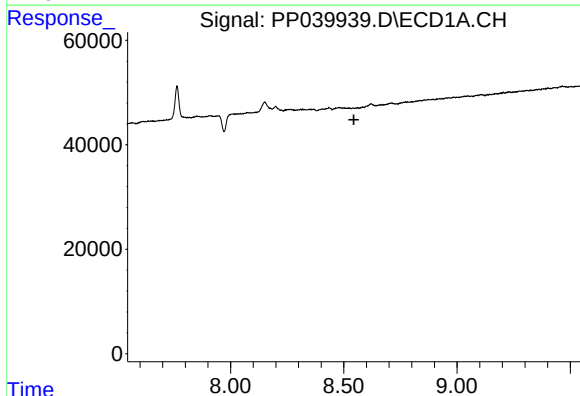

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.544 min
Response: 0
Conc: N.D.

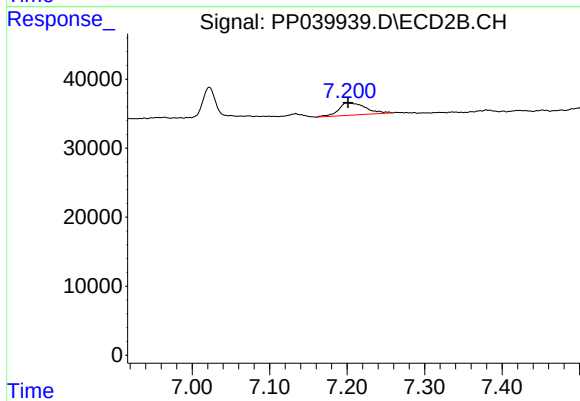

#33 AR-1260-3

R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 43454
Conc: 32.77 ng/ml