

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
 Data File : PP039914.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 15:34
 Operator : AJ\MA
 Sample : M3990-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-836-K1-SO-9-10-092921

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 17:47:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.985	654169	379629	21.487	22.710
2) SA Decachlor...	10.921	9.317	449903	435084	20.012	19.395

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
Data File : PP039914.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 15:34
Operator : AJ\MA
Sample : M3990-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S-836-K1-SO-9-10-092921

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 17:47:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

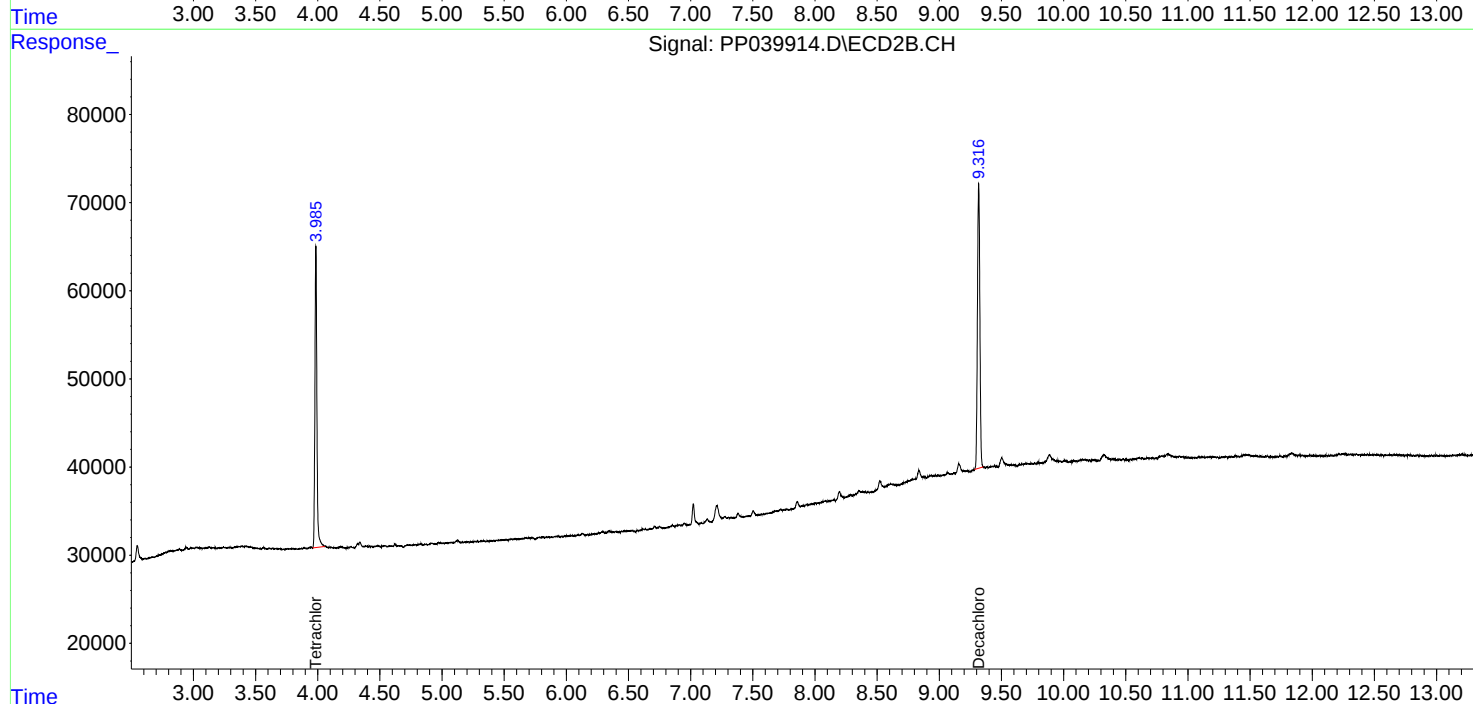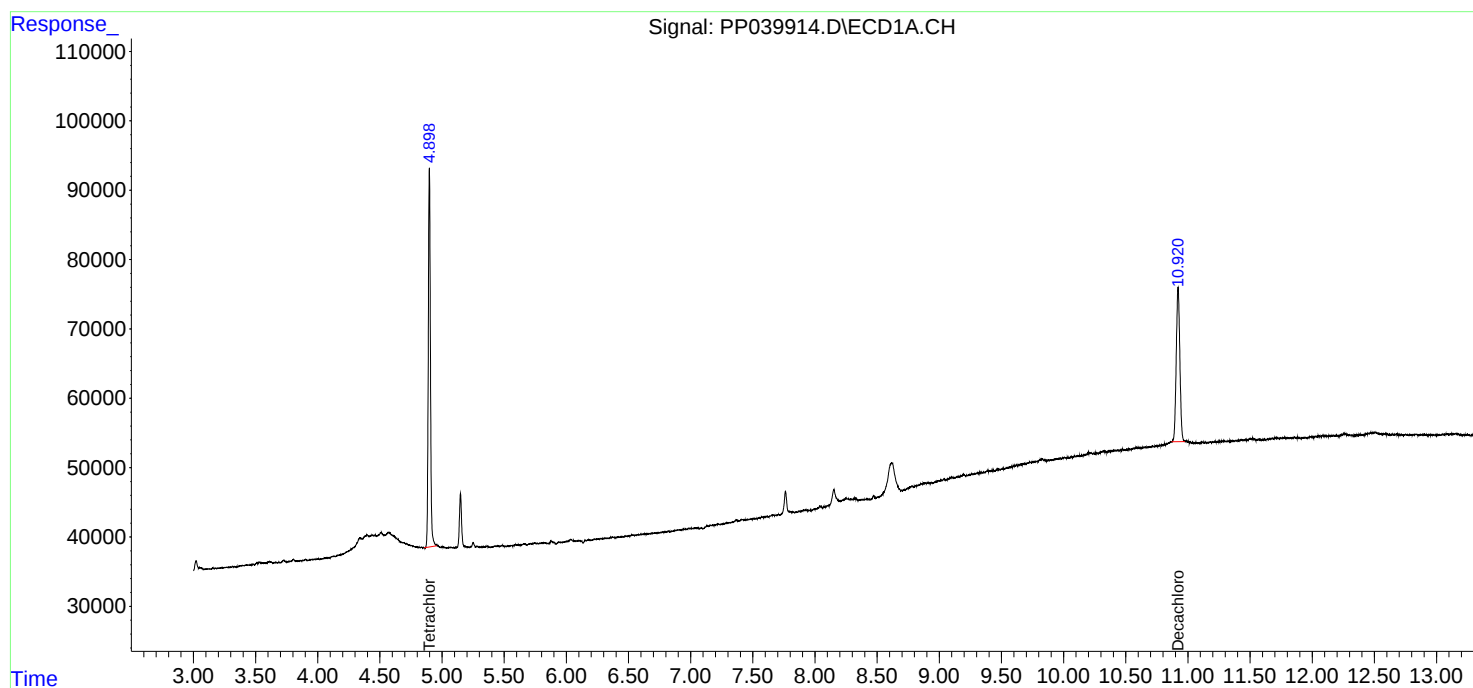


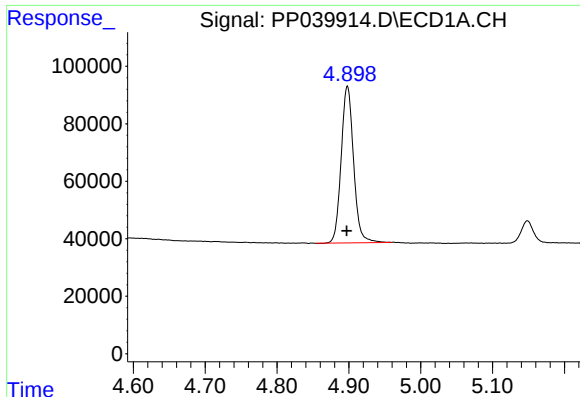

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 654169
Conc: 21.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-836-K1-SO-9-10-092921

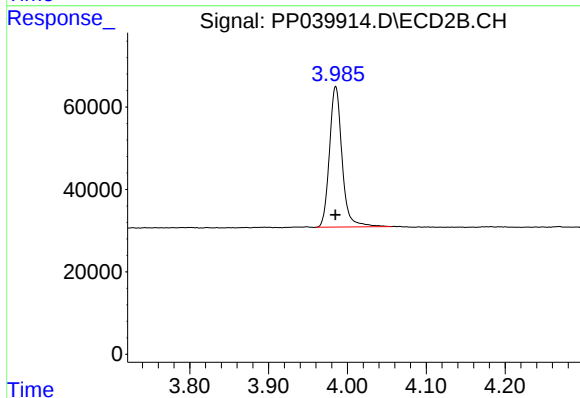


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 379629
Conc: 22.71 ng/ml

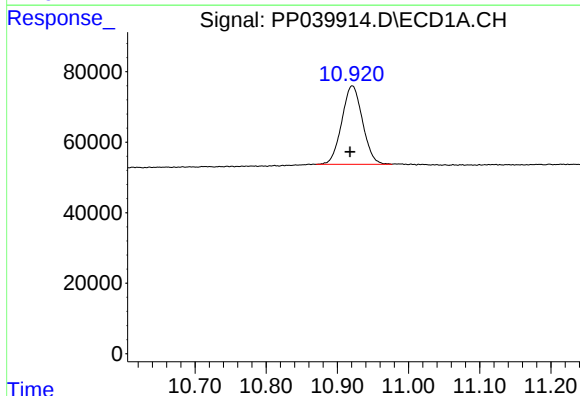

#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: 0.003 min
Response: 449903
Conc: 20.01 ng/ml

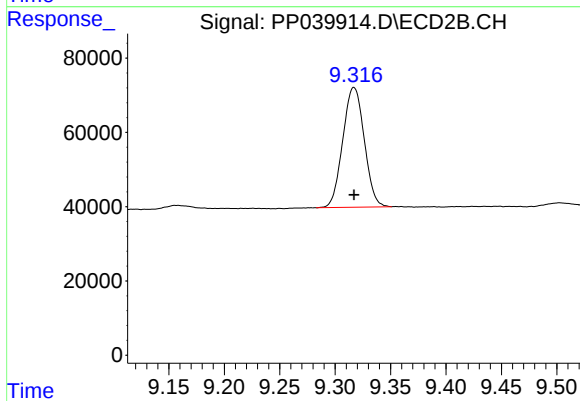

#2 Decachlorobiphenyl

R.T.: 9.317 min
Delta R.T.: 0.000 min
Response: 435084
Conc: 19.40 ng/ml