

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
 Data File : PP039916.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Oct 2021 16:07
 Operator : AJ\MA
 Sample : M4020-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-844-R-SO-4-4.5-093021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 17:47:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.984	654197	379365	21.488	22.694
2) SA Decachlor...	10.920	9.316	464931	456527	20.681	20.351

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100821\
Data File : PP039916.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Oct 2021 16:07
Operator : AJ\MA
Sample : M4020-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S-844-R-SO-4-4.5-093021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 17:47:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

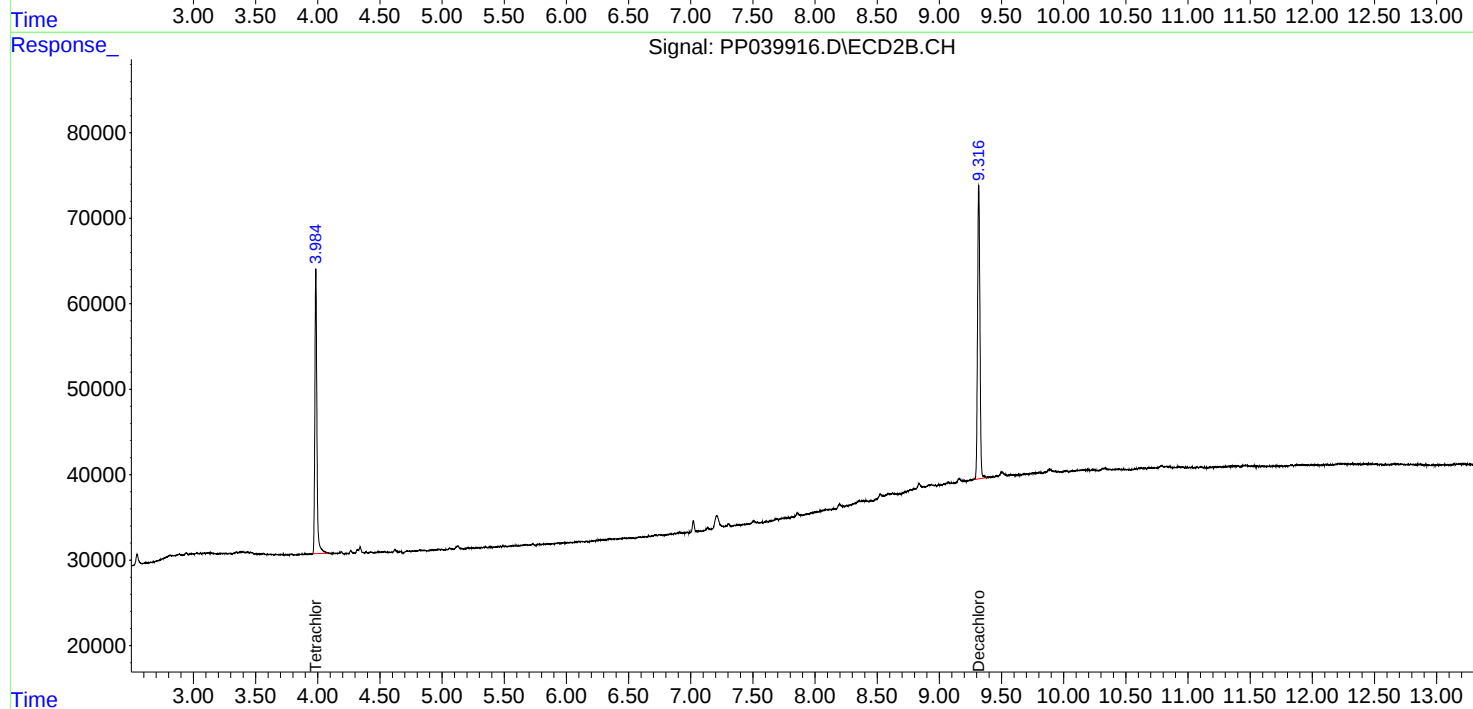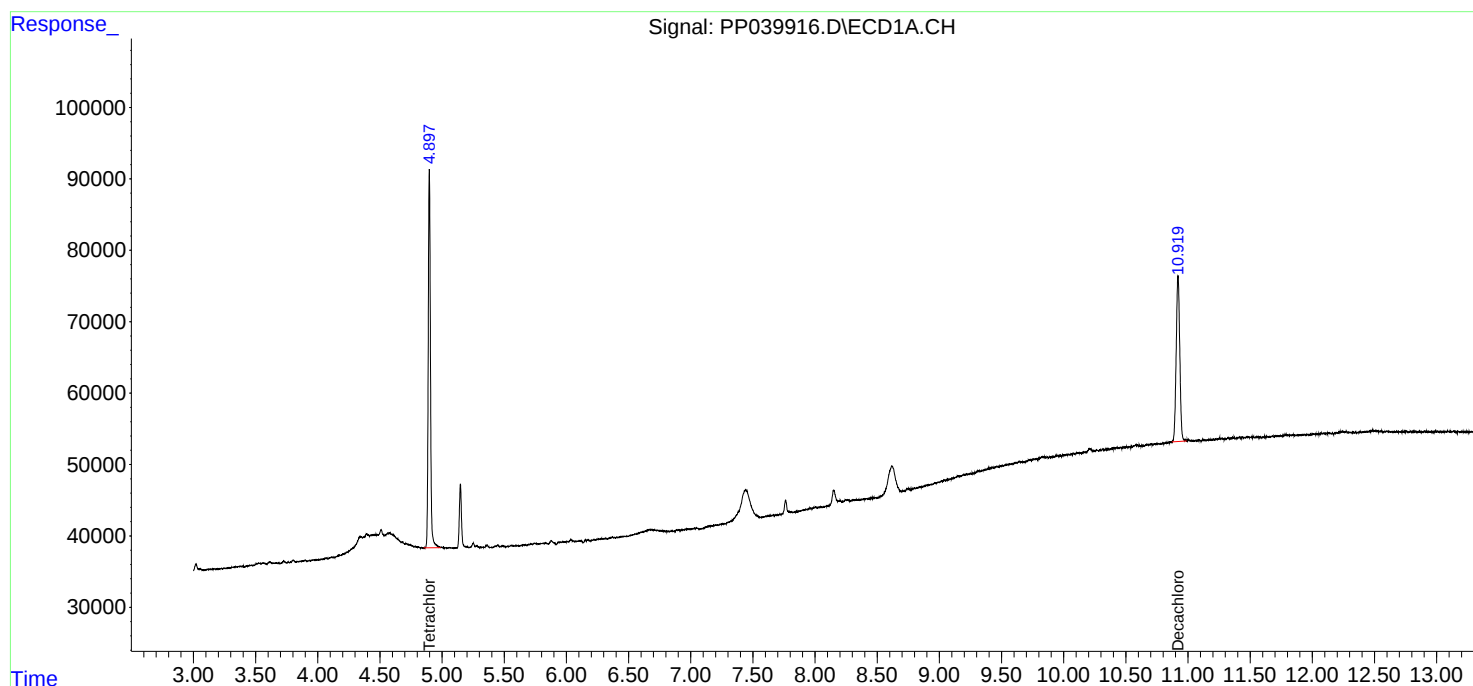


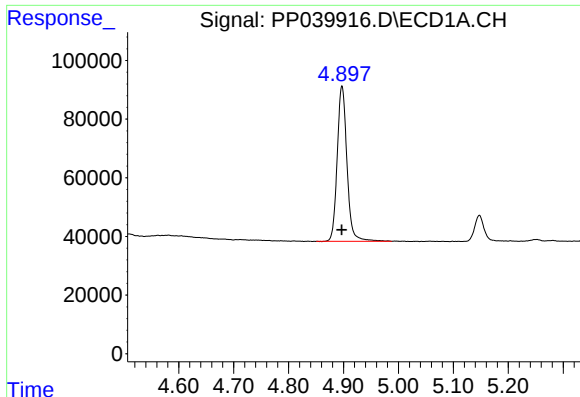

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 654197
Conc: 21.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-844-R-SO-4-4.5-093021

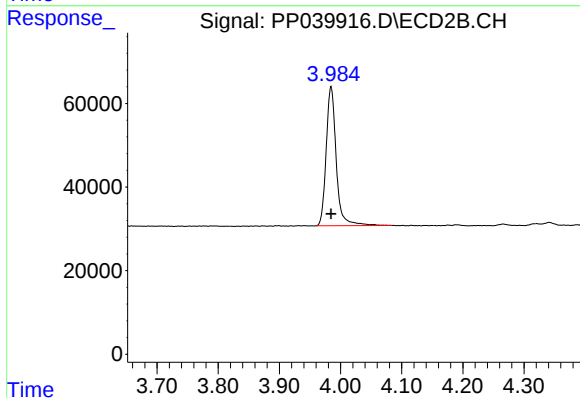


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 379365
Conc: 22.69 ng/ml

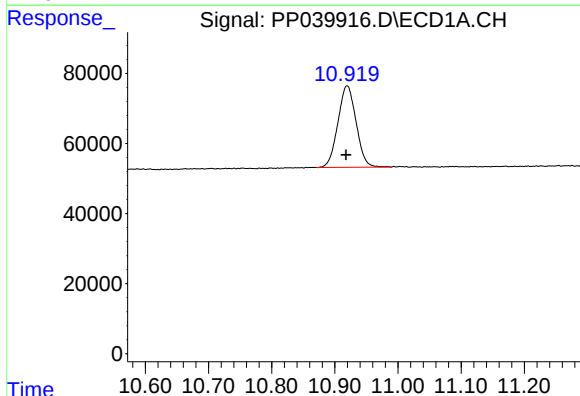

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: 0.002 min
Response: 464931
Conc: 20.68 ng/ml

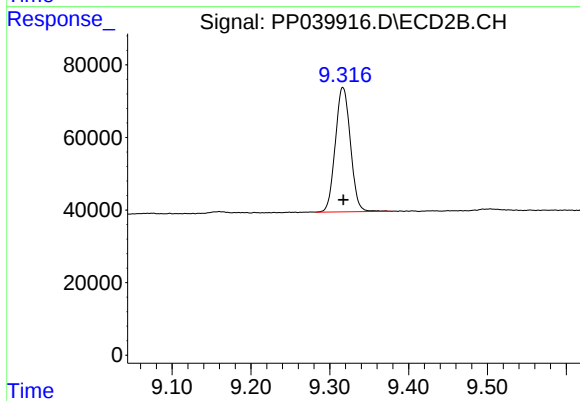

#2 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: 0.000 min
Response: 456527
Conc: 20.35 ng/ml