

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100923\
 Data File : PP060776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2023 20:17
 Operator : YP\AJ
 Sample : 04699-07
 Misc : AR1242 LOD 25 PPB
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 23:53:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.531	3.683	41708239	29118862	18.624	19.562
2) SA Decachlor...	10.460	8.747	35767513	29056704	20.259	17.813
Target Compounds						
16) L4 AR-1242-1	5.719	4.779	1518140	1162622	23.755	22.964
17) L4 AR-1242-2	5.742	4.799	2030562	1512293	22.426	21.777
18) L4 AR-1242-3	5.805	4.976	1298636	803589	23.066	20.867
19) L4 AR-1242-4	5.905	5.060	1120666	842251	23.994	21.386
20) L4 AR-1242-5	6.651	5.588	1144681	1021846	22.759	20.889



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100923\
Data File : PP060776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:17
Operator : YP\AJ
Sample : 04699-07
Misc : AR1242 LOD 25 PPB
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 23:53:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

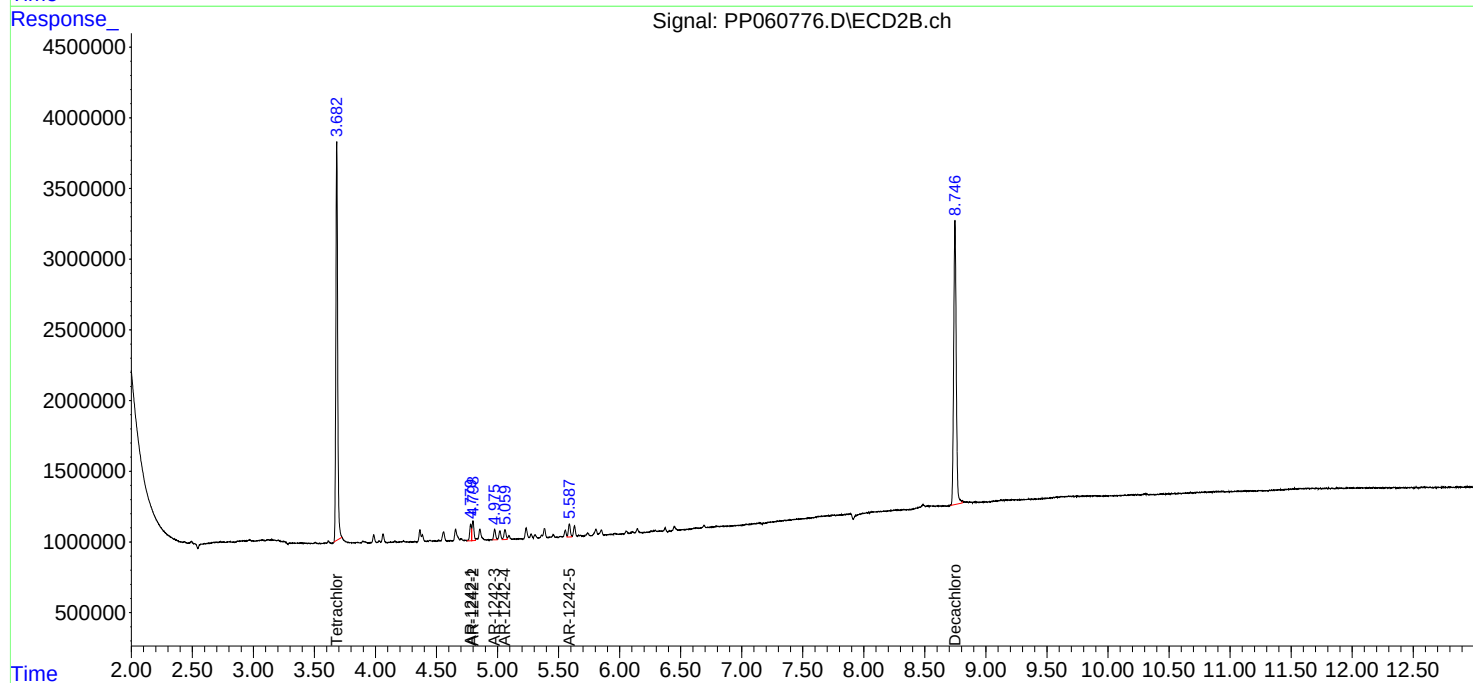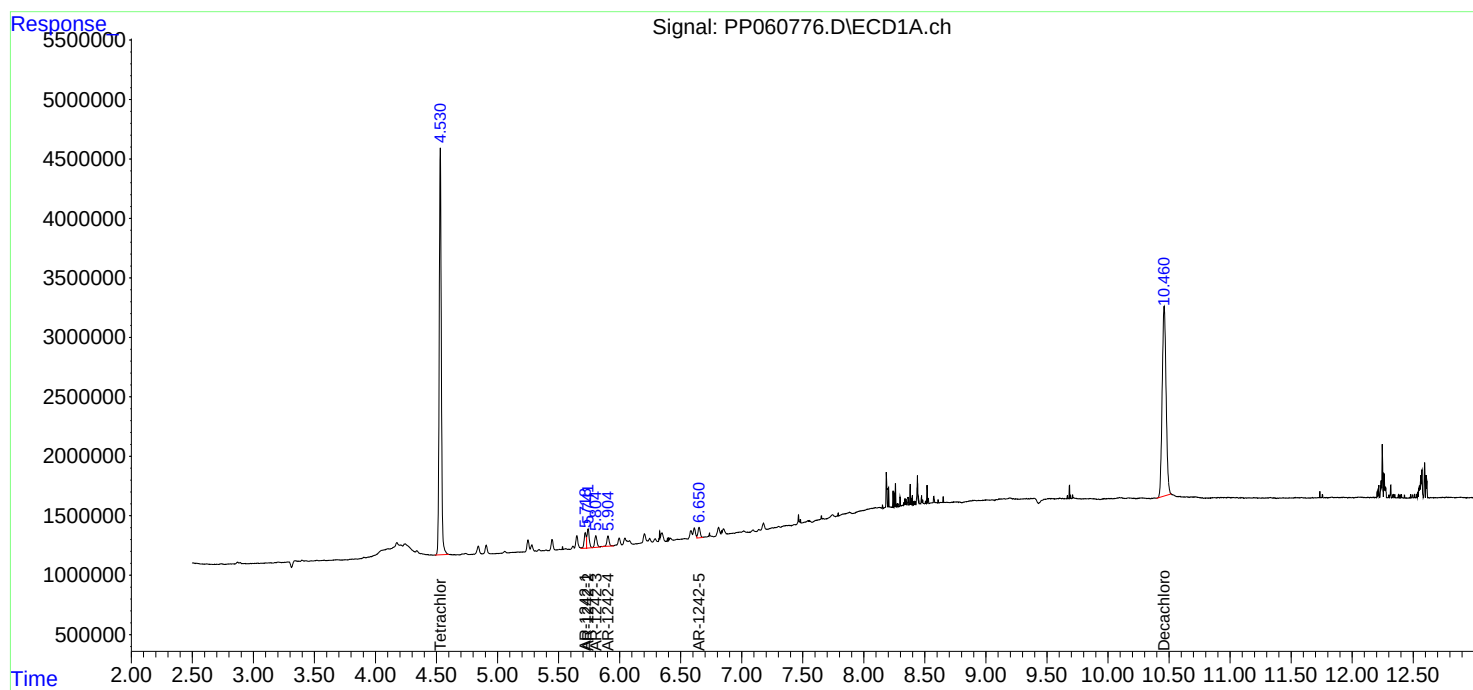


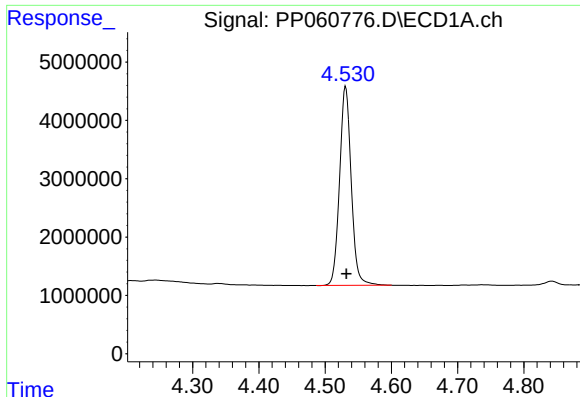

#1 Tetrachloro-m-xylene


R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 41708239
Conc: 18.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

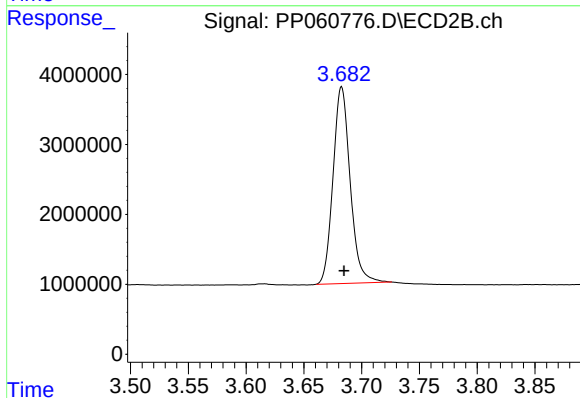


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: -0.002 min
Response: 29118862
Conc: 19.56 ng/ml

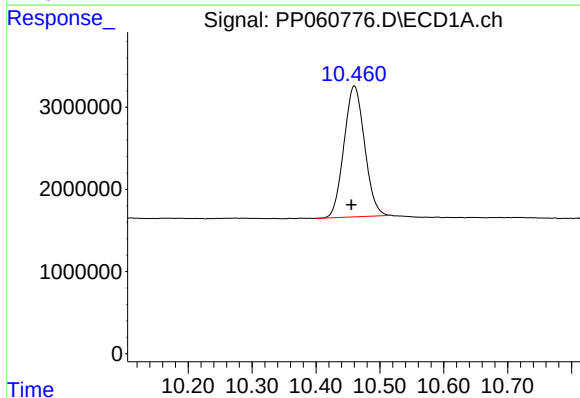


#2 Decachlorobiphenyl

R.T.: 10.460 min
Delta R.T.: 0.005 min
Response: 35767513
Conc: 20.26 ng/ml

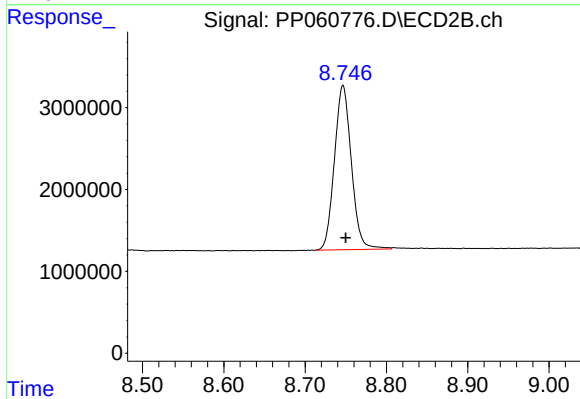

#2 Decachlorobiphenyl


R.T.: 8.747 min
Delta R.T.: -0.003 min
Response: 29056704
Conc: 17.81 ng/ml

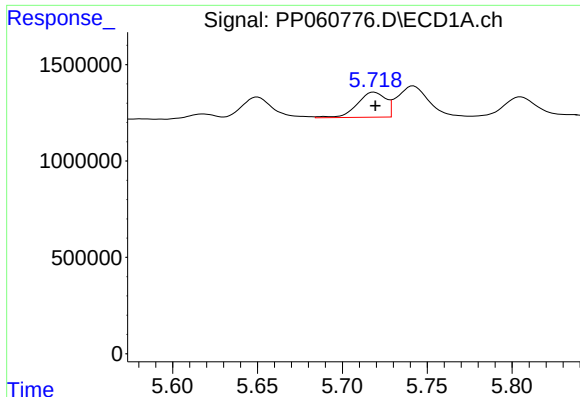

#16 AR-1242-1


R.T.: 5.719 min
Delta R.T.: 0.000 min
Response: 1518140
Conc: 23.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

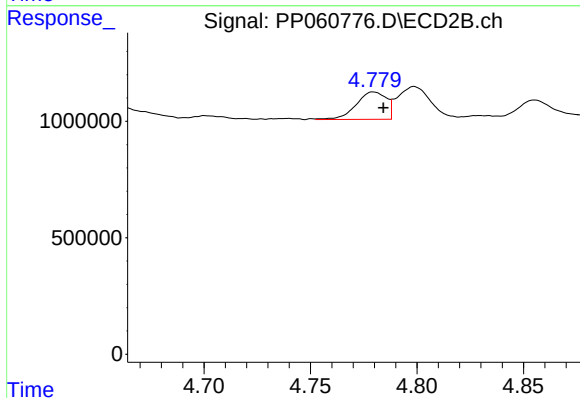


#16 AR-1242-1

R.T.: 4.779 min
Delta R.T.: -0.005 min
Response: 1162622
Conc: 22.96 ng/ml

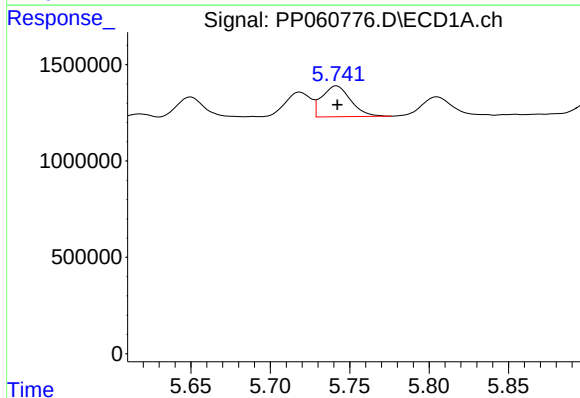


#17 AR-1242-2

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 2030562
Conc: 22.43 ng/ml

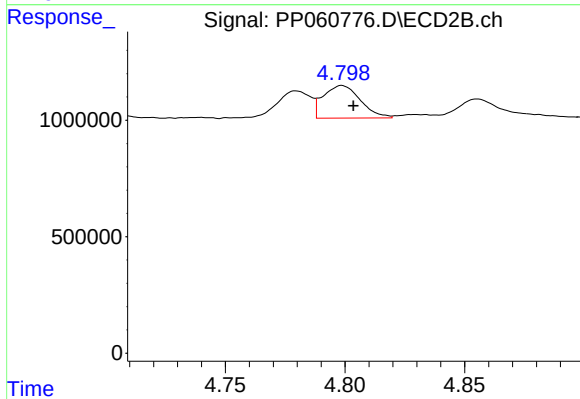

#17 AR-1242-2


R.T.: 4.799 min
Delta R.T.: -0.005 min
Response: 1512293
Conc: 21.78 ng/ml

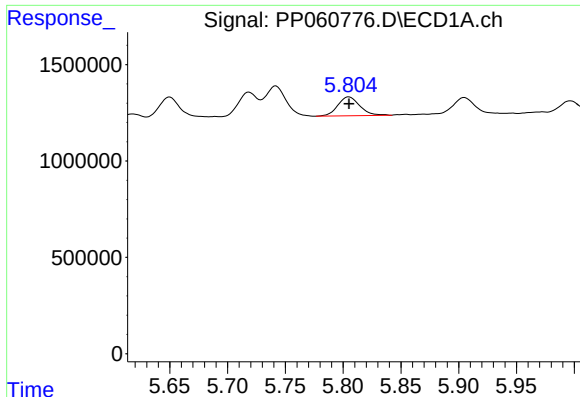

#18 AR-1242-3


R.T.: 5.805 min
Delta R.T.: 0.000 min
Response: 1298636
Conc: 23.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

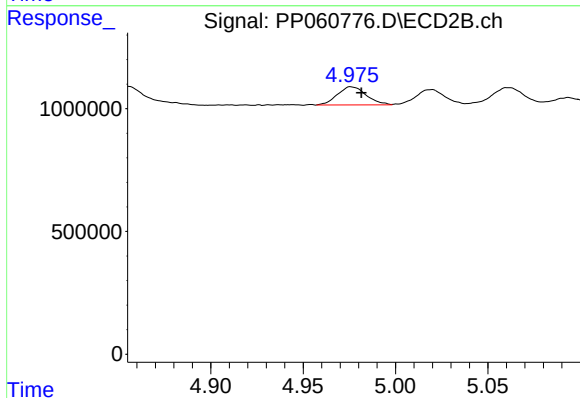


#18 AR-1242-3

R.T.: 4.976 min
Delta R.T.: -0.006 min
Response: 803589
Conc: 20.87 ng/ml

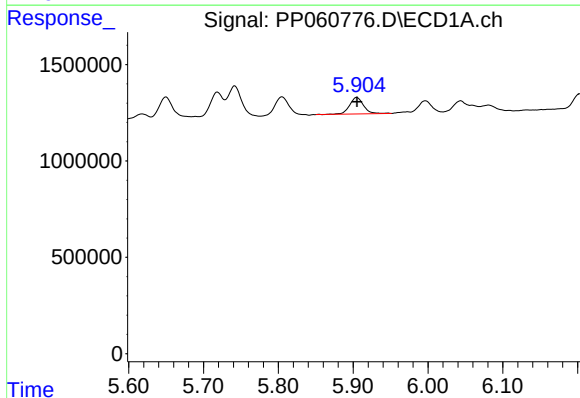


#19 AR-1242-4

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 1120666
Conc: 23.99 ng/ml

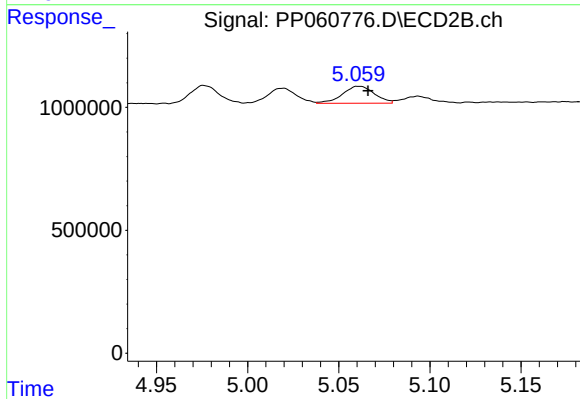

#19 AR-1242-4


R.T.: 5.060 min
Delta R.T.: -0.006 min
Response: 842251
Conc: 21.39 ng/ml

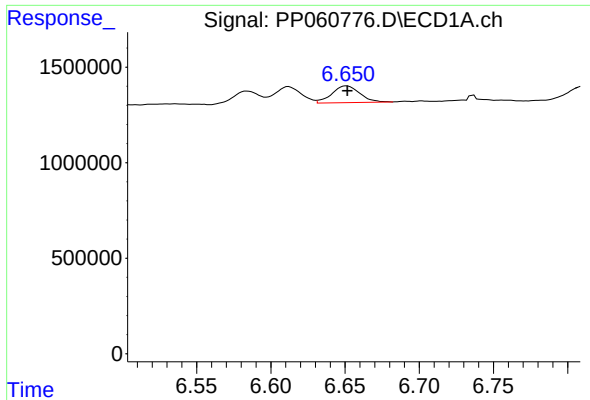

#20 AR-1242-5

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 1144681
Conc: 22.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2023

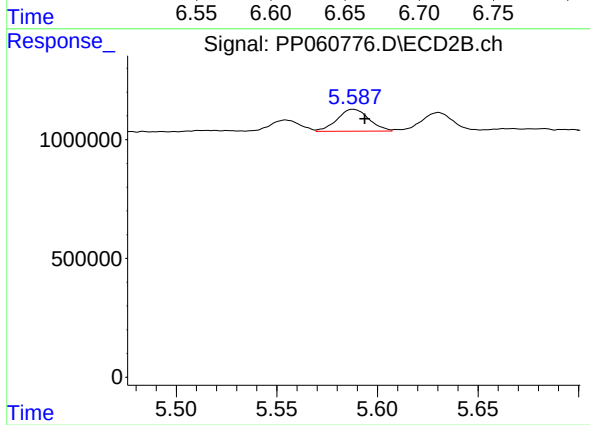

#20 AR-1242-5

R.T.: 5.588 min
Delta R.T.: -0.006 min
Response: 1021846
Conc: 20.89 ng/ml