

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100925\
 Data File : PP075682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2025 18:45
 Operator : YP\AJ
 Sample : Q3314-05 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC278514-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/10/2025
 Supervised By :mohammad ahmed 10/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:50:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.647	3.788	1879455	5683838	1.436m	0.932 #
2) SA Decachlor...	10.419	8.796	1197905	6107323	1.201m	1.012

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100925\
Data File : PP075682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2025 18:45
Operator : YP\AJ
Sample : Q3314-05 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC278514-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/10/2025
Supervised By :mohammad ahmed 10/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:50:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

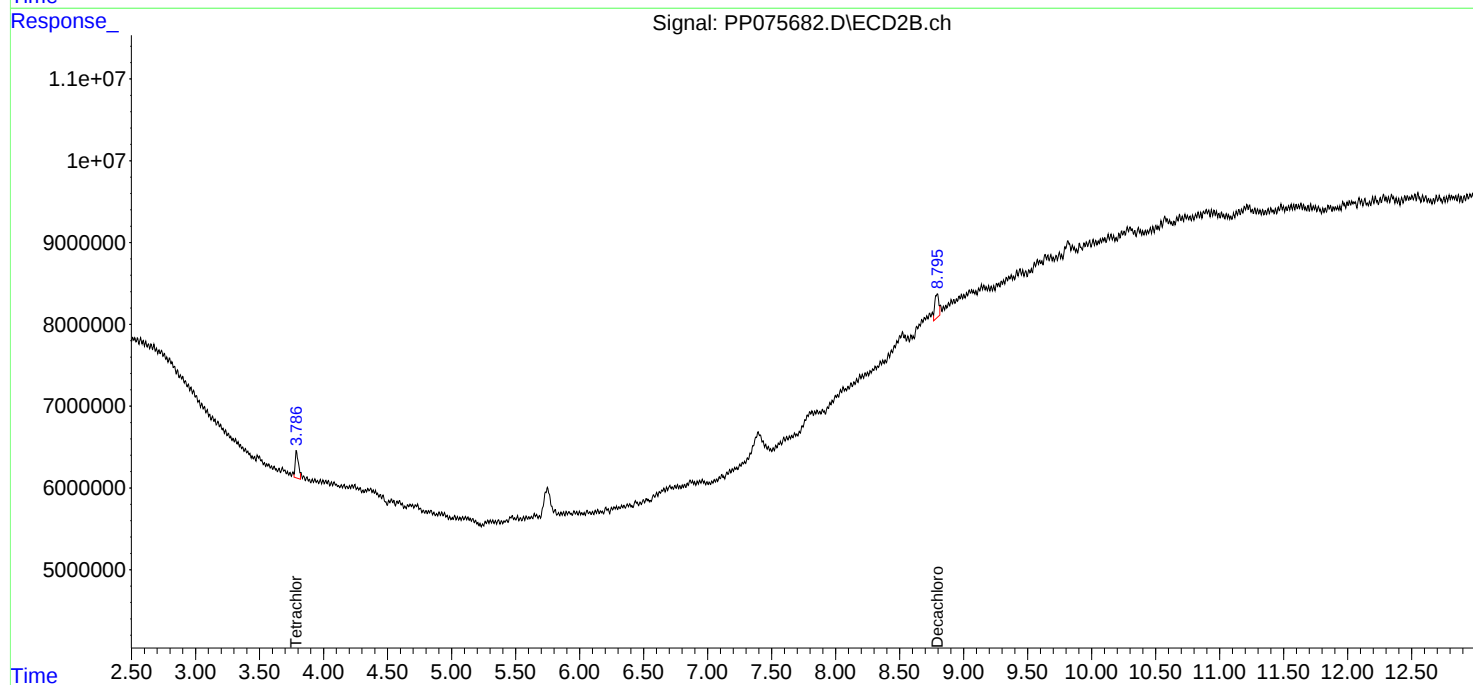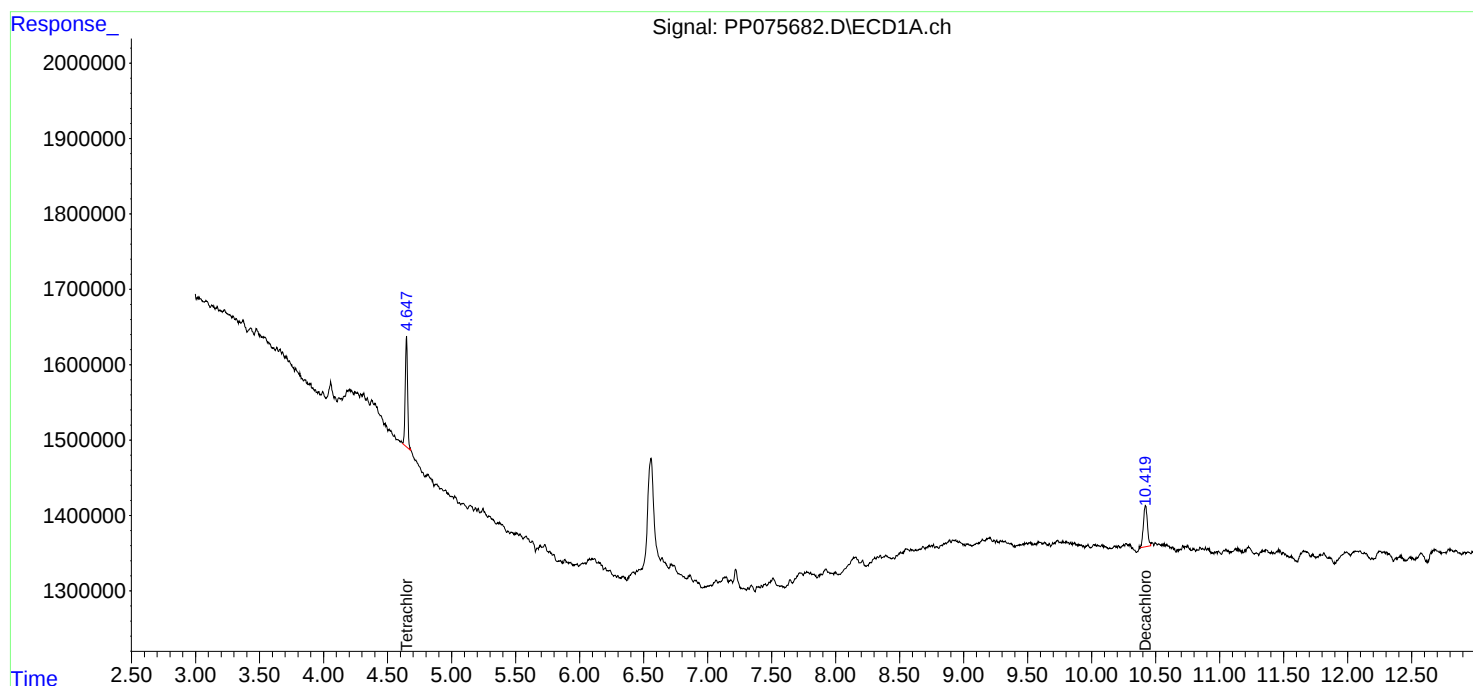

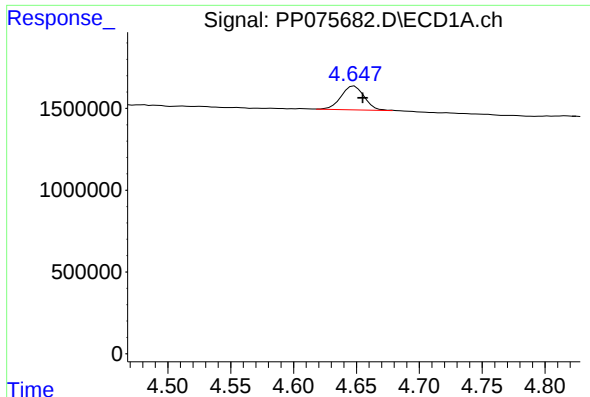


#1 Tetrachloro-m-xylene

R.T.: 4.647 min
Delta R.T.: -0.008 min
Response: 1879455
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC278514-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/10/2025
Supervised By :mohammad ahmed 10/11/2025

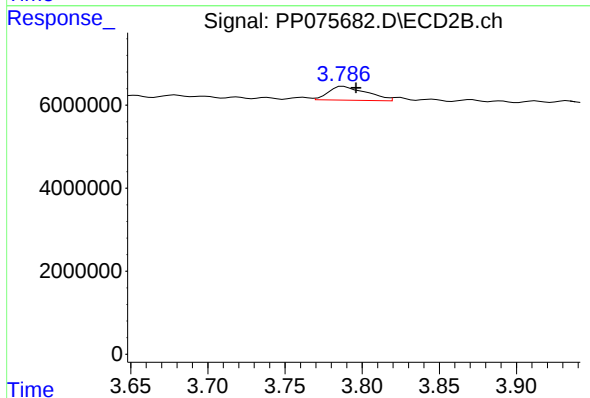


#1 Tetrachloro-m-xylene

R.T.: 3.788 min
Delta R.T.: -0.008 min
Response: 5683838
Conc: 0.93 ng/ml

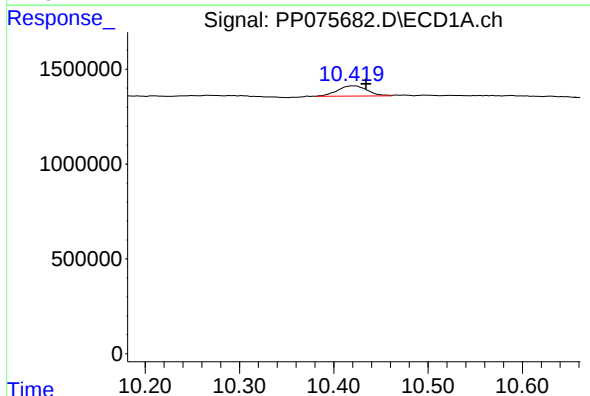

#2 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.015 min
Response: 1197905
Conc: 1.20 ng/ml m

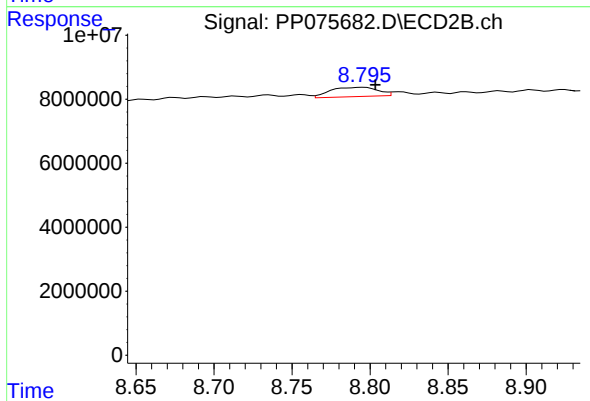

#2 Decachlorobiphenyl

R.T.: 8.796 min
Delta R.T.: -0.008 min
Response: 6107323
Conc: 1.01 ng/ml