

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100925\
 Data File : PP075697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2025 00:10
 Operator : YP\AJ
 Sample : Q3317-04 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2404-0055-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/10/2025
 Supervised By :mohammad ahmed 10/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:54:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.648	3.791	2147262	7051936	1.641m	1.156 #
2) SA Decachlor...	10.421	8.787	1434023	7904577	1.438m	1.310m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP100925\
Data File : PP075697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2025 00:10
Operator : YP\AJ
Sample : Q3317-04 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2404-0055-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/10/2025
Supervised By :mohammad ahmed 10/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:54:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

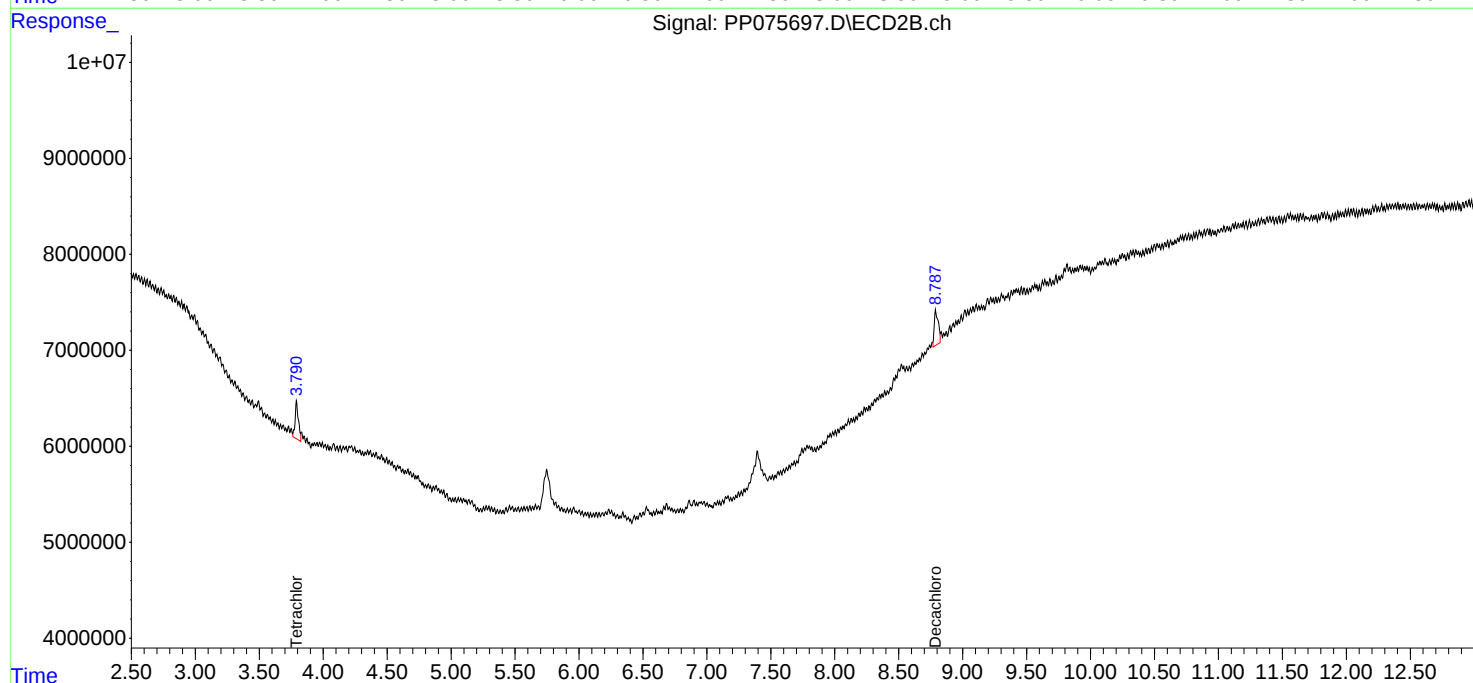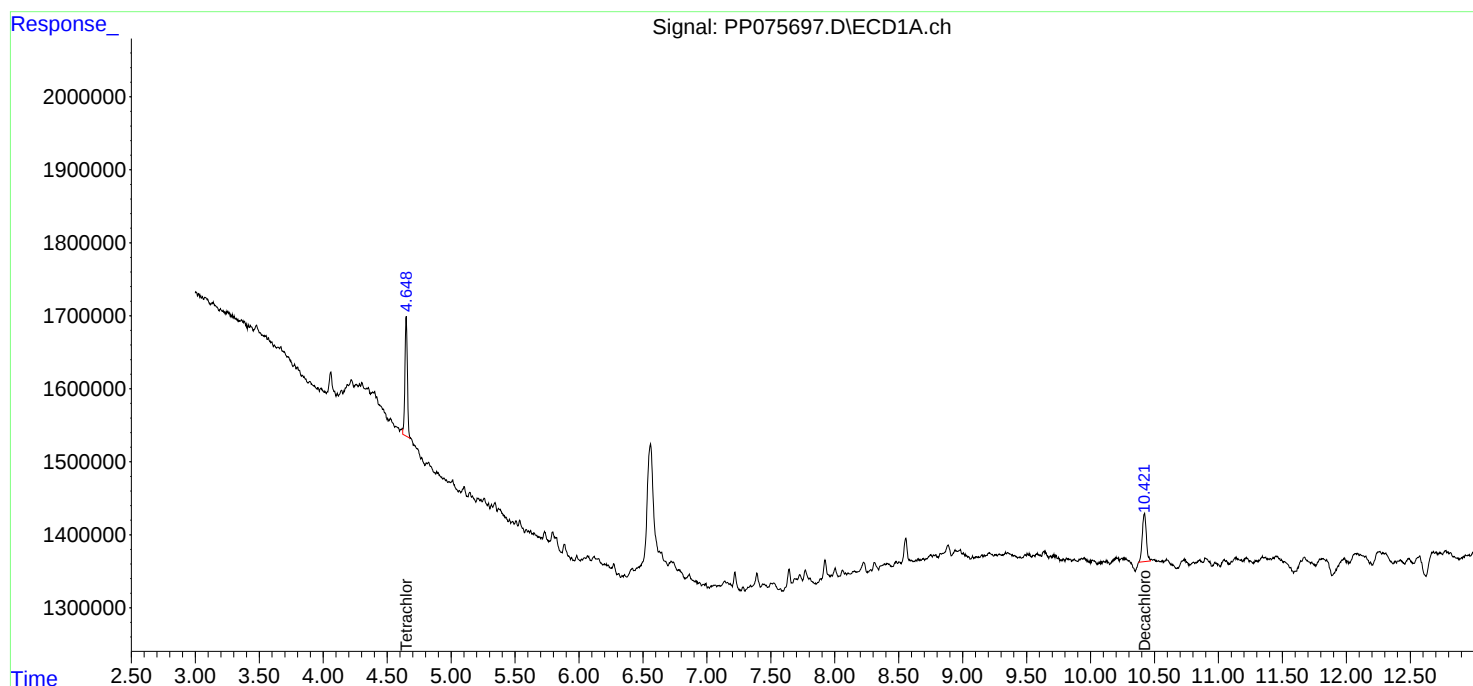

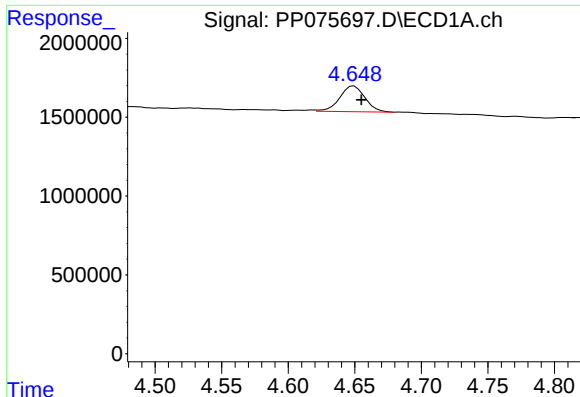


#1 Tetrachloro-m-xylene

R.T.: 4.648 min
Delta R.T.: -0.007 min
Response: 2147262
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2404-0055-1-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/10/2025
Supervised By :mohammad ahmed 10/11/2025

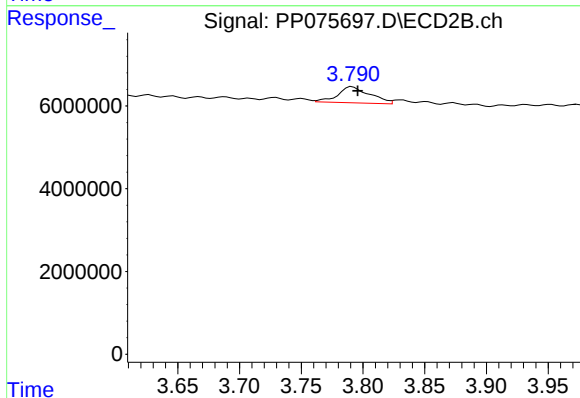

#1 Tetrachloro-m-xylene

R.T.: 3.791 min
Delta R.T.: -0.005 min
Response: 7051936
Conc: 1.16 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.013 min
Response: 1434023
Conc: 1.44 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.017 min
Response: 7904577
Conc: 1.31 ng/ml m