

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101023\
 Data File : PP060844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 15:07
 Operator : YP\AJ
 Sample : 04699-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:34:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.532	3.684	43053702	30101990	19.225	20.223
2) SA Decachlor...	10.465	8.747	38003486	33237929	21.525	20.376
Target Compounds						
21) L5 AR-1248-1	5.720	4.781	1080040	776144	23.214	21.268
22) L5 AR-1248-2	5.997	5.020	1537699	1143333	22.178	21.873
23) L5 AR-1248-3	6.205	5.063	1762948	1191407	23.212	21.457
24) L5 AR-1248-4	6.613	5.236	2156692	1501847	26.077	22.815
25) L5 AR-1248-5	6.652	5.631	2238065	1301439	27.808	20.233 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101023\
Data File : PP060844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 15:07
Operator : YP\AJ
Sample : 04699-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:34:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

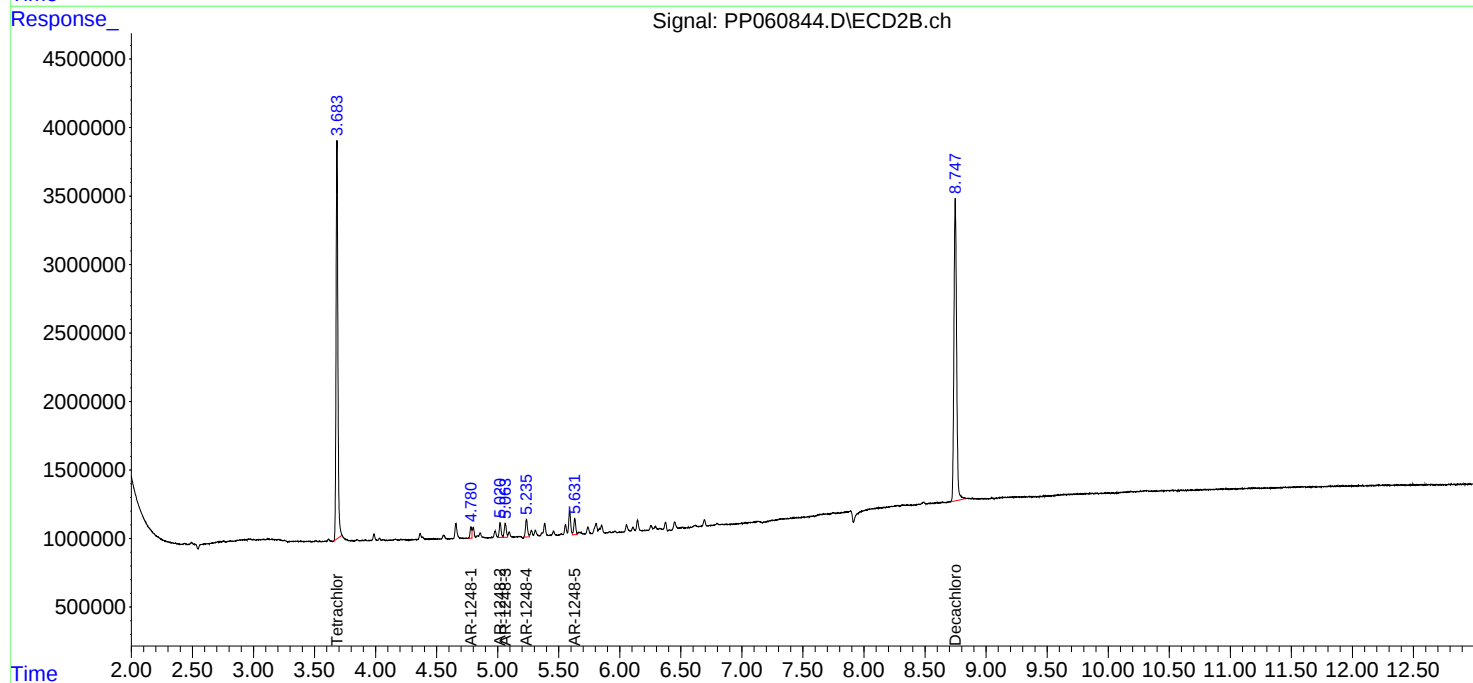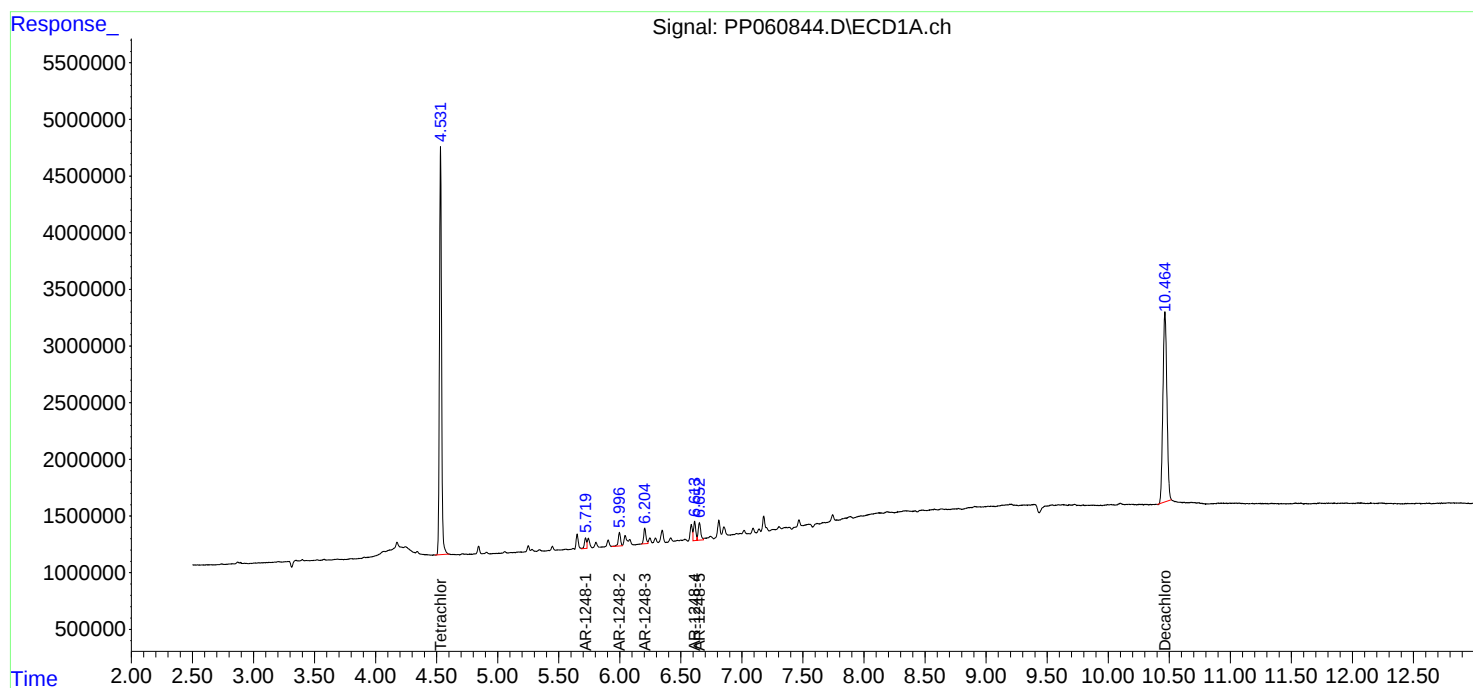


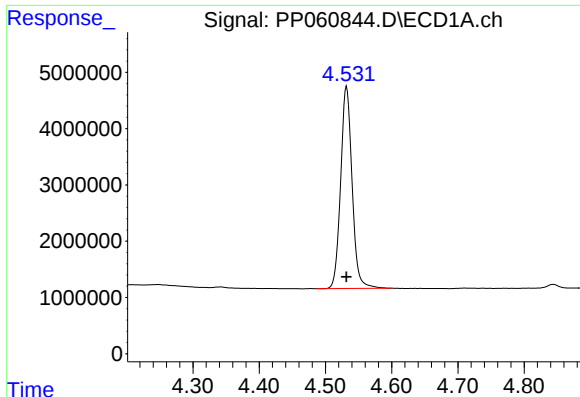

#1 Tetrachloro-m-xylene


R.T.: 4.532 min
Delta R.T.: 0.000 min
Response: 43053702
Conc: 19.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2023

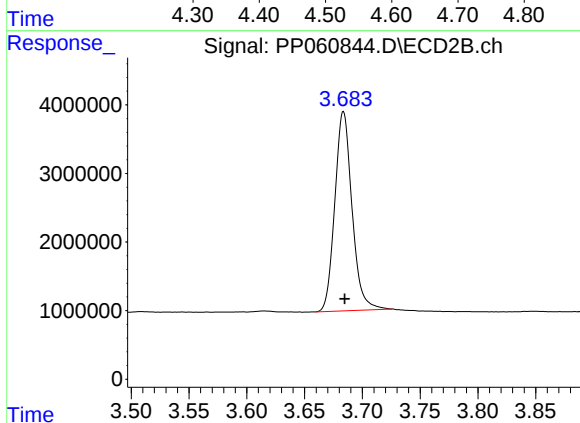


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: -0.001 min
Response: 30101990
Conc: 20.22 ng/ml

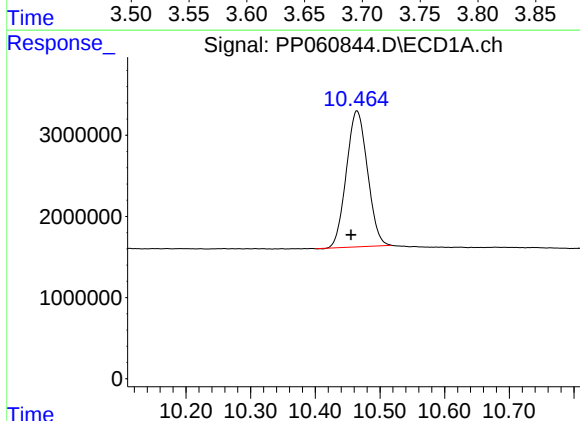


#2 Decachlorobiphenyl

R.T.: 10.465 min
Delta R.T.: 0.009 min
Response: 38003486
Conc: 21.53 ng/ml

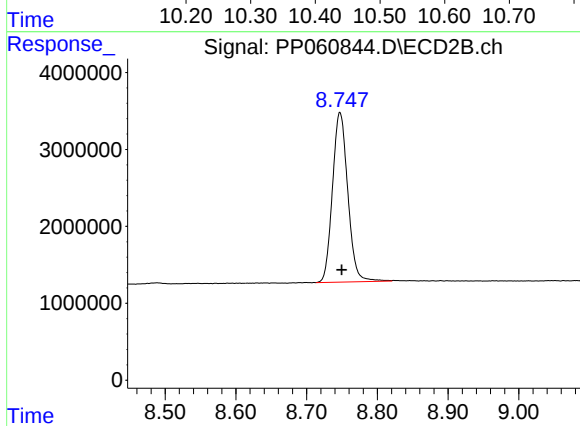

#2 Decachlorobiphenyl


R.T.: 8.747 min
Delta R.T.: -0.003 min
Response: 33237929
Conc: 20.38 ng/ml

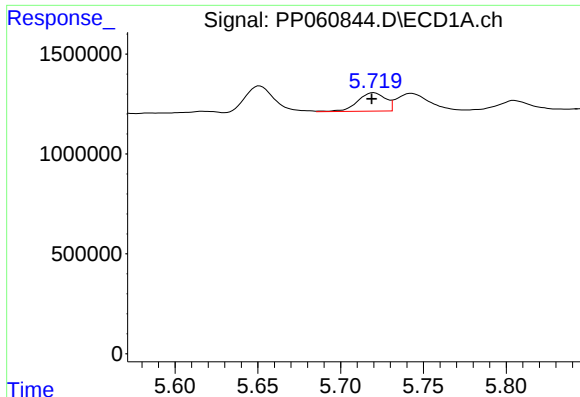

#21 AR-1248-1


R.T.: 5.720 min
Delta R.T.: 0.001 min
Response: 1080040
Conc: 23.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2023

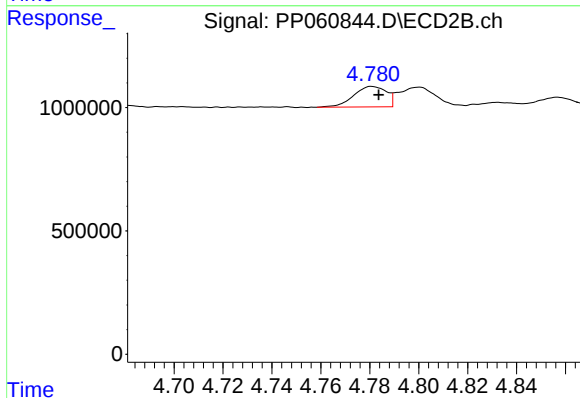


#21 AR-1248-1

R.T.: 4.781 min
Delta R.T.: -0.003 min
Response: 776144
Conc: 21.27 ng/ml

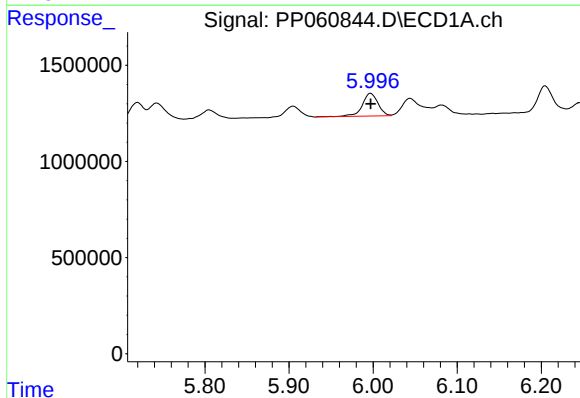


#22 AR-1248-2

R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 1537699
Conc: 22.18 ng/ml

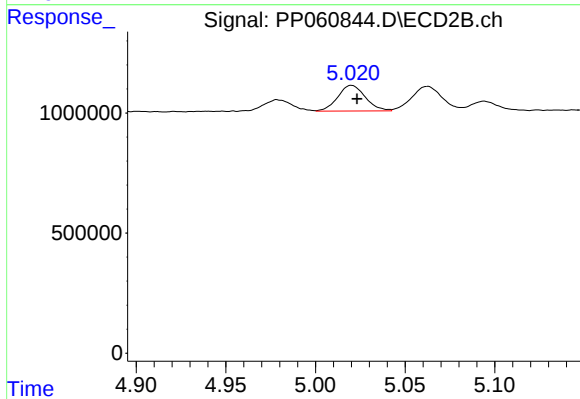

#22 AR-1248-2


R.T.: 5.020 min
Delta R.T.: -0.003 min
Response: 1143333
Conc: 21.87 ng/ml

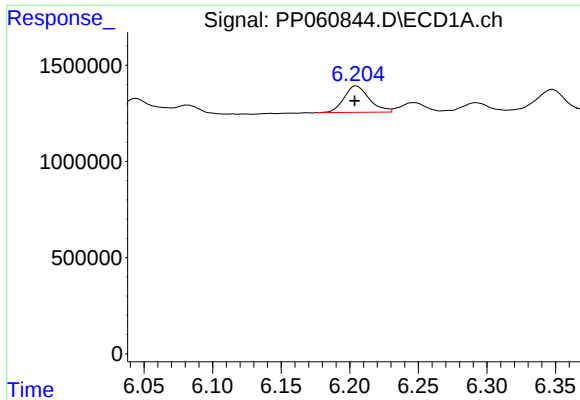

#23 AR-1248-3


R.T.: 6.205 min
Delta R.T.: 0.001 min
Response: 1762948
Conc: 23.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2023

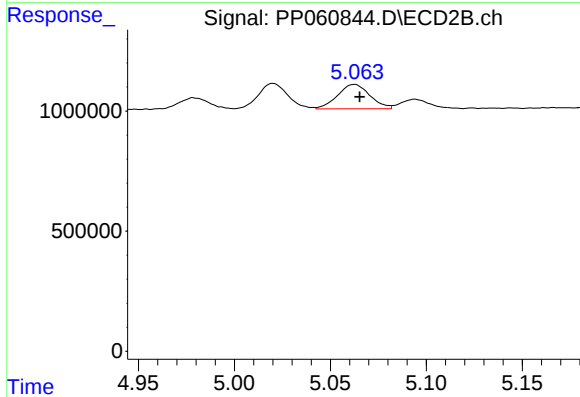


#23 AR-1248-3

R.T.: 5.063 min
Delta R.T.: -0.002 min
Response: 1191407
Conc: 21.46 ng/ml

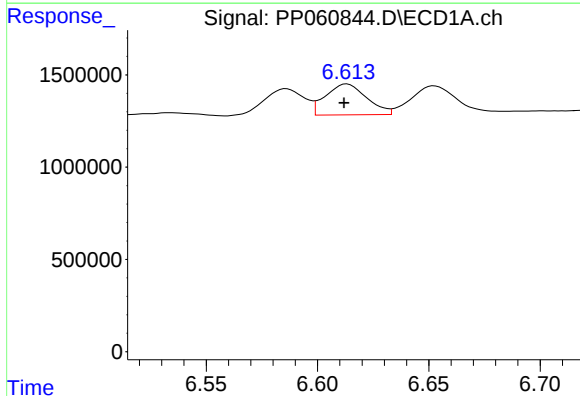


#24 AR-1248-4

R.T.: 6.613 min
Delta R.T.: 0.001 min
Response: 2156692
Conc: 26.08 ng/ml

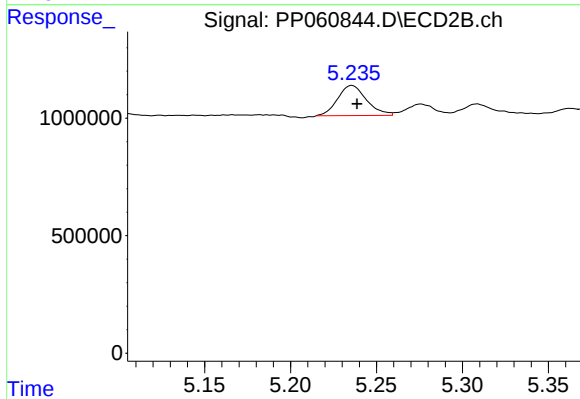

#24 AR-1248-4


R.T.: 5.236 min
Delta R.T.: -0.003 min
Response: 1501847
Conc: 22.82 ng/ml

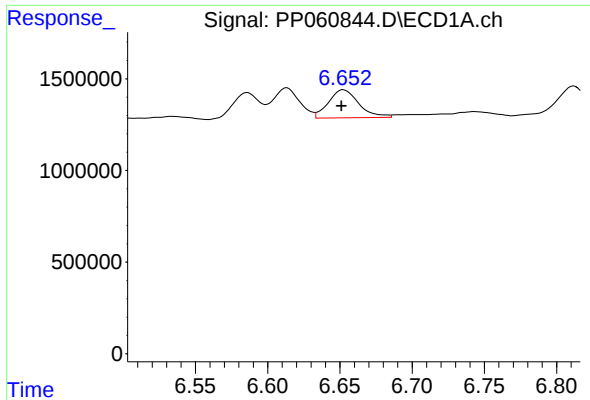

#25 AR-1248-5

R.T.: 6.652 min
Delta R.T.: 0.001 min
Response: 2238065
Conc: 27.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT4-2023

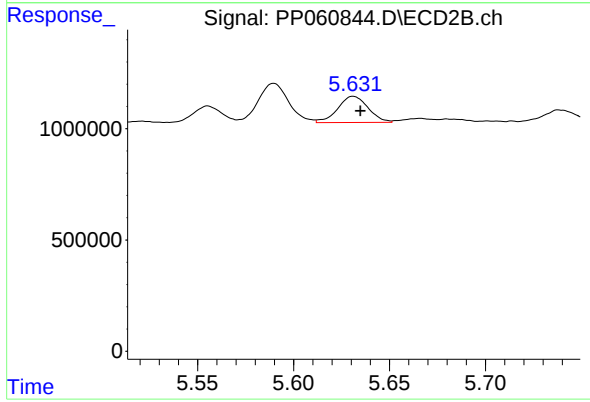

#25 AR-1248-5

R.T.: 5.631 min
Delta R.T.: -0.004 min
Response: 1301439
Conc: 20.23 ng/ml