

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101023\
 Data File : PP060871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 22:51
 Operator : YP\AJ
 Sample : 04815-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-20416

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2023
 Supervised By :Ankita Jodhani 10/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 02:38:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.536	3.690	28722358	20724233	12.825	13.923m
2) SA Decachlor...	10.468	8.750	31456883	24531757	17.817	15.039

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101023\
Data File : PP060871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 22:51
Operator : YP\AJ
Sample : 04815-02
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CHRT-20416


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :Ankita Jodhani 10/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 02:38:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

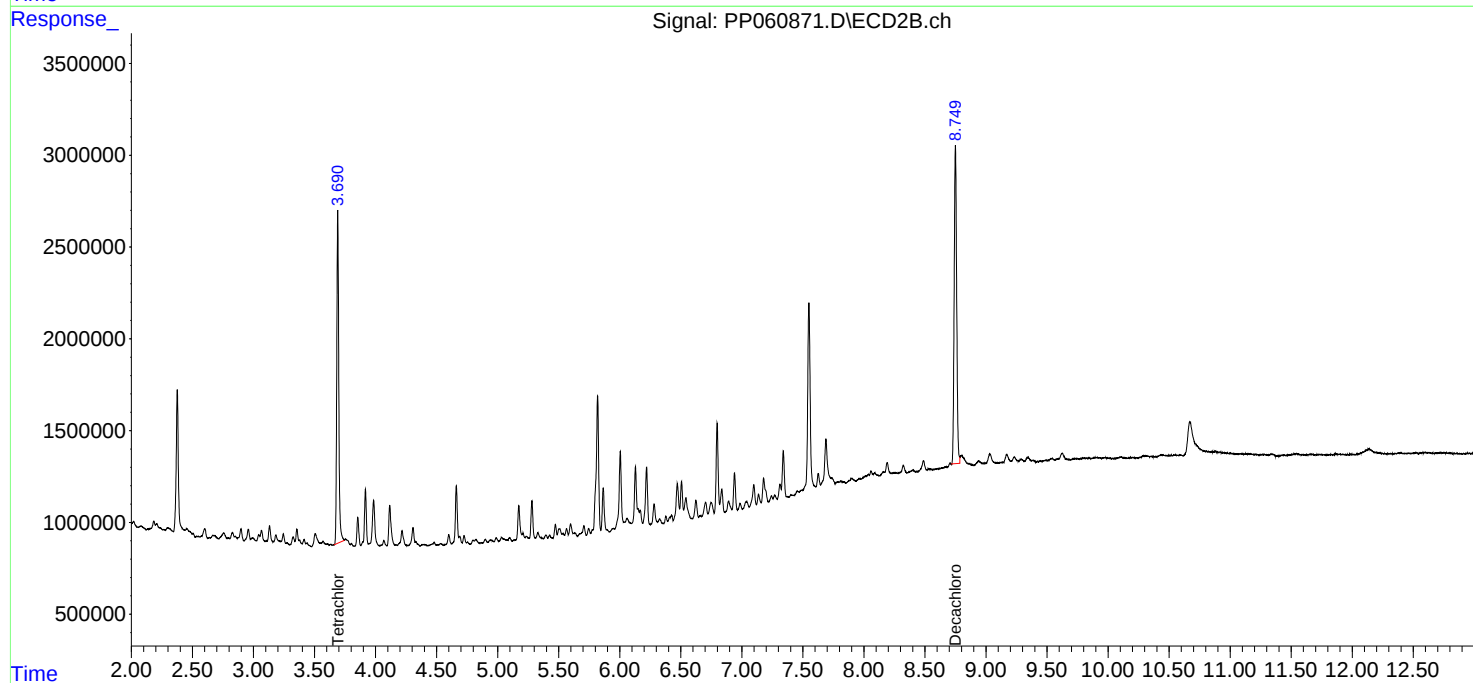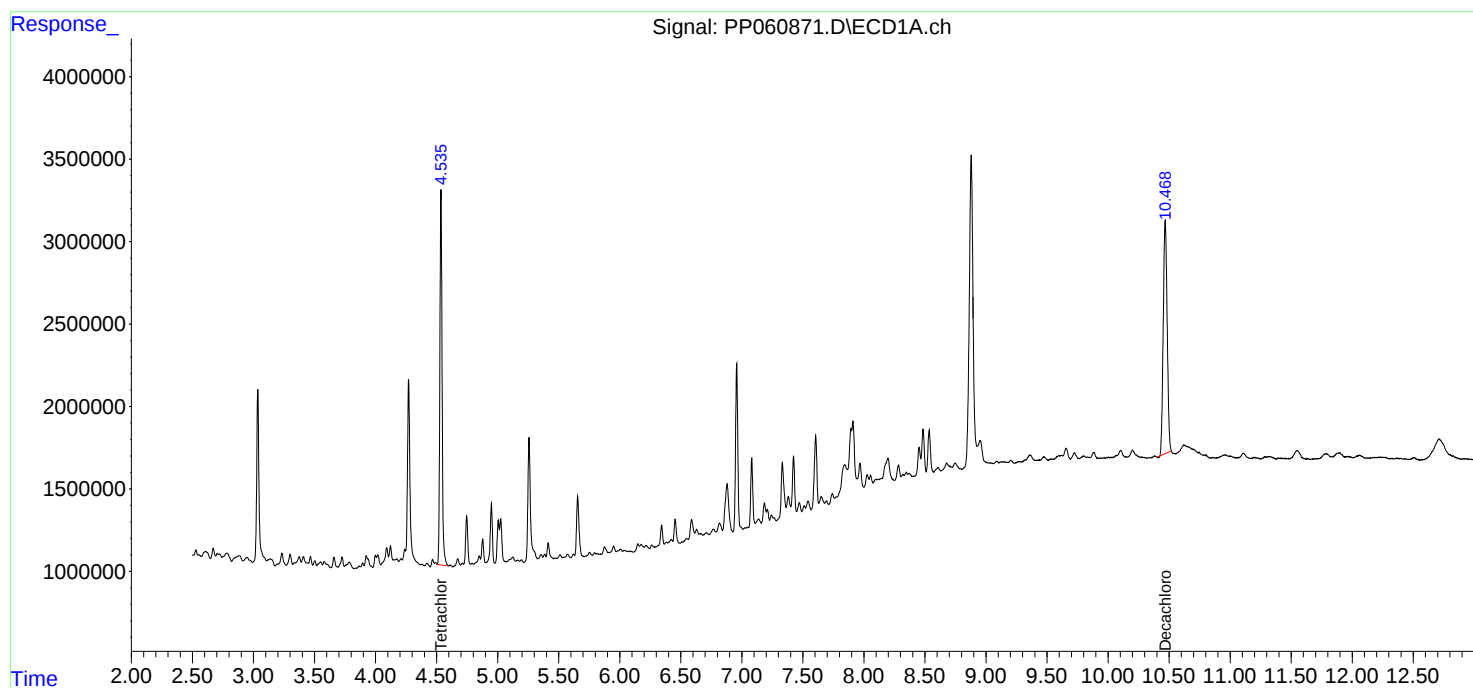

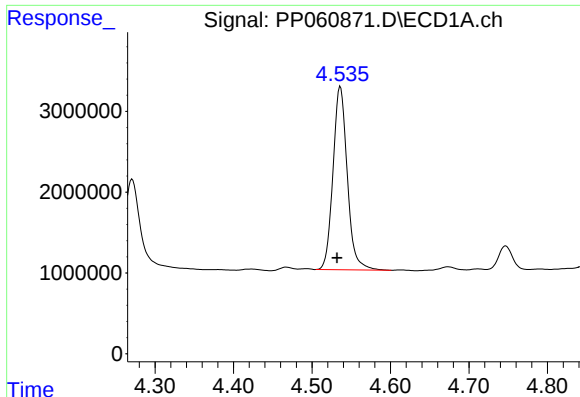


#1 Tetrachloro-m-xylene

R.T.: 4.536 min
Delta R.T.: 0.004 min
Response: 28722358
Conc: 12.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-20416


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :Ankita Jodhani 10/11/2023

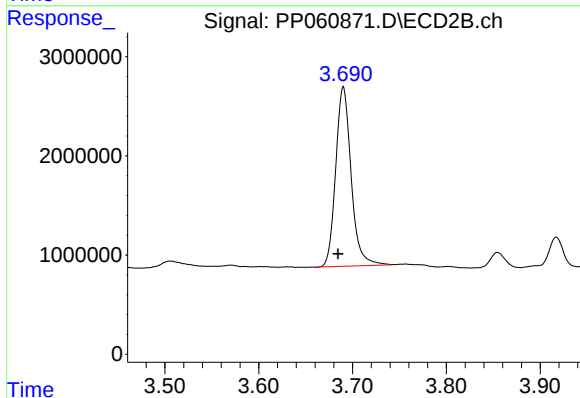


#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: 0.005 min
Response: 20724233
Conc: 13.92 ng/ml m

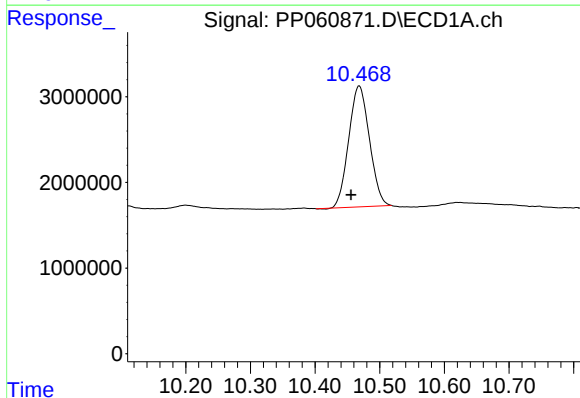

#2 Decachlorobiphenyl

R.T.: 10.468 min
Delta R.T.: 0.013 min
Response: 31456883
Conc: 17.82 ng/ml

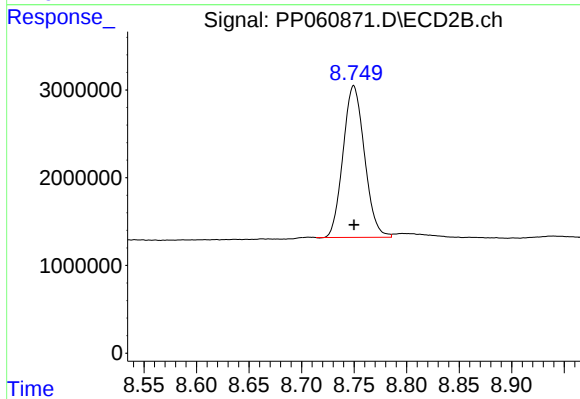

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: 0.000 min
Response: 24531757
Conc: 15.04 ng/ml