

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101121\
 Data File : PP039940.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2021 9:43
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:56:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10)	L2	AR-1221-3	0.000	4.425	0	10528 N.D. 19.663 #
11)	L3	AR-1232-1	0.000	4.425	0	10528 N.D. 26.292 #
20)	L4	AR-1242-5	0.000	6.145f	0	45920 N.D. 92.371 #
25)	L5	AR-1248-5	0.000	6.145f	0	45920 N.D. 71.586 #
26)	L6	AR-1254-1	0.000	6.145f	0	45920 N.D. 46.595 #
30)	L6	AR-1254-5	0.000	7.387	0	5828 N.D. 4.351 #
32)	L7	AR-1260-2	0.000	7.022f	0	68704 N.D. 54.370 #
33)	L7	AR-1260-3	0.000	7.197	0	132768 N.D. 100.132 #
36)	L8	AR-1262-1	0.000	7.387	0	5828 N.D. 8.100 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101121\
Data File : PP039940.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2021 9:43
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:56:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

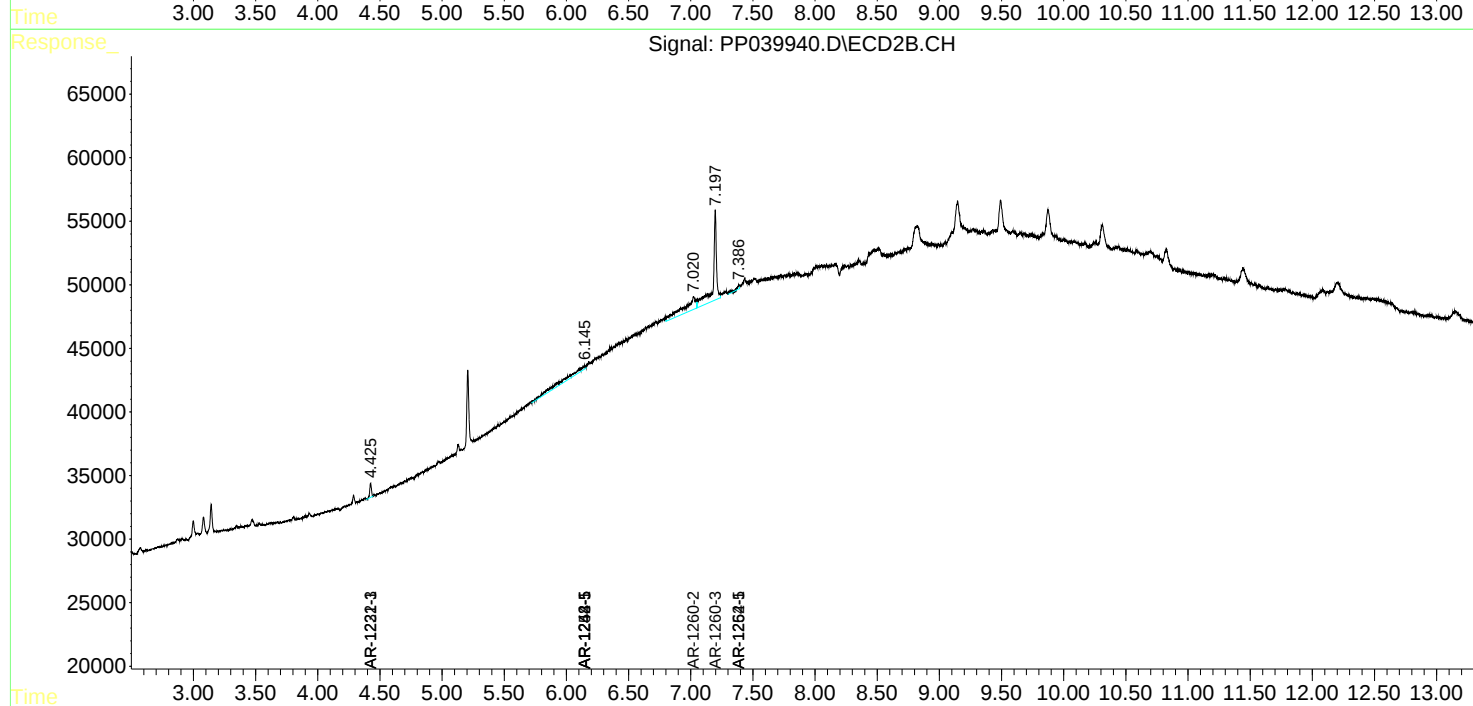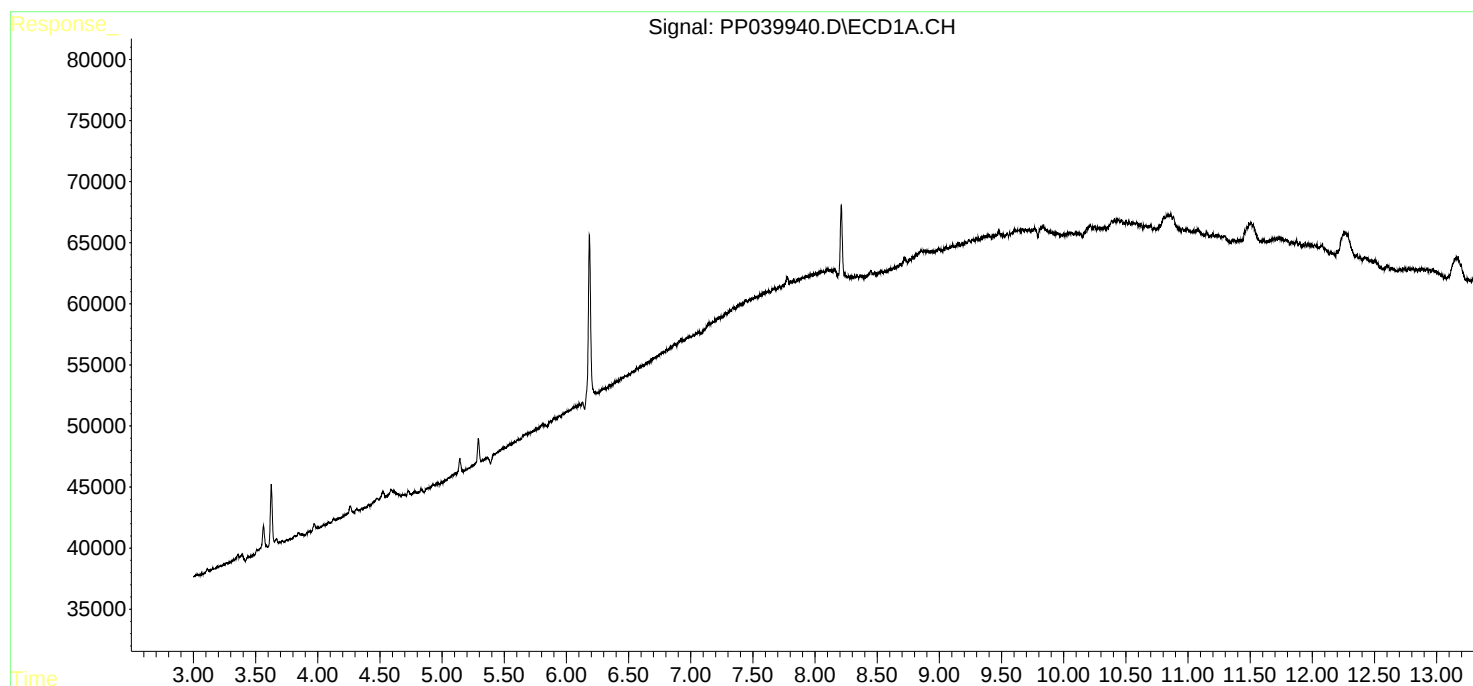


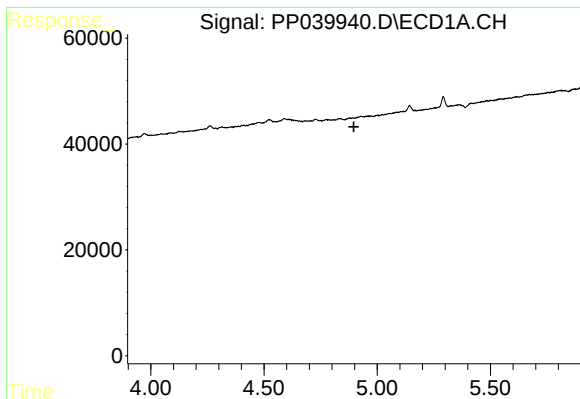

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.897 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

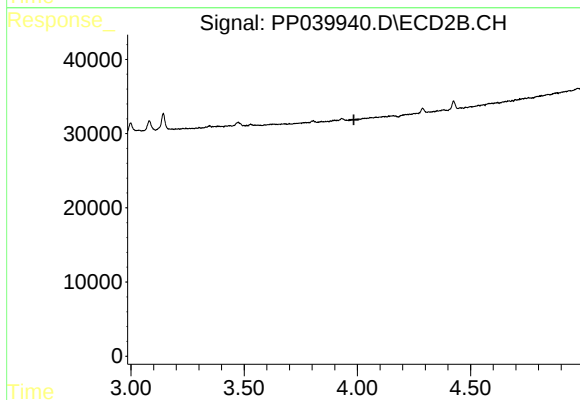


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.985 min
Response: 0
Conc: N.D.

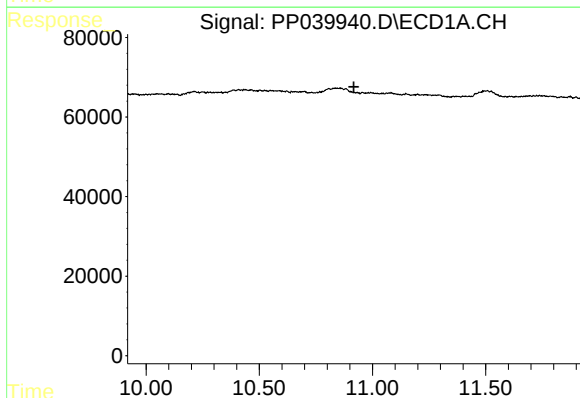


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.918 min
Response: 0
Conc: N.D.

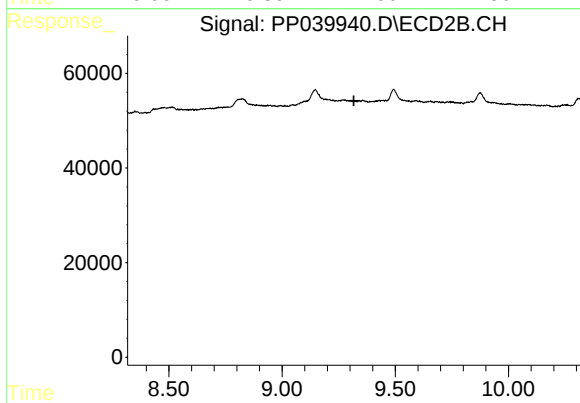

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.317 min
Response: 0
Conc: N.D.

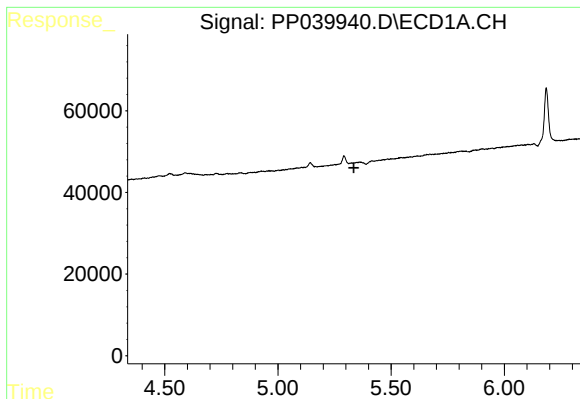

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

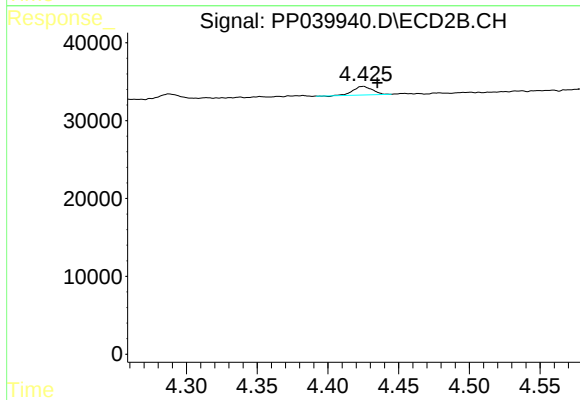


#10 AR-1221-3

R.T.: 4.425 min
Delta R.T.: -0.010 min
Response: 10528
Conc: 19.66 ng/ml

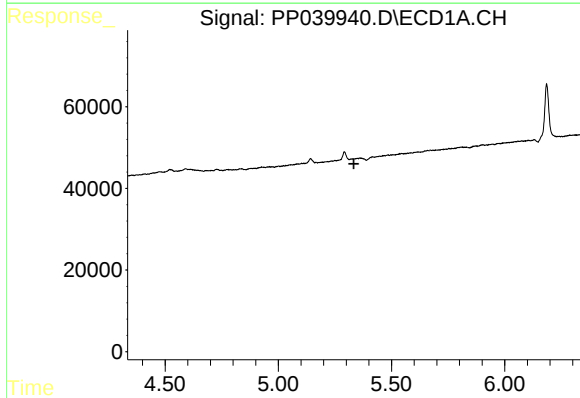


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.334 min
Response: 0
Conc: N.D.

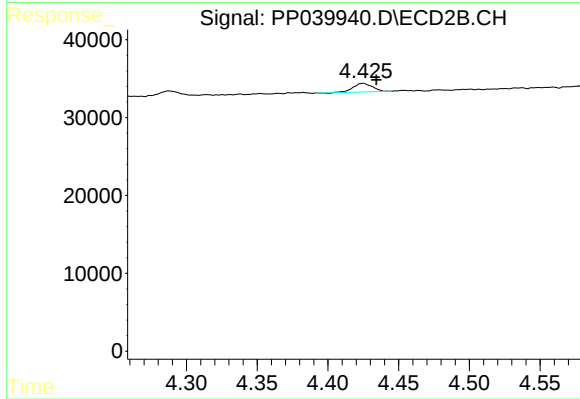

#11 AR-1232-1


R.T.: 4.425 min
Delta R.T.: -0.009 min
Response: 10528
Conc: 26.29 ng/ml

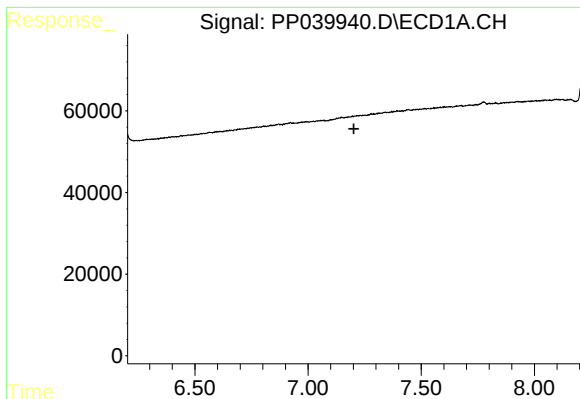

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

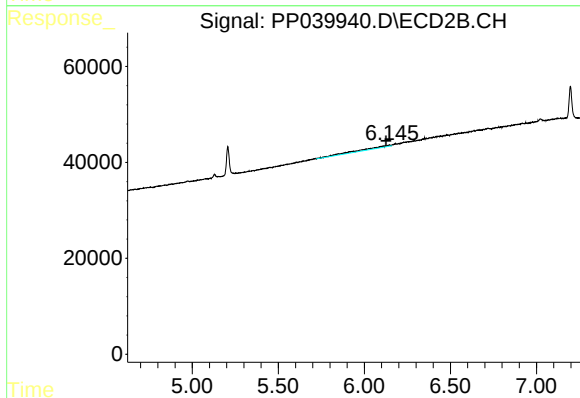


#20 AR-1242-5

R.T.: 6.145 min
Delta R.T.: 0.018 min
Response: 45920
Conc: 92.37 ng/ml

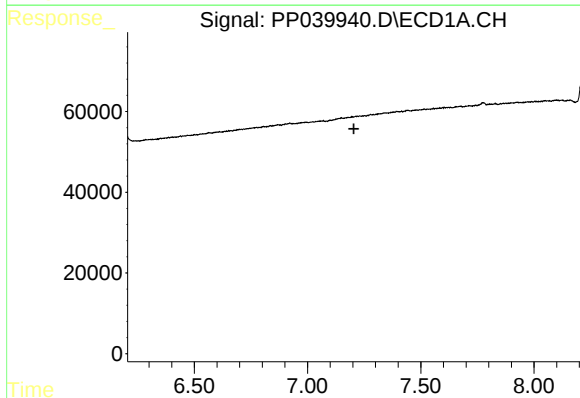


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.205 min
Response: 0
Conc: N.D.

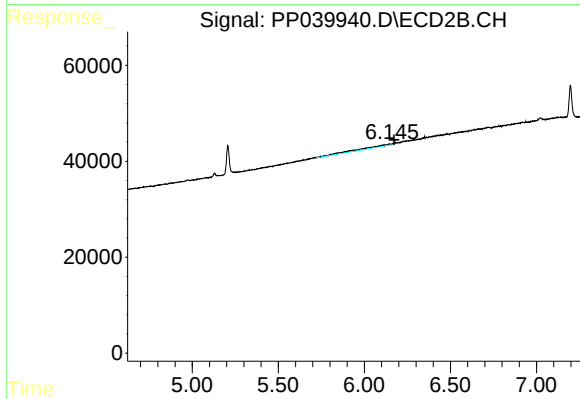

#25 AR-1248-5


R.T.: 6.145 min
Delta R.T.: -0.027 min
Response: 45920
Conc: 71.59 ng/ml

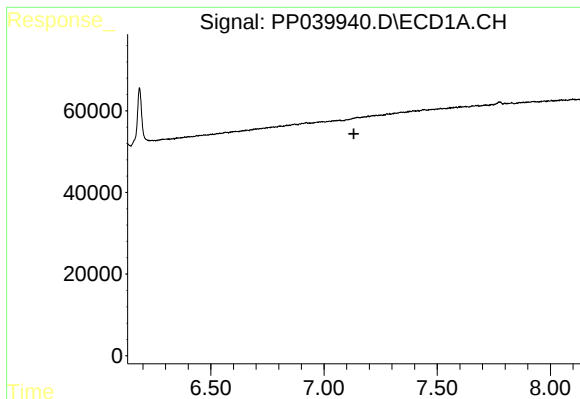

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 7.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

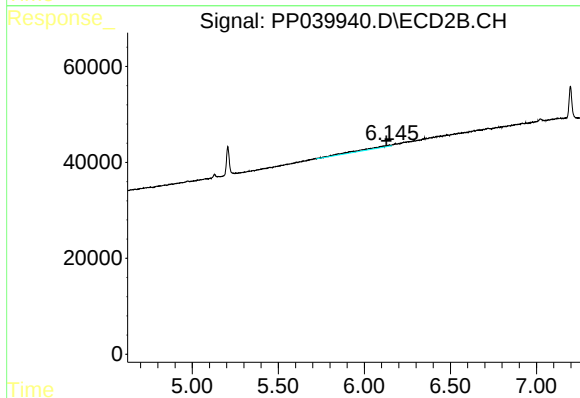


#26 AR-1254-1

R.T.: 6.145 min
Delta R.T.: 0.018 min
Response: 45920
Conc: 46.59 ng/ml

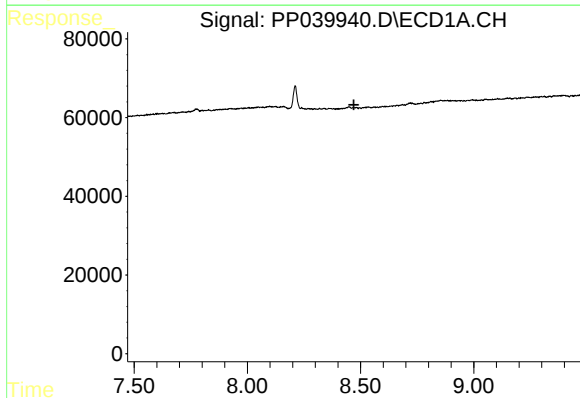


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.470 min
Response: 0
Conc: N.D.

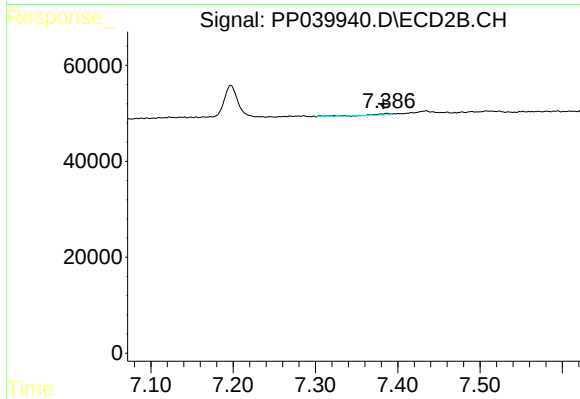

#30 AR-1254-5


R.T.: 7.387 min
Delta R.T.: 0.004 min
Response: 5828
Conc: 4.35 ng/ml

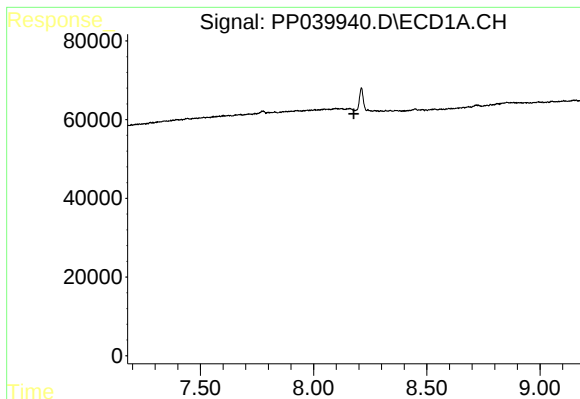

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.178 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

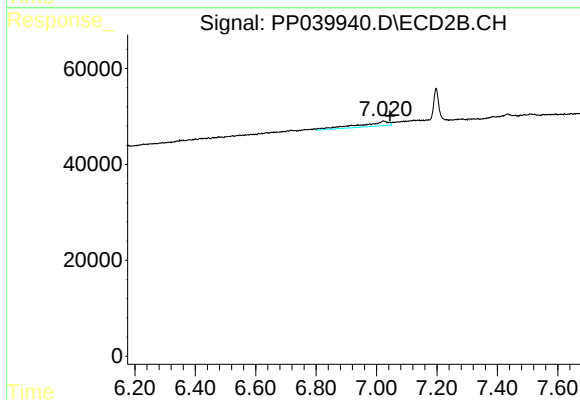


#32 AR-1260-2

R.T.: 7.022 min
Delta R.T.: -0.023 min
Response: 68704
Conc: 54.37 ng/ml

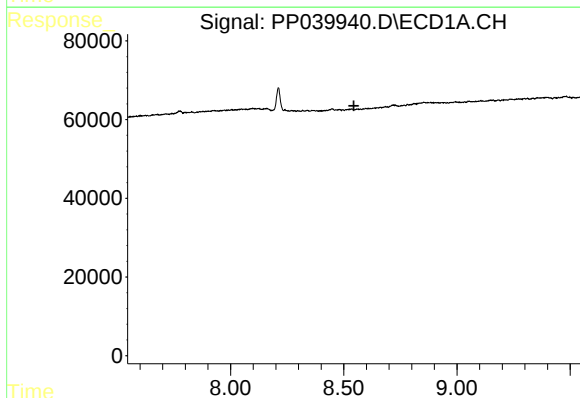


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.544 min
Response: 0
Conc: N.D.

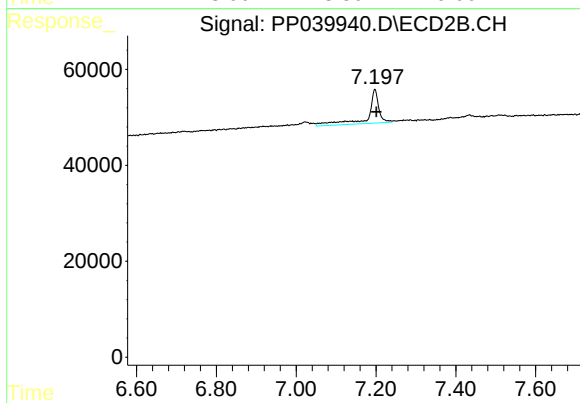

#33 AR-1260-3


R.T.: 7.197 min
Delta R.T.: -0.004 min
Response: 132768
Conc: 100.13 ng/ml

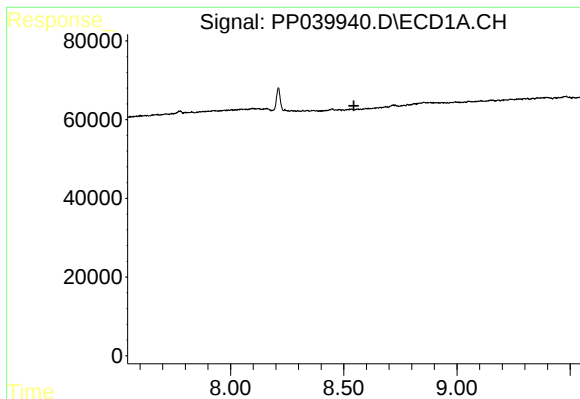

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

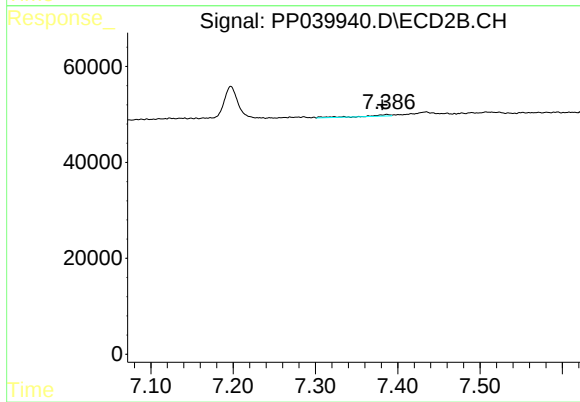

#36 AR-1262-1

R.T.: 7.387 min
Delta R.T.: 0.005 min
Response: 5828
Conc: 8.10 ng/ml