

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101121\
 Data File : PP039970.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2021 19:15
 Operator : AJ\MA
 Sample : M4165-03 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 732910-10-06-21-03

Manual Integrations
 APPROVED

mohammad
 10/13/2021 1:22:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 02:09:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 08 04:46:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.985	58398	33563	1.918	2.008
2) SA Decachlor...	10.920	9.315	58449	44207	2.600m	1.971

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101121\
Data File : PP039970.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2021 19:15
Operator : AJ\MA
Sample : M4165-03 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
732910-10-06-21-03


Manual Integrations
APPROVED

mohammad
10/13/2021 1:22:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 02:09:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 08 04:46:38 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

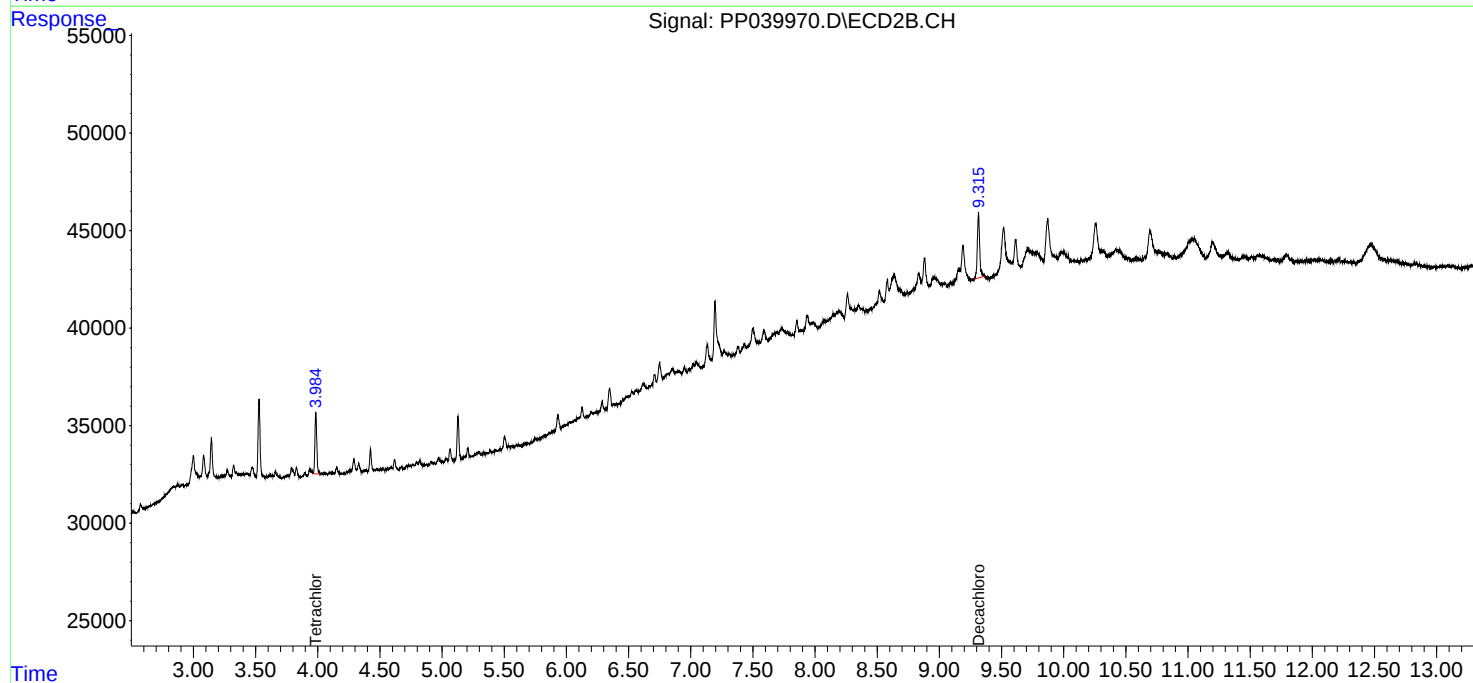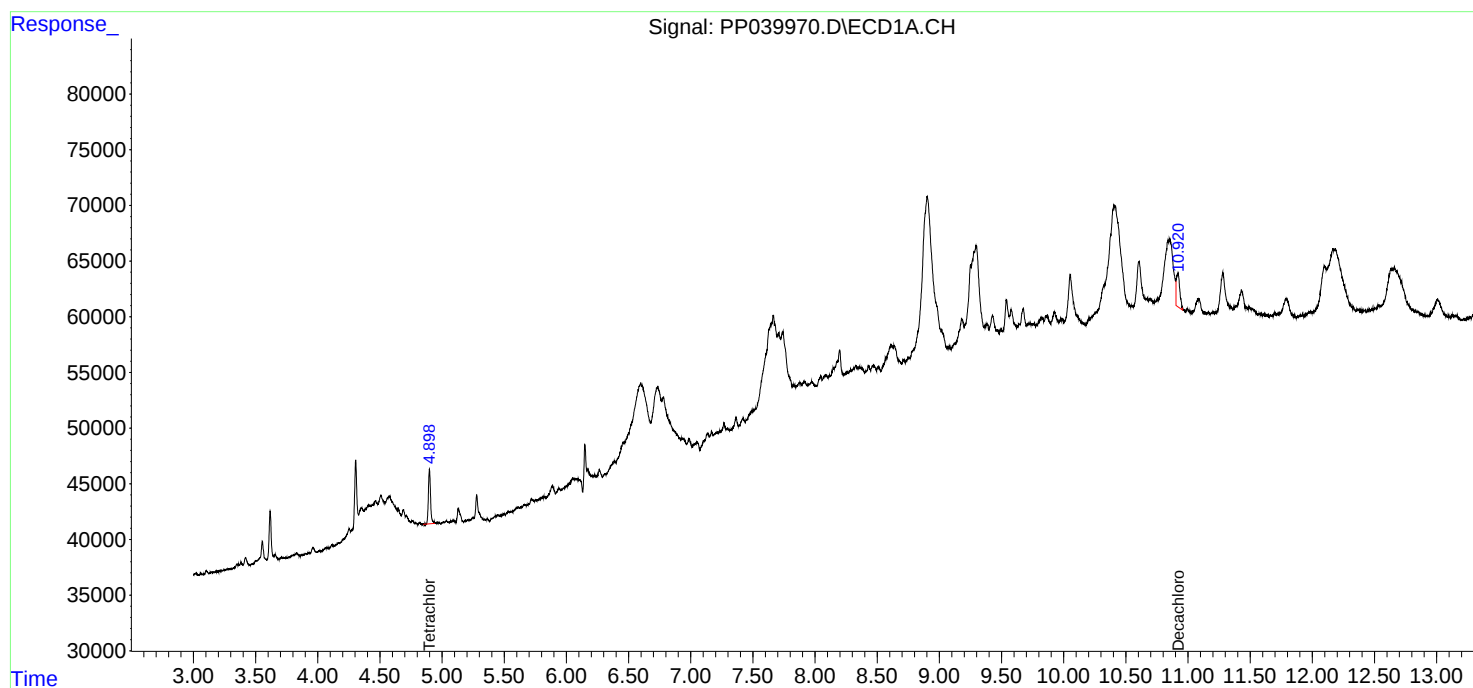

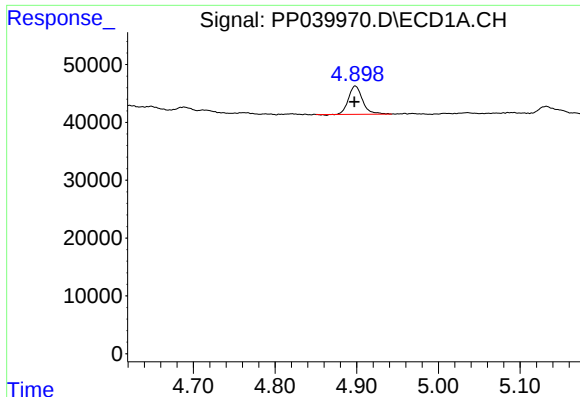


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: 0.001 min
Response: 58398
Conc: 1.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
732910-10-06-21-03


Manual Integrations
APPROVED

mohammad
10/13/2021 1:22:06 PM

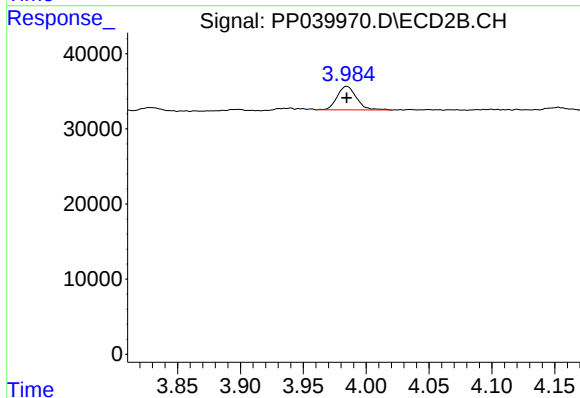


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 33563
Conc: 2.01 ng/ml

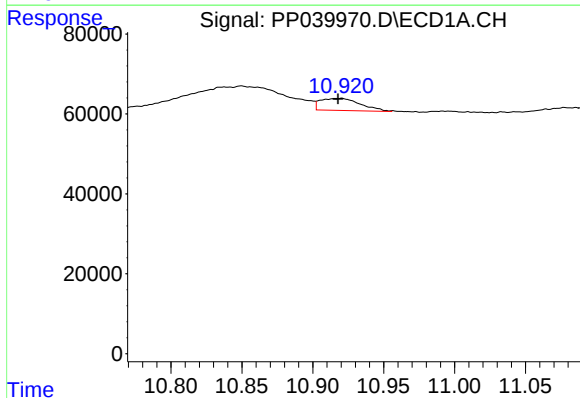

#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: 0.002 min
Response: 58449
Conc: 2.60 ng/ml m

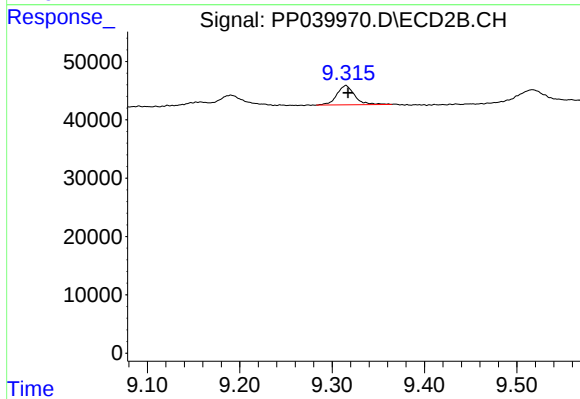

#2 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: -0.002 min
Response: 44207
Conc: 1.97 ng/ml