

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101123\
 Data File : PP060903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 14:01
 Operator : YP\AJ
 Sample : PB156289BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB156289BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/12/2023
 Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 15:43:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.549	3.687	41888757	29462326	18.705	19.793
2) SA Decachlor...	10.507f	8.762	36907379	29978206	20.904m	18.378

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101123\
Data File : PP060903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 14:01
Operator : YP\AJ
Sample : PB156289BL
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB156289BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 15:43:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

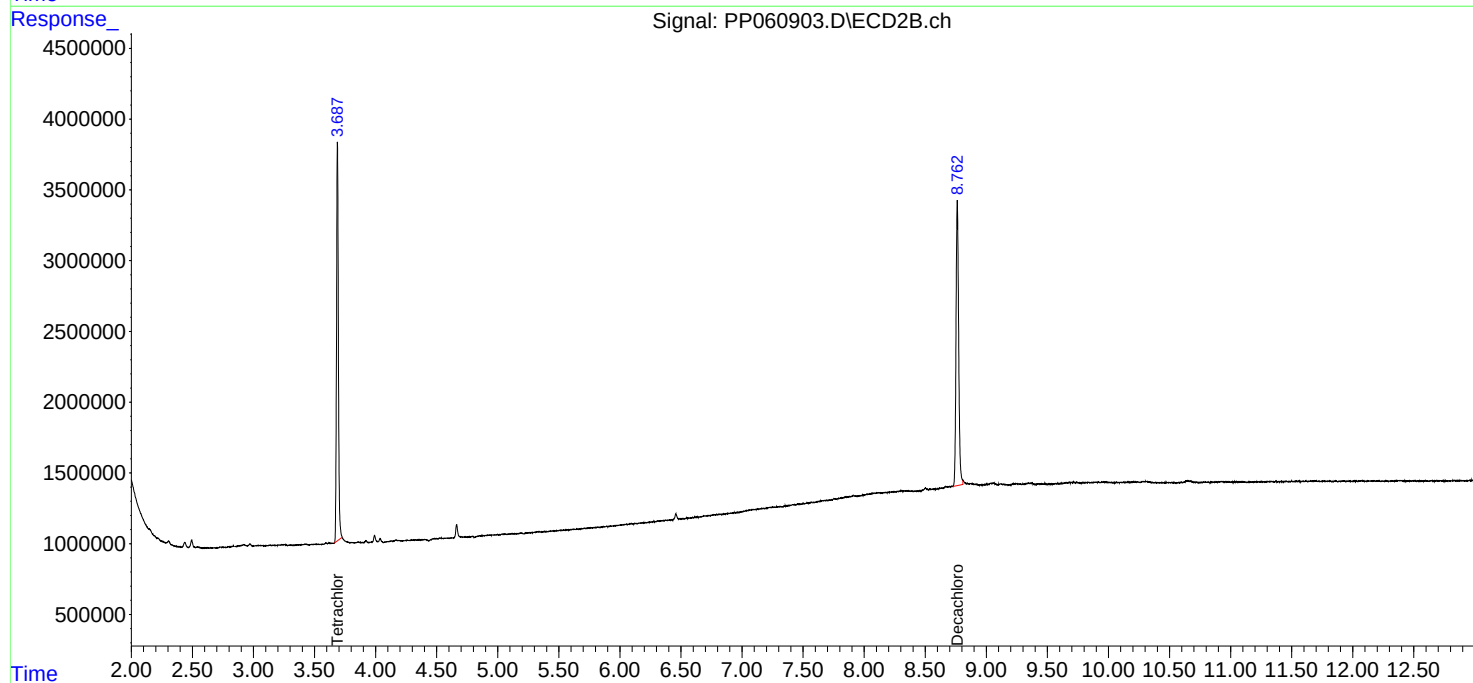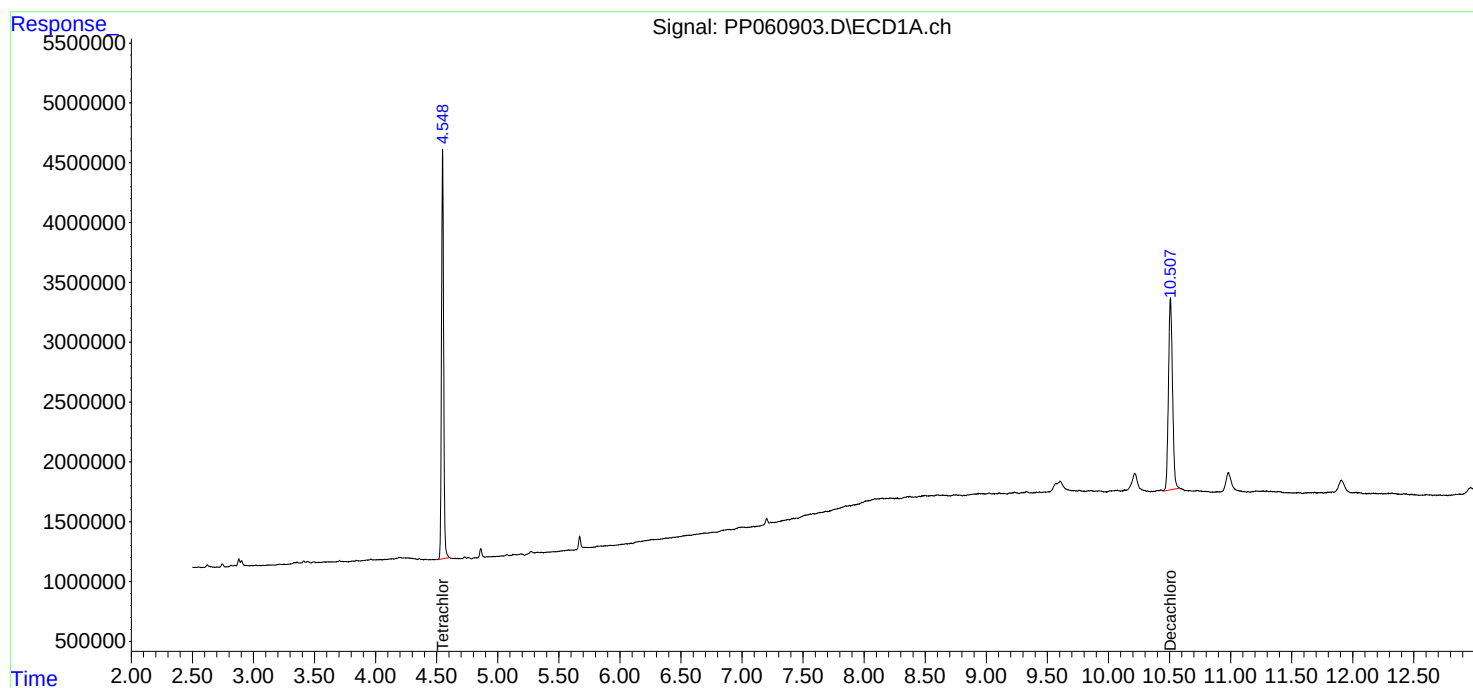

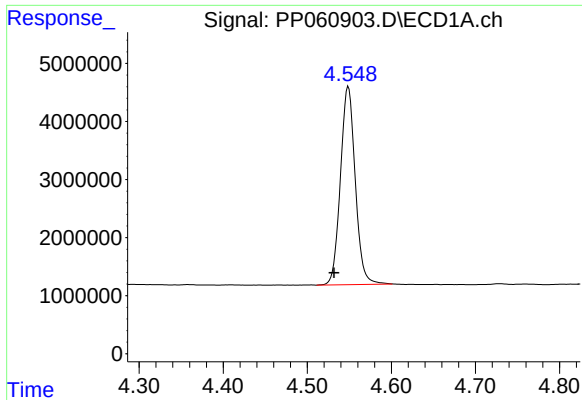


#1 Tetrachloro-m-xylene

R.T.: 4.549 min
Delta R.T.: 0.017 min
Response: 41888757
Conc: 18.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB156289BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

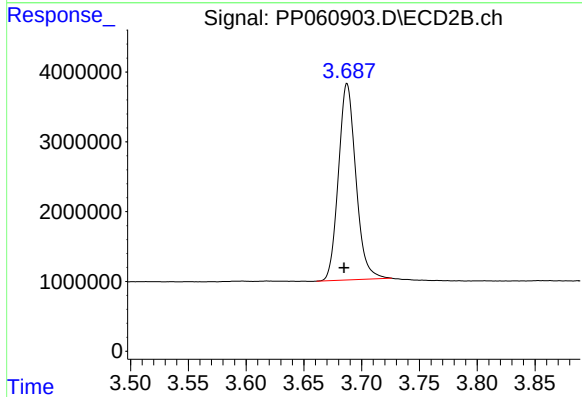


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: 0.003 min
Response: 29462326
Conc: 19.79 ng/ml

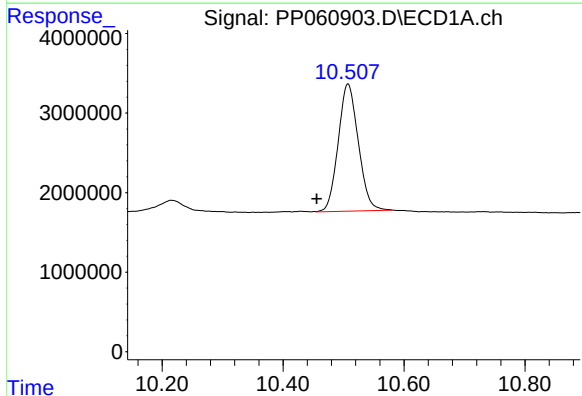

#2 Decachlorobiphenyl

R.T.: 10.507 min
Delta R.T.: 0.051 min
Response: 36907379
Conc: 20.90 ng/ml m

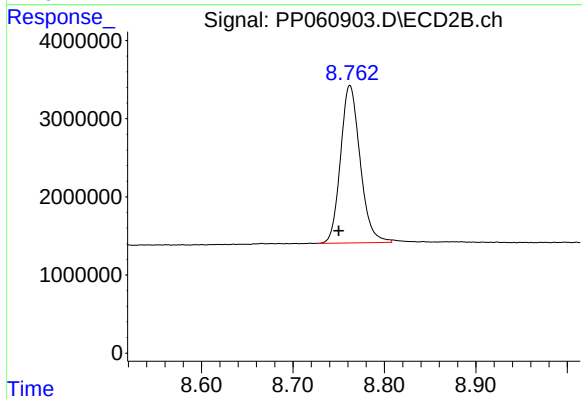

#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.012 min
Response: 29978206
Conc: 18.38 ng/ml