

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101123\
 Data File : PP060934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 23:19
 Operator : YP\AJ
 Sample : 04831-04 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226596-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/12/2023
 Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 00:25:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.536	3.687	3935876	2962816	1.757m	1.990
2) SA Decachlor...	10.480	8.755	3559156	2476538	2.016m	1.518

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101123\
Data File : PP060934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 23:19
Operator : YP\AJ
Sample : 04831-04 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC226596-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 00:25:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

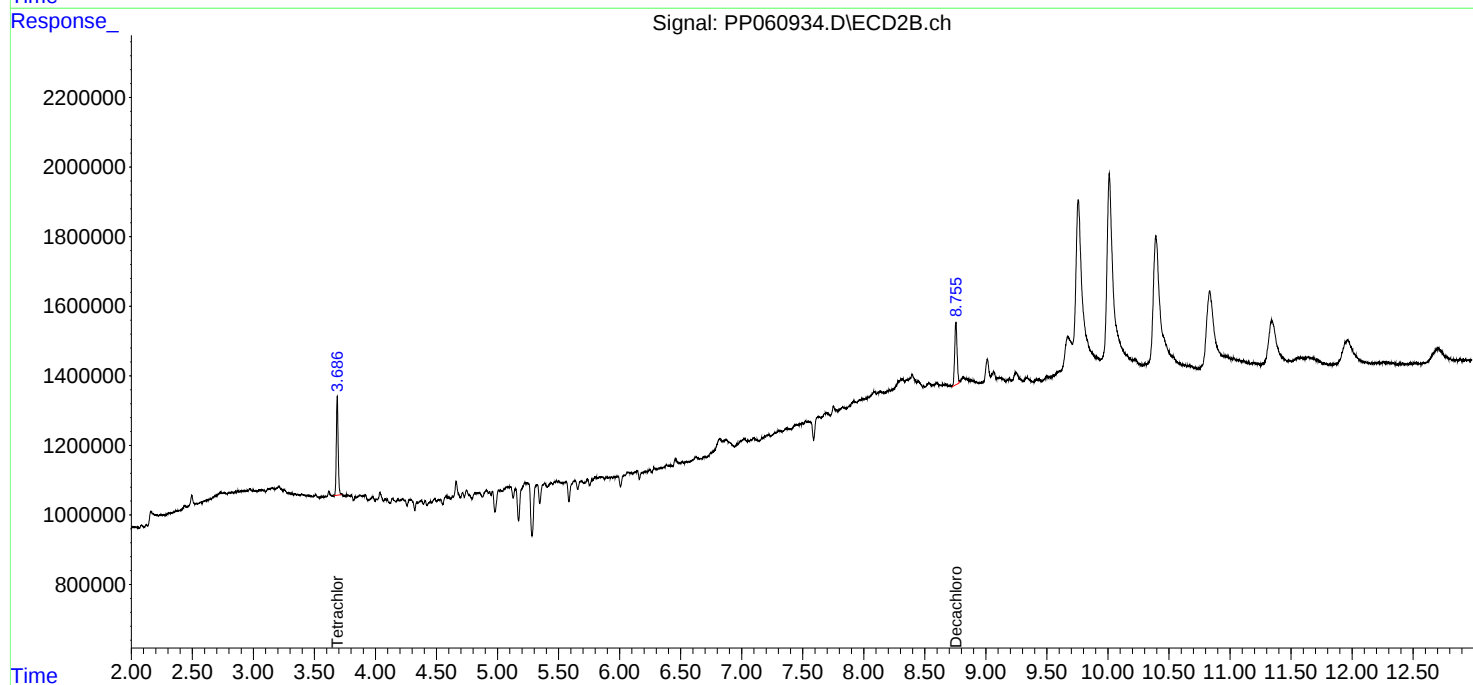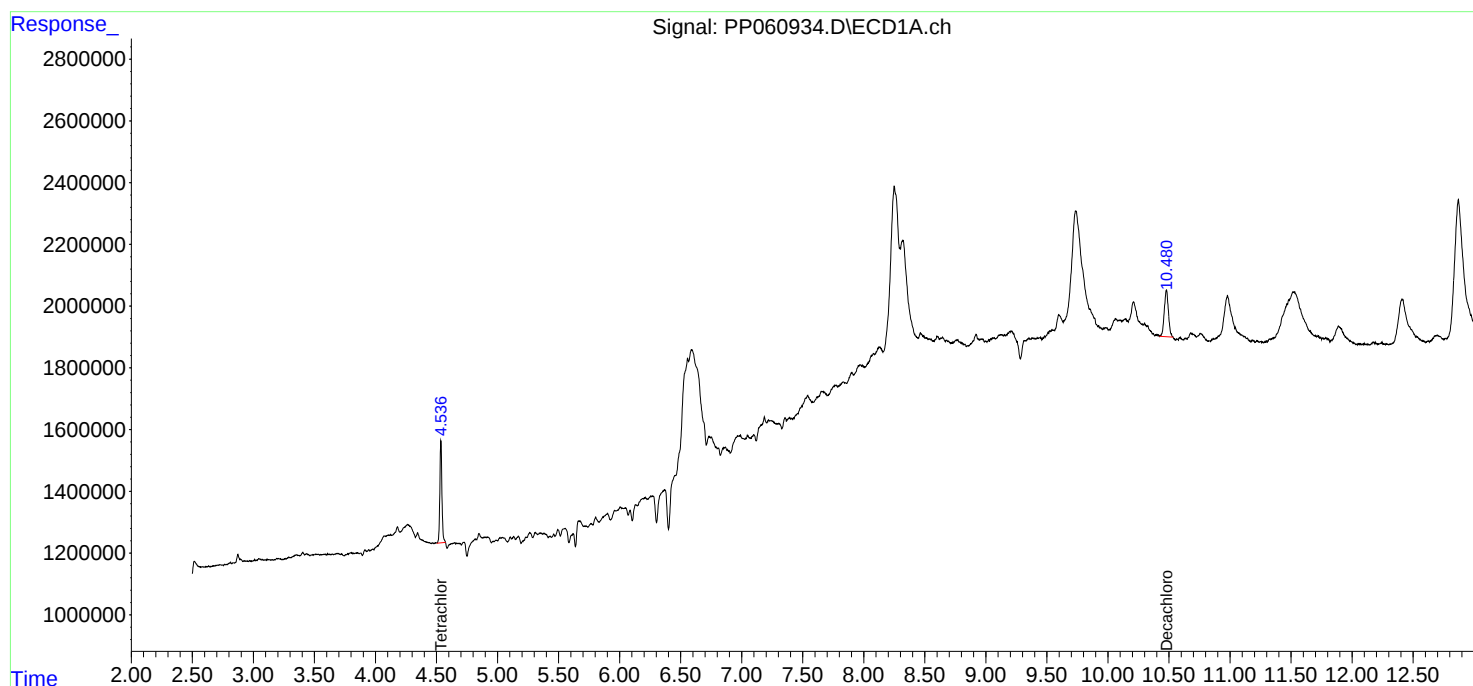

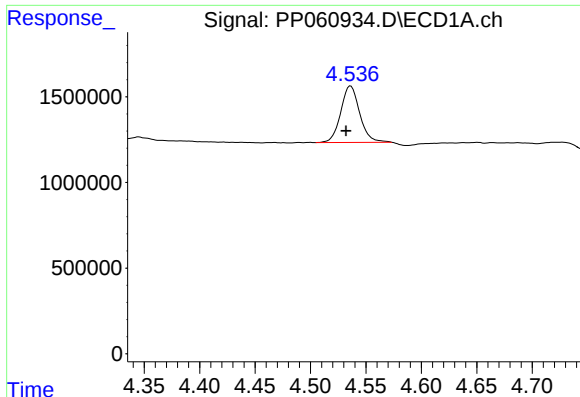


#1 Tetrachloro-m-xylene

R.T.: 4.536 min
Delta R.T.: 0.004 min
Response: 3935876
Conc: 1.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226596-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/12/2023
Supervised By :Ankita Jodhani 10/12/2023

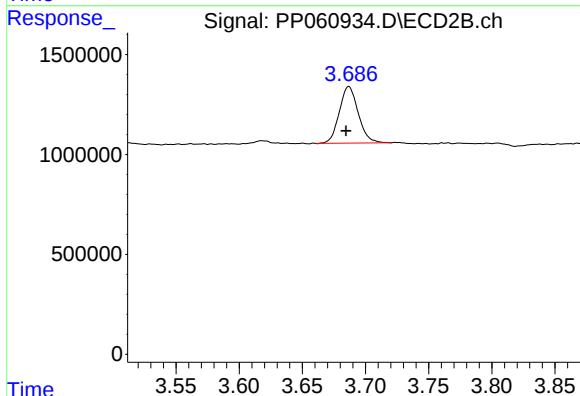


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: 0.002 min
Response: 2962816
Conc: 1.99 ng/ml

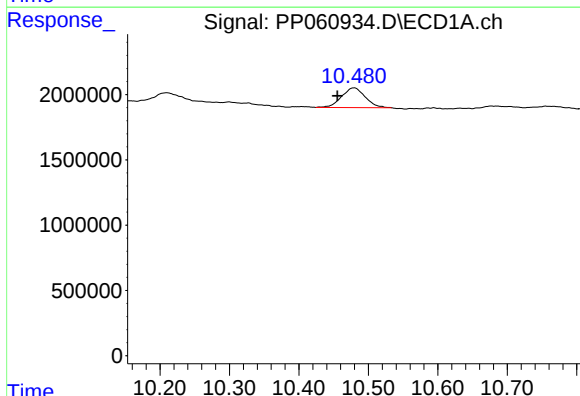

#2 Decachlorobiphenyl

R.T.: 10.480 min
Delta R.T.: 0.024 min
Response: 3559156
Conc: 2.02 ng/ml m

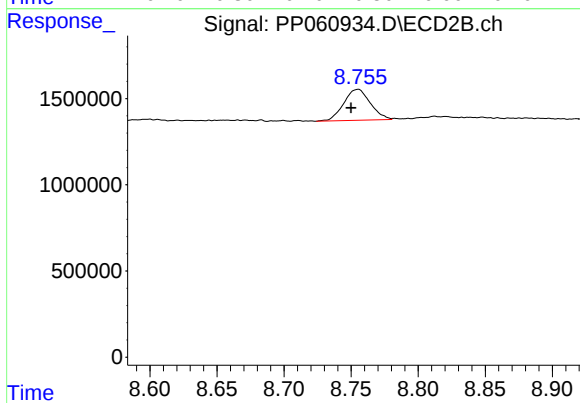

#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: 0.006 min
Response: 2476538
Conc: 1.52 ng/ml