

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:58
 Operator : YP\AJ
 Sample : N5098-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 13:26:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.423	3.674	19696102	14821444	12.530	12.937
2)	SA Decachlor...	10.243	8.769	475.1E6	358.7E6	342.302	321.057
Target Compounds							
3)	L1 AR-1016-1	5.598	4.777	2801745	4801826	61.612	107.964 #
4)	L1 AR-1016-2	5.621	4.795	7542005	4278146	114.564	67.232 #
5)	L1 AR-1016-3	5.683	4.976	4105499	3303026	98.654	99.368
6)	L1 AR-1016-4	5.782	5.017	4165621	6083973	114.646	223.222 #
7)	L1 AR-1016-5	6.079	5.235	7751138	5410404	181.603	152.926
8)	L2 AR-1221-1	4.631	3.895	1559517	2545981	75.469	162.833 #
9)	L2 AR-1221-2	4.717	3.963f	1386002	2767924	90.569	230.799 #
10)	L2 AR-1221-3	4.796	4.055	2380323	2041901	50.837	54.026
11)	L3 AR-1232-1	4.796	4.055	2380323	2041901	66.071	70.454
12)	L3 AR-1232-2	5.329	4.795	4947696	4278146	243.852	142.819 #
13)	L3 AR-1232-3	5.621	4.976	7542005	3303026	250.432	216.203
14)	L3 AR-1232-4	5.782	5.061	4165621	5445511	249.772	384.555 #
15)	L3 AR-1232-5	5.873	5.235	6919523	5410404	461.372	341.776 #
16)	L4 AR-1242-1	5.598	4.777	2801745	4801826	80.544	137.911 #
17)	L4 AR-1242-2	5.621	4.795	7542005	4278146	152.344	86.722 #
18)	L4 AR-1242-3	5.683	4.976	4105499	3303026	129.481	126.534
19)	L4 AR-1242-4	5.782	5.061	4165621	5445511	152.500	200.202 #
20)	L4 AR-1242-5	6.525	5.593	10875063	20076228	292.516	595.732 #
21)	L5 AR-1248-1	5.598	4.777	2801745	4801826	104.221	177.114 #
22)	L5 AR-1248-2	5.873	5.017	6919523	6083973	148.863	163.528
23)	L5 AR-1248-3	6.079	5.061	7751138	5445511	139.983	142.940
24)	L5 AR-1248-4	6.483	5.235	7514804	5410404	118.357	116.767
25)	L5 AR-1248-5	6.525	5.634	10875063	3961811	175.588	94.209 #
26)	L6 AR-1254-1	6.458	5.593	26705125	20076228	375.127	286.957
27)	L6 AR-1254-2	6.677	5.742	40684574	24411347	381.471	389.617
28)	L6 AR-1254-3	7.047	6.133f	22406738	20865657	213.195	210.935
29)	L6 AR-1254-4	7.331	6.381	22989386	10475528	314.628	175.243 #
30)	L6 AR-1254-5	7.743	6.805	335.4E6	134.0E6	4041.769	1511.036 #
31)	L7 AR-1260-1	7.211	6.284	243.0E6	187.0E6	2931.854	2714.239
32)	L7 AR-1260-2	7.468	6.473	511.5E6	423.7E6	5418.958	5118.637
33)	L7 AR-1260-3	7.830	6.634	2437.1E6	453.7E6	40578.506	5876.101 #
34)	L7 AR-1260-4	8.058	7.105	846.9E6	1455.6E6	11043.078	25893.435 #
35)	L7 AR-1260-5	8.380	7.349	3260.6E6	2759.9E6	23786.417	20927.851
36)	L8 AR-1262-1	7.830	6.897	2437.1E6	632.0E6	25134.080	17569.136 #
37)	L8 AR-1262-2	8.380	7.105	3260.6E6	1455.6E6	20250.971	18382.379
38)	L8 AR-1262-3	8.697	7.636	4984.1E6	3793.9E6	45351.320	61437.264 #
39)	L8 AR-1262-4	8.793	7.701	5759.3E6	4477.8E6	112665.750	39222.534 #
40)	L8 AR-1262-5	9.463	8.202	3649.3E6	2735.9E6	57972.219	53826.843
41)	L9 AR-1268-1	8.697	7.636	4984.1E6	3793.9E6	25174.909	20913.270

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 12:58
 Operator : YP\AJ
 Sample : N5098-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 13:26:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.793	7.701	5759.3E6	4477.8E6	31365.077	27405.931
43) L9	AR-1268-3	9.027	7.910	1319.6E6	1038.6E6	8095.221	7386.085
44) L9	AR-1268-4	9.463	8.202	3649.3E6	2735.9E6	50016.428	48414.068
45) L9	AR-1268-5	9.891	8.503	6302.3E6	4479.9E6	12086.312	10649.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 12:58
Operator : YP\AJ
Sample : N5098-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 13:26:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

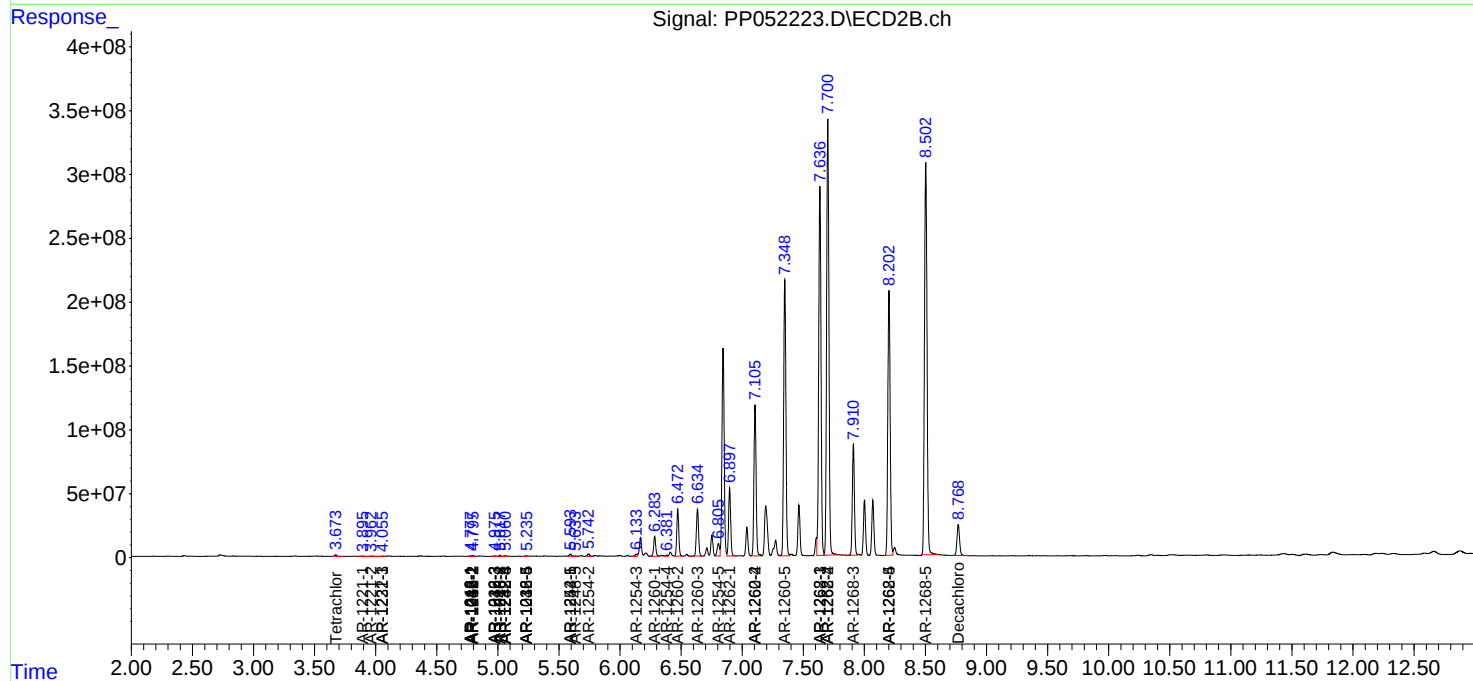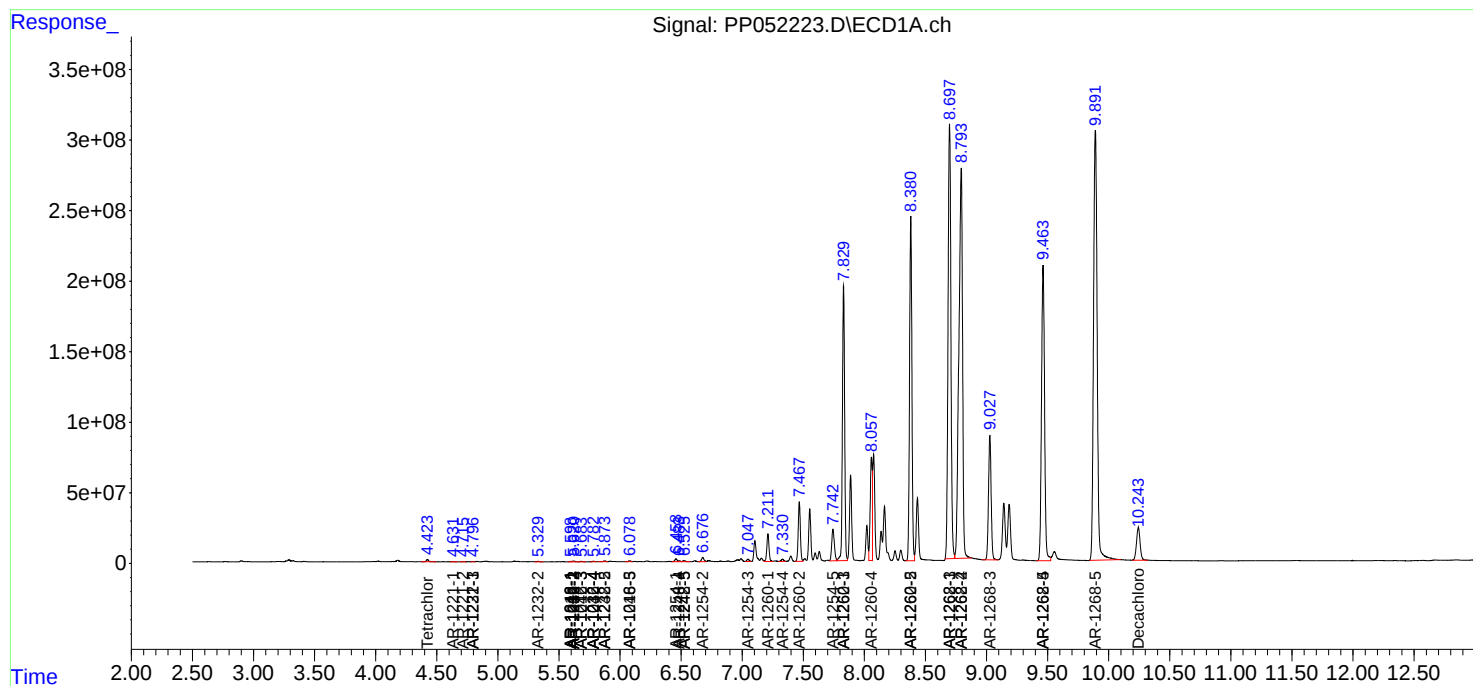


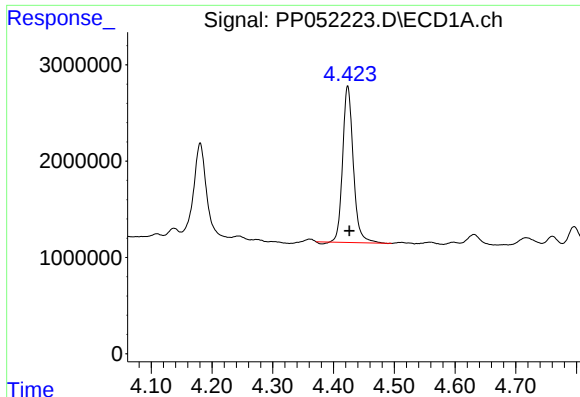

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 19696102
Conc: 12.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

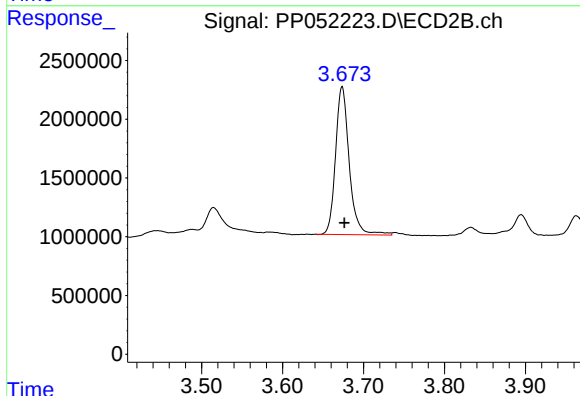


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 14821444
Conc: 12.94 ng/ml

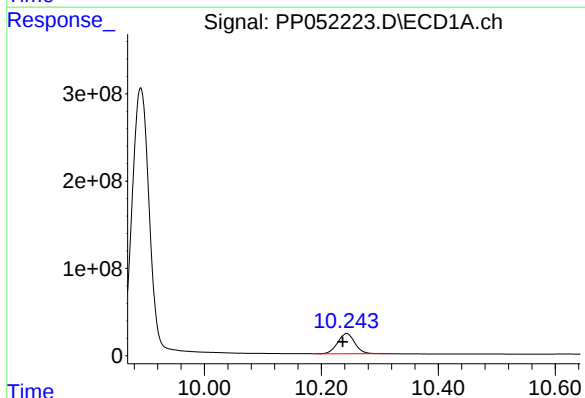


#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: 0.007 min
Response: 475061756
Conc: 342.30 ng/ml

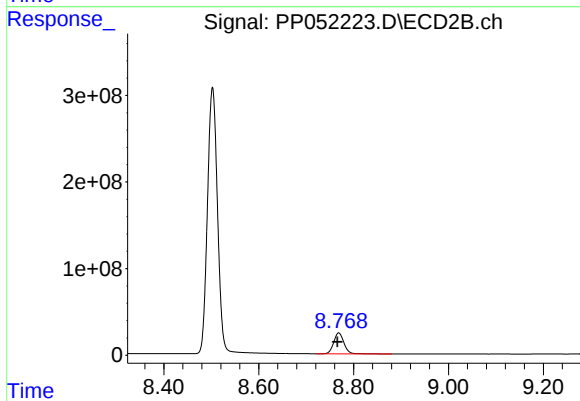

#2 Decachlorobiphenyl


R.T.: 8.769 min
Delta R.T.: 0.003 min
Response: 358736684
Conc: 321.06 ng/ml

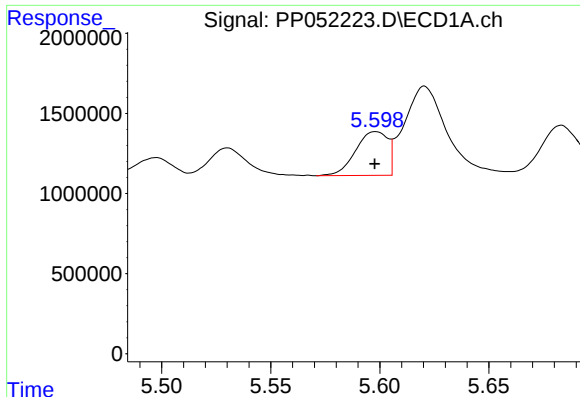

#3 AR-1016-1


R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 2801745
Conc: 61.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

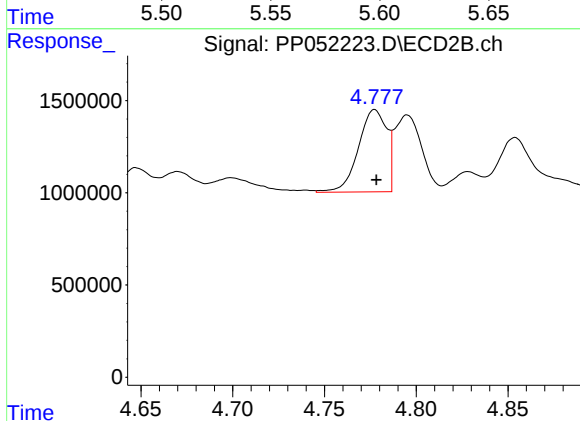


#3 AR-1016-1

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 4801826
Conc: 107.96 ng/ml

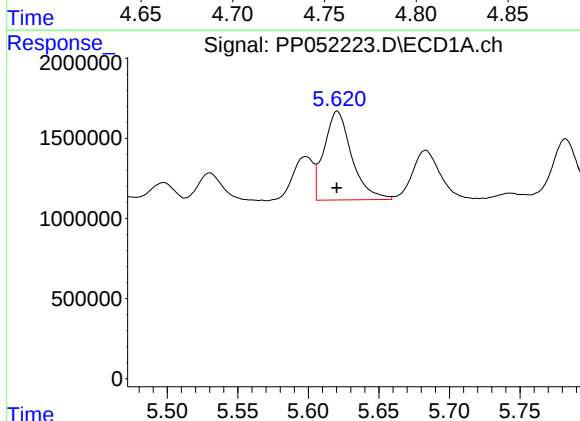


#4 AR-1016-2

R.T.: 5.621 min
Delta R.T.: 0.000 min
Response: 7542005
Conc: 114.56 ng/ml

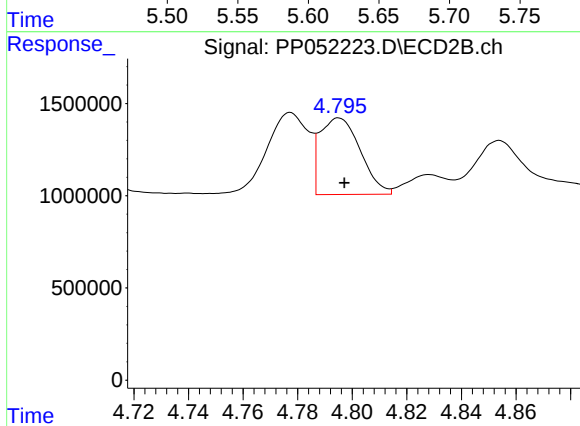

#4 AR-1016-2


R.T.: 4.795 min
Delta R.T.: -0.002 min
Response: 4278146
Conc: 67.23 ng/ml

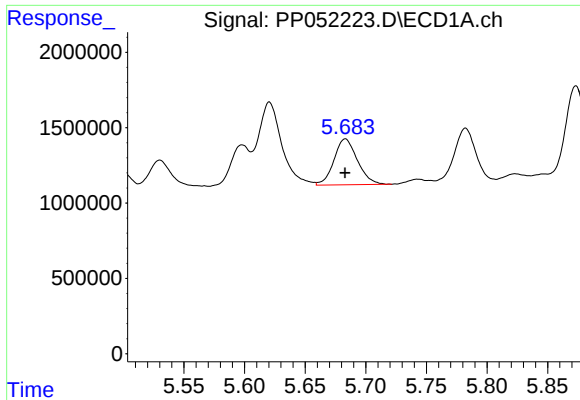

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: 0.000 min
Response: 4105499
Conc: 98.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

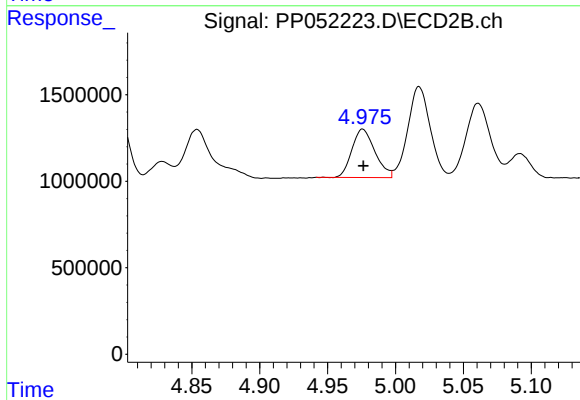


#5 AR-1016-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 3303026
Conc: 99.37 ng/ml

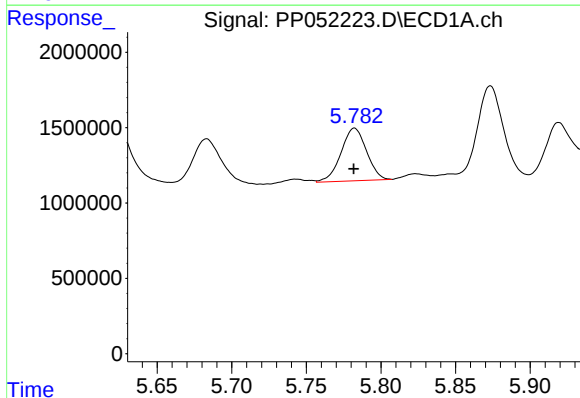


#6 AR-1016-4

R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 4165621
Conc: 114.65 ng/ml

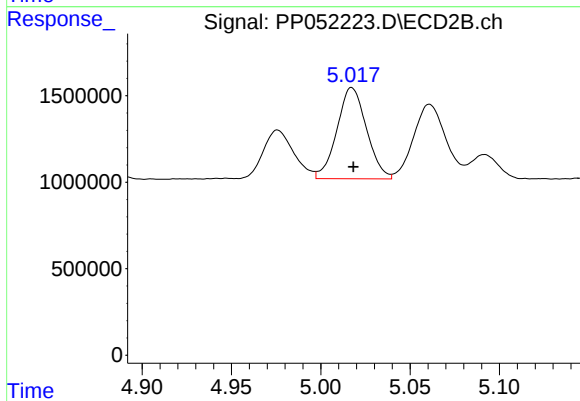

#6 AR-1016-4


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 6083973
Conc: 223.22 ng/ml

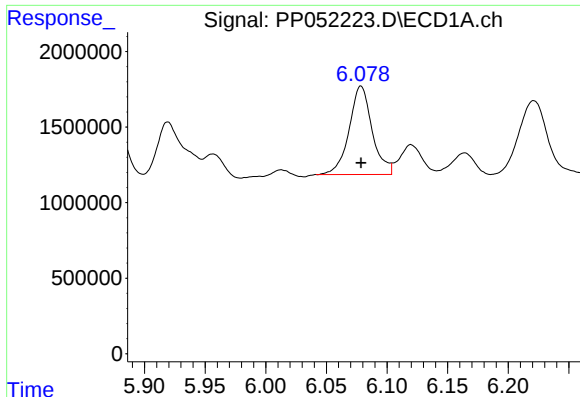

#7 AR-1016-5


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 7751138
Conc: 181.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

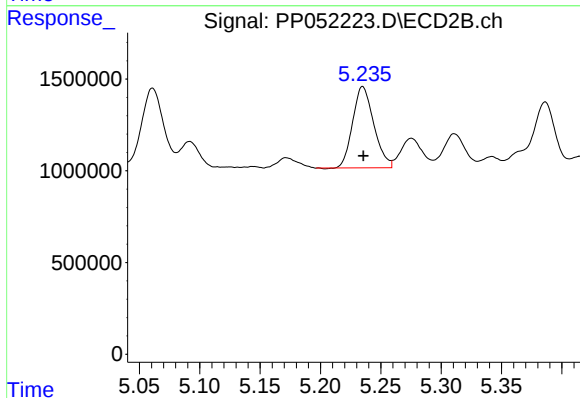


#7 AR-1016-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 5410404
Conc: 152.93 ng/ml

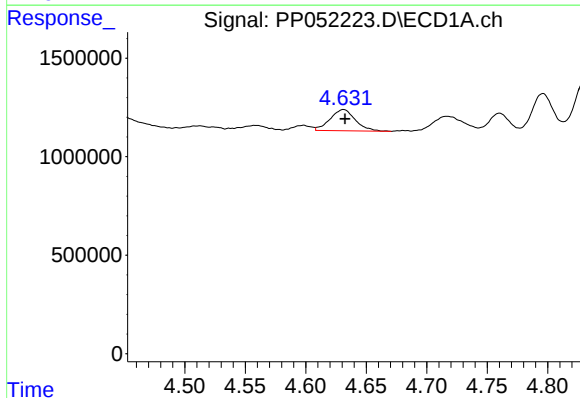


#8 AR-1221-1

R.T.: 4.631 min
Delta R.T.: -0.001 min
Response: 1559517
Conc: 75.47 ng/ml

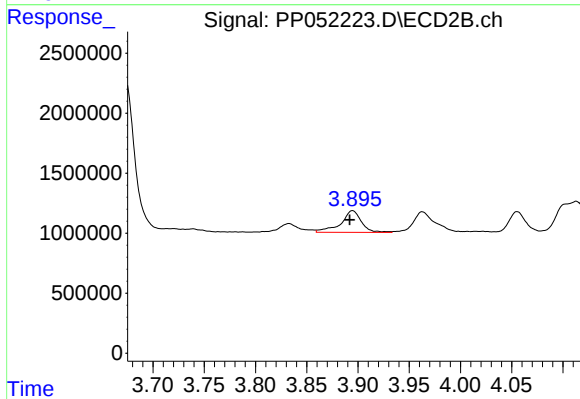

#8 AR-1221-1


R.T.: 3.895 min
Delta R.T.: 0.003 min
Response: 2545981
Conc: 162.83 ng/ml

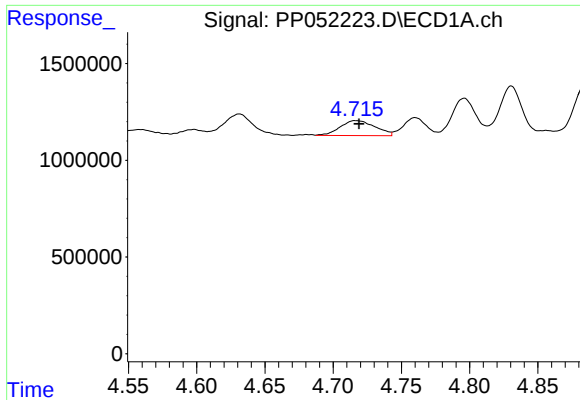

#9 AR-1221-2


R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 1386002
Conc: 90.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

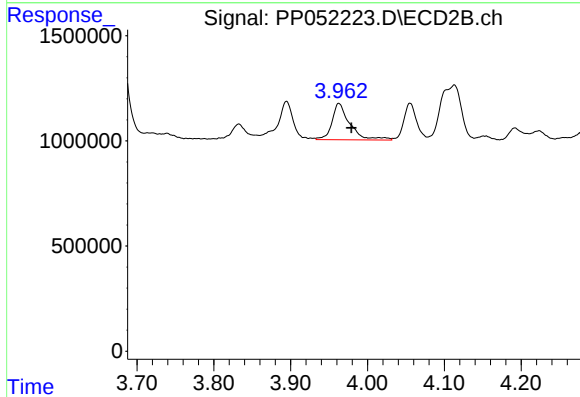


#9 AR-1221-2

R.T.: 3.963 min
Delta R.T.: -0.016 min
Response: 2767924
Conc: 230.80 ng/ml

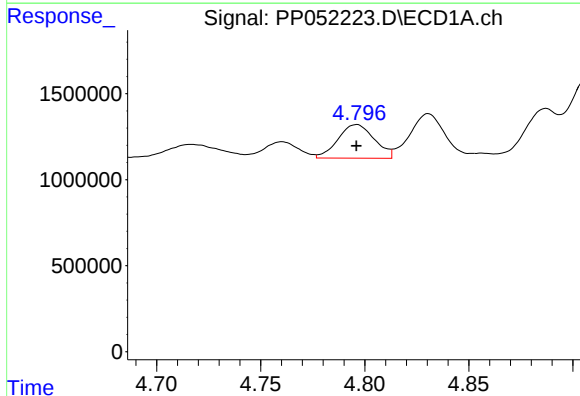


#10 AR-1221-3

R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 2380323
Conc: 50.84 ng/ml

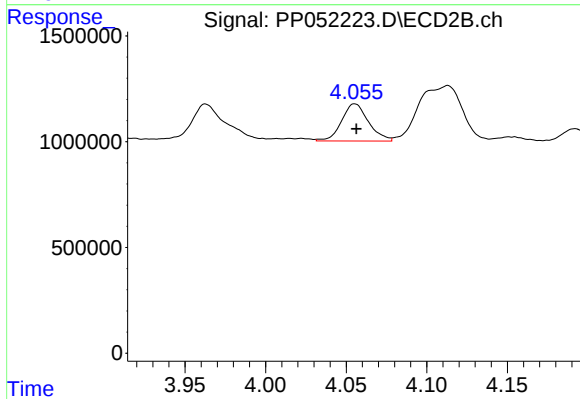

#10 AR-1221-3


R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 2041901
Conc: 54.03 ng/ml

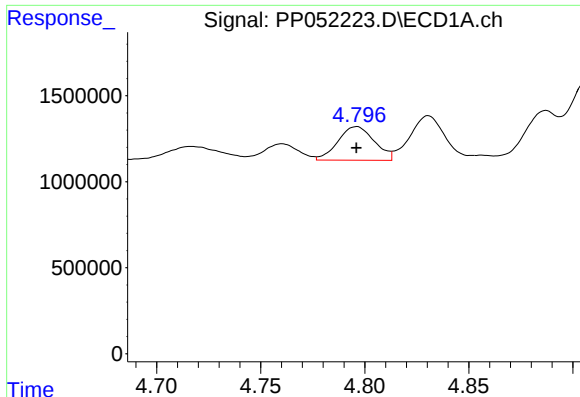

#11 AR-1232-1


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 2380323
Conc: 66.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

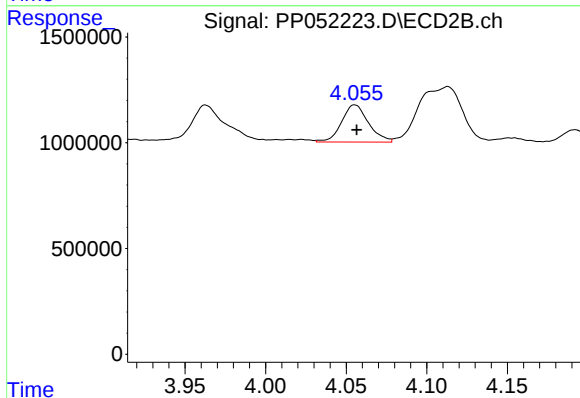


#11 AR-1232-1

R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 2041901
Conc: 70.45 ng/ml

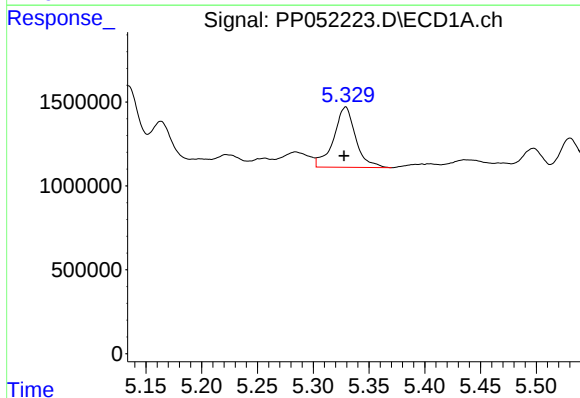


#12 AR-1232-2

R.T.: 5.329 min
Delta R.T.: 0.001 min
Response: 4947696
Conc: 243.85 ng/ml

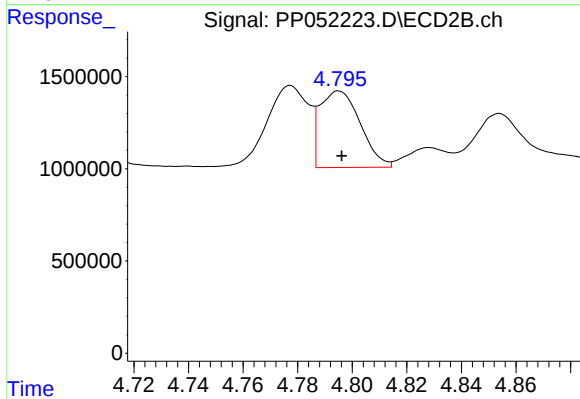

#12 AR-1232-2


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 4278146
Conc: 142.82 ng/ml

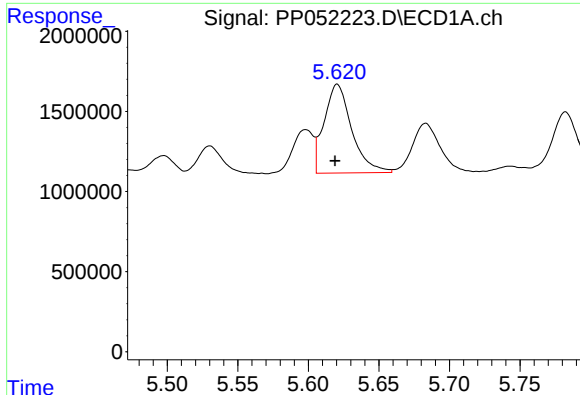

#13 AR-1232-3


R.T.: 5.621 min
Delta R.T.: 0.002 min
Response: 7542005
Conc: 250.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

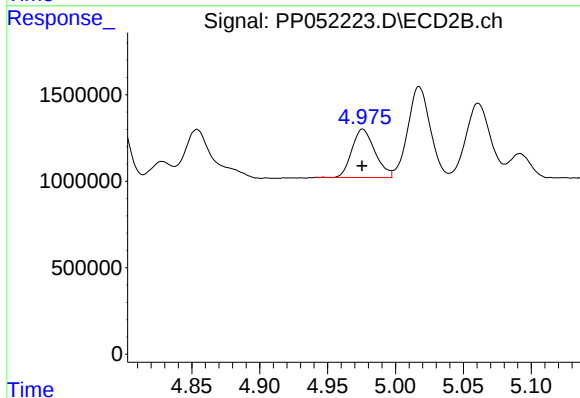


#13 AR-1232-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 3303026
Conc: 216.20 ng/ml

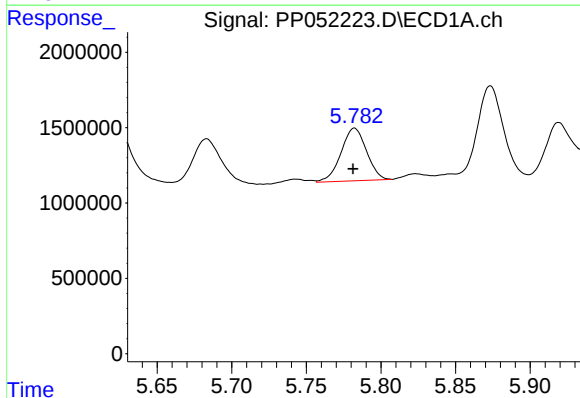


#14 AR-1232-4

R.T.: 5.782 min
Delta R.T.: 0.001 min
Response: 4165621
Conc: 249.77 ng/ml

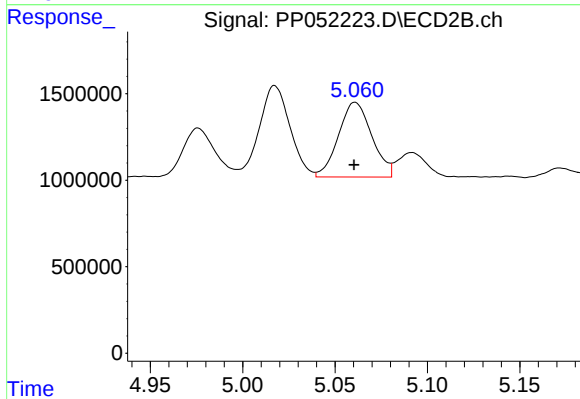

#14 AR-1232-4


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 5445511
Conc: 384.56 ng/ml

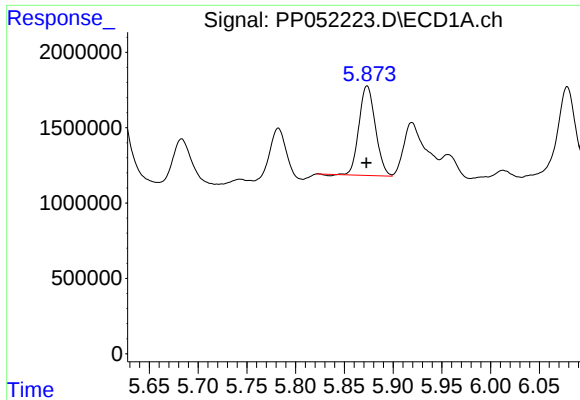

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: 0.000 min
Response: 6919523
Conc: 461.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

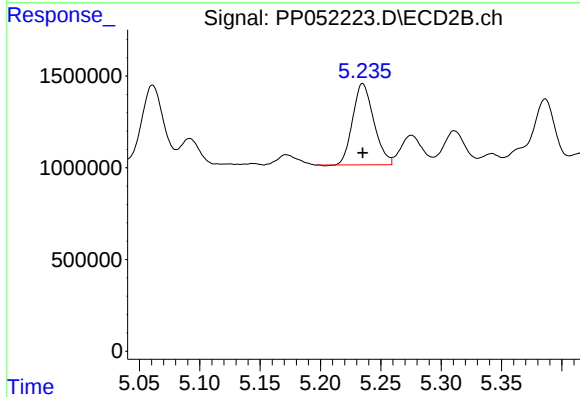


#15 AR-1232-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 5410404
Conc: 341.78 ng/ml

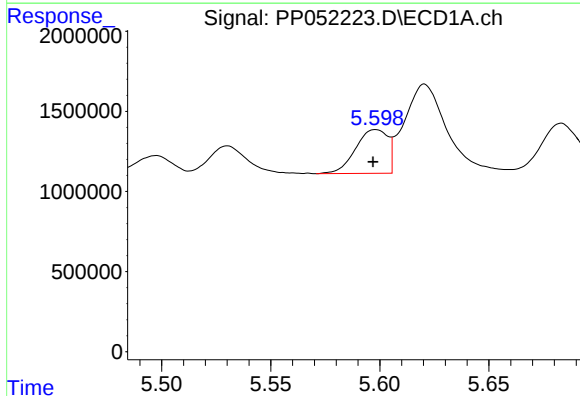


#16 AR-1242-1

R.T.: 5.598 min
Delta R.T.: 0.001 min
Response: 2801745
Conc: 80.54 ng/ml

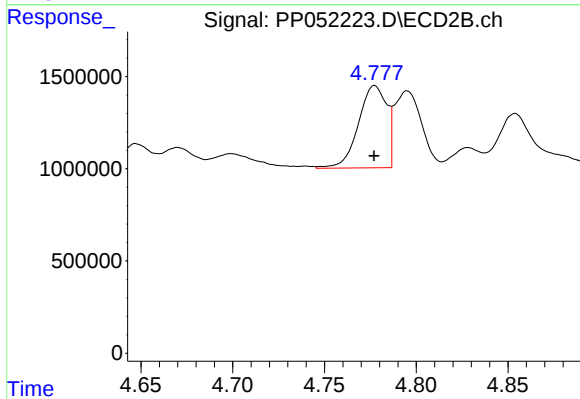

#16 AR-1242-1


R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 4801826
Conc: 137.91 ng/ml

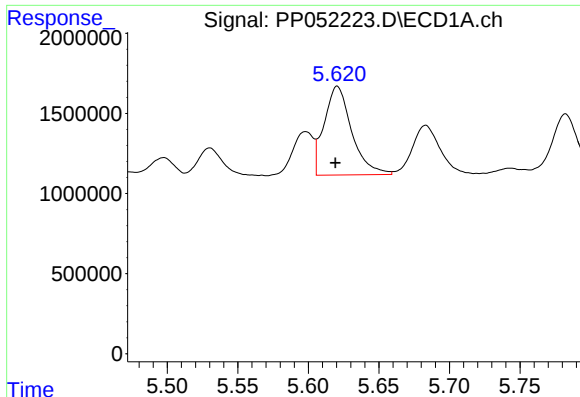

#17 AR-1242-2


R.T.: 5.621 min
Delta R.T.: 0.001 min
Response: 7542005
Conc: 152.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

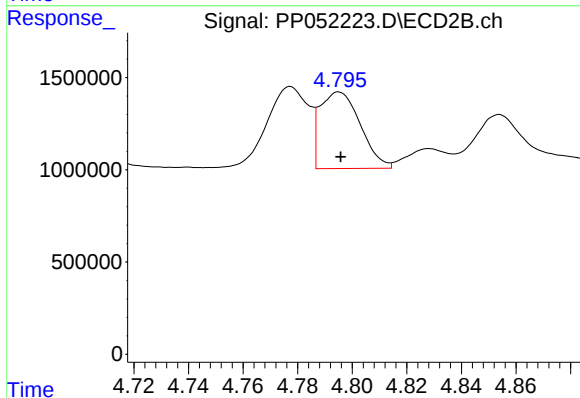


#17 AR-1242-2

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 4278146
Conc: 86.72 ng/ml

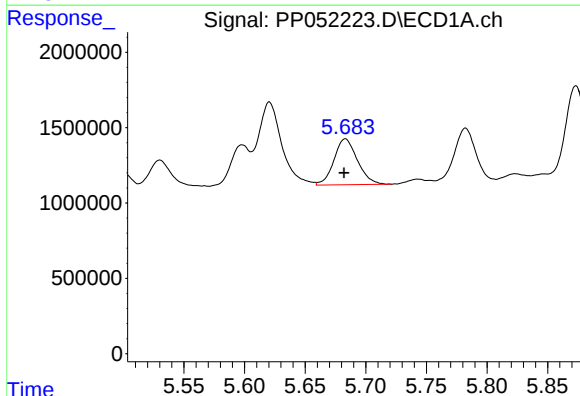


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: 0.001 min
Response: 4105499
Conc: 129.48 ng/ml

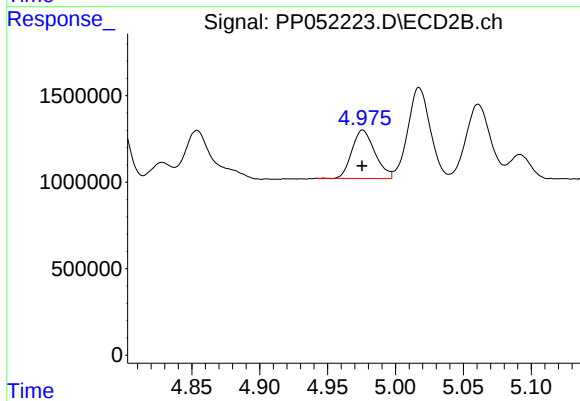

#18 AR-1242-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 3303026
Conc: 126.53 ng/ml

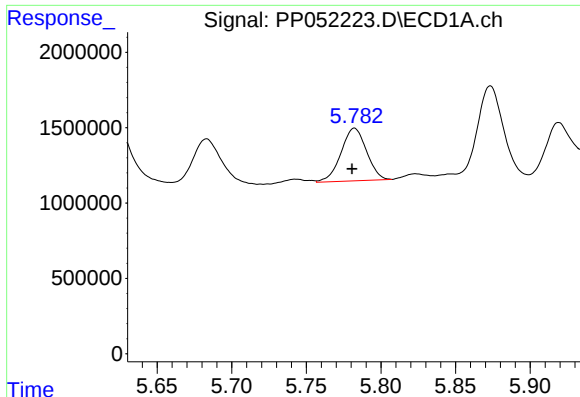

#19 AR-1242-4


R.T.: 5.782 min
Delta R.T.: 0.002 min
Response: 4165621
Conc: 152.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

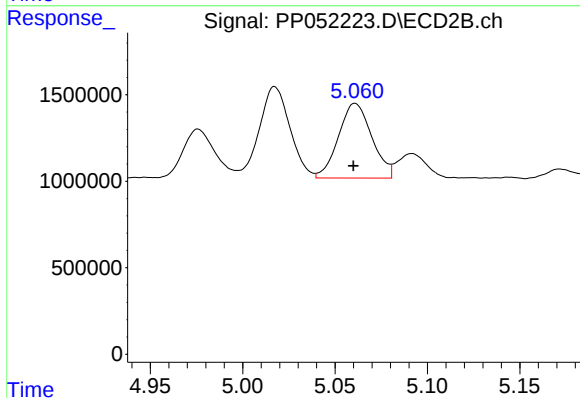


#19 AR-1242-4

R.T.: 5.061 min
Delta R.T.: 0.001 min
Response: 5445511
Conc: 200.20 ng/ml

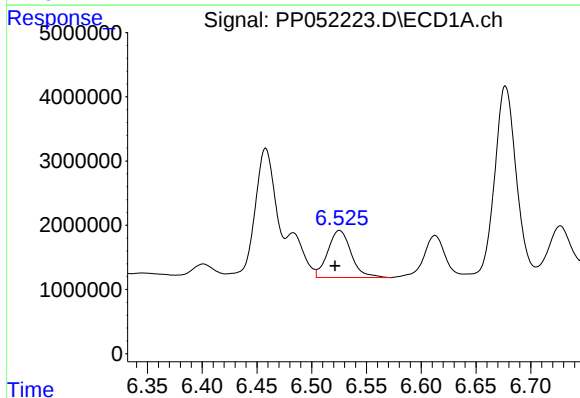


#20 AR-1242-5

R.T.: 6.525 min
Delta R.T.: 0.004 min
Response: 10875063
Conc: 292.52 ng/ml

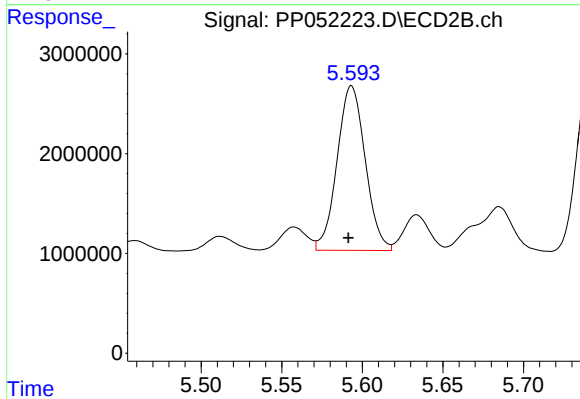

#20 AR-1242-5


R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 20076228
Conc: 595.73 ng/ml

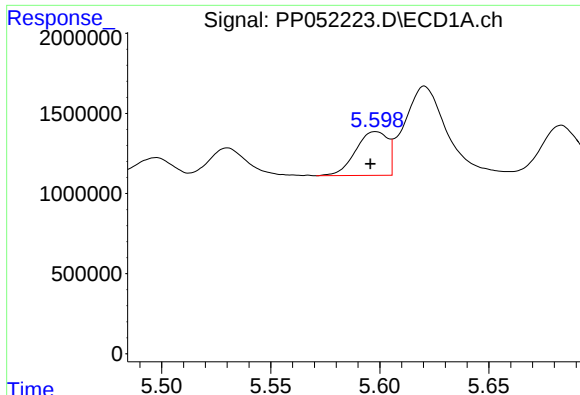

#21 AR-1248-1


R.T.: 5.598 min
Delta R.T.: 0.002 min
Response: 2801745
Conc: 104.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

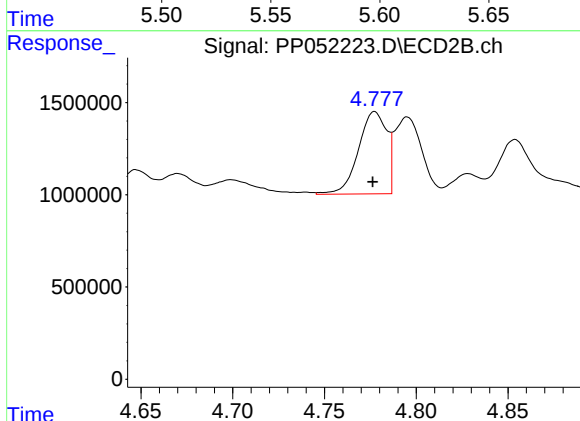


#21 AR-1248-1

R.T.: 4.777 min
Delta R.T.: 0.001 min
Response: 4801826
Conc: 177.11 ng/ml

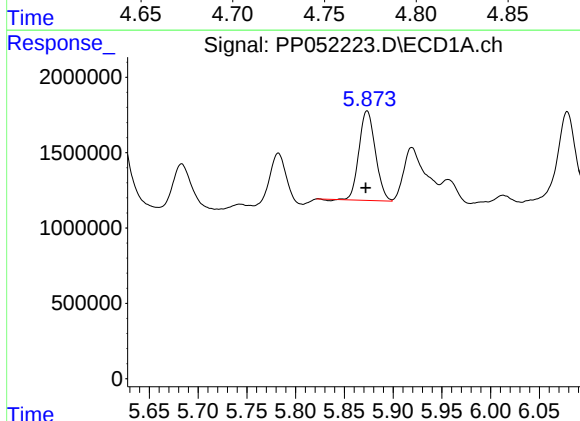


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: 0.002 min
Response: 6919523
Conc: 148.86 ng/ml

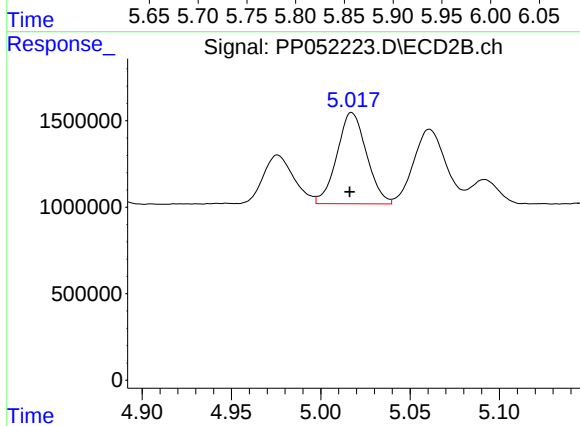

#22 AR-1248-2


R.T.: 5.017 min
Delta R.T.: 0.001 min
Response: 6083973
Conc: 163.53 ng/ml

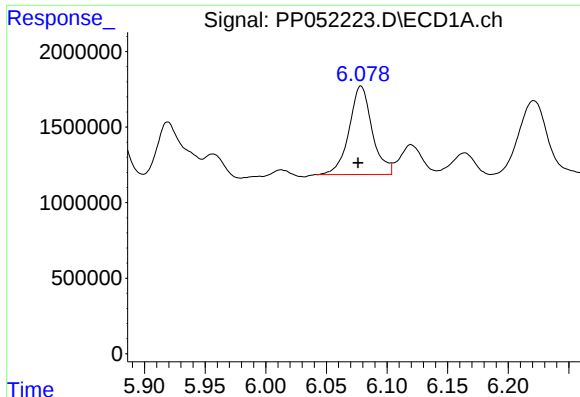

#23 AR-1248-3


R.T.: 6.079 min
Delta R.T.: 0.002 min
Response: 7751138
Conc: 139.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

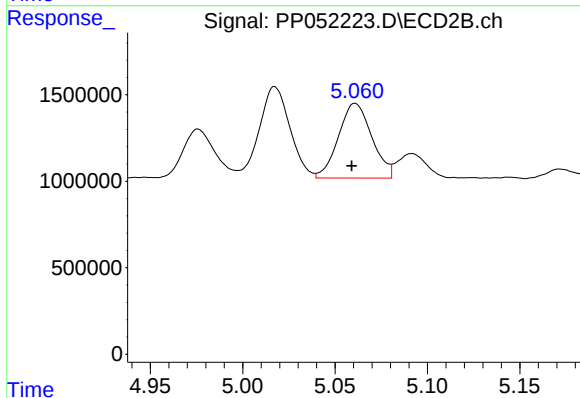


#23 AR-1248-3

R.T.: 5.061 min
Delta R.T.: 0.002 min
Response: 5445511
Conc: 142.94 ng/ml

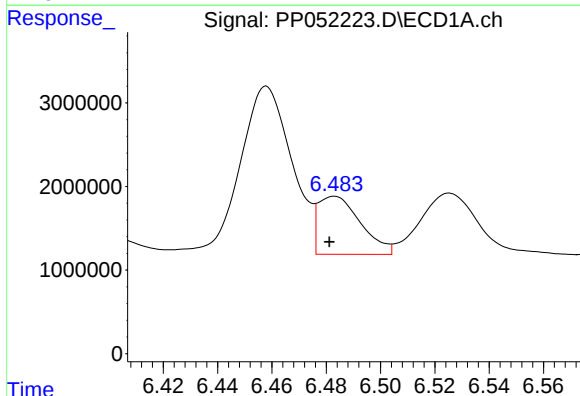


#24 AR-1248-4

R.T.: 6.483 min
Delta R.T.: 0.002 min
Response: 7514804
Conc: 118.36 ng/ml

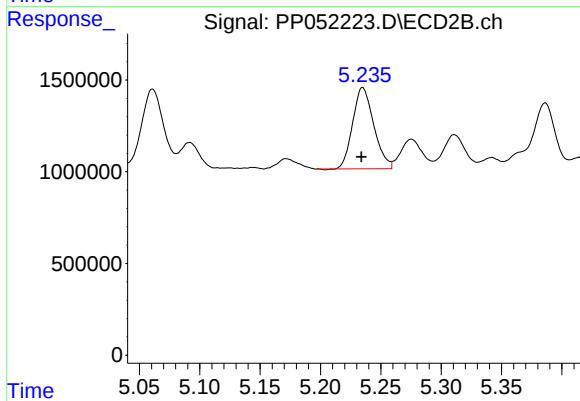

#24 AR-1248-4


R.T.: 5.235 min
Delta R.T.: 0.001 min
Response: 5410404
Conc: 116.77 ng/ml

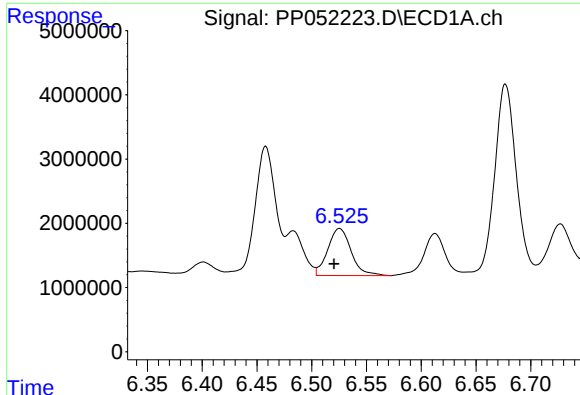

#25 AR-1248-5


R.T.: 6.525 min
Delta R.T.: 0.005 min
Response: 10875063
Conc: 175.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

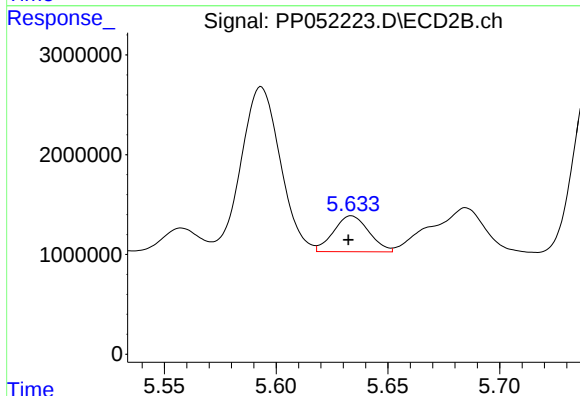


#25 AR-1248-5

R.T.: 5.634 min
Delta R.T.: 0.001 min
Response: 3961811
Conc: 94.21 ng/ml

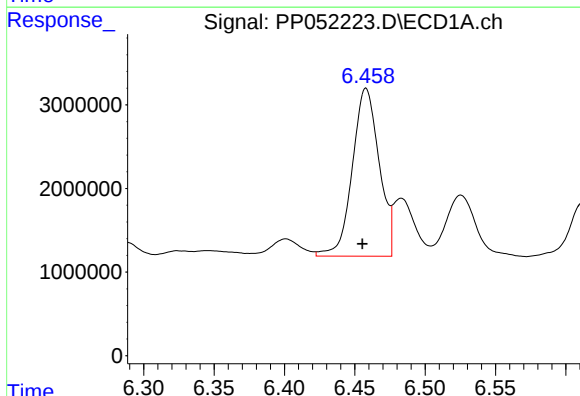


#26 AR-1254-1

R.T.: 6.458 min
Delta R.T.: 0.003 min
Response: 26705125
Conc: 375.13 ng/ml

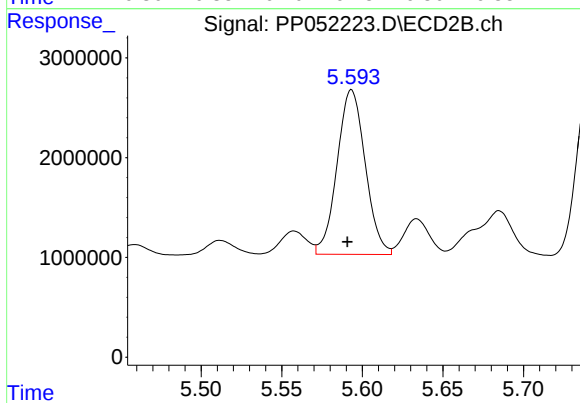

#26 AR-1254-1


R.T.: 5.593 min
Delta R.T.: 0.003 min
Response: 20076228
Conc: 286.96 ng/ml

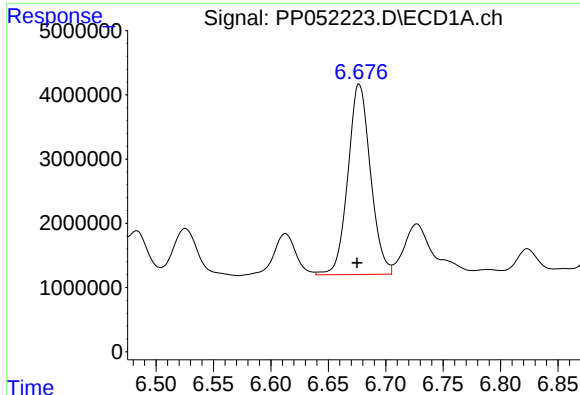

#27 AR-1254-2


R.T.: 6.677 min
Delta R.T.: 0.002 min
Response: 40684574
Conc: 381.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

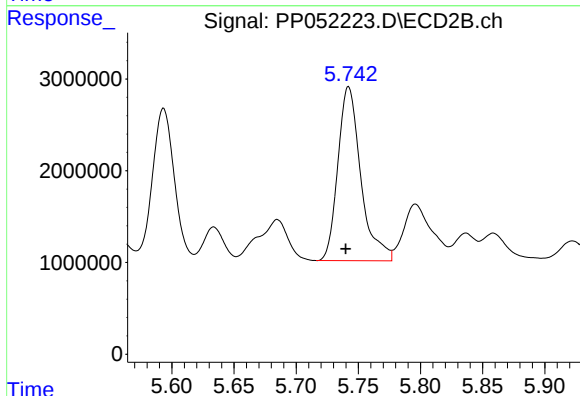


#27 AR-1254-2

R.T.: 5.742 min
Delta R.T.: 0.002 min
Response: 24411347
Conc: 389.62 ng/ml

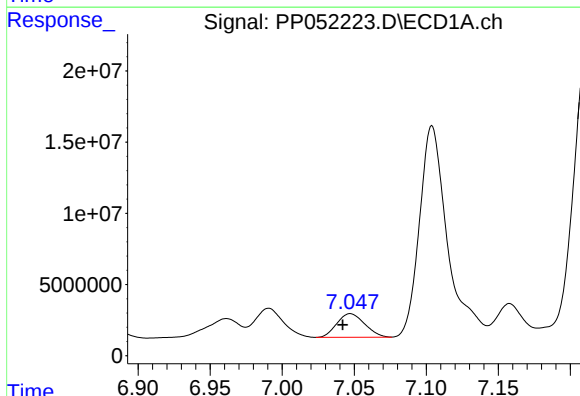


#28 AR-1254-3

R.T.: 7.047 min
Delta R.T.: 0.005 min
Response: 22406738
Conc: 213.19 ng/ml

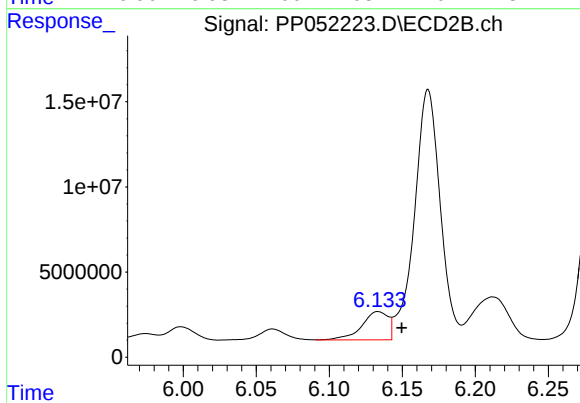

#28 AR-1254-3


R.T.: 6.133 min
Delta R.T.: -0.016 min
Response: 20865657
Conc: 210.94 ng/ml

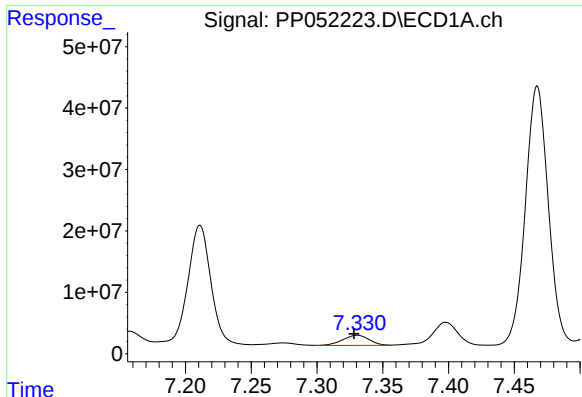

#29 AR-1254-4


R.T.: 7.331 min
Delta R.T.: 0.002 min
Response: 22989386
Conc: 314.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

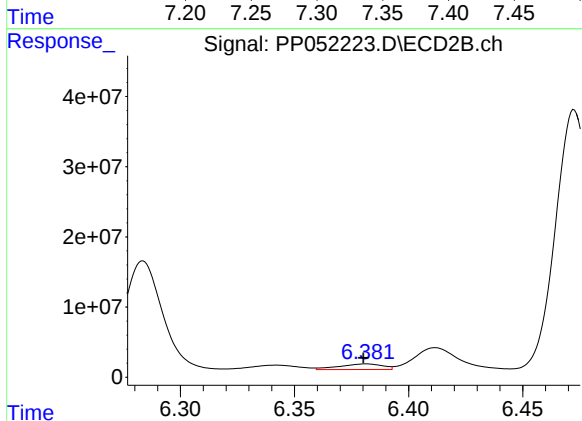


#29 AR-1254-4

R.T.: 6.381 min
Delta R.T.: 0.001 min
Response: 10475528
Conc: 175.24 ng/ml

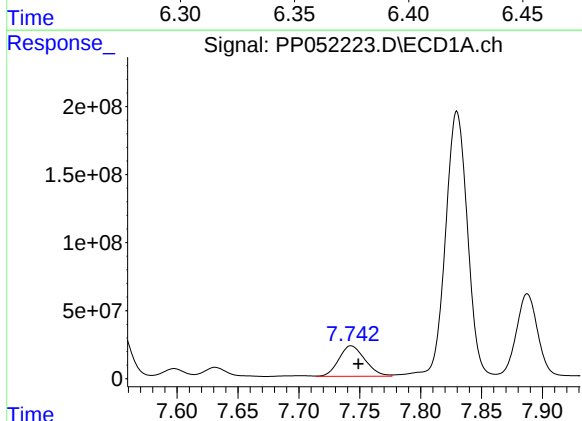


#30 AR-1254-5

R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 335359947
Conc: 4041.77 ng/ml

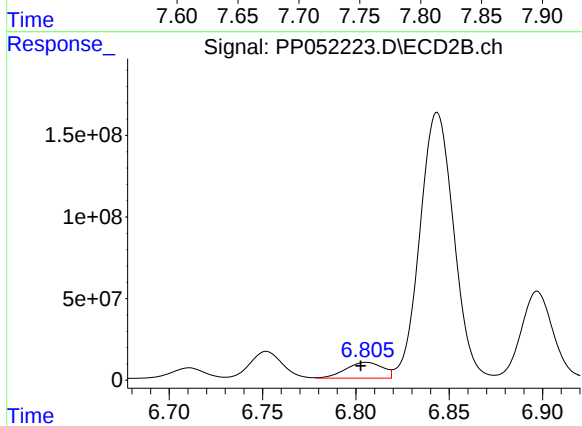

#30 AR-1254-5


R.T.: 6.805 min
Delta R.T.: 0.003 min
Response: 133959708
Conc: 1511.04 ng/ml

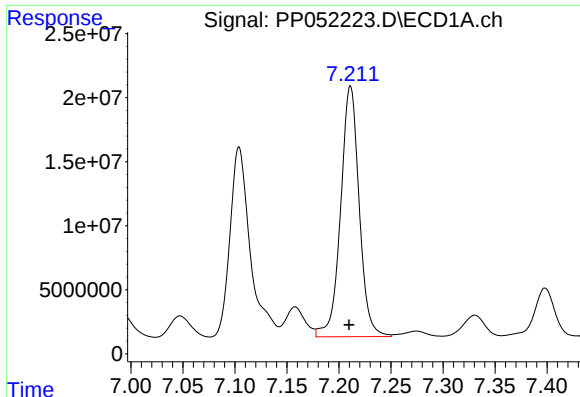

#31 AR-1260-1


R.T.: 7.211 min
Delta R.T.: 0.002 min
Response: 243008989
Conc: 2931.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

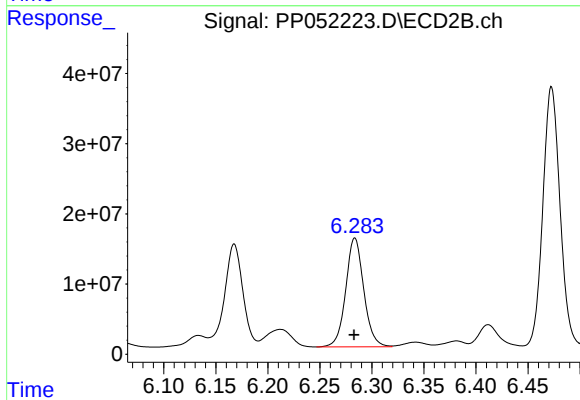


#31 AR-1260-1

R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 186963932
Conc: 2714.24 ng/ml

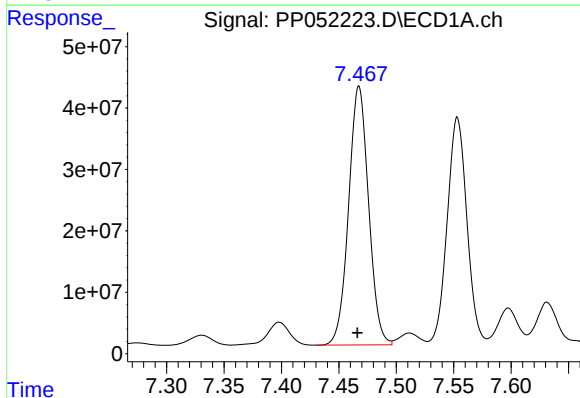


#32 AR-1260-2

R.T.: 7.468 min
Delta R.T.: 0.001 min
Response: 511468289
Conc: 5418.96 ng/ml

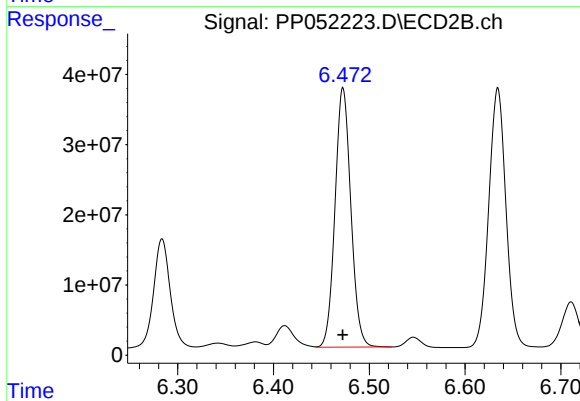

#32 AR-1260-2


R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 423650119
Conc: 5118.64 ng/ml

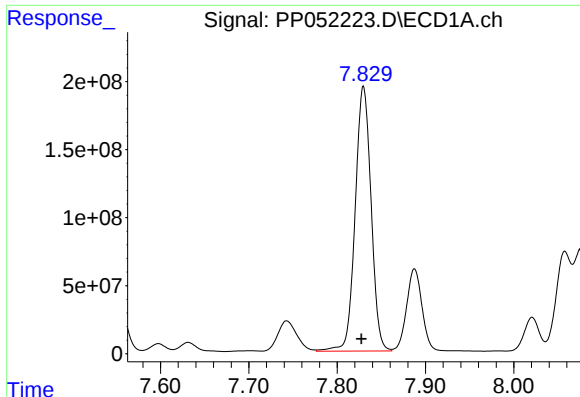

#33 AR-1260-3


R.T.: 7.830 min
Delta R.T.: 0.002 min
Response: 2437102508
Conc: 40578.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

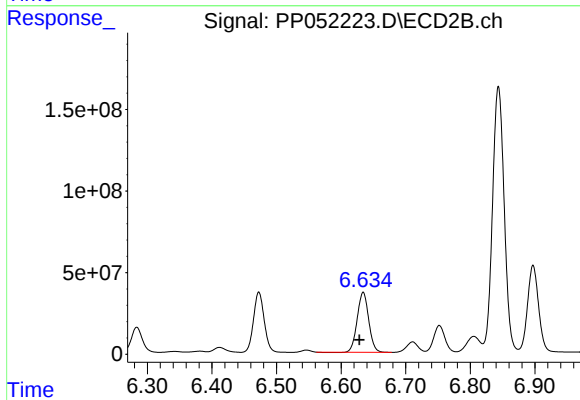


#33 AR-1260-3

R.T.: 6.634 min
Delta R.T.: 0.006 min
Response: 453680071
Conc: 5876.10 ng/ml

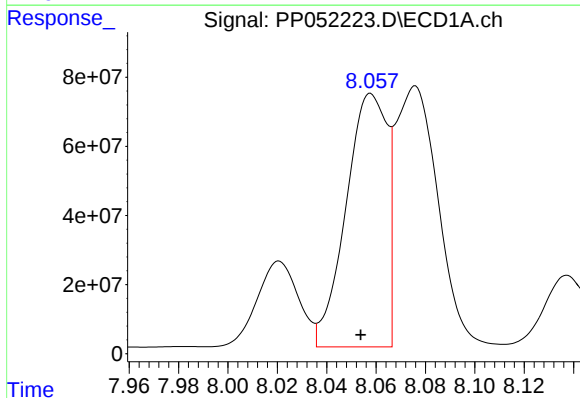


#34 AR-1260-4

R.T.: 8.058 min
Delta R.T.: 0.004 min
Response: 846936394
Conc: 11043.08 ng/ml

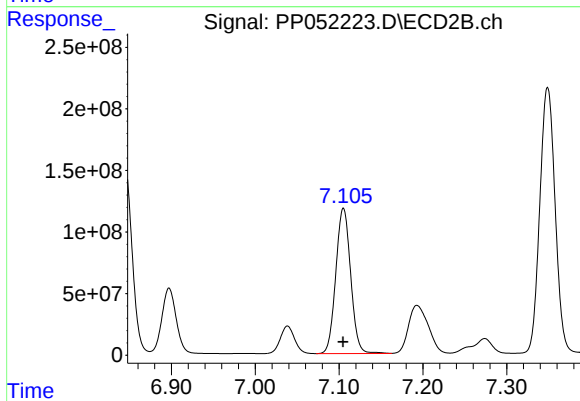

#34 AR-1260-4


R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 1455587928
Conc: 25893.43 ng/ml

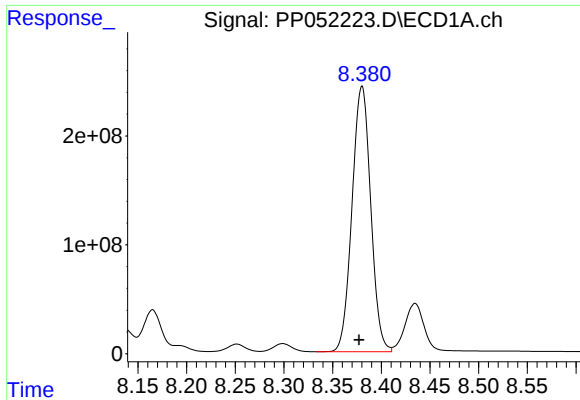

#35 AR-1260-5


R.T.: 8.380 min
Delta R.T.: 0.003 min
Response: 3260595979
Conc: 23786.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

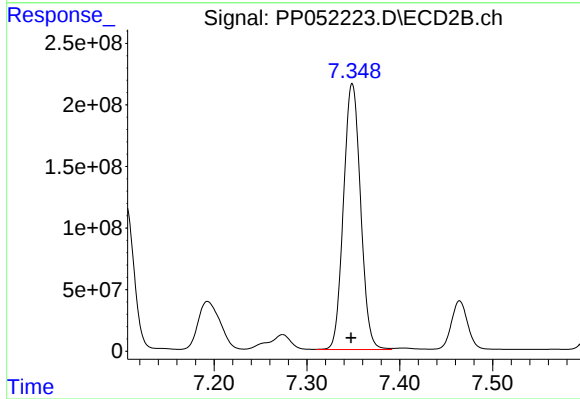


#35 AR-1260-5

R.T.: 7.349 min
Delta R.T.: 0.001 min
Response: 2759904387
Conc: 20927.85 ng/ml

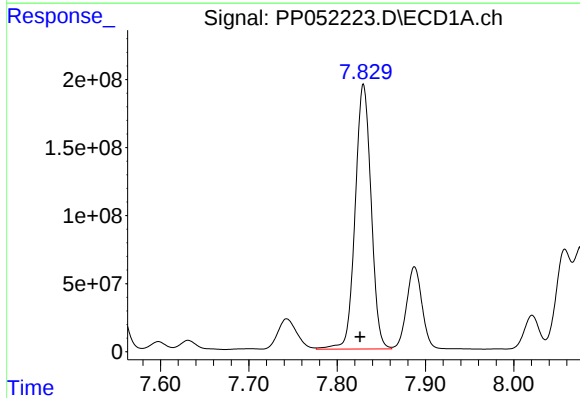


#36 AR-1262-1

R.T.: 7.830 min
Delta R.T.: 0.004 min
Response: 2437102508
Conc: 25134.08 ng/ml

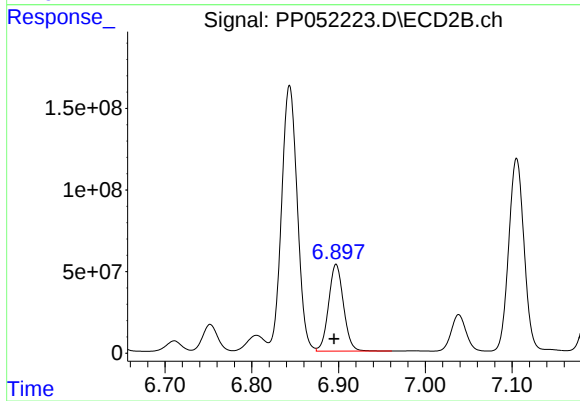

#36 AR-1262-1


R.T.: 6.897 min
Delta R.T.: 0.002 min
Response: 631989395
Conc: 17569.14 ng/ml

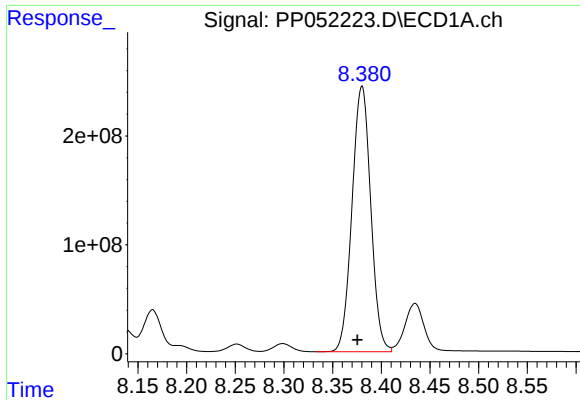

#37 AR-1262-2


R.T.: 8.380 min
Delta R.T.: 0.005 min
Response: 3260595979
Conc: 20250.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

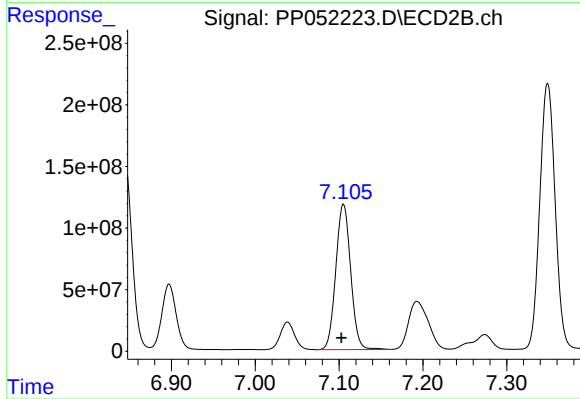


#37 AR-1262-2

R.T.: 7.105 min
Delta R.T.: 0.002 min
Response: 1455587928
Conc: 18382.38 ng/ml

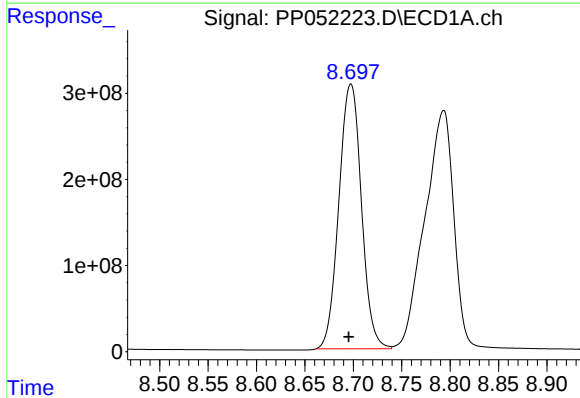


#38 AR-1262-3

R.T.: 8.697 min
Delta R.T.: 0.002 min
Response: 4984101490
Conc: 45351.32 ng/ml

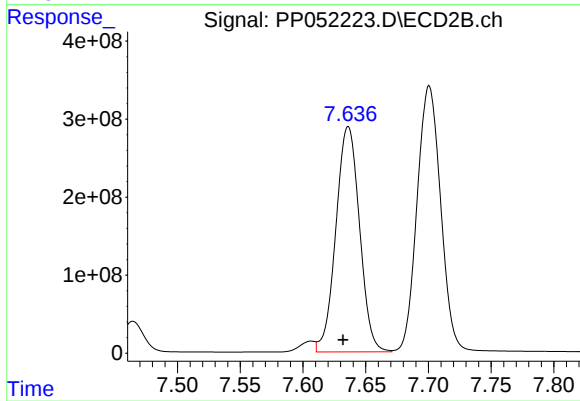

#38 AR-1262-3


R.T.: 7.636 min
Delta R.T.: 0.004 min
Response: 3793879001
Conc: 61437.26 ng/ml

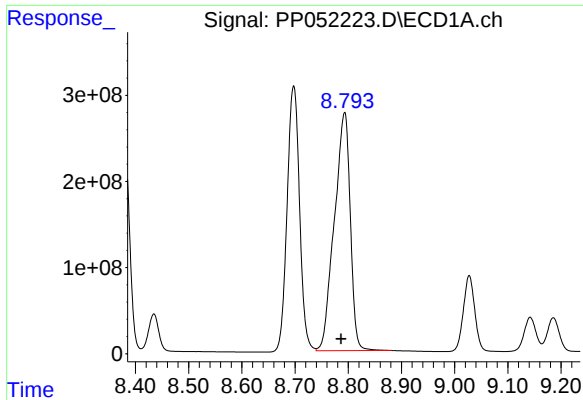

#39 AR-1262-4


R.T.: 8.793 min
Delta R.T.: 0.007 min
Response: 5759323630
Conc: 112665.75 ng

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

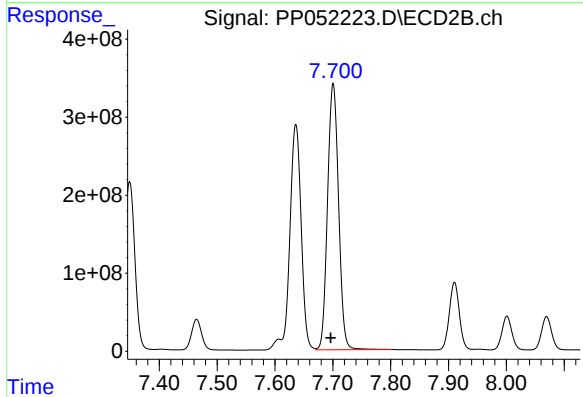


#39 AR-1262-4

R.T.: 7.701 min
Delta R.T.: 0.004 min
Response: 4477774643
Conc: 39222.53 ng/ml

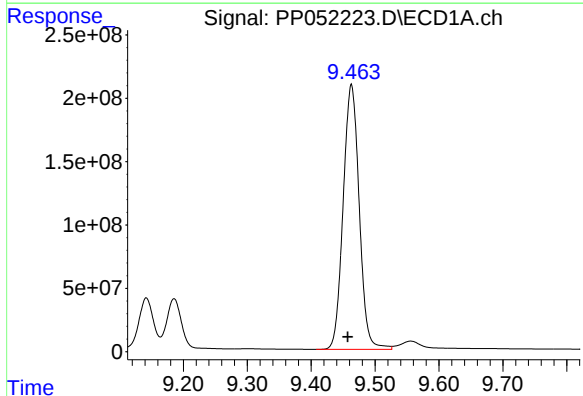


#40 AR-1262-5

R.T.: 9.463 min
Delta R.T.: 0.006 min
Response: 3649294095
Conc: 57972.22 ng/ml

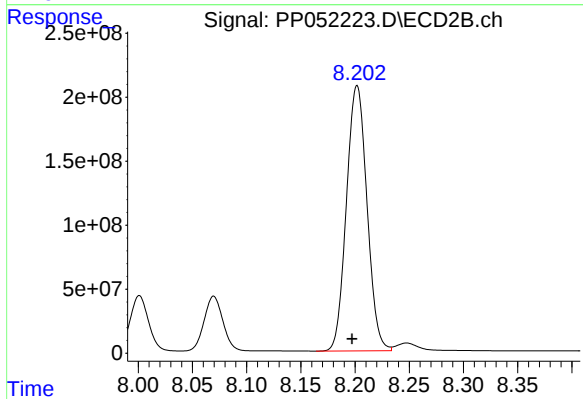

#40 AR-1262-5


R.T.: 8.202 min
Delta R.T.: 0.005 min
Response: 2735942724
Conc: 53826.84 ng/ml

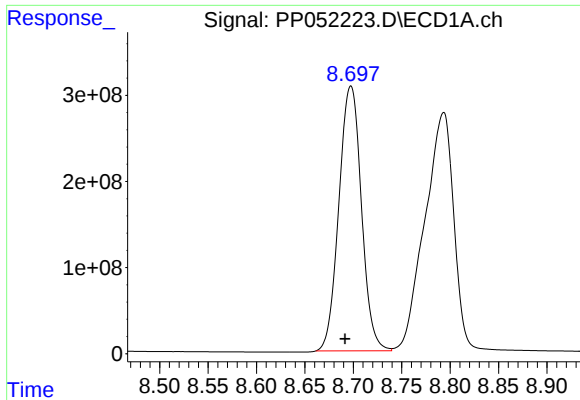

#41 AR-1268-1


R.T.: 8.697 min
Delta R.T.: 0.006 min
Response: 4984101490
Conc: 25174.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

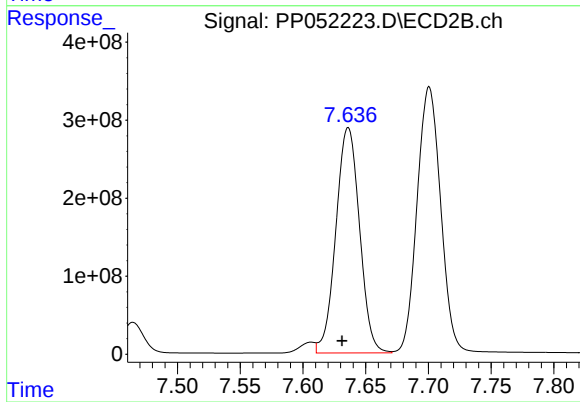


#41 AR-1268-1

R.T.: 7.636 min
Delta R.T.: 0.005 min
Response: 3793879001
Conc: 20913.27 ng/ml

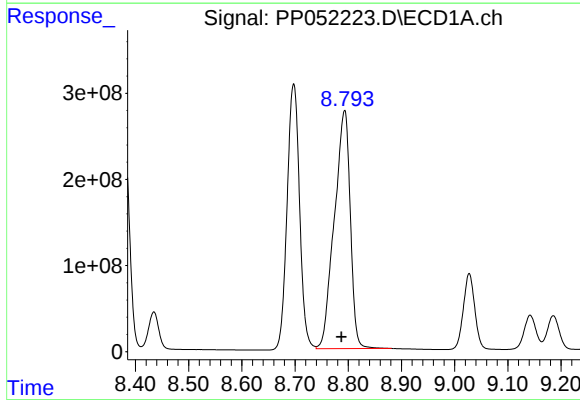


#42 AR-1268-2

R.T.: 8.793 min
Delta R.T.: 0.006 min
Response: 5759323630
Conc: 31365.08 ng/ml

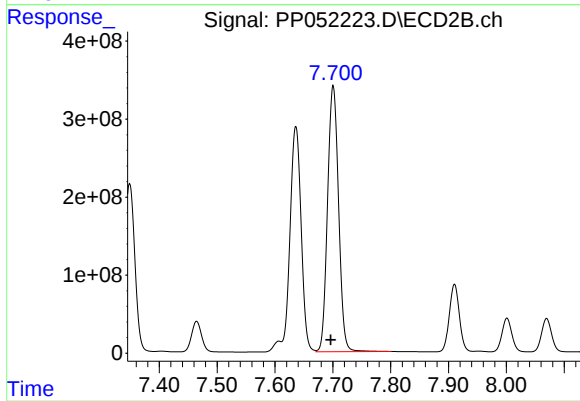

#42 AR-1268-2


R.T.: 7.701 min
Delta R.T.: 0.004 min
Response: 4477774643
Conc: 27405.93 ng/ml

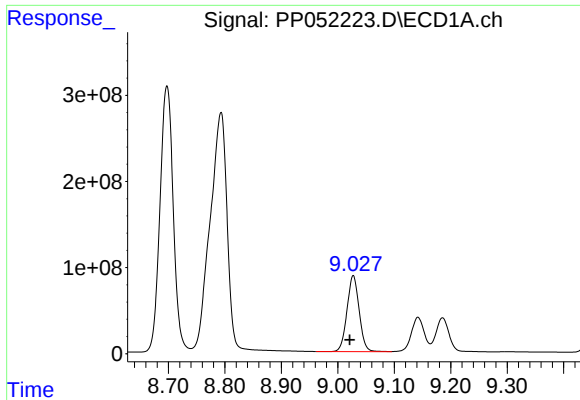

#43 AR-1268-3


R.T.: 9.027 min
Delta R.T.: 0.006 min
Response: 1319630955
Conc: 8095.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

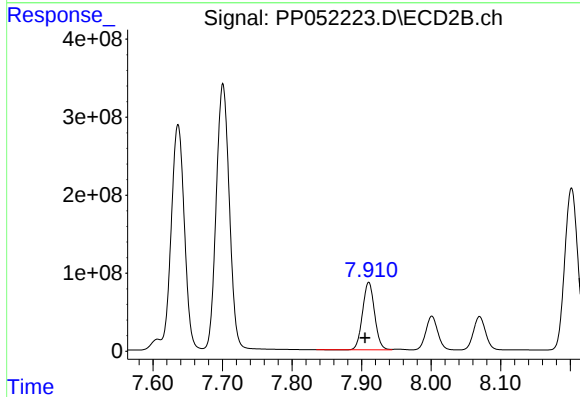


#43 AR-1268-3

R.T.: 7.910 min
Delta R.T.: 0.005 min
Response: 1038649339
Conc: 7386.08 ng/ml

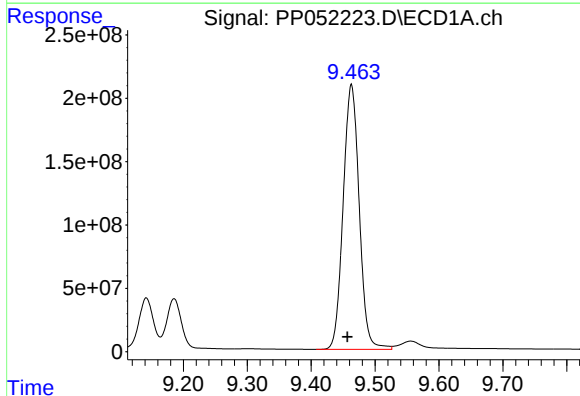


#44 AR-1268-4

R.T.: 9.463 min
Delta R.T.: 0.006 min
Response: 3649294095
Conc: 50016.43 ng/ml

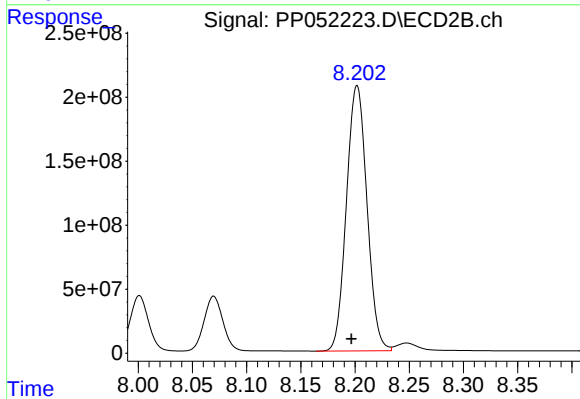

#44 AR-1268-4


R.T.: 8.202 min
Delta R.T.: 0.005 min
Response: 2735942724
Conc: 48414.07 ng/ml

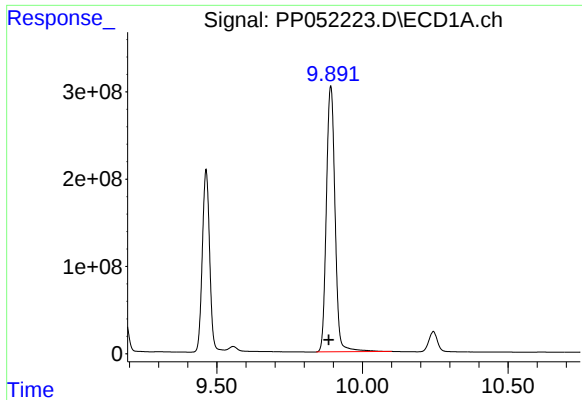

#45 AR-1268-5

R.T.: 9.891 min
Delta R.T.: 0.007 min
Response: 6302323602
Conc: 12086.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

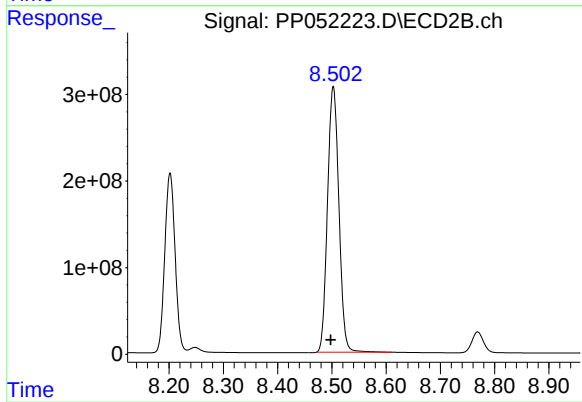

#45 AR-1268-5

R.T.: 8.503 min
Delta R.T.: 0.005 min
Response: 4479900346
Conc: 10649.70 ng/ml