

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 13:15
 Operator : YP\AJ
 Sample : N5098-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 14:45:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.425	3.676	15600273	16245838	9.925	14.180 #
2)	SA Decachlor...	10.242	8.770	176.9E6	116.0E6	127.456	103.839
Target Compounds							
3)	L1 AR-1016-1	5.599	4.778	1911830	5639351	42.042	126.795 #
4)	L1 AR-1016-2	5.622	4.796	6809134	3882621	103.432	61.017 #
5)	L1 AR-1016-3	5.684	4.977	4313962	4601633	103.663	138.435 #
6)	L1 AR-1016-4	5.779	5.019	9859316	7085035	271.347	259.951
7)	L1 AR-1016-5	6.080	5.236	-101568	205239	N.D.	5.801 #
8)	L2 AR-1221-1	4.633	3.895	4196452	4614565	203.077	295.133 #
9)	L2 AR-1221-2	4.720	3.978	3986762	6149489	260.516	512.765 #
10)	L2 AR-1221-3	4.797	4.057	7074291	4643317	151.086	122.855
11)	L3 AR-1232-1	4.797	4.057	7074291	4643317	196.362	160.215
12)	L3 AR-1232-2	5.328	4.796	11576883	3882621	570.578	129.615 #
13)	L3 AR-1232-3	5.622	4.977	6809134	4601633	226.097	301.205 #
14)	L3 AR-1232-4	5.779	5.062	9859316	5414694	591.168	382.379 #
15)	L3 AR-1232-5	5.875	5.236	9604366	205239	640.388	12.965 #
16)	L4 AR-1242-1	5.599	4.778	1911830	5639351	54.961	161.965 #
17)	L4 AR-1242-2	5.622	4.796	6809134	3882621	137.540	78.704 #
18)	L4 AR-1242-3	5.684	4.977	4313962	4601633	136.056	176.282 #
19)	L4 AR-1242-4	5.779	5.062	9859316	5414694	360.943	199.069 #
20)	L4 AR-1242-5	6.525	5.595	18359278	20414013	493.826	605.756
21)	L5 AR-1248-1	5.599	4.778	1911830	5639351	71.118	208.006 #
22)	L5 AR-1248-2	5.875	5.019	9604366	7085035	206.624	190.435
23)	L5 AR-1248-3	6.080	5.062	-101568	5414694	N.D.	142.132 #
24)	L5 AR-1248-4	6.485	5.236	11724550	205239	184.659	4.429 #
25)	L5 AR-1248-5	6.525	5.635	18359278	5364714	296.428	127.569 #
26)	L6 AR-1254-1	6.459	5.595	32033512	20414013	449.975	291.785 #
27)	L6 AR-1254-2	6.678	5.743	46287465	23951561	434.006	382.279
28)	L6 AR-1254-3	7.048	6.134f	25262515	32497250	240.367	328.521 #
29)	L6 AR-1254-4	7.330	6.382	24299167	11260744	332.554	188.378 #
30)	L6 AR-1254-5	7.743	6.806	280.1E6	136.7E6	3375.931	1542.189 #
31)	L7 AR-1260-1	7.211	6.285	251.2E6	183.1E6	3030.575	2657.670
32)	L7 AR-1260-2	7.469	6.474	468.8E6	395.8E6	4966.981	4782.389
33)	L7 AR-1260-3	7.830	6.635	1705.7E6	372.0E6	28400.028	4817.662 #
34)	L7 AR-1260-4	8.057	7.106	1225.4E6	1004.5E6	15978.264	17868.515
35)	L7 AR-1260-5	8.379	7.350	2486.5E6	2148.2E6	18139.449	16289.441
36)	L8 AR-1262-1	7.830	6.898	1705.7E6	555.3E6	17590.805	15436.304
37)	L8 AR-1262-2	8.379	7.106	2486.5E6	1004.5E6	15443.328	12685.294
38)	L8 AR-1262-3	8.697	7.637	2947.2E6	2177.9E6	26817.482	35269.159 #
39)	L8 AR-1262-4	8.792	7.702	3486.1E6	2922.3E6	68195.657	25597.427 #
40)	L8 AR-1262-5	9.463	8.202	2157.8E6	1600.2E6	34278.276	31481.720
41)	L9 AR-1268-1	8.697	7.637	2947.2E6	2177.9E6	14886.616	12005.636

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 13:15
Operator : YP\AJ
Sample : N5098-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 14:45:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.792	7.702	3486.1E6	2922.3E6	18985.024	17885.670
43)	L9 AR-1268-3	9.027	7.911	531.3E6	424.5E6	3259.345	3018.878
44)	L9 AR-1268-4	9.463	8.202	2157.8E6	1600.2E6	29574.112	28315.949
45)	L9 AR-1268-5	9.892	8.503	2856.9E6	2109.6E6	5478.740	5014.918



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 13:15
Operator : YP\AJ
Sample : N5098-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 14:45:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

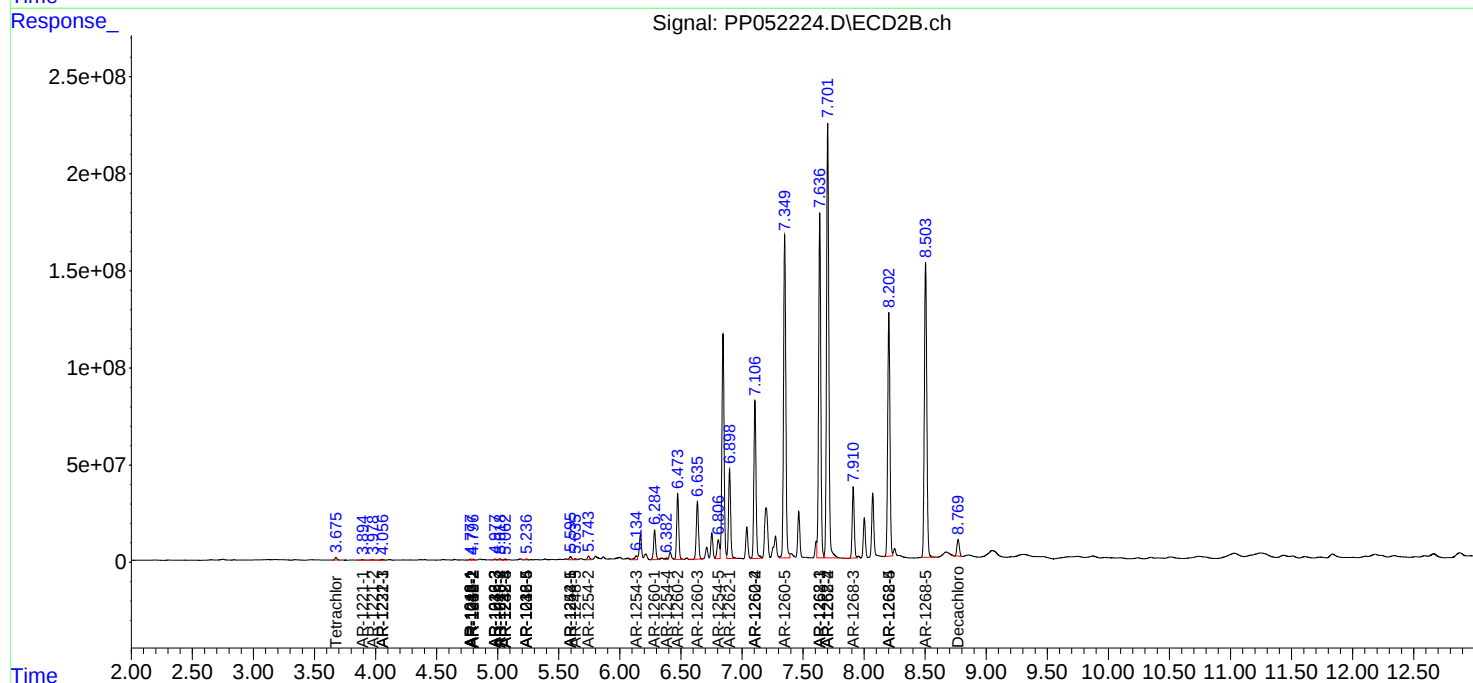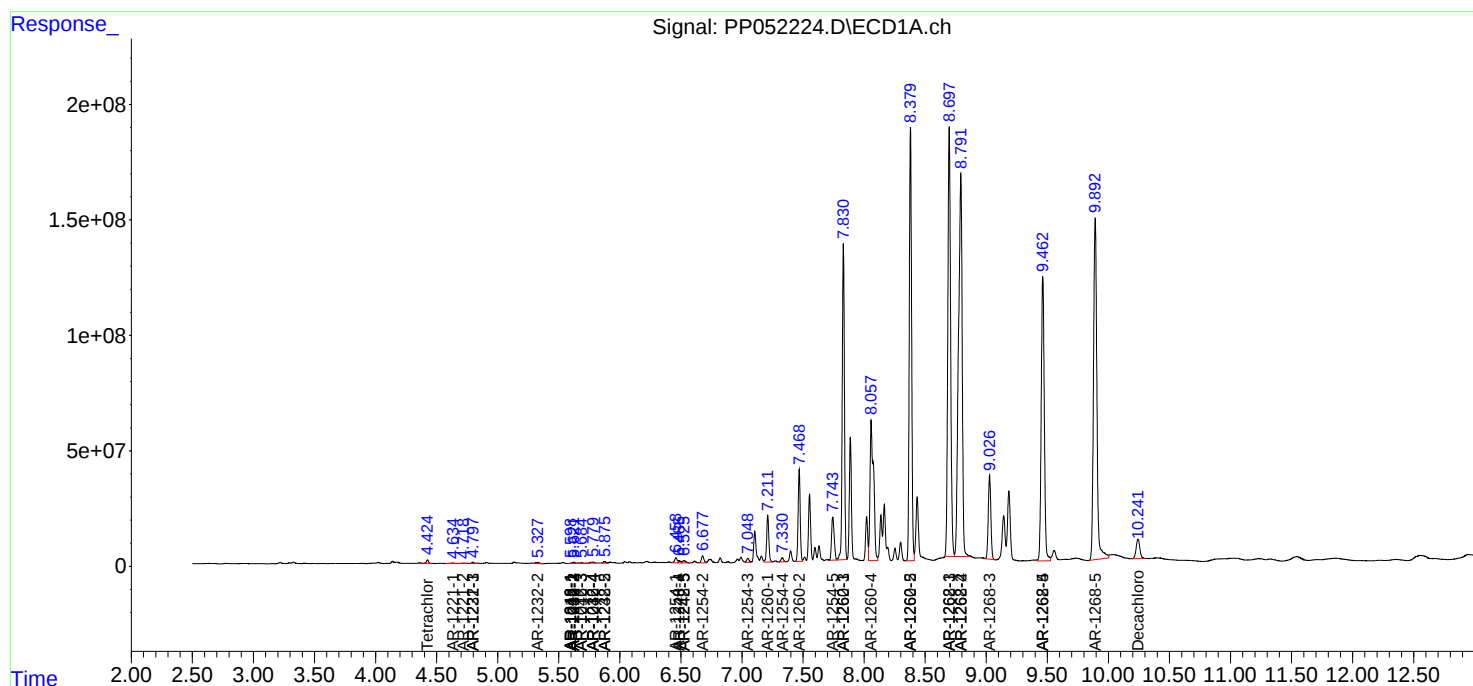


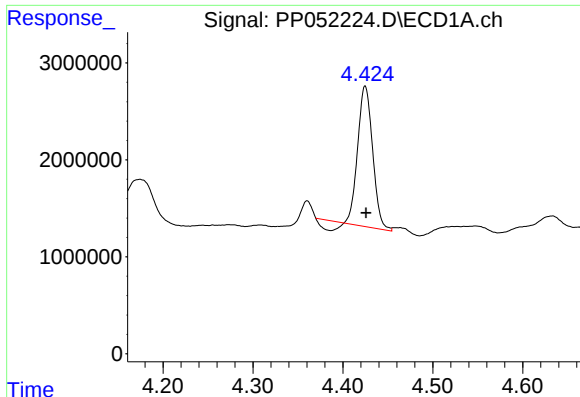

#1 Tetrachloro-m-xylene


R.T.: 4.425 min
Delta R.T.: -0.001 min
Response: 15600273
Conc: 9.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

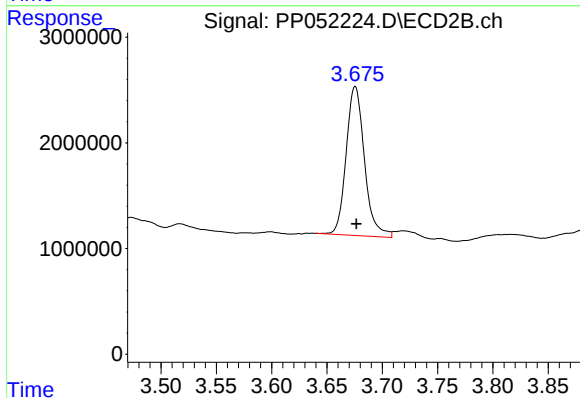


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 16245838
Conc: 14.18 ng/ml

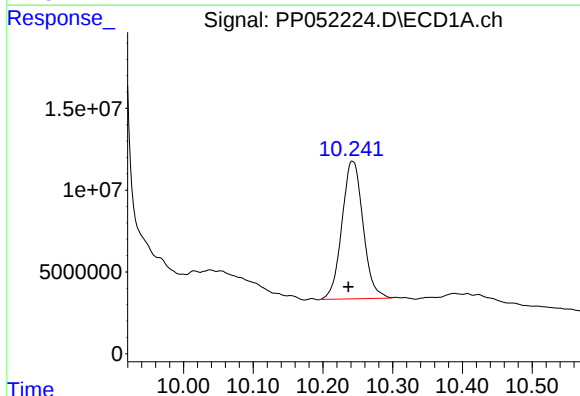


#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: 0.006 min
Response: 176889707
Conc: 127.46 ng/ml

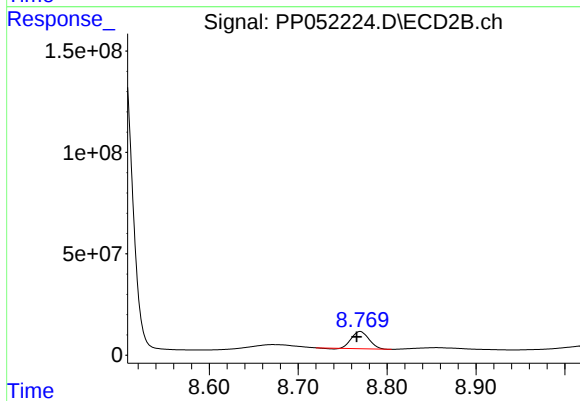

#2 Decachlorobiphenyl


R.T.: 8.770 min
Delta R.T.: 0.004 min
Response: 116026030
Conc: 103.84 ng/ml

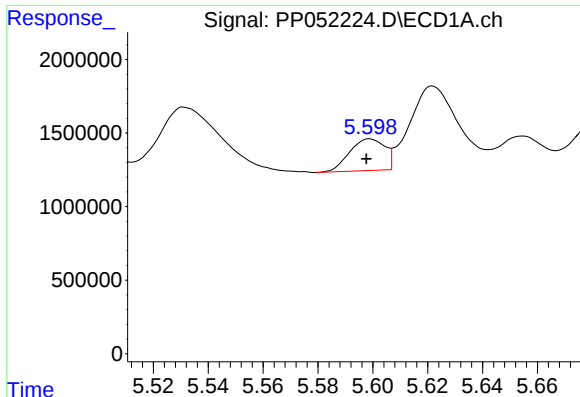

#3 AR-1016-1


R.T.: 5.599 min
Delta R.T.: 0.001 min
Response: 1911830
Conc: 42.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

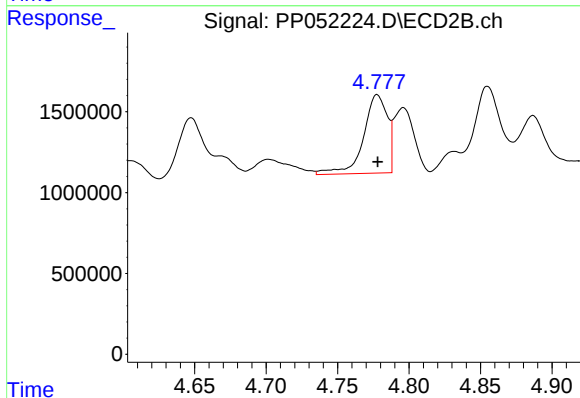


#3 AR-1016-1

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 5639351
Conc: 126.80 ng/ml

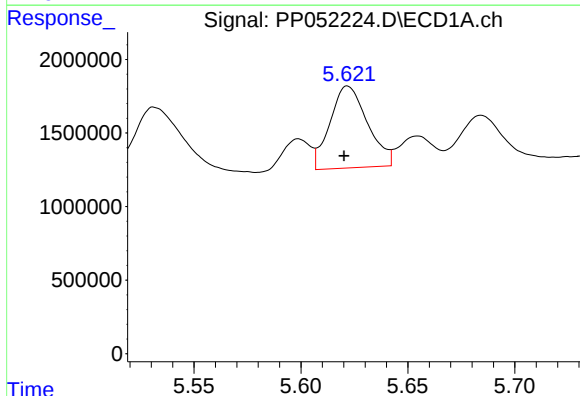


#4 AR-1016-2

R.T.: 5.622 min
Delta R.T.: 0.002 min
Response: 6809134
Conc: 103.43 ng/ml

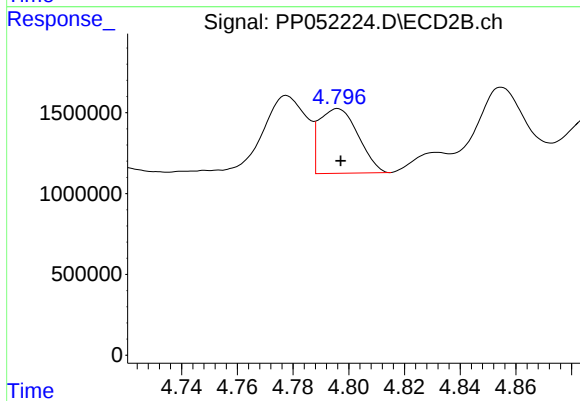

#4 AR-1016-2


R.T.: 4.796 min
Delta R.T.: -0.001 min
Response: 3882621
Conc: 61.02 ng/ml

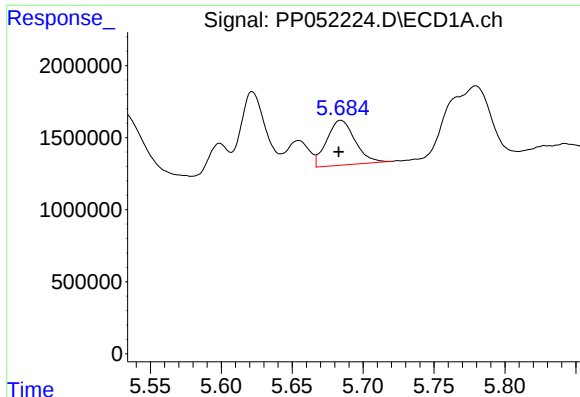

#5 AR-1016-3


R.T.: 5.684 min
Delta R.T.: 0.002 min
Response: 4313962
Conc: 103.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

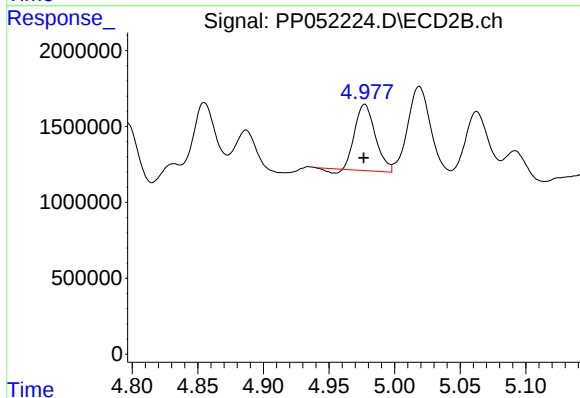


#5 AR-1016-3

R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 4601633
Conc: 138.44 ng/ml

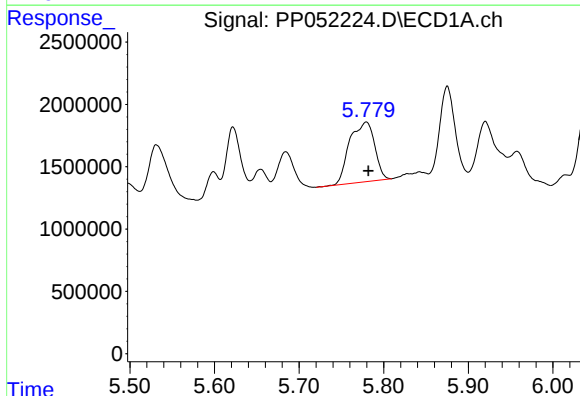


#6 AR-1016-4

R.T.: 5.779 min
Delta R.T.: -0.002 min
Response: 9859316
Conc: 271.35 ng/ml

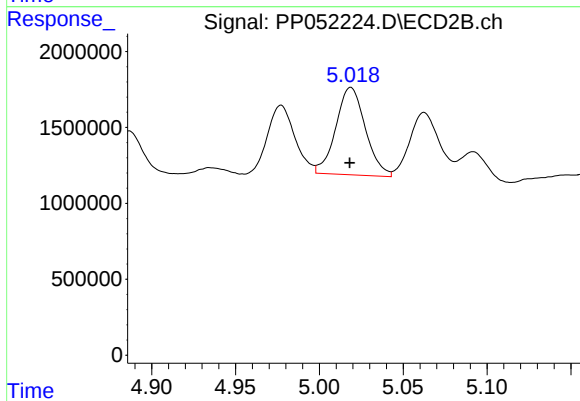

#6 AR-1016-4


R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 7085035
Conc: 259.95 ng/ml

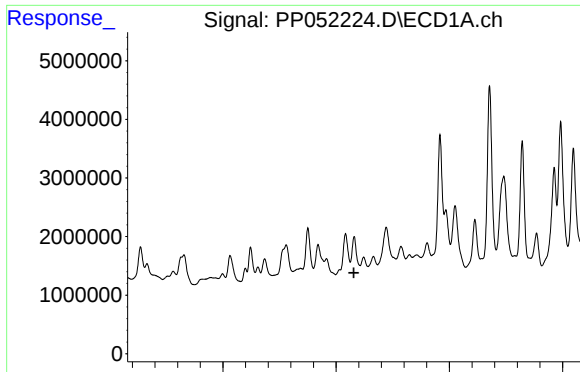

#7 AR-1016-5


R.T.: 6.080 min
Delta R.T.: 0.001 min
Response: -101568
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

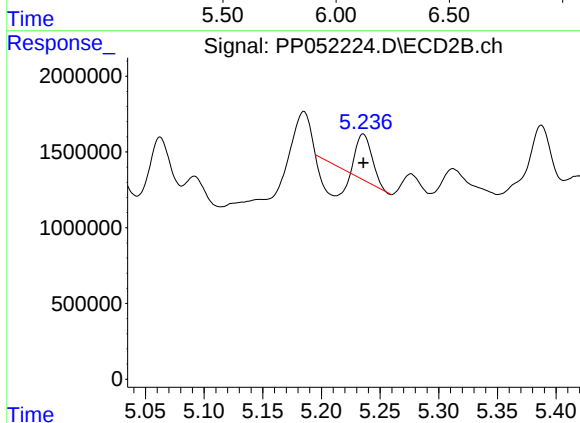


#7 AR-1016-5

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 205239
Conc: 5.80 ng/ml

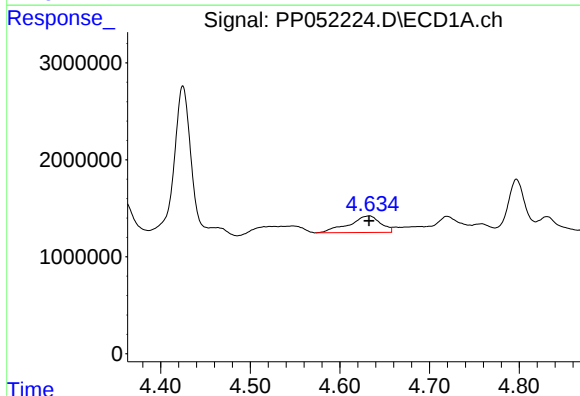


#8 AR-1221-1

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 4196452
Conc: 203.08 ng/ml

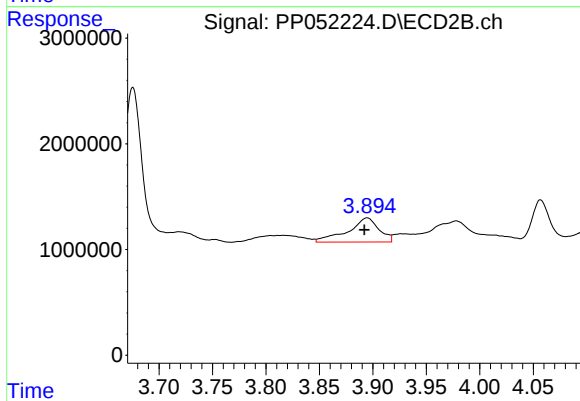

#8 AR-1221-1


R.T.: 3.895 min
Delta R.T.: 0.003 min
Response: 4614565
Conc: 295.13 ng/ml

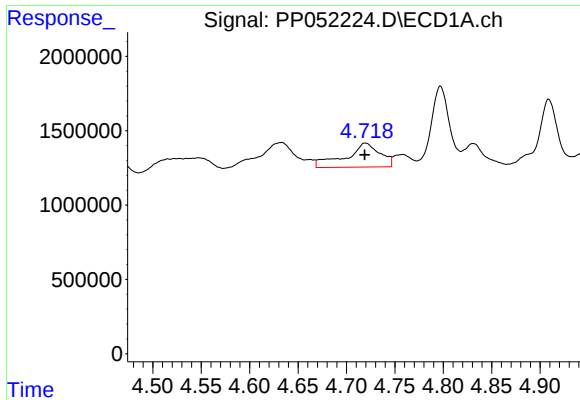

#9 AR-1221-2


R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 3986762
Conc: 260.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

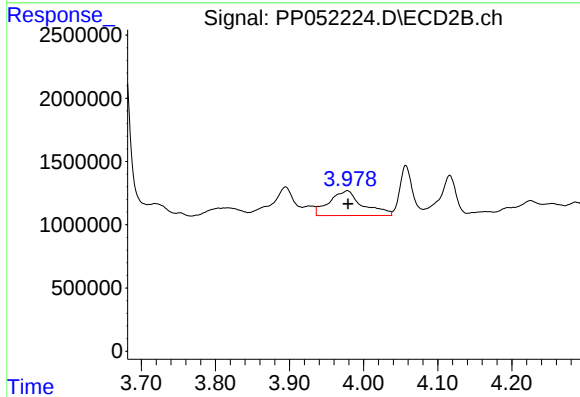


#9 AR-1221-2

R.T.: 3.978 min
Delta R.T.: -0.001 min
Response: 6149489
Conc: 512.77 ng/ml

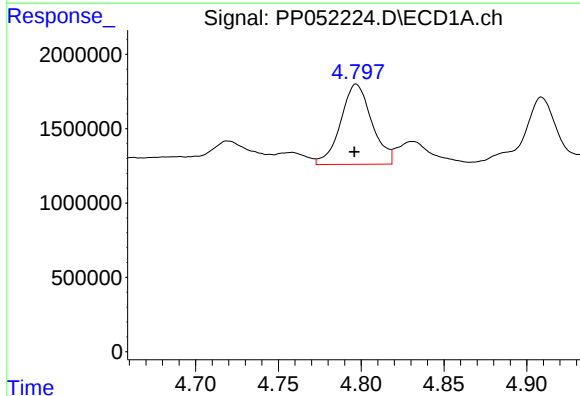


#10 AR-1221-3

R.T.: 4.797 min
Delta R.T.: 0.001 min
Response: 7074291
Conc: 151.09 ng/ml

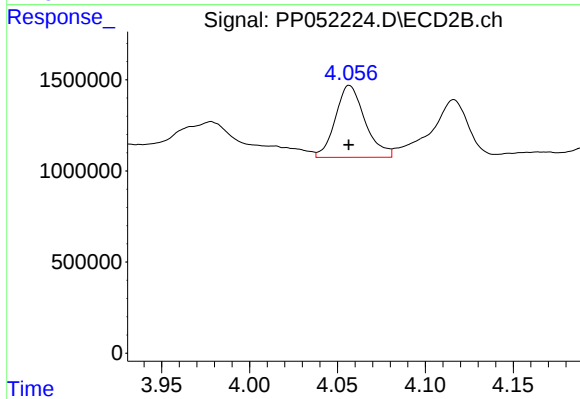

#10 AR-1221-3


R.T.: 4.057 min
Delta R.T.: 0.000 min
Response: 4643317
Conc: 122.86 ng/ml

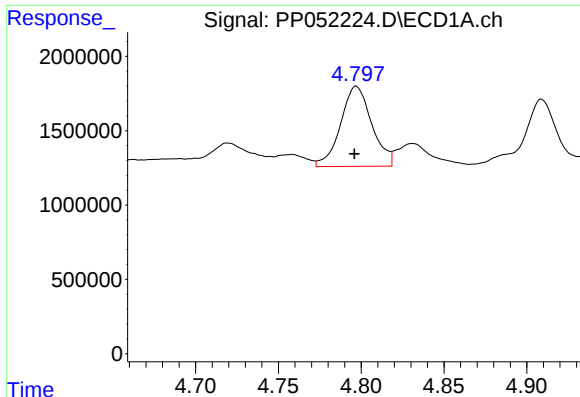

#11 AR-1232-1


R.T.: 4.797 min
Delta R.T.: 0.001 min
Response: 7074291
Conc: 196.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

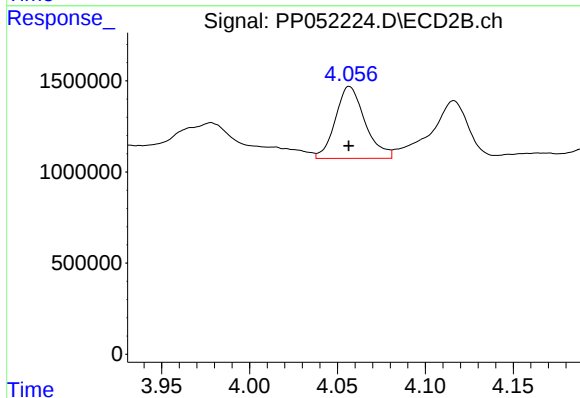


#11 AR-1232-1

R.T.: 4.057 min
Delta R.T.: 0.000 min
Response: 4643317
Conc: 160.21 ng/ml

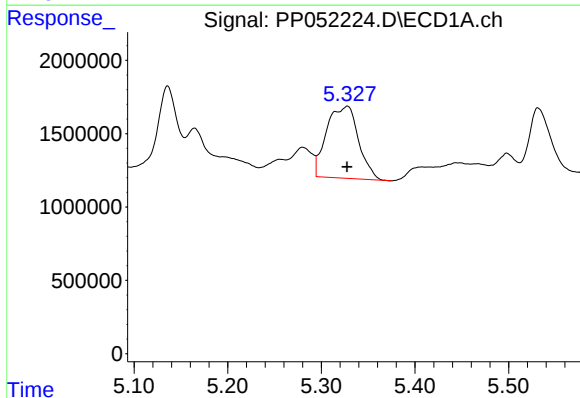


#12 AR-1232-2

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 11576883
Conc: 570.58 ng/ml

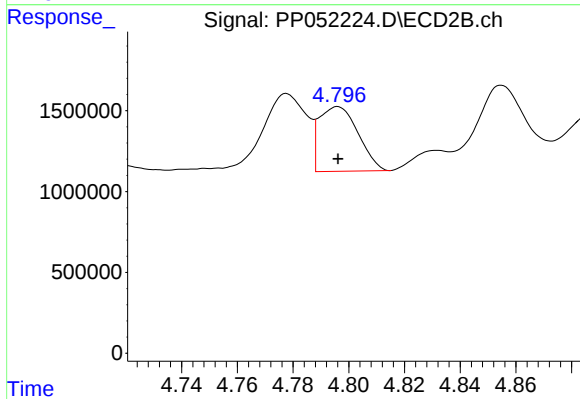

#12 AR-1232-2


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 3882621
Conc: 129.62 ng/ml

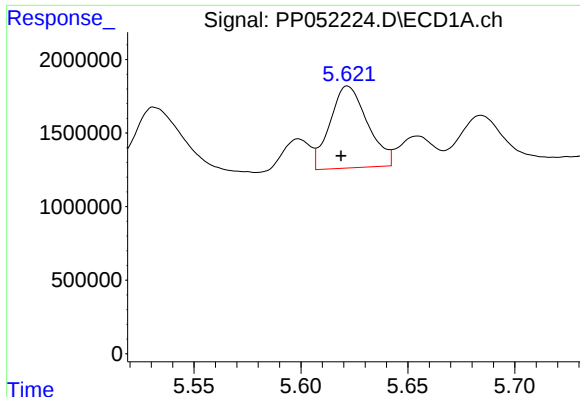

#13 AR-1232-3


R.T.: 5.622 min
Delta R.T.: 0.003 min
Response: 6809134
Conc: 226.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

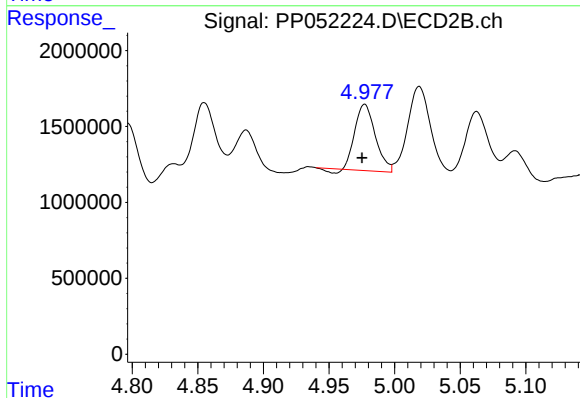


#13 AR-1232-3

R.T.: 4.977 min
Delta R.T.: 0.002 min
Response: 4601633
Conc: 301.20 ng/ml

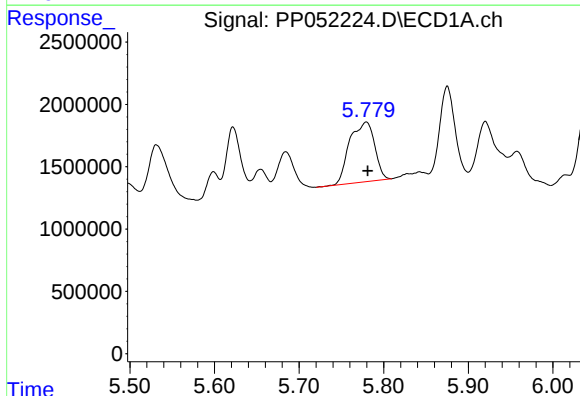


#14 AR-1232-4

R.T.: 5.779 min
Delta R.T.: -0.002 min
Response: 9859316
Conc: 591.17 ng/ml

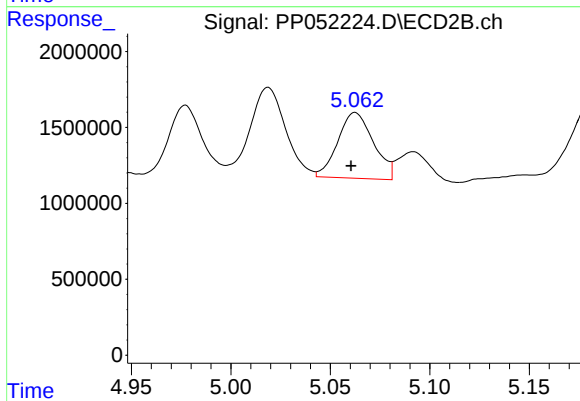

#14 AR-1232-4


R.T.: 5.062 min
Delta R.T.: 0.002 min
Response: 5414694
Conc: 382.38 ng/ml

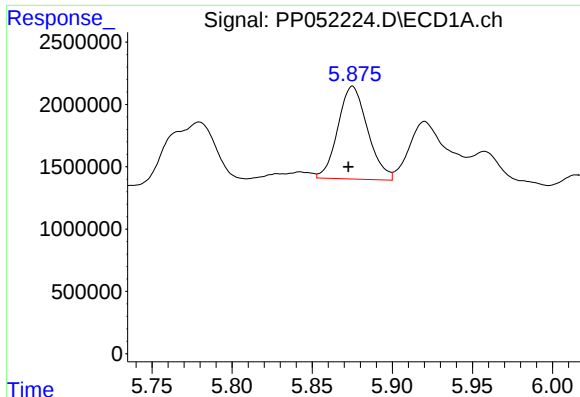

#15 AR-1232-5


R.T.: 5.875 min
Delta R.T.: 0.003 min
Response: 9604366
Conc: 640.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

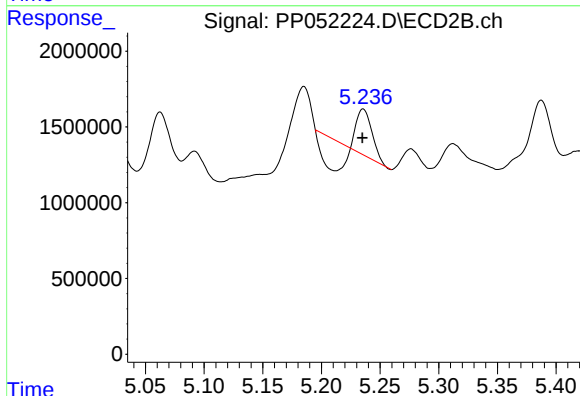


#15 AR-1232-5

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 205239
Conc: 12.96 ng/ml

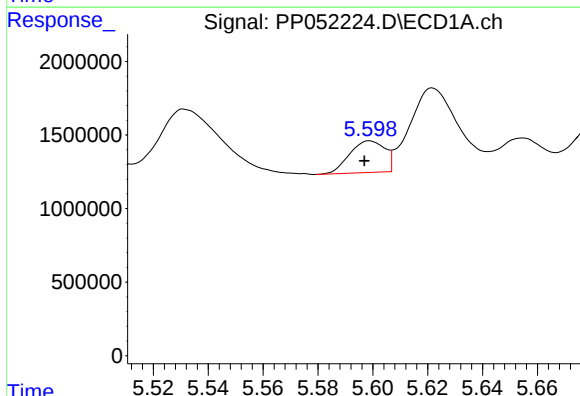


#16 AR-1242-1

R.T.: 5.599 min
Delta R.T.: 0.002 min
Response: 1911830
Conc: 54.96 ng/ml

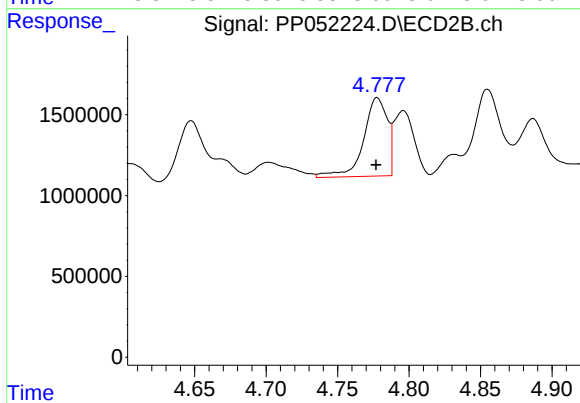

#16 AR-1242-1


R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 5639351
Conc: 161.97 ng/ml

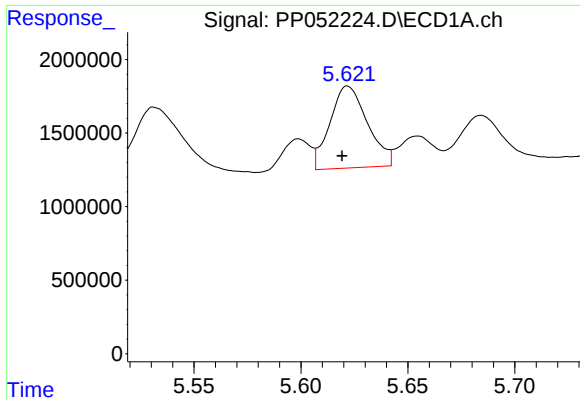

#17 AR-1242-2


R.T.: 5.622 min
Delta R.T.: 0.003 min
Response: 6809134
Conc: 137.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

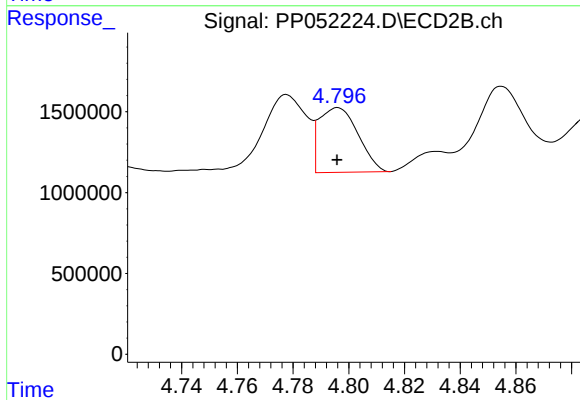


#17 AR-1242-2

R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 3882621
Conc: 78.70 ng/ml

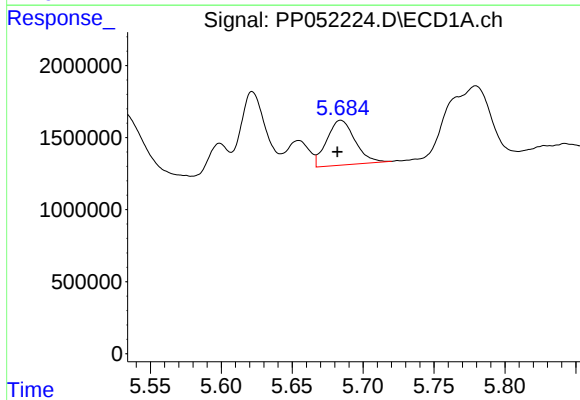


#18 AR-1242-3

R.T.: 5.684 min
Delta R.T.: 0.002 min
Response: 4313962
Conc: 136.06 ng/ml

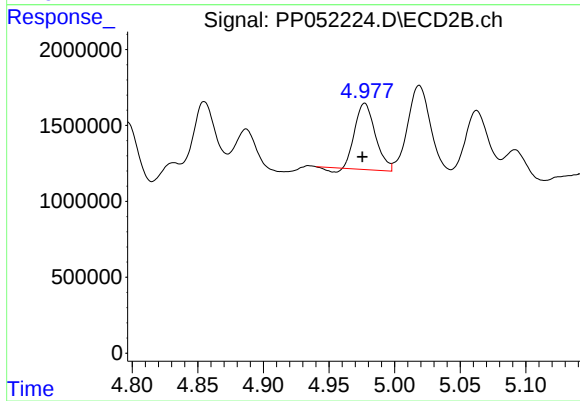

#18 AR-1242-3


R.T.: 4.977 min
Delta R.T.: 0.002 min
Response: 4601633
Conc: 176.28 ng/ml

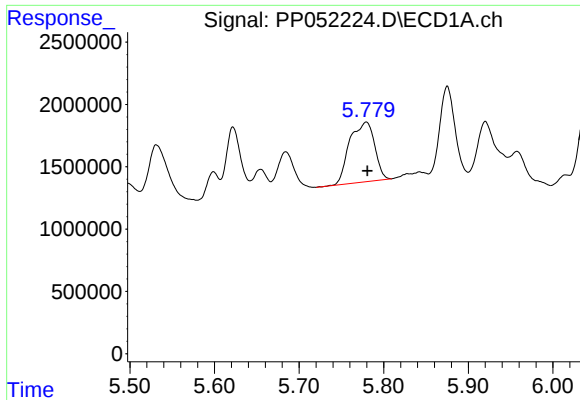

#19 AR-1242-4


R.T.: 5.779 min
Delta R.T.: -0.001 min
Response: 9859316
Conc: 360.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

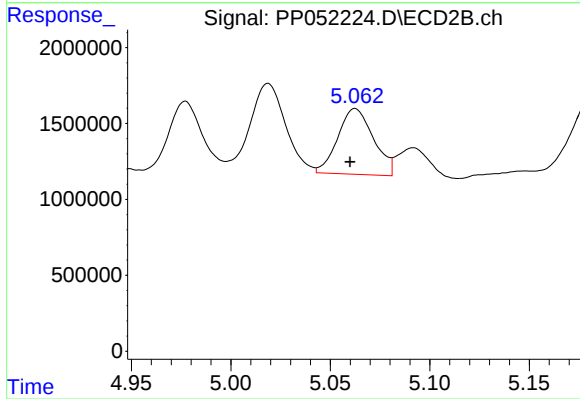


#19 AR-1242-4

R.T.: 5.062 min
Delta R.T.: 0.003 min
Response: 5414694
Conc: 199.07 ng/ml

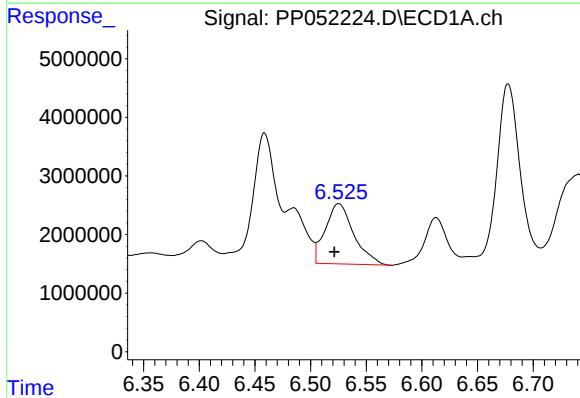


#20 AR-1242-5

R.T.: 6.525 min
Delta R.T.: 0.004 min
Response: 18359278
Conc: 493.83 ng/ml

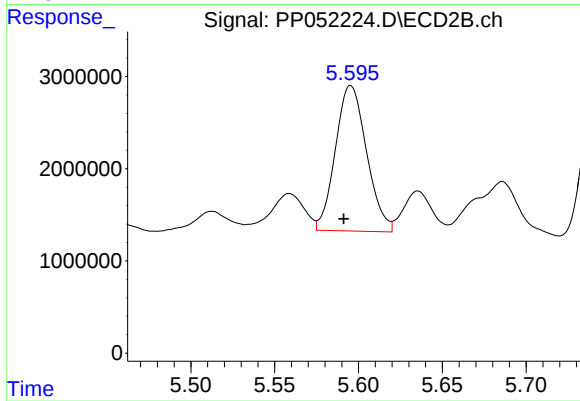

#20 AR-1242-5


R.T.: 5.595 min
Delta R.T.: 0.004 min
Response: 20414013
Conc: 605.76 ng/ml

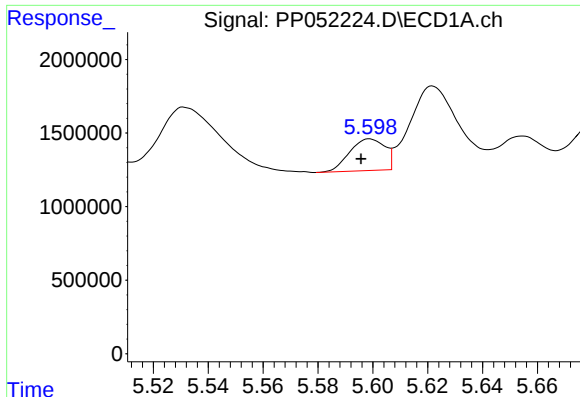

#21 AR-1248-1


R.T.: 5.599 min
Delta R.T.: 0.003 min
Response: 1911830
Conc: 71.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

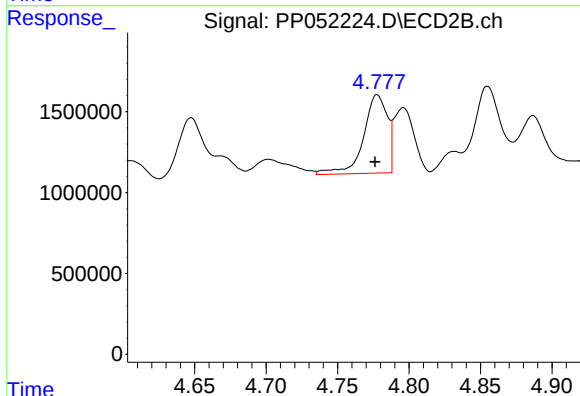


#21 AR-1248-1

R.T.: 4.778 min
Delta R.T.: 0.001 min
Response: 5639351
Conc: 208.01 ng/ml

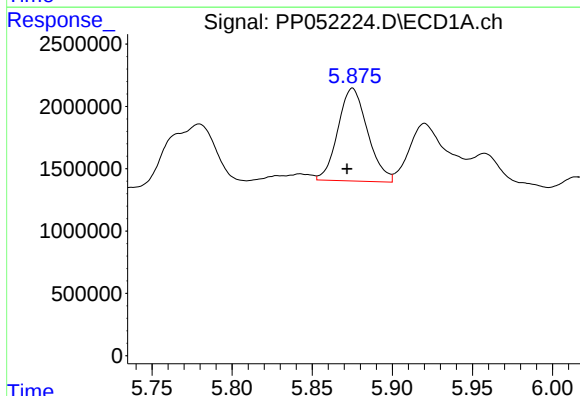


#22 AR-1248-2

R.T.: 5.875 min
Delta R.T.: 0.003 min
Response: 9604366
Conc: 206.62 ng/ml

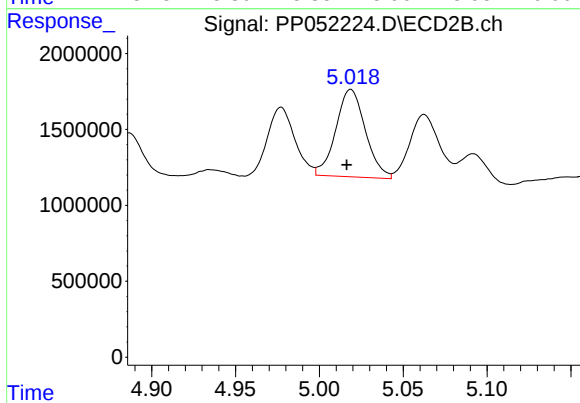

#22 AR-1248-2


R.T.: 5.019 min
Delta R.T.: 0.002 min
Response: 7085035
Conc: 190.44 ng/ml

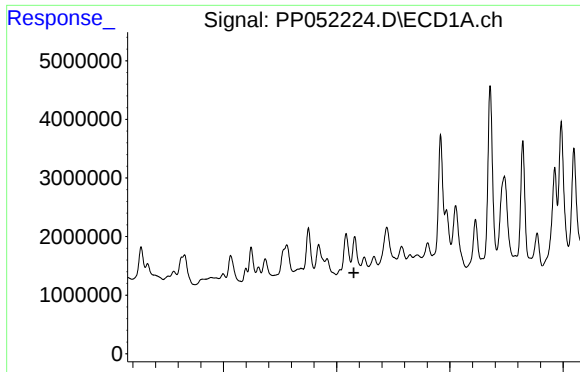

#23 AR-1248-3


R.T.: 6.080 min
Delta R.T.: 0.003 min
Response: -101568
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

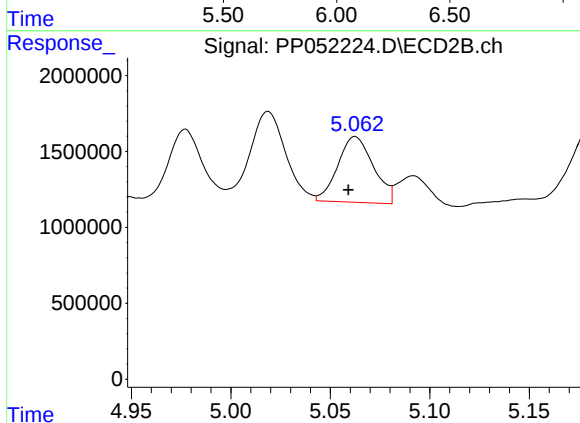


#23 AR-1248-3

R.T.: 5.062 min
Delta R.T.: 0.003 min
Response: 5414694
Conc: 142.13 ng/ml

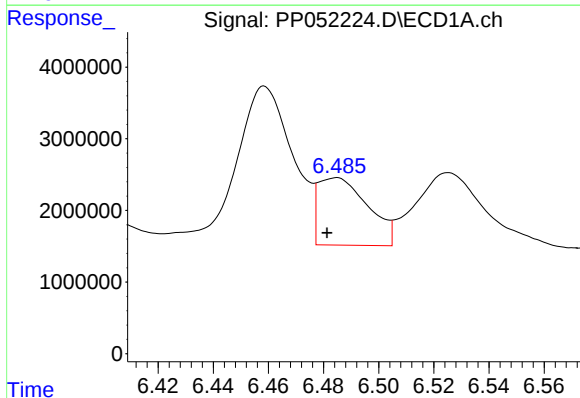


#24 AR-1248-4

R.T.: 6.485 min
Delta R.T.: 0.003 min
Response: 11724550
Conc: 184.66 ng/ml

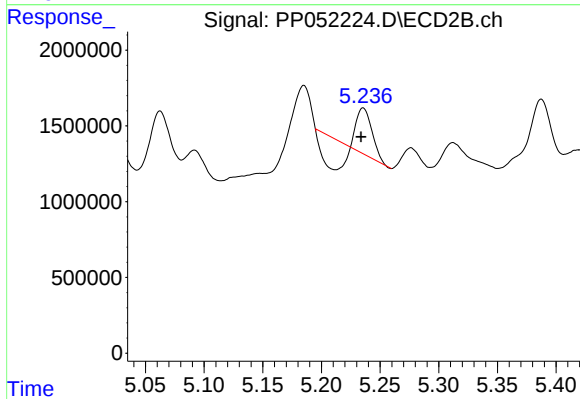

#24 AR-1248-4


R.T.: 5.236 min
Delta R.T.: 0.002 min
Response: 205239
Conc: 4.43 ng/ml

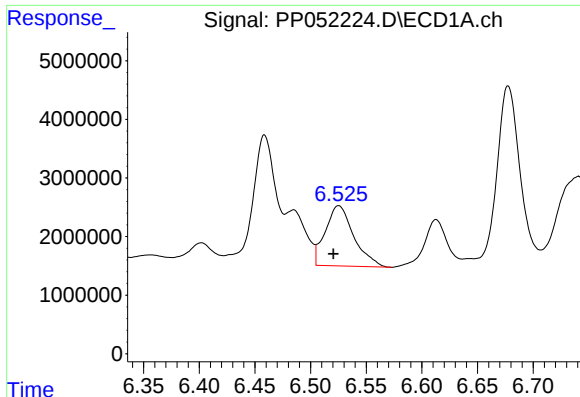

#25 AR-1248-5


R.T.: 6.525 min
Delta R.T.: 0.005 min
Response: 18359278
Conc: 296.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

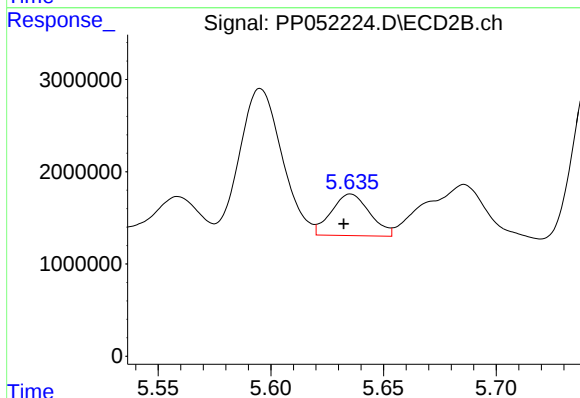


#25 AR-1248-5

R.T.: 5.635 min
Delta R.T.: 0.003 min
Response: 5364714
Conc: 127.57 ng/ml

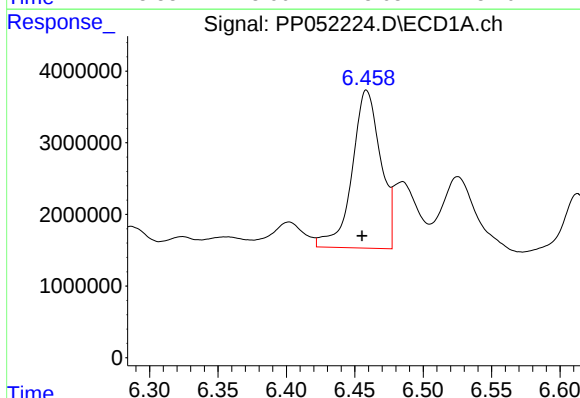


#26 AR-1254-1

R.T.: 6.459 min
Delta R.T.: 0.003 min
Response: 32033512
Conc: 449.97 ng/ml

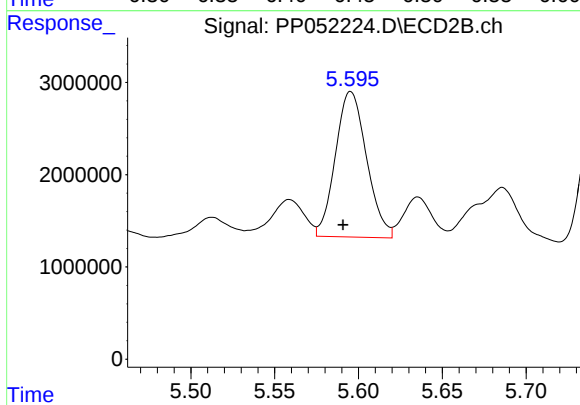

#26 AR-1254-1


R.T.: 5.595 min
Delta R.T.: 0.005 min
Response: 20414013
Conc: 291.78 ng/ml

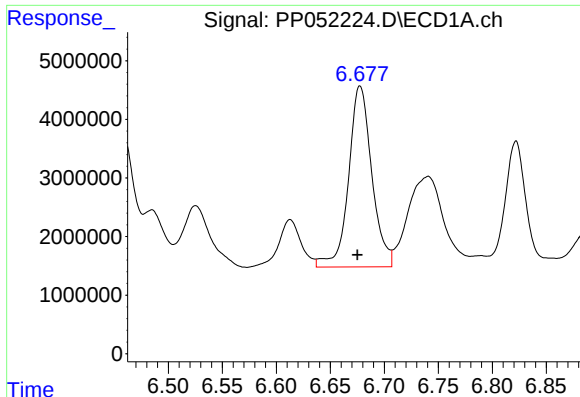

#27 AR-1254-2


R.T.: 6.678 min
Delta R.T.: 0.003 min
Response: 46287465
Conc: 434.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

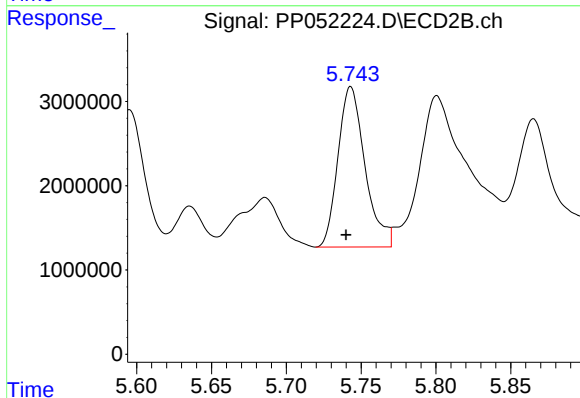


#27 AR-1254-2

R.T.: 5.743 min
Delta R.T.: 0.003 min
Response: 23951561
Conc: 382.28 ng/ml

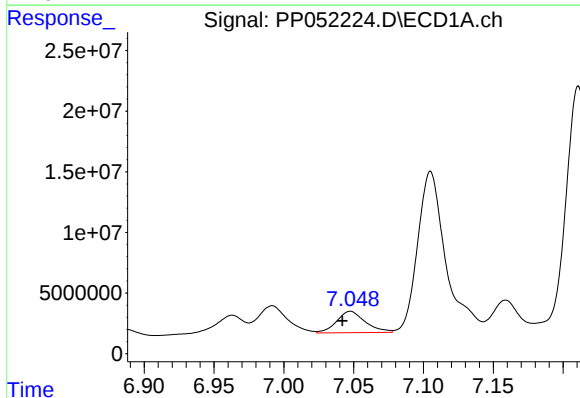


#28 AR-1254-3

R.T.: 7.048 min
Delta R.T.: 0.006 min
Response: 25262515
Conc: 240.37 ng/ml

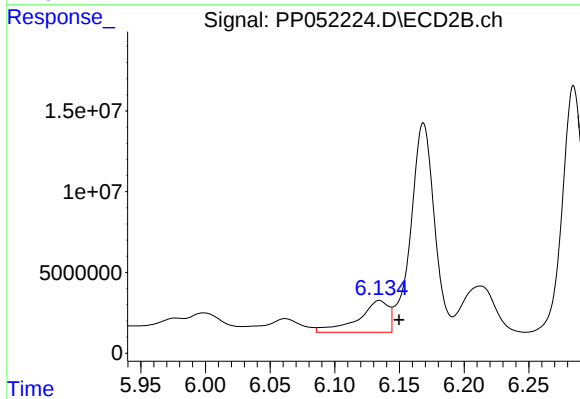

#28 AR-1254-3


R.T.: 6.134 min
Delta R.T.: -0.015 min
Response: 32497250
Conc: 328.52 ng/ml

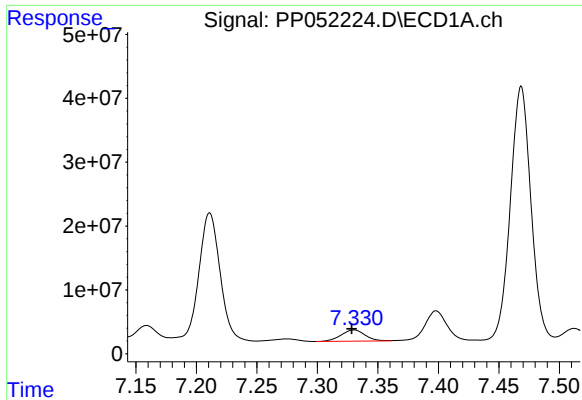

#29 AR-1254-4


R.T.: 7.330 min
Delta R.T.: 0.002 min
Response: 24299167
Conc: 332.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

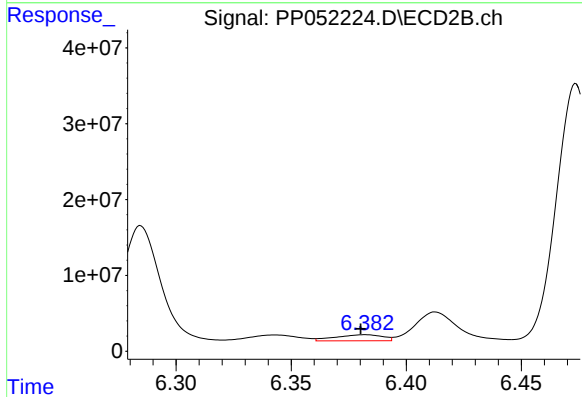


#29 AR-1254-4

R.T.: 6.382 min
Delta R.T.: 0.002 min
Response: 11260744
Conc: 188.38 ng/ml

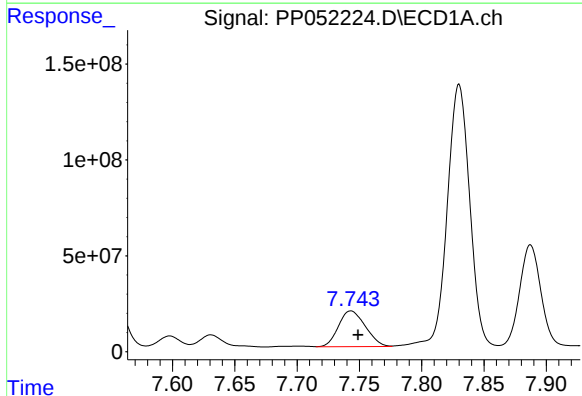


#30 AR-1254-5

R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 280112998
Conc: 3375.93 ng/ml

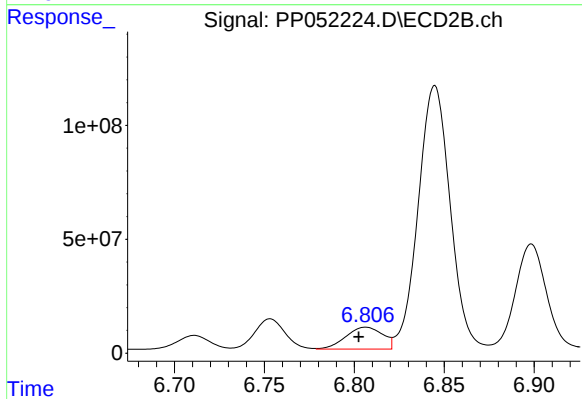

#30 AR-1254-5


R.T.: 6.806 min
Delta R.T.: 0.004 min
Response: 136721558
Conc: 1542.19 ng/ml

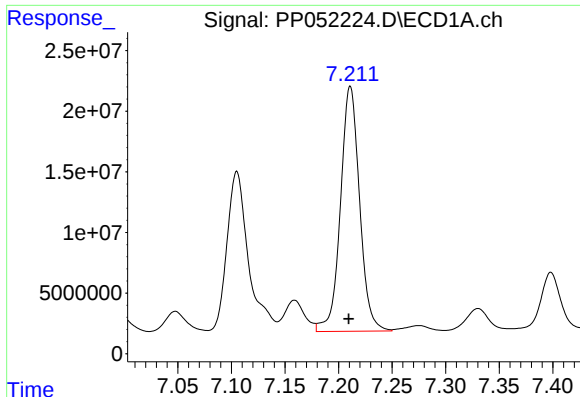

#31 AR-1260-1


R.T.: 7.211 min
Delta R.T.: 0.001 min
Response: 251191581
Conc: 3030.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

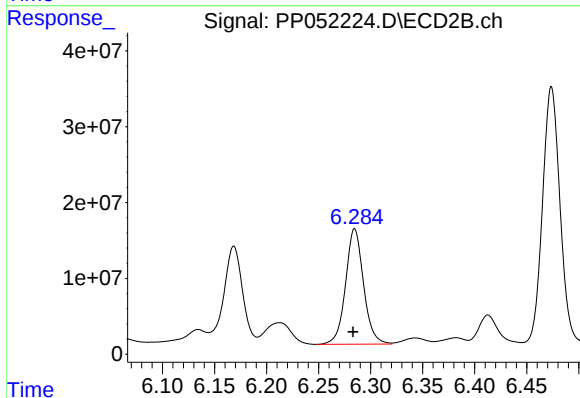


#31 AR-1260-1

R.T.: 6.285 min
Delta R.T.: 0.002 min
Response: 183067292
Conc: 2657.67 ng/ml

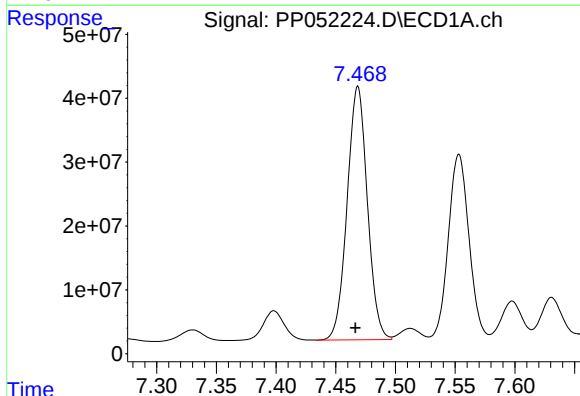


#32 AR-1260-2

R.T.: 7.469 min
Delta R.T.: 0.002 min
Response: 468808473
Conc: 4966.98 ng/ml

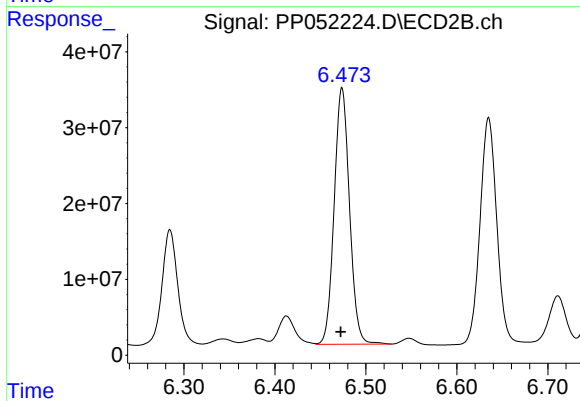

#32 AR-1260-2


R.T.: 6.474 min
Delta R.T.: 0.001 min
Response: 395820188
Conc: 4782.39 ng/ml

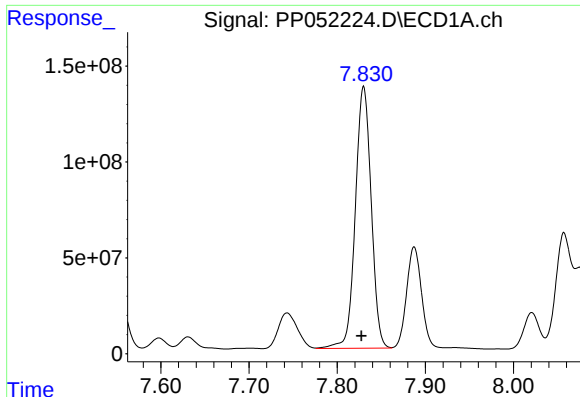

#33 AR-1260-3


R.T.: 7.830 min
Delta R.T.: 0.003 min
Response: 1705675908
Conc: 28400.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

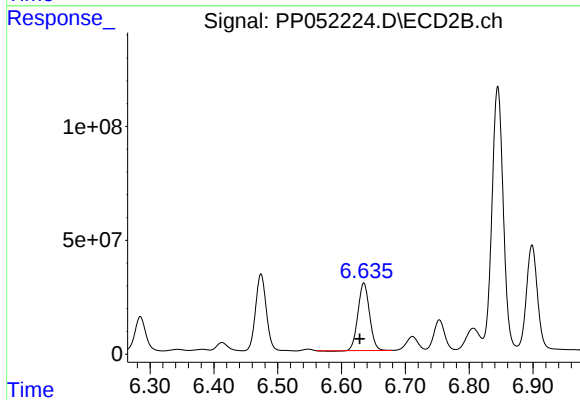


#33 AR-1260-3

R.T.: 6.635 min
Delta R.T.: 0.006 min
Response: 371960483
Conc: 4817.66 ng/ml

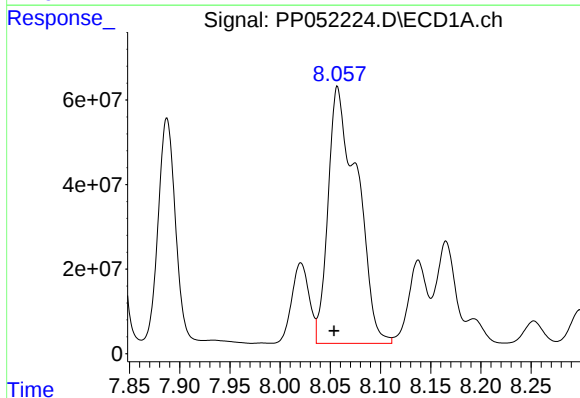


#34 AR-1260-4

R.T.: 8.057 min
Delta R.T.: 0.003 min
Response: 1225434862
Conc: 15978.26 ng/ml

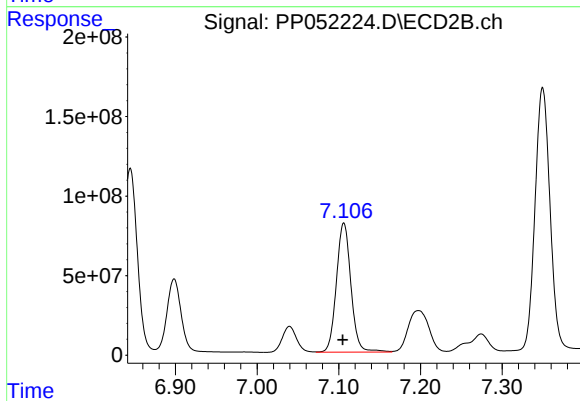

#34 AR-1260-4


R.T.: 7.106 min
Delta R.T.: 0.001 min
Response: 1004470648
Conc: 17868.52 ng/ml

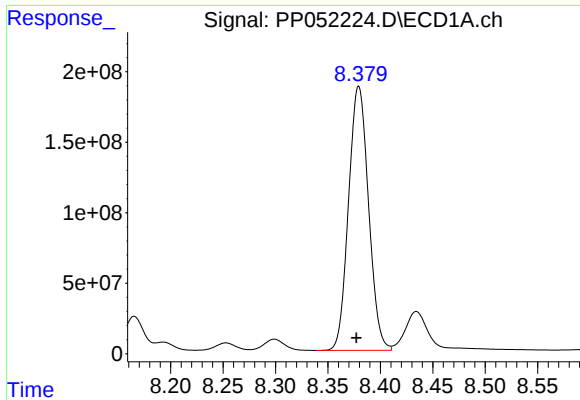

#35 AR-1260-5


R.T.: 8.379 min
Delta R.T.: 0.002 min
Response: 2486520497
Conc: 18139.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

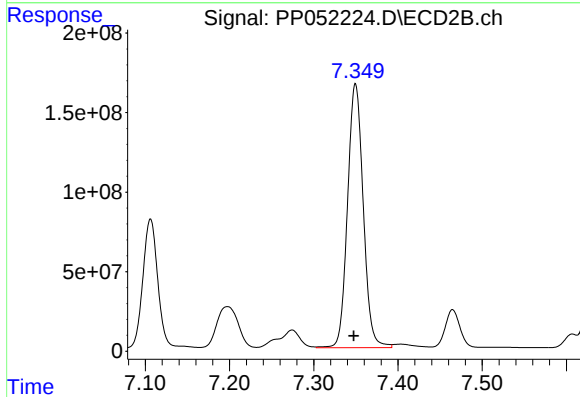


#35 AR-1260-5

R.T.: 7.350 min
Delta R.T.: 0.002 min
Response: 2148204314
Conc: 16289.44 ng/ml

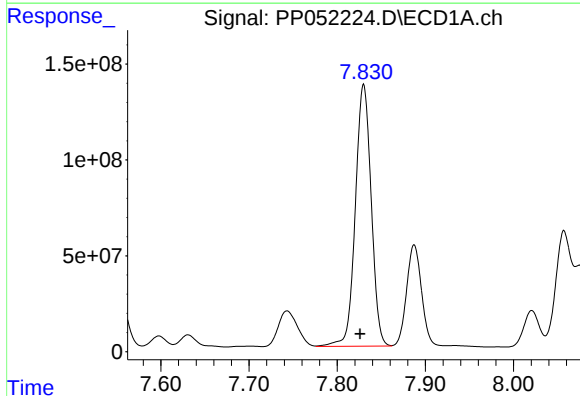


#36 AR-1262-1

R.T.: 7.830 min
Delta R.T.: 0.004 min
Response: 1705675908
Conc: 17590.81 ng/ml

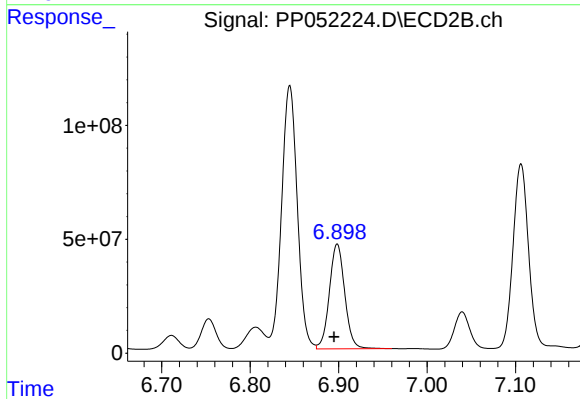

#36 AR-1262-1


R.T.: 6.898 min
Delta R.T.: 0.004 min
Response: 555268066
Conc: 15436.30 ng/ml

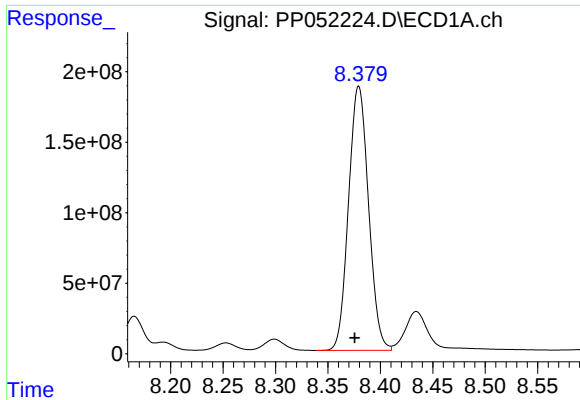

#37 AR-1262-2


R.T.: 8.379 min
Delta R.T.: 0.004 min
Response: 2486520497
Conc: 15443.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

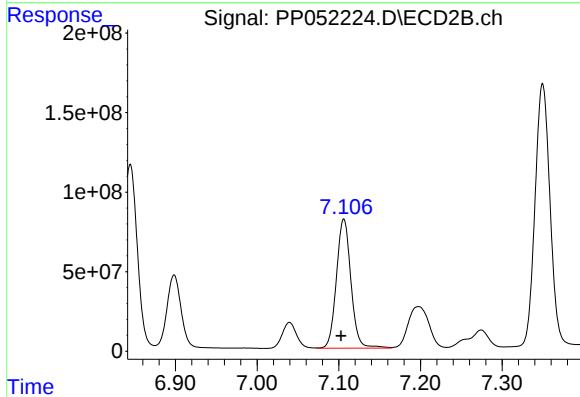


#37 AR-1262-2

R.T.: 7.106 min
Delta R.T.: 0.003 min
Response: 1004470648
Conc: 12685.29 ng/ml

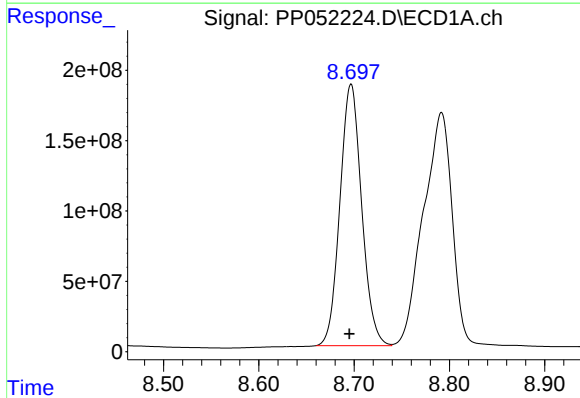


#38 AR-1262-3

R.T.: 8.697 min
Delta R.T.: 0.002 min
Response: 2947236209
Conc: 26817.48 ng/ml

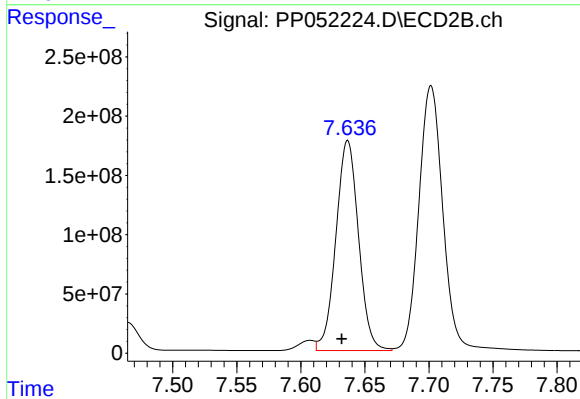

#38 AR-1262-3


R.T.: 7.637 min
Delta R.T.: 0.005 min
Response: 2177944051
Conc: 35269.16 ng/ml

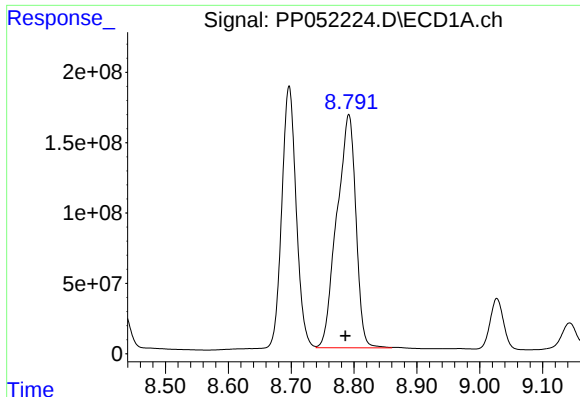

#39 AR-1262-4


R.T.: 8.792 min
Delta R.T.: 0.006 min
Response: 3486071482
Conc: 68195.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

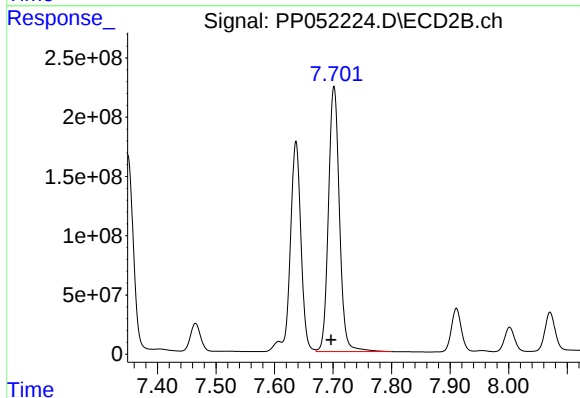


#39 AR-1262-4

R.T.: 7.702 min
Delta R.T.: 0.005 min
Response: 2922287163
Conc: 25597.43 ng/ml

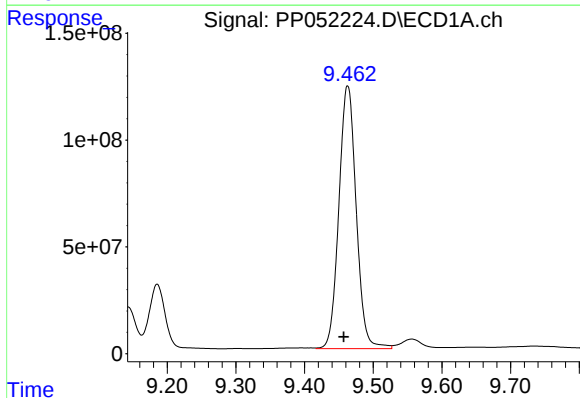


#40 AR-1262-5

R.T.: 9.463 min
Delta R.T.: 0.006 min
Response: 2157783716
Conc: 34278.28 ng/ml

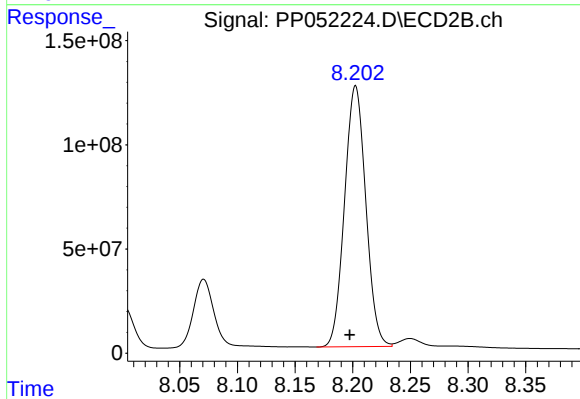

#40 AR-1262-5


R.T.: 8.202 min
Delta R.T.: 0.005 min
Response: 1600171545
Conc: 31481.72 ng/ml

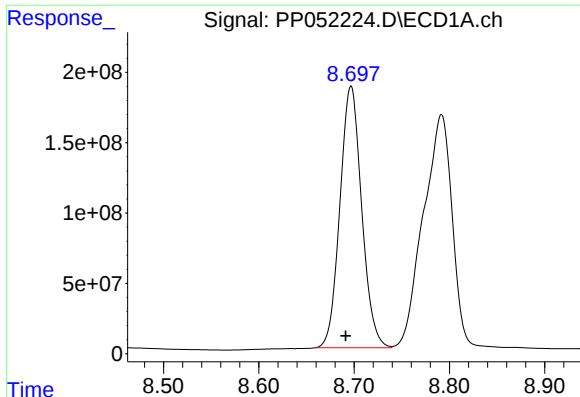

#41 AR-1268-1


R.T.: 8.697 min
Delta R.T.: 0.005 min
Response: 2947236209
Conc: 14886.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

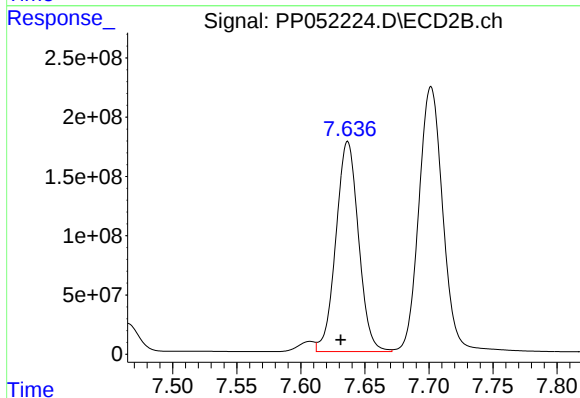


#41 AR-1268-1

R.T.: 7.637 min
Delta R.T.: 0.005 min
Response: 2177944051
Conc: 12005.64 ng/ml

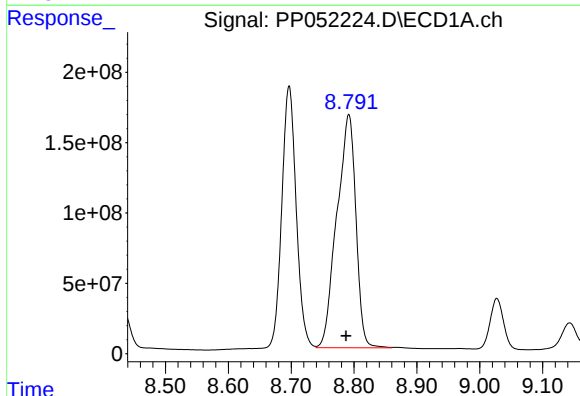


#42 AR-1268-2

R.T.: 8.792 min
Delta R.T.: 0.004 min
Response: 3486071482
Conc: 18985.02 ng/ml

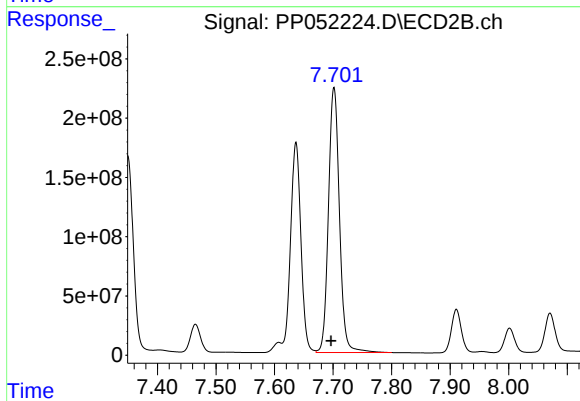

#42 AR-1268-2


R.T.: 7.702 min
Delta R.T.: 0.005 min
Response: 2922287163
Conc: 17885.67 ng/ml

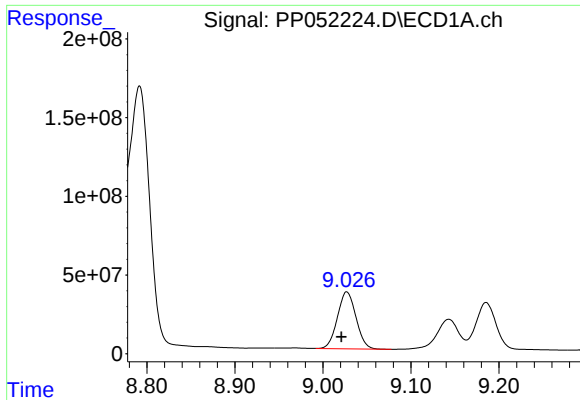

#43 AR-1268-3


R.T.: 9.027 min
Delta R.T.: 0.006 min
Response: 531317455
Conc: 3259.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

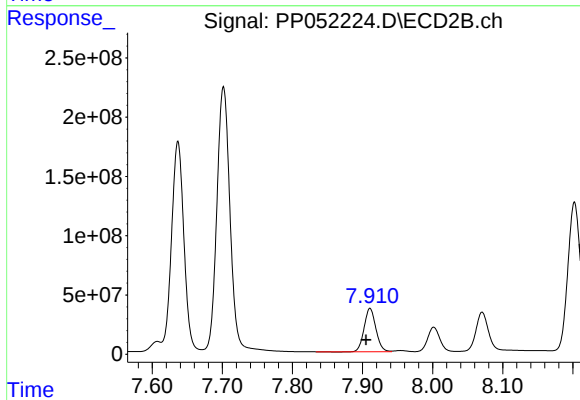


#43 AR-1268-3

R.T.: 7.911 min
Delta R.T.: 0.006 min
Response: 424521966
Conc: 3018.88 ng/ml

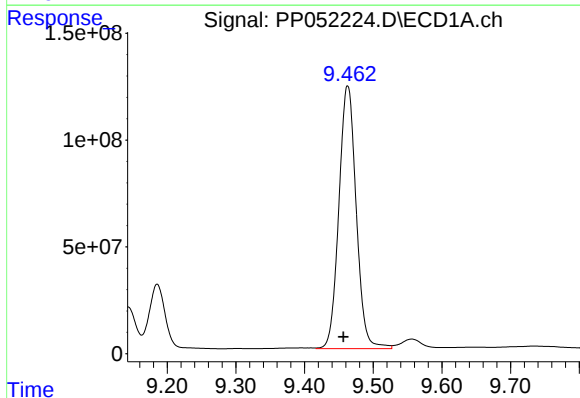


#44 AR-1268-4

R.T.: 9.463 min
Delta R.T.: 0.006 min
Response: 2157783716
Conc: 29574.11 ng/ml

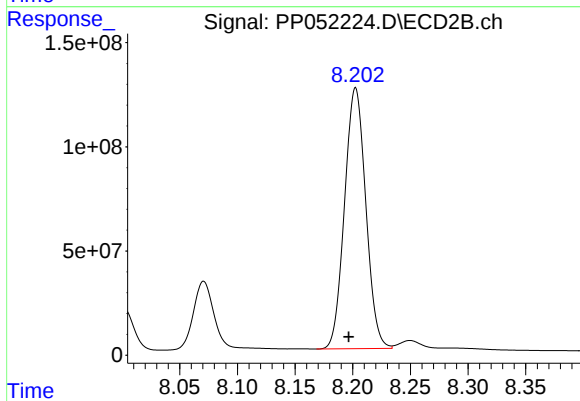

#44 AR-1268-4


R.T.: 8.202 min
Delta R.T.: 0.006 min
Response: 1600171545
Conc: 28315.95 ng/ml

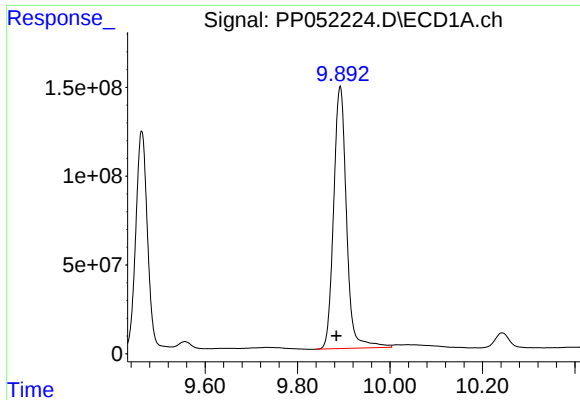

#45 AR-1268-5

R.T.: 9.892 min
Delta R.T.: 0.008 min
Response: 2856851294
Conc: 5478.74 ng/m

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

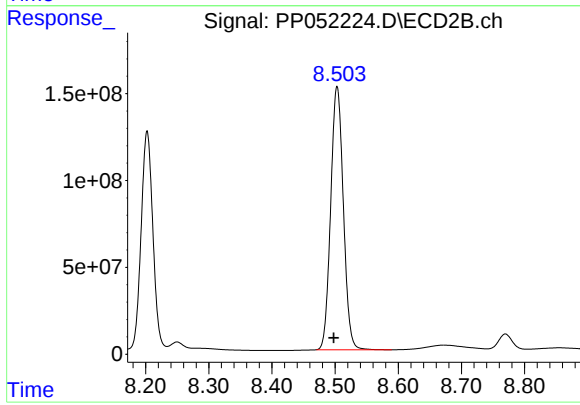

#45 AR-1268-5

R.T.: 8.503 min
Delta R.T.: 0.005 min
Response: 2109574190
Conc: 5014.92 ng/ml