

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 18:13
 Operator : YP\AJ
 Sample : N5098-03DL 25X (Sig #1); N5028-03DL 25X (Sig #2)
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-3DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 19:01:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.423	3.674	1390815	1204497	0.885	1.051
2)	SA Decachlor...	10.242	8.768	9966815	7258400	7.182	6.496
Target Compounds							
3)	L1 AR-1016-1	5.620f	4.778	512820	1089427	11.277	24.495 #
4)	L1 AR-1016-2	5.620	4.778f	512820	1089427	7.790	17.121 #
5)	L1 AR-1016-3	5.683	4.976	309888	256915	7.447	7.729
6)	L1 AR-1016-4	5.761f	5.018	1556496	1075072	42.838	39.445
8)	L2 AR-1221-1	4.632	3.885	183620	2410520	8.886	154.169 #
9)	L2 AR-1221-2	4.709	3.978	198370	2002306	12.963	166.959 #
10)	L2 AR-1221-3	4.797	4.057	488852	1449053	10.440	38.340 #
11)	L3 AR-1232-1	4.797	4.057	488852	1449053	13.569	49.999 #
12)	L3 AR-1232-2	5.312f	4.778f	2941701	1089427	144.985	36.369 #
13)	L3 AR-1232-3	5.620	4.976	512820	256915	17.028	16.817
14)	L3 AR-1232-4	5.761f	5.060	1556496	569798	93.328	40.238 #
15)	L3 AR-1232-5	5.873	5.235	1347426	125155	89.842	7.906 #
16)	L4 AR-1242-1	5.620f	4.778	512820	1089427	14.742	31.289 #
17)	L4 AR-1242-2	5.620	4.778f	512820	1089427	10.359	22.084 #
18)	L4 AR-1242-3	5.683	4.976	309888	256915	9.773	9.842
19)	L4 AR-1242-4	5.761f	5.060	1556496	569798	56.982	20.948 #
20)	L4 AR-1242-5	6.524	5.594	2449462	4716044	65.885	139.942 #
21)	L5 AR-1248-1	5.620f	4.778	512820	1089427	19.076	40.183 #
22)	L5 AR-1248-2	5.873	5.018	1347426	1075072	28.988	28.896
23)	L5 AR-1248-3	6.078	5.060	-587913	569798	N.D.	14.957 #
24)	L5 AR-1248-4	6.458f	5.235	8392214	125155	132.176	2.701 #
25)	L5 AR-1248-5	6.524	5.634	2449462	603262	39.549	14.345 #
26)	L6 AR-1254-1	6.458	5.594	8392214	4716044	117.885	67.408 #
27)	L6 AR-1254-2	6.676	5.742	10028399	4728744	94.029	75.473
28)	L6 AR-1254-3	7.045	6.165f	8399751	17882501	79.922	180.778 #
29)	L6 AR-1254-4	7.331	6.382	6631832	4878175	90.762	81.606
30)	L6 AR-1254-5	7.747	6.805	20674434	11970981	249.169	135.030 #
31)	L7 AR-1260-1	7.209	6.283	15031135	13170401	181.348	191.201
32)	L7 AR-1260-2	7.466	6.472	24809569	20099247	262.855	242.844
33)	L7 AR-1260-3	7.828	6.633	73305895	19515760	1220.566	252.770 #
34)	L7 AR-1260-4	8.056	7.104	31381804	44283450	409.183	787.758 #
35)	L7 AR-1260-5	8.378	7.348	90355593	92042654	659.154	697.943
36)	L8 AR-1262-1	7.828	6.897	73305895	23476900	756.011	652.652
37)	L8 AR-1262-2	8.378	7.104	90355593	44283450	561.182	559.248
38)	L8 AR-1262-3	8.695	7.635	117.9E6	104.4E6	1072.477	1691.167 #
39)	L8 AR-1262-4	8.791	7.700	130.9E6	129.8E6	2559.955	1137.278 #
40)	L8 AR-1262-5	9.462	8.201	79565157	67730773	1263.962	1332.533
41)	L9 AR-1268-1	8.695	7.635	117.9E6	104.4E6	595.341	575.674
42)	L9 AR-1268-2	8.791	7.700	130.9E6	129.8E6	712.667	794.649

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 18:13
Operator : YP\AJ
Sample : N5098-03DL 25X (Sig #1); N5028-03DL 25X (Sig #2)
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 19:01:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	9.025	7.909	24569279	21479533	150.719	152.746
44)	L9 AR-1268-4	9.462	8.201	79565157	67730773	1090.503	1198.535
45)	L9 AR-1268-5	9.888	8.502	118.1E6	95588195	226.485	227.234



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 18:13
Operator : YP\AJ
Sample : N5098-03DL 25X (Sig #1); N5028-03DL 25X (Sig #2)
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 19:01:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

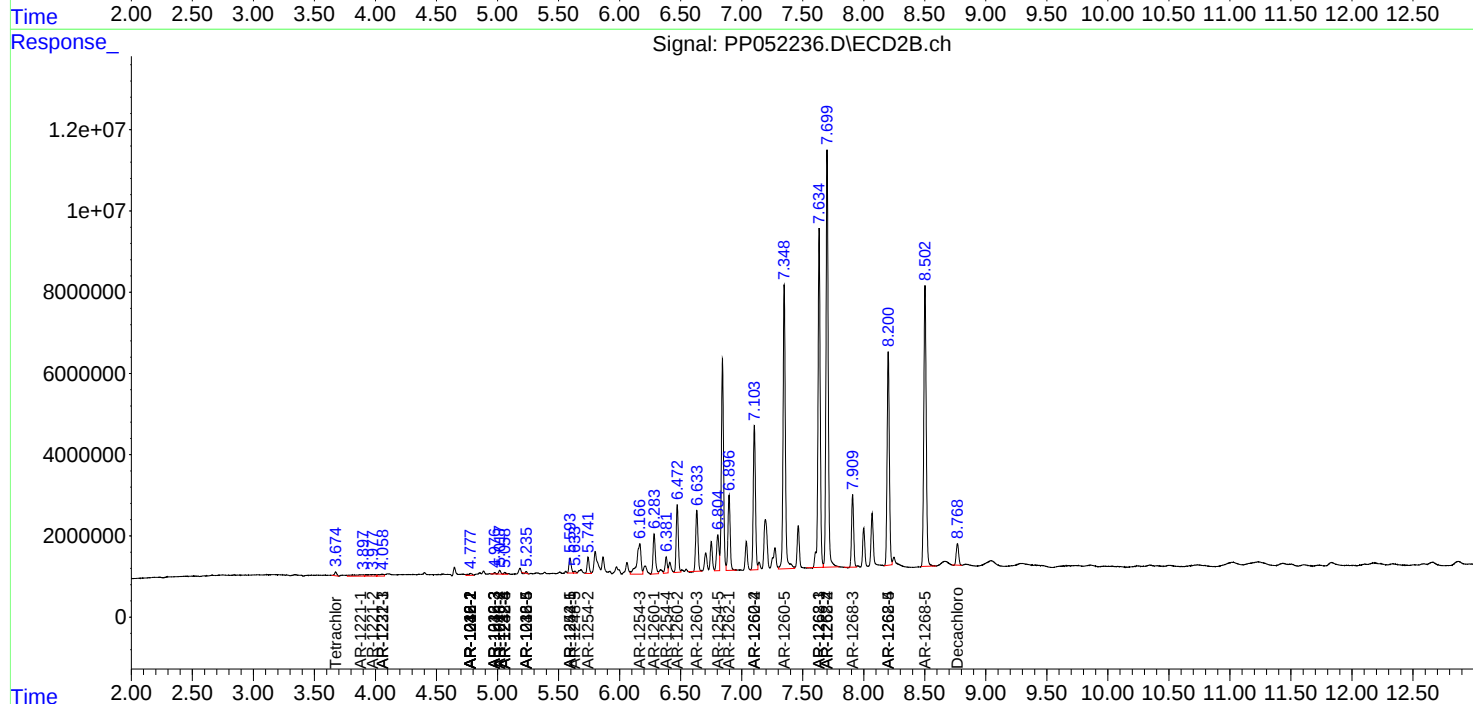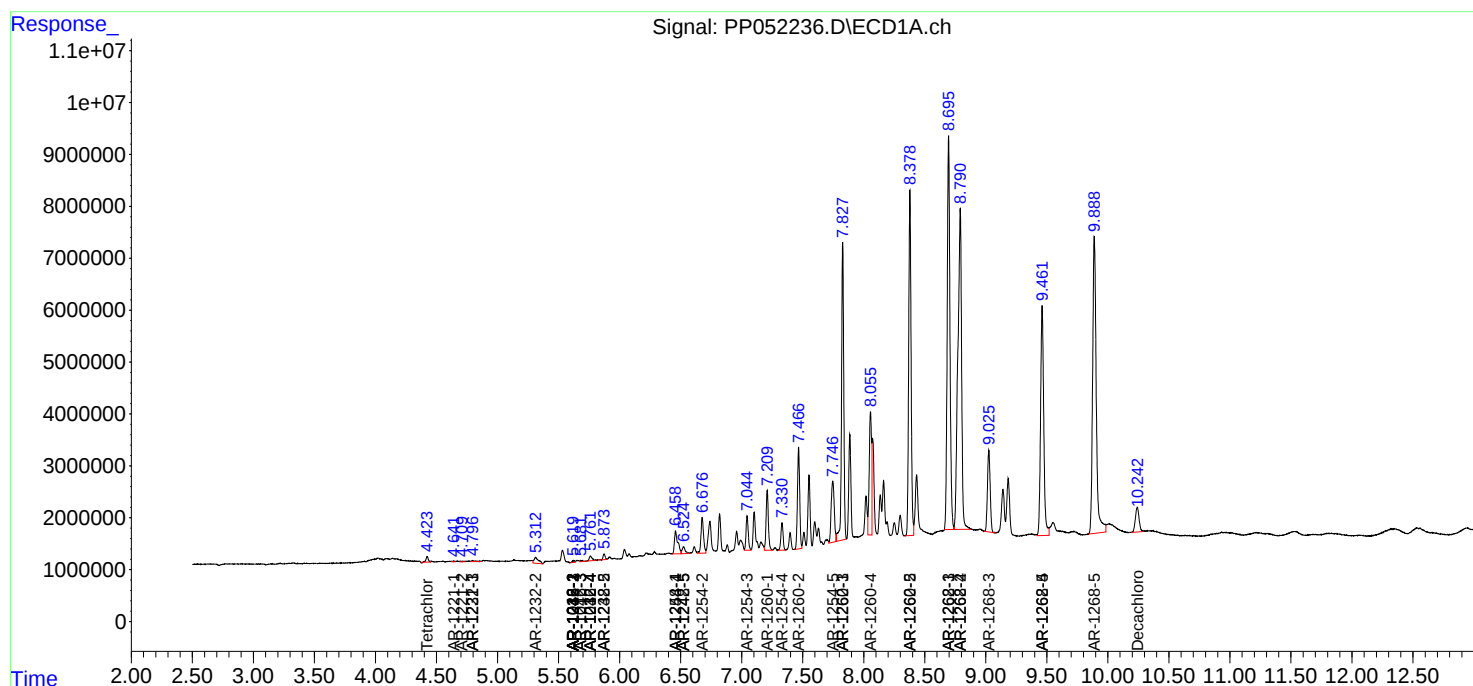


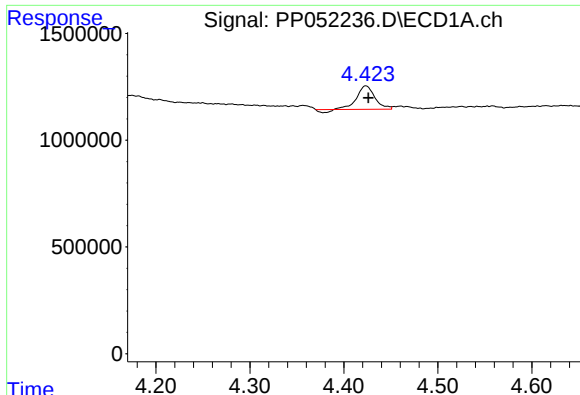

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 1390815
Conc: 0.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

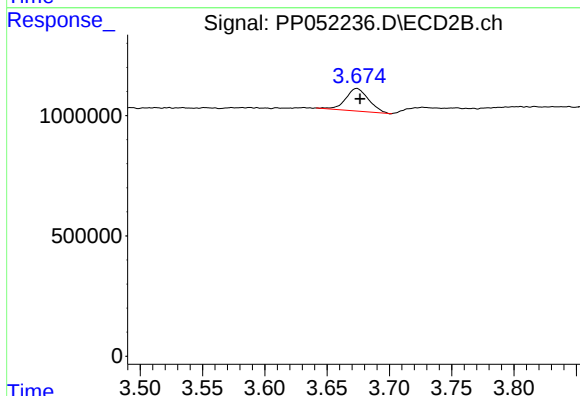


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 1204497
Conc: 1.05 ng/ml

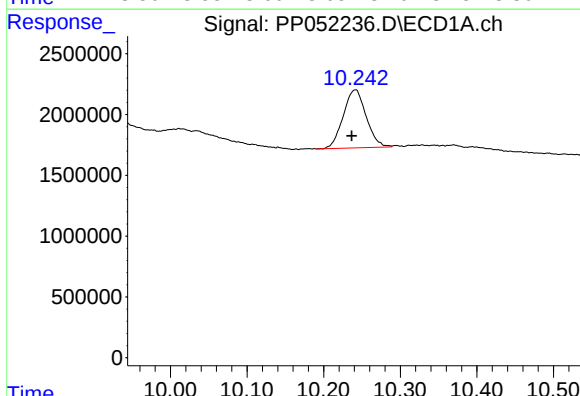


#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: 0.005 min
Response: 9966815
Conc: 7.18 ng/ml

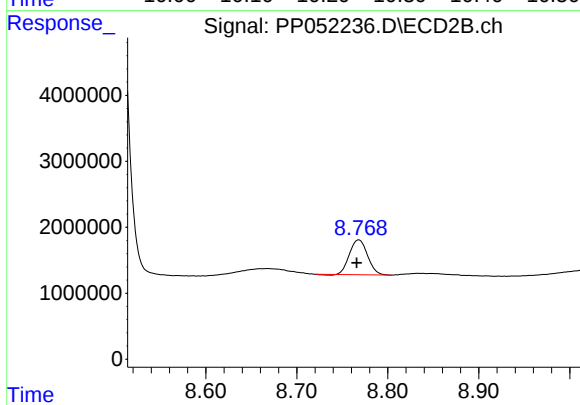

#2 Decachlorobiphenyl


R.T.: 8.768 min
Delta R.T.: 0.002 min
Response: 7258400
Conc: 6.50 ng/ml

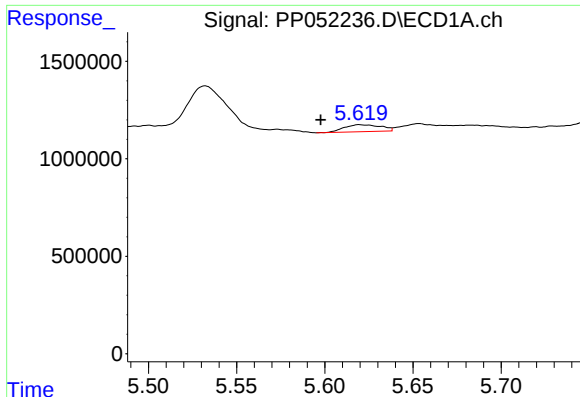

#3 AR-1016-1


R.T.: 5.620 min
Delta R.T.: 0.022 min
Response: 512820
Conc: 11.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

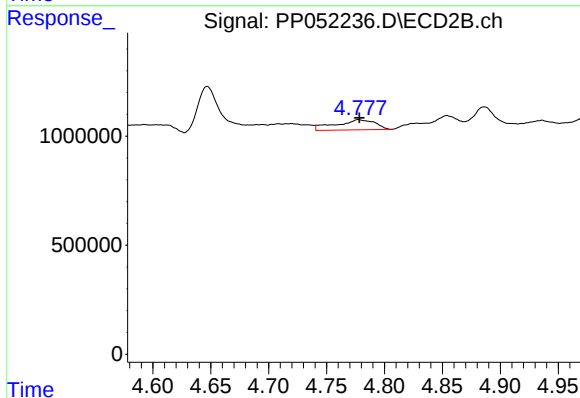


#3 AR-1016-1

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 1089427
Conc: 24.49 ng/ml

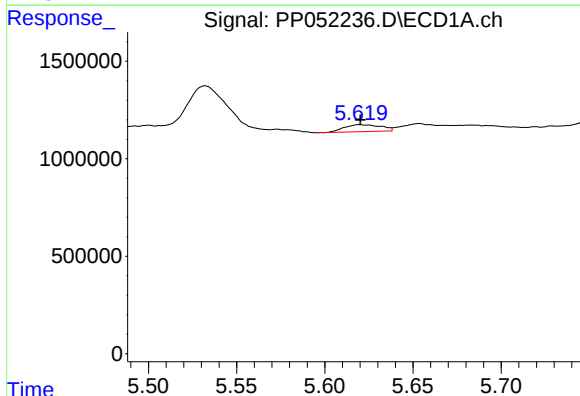


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 512820
Conc: 7.79 ng/ml

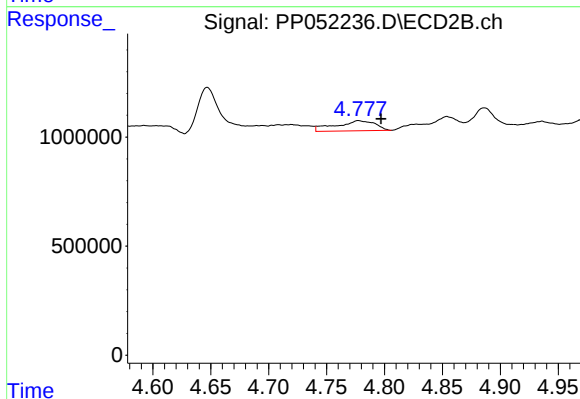

#4 AR-1016-2


R.T.: 4.778 min
Delta R.T.: -0.019 min
Response: 1089427
Conc: 17.12 ng/ml

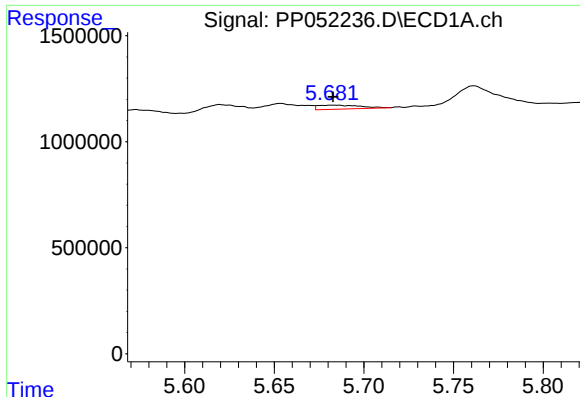

#5 AR-1016-3


R.T.: 5.683 min
Delta R.T.: 0.000 min
Response: 309888
Conc: 7.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

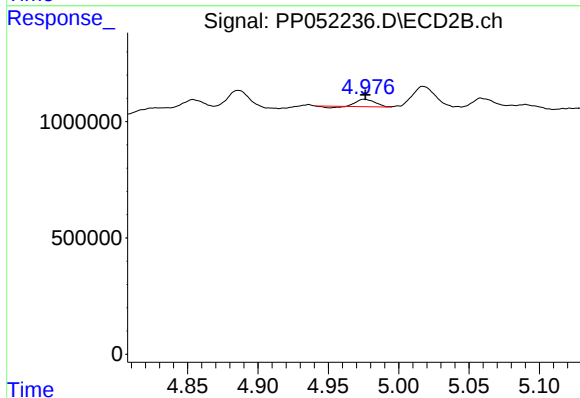


#5 AR-1016-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 256915
Conc: 7.73 ng/ml

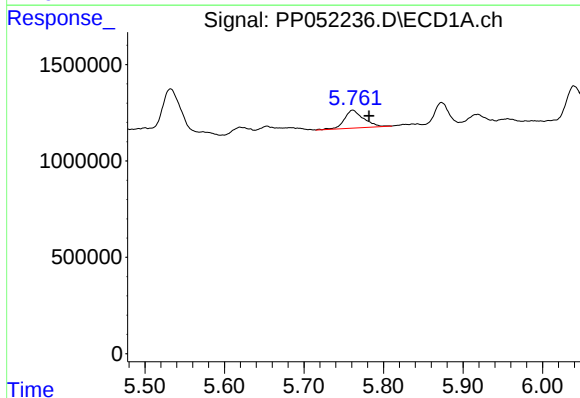


#6 AR-1016-4

R.T.: 5.761 min
Delta R.T.: -0.021 min
Response: 1556496
Conc: 42.84 ng/ml

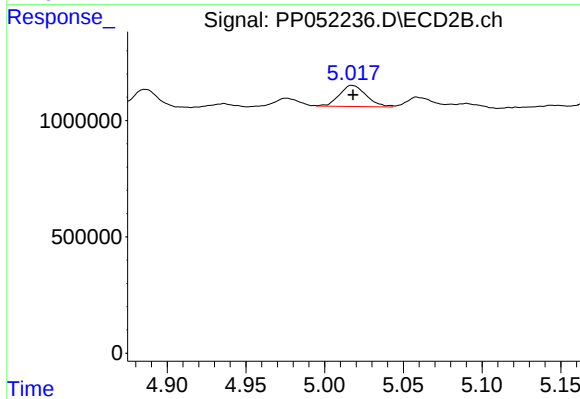

#6 AR-1016-4


R.T.: 5.018 min
Delta R.T.: 0.000 min
Response: 1075072
Conc: 39.44 ng/ml

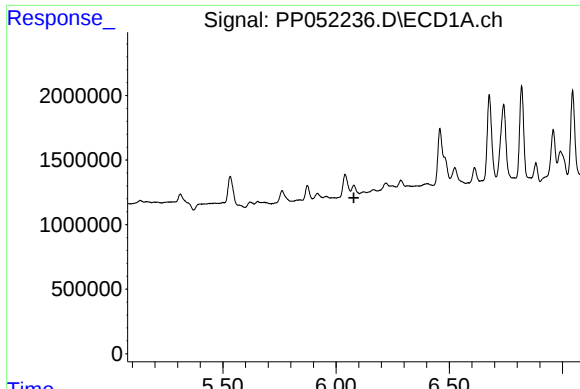

#7 AR-1016-5


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: -587913
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

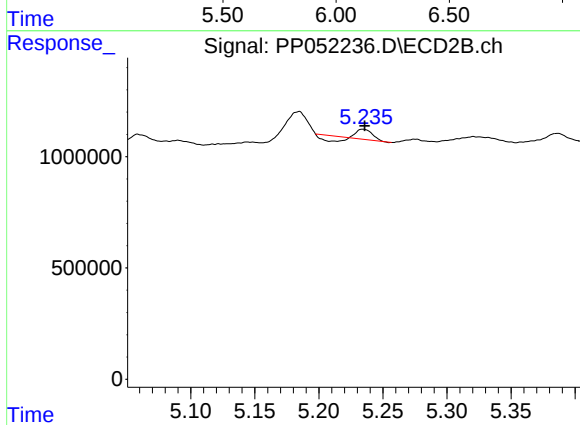


#7 AR-1016-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 125155
Conc: 3.54 ng/ml

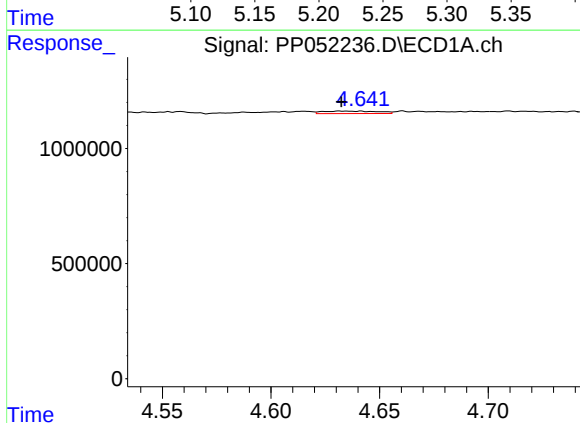


#8 AR-1221-1

R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 183620
Conc: 8.89 ng/ml

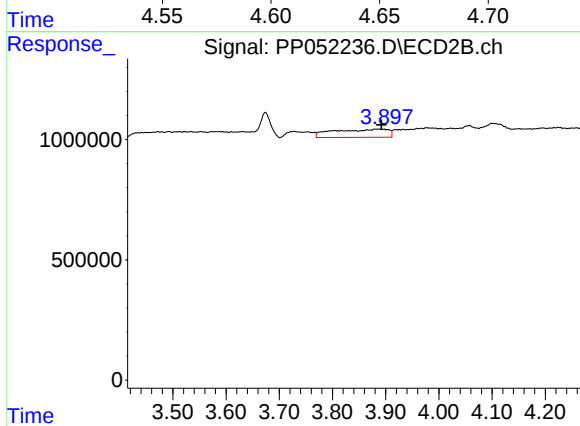

#8 AR-1221-1


R.T.: 3.885 min
Delta R.T.: -0.007 min
Response: 2410520
Conc: 154.17 ng/ml

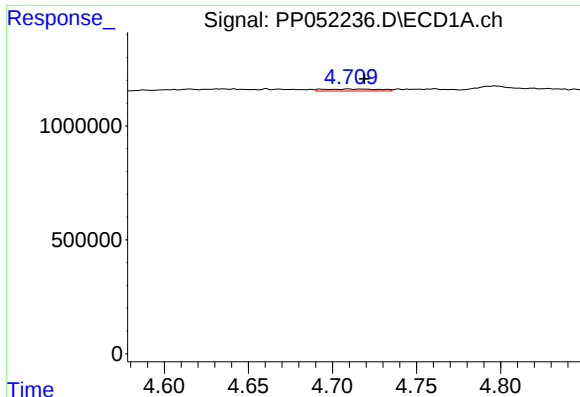

#9 AR-1221-2


R.T.: 4.709 min
Delta R.T.: -0.010 min
Response: 198370
Conc: 12.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

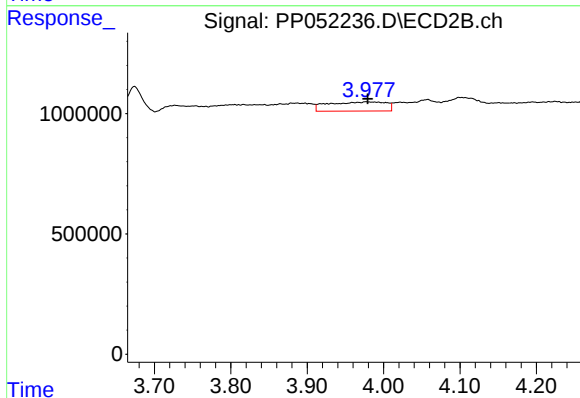


#9 AR-1221-2

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 2002306
Conc: 166.96 ng/ml

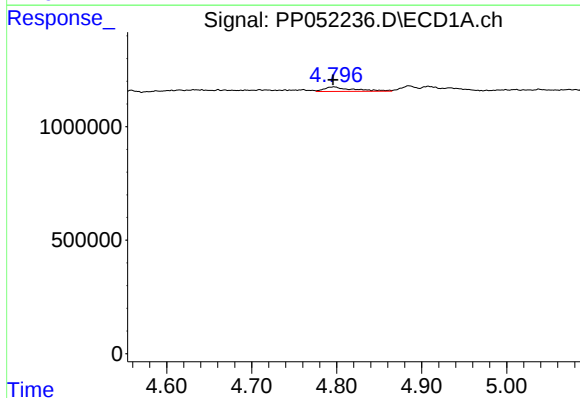


#10 AR-1221-3

R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 488852
Conc: 10.44 ng/ml

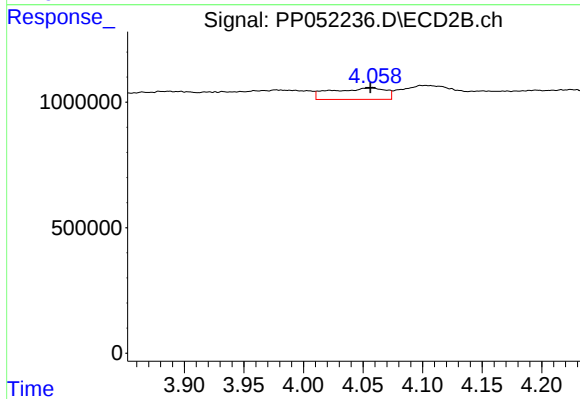

#10 AR-1221-3


R.T.: 4.057 min
Delta R.T.: 0.000 min
Response: 1449053
Conc: 38.34 ng/ml

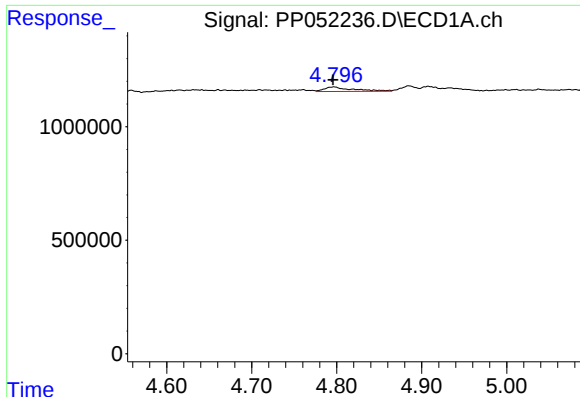

#11 AR-1232-1


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 488852
Conc: 13.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

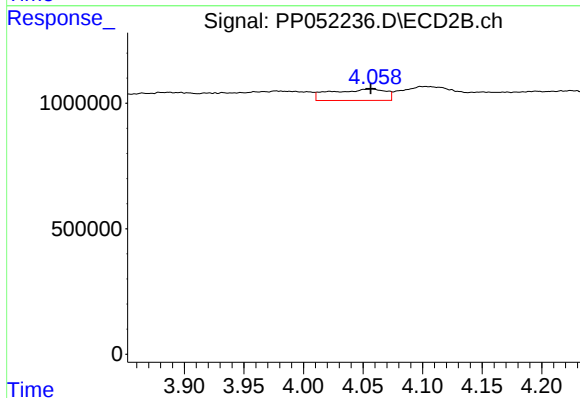


#11 AR-1232-1

R.T.: 4.057 min
Delta R.T.: 0.000 min
Response: 1449053
Conc: 50.00 ng/ml

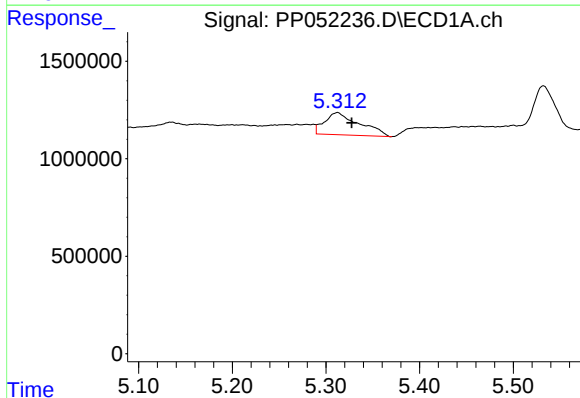


#12 AR-1232-2

R.T.: 5.312 min
Delta R.T.: -0.015 min
Response: 2941701
Conc: 144.98 ng/ml

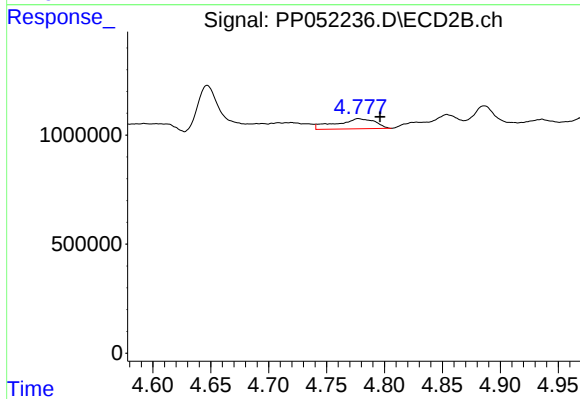

#12 AR-1232-2


R.T.: 4.778 min
Delta R.T.: -0.018 min
Response: 1089427
Conc: 36.37 ng/ml

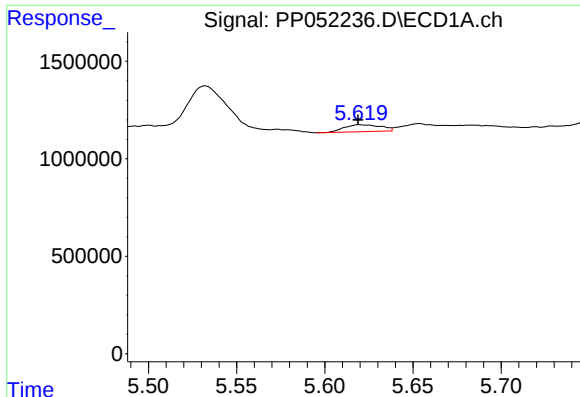

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.001 min
Response: 512820
Conc: 17.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

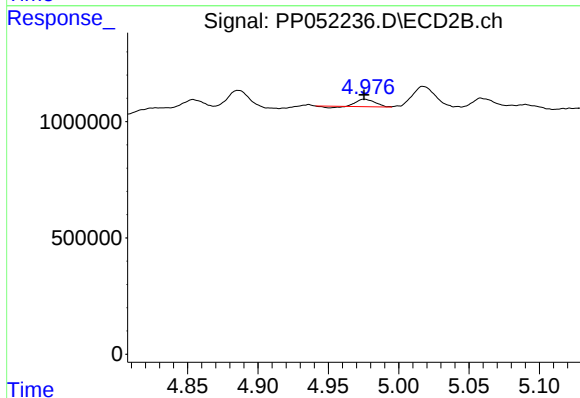


#13 AR-1232-3

R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 256915
Conc: 16.82 ng/ml

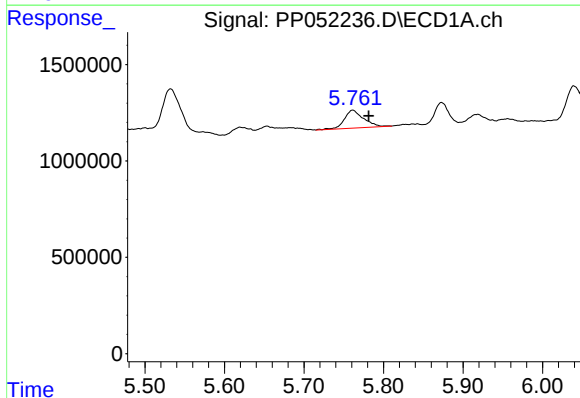


#14 AR-1232-4

R.T.: 5.761 min
Delta R.T.: -0.020 min
Response: 1556496
Conc: 93.33 ng/ml

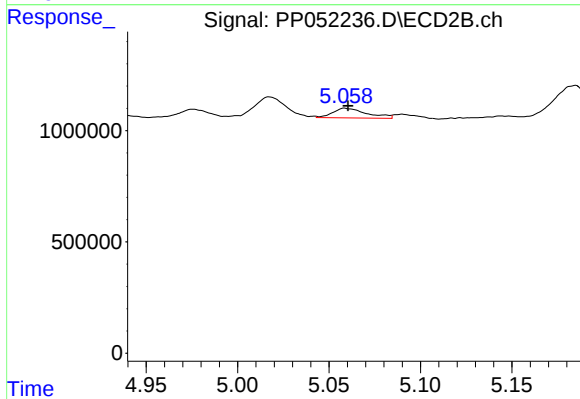

#14 AR-1232-4


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 569798
Conc: 40.24 ng/ml

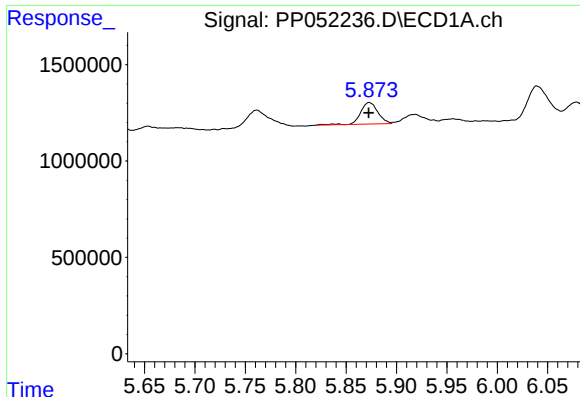

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: 0.000 min
Response: 1347426
Conc: 89.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

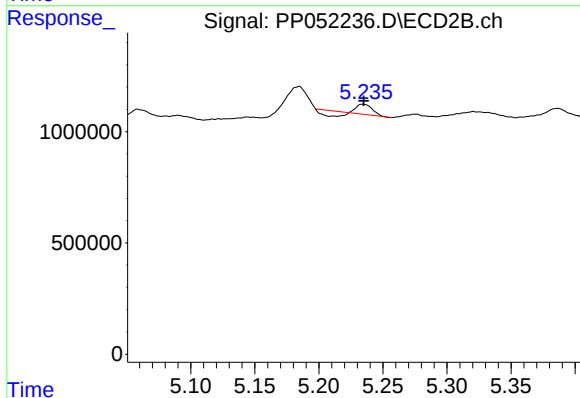


#15 AR-1232-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 125155
Conc: 7.91 ng/ml

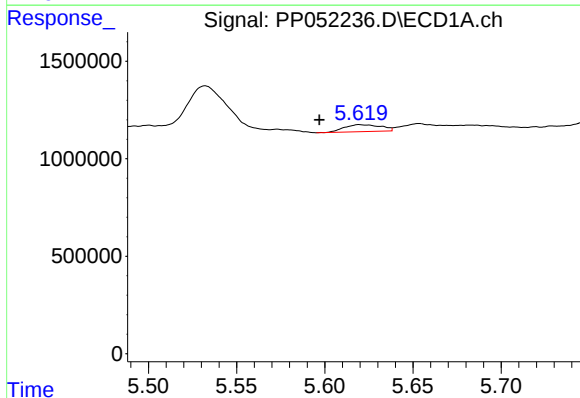


#16 AR-1242-1

R.T.: 5.620 min
Delta R.T.: 0.023 min
Response: 512820
Conc: 14.74 ng/ml

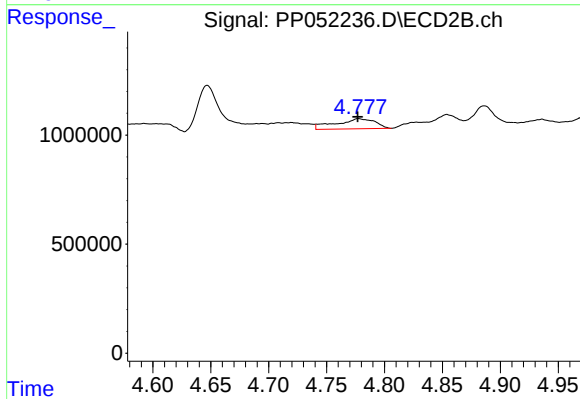

#16 AR-1242-1


R.T.: 4.778 min
Delta R.T.: 0.001 min
Response: 1089427
Conc: 31.29 ng/ml

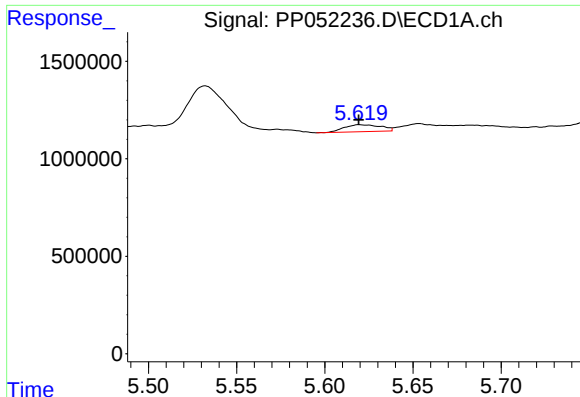

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 512820
Conc: 10.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

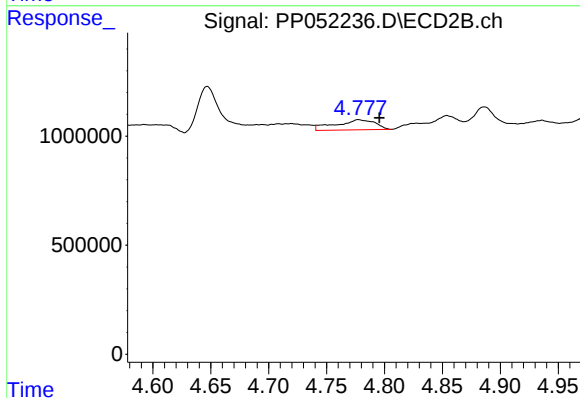


#17 AR-1242-2

R.T.: 4.778 min
Delta R.T.: -0.017 min
Response: 1089427
Conc: 22.08 ng/ml

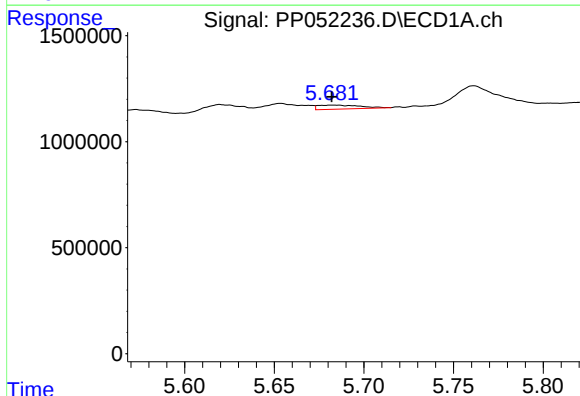


#18 AR-1242-3

R.T.: 5.683 min
Delta R.T.: 0.000 min
Response: 309888
Conc: 9.77 ng/ml

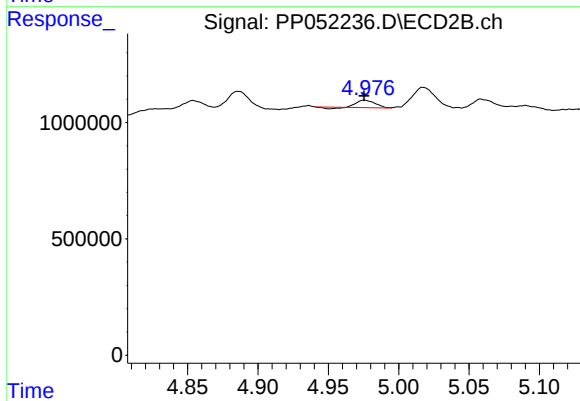

#18 AR-1242-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 256915
Conc: 9.84 ng/ml

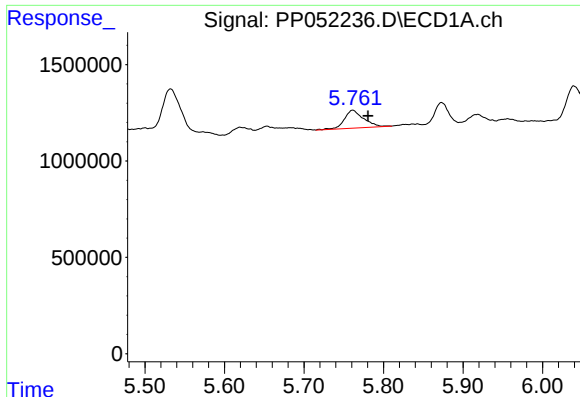

#19 AR-1242-4


R.T.: 5.761 min
Delta R.T.: -0.019 min
Response: 1556496
Conc: 56.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

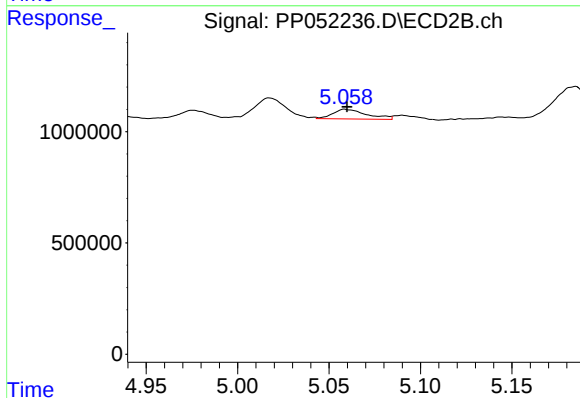


#19 AR-1242-4

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 569798
Conc: 20.95 ng/ml

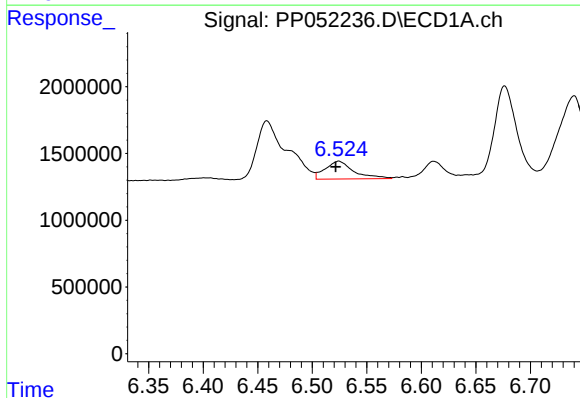


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: 0.003 min
Response: 2449462
Conc: 65.89 ng/ml

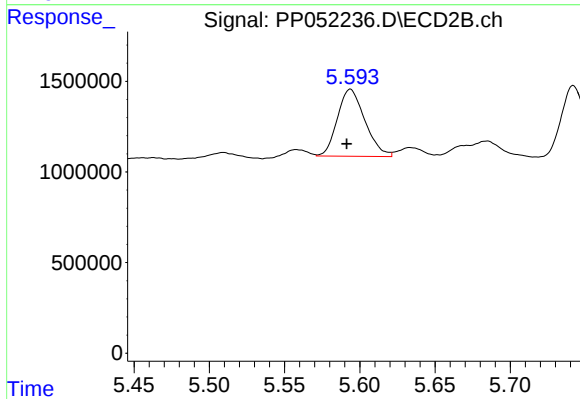

#20 AR-1242-5


R.T.: 5.594 min
Delta R.T.: 0.003 min
Response: 4716044
Conc: 139.94 ng/ml

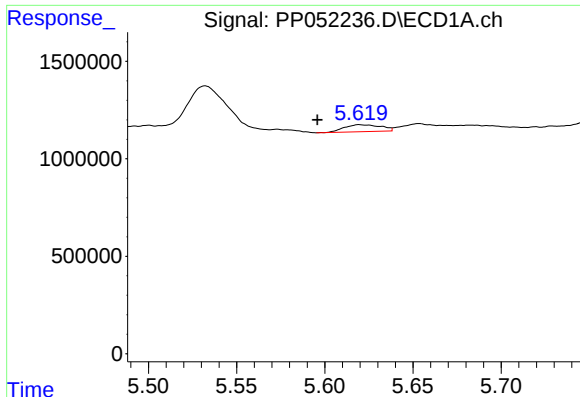

#21 AR-1248-1


R.T.: 5.620 min
Delta R.T.: 0.024 min
Response: 512820
Conc: 19.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

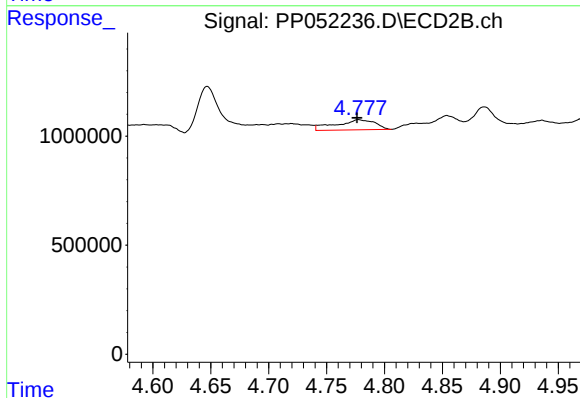


#21 AR-1248-1

R.T.: 4.778 min
Delta R.T.: 0.002 min
Response: 1089427
Conc: 40.18 ng/ml

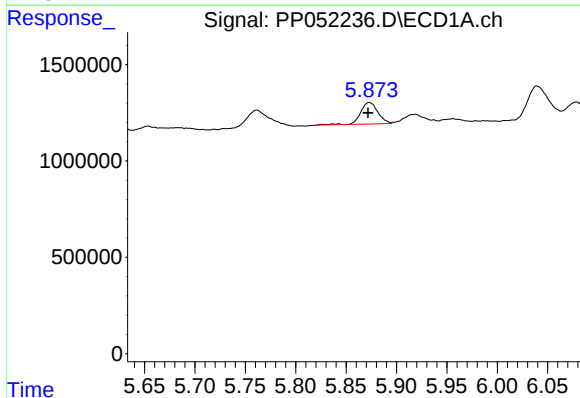


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: 0.001 min
Response: 1347426
Conc: 28.99 ng/ml

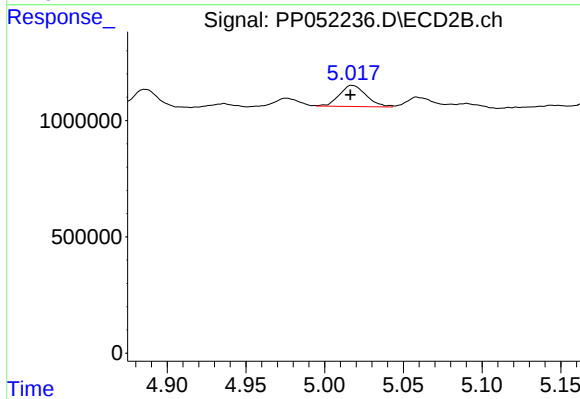

#22 AR-1248-2


R.T.: 5.018 min
Delta R.T.: 0.002 min
Response: 1075072
Conc: 28.90 ng/ml

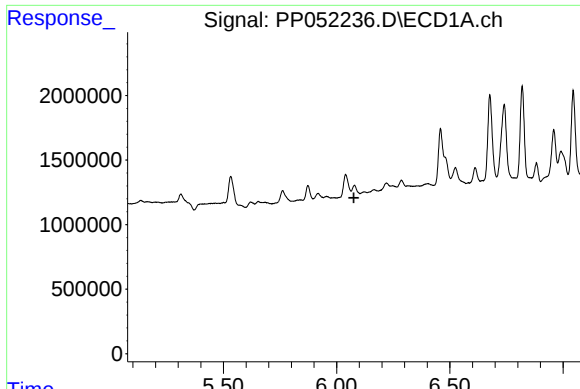

#23 AR-1248-3


R.T.: 6.078 min
Delta R.T.: 0.002 min
Response: -587913
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

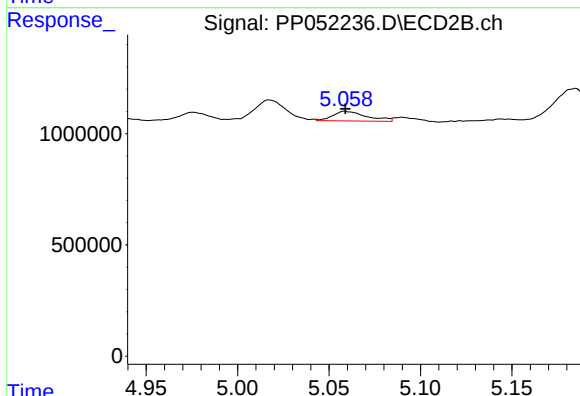


#23 AR-1248-3

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 569798
Conc: 14.96 ng/ml

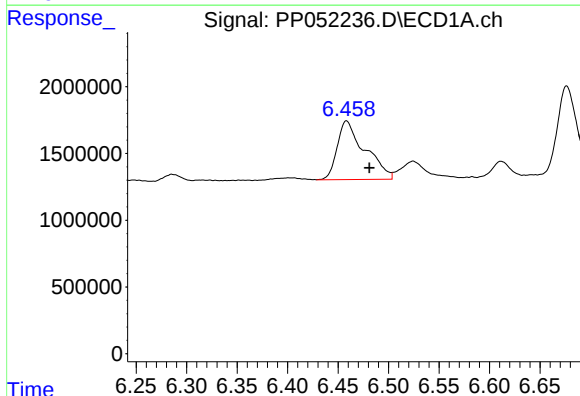


#24 AR-1248-4

R.T.: 6.458 min
Delta R.T.: -0.023 min
Response: 8392214
Conc: 132.18 ng/ml

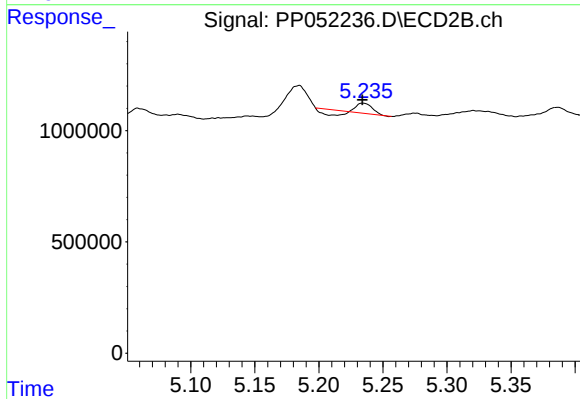

#24 AR-1248-4


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 125155
Conc: 2.70 ng/ml

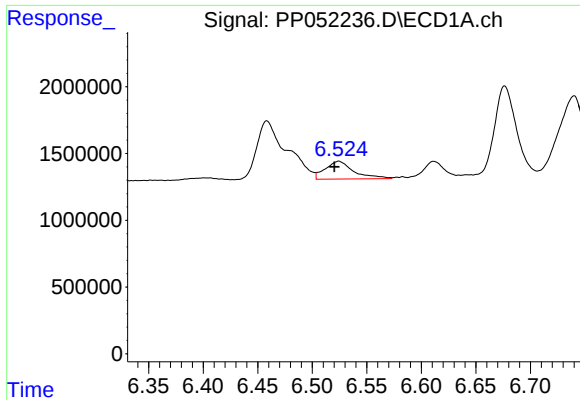

#25 AR-1248-5


R.T.: 6.524 min
Delta R.T.: 0.004 min
Response: 2449462
Conc: 39.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

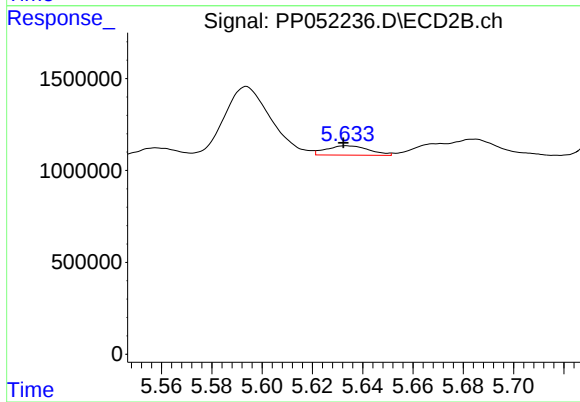


#25 AR-1248-5

R.T.: 5.634 min
Delta R.T.: 0.002 min
Response: 603262
Conc: 14.35 ng/ml

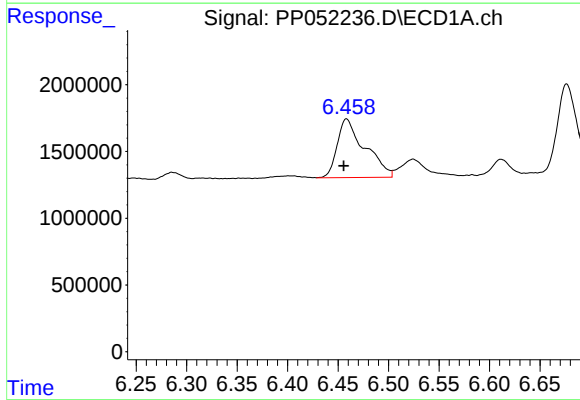


#26 AR-1254-1

R.T.: 6.458 min
Delta R.T.: 0.003 min
Response: 8392214
Conc: 117.89 ng/ml

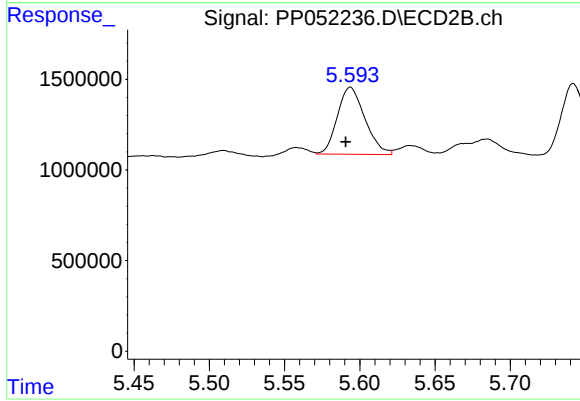

#26 AR-1254-1


R.T.: 5.594 min
Delta R.T.: 0.003 min
Response: 4716044
Conc: 67.41 ng/ml

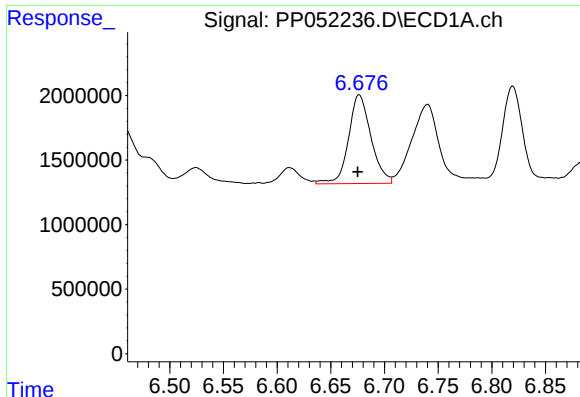

#27 AR-1254-2


R.T.: 6.676 min
Delta R.T.: 0.001 min
Response: 10028399
Conc: 94.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

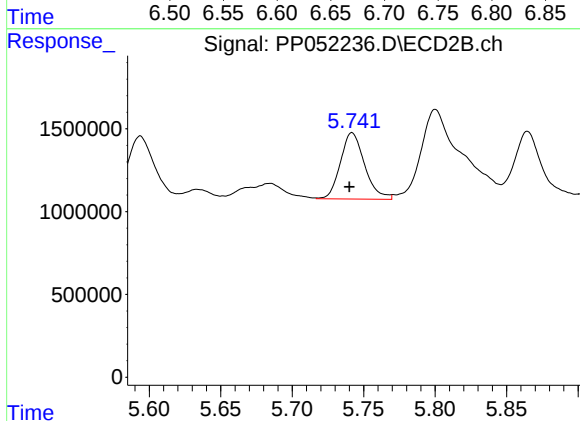


#27 AR-1254-2

R.T.: 5.742 min
Delta R.T.: 0.002 min
Response: 4728744
Conc: 75.47 ng/ml

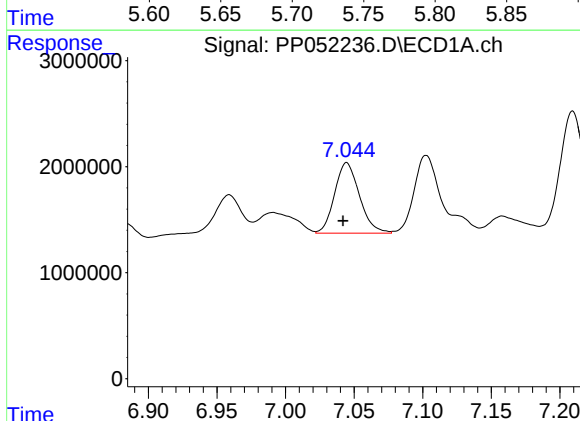


#28 AR-1254-3

R.T.: 7.045 min
Delta R.T.: 0.003 min
Response: 8399751
Conc: 79.92 ng/ml

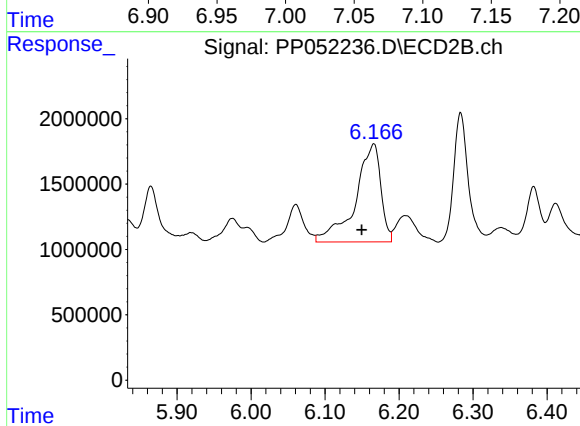

#28 AR-1254-3


R.T.: 6.165 min
Delta R.T.: 0.016 min
Response: 17882501
Conc: 180.78 ng/ml

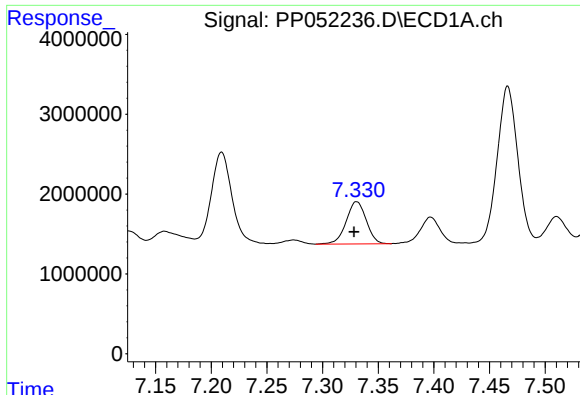

#29 AR-1254-4


R.T.: 7.331 min
Delta R.T.: 0.002 min
Response: 6631832
Conc: 90.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

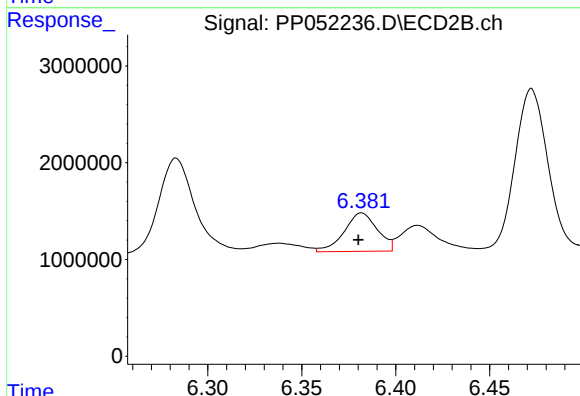


#29 AR-1254-4

R.T.: 6.382 min
Delta R.T.: 0.002 min
Response: 4878175
Conc: 81.61 ng/ml

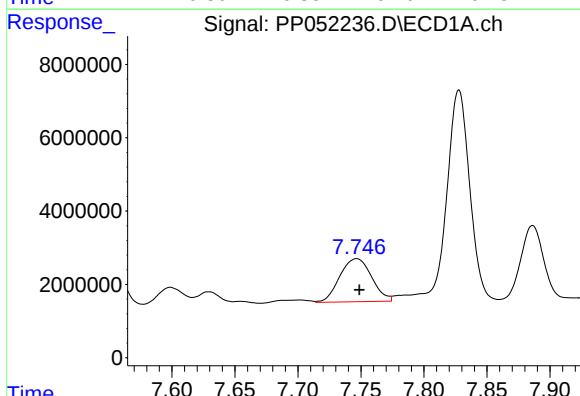


#30 AR-1254-5

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 20674434
Conc: 249.17 ng/ml

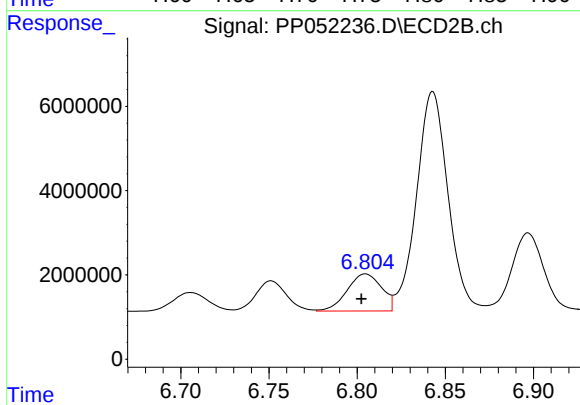

#30 AR-1254-5


R.T.: 6.805 min
Delta R.T.: 0.002 min
Response: 11970981
Conc: 135.03 ng/ml

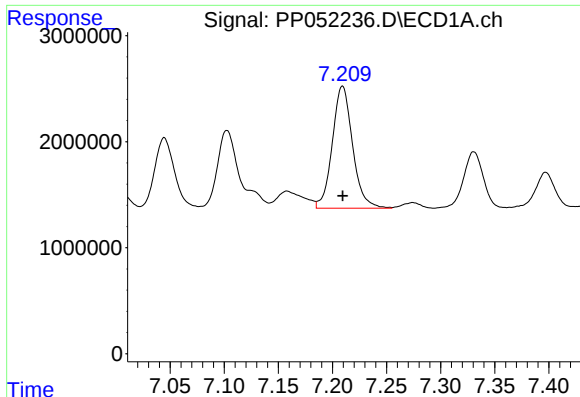

#31 AR-1260-1


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 15031135
Conc: 181.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

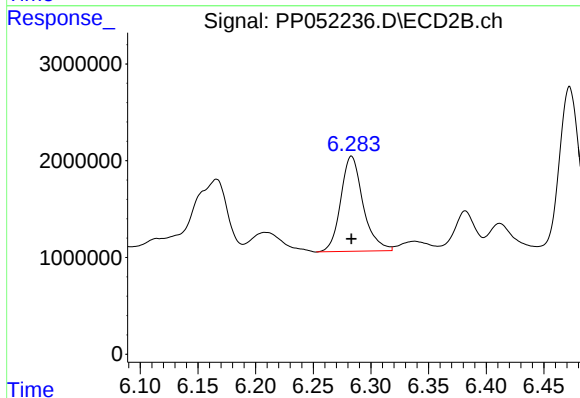


#31 AR-1260-1

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 13170401
Conc: 191.20 ng/ml

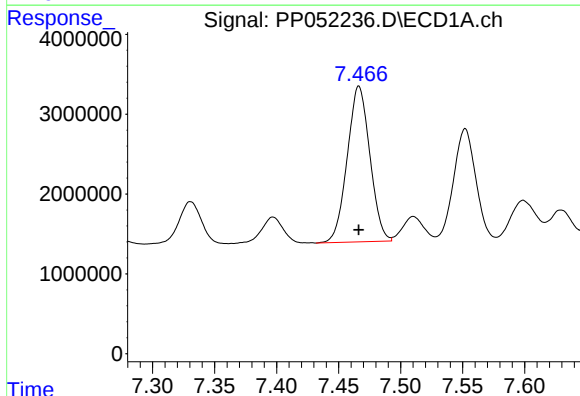


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 24809569
Conc: 262.86 ng/ml

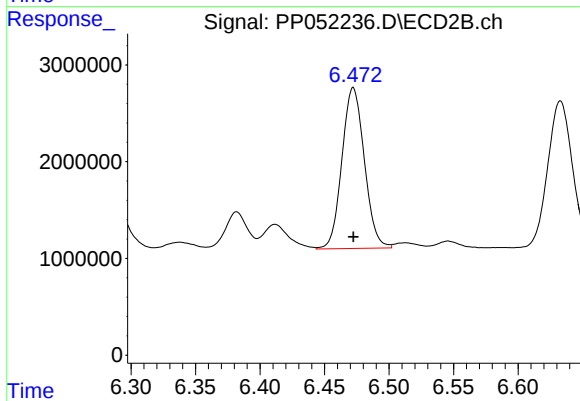

#32 AR-1260-2


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 20099247
Conc: 242.84 ng/ml

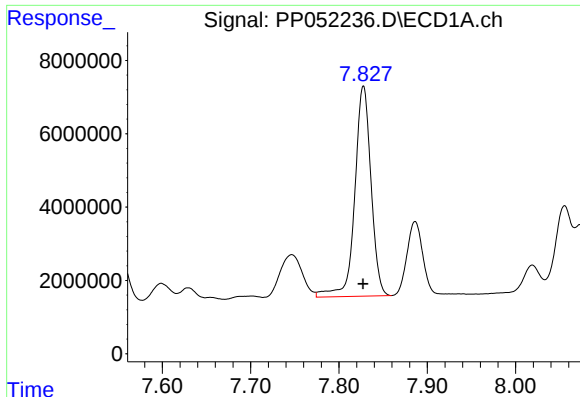

#33 AR-1260-3


R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 73305895
Conc: 1220.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

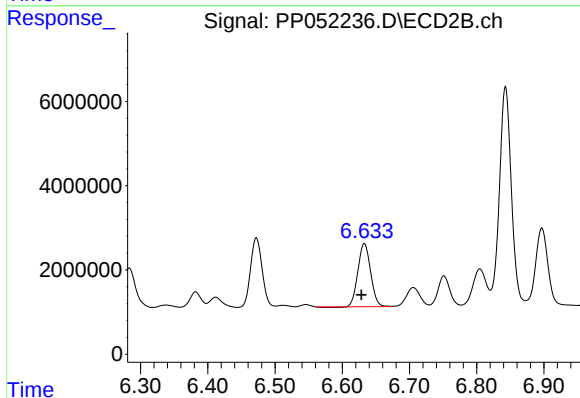


#33 AR-1260-3

R.T.: 6.633 min
Delta R.T.: 0.004 min
Response: 19515760
Conc: 252.77 ng/ml

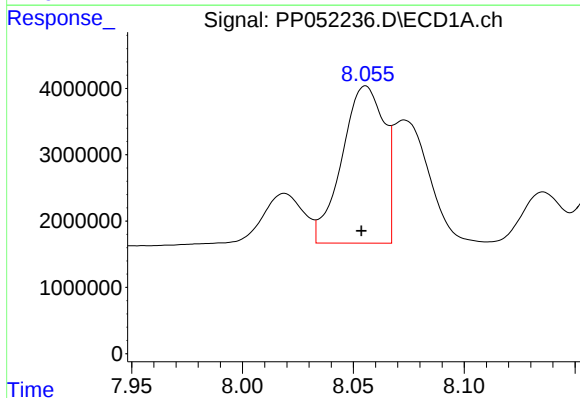


#34 AR-1260-4

R.T.: 8.056 min
Delta R.T.: 0.002 min
Response: 31381804
Conc: 409.18 ng/ml

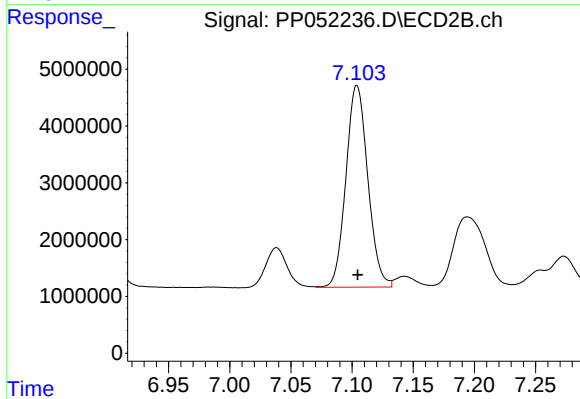

#34 AR-1260-4


R.T.: 7.104 min
Delta R.T.: 0.000 min
Response: 44283450
Conc: 787.76 ng/ml

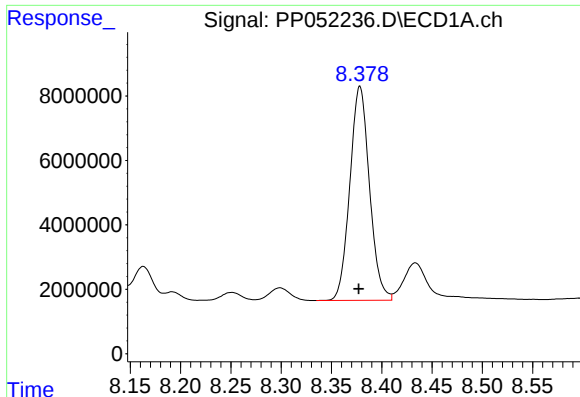

#35 AR-1260-5


R.T.: 8.378 min
Delta R.T.: 0.001 min
Response: 90355593
Conc: 659.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

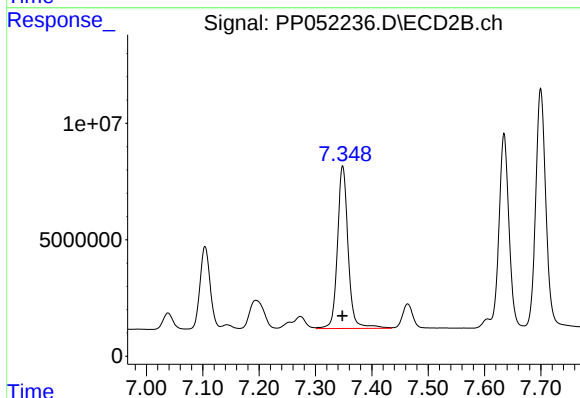


#35 AR-1260-5

R.T.: 7.348 min
Delta R.T.: 0.000 min
Response: 92042654
Conc: 697.94 ng/ml

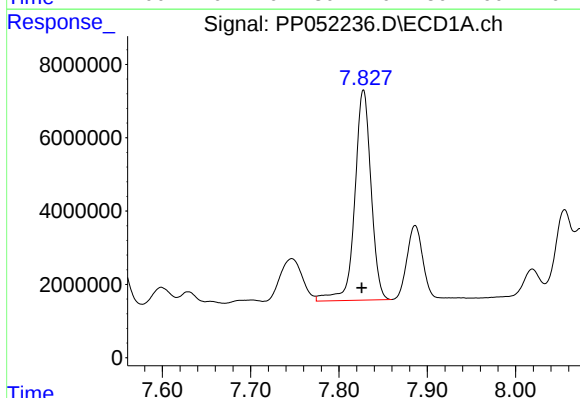


#36 AR-1262-1

R.T.: 7.828 min
Delta R.T.: 0.002 min
Response: 73305895
Conc: 756.01 ng/ml

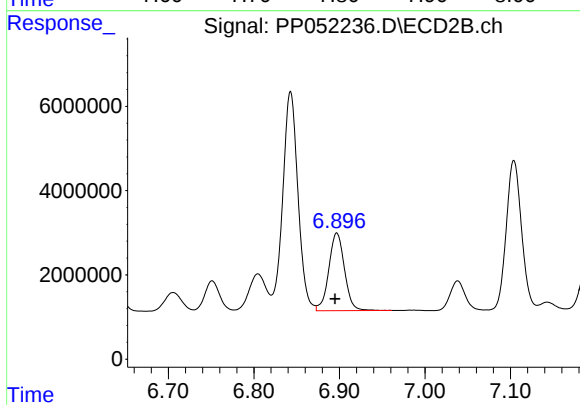

#36 AR-1262-1


R.T.: 6.897 min
Delta R.T.: 0.002 min
Response: 23476900
Conc: 652.65 ng/ml

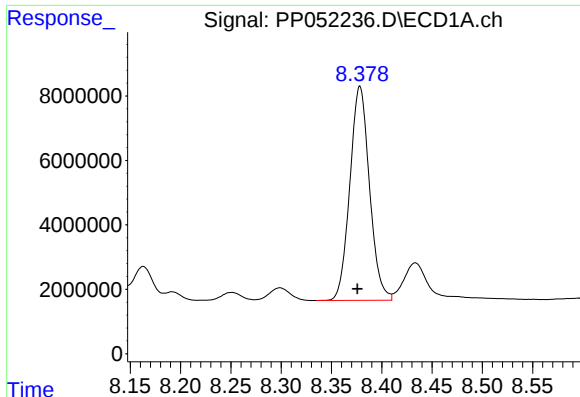

#37 AR-1262-2


R.T.: 8.378 min
Delta R.T.: 0.003 min
Response: 90355593
Conc: 561.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

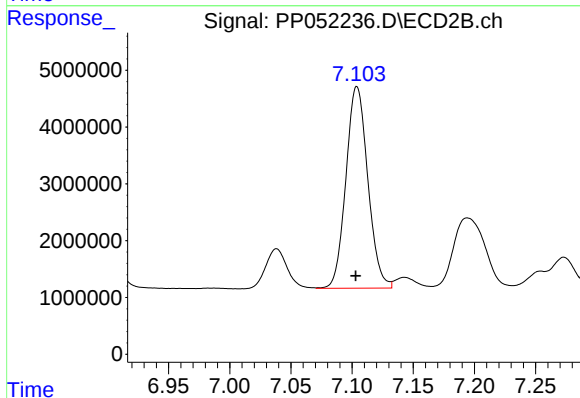


#37 AR-1262-2

R.T.: 7.104 min
Delta R.T.: 0.001 min
Response: 44283450
Conc: 559.25 ng/ml

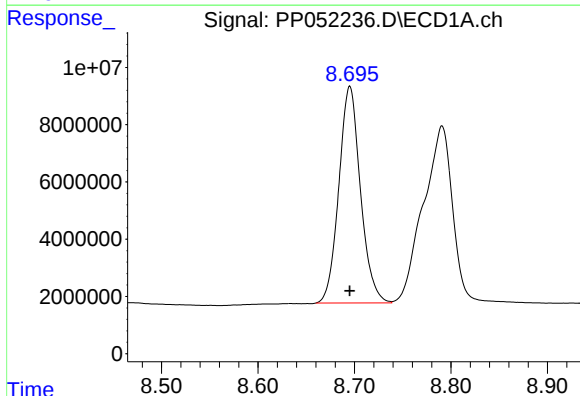


#38 AR-1262-3

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 117865000
Conc: 1072.48 ng/ml

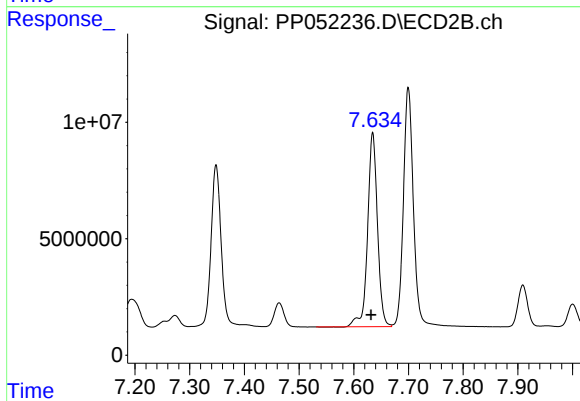

#38 AR-1262-3


R.T.: 7.635 min
Delta R.T.: 0.003 min
Response: 104433114
Conc: 1691.17 ng/ml

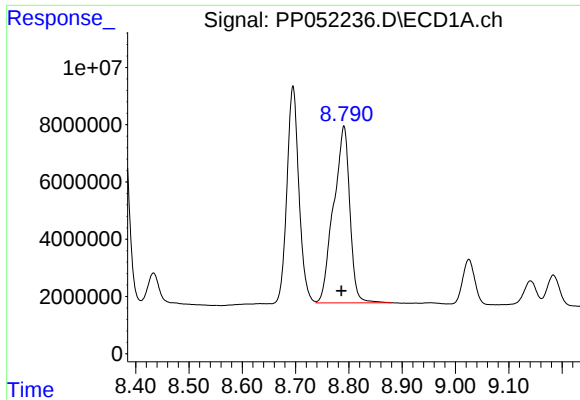

#39 AR-1262-4


R.T.: 8.791 min
Delta R.T.: 0.005 min
Response: 130861503
Conc: 2559.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

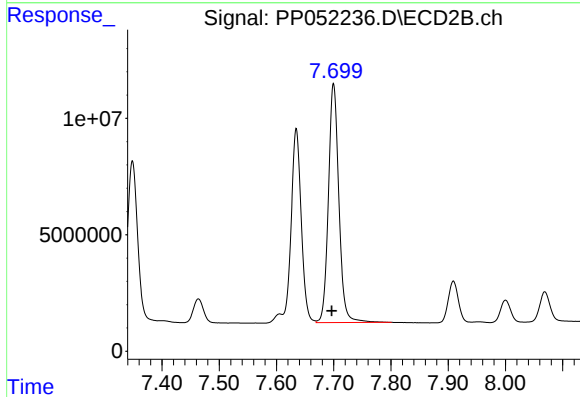


#39 AR-1262-4

R.T.: 7.700 min
Delta R.T.: 0.003 min
Response: 129835386
Conc: 1137.28 ng/ml

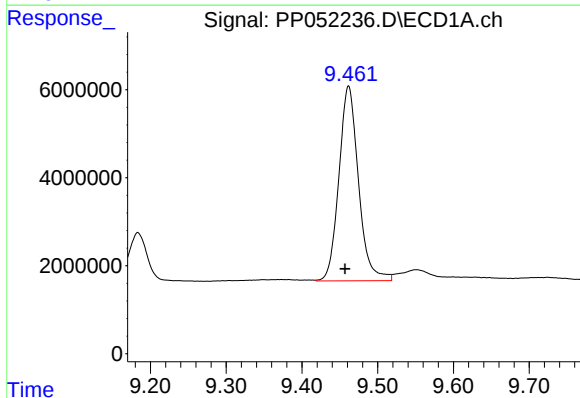


#40 AR-1262-5

R.T.: 9.462 min
Delta R.T.: 0.005 min
Response: 79565157
Conc: 1263.96 ng/ml

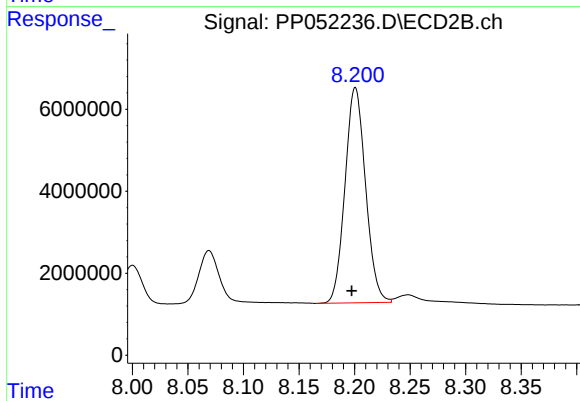

#40 AR-1262-5


R.T.: 8.201 min
Delta R.T.: 0.003 min
Response: 67730773
Conc: 1332.53 ng/ml

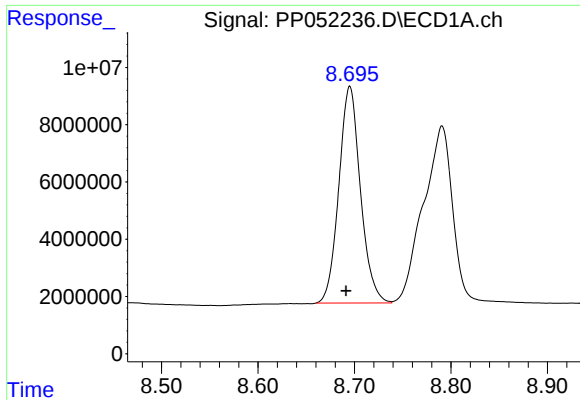

#41 AR-1268-1


R.T.: 8.695 min
Delta R.T.: 0.004 min
Response: 117865000
Conc: 595.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

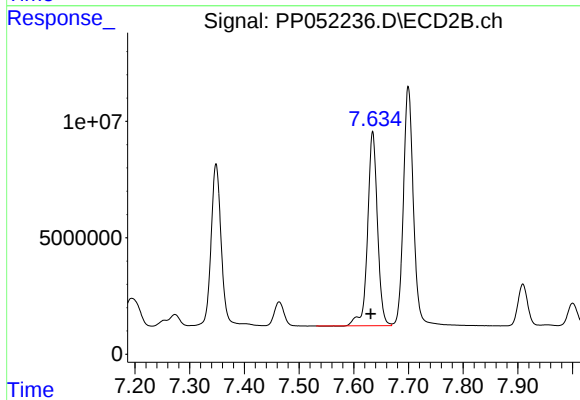


#41 AR-1268-1

R.T.: 7.635 min
Delta R.T.: 0.004 min
Response: 104433114
Conc: 575.67 ng/ml

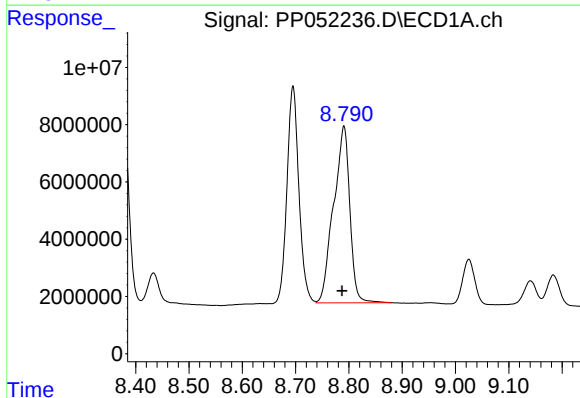


#42 AR-1268-2

R.T.: 8.791 min
Delta R.T.: 0.003 min
Response: 130861503
Conc: 712.67 ng/ml

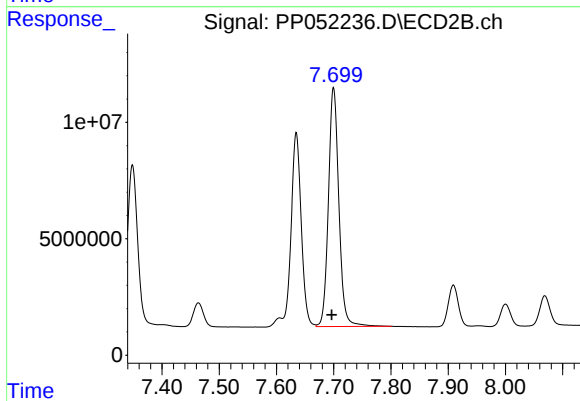

#42 AR-1268-2


R.T.: 7.700 min
Delta R.T.: 0.003 min
Response: 129835386
Conc: 794.65 ng/ml

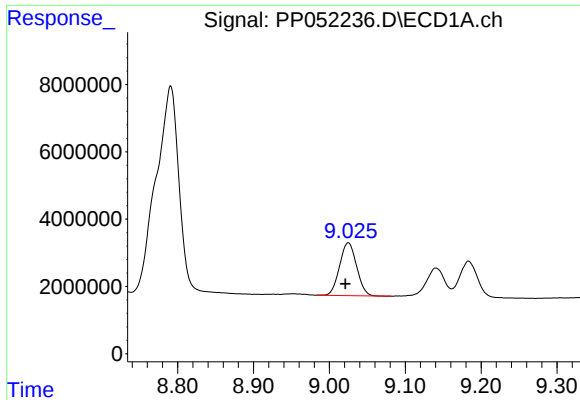

#43 AR-1268-3


R.T.: 9.025 min
Delta R.T.: 0.004 min
Response: 24569279
Conc: 150.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

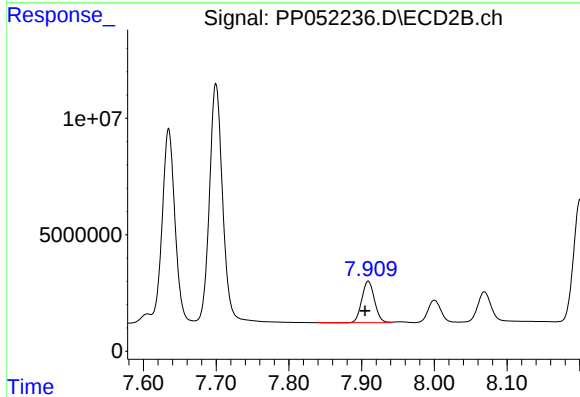


#43 AR-1268-3

R.T.: 7.909 min
Delta R.T.: 0.004 min
Response: 21479533
Conc: 152.75 ng/ml

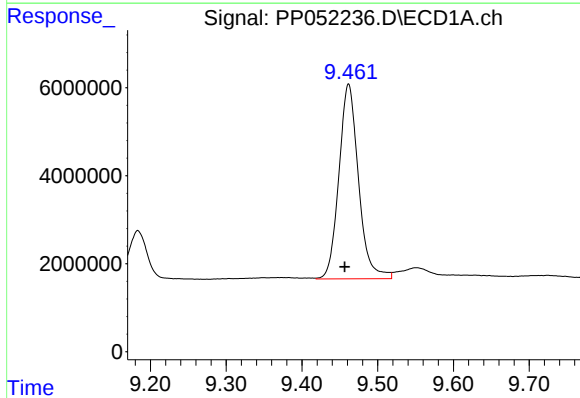


#44 AR-1268-4

R.T.: 9.462 min
Delta R.T.: 0.005 min
Response: 79565157
Conc: 1090.50 ng/ml

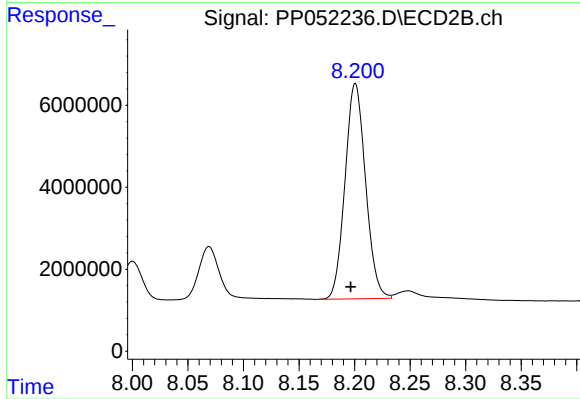

#44 AR-1268-4


R.T.: 8.201 min
Delta R.T.: 0.004 min
Response: 67730773
Conc: 1198.53 ng/ml

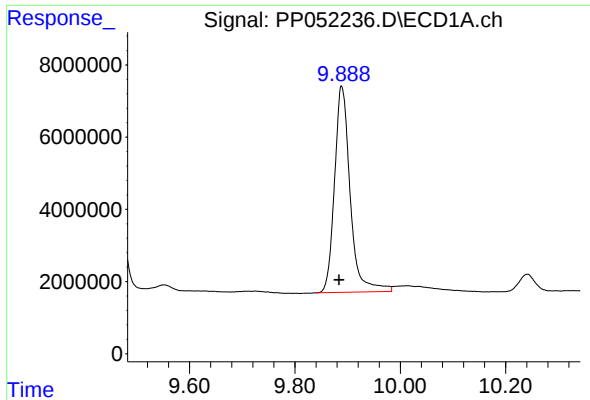

#45 AR-1268-5

R.T.: 9.888 min
Delta R.T.: 0.005 min
Response: 118098972
Conc: 226.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-3DL

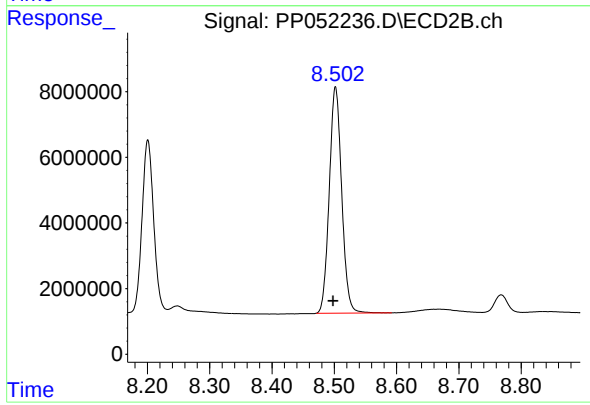

#45 AR-1268-5

R.T.: 8.502 min
Delta R.T.: 0.004 min
Response: 95588195
Conc: 227.23 ng/ml