

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 19:02
 Operator : YP\AJ
 Sample : N5098-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 07:13:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 31 18:43:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.423	3.673	20293743	14800070	12.911	12.919
2)	SA Decachlor...	10.238	8.766	455.6E6	376.9E6	328.300	337.283
Target Compounds							
3)	L1 AR-1016-1	5.596	4.776	2827216	4865844	62.172	109.404 #
4)	L1 AR-1016-2	5.620	4.795	7792895	4378150	118.375	68.804 #
5)	L1 AR-1016-3	5.682	4.975	4315638	3500454	103.703	105.308
6)	L1 AR-1016-4	5.781	5.017	4401809	6466695	121.146	237.264 #
7)	L1 AR-1016-5	6.077	5.235	8242464	6034914	193.114	170.578
8)	L2 AR-1221-1	4.630	3.895	1641305	2723900	79.427	174.212 #
9)	L2 AR-1221-2	4.716	3.963f	1468257	2933973	95.944	244.644 #
10)	L2 AR-1221-3	4.795	4.055	2500748	2387526	53.409	63.170
11)	L3 AR-1232-1	4.795	4.055	2500748	2387526	69.414	82.380
12)	L3 AR-1232-2	5.327	4.795	5158950	4378150	254.264	146.158 #
13)	L3 AR-1232-3	5.620	4.975	7792895	3500454	258.763	229.126
14)	L3 AR-1232-4	5.781	5.060	4401809	5749727	263.934	406.039 #
15)	L3 AR-1232-5	5.872	5.235	7103576	6034914	473.644	381.227
16)	L4 AR-1242-1	5.596	4.776	2827216	4865844	81.276	139.750 #
17)	L4 AR-1242-2	5.620	4.795	7792895	4378150	157.412	88.749 #
18)	L4 AR-1242-3	5.682	4.975	4315638	3500454	136.108	134.097
19)	L4 AR-1242-4	5.781	5.060	4401809	5749727	161.147	211.387 #
20)	L4 AR-1242-5	6.523	5.593	11548748	20658860	310.637	613.021 #
21)	L5 AR-1248-1	5.596	4.776	2827216	4865844	105.169	179.476 #
22)	L5 AR-1248-2	5.872	5.017	7103576	6466695	152.823	173.815
23)	L5 AR-1248-3	6.077	5.060	8242464	5749727	148.856	150.926
24)	L5 AR-1248-4	6.482	5.235	7996328	6034914	125.940	130.245
25)	L5 AR-1248-5	6.523	5.633	11548748	4215274	186.466	100.236 #
26)	L6 AR-1254-1	6.456	5.593	27839415	20658860	391.060	295.284
27)	L6 AR-1254-2	6.675	5.741	43497371	25170278	407.845	401.730
28)	L6 AR-1254-3	7.045	6.166f	23070306	186.9E6	219.508	1888.916 #
29)	L6 AR-1254-4	7.329	6.380	23580160	10943694	322.714	183.075 #
30)	L6 AR-1254-5	7.740	6.804	355.5E6	140.1E6	4284.372	1579.826 #
31)	L7 AR-1260-1	7.209	6.283	255.1E6	192.7E6	3077.363	2797.020
32)	L7 AR-1260-2	7.466	6.472	544.8E6	438.6E6	5771.870	5299.465
33)	L7 AR-1260-3	7.828	6.633	2549.1E6	474.7E6	42442.862	6148.518 #
34)	L7 AR-1260-4	8.055	7.103	860.0E6	1508.3E6	11212.968	26830.631 #
35)	L7 AR-1260-5	8.377	7.347	3357.6E6	2857.9E6	24494.357	21670.657
36)	L8 AR-1262-1	7.828	6.896	2549.1E6	657.7E6	26288.851	18283.007 #
37)	L8 AR-1262-2	8.377	7.103	3357.6E6	1508.3E6	20853.687	19047.718
38)	L8 AR-1262-3	8.694	7.634	5025.9E6	4057.4E6	45731.815	65705.341 #
39)	L8 AR-1262-4	8.790	7.699	5818.8E6	4648.2E6	113828.319	40715.010 #
40)	L8 AR-1262-5	9.460	8.200	3677.9E6	2869.9E6	58426.356	56462.644
41)	L9 AR-1268-1	8.694	7.634	5025.9E6	4057.4E6	25386.125	22366.125

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 19:02
Operator : YP\AJ
Sample : N5098-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 07:13:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 31 18:43:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.790	7.699	5818.8E6	4648.2E6	31688.725	28448.768
43)	L9 AR-1268-3	9.024	7.908	1336.4E6	1089.7E6	8198.339	7749.089
44)	L9 AR-1268-4	9.460	8.200	3677.9E6	2869.9E6	50408.241	50784.816
45)	L9 AR-1268-5	9.887	8.501	6081.0E6	4643.7E6	11661.937	11039.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 19:02
Operator : YP\AJ
Sample : N5098-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 07:13:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 31 18:43:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

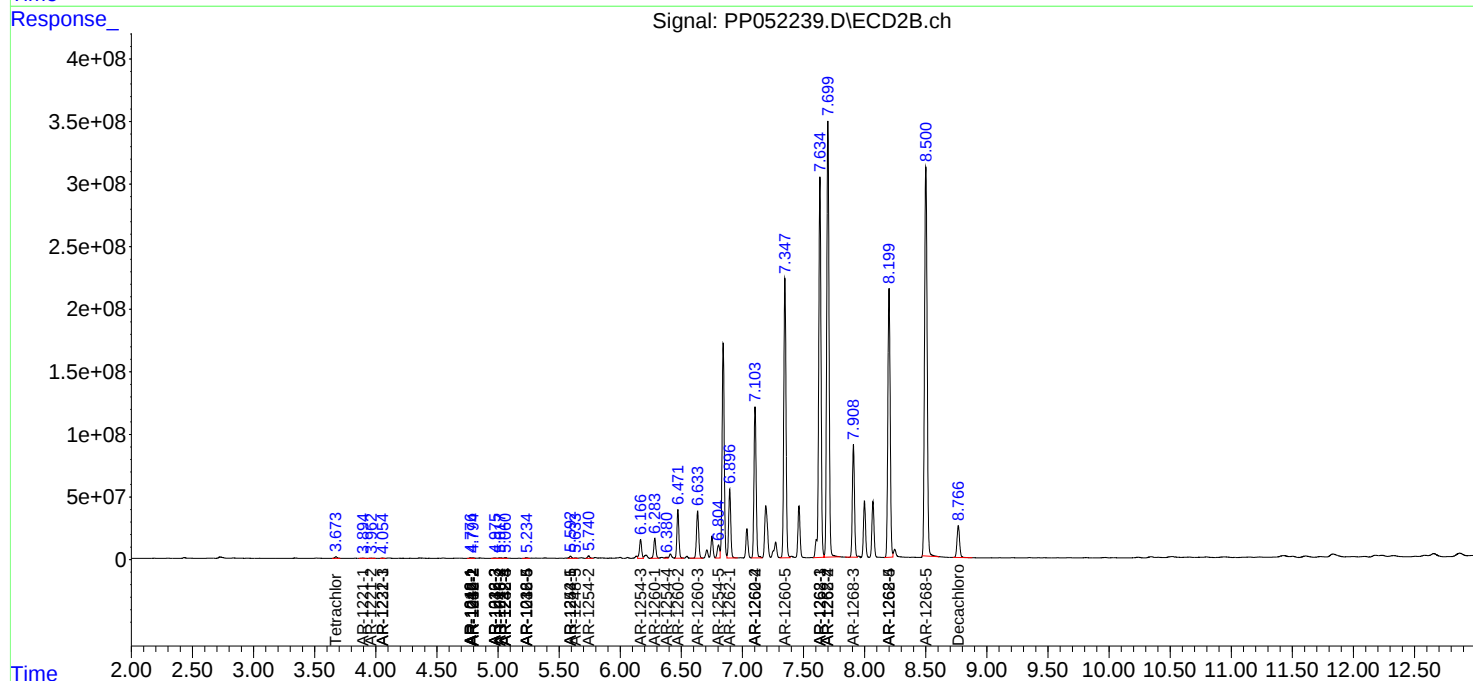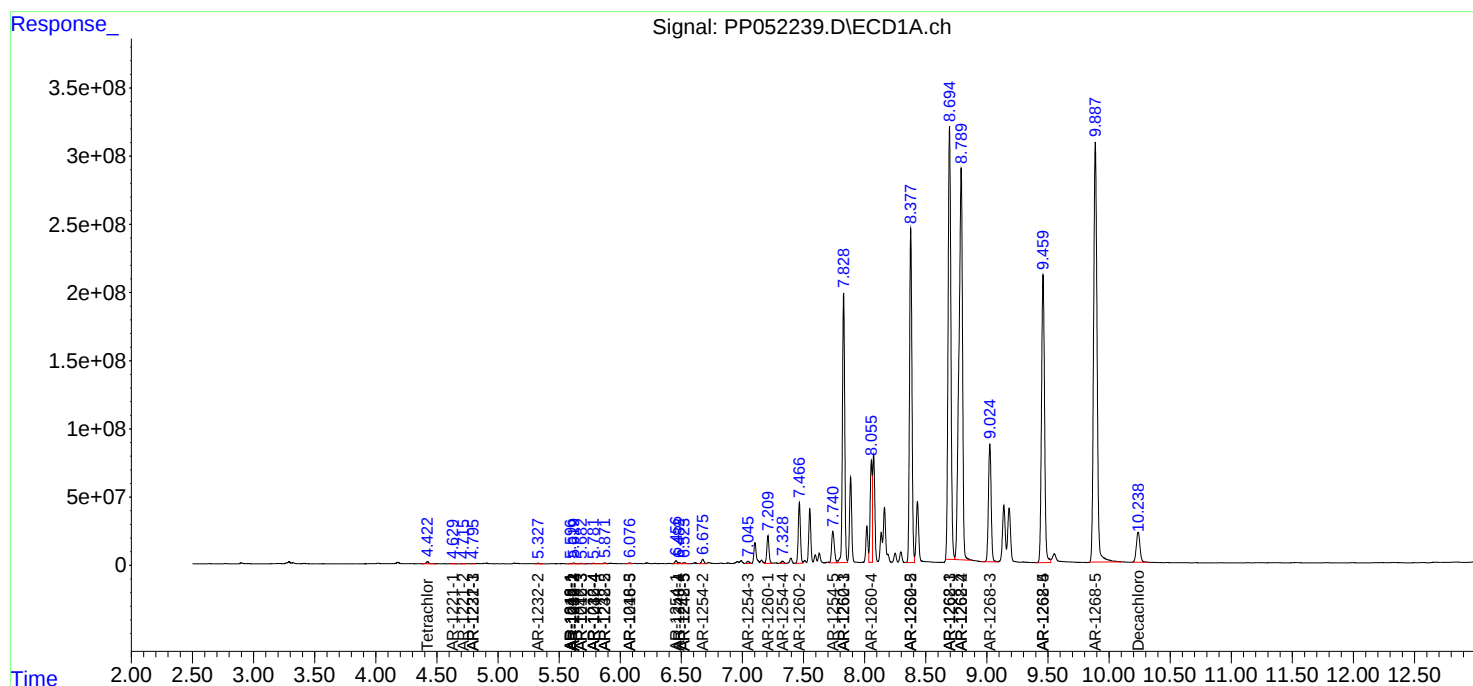


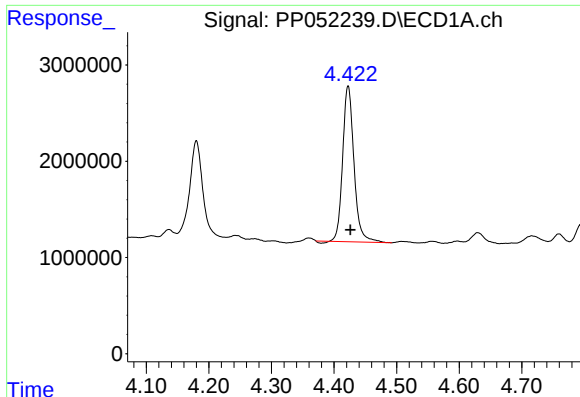

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 20293743
Conc: 12.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

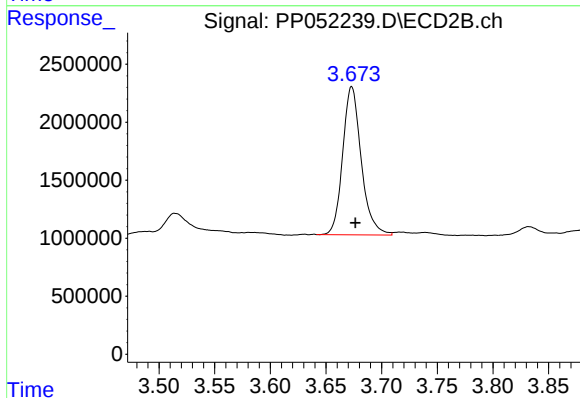


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.003 min
Response: 14800070
Conc: 12.92 ng/ml

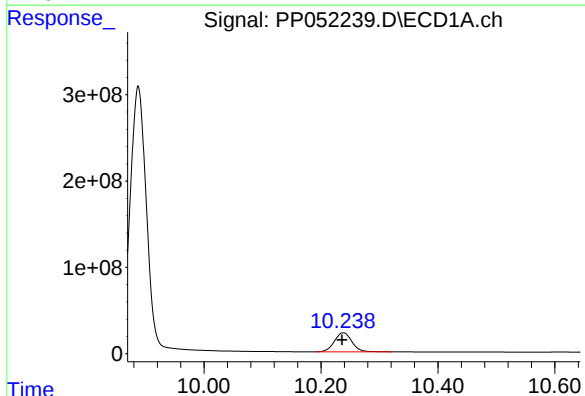


#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: 0.002 min
Response: 455629040
Conc: 328.30 ng/ml

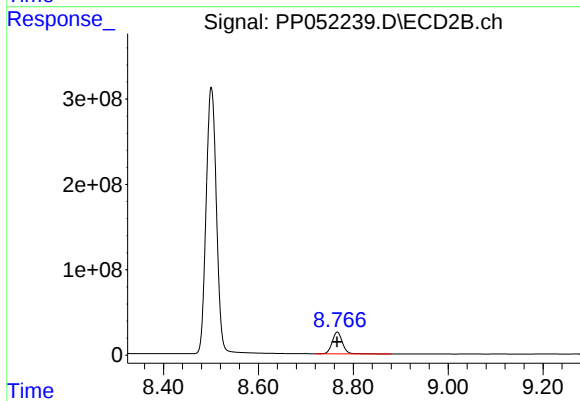

#2 Decachlorobiphenyl


R.T.: 8.766 min
Delta R.T.: 0.000 min
Response: 376866474
Conc: 337.28 ng/ml

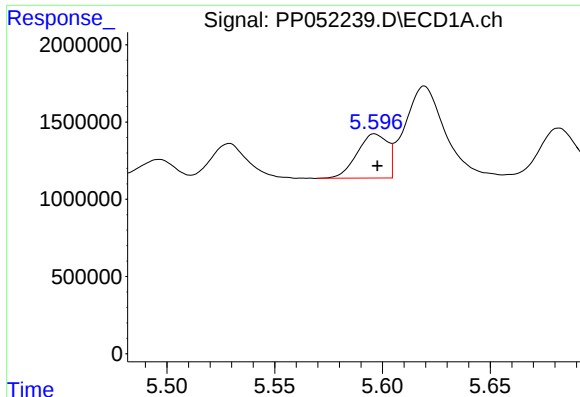

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: -0.001 min
Response: 2827216
Conc: 62.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

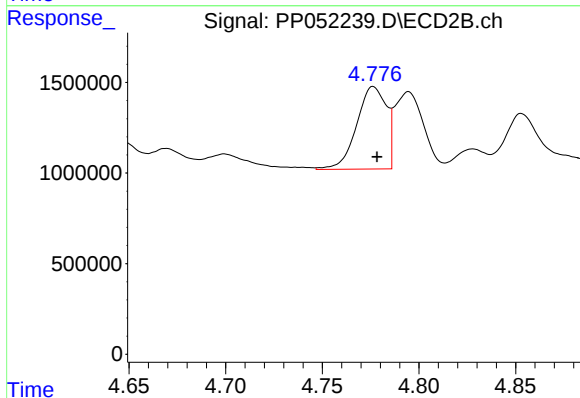


#3 AR-1016-1

R.T.: 4.776 min
Delta R.T.: -0.002 min
Response: 4865844
Conc: 109.40 ng/ml

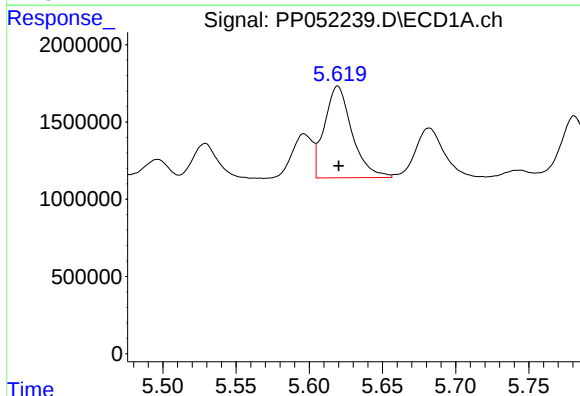


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 7792895
Conc: 118.38 ng/ml

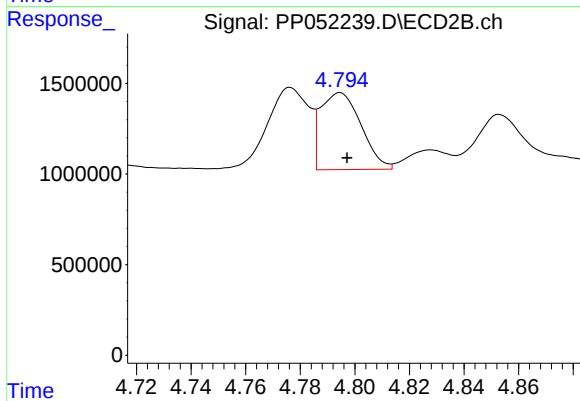

#4 AR-1016-2


R.T.: 4.795 min
Delta R.T.: -0.003 min
Response: 4378150
Conc: 68.80 ng/ml

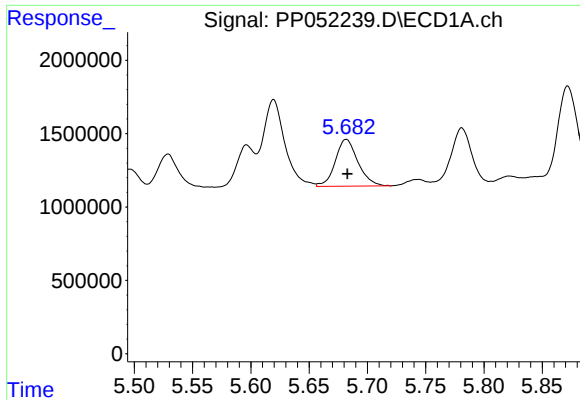

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 4315638
Conc: 103.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

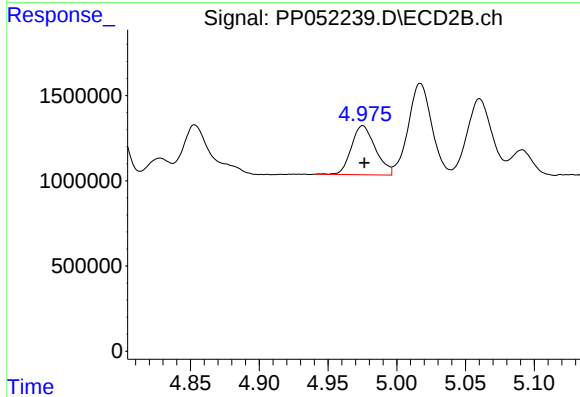


#5 AR-1016-3

R.T.: 4.975 min
Delta R.T.: -0.001 min
Response: 3500454
Conc: 105.31 ng/ml

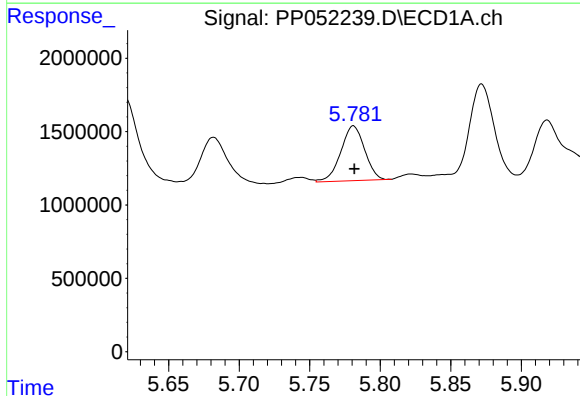


#6 AR-1016-4

R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 4401809
Conc: 121.15 ng/ml

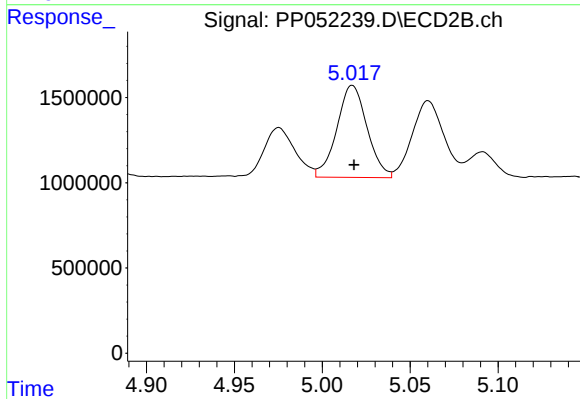

#6 AR-1016-4


R.T.: 5.017 min
Delta R.T.: -0.001 min
Response: 6466695
Conc: 237.26 ng/ml

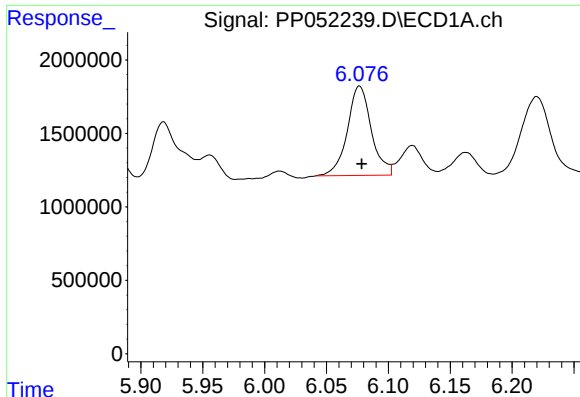

#7 AR-1016-5


R.T.: 6.077 min
Delta R.T.: -0.002 min
Response: 8242464
Conc: 193.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

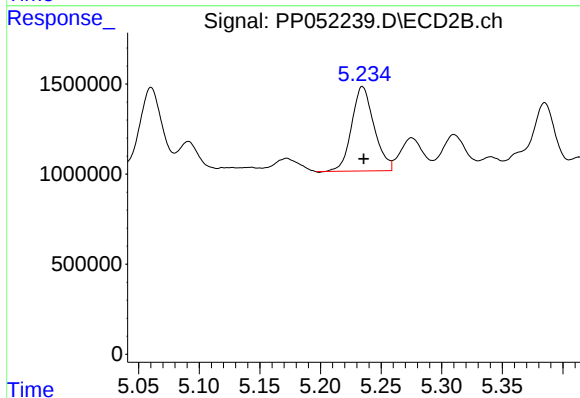


#7 AR-1016-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 6034914
Conc: 170.58 ng/ml

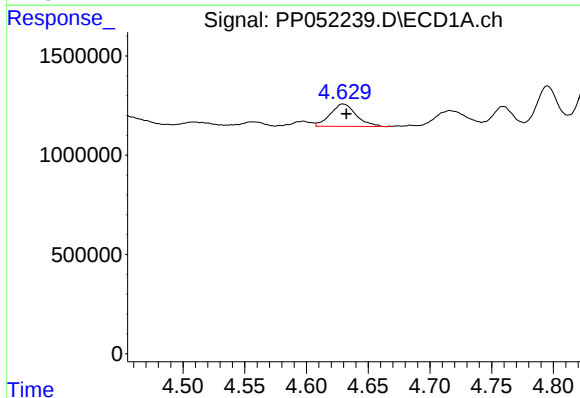


#8 AR-1221-1

R.T.: 4.630 min
Delta R.T.: -0.003 min
Response: 1641305
Conc: 79.43 ng/ml

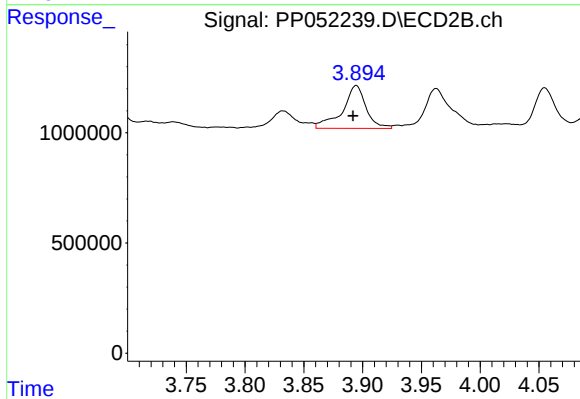

#8 AR-1221-1


R.T.: 3.895 min
Delta R.T.: 0.002 min
Response: 2723900
Conc: 174.21 ng/ml

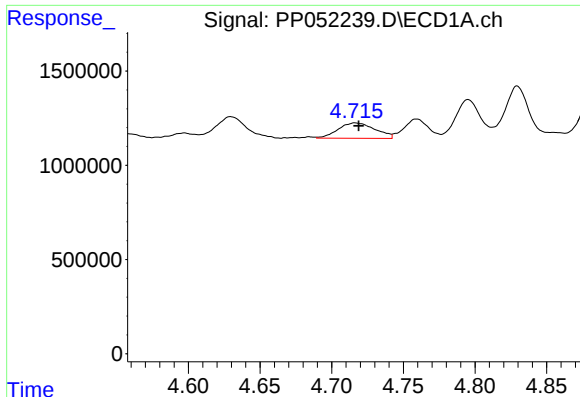

#9 AR-1221-2


R.T.: 4.716 min
Delta R.T.: -0.003 min
Response: 1468257
Conc: 95.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

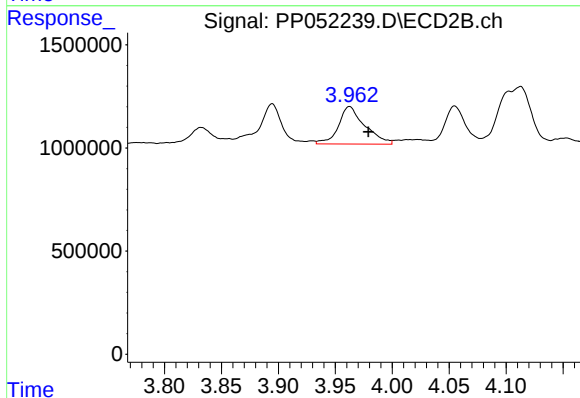


#9 AR-1221-2

R.T.: 3.963 min
Delta R.T.: -0.017 min
Response: 2933973
Conc: 244.64 ng/ml

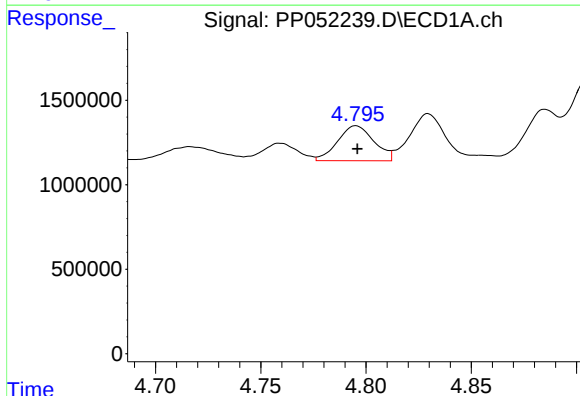


#10 AR-1221-3

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 2500748
Conc: 53.41 ng/ml

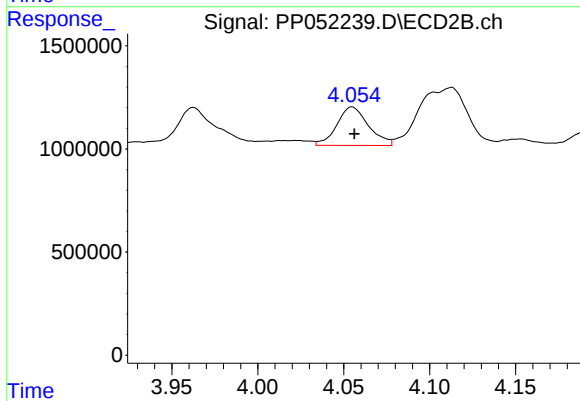

#10 AR-1221-3


R.T.: 4.055 min
Delta R.T.: -0.001 min
Response: 2387526
Conc: 63.17 ng/ml

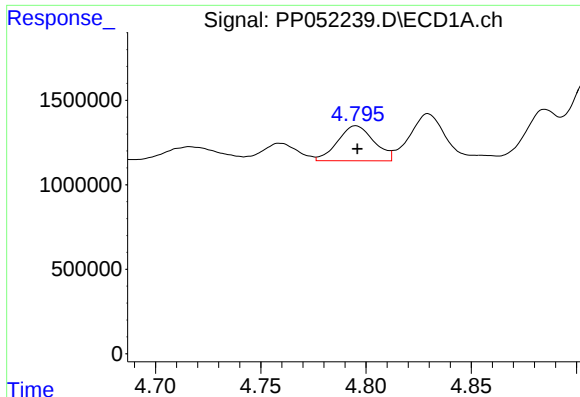

#11 AR-1232-1


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 2500748
Conc: 69.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

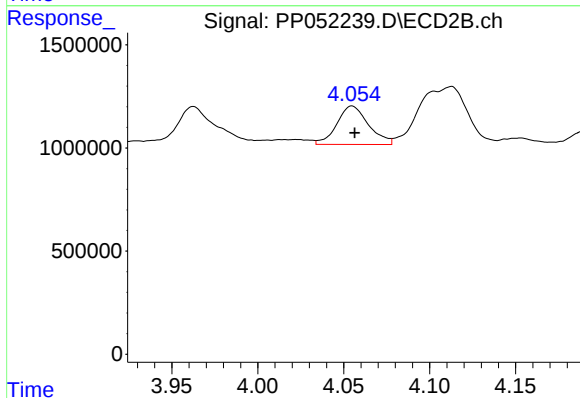


#11 AR-1232-1

R.T.: 4.055 min
Delta R.T.: -0.002 min
Response: 2387526
Conc: 82.38 ng/ml

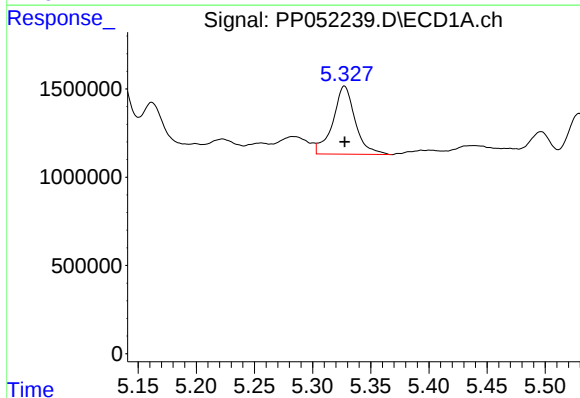


#12 AR-1232-2

R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 5158950
Conc: 254.26 ng/ml

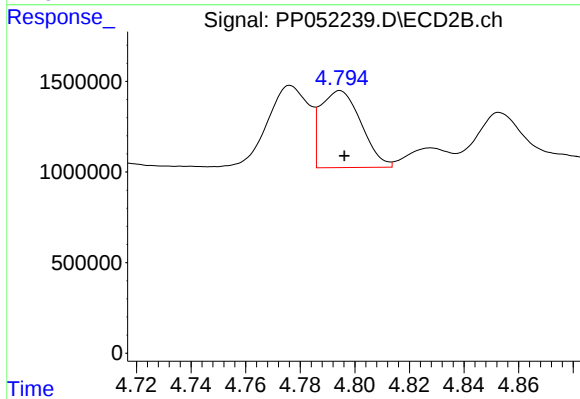

#12 AR-1232-2


R.T.: 4.795 min
Delta R.T.: -0.002 min
Response: 4378150
Conc: 146.16 ng/ml

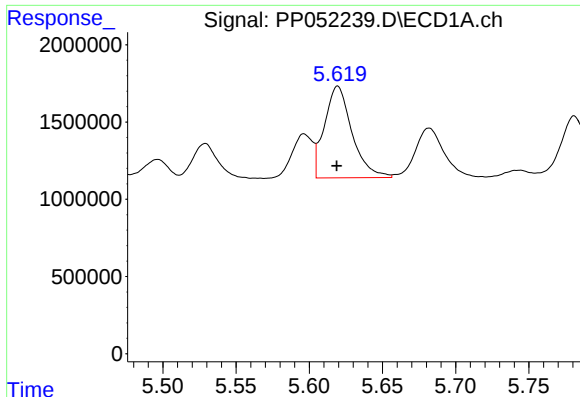

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 7792895
Conc: 258.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

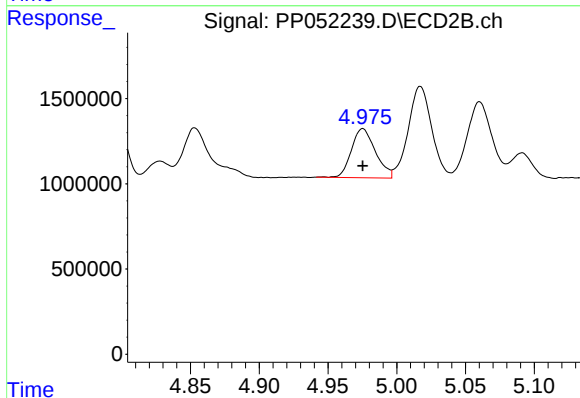


#13 AR-1232-3

R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 3500454
Conc: 229.13 ng/ml

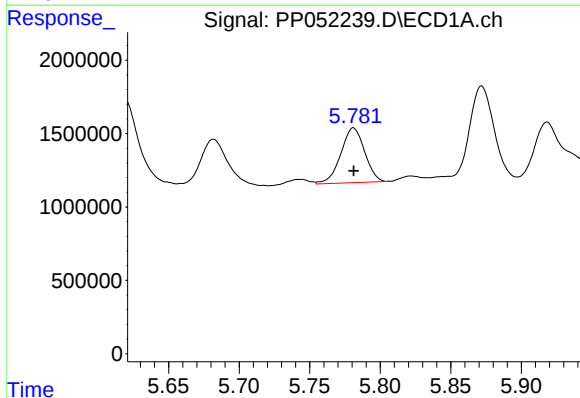


#14 AR-1232-4

R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 4401809
Conc: 263.93 ng/ml

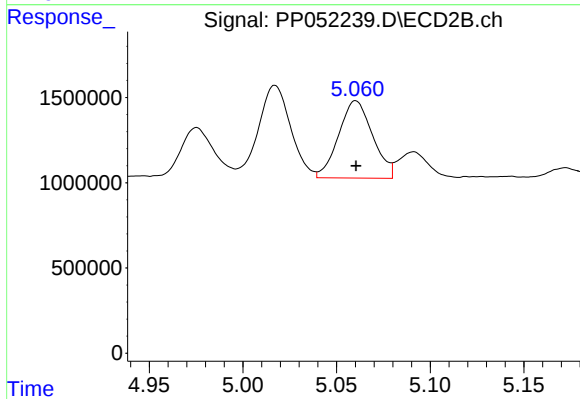

#14 AR-1232-4


R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 5749727
Conc: 406.04 ng/ml

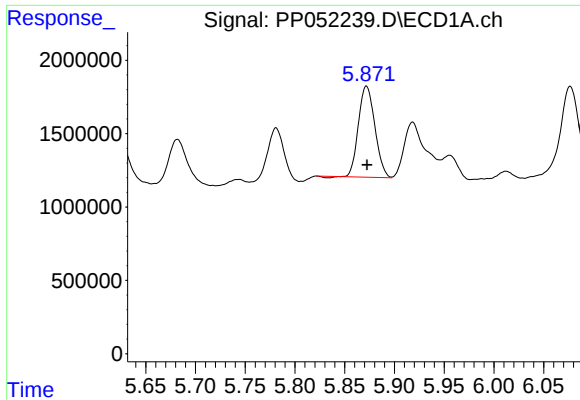

#15 AR-1232-5


R.T.: 5.872 min
Delta R.T.: 0.000 min
Response: 7103576
Conc: 473.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

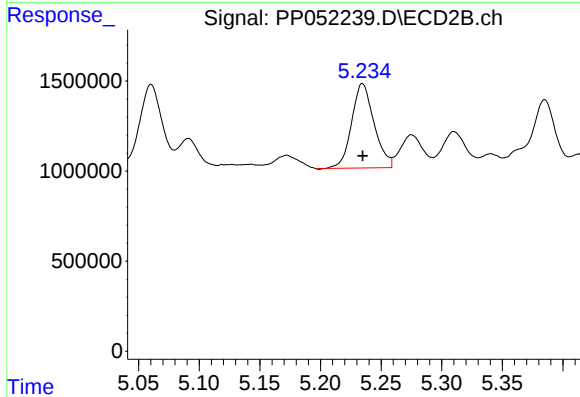


#15 AR-1232-5

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 6034914
Conc: 381.23 ng/ml

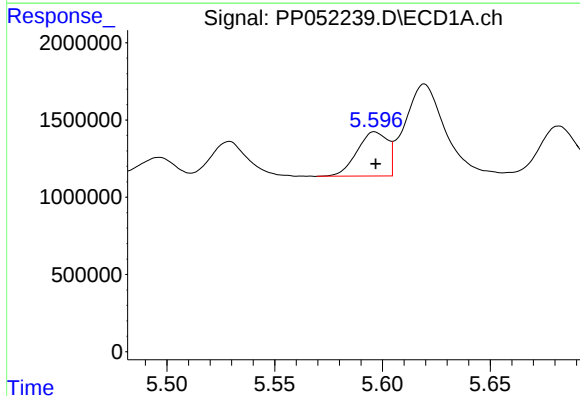


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 2827216
Conc: 81.28 ng/ml

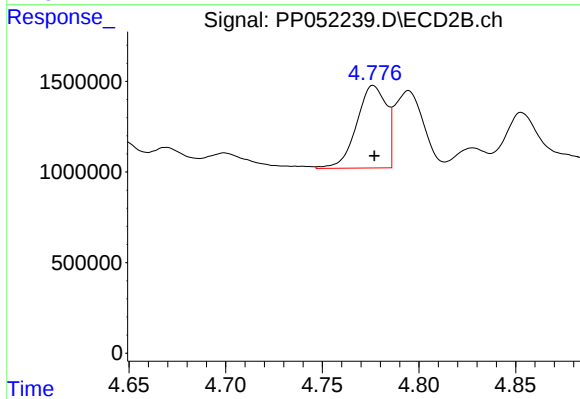

#16 AR-1242-1


R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 4865844
Conc: 139.75 ng/ml

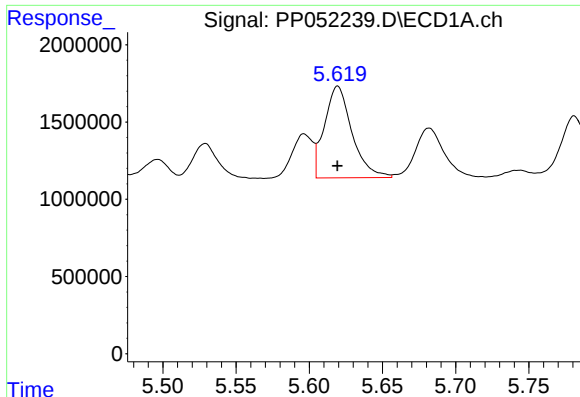

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 7792895
Conc: 157.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

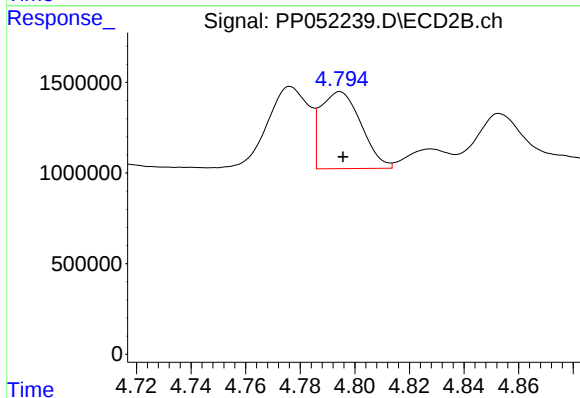


#17 AR-1242-2

R.T.: 4.795 min
Delta R.T.: -0.001 min
Response: 4378150
Conc: 88.75 ng/ml

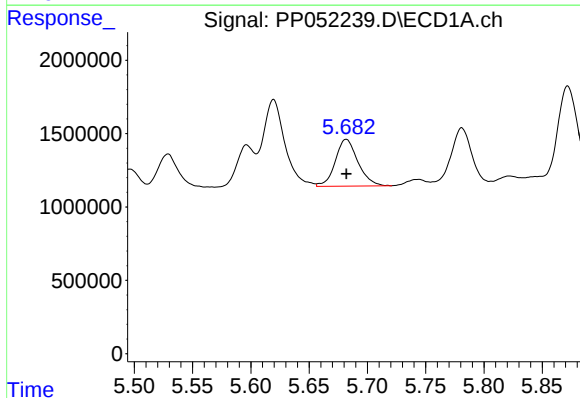


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 4315638
Conc: 136.11 ng/ml

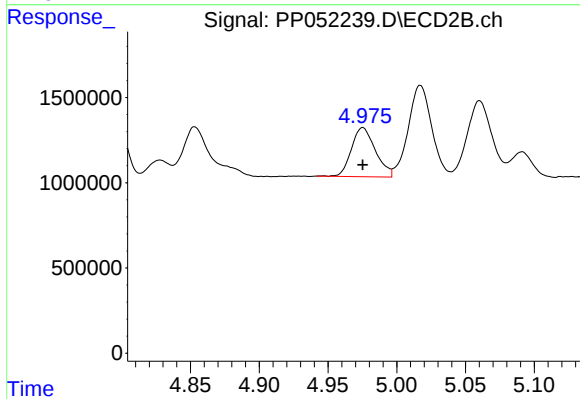

#18 AR-1242-3


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 3500454
Conc: 134.10 ng/ml

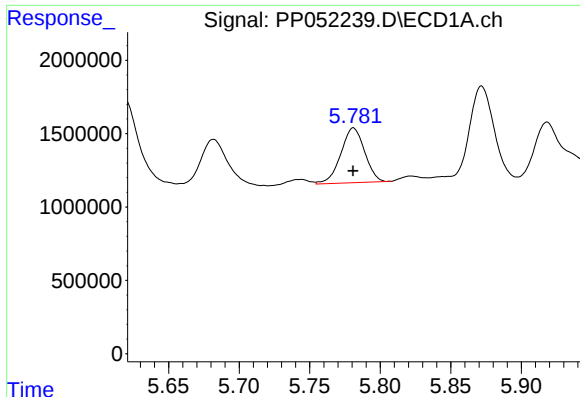

#19 AR-1242-4


R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 4401809
Conc: 161.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

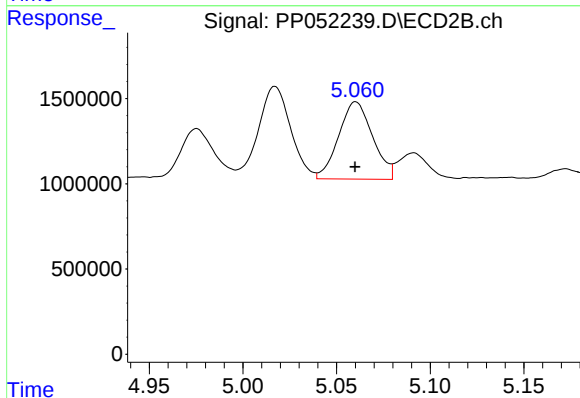


#19 AR-1242-4

R.T.: 5.060 min
Delta R.T.: 0.000 min
Response: 5749727
Conc: 211.39 ng/ml

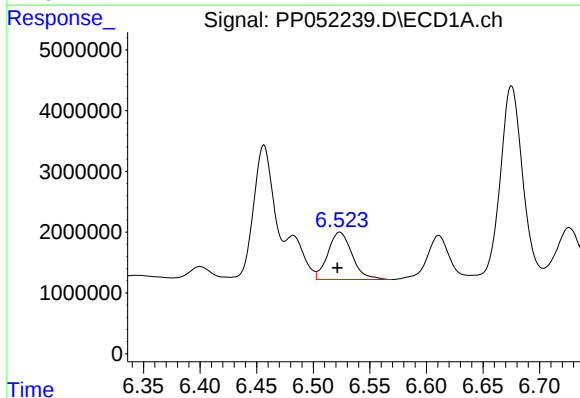


#20 AR-1242-5

R.T.: 6.523 min
Delta R.T.: 0.002 min
Response: 11548748
Conc: 310.64 ng/ml

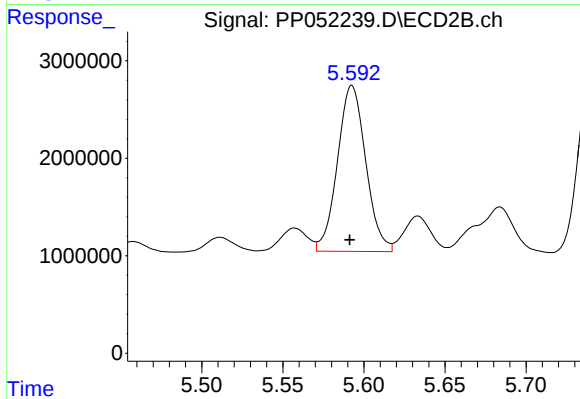

#20 AR-1242-5


R.T.: 5.593 min
Delta R.T.: 0.001 min
Response: 20658860
Conc: 613.02 ng/ml

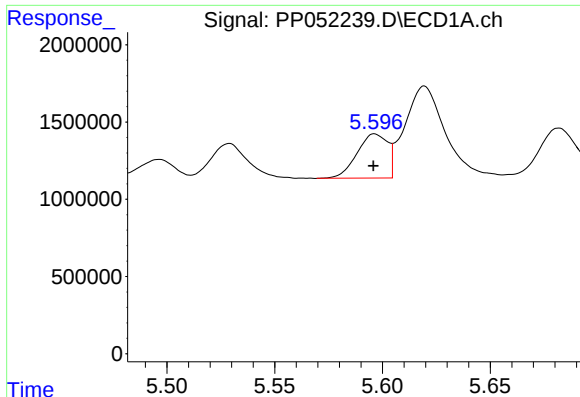

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 2827216
Conc: 105.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

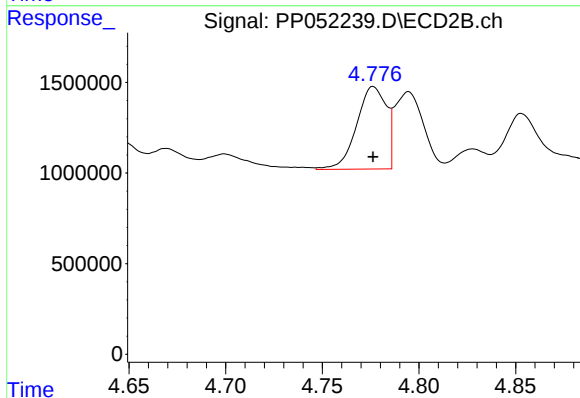


#21 AR-1248-1

R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 4865844
Conc: 179.48 ng/ml

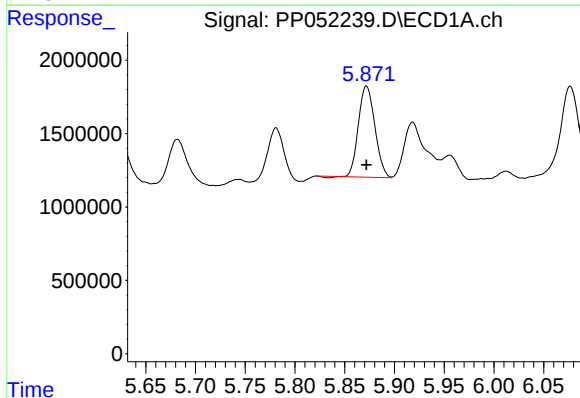


#22 AR-1248-2

R.T.: 5.872 min
Delta R.T.: 0.000 min
Response: 7103576
Conc: 152.82 ng/ml

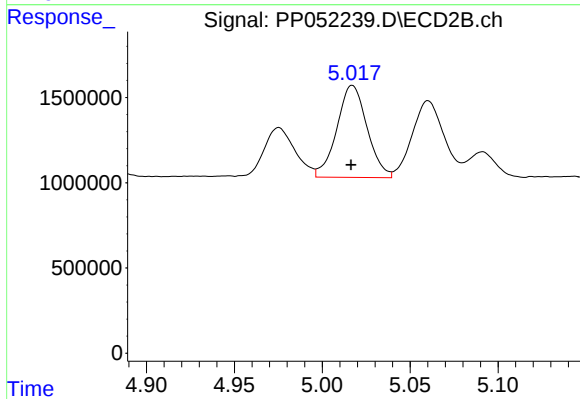

#22 AR-1248-2


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 6466695
Conc: 173.82 ng/ml

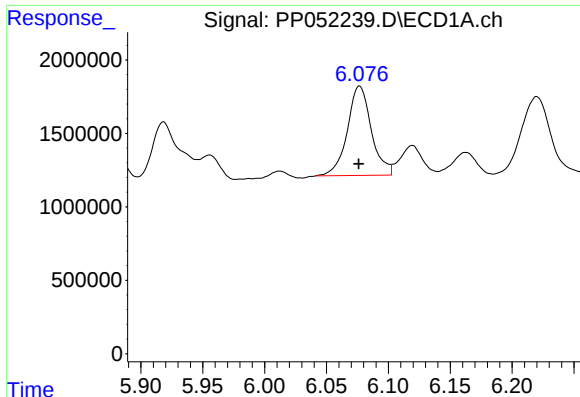

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 8242464
Conc: 148.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

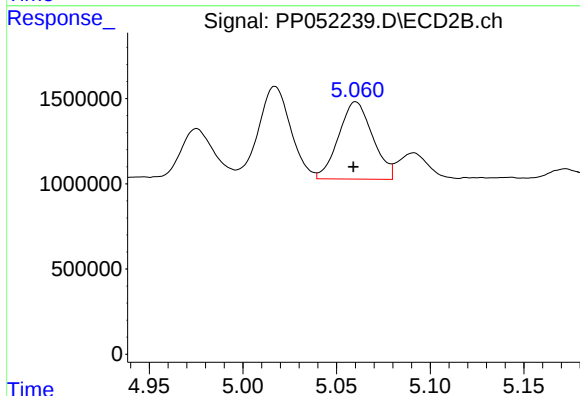


#23 AR-1248-3

R.T.: 5.060 min
Delta R.T.: 0.001 min
Response: 5749727
Conc: 150.93 ng/ml

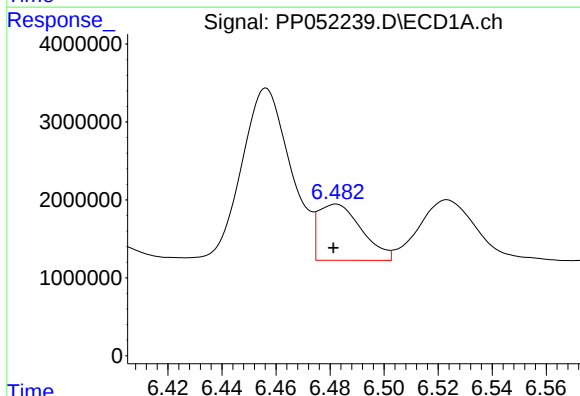


#24 AR-1248-4

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 7996328
Conc: 125.94 ng/ml

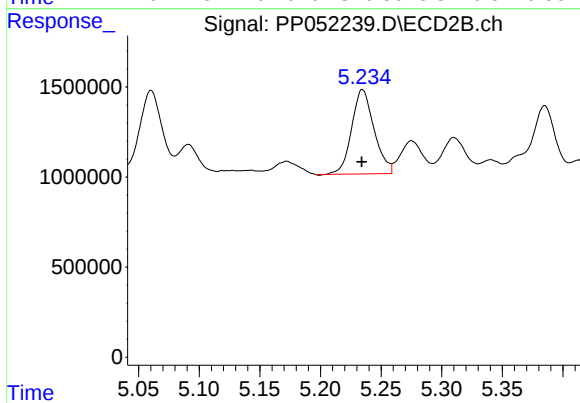

#24 AR-1248-4


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 6034914
Conc: 130.24 ng/ml

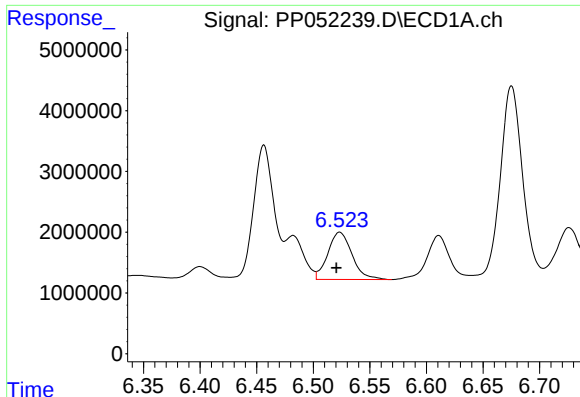

#25 AR-1248-5


R.T.: 6.523 min
Delta R.T.: 0.003 min
Response: 11548748
Conc: 186.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

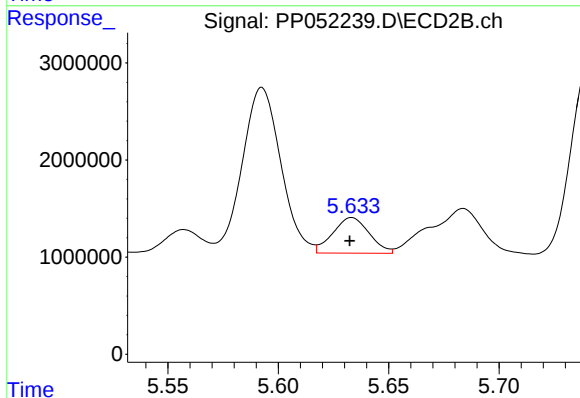


#25 AR-1248-5

R.T.: 5.633 min
Delta R.T.: 0.000 min
Response: 4215274
Conc: 100.24 ng/ml

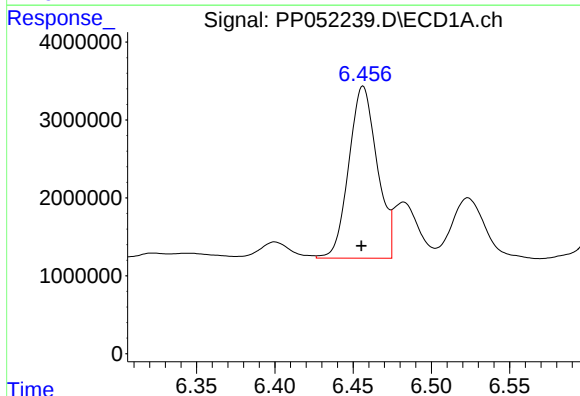


#26 AR-1254-1

R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 27839415
Conc: 391.06 ng/ml

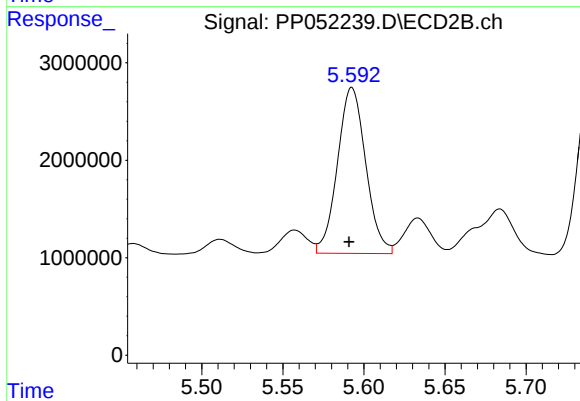

#26 AR-1254-1


R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 20658860
Conc: 295.28 ng/ml

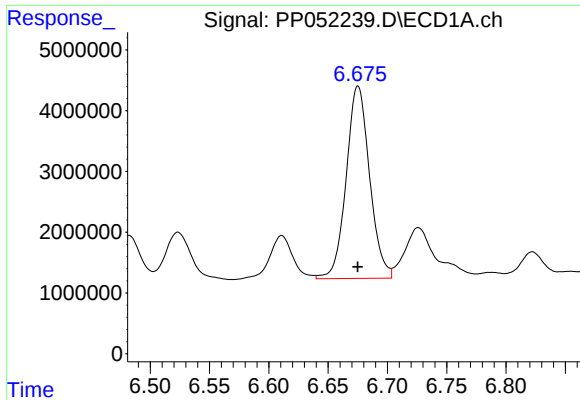

#27 AR-1254-2


R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 43497371
Conc: 407.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

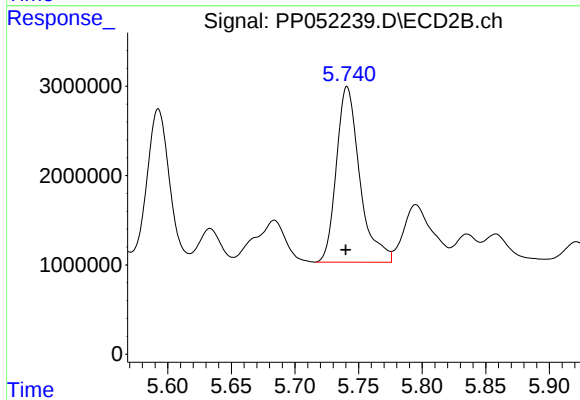


#27 AR-1254-2

R.T.: 5.741 min
Delta R.T.: 0.000 min
Response: 25170278
Conc: 401.73 ng/ml

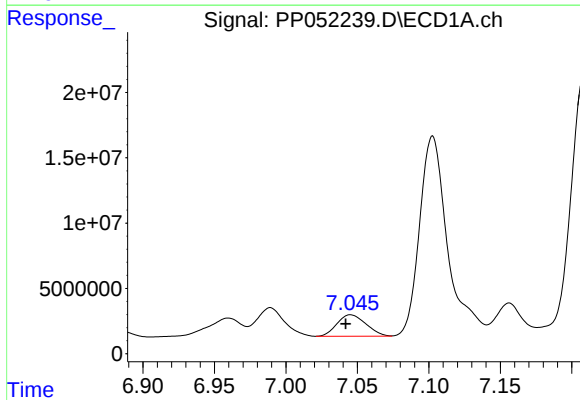


#28 AR-1254-3

R.T.: 7.045 min
Delta R.T.: 0.003 min
Response: 23070306
Conc: 219.51 ng/ml

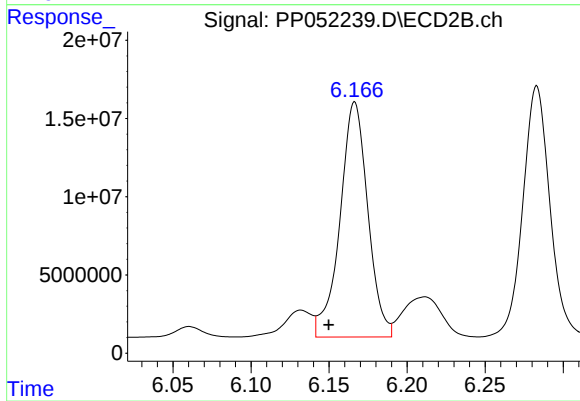

#28 AR-1254-3


R.T.: 6.166 min
Delta R.T.: 0.017 min
Response: 186851070
Conc: 1888.92 ng/ml

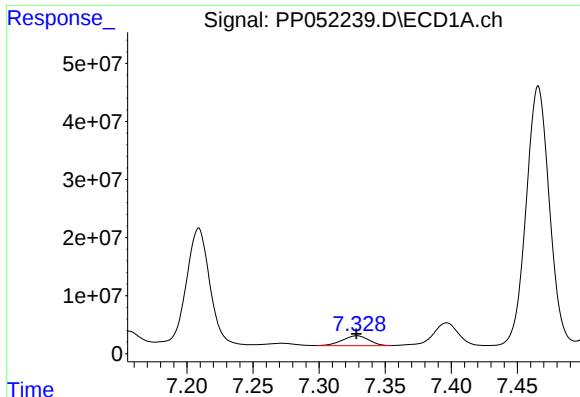

#29 AR-1254-4


R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 23580160
Conc: 322.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

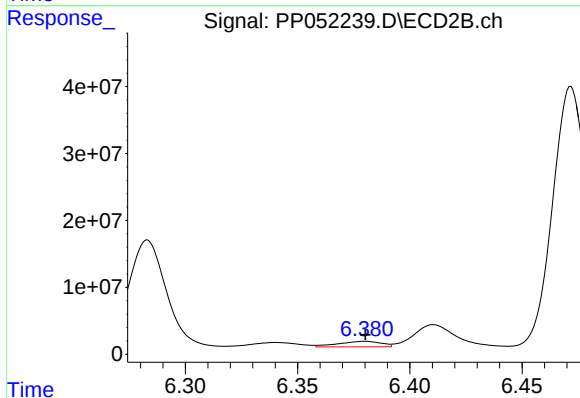


#29 AR-1254-4

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 10943694
Conc: 183.07 ng/ml

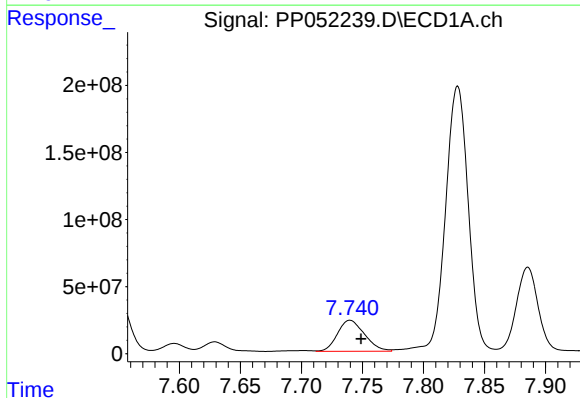


#30 AR-1254-5

R.T.: 7.740 min
Delta R.T.: -0.009 min
Response: 355489521
Conc: 4284.37 ng/ml

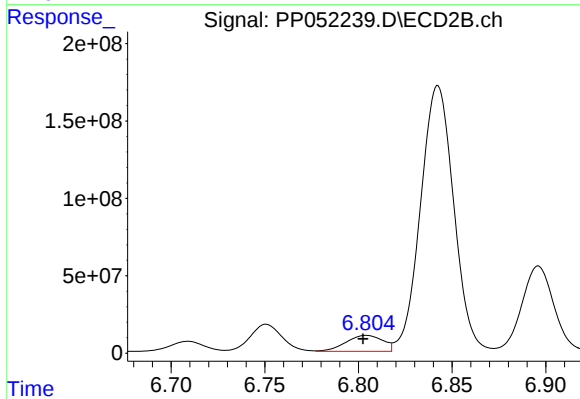

#30 AR-1254-5


R.T.: 6.804 min
Delta R.T.: 0.002 min
Response: 140058245
Conc: 1579.83 ng/ml

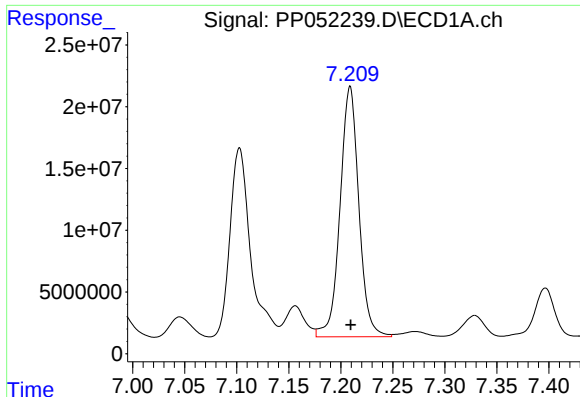

#31 AR-1260-1


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 255069588
Conc: 3077.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

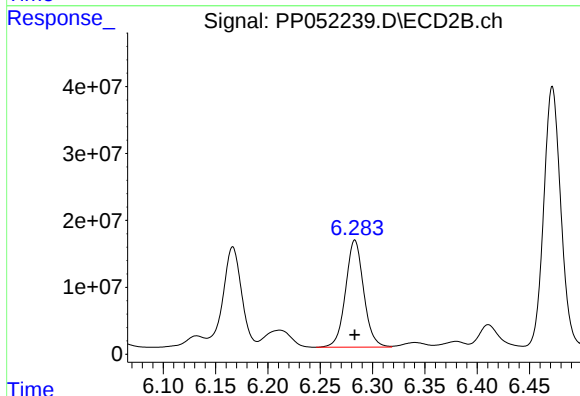


#31 AR-1260-1

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 192666092
Conc: 2797.02 ng/ml

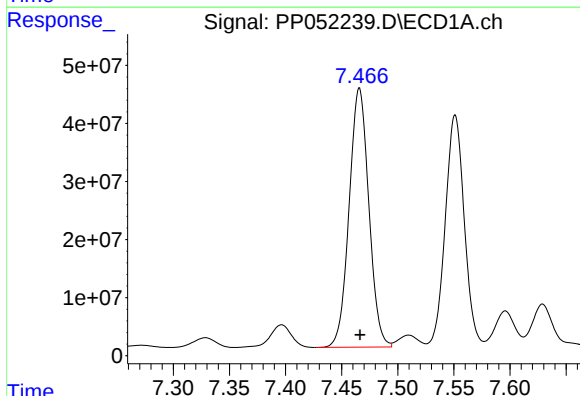


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 544777888
Conc: 5771.87 ng/ml

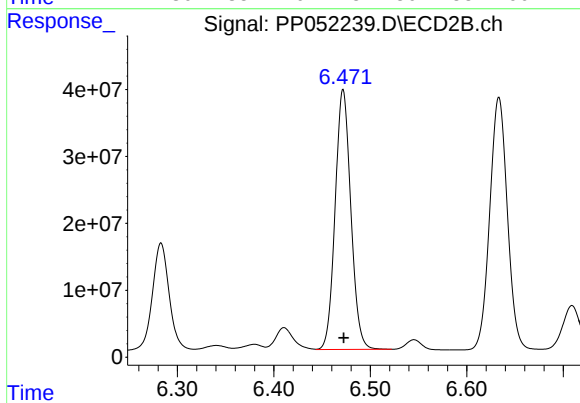

#32 AR-1260-2


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 438616599
Conc: 5299.47 ng/ml

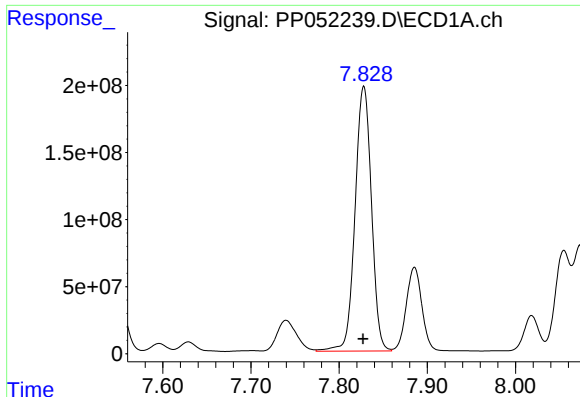

#33 AR-1260-3


R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 2549073769
Conc: 42442.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

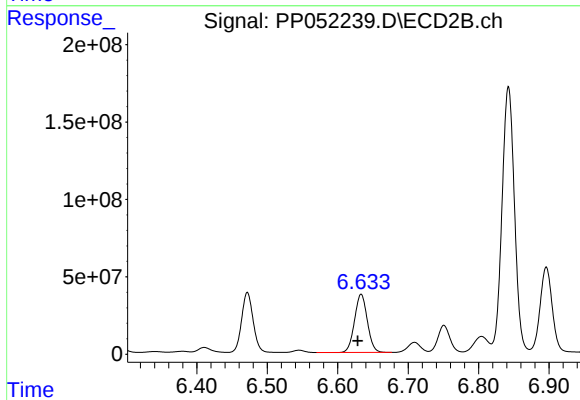


#33 AR-1260-3

R.T.: 6.633 min
Delta R.T.: 0.005 min
Response: 474712773
Conc: 6148.52 ng/ml

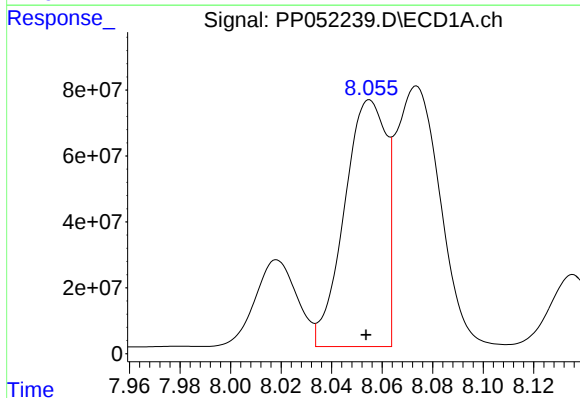


#34 AR-1260-4

R.T.: 8.055 min
Delta R.T.: 0.001 min
Response: 859965895
Conc: 11212.97 ng/ml

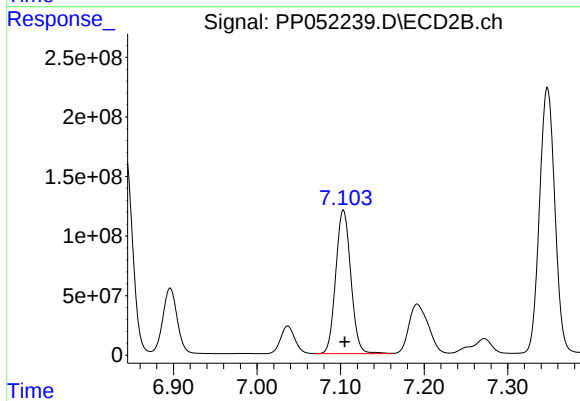

#34 AR-1260-4


R.T.: 7.103 min
Delta R.T.: -0.002 min
Response: 1508272015
Conc: 26830.63 ng/ml

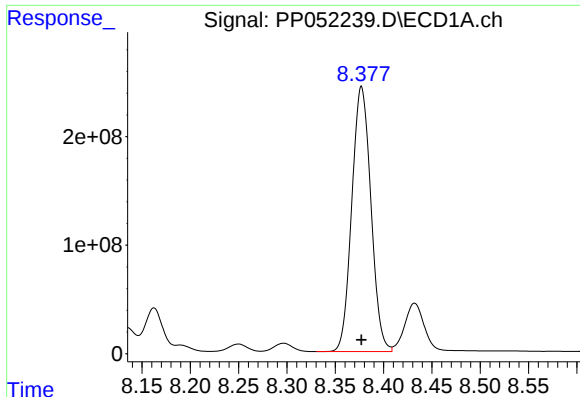

#35 AR-1260-5


R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 3357639006
Conc: 24494.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

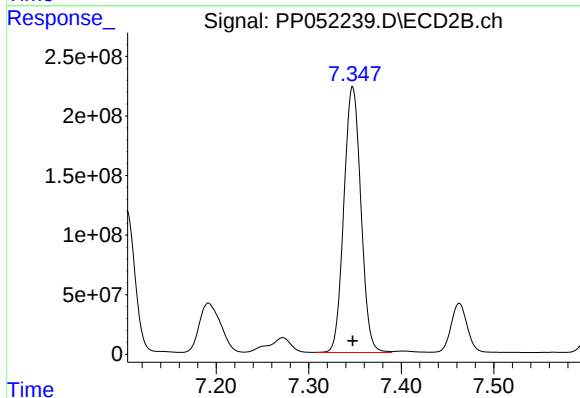


#35 AR-1260-5

R.T.: 7.347 min
Delta R.T.: 0.000 min
Response: 2857863588
Conc: 21670.66 ng/ml

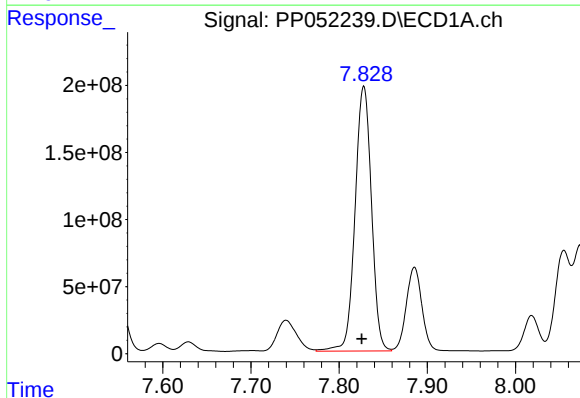


#36 AR-1262-1

R.T.: 7.828 min
Delta R.T.: 0.002 min
Response: 2549073769
Conc: 26288.85 ng/ml

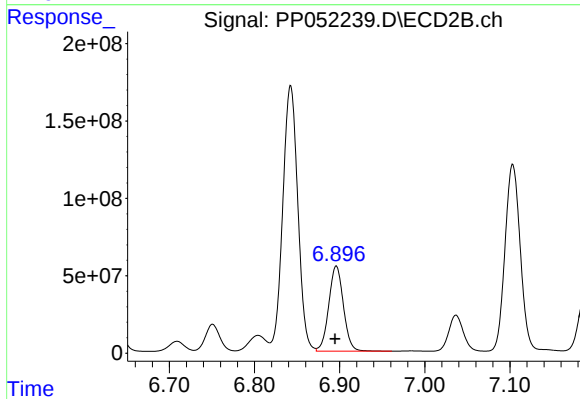

#36 AR-1262-1


R.T.: 6.896 min
Delta R.T.: 0.001 min
Response: 657668439
Conc: 18283.01 ng/ml

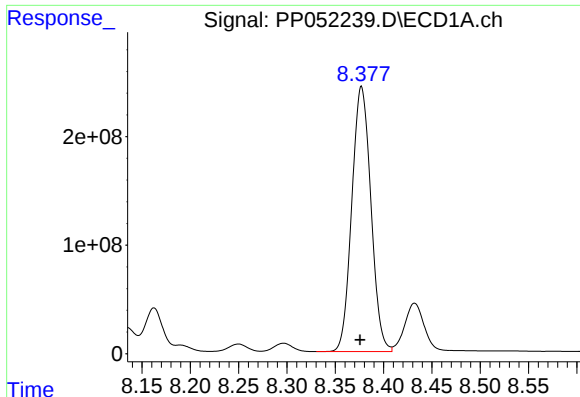

#37 AR-1262-2


R.T.: 8.377 min
Delta R.T.: 0.001 min
Response: 3357639006
Conc: 20853.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

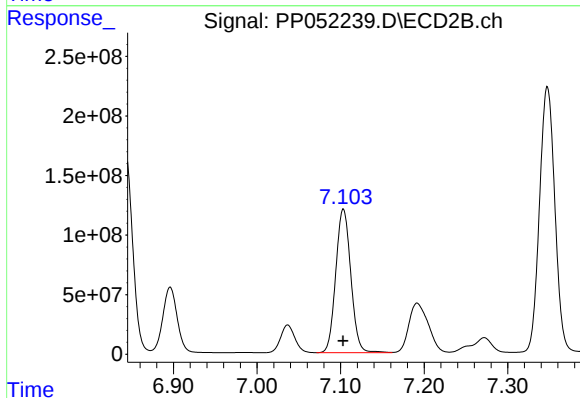


#37 AR-1262-2

R.T.: 7.103 min
Delta R.T.: 0.000 min
Response: 1508272015
Conc: 19047.72 ng/ml

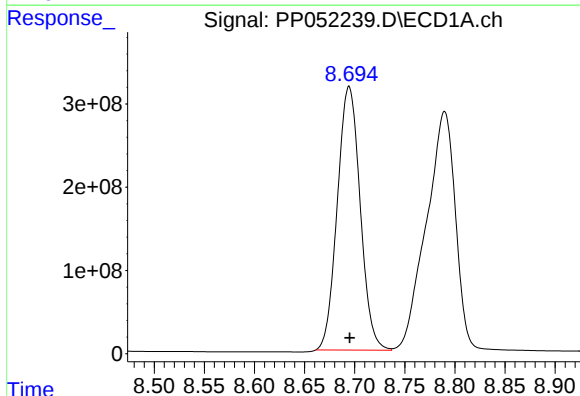


#38 AR-1262-3

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 5025917798
Conc: 45731.81 ng/ml

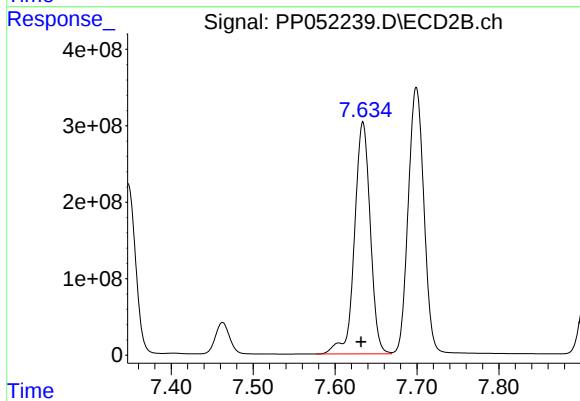

#38 AR-1262-3


R.T.: 7.634 min
Delta R.T.: 0.002 min
Response: 4057441679
Conc: 65705.34 ng/ml

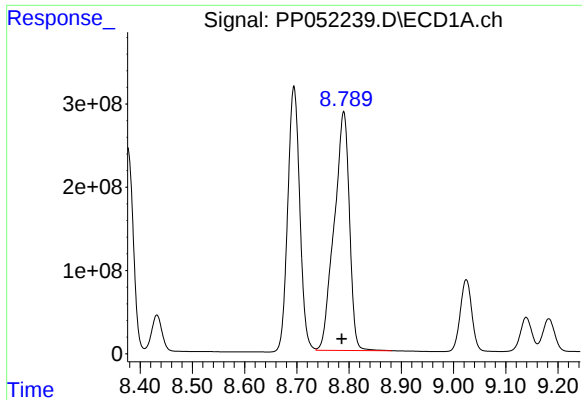

#39 AR-1262-4


R.T.: 8.790 min
Delta R.T.: 0.004 min
Response: 5818752642
Conc: 113828.32 ng

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

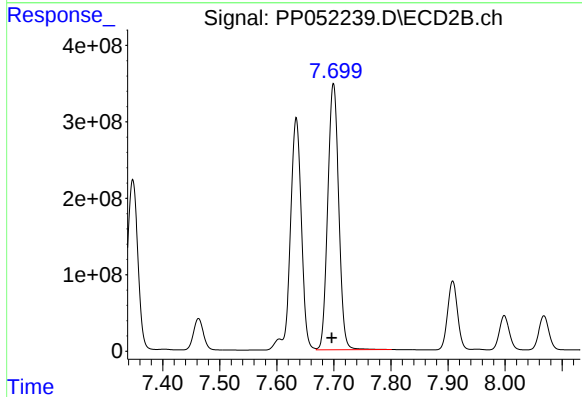


#39 AR-1262-4

R.T.: 7.699 min
Delta R.T.: 0.003 min
Response: 4648160602
Conc: 40715.01 ng/ml

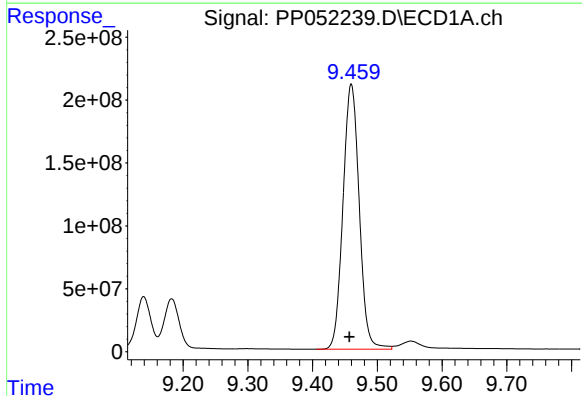


#40 AR-1262-5

R.T.: 9.460 min
Delta R.T.: 0.003 min
Response: 3677881559
Conc: 58426.36 ng/ml

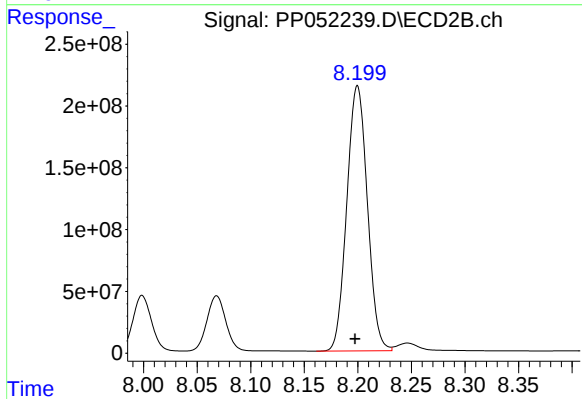

#40 AR-1262-5


R.T.: 8.200 min
Delta R.T.: 0.002 min
Response: 2869916808
Conc: 56462.64 ng/ml

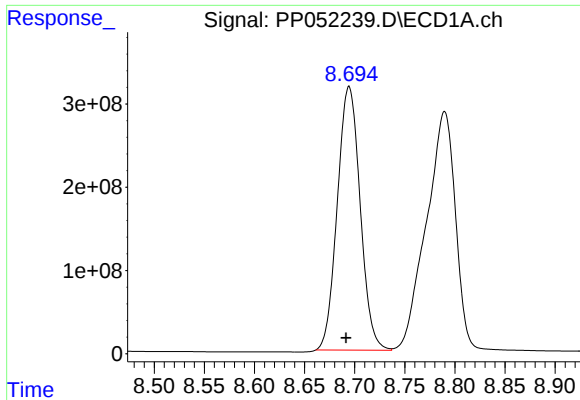

#41 AR-1268-1


R.T.: 8.694 min
Delta R.T.: 0.003 min
Response: 5025917798
Conc: 25386.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

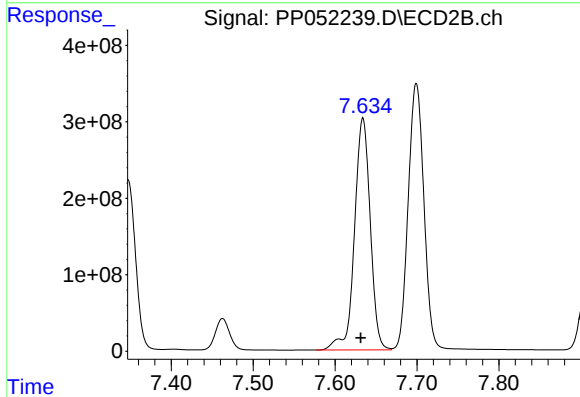


#41 AR-1268-1

R.T.: 7.634 min
Delta R.T.: 0.003 min
Response: 4057441679
Conc: 22366.12 ng/ml

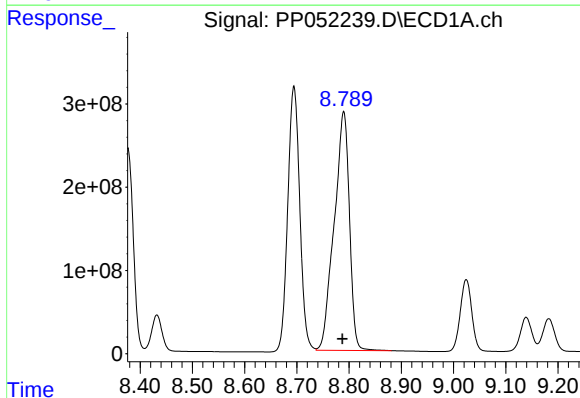


#42 AR-1268-2

R.T.: 8.790 min
Delta R.T.: 0.002 min
Response: 5818752642
Conc: 31688.72 ng/ml

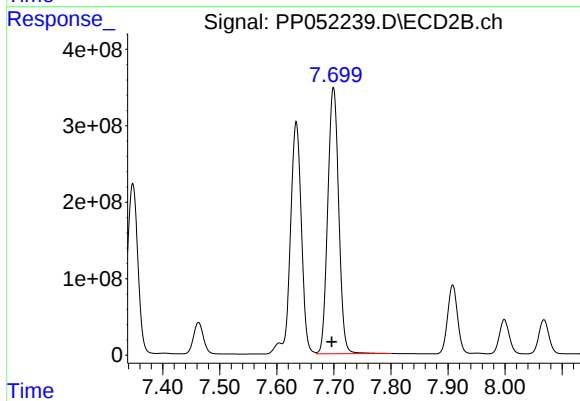

#42 AR-1268-2


R.T.: 7.699 min
Delta R.T.: 0.003 min
Response: 4648160602
Conc: 28448.77 ng/ml

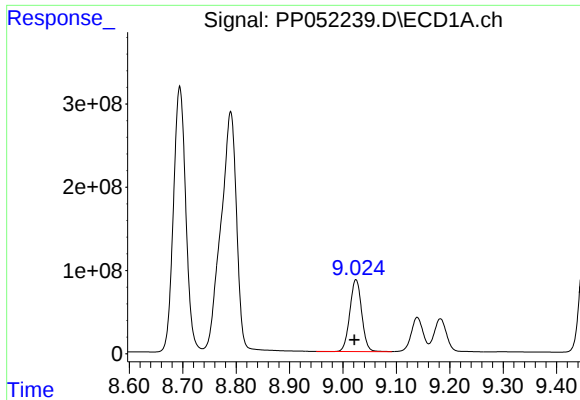

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.003 min
Response: 1336440579
Conc: 8198.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

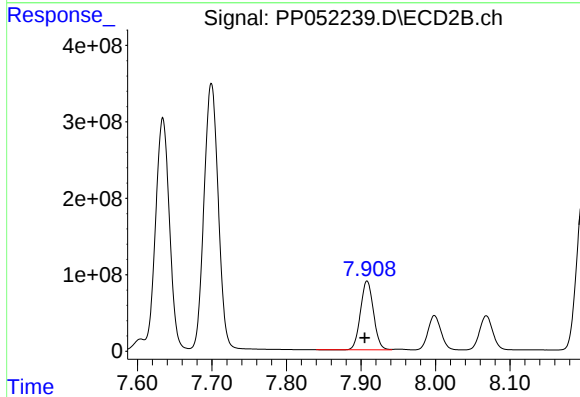


#43 AR-1268-3

R.T.: 7.908 min
Delta R.T.: 0.003 min
Response: 1089695929
Conc: 7749.09 ng/ml

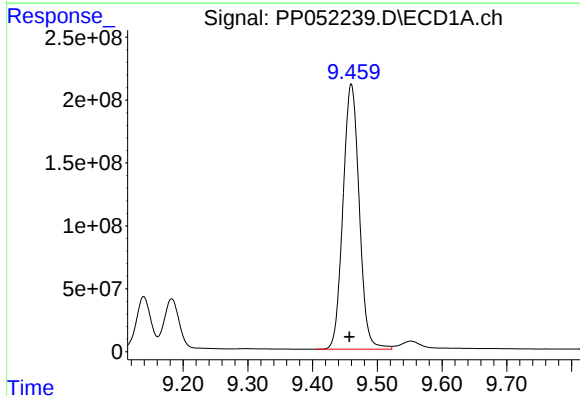


#44 AR-1268-4

R.T.: 9.460 min
Delta R.T.: 0.003 min
Response: 3677881559
Conc: 50408.24 ng/ml

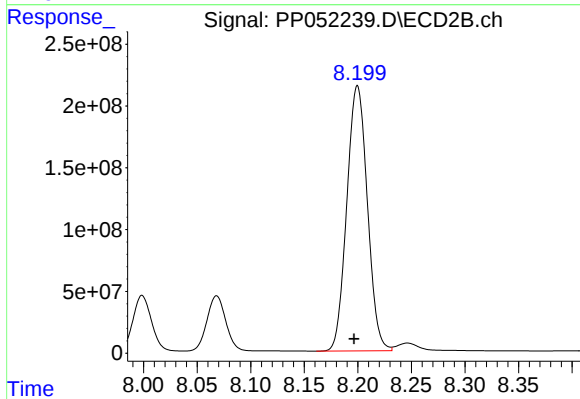

#44 AR-1268-4


R.T.: 8.200 min
Delta R.T.: 0.003 min
Response: 2869916808
Conc: 50784.82 ng/ml

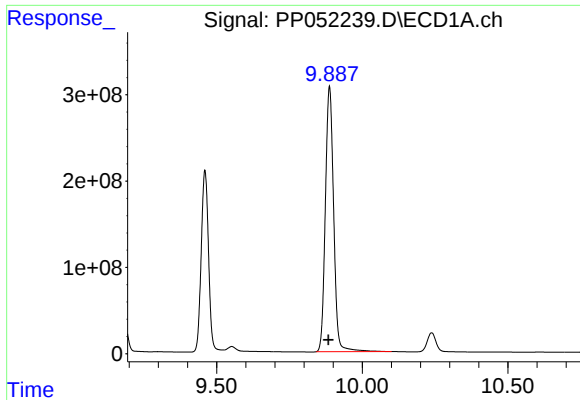

#45 AR-1268-5

R.T.: 9.887 min
Delta R.T.: 0.004 min
Response: 6081036563
Conc: 11661.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-1

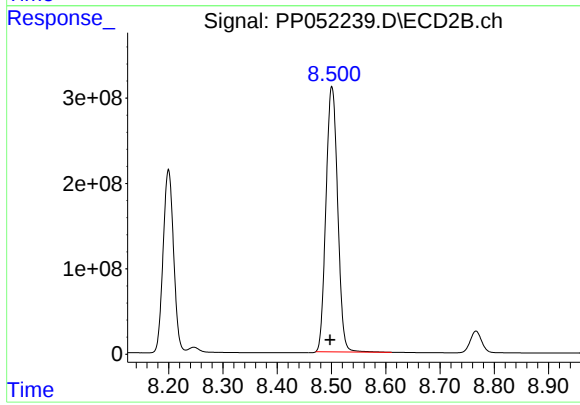

#45 AR-1268-5

R.T.: 8.501 min
Delta R.T.: 0.003 min
Response: 4643720100
Conc: 11039.14 ng/ml