

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
 Data File : PP052240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 19:19
 Operator : YP\AJ
 Sample : N5098-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 250FERRYBLVD-PCB-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 05:40:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.423	3.673	18969203	16225680	12.068	14.163
2)	SA Decachlor...	10.236	8.766	168.4E6	114.7E6	121.345	102.649
Target Compounds							
3)	L1 AR-1016-1	5.596	4.776	1975584	5624212	43.444	126.455 #
4)	L1 AR-1016-2	5.620	4.795	7153124	3720042	108.657	58.462 #
5)	L1 AR-1016-3	5.682	4.975	5559462	4709733	133.592	141.688
6)	L1 AR-1016-4	5.778	5.017	11470989	7261674	315.704	266.432
7)	L1 AR-1016-5	6.077	5.233	-68256	3036463	N.D.	85.826 #
8)	L2 AR-1221-1	4.629	3.893	4777855	5152076	231.213	329.511 #
9)	L2 AR-1221-2	4.718	3.976	3838154	7906857	250.805	659.300 #
10)	L2 AR-1221-3	4.795	4.055	7401432	4995239	158.073	132.166
11)	L3 AR-1232-1	4.795	4.055	7401432	4995239	205.442	172.357
12)	L3 AR-1232-2	5.325	4.795	12144755	3720042	598.566	124.188 #
13)	L3 AR-1232-3	5.620	4.975	7153124	4709733	237.520	308.281 #
14)	L3 AR-1232-4	5.778	5.061	11470989	5490077	687.805	387.703 #
15)	L3 AR-1232-5	5.873	5.233	7954770	3036463	530.399	191.814 #
16)	L4 AR-1242-1	5.596	4.776	1975584	5624212	56.793	161.531 #
17)	L4 AR-1242-2	5.620	4.795	7153124	3720042	144.489	75.409 #
18)	L4 AR-1242-3	5.682	4.975	5559462	4709733	175.337	180.423
19)	L4 AR-1242-4	5.778	5.061	11470989	5490077	419.945	201.841 #
20)	L4 AR-1242-5	6.523	5.593	18117081	20247894	487.311	600.826
21)	L5 AR-1248-1	5.596	4.776	1975584	5624212	73.489	207.448 #
22)	L5 AR-1248-2	5.873	5.017	7954770	7261674	171.135	195.183
23)	L5 AR-1248-3	6.077	5.061	-68256	5490077	N.D.	144.110 #
24)	L5 AR-1248-4	6.456f	5.233	43941915	3036463	692.076	65.533 #
25)	L5 AR-1248-5	6.523	5.633	18117081	5906294	292.518	140.448 #
26)	L6 AR-1254-1	6.456	5.593	43941915	20247894	617.252	289.410 #
27)	L6 AR-1254-2	6.676	5.741	47832824	25003917	448.496	399.075
28)	L6 AR-1254-3	7.045	6.166f	22085282	167.5E6	210.136	1693.197 #
29)	L6 AR-1254-4	7.328	6.379	23598561	13231427	322.965	221.345 #
30)	L6 AR-1254-5	7.740	6.804	287.1E6	145.0E6	3459.886	1635.033 #
31)	L7 AR-1260-1	7.209	6.282	256.5E6	189.5E6	3095.201	2751.591
32)	L7 AR-1260-2	7.466	6.471	479.7E6	408.4E6	5082.074	4933.942
33)	L7 AR-1260-3	7.828	6.632	1743.3E6	396.0E6	29026.465	5129.469 #
34)	L7 AR-1260-4	8.054	7.103	1259.5E6	1030.4E6	16422.206	18329.786
35)	L7 AR-1260-5	8.377	7.347	2527.5E6	2197.6E6	18438.253	16664.200
36)	L8 AR-1262-1	7.828	6.895	1743.3E6	570.8E6	17978.816	15867.217
37)	L8 AR-1262-2	8.377	7.103	2527.5E6	1030.4E6	15697.721	13012.761
38)	L8 AR-1262-3	8.694	7.634	2926.2E6	2280.9E6	26625.772	36935.672 #
39)	L8 AR-1262-4	8.788	7.699	3471.1E6	2909.7E6	67903.413	25487.296 #
40)	L8 AR-1262-5	9.459	8.199	2129.1E6	1601.8E6	33822.300	31514.305
41)	L9 AR-1268-1	8.694	7.634	2926.2E6	2280.9E6	14780.196	12572.918

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 19:19
Operator : YP\AJ
Sample : N5098-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:40:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.788	7.699	3471.1E6	2909.7E6	18903.666	17808.719
43)	L9 AR-1268-3	9.024	7.908	519.7E6	422.1E6	3187.845	3001.595
44)	L9 AR-1268-4	9.459	8.199	2129.1E6	1601.8E6	29180.712	28345.257
45)	L9 AR-1268-5	9.887	8.501	2727.5E6	2050.0E6	5230.680	4873.344



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101222\
Data File : PP052240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 19:19
Operator : YP\AJ
Sample : N5098-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 05:40:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

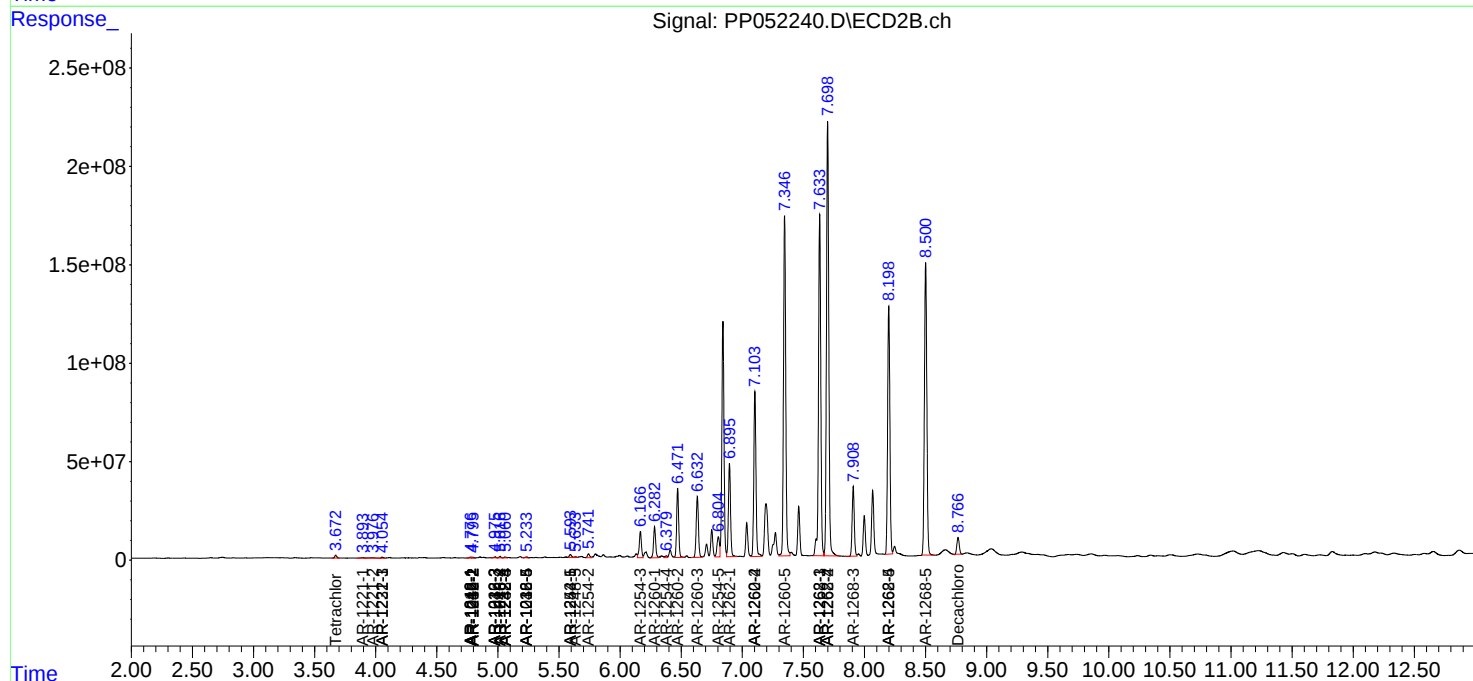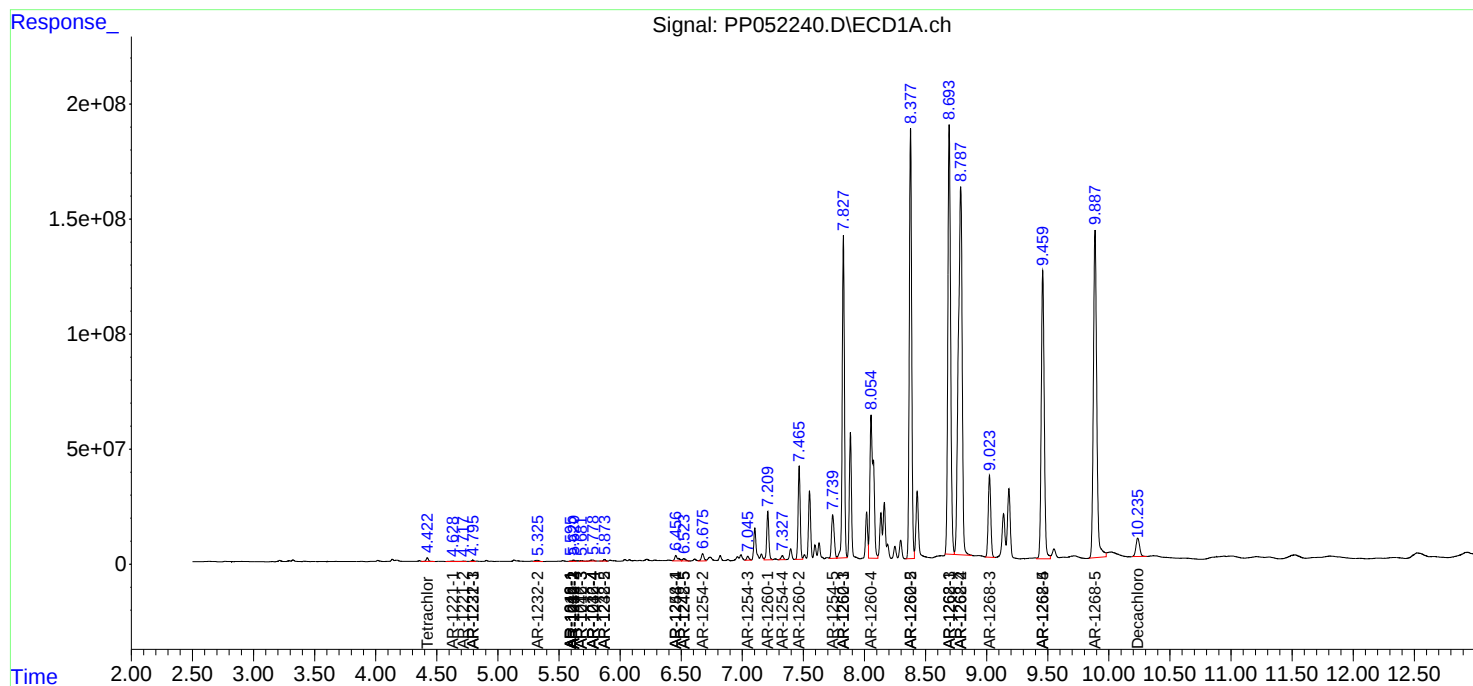


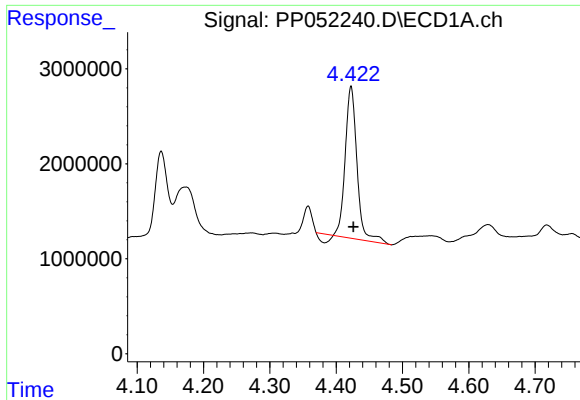

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: -0.003 min
Response: 18969203
Conc: 12.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

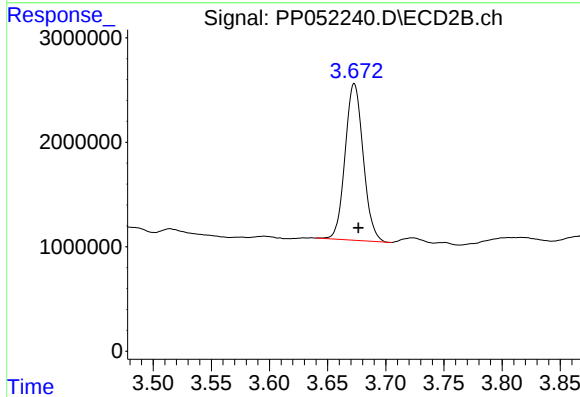


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.004 min
Response: 16225680
Conc: 14.16 ng/ml

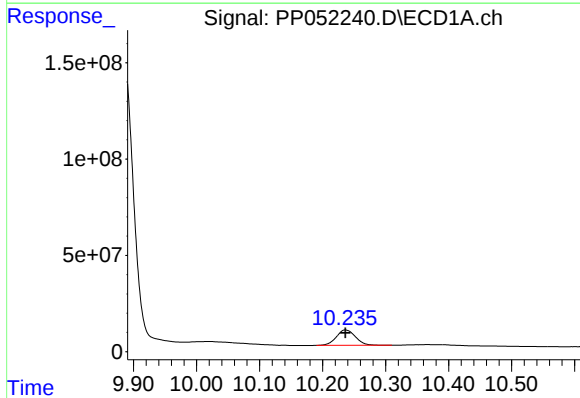


#2 Decachlorobiphenyl

R.T.: 10.236 min
Delta R.T.: 0.000 min
Response: 168407930
Conc: 121.34 ng/ml

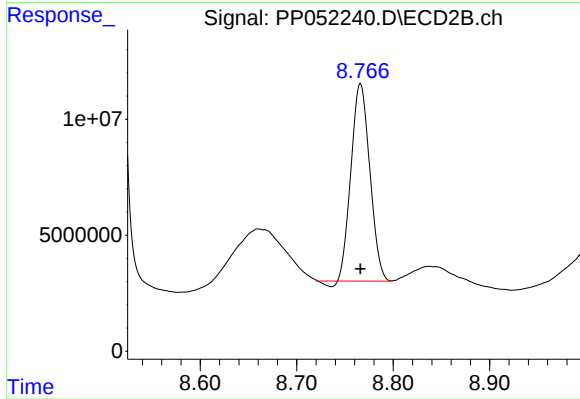

#2 Decachlorobiphenyl


R.T.: 8.766 min
Delta R.T.: 0.000 min
Response: 114695897
Conc: 102.65 ng/ml

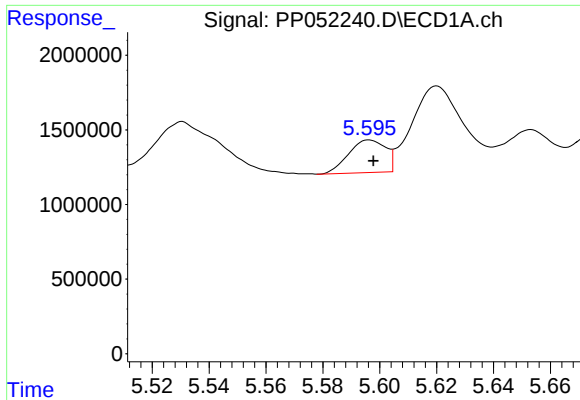

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: -0.001 min
Response: 1975584
Conc: 43.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

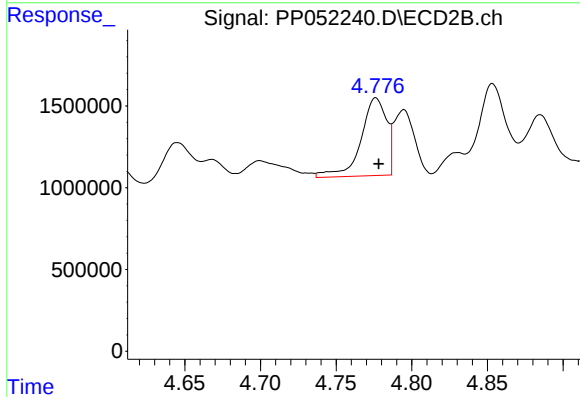


#3 AR-1016-1

R.T.: 4.776 min
Delta R.T.: -0.002 min
Response: 5624212
Conc: 126.45 ng/ml

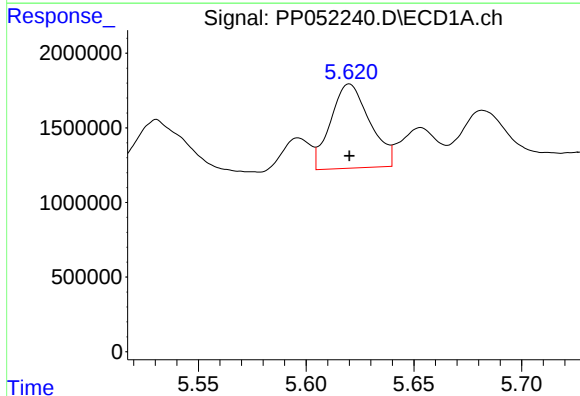


#4 AR-1016-2

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 7153124
Conc: 108.66 ng/ml

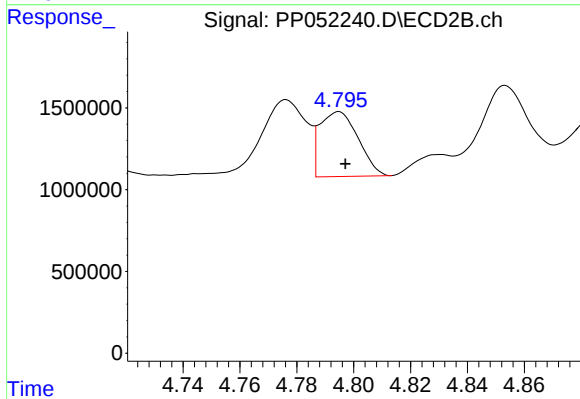

#4 AR-1016-2


R.T.: 4.795 min
Delta R.T.: -0.002 min
Response: 3720042
Conc: 58.46 ng/ml

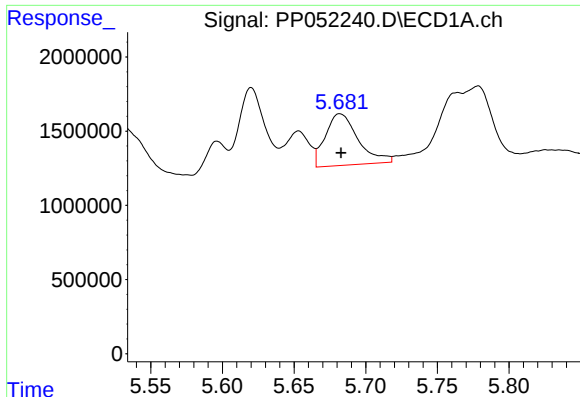

#5 AR-1016-3


R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 5559462
Conc: 133.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

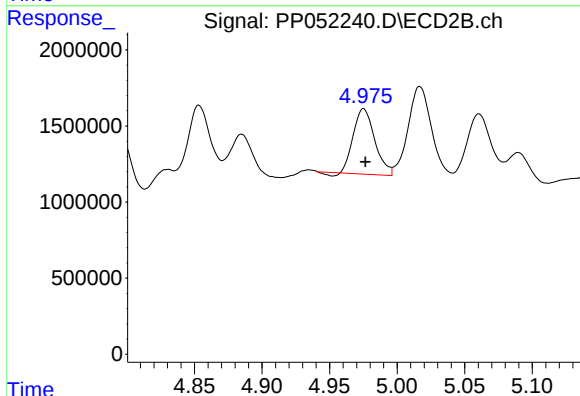


#5 AR-1016-3

R.T.: 4.975 min
Delta R.T.: -0.001 min
Response: 4709733
Conc: 141.69 ng/ml

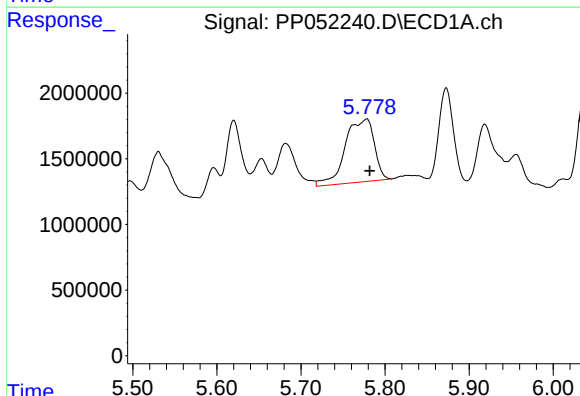


#6 AR-1016-4

R.T.: 5.778 min
Delta R.T.: -0.004 min
Response: 11470989
Conc: 315.70 ng/ml

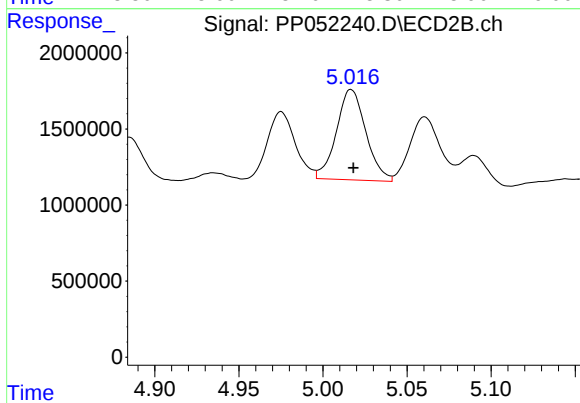

#6 AR-1016-4


R.T.: 5.017 min
Delta R.T.: -0.001 min
Response: 7261674
Conc: 266.43 ng/ml

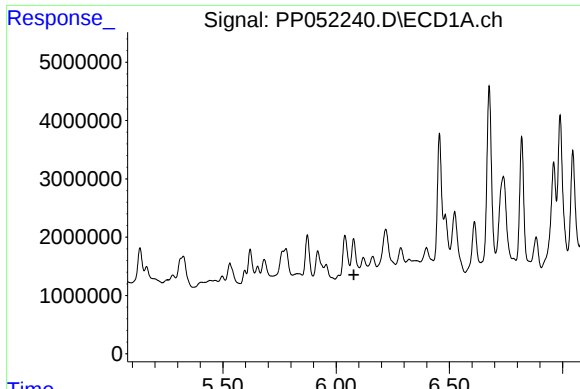

#7 AR-1016-5


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: -68256
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

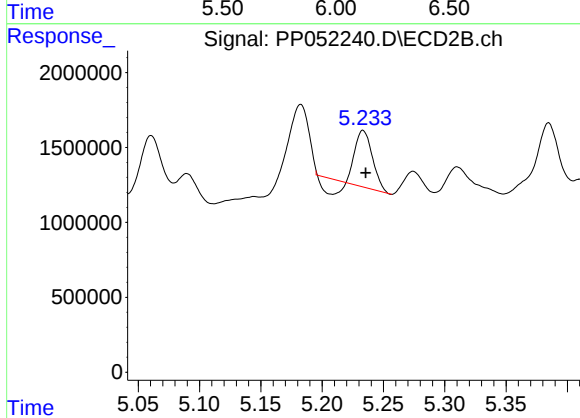


#7 AR-1016-5

R.T.: 5.233 min
Delta R.T.: -0.002 min
Response: 3036463
Conc: 85.83 ng/ml

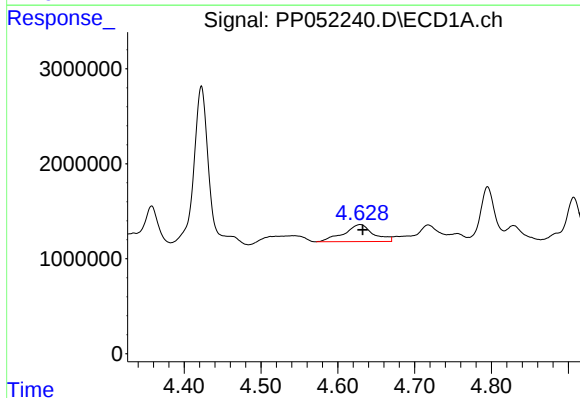


#8 AR-1221-1

R.T.: 4.629 min
Delta R.T.: -0.004 min
Response: 4777855
Conc: 231.21 ng/ml

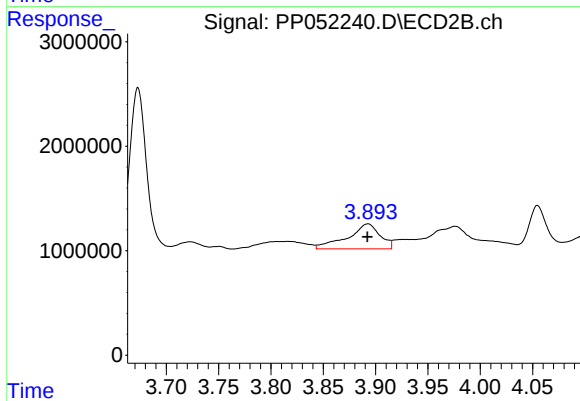

#8 AR-1221-1


R.T.: 3.893 min
Delta R.T.: 0.000 min
Response: 5152076
Conc: 329.51 ng/ml

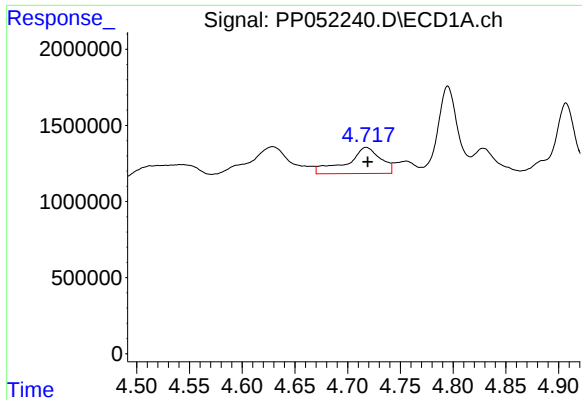

#9 AR-1221-2


R.T.: 4.718 min
Delta R.T.: -0.001 min
Response: 3838154
Conc: 250.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

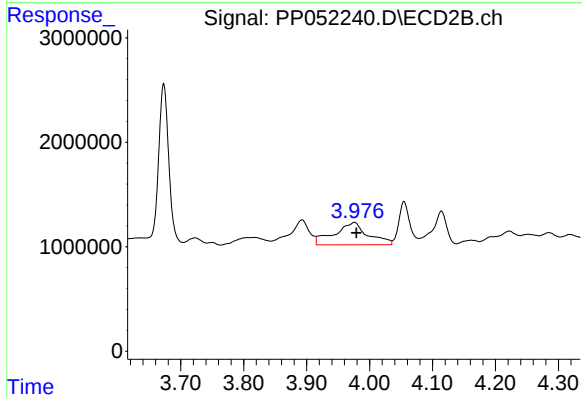


#9 AR-1221-2

R.T.: 3.976 min
Delta R.T.: -0.003 min
Response: 7906857
Conc: 659.30 ng/ml

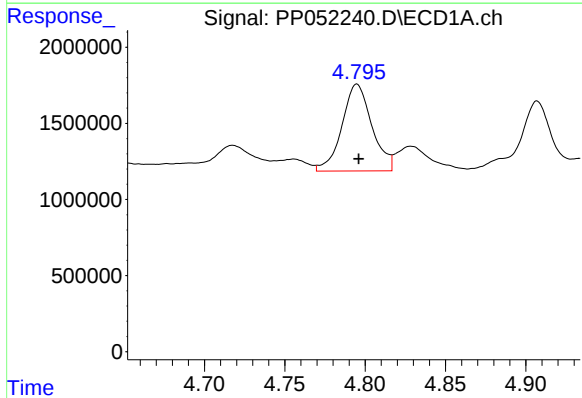


#10 AR-1221-3

R.T.: 4.795 min
Delta R.T.: -0.001 min
Response: 7401432
Conc: 158.07 ng/ml

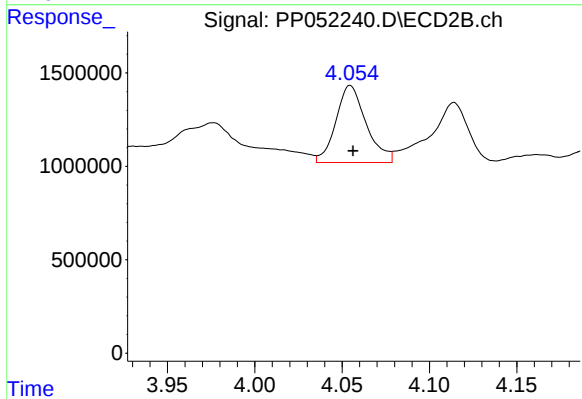

#10 AR-1221-3


R.T.: 4.055 min
Delta R.T.: -0.002 min
Response: 4995239
Conc: 132.17 ng/ml

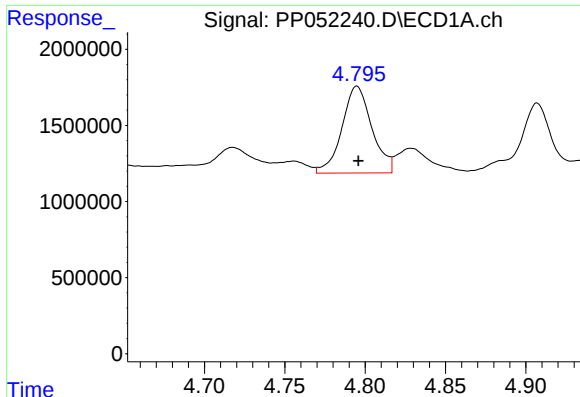

#11 AR-1232-1


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 7401432
Conc: 205.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

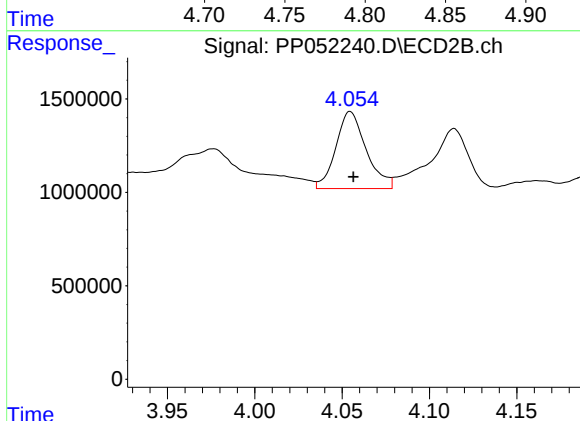


#11 AR-1232-1

R.T.: 4.055 min
Delta R.T.: -0.002 min
Response: 4995239
Conc: 172.36 ng/ml

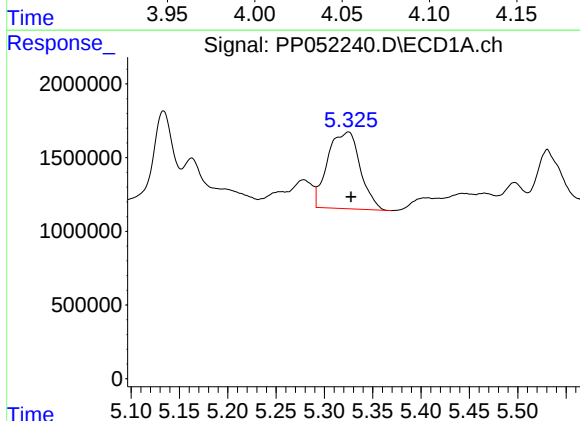


#12 AR-1232-2

R.T.: 5.325 min
Delta R.T.: -0.003 min
Response: 12144755
Conc: 598.57 ng/ml

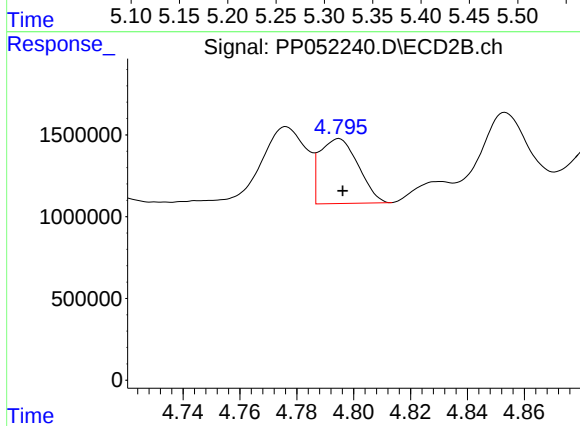

#12 AR-1232-2


R.T.: 4.795 min
Delta R.T.: -0.001 min
Response: 3720042
Conc: 124.19 ng/ml

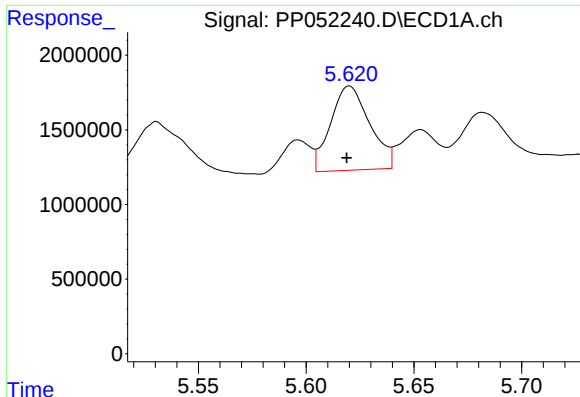

#13 AR-1232-3


R.T.: 5.620 min
Delta R.T.: 0.001 min
Response: 7153124
Conc: 237.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

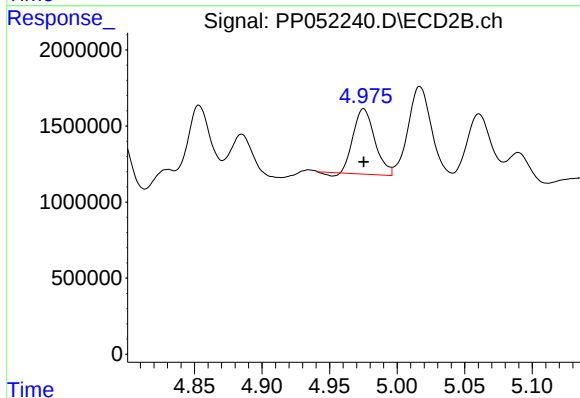


#13 AR-1232-3

R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 4709733
Conc: 308.28 ng/ml

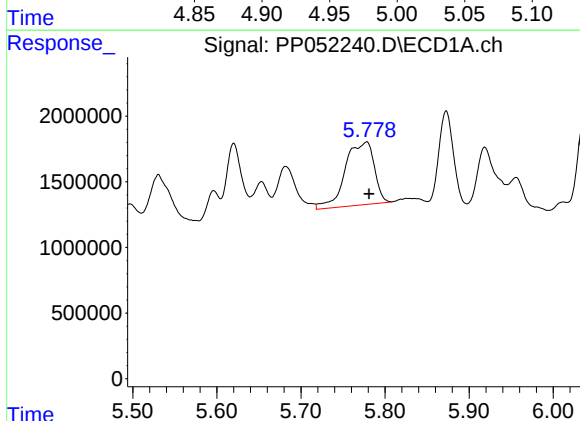


#14 AR-1232-4

R.T.: 5.778 min
Delta R.T.: -0.003 min
Response: 11470989
Conc: 687.80 ng/ml

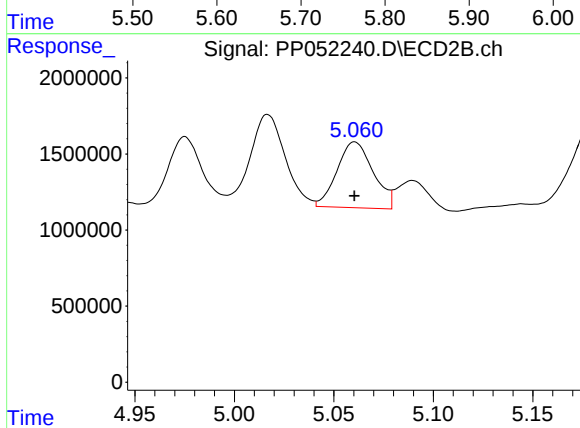

#14 AR-1232-4


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 5490077
Conc: 387.70 ng/ml

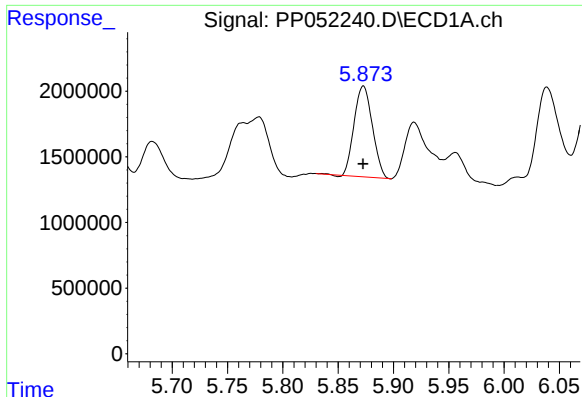

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: 0.000 min
Response: 7954770
Conc: 530.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

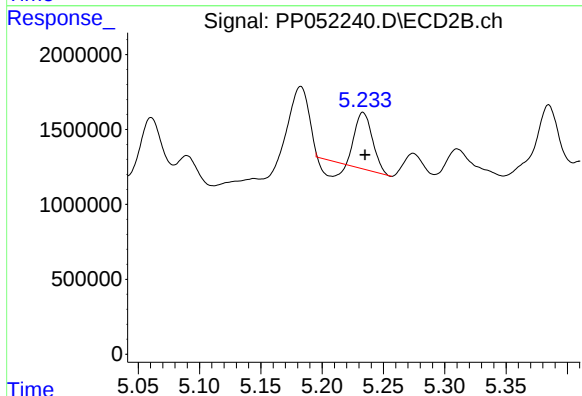


#15 AR-1232-5

R.T.: 5.233 min
Delta R.T.: -0.002 min
Response: 3036463
Conc: 191.81 ng/ml

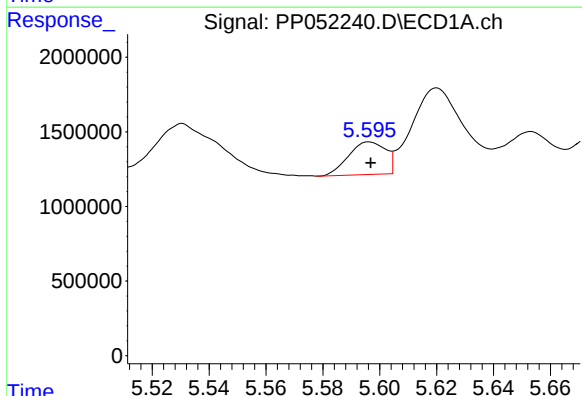


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 1975584
Conc: 56.79 ng/ml

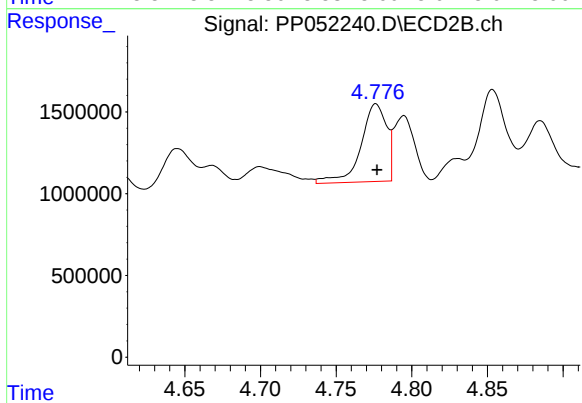

#16 AR-1242-1


R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 5624212
Conc: 161.53 ng/ml

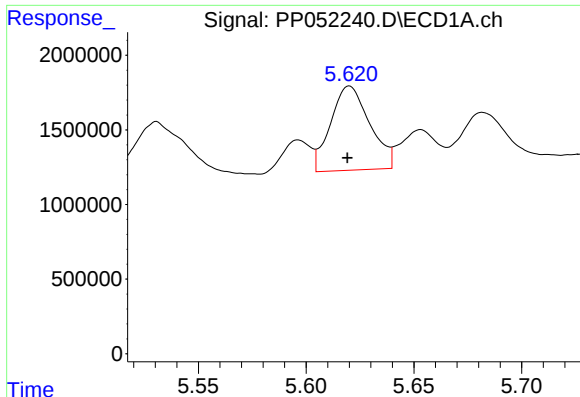

#17 AR-1242-2


R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 7153124
Conc: 144.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

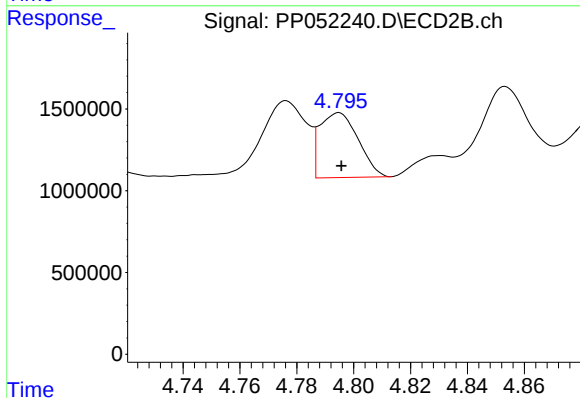


#17 AR-1242-2

R.T.: 4.795 min
Delta R.T.: -0.001 min
Response: 3720042
Conc: 75.41 ng/ml

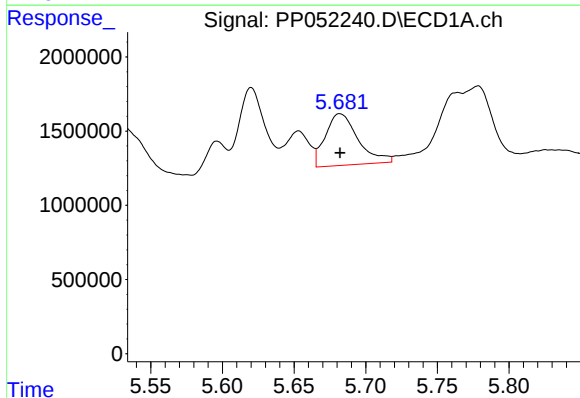


#18 AR-1242-3

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 5559462
Conc: 175.34 ng/ml

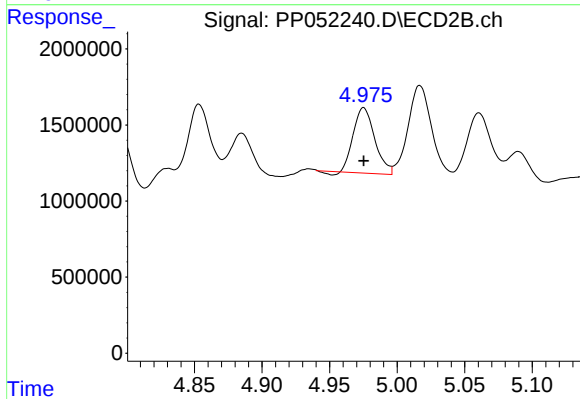

#18 AR-1242-3


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 4709733
Conc: 180.42 ng/ml

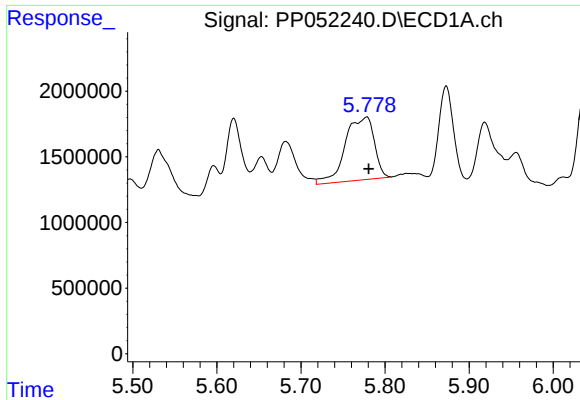

#19 AR-1242-4


R.T.: 5.778 min
Delta R.T.: -0.003 min
Response: 11470989
Conc: 419.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

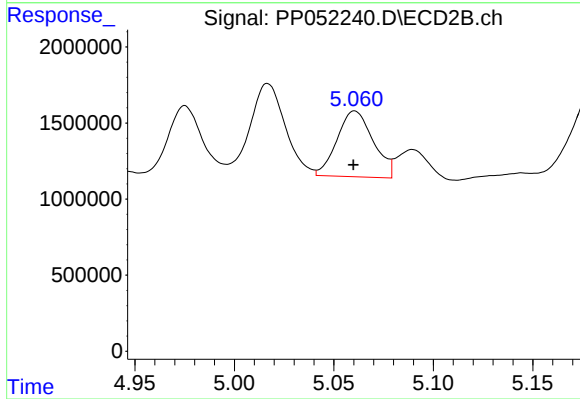


#19 AR-1242-4

R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 5490077
Conc: 201.84 ng/ml

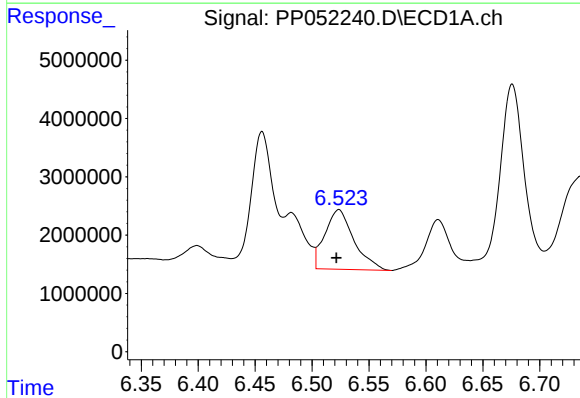


#20 AR-1242-5

R.T.: 6.523 min
Delta R.T.: 0.002 min
Response: 18117081
Conc: 487.31 ng/ml

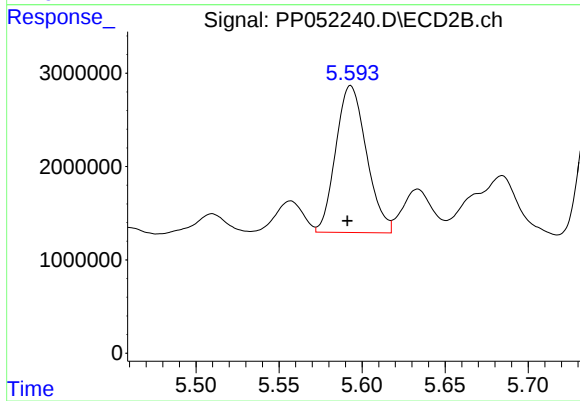

#20 AR-1242-5


R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 20247894
Conc: 600.83 ng/ml

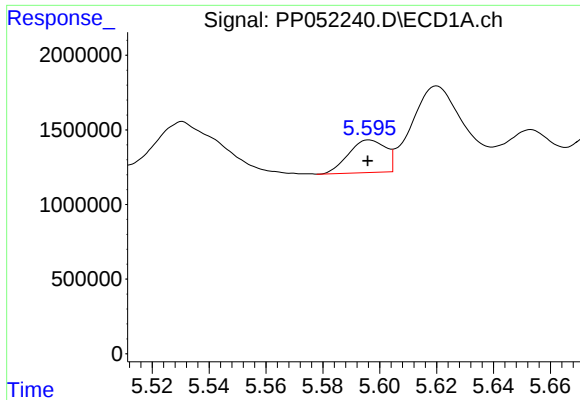

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 1975584
Conc: 73.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

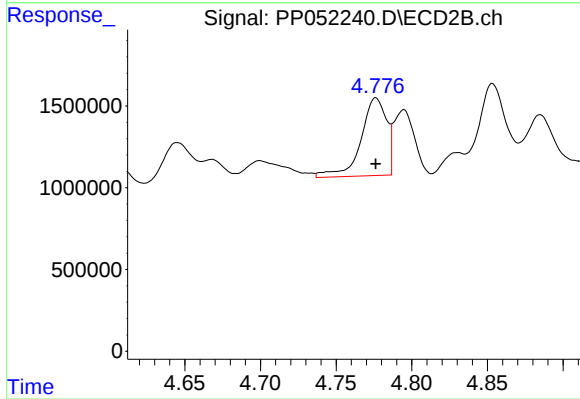


#21 AR-1248-1

R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 5624212
Conc: 207.45 ng/ml

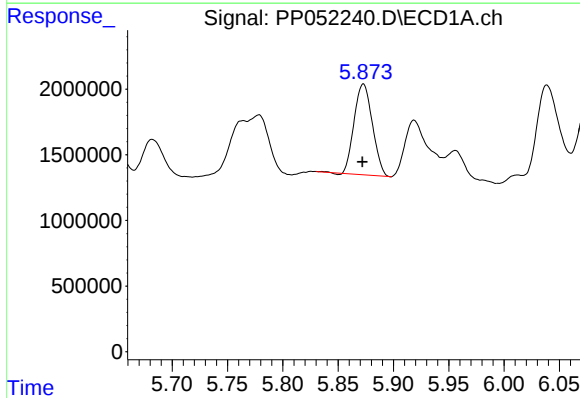


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: 0.001 min
Response: 7954770
Conc: 171.14 ng/ml

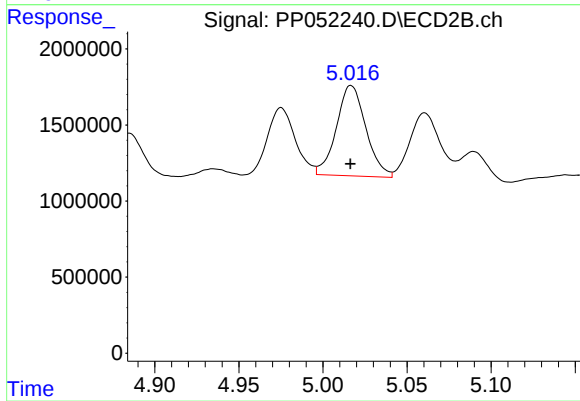

#22 AR-1248-2


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 7261674
Conc: 195.18 ng/ml

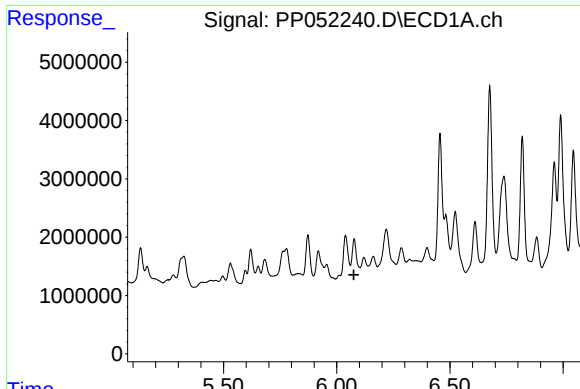

#23 AR-1248-3


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: -68256
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

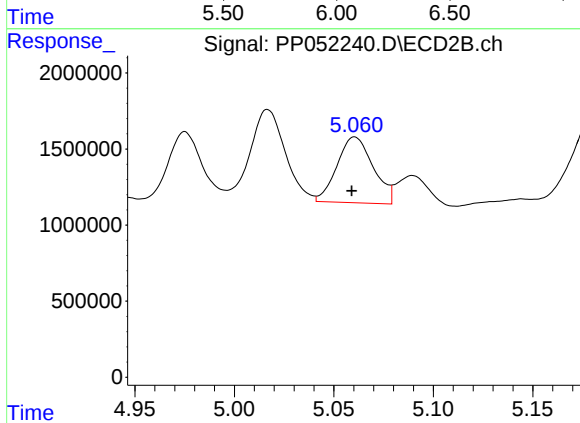


#23 AR-1248-3

R.T.: 5.061 min
Delta R.T.: 0.002 min
Response: 5490077
Conc: 144.11 ng/ml

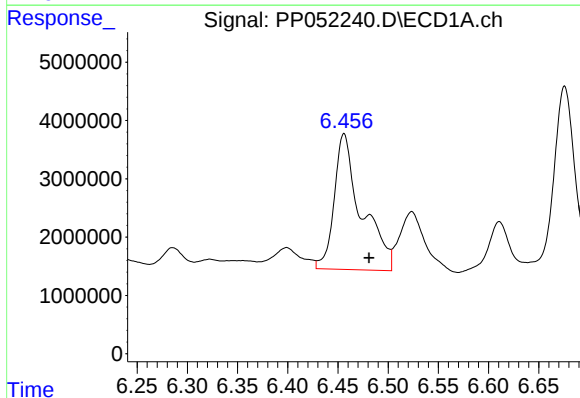


#24 AR-1248-4

R.T.: 6.456 min
Delta R.T.: -0.025 min
Response: 43941915
Conc: 692.08 ng/ml

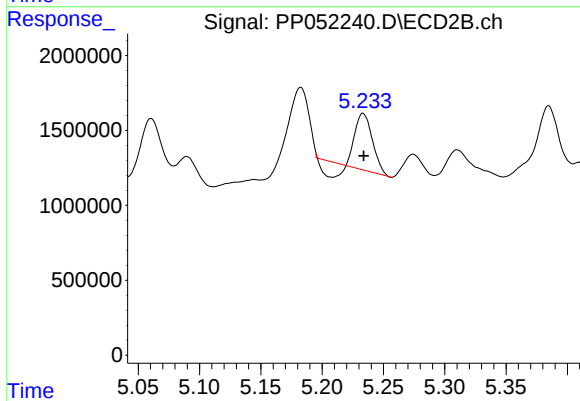

#24 AR-1248-4


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 3036463
Conc: 65.53 ng/ml

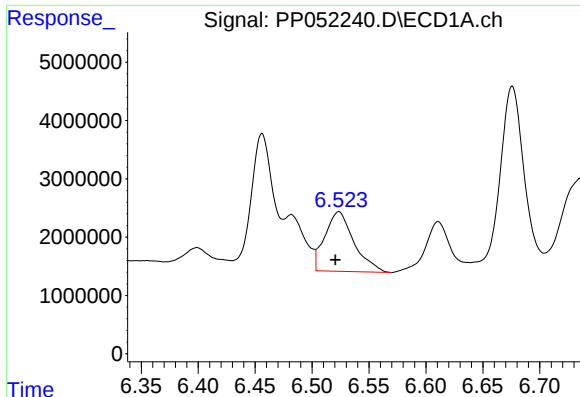

#25 AR-1248-5


R.T.: 6.523 min
Delta R.T.: 0.003 min
Response: 18117081
Conc: 292.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

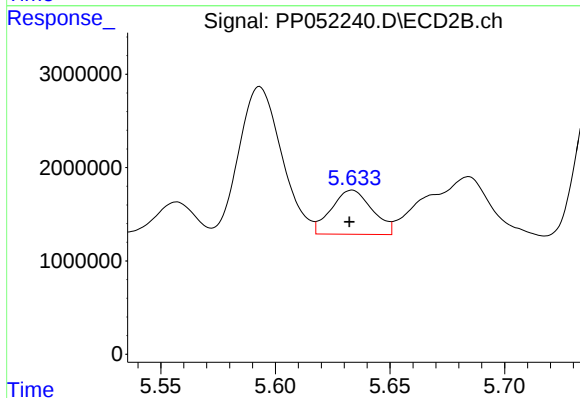


#25 AR-1248-5

R.T.: 5.633 min
Delta R.T.: 0.001 min
Response: 5906294
Conc: 140.45 ng/ml

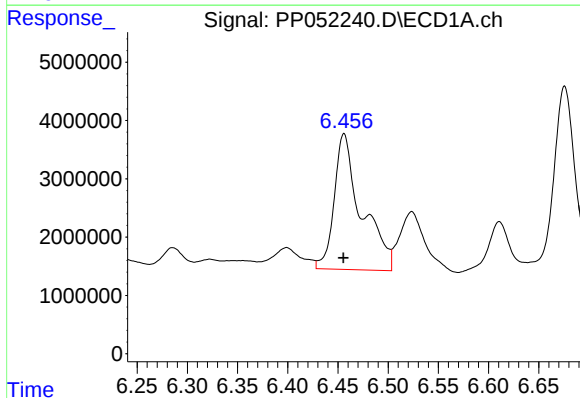


#26 AR-1254-1

R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 43941915
Conc: 617.25 ng/ml

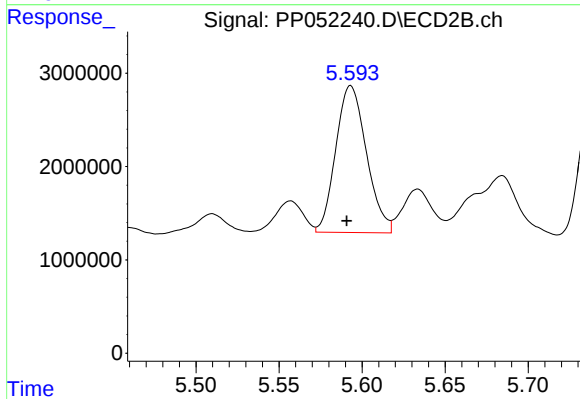

#26 AR-1254-1


R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 20247894
Conc: 289.41 ng/ml

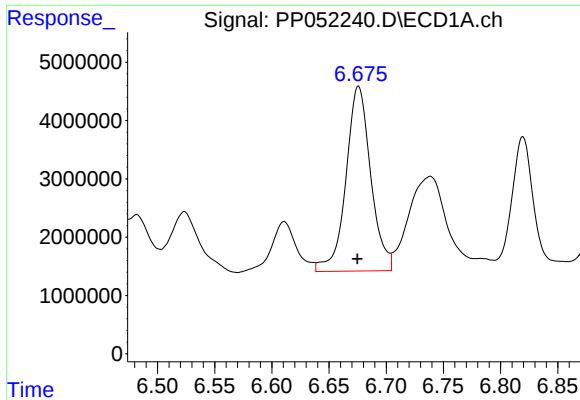

#27 AR-1254-2


R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 47832824
Conc: 448.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

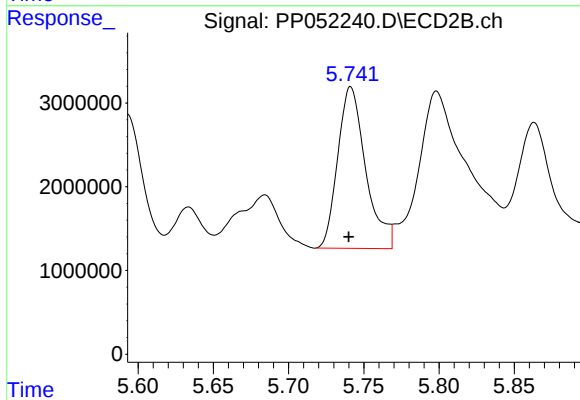


#27 AR-1254-2

R.T.: 5.741 min
Delta R.T.: 0.001 min
Response: 25003917
Conc: 399.07 ng/ml

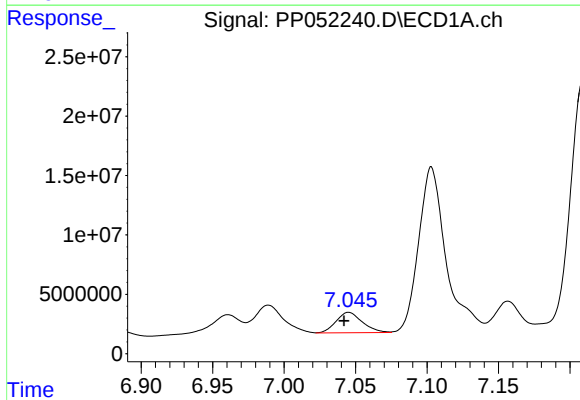


#28 AR-1254-3

R.T.: 7.045 min
Delta R.T.: 0.003 min
Response: 22085282
Conc: 210.14 ng/ml

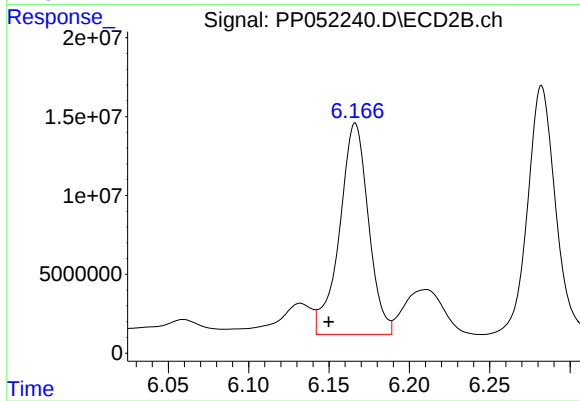

#28 AR-1254-3


R.T.: 6.166 min
Delta R.T.: 0.017 min
Response: 167490615
Conc: 1693.20 ng/ml

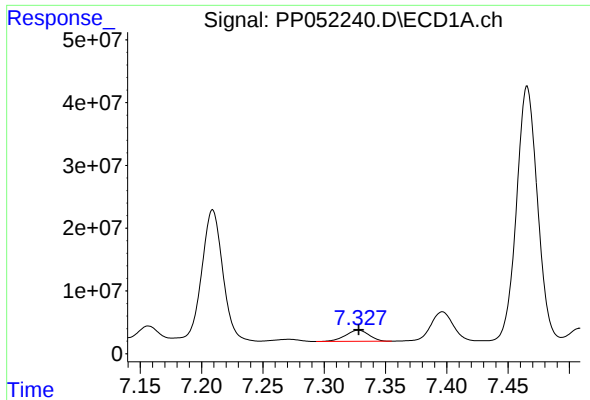

#29 AR-1254-4


R.T.: 7.328 min
Delta R.T.: 0.000 min
Response: 23598561
Conc: 322.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

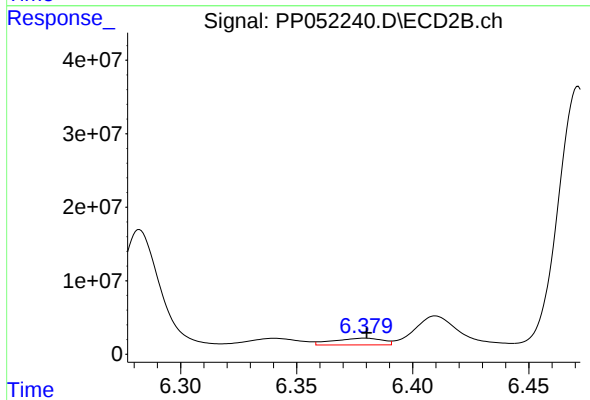


#29 AR-1254-4

R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 13231427
Conc: 221.35 ng/ml

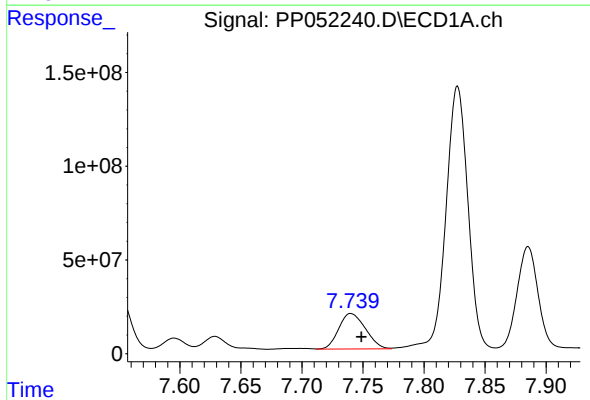


#30 AR-1254-5

R.T.: 7.740 min
Delta R.T.: -0.008 min
Response: 287078975
Conc: 3459.89 ng/ml

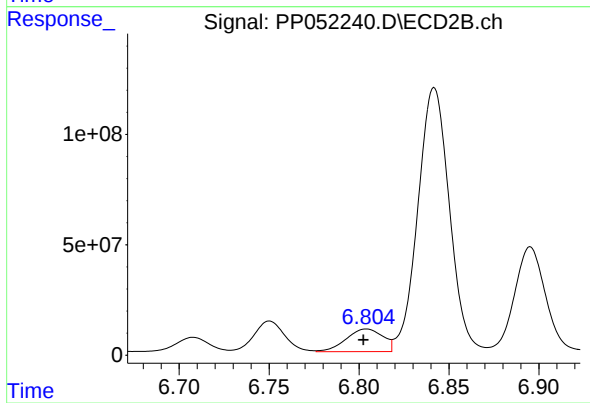

#30 AR-1254-5


R.T.: 6.804 min
Delta R.T.: 0.002 min
Response: 144952593
Conc: 1635.03 ng/ml

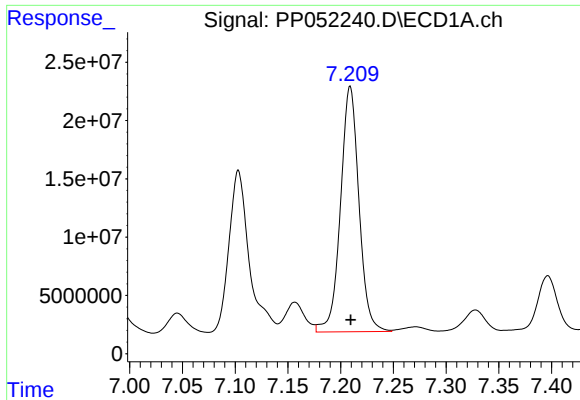

#31 AR-1260-1


R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 256548146
Conc: 3095.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

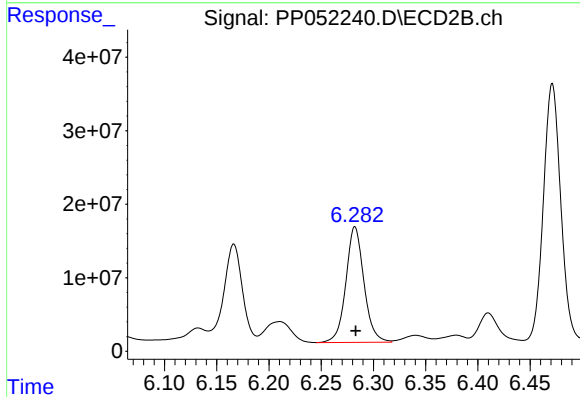


#31 AR-1260-1

R.T.: 6.282 min
Delta R.T.: 0.000 min
Response: 189536847
Conc: 2751.59 ng/ml

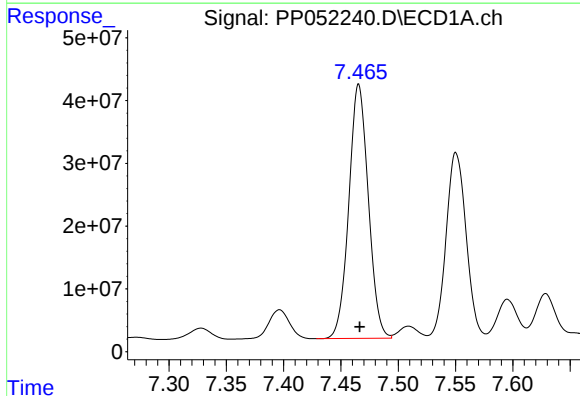


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 479671544
Conc: 5082.07 ng/ml

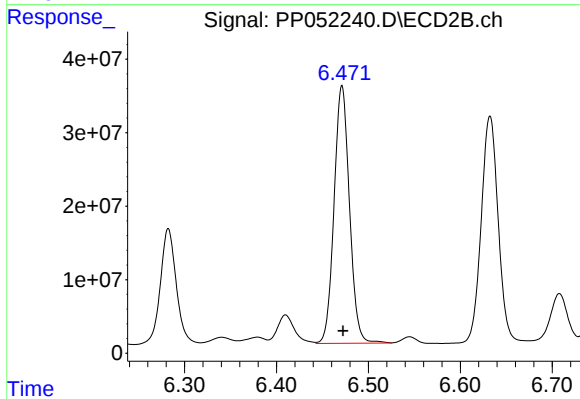

#32 AR-1260-2


R.T.: 6.471 min
Delta R.T.: -0.001 min
Response: 408363619
Conc: 4933.94 ng/ml

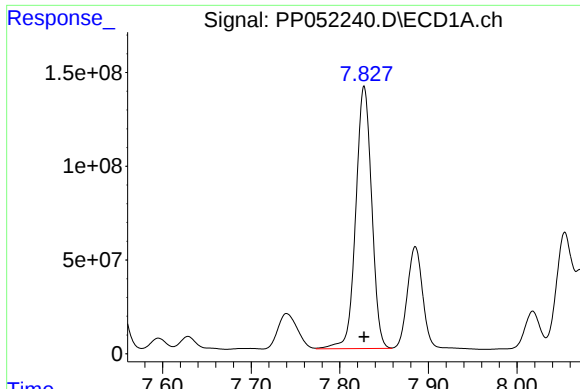

#33 AR-1260-3


R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 1743299036
Conc: 29026.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

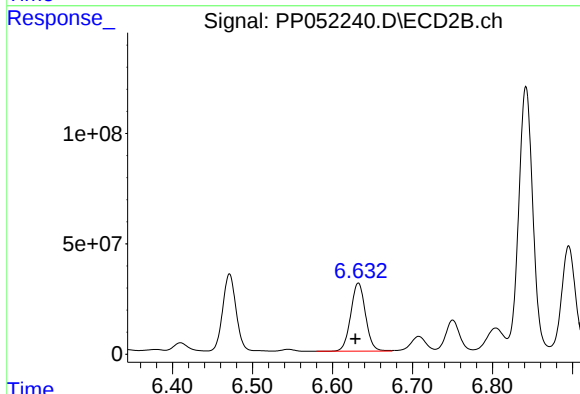


#33 AR-1260-3

R.T.: 6.632 min
Delta R.T.: 0.004 min
Response: 396034346
Conc: 5129.47 ng/ml

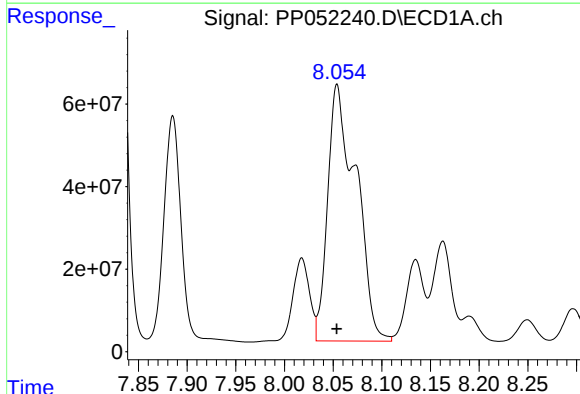


#34 AR-1260-4

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 1259482495
Conc: 16422.21 ng/ml

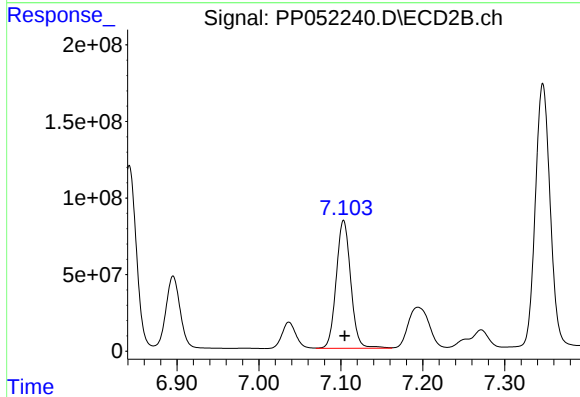

#34 AR-1260-4


R.T.: 7.103 min
Delta R.T.: -0.001 min
Response: 1030400802
Conc: 18329.79 ng/ml

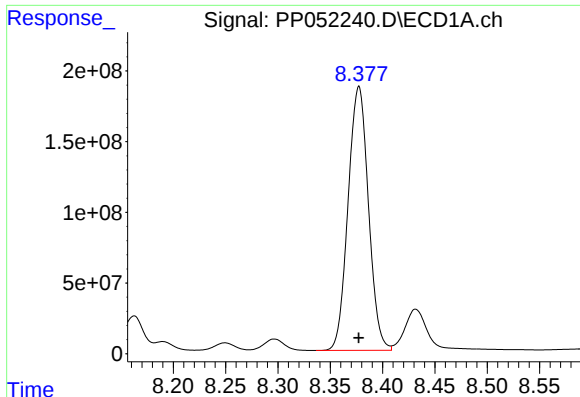

#35 AR-1260-5


R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 2527480067
Conc: 18438.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

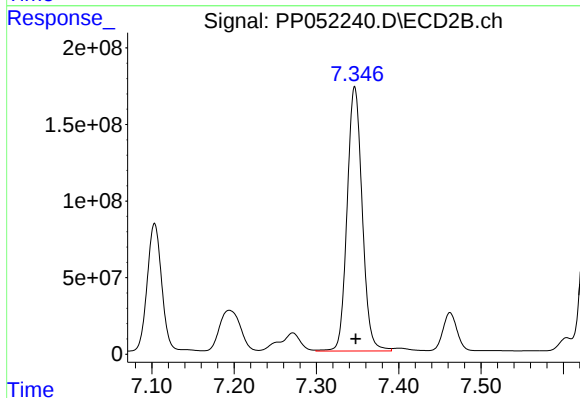


#35 AR-1260-5

R.T.: 7.347 min
Delta R.T.: -0.001 min
Response: 2197626449
Conc: 16664.20 ng/ml

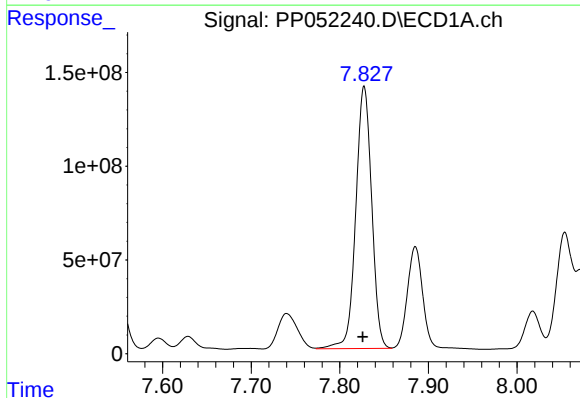


#36 AR-1262-1

R.T.: 7.828 min
Delta R.T.: 0.002 min
Response: 1743299036
Conc: 17978.82 ng/ml

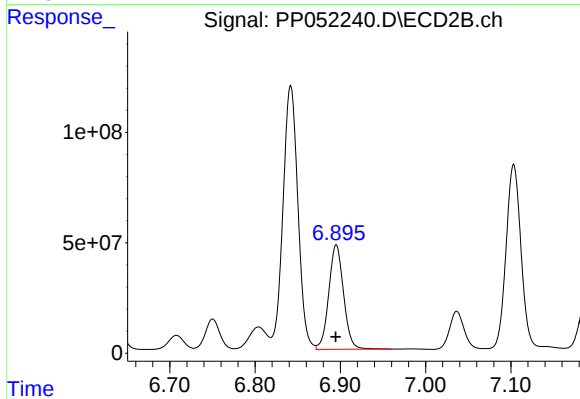

#36 AR-1262-1


R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 570768713
Conc: 15867.22 ng/ml

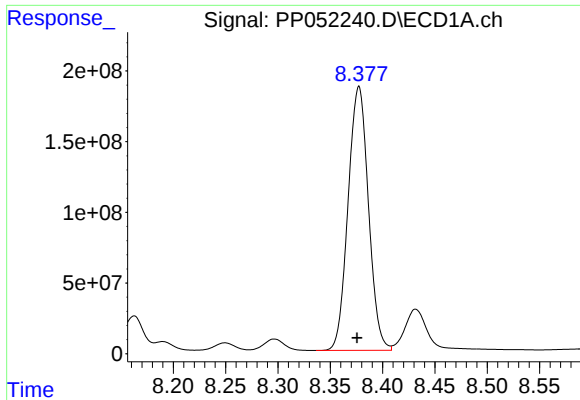

#37 AR-1262-2


R.T.: 8.377 min
Delta R.T.: 0.002 min
Response: 2527480067
Conc: 15697.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

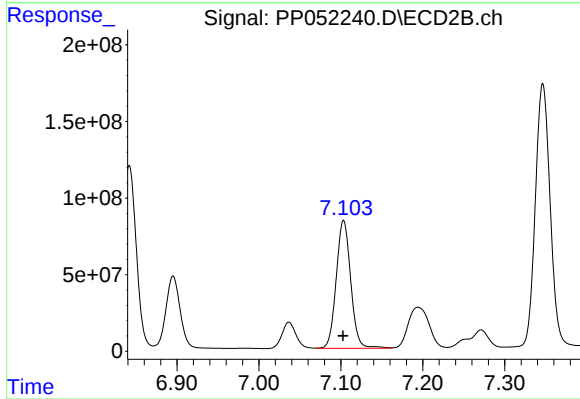


#37 AR-1262-2

R.T.: 7.103 min
Delta R.T.: 0.000 min
Response: 1030400802
Conc: 13012.76 ng/ml

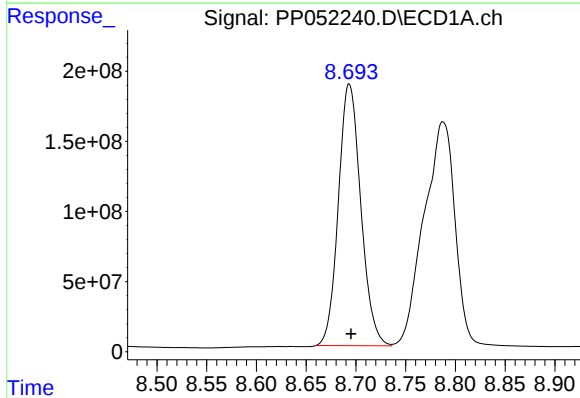


#38 AR-1262-3

R.T.: 8.694 min
Delta R.T.: -0.002 min
Response: 2926167325
Conc: 26625.77 ng/ml

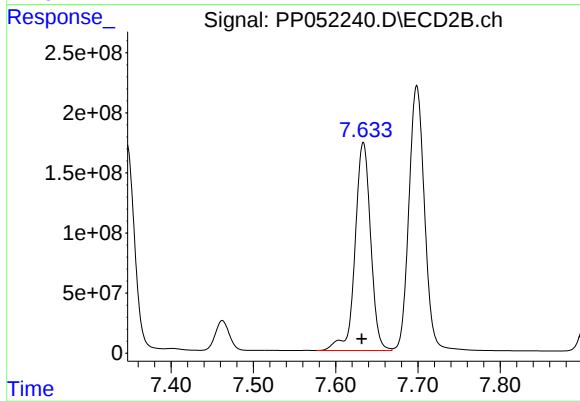

#38 AR-1262-3


R.T.: 7.634 min
Delta R.T.: 0.002 min
Response: 2280854709
Conc: 36935.67 ng/ml

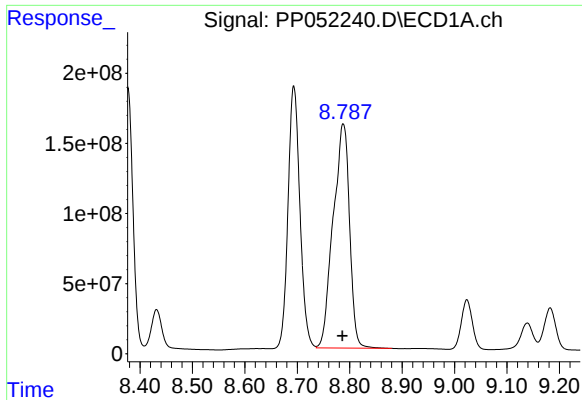

#39 AR-1262-4


R.T.: 8.788 min
Delta R.T.: 0.002 min
Response: 3471132363
Conc: 67903.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

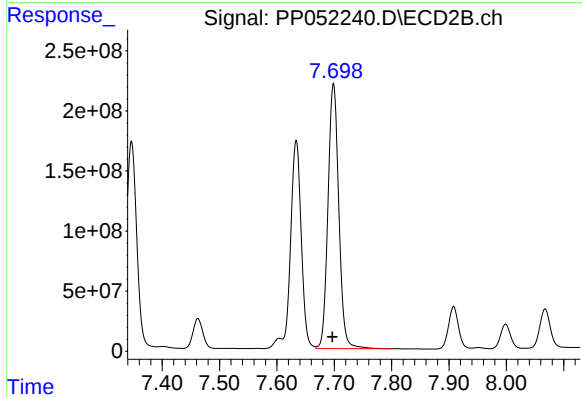


#39 AR-1262-4

R.T.: 7.699 min
Delta R.T.: 0.002 min
Response: 2909714305
Conc: 25487.30 ng/ml

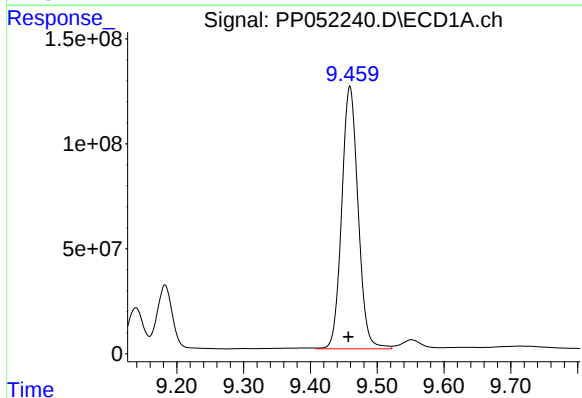


#40 AR-1262-5

R.T.: 9.459 min
Delta R.T.: 0.002 min
Response: 2129080493
Conc: 33822.30 ng/ml

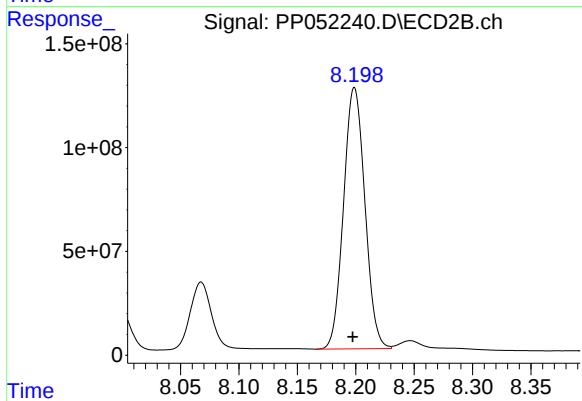

#40 AR-1262-5


R.T.: 8.199 min
Delta R.T.: 0.001 min
Response: 1601827795
Conc: 31514.30 ng/ml

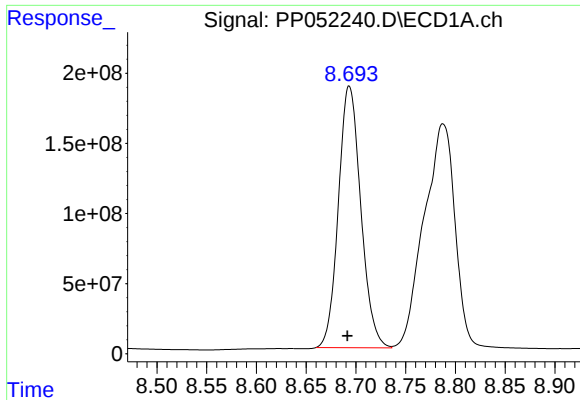

#41 AR-1268-1


R.T.: 8.694 min
Delta R.T.: 0.002 min
Response: 2926167325
Conc: 14780.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

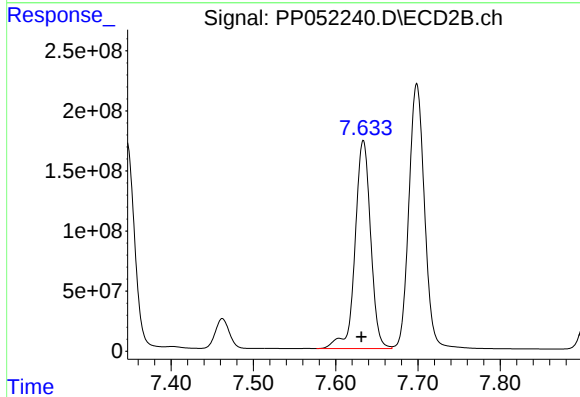


#41 AR-1268-1

R.T.: 7.634 min
Delta R.T.: 0.002 min
Response: 2280854709
Conc: 12572.92 ng/ml

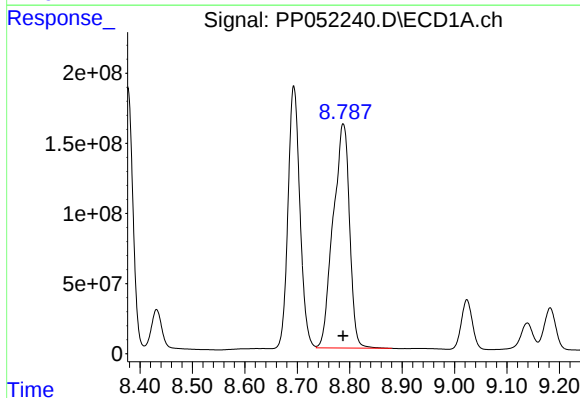


#42 AR-1268-2

R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 3471132363
Conc: 18903.67 ng/ml

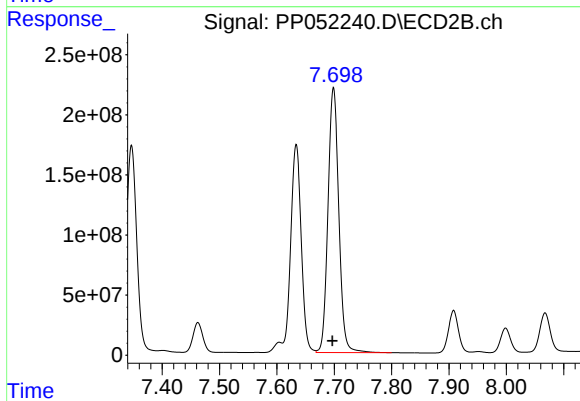

#42 AR-1268-2


R.T.: 7.699 min
Delta R.T.: 0.002 min
Response: 2909714305
Conc: 17808.72 ng/ml

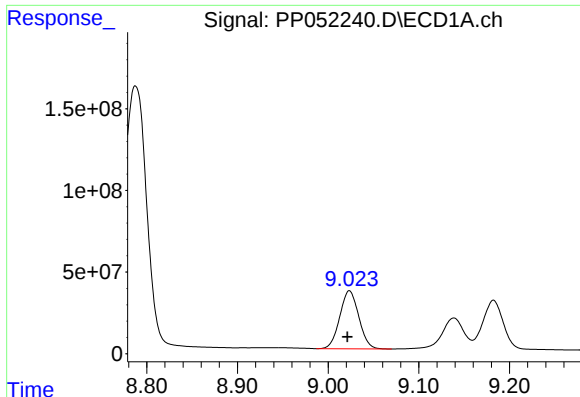

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.002 min
Response: 519661952
Conc: 3187.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

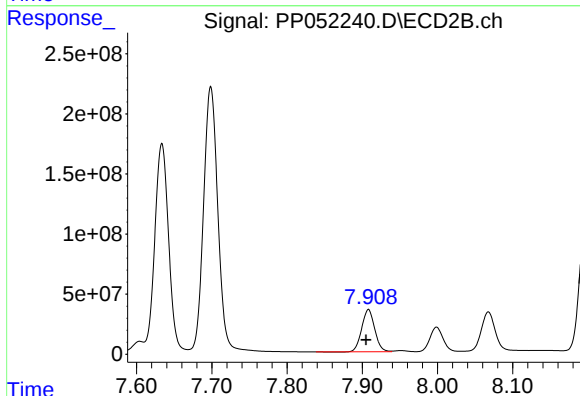


#43 AR-1268-3

R.T.: 7.908 min
Delta R.T.: 0.003 min
Response: 422091654
Conc: 3001.60 ng/ml

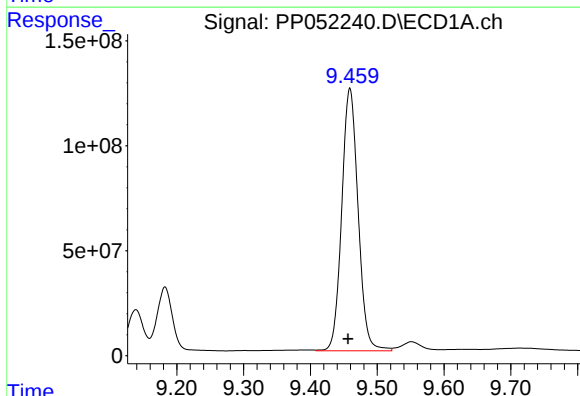


#44 AR-1268-4

R.T.: 9.459 min
Delta R.T.: 0.003 min
Response: 2129080493
Conc: 29180.71 ng/ml

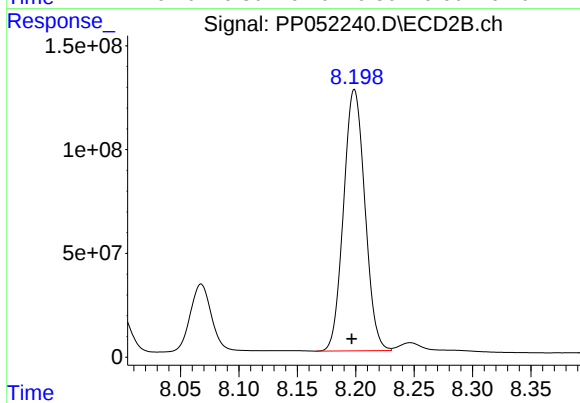

#44 AR-1268-4


R.T.: 8.199 min
Delta R.T.: 0.002 min
Response: 1601827795
Conc: 28345.26 ng/ml

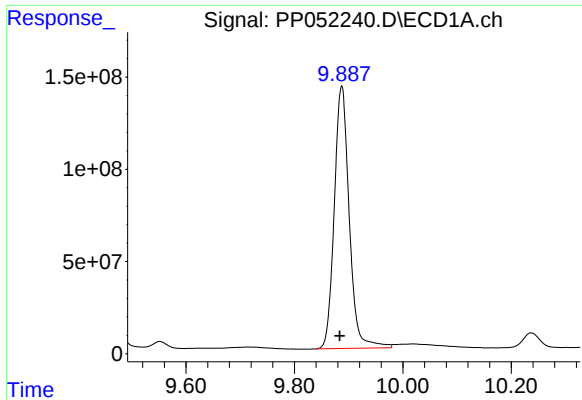

#45 AR-1268-5

R.T.: 9.887 min
Delta R.T.: 0.003 min
Response: 2727502161
Conc: 5230.68 ng/m

Instrument :
ECD_P
ClientSampleId :
250FERRYBLVD-PCB-2

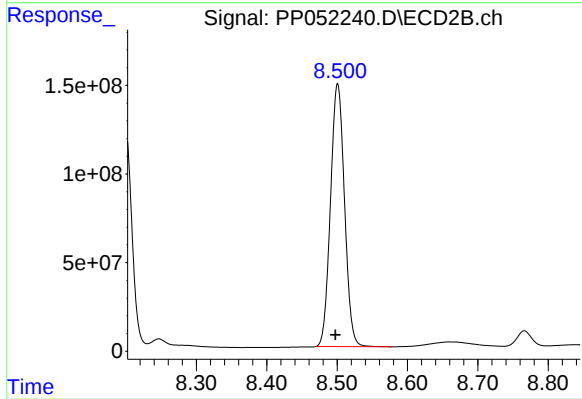

#45 AR-1268-5

R.T.: 8.501 min
Delta R.T.: 0.003 min
Response: 2050019668
Conc: 4873.34 ng/ml